ROHDE&SCHWARZ

DOCUMENTATION

DOCUMENTATION

DOCUMENTATION

DOCUMENTATION

DOCUMENTATION

DOCUMENTATION

DOCUMENTATION

DOCUMENTATION

DOCUMENTATION

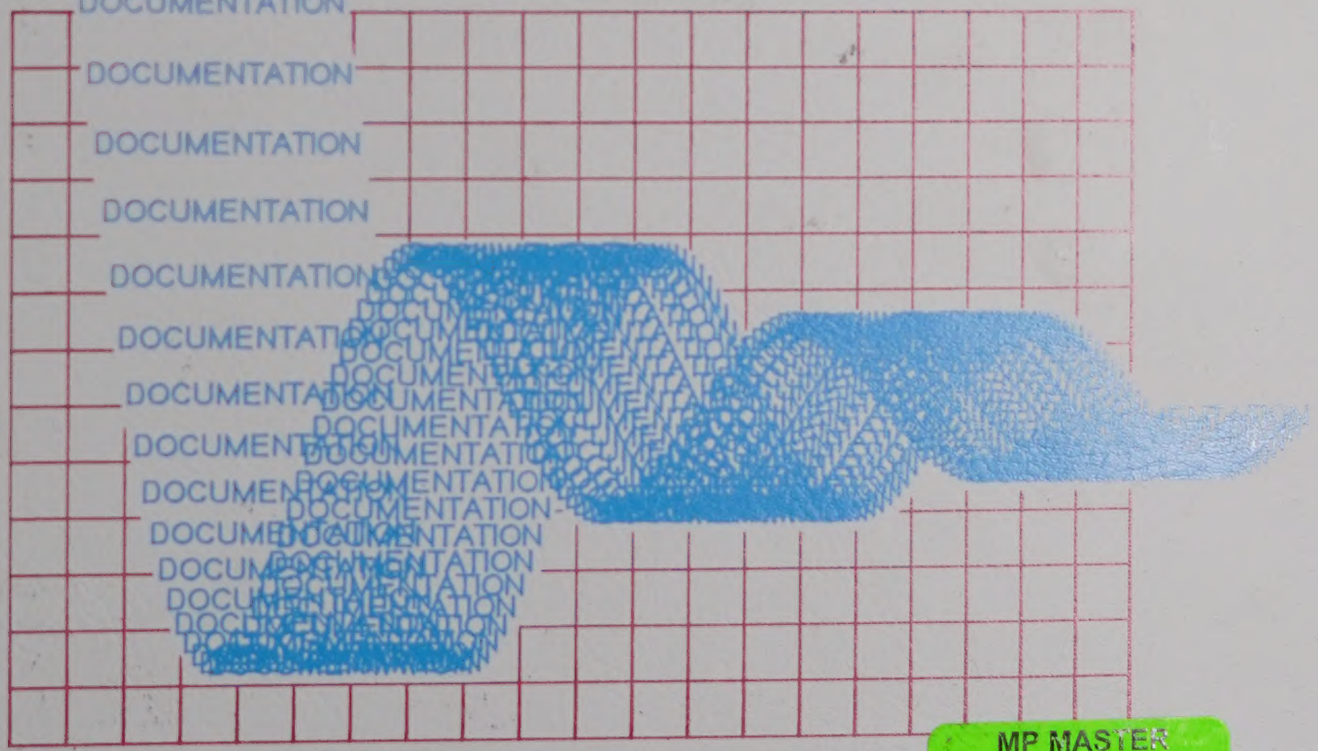

MP MASTER
MA34482

ROHDE&SCHWARZ

Test and Measurement
Division

Operating Manual

SPECTRUM ANALYZER

FSP3
1093.4495.03

FSP7
1093.4495.07

FSP13
1093.4495.13

FSP30

1093.4495.30

Printed in the Federal
Republic of Germany

bbed

Table of Contents

1
2
3
5
6
7
8
9
10

Tabbed Divider Overview

Contents

Data Sheet

Safety Instructions
Certificate of Quality
EU Certificate of Conformity
List of R&S Representatives

Manuals for Spectrum Analyzer FSP

Tabbed Divider

1	Chapter 1:	Putting into Operation
2	Chapter 2:	Getting Started
3	Chapter 3:	Operation
4	Chapter 4:	Functional Description
5	Chapter 5:	Remote Control – Basics
6	Chapter 6:	Remote Control – Commands
7	Chapter 7:	Remote Control – Program Examples
8	Chapter 8:	Maintenance and Hardware Interfaces
9	Chapter 9:	Error Messages
10	Index	

Digitized by the Internet Archive
in 2026

https://archive.org/details/manualsplus_12270

Spectrum Analyzer FSP

The new medium-class standard

Features

- 21 cm TFT colour display
- 1 Hz to 10 MHz RBW
- RMS detector for fast and reproducible measurements on digitally modulated signals
- Measurement routines for TOI, ACPR, OBW, amplitude statistics
- EMI bandwidths and quasi-peak detector

Speed

- 2.5 ms minimum sweep time in frequency domain
- 1 µs sweep time in time domain
- Up to 30 GPIB measurements/s in frequency domain (incl. trace transfer)
- Up to 70 GPIB measurements/s in time domain (including trace transfer)
- Fast ACP measurement routine in time domain

Performance

- Total measurement uncertainty: 0.5 dB
- Displayed average noise level: –155 dBm/Hz
- Phase noise: –113 dBc/Hz at 10 kHz
- Dynamic range of RMS detector: 100 dB
- Synthesized frequency setting

ROHDE&SCHWARZ

The new Spectrum Analyzers FSP from Rohde & Schwarz...

- Unparalleled range of functions
- Highest measurement speed
- Maximum in precision

With the new FSP family, the well-known advantages of high-end Analyzers FSE and FSIQ have been systematically integrated into the medium class of analyzers. FSP sets the standard for the medium class regarding the vital criteria of functionality, measurement speed and accuracy. The use of innovative techniques such as an highly integrated front-end and fully digital signal processing in the back-end, together with ASICs developed by Rohde & Schwarz, has resulted in a product of top-class specifications and high reliability.

...the new medium class standard

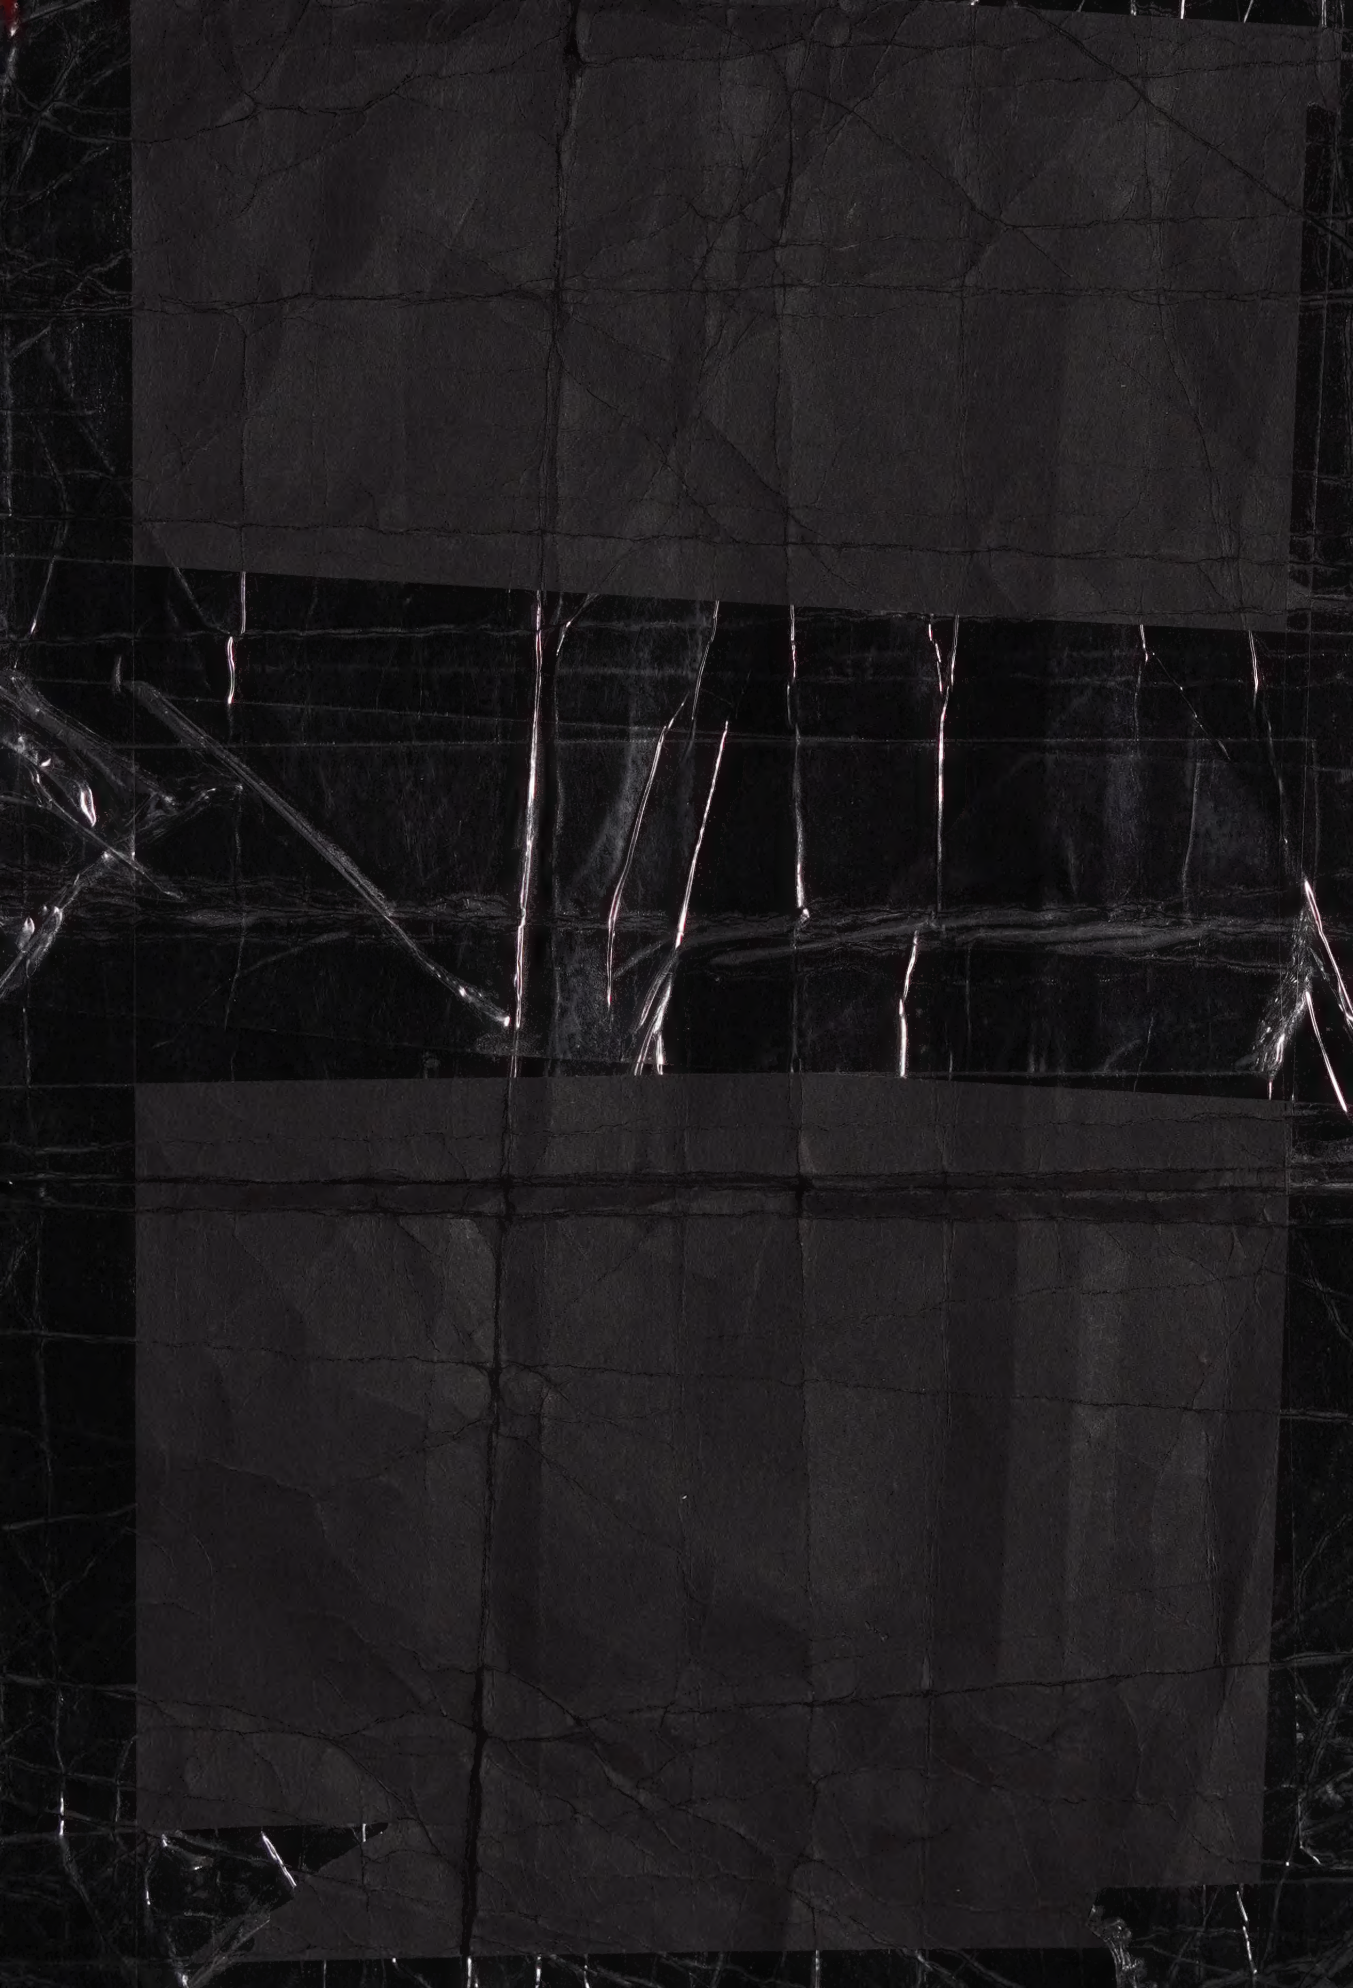

A wealth of functions...

The FSP option list is short – all important functions and interfaces are implemented as standard. FSP features future-oriented characteristics such as an RMS detector and a CCDF routine for fast statistical measurements on digitally modulated signals not offered by any other medium-class spectrum analyzer.

Function / Option	Standard	Option
Highly selective digital filters from 10 Hz to 100 kHz	●	
Fast FFT filters from 1 Hz to 30 kHz	●	
QP detector & EMI bandwidths 200 Hz, 9 kHz, 120 kHz	●	
2.5 ms sweep time in frequency domain	●	
1 µs sweep time in time domain	●	
Time-selective spectrum analysis with gating	●	
GPIB interface, IEEE 488.2	●	
RS232C serial interface, 9-pin sub-D	●	
VGA output, 15-pin sub-D	●	
PC-compatible screen shots on floppy disk or hard disk	●	
Measurement speed manually up to 20 measurements/s	●	
Measurement speed GPIB up to 30 measurements/s	●	
SCPI-compatible GPIB command set	●	
FSE/FSIQ-compatible GPIB command set	●	
Fast ACP measurements in time domain	●	
CCDF measurement functions	●	
RMS detector with 100 dB dynamic range	●	
2-year calibration interval	●	
3-year warranty	●	
Cabinet for portable use	–	B1
AM/FM audio demodulator	–	B3
OCXO reference frequency	–	B4
Tracking generator	–	B9
External generator control	–	B10
LAN interface	–	B16
Electronic attenuator	–	B25

...the new standard in the medium class

The new standard in the medium class...

Features

The new FSP Spectrum Analyzers from Rohde & Schwarz are outstanding for their innovative measurements and a host of standard functions.

Instead of a wide choice of options, FSP offers as standard all the functions and interfaces you may expect from a state-of-the-art spectrum analyzer:

- Largest colour display in its class
- Resolution bandwidths from 1 Hz to 10 MHz
- Highly selective digital filters and FFT
- Quasi-peak detector and EMI bandwidths
- Convenient documentation of results as a hardcopy or file in PC-compatible formats
- Interfaces: GPIB, Centronics, RS232, LAN (option)
- Automatic test routines for measuring TOI, OBW, phase noise and ACP (R)
- Split screen with separate settings and up to 3 traces per screen
- Editable limit lines including PASS/FAIL indication
- Fast measurements in the time domain : minimum sweep time 1 µs
- Gated sweep for measurements on TDMA signals

On top of this, FSP features as standard the following unique attributes:

- RMS detector for fast and reproducible power measurements on digitally modulated signals in frequency and time domain
- Statistical measurement functions for determining crest factor and CCDF (complementary cumulative distribution function)

Featuring such a wealth of functions, FSP offers state-of-the-art spectrum analysis at an extremely attractive price-performance ratio.

Speed

Time is a finite resource – so high measurement speed is indispensable for competitiveness and cost-effective testing.

Here, too, the new FSP offers characteristics that make it top of the class:

- Up to 30 measurements/s on GPIB interface including trace transfer of 501 binary data
- 70 measurements/s on GPIB interface in zero span mode including trace transfer of 501 binary data
- Minimum sweep time of 2.5 ms

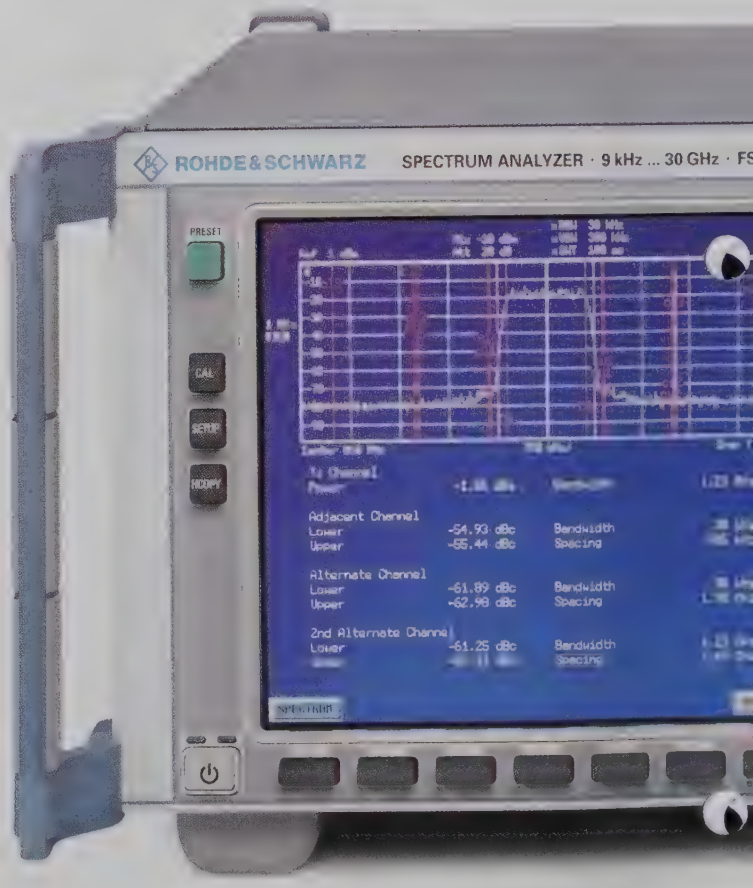

- 1 µs time domain measurements
- Unique fast ACP mode for high-speed ACPR measurements in time domain using the standard-stipulated test filters

With 30 measurements/s in manual operation and digital filters with sweep time 2.5 times faster than comparable analog filters, FSP will also help in your day-to-day work to develop your product much faster.

Performance

Modern communication systems are required to achieve optimum spectral efficiency at high data rates. For the 3rd generation of CDMA mobile radio systems currently under development this is achieved, among other things, by high-precision power control.

FSP is the ideal partner in development and production, featuring small level measurement uncertainty, as well as excellent RF characteristics:

- 0.5 dB total measurement uncertainty allows higher tolerances for the DUT, thus increasing production yield
- 0.07 dB linearity uncertainty (1 σ) is ideal for precise measurements, for example of gain control and ACPR
- RMS detector with >100 dB dynamic range measures power fast and accurately irrespective of the signal shape – almost like a thermal power sensor
- The displayed average noise level of typ. –155 dBm (1 Hz) is attained without the use of preamplifiers and thus without any reduction in dynamic range
- Typ. –145 dBc (1 Hz) phase noise at 10 MHz offset offers optimum conditions for ACPR measurements on WCDMA systems

Resolution bandwidths of up to 100 kHz are fully digital and provide – in addition to high selectivity – an ideal basis for accurate (adjacent-) channel power measurements thanks to a maximum bandwidth deviation of 3%.

. . . with high-end characteristics

High-end characteristics...

Rohde&Schwarz ASICs

Top-class performance as offered by FSP essentially depends on the extensive use of digital signal processing and large-scale integration of components.

For these demanding tasks, Rohde&Schwarz has developed ASICs tailored to the requirements of signal analysis. Key functions such as

- RMS detection,
- digital IF filtering,
- logarithmation,
- CCDF measurement

are "cast into silicon" and are thus faster than conventional solutions.

Logarithmic amplifier

FSP is equipped as standard with digital resolution filters between 10 Hz and 100 kHz of high selectivity and very small bandwidth error. The filters have an extremely small logarithmic level deviation of <0.2 dB in the range 0 dB to –70 dB. They are implemented as ASIC functions, so their great precision is attained without any reduction in measurement speed.

furnishes 10^6 single values in only 250 ms, thus enabling extremely accurate statistical analysis even of rarely occurring signal peaks.

This analysis function, which is becoming more and more important, has been realized for the first time in Spectrum Analyzer FSP as a fast and cost-effective solution based on ASICs.

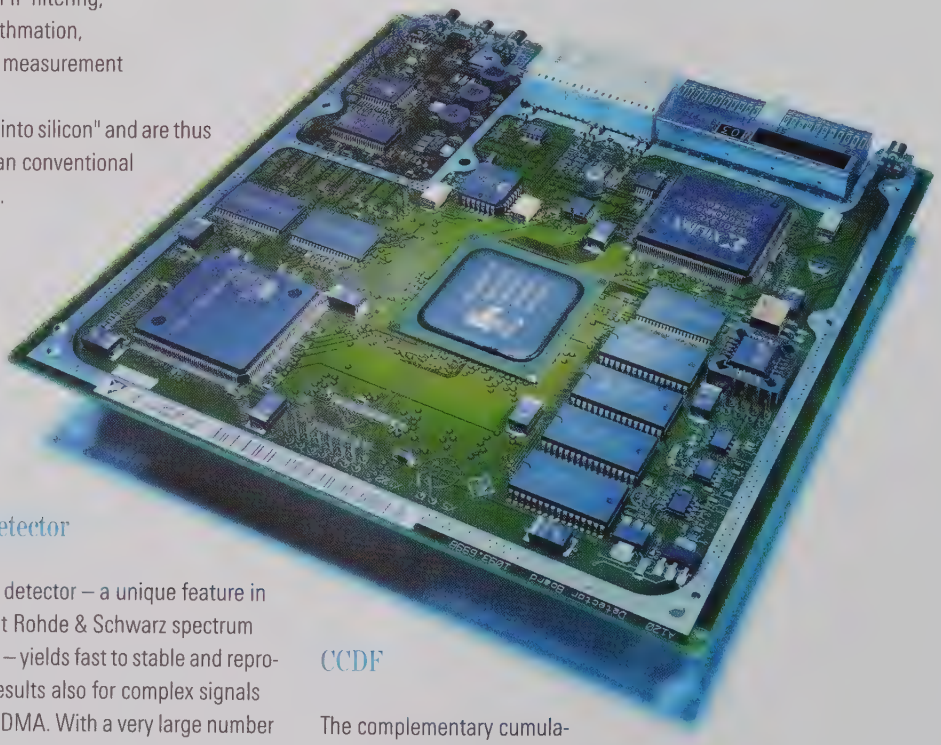

RMS detector

The RMS detector – a unique feature in all current Rohde & Schwarz spectrum analyzers – yields fast to stable and reproducible results also for complex signals such as CDMA. With a very large number of linear single measurements performed, followed by power integration, the detector avoids the measurement error inherent in conventional analyzers which results from the averaging of the log video signal. The RMS detector of the FSP spectrum analyzer measures all modern communication signals with an accuracy and speed unparalleled so far.

CCDF

The complementary cumulative distribution function, or briefly CCDF, describes the probability of a signal power exceeding a specific (usually the average) power. CCDF analysis is indispensable for determining the optimal transmitting power for CDMA signals assuming that clipping over known, short intervals is tolerable. FSP with its dedicated CCDF measurement routine

The platform

Excellent technical data like those of FSP require a high-grade and service-friendly platform. All the modules are optimally shielded and easy to exchange, and are accommodated in a lightweight but stable frame. A low-noise powerful fan in conjunction with low power consumption of 70 VA to 150 VA (depending on model) makes for high reliability.

A 2-year calibration interval (excluding the reference frequency) and a 3-year warranty worldwide are offered with the FSP.

Fit for the future

Thanks to its modular design, FSP is optimally equipped to cope with all present and future tasks. The design takes into account both hardware and firmware extensions to safeguard your investment far into the future. So you can rely on your FSP to meet all requirements also in the years to come.

Ergonomics & design

FSP sets the ergonomic standard in this class of analyzers. The 21 cm (8.4") colour display is the largest and most brilliant in its category. Vertical and horizontal rows of softkeys allow the convenient handling even of complex measurement tasks. Parameters like frequency and amplitude are entered by means of dedicated hardkeys and unit keys.

...through innovative solutions

Innovative solutions...

Optimum dynamic range

Featuring the lowest displayed average noise level in its class (DANL <–145 dBm at 10 Hz RBW), FSP measures even small signals accurately without the use of preamplifiers whilst maintaining the full dynamic range. Together with the high intercept point this yields an intermodulation-free range of typically 100 dB – again a record in the medium class of analyzers.

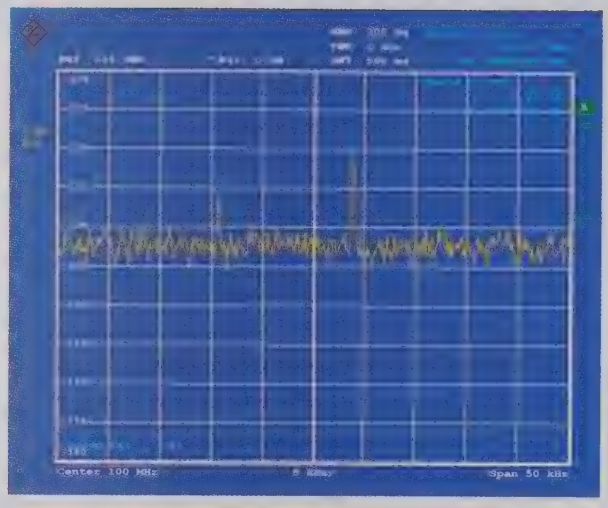

Ultralow measurement uncertainty

In the vital frequency range below 3 GHz, FSP is outstanding for its ultra-low measurement uncertainty. The total measurement uncertainty is less than 0.5 dB. Due to this excellent value, the use of power meters in routine lab applications very often becomes superfluous and DUTs may be allowed greater tolerances.

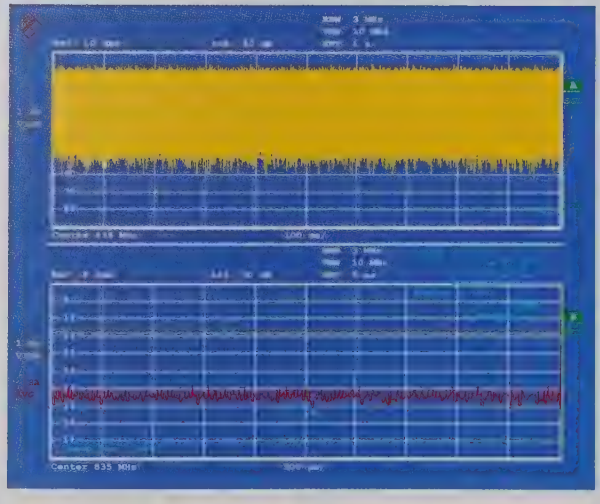

RMS detector

The unique RMS detector used in spectrum analyzers from Rohde&Schwarz measures modern, noise-like communication signals with best repeat accuracy and stability.

There are neither correction factors nor the typical errors caused by averaging of logarithmic trace data, so the correct average power is displayed with high stability for all signal types – almost like in measurements with a thermal power meter.

Phase noise

The low phase noise of FSP makes it suitable for demanding measurement tasks both in the vicinity of the carrier (typ. –113 dBc (1 Hz) at 10 kHz) and far from the carrier (typ. –125 dBc (1 Hz) at 1 MHz). FSP is thus optimally equipped for performing spectral analysis and ACPR measurements on narrowband systems like IS-136 or PDC as well as on wideband systems like IS-95 or WCDMA.

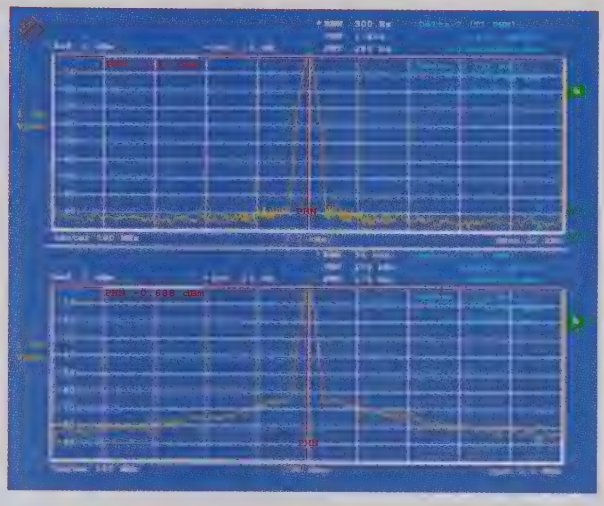

Phase noise measurement with FSP

CCDF analysis

FSP is the first spectrum analyzer to offer statistical analysis of signals by means of the complementary cumulative distribution function (CCDF) as standard and at an impressively high speed. FSP furnishes in only 250 ms the exact CCDF characteristic, average and peak power as well as the crest factor over 1 million measured values.

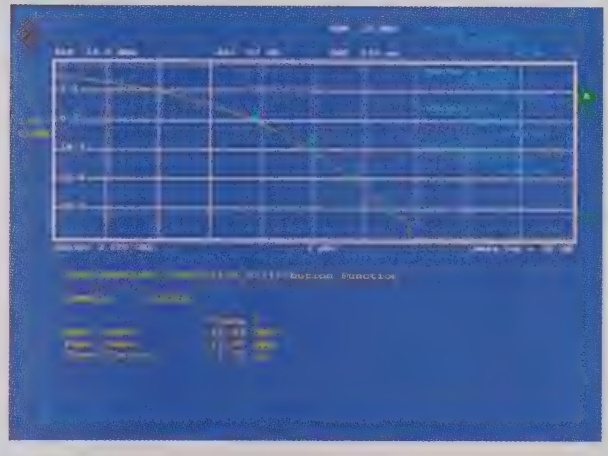

CCDF of wideband CDMA signal

ACPR measurements

Adjacent-channel power ratio (ACPR) measurements, which many mobile radio standards stipulate for components and units, are implemented in FSP by means of automatic test routines. All settings, measurements and filters required for a selected standard are activated at a keystroke. In addition to a large number of preprogrammed standards, the channel width and channel spacing can be individually selected. Thanks to the excellent dynamic range, lowest phase noise in its class and the RMS detector, FSP sets the standard in the medium class also for ACPR measurements.

(Adjacent-) channel measurement on wideband CDMA signal

...for research & development

Innovative solutions...

High measurement speed

With 30 measurements/s in manual operation, minimum sweep time of 2.5 ms and 1 µs zero span as a standard, FSP is ideal for time-critical applications. The highly selective, fast-sweeping digital filters featuring "analog" response allow measurements on pulsed signals as well as the use of the built-in frequency counter.

FSP comes standard with different filter types for digital resolution bandwidths up to 100 kHz such as Gaussian filter, raised root cosine (RRC) filter and steep-sided channel filters. Up to a resolution bandwidth of 30 kHz fast Fourier transform (FFT) is available in addition. In the analyzer mode, the Gaussian filters have the advantage of high sweep speed plus excellent resolution. At high span/RBW ratios, measurements using FFT can be as much as 300 times faster than measurements with digital filters. Some mobile radio standards such as TETRA and IS-136 require RRC filters for power measurement, this type of filter already being included in FSP. In addition, FSP provides channel filters for other analog and digital methods, e.g. cdmaOne, AM/FM radio and ETS 300 113. Adjacent-channel power due to switching can also be measured using the channel filters.
For the common mobile radio standards, FSP is equipped with test routines that allow the adjacent-channel power in the time domain to be determined, which reduces measurement time and increases reproducibility.

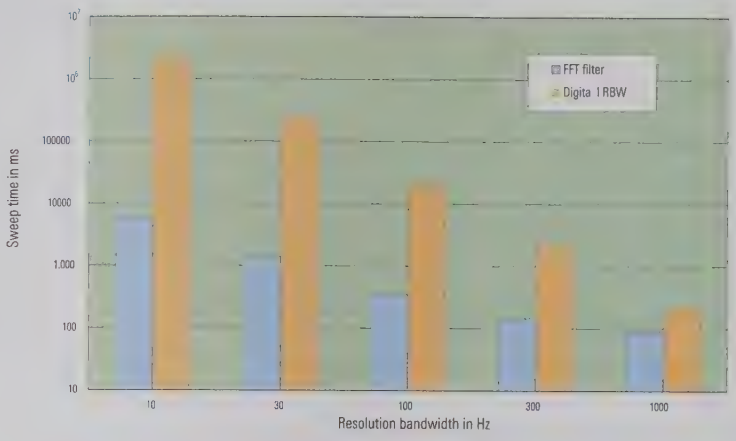

Comparison of sweep times for 200 kHz span using digital filters or FFT

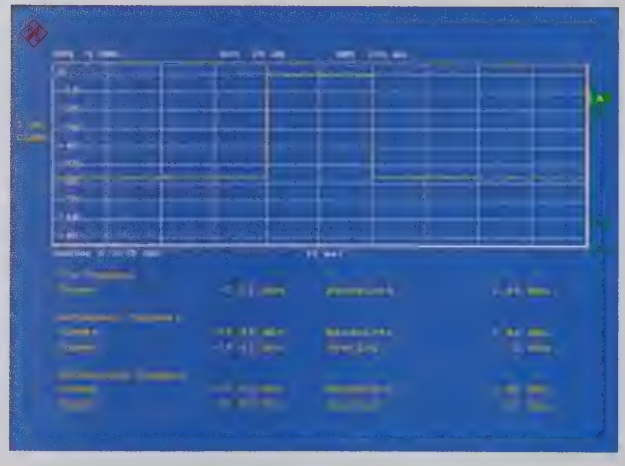

Measurement of adjacent-channel power in time domain: FAST ACP

30 measurements per second on GPIB interface

The standard high-speed GPIB interface enables up to 30 measurements per second including trace data transfer of 501 test points with the display switched off.

	Sweeps/s Span 10 MHz, sweep time 2.5 ms	Sweeps/s Span 0 Hz, sweep time 100 µs
ASCII format	25	40
Binary IEEE754 format	30	70

Measurement speed on GPIB interface

Settings:display off, default coupling, single trace, 501 points

In the zero span mode, 70 measurements/s are possible. This characteristic makes FSP by far the fastest spectrum analyzer on the GPIB interface. Valuable time can be saved in production and the throughput boosted enormously. FSP thus supports you in getting your products more cost-effective on the market.

0.5 dB total measurement uncertainty

Measurement uncertainty can be split into the contribution from the instrument and that introduced by the test setup. With a smaller uncertainty of the spectrum analyzer, greater tolerances can be allowed for the test setup. If the small uncertainty of the analyzer is utilized to allow for higher DUT tolerances, the result will be a marked reduction of manufacturing rejects – an advantage that pays off immediately. With a total measurement uncertainty of 0.5 dB, FSP undisputedly ranks top way ahead of other medium class analyzers.

0.2 dB maximum linearity uncertainty

All modern mobile radio systems achieve high spectral efficiency through precise control of transmitter output power, among other measures. The correct functioning of gain control, which may be as much as –70 dB depending on the system, is checked against the nominal value in a large number of individual measurements. Featuring a maximum linearity uncertainty of only 0.2 dB and fast power measurement routines especially for digitally modulated signals, FSP is the ideal choice wherever the reduction of the test time and the number of rejects is of primary importance.

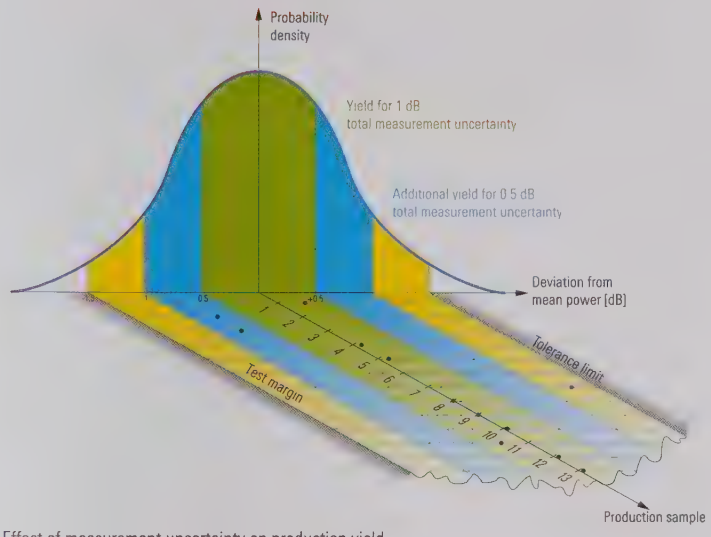
Probability density
Yield for 1 dB total measurement uncertainty
Additional yield for 0.5 dB total measurement uncertainty
Deviation from mean power [dB]
Tolerance limit
Test margin
Production sample

Effect of measurement uncertainty on production yield

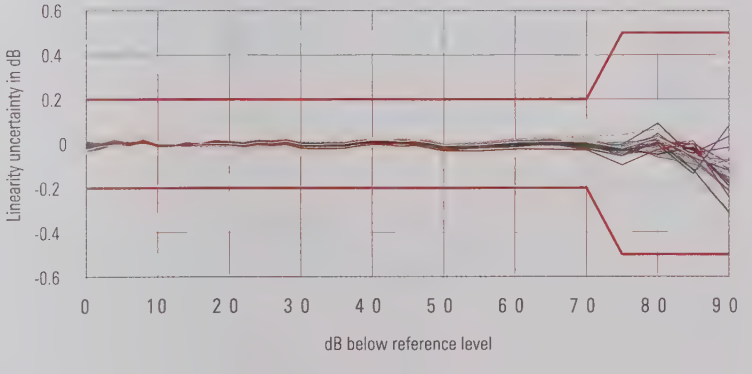

Display linearity with ≤100 kHz resolution bandwidth (measurement on 30 units)

...for production

Innovative solutions...

Measurement routines TOI, OBW

FSP offers fast routines for a multitude of typical measurement tasks, which make result postprocessing superfluous by supplying the desired data directly:

- Determination of TOI
- Occupied bandwidth (OBW)
- Burst power with peak, average and RMS indication as well as standard deviation
- Modulation depth of AM signals
- Phase noise
- Bandwidth marker

Of course these functions can also be used via the fast GPIB interface.

Environmental compatibility

- Fast and easy disassembly
- Small number of materials
- Compatibility of materials
- Easy identification of substances through appropriate marking (plastics)
- Recycling of enclosure

DESIGN AWARD WINNER 1998
INDUSTRIE FORUM DESIGN HANNOVER

Certified Environmental System
ISO 14001
REG. NO. 1231-03

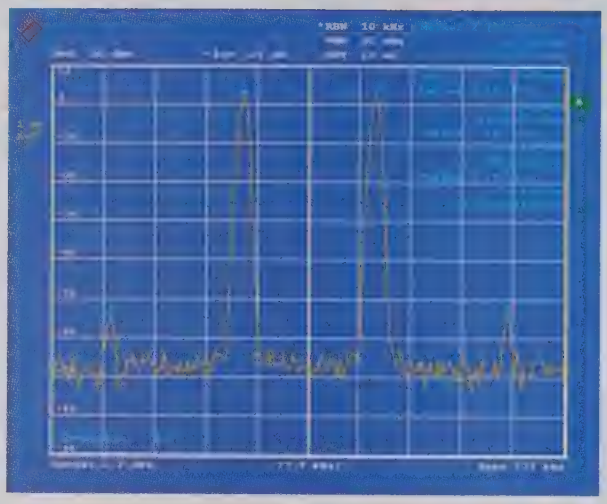

Measurement of TOI

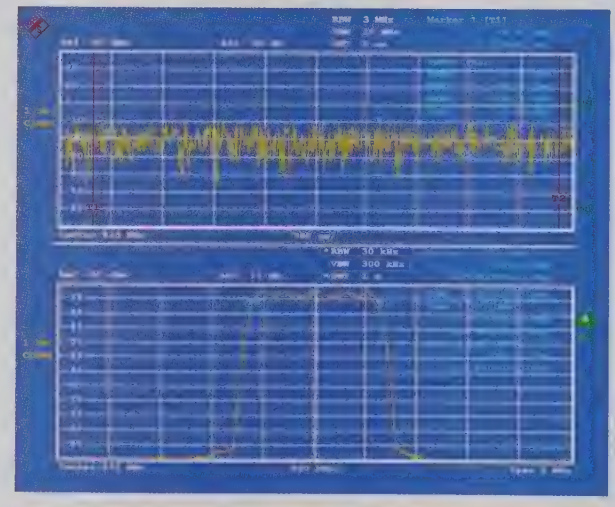

Measurement of burst power (top)

Determination of occupied bandwidth (OBW) (bottom)

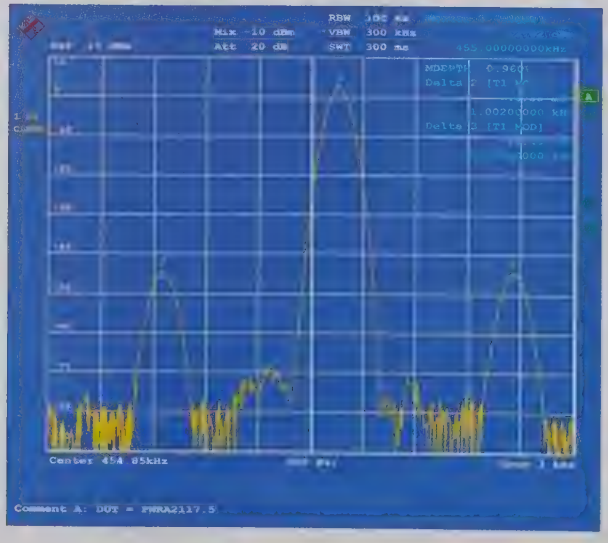

Measurement of modulation depth of AM signal

Electronic attenuator for high production throughput

The optional Electronic Attenuator **FSP-B25** supplements the standard mechanical attenuator and provides a wear-and-tear-free setting range of 30 dB in 5 dB steps. The option does away with frequent switching of the mechanical attenuator as called for in high production throughput and so increases the availability and reliability of the measurement facility. The limit of 10^7 switching operations, which is typical of mechanical attenuators, means a breakdown after approx. 6 months already at 1.5 switching operations/s whereas Electronic Attenuator FSP-B25 can be switched any number of times without degrading the specifications.

The integrated switchable 20 dB preamplifier allows high-sensitivity measurements in the useful frequency range from 10 MHz to 7000 MHz.

LAN interface

With the aid of the optional LAN Interface **FSP-B16**, FSP can be connected to common networks such as 100Base-T so that functions like file logging on network drives or documentation of measurement results via network printer are available. In addition, FSP can be remote-controlled via LAN. This yields a clear speed advantage over the IEC/IEEE bus in particular for the transmission of large data blocks.

Noise measurements

Thanks to its excellent display linearity, FSP is especially suited for noise measurements. With the aid of the optional Noise Measurement Software **FS-K3**, FSP can be enhanced to a noise test system offering analyzer-specific advantages (see data sheet PD 757.2380)

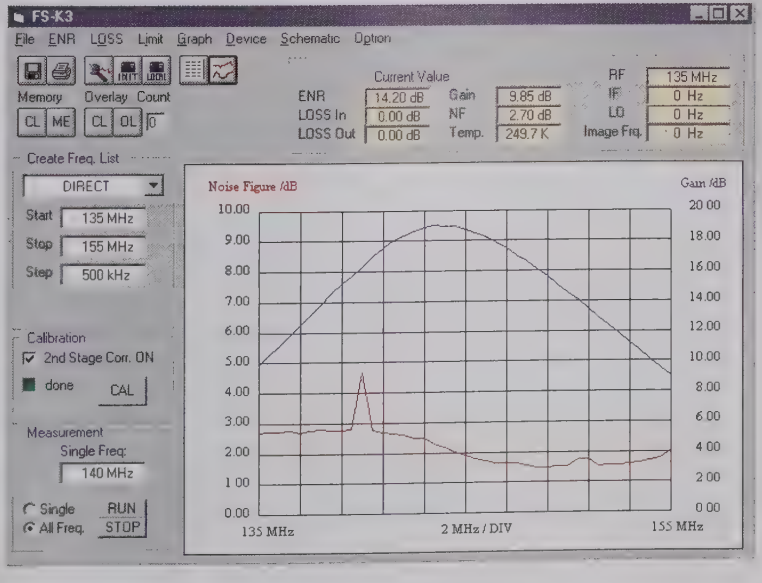

Measurement of noise figure using Noise Measurement Software FS-K3

GSM/EDGE measurements

The Application Firmware **FS-K5** allows the user to perform the most important GSM and EDGE transmitter measurements with the push of a button:

- Phase/frequency error (GSM)
- Modulation accuracy (EDGE) including 95:th percentile and origin offset suppression
- Power-versus-time
- Carrier power
- Modulation spectrum
- Transient spectrum
- Spurious emissions

Phase noise measurements

Phase Noise Measurement Software **FS-K4** extends the measurement capabilities of Rohde & Schwarz Spectrum Analyzer FSP to give a phase noise tester. FSP is ideal for this purpose because of its low inherent phase noise and noise figure. High measurement speed is achieved through the high sweep rates of FSP. It is possible to trade off speed against accuracy at small resolution band-widths (≤1kHz) by using either FFT or digital filters. FSE-K4 allows for different settings in one phase noise graph, eg FFT close and analog/digital filters far off the carrier.

...for production

Innovative solutions...

Scalar network analysis in wide dynamic range and at any frequency offset

The optional Internal Tracking Generator **FSP-B9** up to 3 GHz and External Generator Control FSP-B10 extend the FSP spectrum analyzers to scalar network analyzer functionality. The gain, frequency response, insertion and return loss are measured using a selective method in a wide dynamic range without any influence from the harmonics or spurious of the generator. Internal Tracking Generator FSP-B9 can be used in any FSP models and covers the frequency range from 9 kHz to 3 GHz.
A frequency offset of ±150 MHz can be set for measurements on frequency-converting modules. The tracking generator can be broadband-modulated by an external IQ baseband signal.

Option **FSP-B10** uses commercial RF signal generators as its external tracking source that can be controlled via the GPIB or a TTL bus. With this option the functionality of the internal tracking generator can be utilized:

- Normalization with interpolation also for reflection measurements with open and short
- Automatic bandwidth measurement with "n dB down" function
- Tolerance lines with PASS/FAIL verdict

Option **FSP-B6** makes the Spectrum Analyzers FSP suitable for analog TV measurement applications and provides a settable RF level trigger for measurements on pulsed RF signals that are used in TDMA transmission systems.

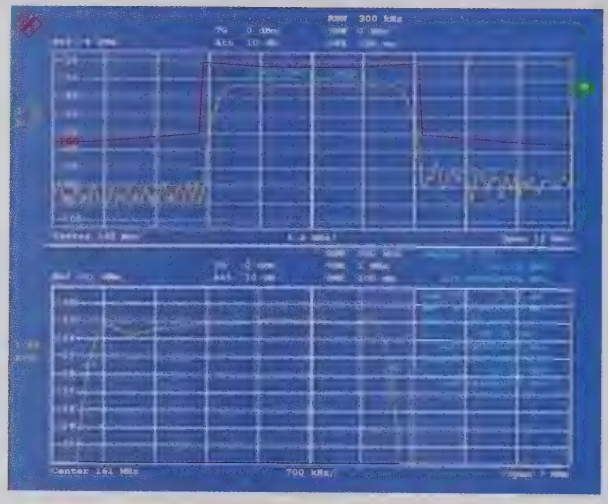

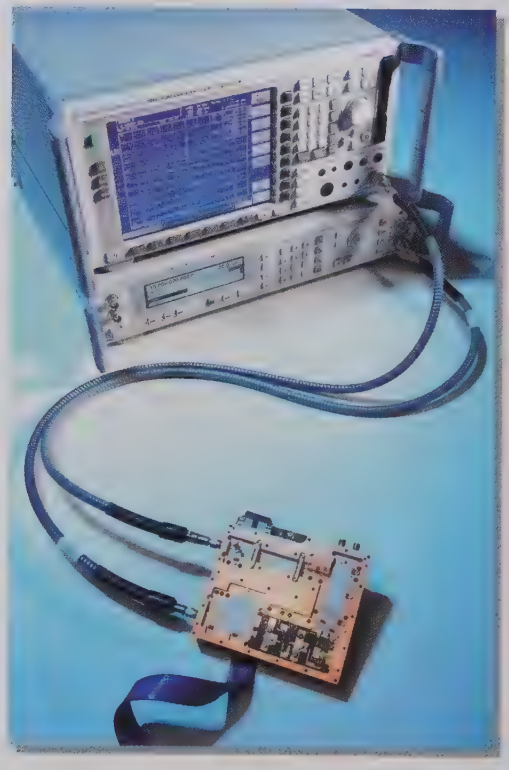

...through custom-made options

Complete measurement solutions...

Open for the PC world.

- PC-compatible screen shots, no conversion software needed
- Windows™ printer support
- LabWindows driver
- LabView driver
- SCPI-compatible
- FSE/FSIQ-compatible GPIB command set
- GPIB command set with search function on CD-ROM
- Customized training
- Solution-oriented consulting
- Application notes
- 3-year warranty
- 2-year calibration cycle

...and much more

...no guessing games

Specifications

Specifications are guaranteed under the following conditions:
15 minutes warm-up time at ambient temperature, specified environmental conditions met, calibration cycle adhered to, and total calibration performed.
Data without tolerances: typical values only.
Data designated "nominal" apply to design parameters and are not tested.
Data designated "σ = xx dB" are shown as standard deviation.

	FSP3	FSP7	FSP13	FSP30
Frequency				
Frequency range	9 kHz to 3 GHz	9 kHz to 7 GHz	9 kHz to 13.6 GHz	9 kHz to 30 GHz
Frequency resolution	0.01 Hz			
Internal reference frequency (nominal)				
Aging per year [1]	1×10^{-6}			
Temperature drift	1×10^{-6}			
with option FSP-B4 (OCXO)				
Aging per year [1]	1×10^{-7}			
Temperature drift	1×10^{-8}			
External reference frequency	10 MHz			
Frequency display	with marker or frequency counter			
Marker resolution	span/500			
Max. deviation (sweep time >3 x auto sweep time)	± (frequency x reference frequency + 0.5% x span + 10% x resolution bandwidth + ½ (last digit))			
Frequency counter resolution	0.1 Hz to 10 kHz (selectable)			
Count accuracy (S/N >25 dB)	±(frequency x reference frequency + ½ (last digit))			
Frequency span	0 Hz, 10 Hz to 3 GHz	0 Hz, 10 Hz to 7 GHz	0 Hz, 10 Hz to 13.6 GHz	0 Hz, 10 Hz to 30 GHz
Max. span deviation	0.1%			
Spectral purity (dBc (1 Hz)) SSB phase noise, f = 500 MHz, for f > 500 MHz see diagrams				
Carrier offset				
100 Hz	<–84, typ. –90			
1 kHz	<–100, typ. –108			
10 kHz	<–106, typ. –113			
100 kHz [2]	<–110, typ. –113			
1 MHz [2]	<–120, typ. –125			
10 MHz	typ. –145			
Residual FM				
f = 500 MHz, RBW 1 kHz, sweep time 100 ms	typ. 3 Hz			

[1] After 30 days of operation.
[2] Valid for span >100 kHz.

Typical values for SSB phase noise (referred to 1 Hz bandwidth):

Offset	f_{in} = 3 GHz	f_{in} = 7 GHz	f_{in} = 13 GHz	f_{in} = 22 GHz	f_{in} = 26 GHz
100 Hz	–74 dBc	–67 dBc	–61 dBc	–57 dBc	–55 dBc
1 kHz	–100 dBc	–94 dBc	–88 dBc	–84 dBc	–82 dBc
10 kHz	–108 dBc	–104 dBc	–98 dBc	–94 dBc	–92 dBc
100 kHz	–108 dBc	–106 dBc	–100 dBc	–96 dBc	–94 dBc
1 MHz	–118 dBc	–118 dBc	–112 dBc	–108 dBc	–106 dBc

SSB phase noise vs offset

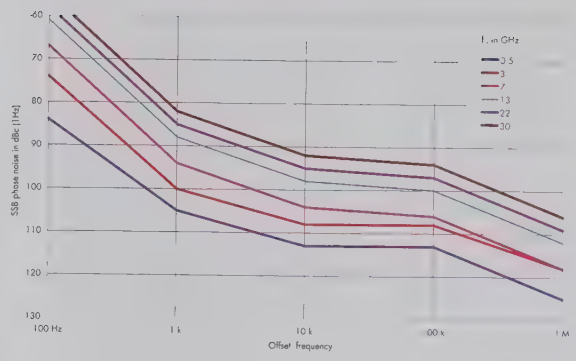

SSB phase noise vs frequency

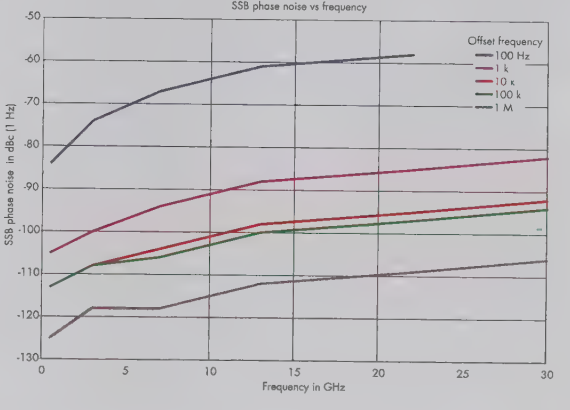

	FSP 3	FSP 7	FSP13	FSP30
Sweep time				
Span ≥10 Hz	2.5 ms to 16000 s			
Max. deviation	1%			
Span 0 Hz	1 µs to 16000 s			
Resolution	125 ns			
Resolution bandwidths				
Bandwidths	10 Hz to 10 MHz (–3 dB) in 1, 3 sequence			
EMI bandwidths	200 Hz, 9 kHz, 120 kHz (–6 dB)			
Bandwidth accuracy				
≤100 kHz	<3%			
300 kHz to 3 MHz	<10%			
10 MHz	+10%, –30%			
Shape factor –60 dB: –3 dB				
≤100 kHz	<5:1 (Gaussian filters)			
300 kHz to 3 MHz	<15:1 (4-pole synchronously tuned filters)			
10 MHz	<7:1			
Shape factor –60 dB: –6 dB				
EMI bandwidths	<5:1			
Video bandwidths	1 Hz to 10 MHz in 1, 3 sequence			
FFT filter				
Bandwidths	1 Hz to 30 kHz (– 3 dB) in 1, 3 sequence			
Bandwidth accuracy	5%, nominal			
Shape factor –60 dB:–3 dB	2.5:1 nominal			

	FSP 3	FSP 7	FSP13	FSP30
Level				
Display range	displayed average noise level to 30 dBm			
Maximum input level				
DC voltage	50 V		0 V	
RF attenuation 0 dB				
CW RF power	20 dBm			
Pulse spectral density	97 dBµV (1 MHz)			
RF attenuation ≥10 dB				
CW RF power	30 dBm			
Max. pulse voltage	150 V		50 V	
Max. pulse energy (10 µs)	1 mWs		0.5 mWs	
1 dB compression of input mixer				
0 dB RF attenuation, f>200 MHz	0 dBm nominal			
Intermodulation				
3rd-order intermodulation				
Intermodulation-free dynamic range, level 2 x –30 dBm, Δf > 5 x RBW or 10 kHz, whichever the greater value				
20 MHz to 200 MHz	>70 dBc, TOI >5 dBm			
200 MHz to 3 GHz	>74 dBc, TOI >7 dBm (typ. 10 dBm)			
3 GHz to 7 GHz	–	>80 dBc, TOI >10 dBm (typ. 15 dBm)		
7 GHz to 20 GHz	–	–	>80 dBc, TOI >10 dBm	
20 GHz to 30 GHz	–	–	–	>76 dBc, TOI >8 dBm
with optional Electronic Attenuator FSP-B25 switched on				
20 MHz to 200 MHz	>74 dBc, TOI >7 dBm		–	
200 MHz to 3 GHz	>80 dBc, TOI >10 dBm		–	
3 GHz to 7 GHz	>84 dBc, TOI >12 dBm		–	
Second harmonic intercept point (SHI)				
Frequency				
<100 MHz	>25 dBm			
100 MHz to 3 GHz	>35 dBm			
3 GHz to 7 GHz	–	>45 dBm		
7 GHz to 13.6 GHz	–	–	typ. 45 dBm	
13.6 GHz to 30 GHz	–	–	–	typ. 45 dBm
Displayed average noise level				
(0 dB RF attenuation, RBW 10 Hz, VBW 1 Hz, 20 averages, trace average, span 0 Hz, termination 50 Ω)				
Frequency				
9 kHz	<–95 dBm			
100 kHz	<–100 dBm			
1 MHz	<–120 dBm, typ. –125 dBm			
10 MHz to 1 GHz	<–142 dBm, typ. –145 dBm	<–140 dBm, typ. –145 dBm		
1 GHz to 3 GHz	<–140 dBm, typ. –145 dBm	<–138 dBm, typ. –143 dBm		
3 GHz to 7 GHz	–	<–138 dBm, typ. –143 dBm	<–135 dBm, typ. –145 dBm	
7 GHz to 13.6 GHz	–	–	<–132 dBm, typ. –138 dBm	
13.6 GHz to 22 GHz	–	–	–	<–120 dBm, typ. –130 dBm
22 GHz to 30 GHz	–	–	–	<–115 dBm, typ. –123 dBm
Displayed average noise level with preamplifier on (option FSP-B25)				
10 MHz to 2 GHz	<–152 dBm	–		
2 GHz to 7 GHz	<–150 dBm	–		

	FSP 3	FSP 7	FSP13	FSP30
Immunity to interference				
Image frequency	>70 dB			
Intermediate frequency (f <3 GHz)	>70 dB			
Spurious responses (f >1 MHz, without input signal, 0 dB attenuation)	<–103 dBm			
Other spurious (with input signal, mixer level <–10 dBm, Δf >100 kHz)	f <7 GHz: <–70 dBc f <13.6 GHz: <–64 dBc f <30 GHz: <–56 dBc			
Level display				
Screen	501 × 400 pixels (one diagram), max. 2 diagrams with independent settings			
Log level scale	10 dB to 200 dB, in steps of 10 dB			
Linear level scale	10% of reference level per level division, (10 divisions)			
Traces	max. 3, with two diagrams on screen max. 3 per diagram			
Trace detector	Max Peak, Min Peak, Auto Peak, Sample, Quasi-Peak, Average, RMS			
Trace functions	Clear/Write, Max. Hold, Min Hold, Average			
Setting range of reference level				
Logarithmic level display	–130 dBm to 30 dBm, in steps of 0.1 dB			
Linear level display	70.71 nV to 7.07 V in steps of 1%			
Units of level scale	dBm, dBmV, dBµV, dBµA, dBpW (log level display), mV, µV, mA, µA, pW, nW (linear level display)			
Max. uncertainty of level measurement				
at 128 MHz, –30 dBm (RF attenuation 10 dB, RBW 10 kHz, ref. level –20 dBm)	<0.2 dB (σ = 0.07 dB)			
Frequency response				
<50 kHz	<+0.5/– 1.0 dB			
50 kHz to 3 GHz	< 0.5 dB (σ = 0.17 dB)			
3 GHz to 7 GHz	–	<2 dB (σ = 0.7 dB)		
7 GHz to 13.6 GHz	–	–	<2.5 dB [1]	
13.6 GHz to 30 GHz	–	–	–	<3 dB [1]
Frequency response with preamplifier, electronic attenuator option FSP-B25 switched on				
10 MHz to 3 GHz	<1 dB (σ = 0.33 dB)		–	
3 GHz to 7 GHz	–	<2 dB (σ = 0.7 dB)	–	
Attenuator	<0.2 dB (σ = 0.07 dB)			
Reference level switching	<0.2 dB (σ = 0.07 dB)			
Display nonlinearity LOG/LIN (S/N >16 dB)				
RBW ≤100 kHz				
0 dB to –70 dB	<0.2 dB (σ = 0.07 dB)			
–70 dB to –90 dB	<0.5 dB (σ = 0.17 dB)			
RBW ≥300 kHz				
0 dB to –50 dB	<0.2 dB (σ = 0.07 dB)			
–50 dB to –70 dB	<0.5 dB (σ = 0.17 dB)			
Bandwidth switching uncertainty (ref. to RBW = 10 kHz)				
10 Hz to 100 kHz	<0.1 dB (σ = 0.03 dB)			
300 kHz to 10 MHz	<0.2 dB (σ = 0.07 dB)			
1 Hz to 3 kHz, FFT	<0.2 dB (σ = 0.03 dB)			
Total measurement uncertainty				
0 GHz to 3 GHz	0.5 dB			

[1] RF attenuation 10 dB, sweep time >1 s/1 GHz

	FSP 3	FSP 7	FSP13	FSP30
Trigger functions				
Trigger				
Span ≥10 Hz				
Trigger source	free run, video, external, IF level			
Trigger offset	125 ns to 100 s, resolution 125 ns min. (or 1% of offset)			
Span = 0 Hz				
Trigger source	free run, video, external, IF level			
Trigger offset	±125 ns to 100 s, resolution 125 ns min., dependent on sweep time			
Max. deviation of trigger offset	±(125 ns + (0.1% x delay time))			
Gated sweep				
Trigger source	external, IF level, video			
Gate delay	1 µs to 100 s			
Gate length	125 ns to 100 s, resolution min. 125 ns or 1% of gate length			
Max. deviation of gate length	±(125 ns + (0.05% x gate length))			
Inputs and outputs (front panel)				
RF input	N female, 50 Ω			test port system 50 Ω, N female, 3.5 mm female[1]
VSWR (RF attenuation >0 dB)				
f <3 GHz	1.5:1			
f <7 GHz	–	2.0:1		
f <13 GHz	–	–	2.5:1	
f <30 GHz	–	–	–	3.0:1
Input attenuator	0 dB to 70 dB in 10 dB steps			
With option FSP-B25	0 dB to 75 dB in 5 dB steps		not available	
Probe power supply	+15 V DC, –12.6 V DC and ground, max. 150 mA			
Keyboard connector	PS/2 female for MF2 keyboard			
AF output (only with option FSP-B3)	3.5 mm mini jack			
Output impedance	10 Ω			
Open-circuit voltage	up to 1.5 V, adjustable			
Inputs and outputs (rear panel)				
IF 20.4 MHz	Z_{out} = 50 Ω, BNC female			
Level				
RBW ≤100 kHz, FFT	–10 dBm at reference level, mixer level >–60 dBm			
RBW ≥300 kHz	0 dBm at reference level, mixer level >–60 dBm			
Reference frequency				
Output	BNC female			
Output frequency	10 MHz			
Level	0 dBm nominal			
Input	10 MHz			
Required level	0 dBm from 50 Ω			
Others				
Power supply for noise source	BNC female, 0 V and 28 V, switchable, max. 100 mA			
External trigger/gate input	BNC female, >10 kΩ			
Trigger voltage	1.4 V			

	FSP 3	FSP 7	FSP13	FSP30
IEC/IEEE-bus remote control	interface to IEC 625-2 (IEEE 488.2)			
Command set	SCPI 1997.0			
Connector	24-pin Amphenol female			
Interface functions	SH1, AH1, T6, L4, SR1, RL1, PP1, DC1, DT1, C0			
Serial interface	RS 232 C (COM), 9-pin sub-D connector			
Printer interface	parallel (Centronics-compatible)			
Mouse connector	PS/2 female			
Connector for ext. monitor (VGA)	15-pin sub-D connector			
General data				
Display	21 cm TFT colour display (8.4")			
Resolution	640 x 480 pixels (VGA resolution)			
Pixel failure rate	$<2 \times 10^{-5}$			
Mass memory	1.44 Mbyte 3 ½" disk drive (built-in), hard disk			
Data storage	>500 instrument settings and traces			
Temperatures				
Rated temperature range	+ 5 °C to +40 °C			
Limit temperature range	+ 5 °C to +45 °C			
Storage temperature range	–40 °C to +70 °C			
Damp heat	+40 °C at 95% relative humidity (IEC 68–2–3)			
Mechanical resistance				
Vibration test, sinusoidal	5 Hz to 150 Hz, max. 2 g at 55 Hz; 0.5 g from 55 Hz to 150 Hz; meets IEC 68-2-6, IEC 68-2-3, IEC 1010-1, MIL-T-28800D, class 5			
Vibration test, random	10 Hz to 100 Hz, acceleration 1 g (rms)			
Shock test	40 g shock spectrum, meets MIL-STD-810C and MIL-T-28800D, classes 3 and 5			
Recommended calibration interval	2 years for operation with external reference, 1 year with internal reference			
Power supply				
AC supply	100 V AC to 240 V AC, 50 Hz to 400 Hz, 3.1 A to 1.3 A, class of protection I to VDE 411			
Typical power consumption	70 VA	120 VA	150 VA	
Safety	meets EN 61010-1, UL 3111-1, CSA C22.2 No. 1010-1, IEC 1010-1			
RFI suppression	meets EMC Directive of EU (89/336/EEC) and German EMC law			
Test mark	VDE, GS, CSA, CSA-NRTL/C			
Dimensions in mm (W x H x D)	412 x 197 x 417			
Weight	10.5 kg	11.3 kg	12 kg	

[1] See recommended extras for alternate connectors

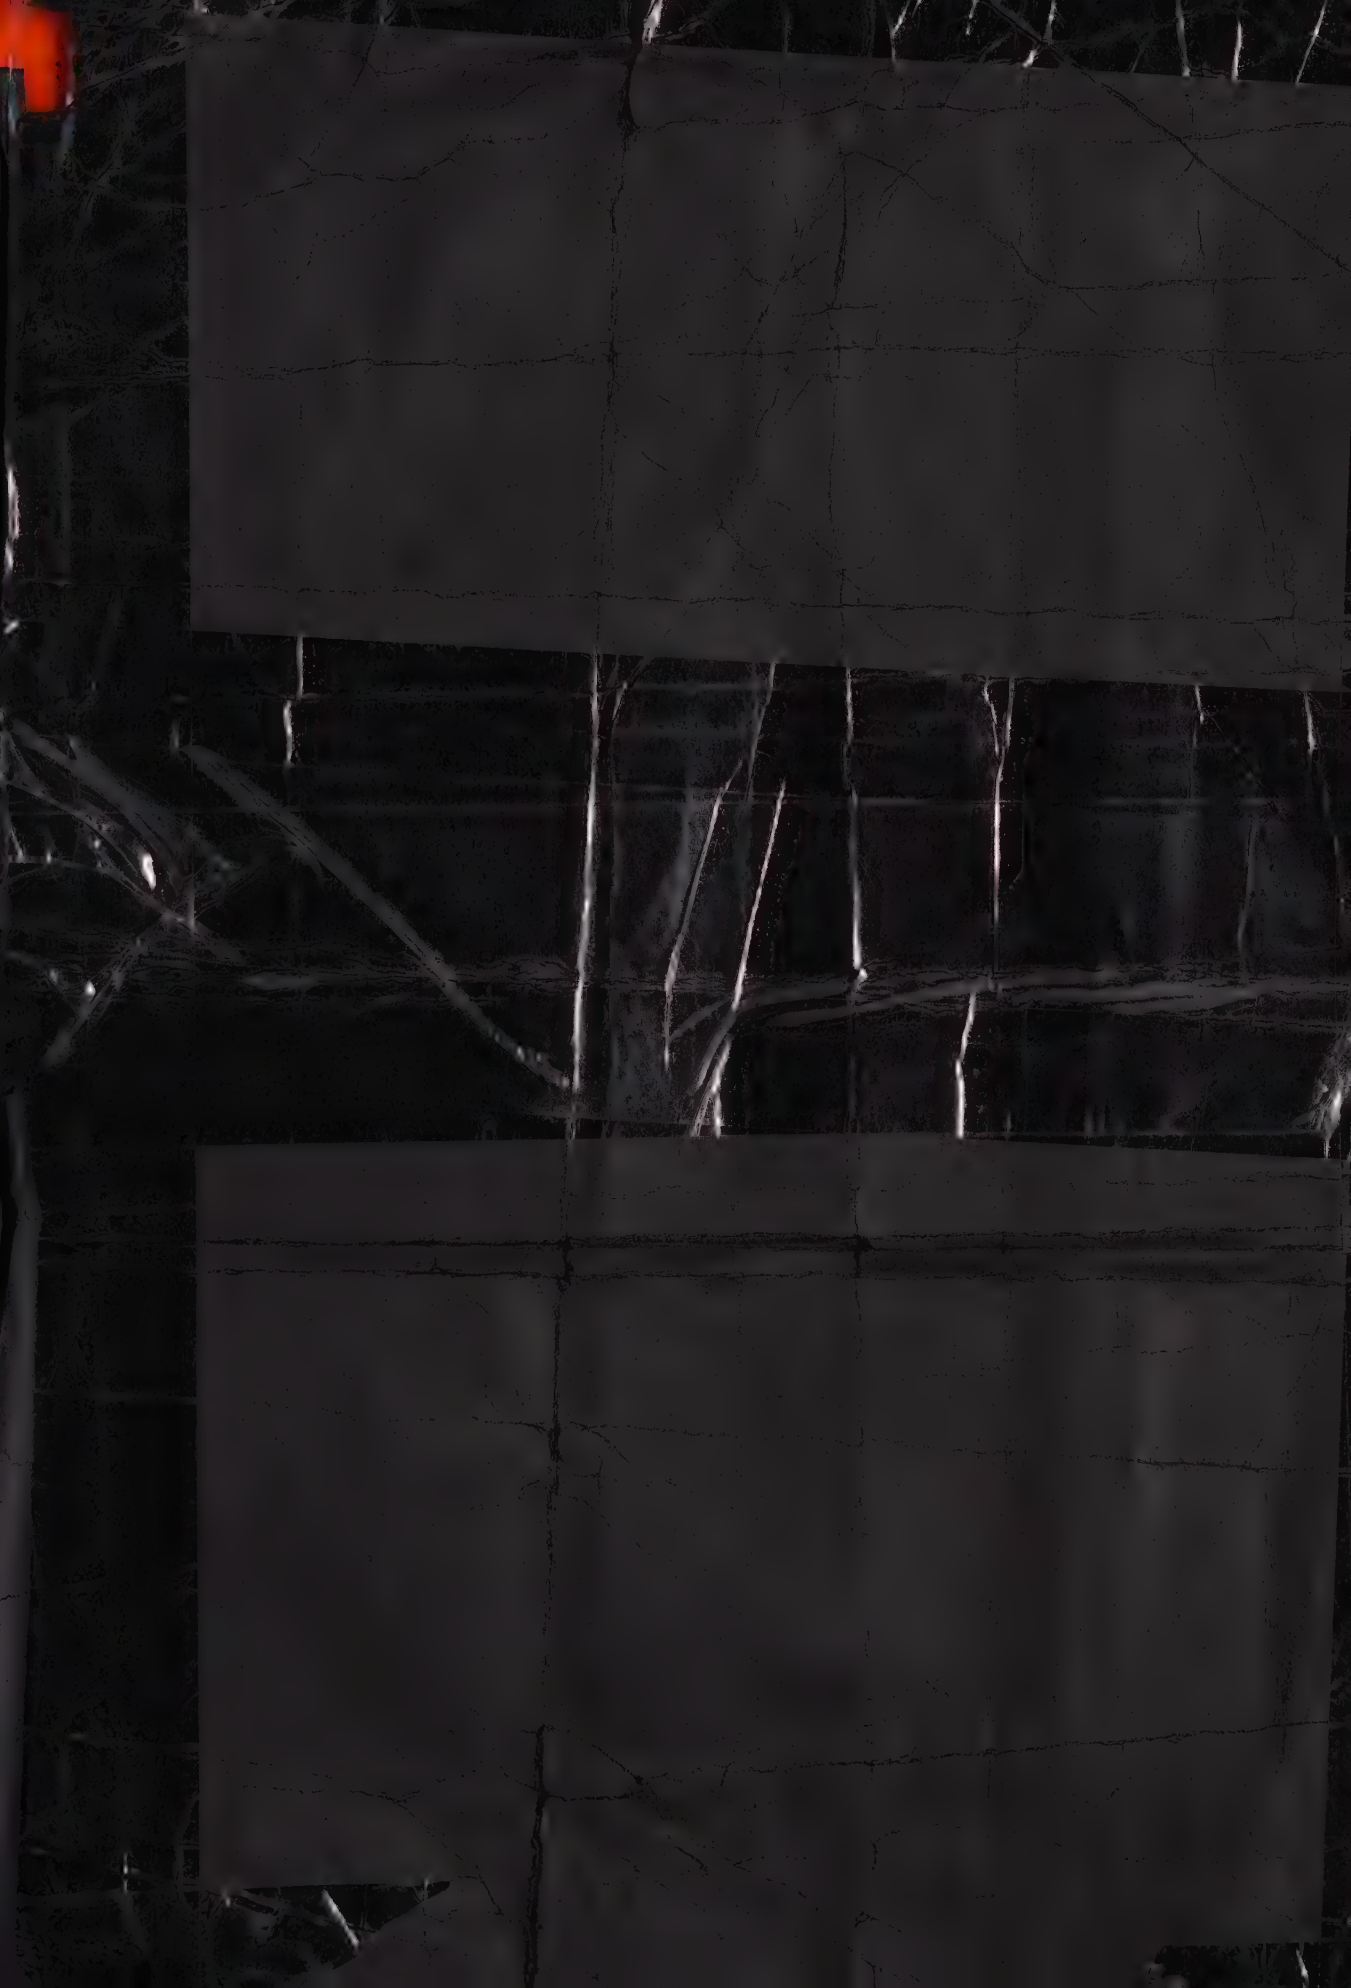

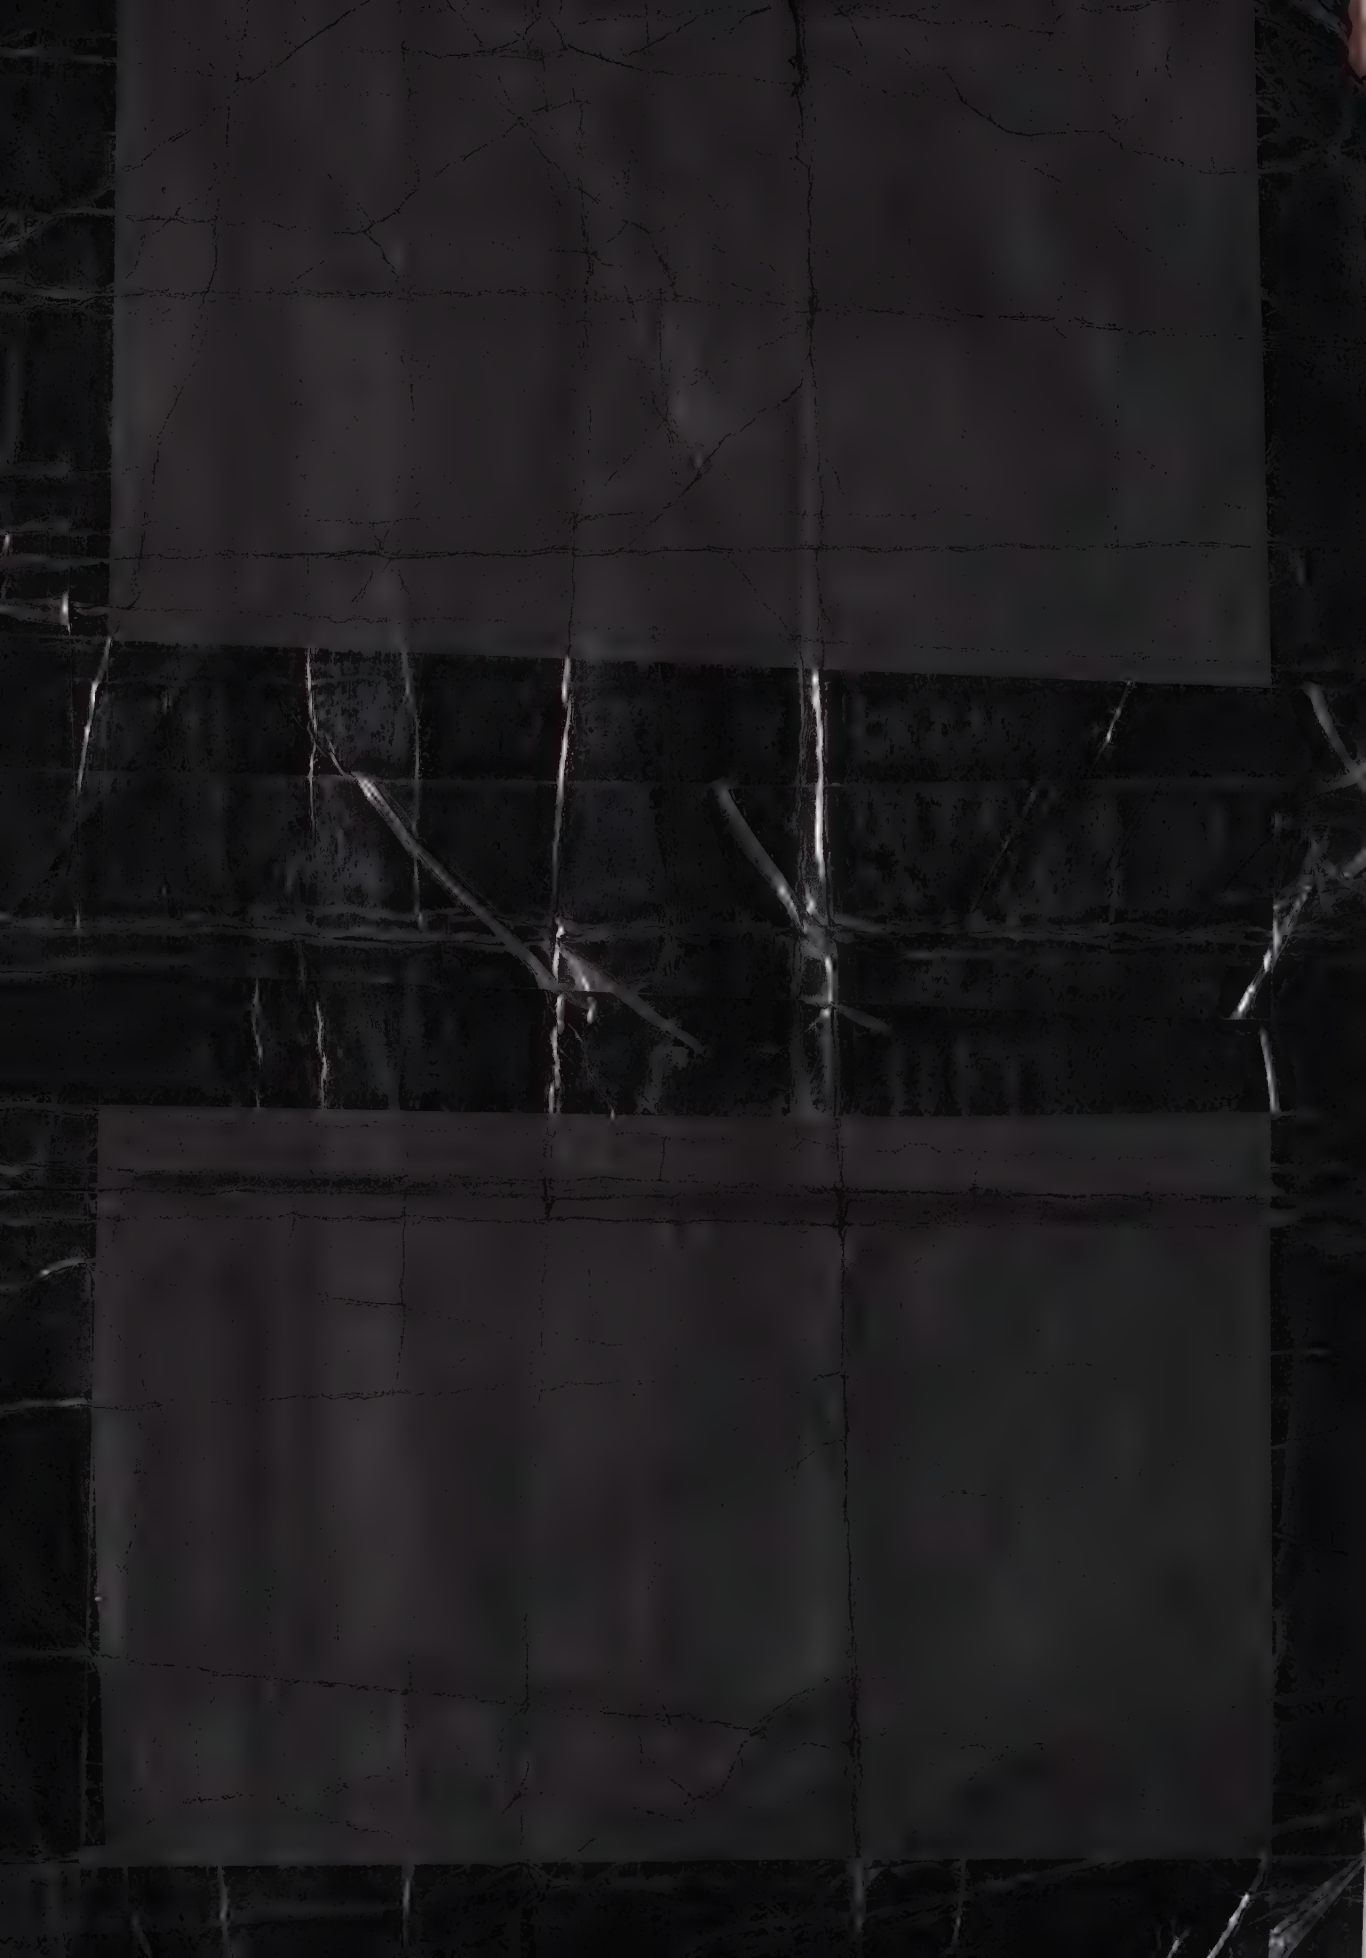

Specifications of options

Tracking Generator FSP-B9

Unless specified otherwise, specifications not valid for frequency range from –3 x RBW to +3 x RBW, however at least not valid from –9 kHz to +9 kHz.[1]

Frequency	
Frequency range	9 kHz to 3000 MHz
Frequency offset	
Setting range	±150 MHz
Resolution	1 Hz
Spectral purity (dBc (1 Hz)) SSB phase noise, f = 500 MHz, carrier offset 100 kHz	
Normal mode	typ. –90
With FM modulation on	typ. –70
Level	
Level range	–30 dBm to 0 dBm in steps of 0.1 dB
Level range with AM	–30 dBm to –6 dBm in steps of 0.1 dB
Max. deviation of output level, 128 MHz, 0 dBm	<1 dB
Frequency response	
Output level 0 dBm, 100 kHz to 2 GHz	<1 dB
Output level 0 dBm to –25 dBm, 9 kHz to 3 GHz	<3 dB
Dynamic range	
Attenuation measurement range, RBW = 1 kHz, f >10 MHz	120 dB
Spurious	
Harmonics, output level –10 dBm	typ. –30 dBc
Nonharmonics, output level 0 dBm	typ. –30 dBc

Modulation

Modulation format (external)	I/Q, AM, FM, FM-DC, PM, ASK, FSK
AM, f >10 MHz	
Modulation depth	0% to 99%
Modulation frequency range	0 Hz to 1 MHz
FM, f >10 MHz	
Frequency deviation	0 Hz to 20 MHz
Modulation frequency range	0 Hz to 100 kHz
I/Q modulation, f >10 MHz	
0 Hz to 30 MHz	typ. 1 dB
Inputs and outputs (front panel)	
RF output	N female, 50 Ω
VSWR	typ. 2:1
Inputs and outputs (rear panel)	
TG/AM In	$V_{max(pp)}$=1 V; Z_{in} = 50 Ω, BNC female
TG Q/FM In	$V_{max(pp)}$=1 V; Z_{in} = 50 Ω, BNC female

External Generator Control FSP-B10

Supported signal generators	SME02/03/06, SMG, SMGL, SMGU, SMH, SMHU, SMIQ 02B/02E/03B/03E/04B/06B SML01, SMR 20/27/30/40 SMP 02/22/03/04, SMX SMT 02/03/06

LAN Interface FSP-B16

Connector (rear panel)	RJ-45
Supported protocols	10Base-T (IEEE standard 10 Mbit/s 802.3) 100Base-Tx (IEEE standard 100 Mbit/s 802.3u)

Electronic Attenuator FSP-B25 (only for FSP3 and FSP7)

Frequency	
Frequency range	10 MHz to 7000 MHz
Input attenuator range (mechanical)	0 dB to 75 dB in 5 dB steps
Electronic attenuation range	0 dB to 30 dB in 5 dB steps
Preamplifier	20 dB, switchable
Displayed average noise level with preamplifier on (0 dB RF attenuation, RBW 10 Hz, VBW 1 Hz, 20 averages, trace average, span 0 Hz, termination 50 Ω)	
10 MHz to 2 GHz	<–152 dBm
2 GHz to 7 GHz	<–150 dBm
Intermodulation with electronic attenuator on	
3rd-order intermodulation, intermodulation-free dynamic range, level 2 x –30 dBm, Δf >5 x RBW or 10 kHz, whichever the greater value	
20 MHz to 200 MHz	>74 dBc, TOI >7 dBm
200 MHz to 3 GHz	>80 dBc, TOI >10 dBm
3 GHz to 7 GHz	>84 dBc, TOI >12 dBm
Max. deviation of level measurement	
128 MHz, –30 dBm (RF attenuation 10 dB, RBW 10 kHz, ref. level –20 dBm), preamplifier ON	<0.2 dB (σ = 0.07 dB)
Electronic attenuator	<0.2 dB (σ = 0.07 dB)
Frequency response with preamplifier, electronic attenuator	
10 MHz to 3 GHz	<1.0 dB (σ = 0.33 dB)
3 GHz to 7 GHz	<2 dB (σ = 0.7 dB)

[1] The specified level accuracy is valid for an RF attenuation of at least 20 dB or for sweep times of min. 100 ms (FSP3, FSP7) or 1000 ms (FSP13, FSP30).

Ordering information

Order designation	Type	Order No.
Spectrum Analyzer 9 kHz to 3 GHz	FSP 3	1093.4495.03
Spectrum Analyzer 9 kHz to 7 GHz	FSP 7	1093.4495.07
Spectrum Analyzer 9 kHz to 13.6 GHz	FSP13	1093.4495.13
Spectrum Analyzer 9 kHz to 30 GHz	FSP30	1093.4495.30

Accessories supplied

Power cable, operating manual, service manual
FSP30: test port adapter 3.5 mm female (1021.0512.00) and N female (1021.0535.00)

Options

Order designation	Type	Order No.
Delete Manuals	FSP-B0	1129.8394.02
Rugged case, carrying handle (factory-fitted)	FSP-B1	1129.7998.02
AM/FM Audio Demodulator	FSP-B3	1129.6491.02
TV Trigger/RF Power Trigger	FSP-B6	1129.859.4.02
OCXO Reference Frequency	FSP-B4	1129.6740.02
Internal tracking Generator 9 kHz to 3 GHz, IQ modulator, for all FSP models	FSP-B9	1129.6991.02
External Generator Control for all FSP models	FSP-B10	1129.7246.02
LAN Interface 100BT for all FSP models	FSP-B16	1129.8042.02
Electronic Attenuator, 0 dB to 30 dB, 5 dB steps, integrated preamplifier for FSP3 and FSP7	FSP-B25	1129.7746.02
Software		
Noise Measurement Software	FS-K3	1057.3028.02
Phase Noise Measurement Software	FS-K4	1108.0088.02
GSM/EDGE Application Firmware, Mobile	FS-K5	1141.1496.02
AM/FM Measurement Demodulator	FS-K7	1141.1796.02

Recommended extras

Order designation	Type	Order No.
Headphones		0708.9010.00
US Keyboard with trackball	PSP-Z2	1091.4100.02
PS/2 Mouse	FSE-Z2	1084.7043.02
Colour Monitor, 15", 230 V	PMC3	1082.6004.02
IEC/IEEE-Bus Cable, 1 m	PCK	0292.2013.10
IEC/IEEE-Bus Cable, 2 m	PCK	0292.2013.20
19" Rack Adapter (not for FSP-B1)	ZZA 478	1096.3248.00
Trolley	ZZK-1	1014.0510.00
Soft carrying case, grey	ZZT473	1109.5048.00
Matching Pads, 75 Ω		
L Section	RAM	0358.5414.02
Series Resistor, 25 Ω *)	RAZ	0358.5714.02
SWR Bridge, 5 MHz to 3000 MHz	ZRB2	0373.9017.52
SWR Bridge, 40 kHz to 4 GHz	ZRC	1039.9492.52
High-Power Attenuators, 100 W		
3/6/10/20/30 dB	RBU 100	1073.8820.XX (XX=03/06/10/20/30)
High-Power Attenuators, 50 W		
3/6/10/20/30 dB	RBU 50	1073.8895.XX (XX=03/06/10/20/30)
For FSP30		
Test port Adapter, 3.5 mm male	–	1021.0529.00
Test port Adapter, N male	–	1021.0541.00

*) Taken into account in device function RF INPUT 75 Ω.

Related data sheets

TV Trigger/RF Power Trigger FSP-B6	PD 757.6433
Noise Measurement Software FS-K3 for Spectrum Analyzers FSE,FSIQ and FSP	PD 757.2380
Phase Noise Measurement Software FSE-K4	PD 757.4201
GGSM/EDGE Application Firmware FS-K5 for FSP	PD 757.6185

Certified Quality System
ISO 9001
DQS REG. NO 1954-04

ROHDE&SCHWARZ

ROHDE&SCHWARZ GmbH & Co. KG · Mühldorfstraße 15 · D-81671 München · Germany · P.O.B. 80 14 69 · D-81614 München · Germany · Telephone +49 89 41 29-0
www.rohde-schwarz.com · CustomerSupport: Tel. +49 1805 12 42 42, Fax +49 89 41 29-13777, E-mail: CustomerSupport@rohde-schwarz.com

Safety Instructions

This unit has been designed and tested in accordance with the EC Certificate of Conformity and has left the manufacturer's plant in a condition fully complying with safety standards.

To maintain this condition and to ensure safe operation, the user must observe all instructions and warnings given in this operating manual.

Safety-related symbols used on equipment and documentation from R&S:

Observe operating instructions

Weight indication for units >18 kg

PE terminal

Ground terminal

Danger! Shock hazard

Warning! Hot surfaces

Ground

Attention! Electrostatic sensitive devices require special care

1. The unit may be used only in the operating conditions and positions specified by the manufacturer. Unless otherwise agreed, the following applies to R&S products:

   IP degree of protection 2X, pollution severity 2 overvoltage category 2, only for indoor use, altitude max. 2000 m.

   The unit may be operated only from supply networks fused with max. 16 A.

   Unless specified otherwise in the data sheet, a tolerance of ±10% shall apply to the nominal voltage and of ±5% to the nominal frequency.

2. For measurements in circuits with voltages V_{rms} > 30 V, suitable measures should be taken to avoid any hazards.

   (using, for example, appropriate measuring equipment, fusing, current limiting, electrical separation, insulation).

3. If the unit is to be permanently wired, the PE terminal of the unit must first be connected to the PE conductor on site before any other connections are made. Installation and cabling of the unit to be performed only by qualified technical personnel.

4. For permanently installed units without built-in fuses, circuit breakers or similar protective devices, the supply circuit must be fused such as to provide suitable protection for the users and equipment.

5. Prior to switching on the unit, it must be ensured that the nominal voltage set on the unit matches the nominal voltage of the AC supply network.

   If a different voltage is to be set, the power fuse of the unit may have to be changed accordingly.

6. Units of protection class I with disconnectible AC supply cable and appliance connector may be operated only from a power socket with earthing contact and with the PE conductor connected.

7. It is not permissible to interrupt the PE conductor intentionally, neither in the incoming cable nor on the unit itself as this may cause the unit to become electrically hazardous.

   Any extension lines or multiple socket outlets used must be checked for compliance with relevant safety standards at regular intervals.

8. If the unit has no power switch for disconnection from the AC supply, the plug of the connecting cable is regarded as the disconnecting device. In such cases it must be ensured that the power plug is easily reachable and accessible at all times (length of connecting cable approx. 2 m). Functional or electronic switches are not suitable for providing disconnection from the AC supply.

   If units without power switches are integrated in racks or systems, a disconnecting device must be provided at system level.

9. Applicable local or national safety regulations and rules for the prevention of accidents must be observed in all work performed.

   Prior to performing any work on the unit or opening the unit, the latter must be disconnected from the supply network.

   Any adjustments, replacements of parts, maintenance or repair may be carried out only by authorized R&S technical personnel.

   Only original parts may be used for replacing parts relevant to safety (eg power switches, power transformers, fuses). A safety test must be performed after each replacement of parts relevant to safety.

   (visual inspection, PE conductor test, insulation-resistance, leakage-current measurement, functional test).

continued overleaf

10. Ensure that the connections with information technology equipment comply with IEC950 / EN60950.
11. Lithium batteries must not be exposed to high temperatures or fire.

    Keep batteries away from children.

    If the battery is replaced improperly, there is danger of explosion. Only replace the battery by R&S type (see spare part list).

    Lithium batteries are suitable for environmentally-friendly disposal or specialized recycling. Dispose them into appropriate containers, only.

    Do not short-circuit the battery.
12. Equipment returned or sent in for repair must be packed in the original packing or in packing with electrostatic and mechanical protection.
13. Electrostatics via the connectors may damage the equipment. For the safe handling and operation of the equipment, appropriate measures against electrostatics should be implemented.
14. The outside of the instrument is suitably cleaned using a soft, lint-free dustcloth. Never use solvents such as thinners, acetone and similar things, as they may damage the front panel labeling or plastic parts.
15. Any additional safety instructions given in this manual are also to be observed.

Certified Quality System

ISO 9001

DQS REG. NO 1954-04

Qualitätszertifikat

Sehr geehrter Kunde,

Sie haben sich für den Kauf eines Rohde & Schwarz-Produktes entschieden. Hiermit erhalten Sie ein nach modernsten Fertigungsmethoden hergestelltes Produkt. Es wurde nach den Regeln unseres Qualitätsmanagementsystems entwickelt, gefertigt und geprüft. Das Rohde & Schwarz-Qualitätsmanagementsystem ist nach ISO 9001 zertifiziert.

Certificate of quality

Dear Customer,

You have decided to buy a Rohde & Schwarz product. You are thus assured of receiving a product that is manufactured using the most modern methods available. This product was developed, manufactured and tested in compliance with our quality management system standards.
The Rohde & Schwarz quality management system is certified according to ISO 9001.

Certificat de qualité

Cher client,

Vous avez choisi d'acheter un produit Rohde & Schwarz. Vous disposez donc d'un produit fabriqué d'après les méthodes les plus avancées. Le développement, la fabrication et les tests respectent nos normes de gestion qualité.
Le système de gestion qualité de Rohde & Schwarz a été homologué conformément à la norme ISO 9001.

ROHDE & SCHWARZ

ROHDE&SCHWARZ

EC Certificate of Conformity

CE

Certificate No.: 99049

This is to certify that:

Equipment type	Stock No.	Designation
FSP3	1093.4495.03	Spectrumanalyzer
FSP7	1093.4495.07	
FSP13	1093.4495.13	
FSP30	1093.4495.30/.39	
FSP-B3	1129.6491.02	Audio Modulator AM/FM
FSP-B4	1129.6740.02	OCXO 10 MHz
FSP-B9	1129.6991.02	Tracking Generator
FSP-B10	1129.7246.02	External Generator Control
FSP-B16	1129.8042.02	Lan Interface 10/1000 Base T
FSP-B25	1129.7746.02	Electronic Attenuator

complies with the provisions of the Directive of the Council of the European Union on the approximation of the laws of the Member States

- relating to electrical equipment for use within defined voltage limits (73/23/EEC revised by 93/68/EEC)
- relating to electromagnetic compatibility (89/336/EEC revised by 91/263/EEC, 92/31/EEC, 93/68/EEC)

Conformity is proven by compliance with the following standards:

EN61010-1 : 1993 + A2 : 1995
EN50081-1 : 1992
EN50082-2 : 1995

Affixing the EC conformity mark as from 1999

ROHDE & SCHWARZ GmbH & Co. KG
Mühldorfstr. 15, D-81671 München

Munich, 2000-08-02

Central Quality Management FS-QZ / Becker

Support Center

Telefon / Telephone: **(0180) 512 42 42**

Fax: **(++89) 41 29 - 137 77**

e-mail: **CustomerSupport@rsd.rohde-schwarz.com**

Für technische Fragen zu diesem Rohde & Schwarz-Gerät steht Ihnen ab sofort unsere Hotline der Rohde & Schwarz Vertriebs-GmbH, Support Center, zur Verfügung.

Unser Team bespricht mit Ihnen Ihre Fragen und sucht Lösungen für Ihre Probleme.

Die Hotline ist Montag bis Freitag von 8.00 bis 17.00 Uhr besetzt.

Bei Anfragen außerhalb der Geschäftszeiten hinterlassen Sie bitte eine Nachricht oder senden Sie eine Notiz per Fax oder e-mail. Wir setzen uns dann baldmöglichst mit Ihnen in Verbindung.

Should you have any technical questions concerning this Rohde & Schwarz product, please contact the hotline of Rohde & Schwarz Vertriebs-GmbH, Support Center.

Our hotline team will answer your questions and find solutions to your problems.

You can reach the hotline Monday through Friday from 8:00 until 17:00.

If you need assistance outside office hours, please leave a message or send us a fax or e-mail. We will contact you as soon as possible.

ROHDE&SCHWARZ

Adressen/Addresses

FIRMENSITZ/HEADQUARTERS

Telefon/Phone
Telefax
E-mail

ROHDE & SCHWARZ GmbH & Co. KG
Mühldorfstraße 15 · 81671 München — +49 89 41 29- 0
Postfach 801469 · 81614 München — +49 89 41 29- 12164
Internet: www.rohde-schwarz.com — –

WERKE/PLANTS

ROHDE & SCHWARZ Messgerätebau GmbH — +49 83 31 10 8-0
Riedbachstraße 58 · 87700 Memmingen — +49 83 31 10 81 124
Postfach 16 52 · 87686 Memmingen — –

ROHDE & SCHWARZ GmbH & Co. KG
Werk Teisnach — +49 99 23 8 57-0
Kaikenrieder Straße 27 · 94244 Teisnach — +49 99 23 8 571-1 74
Postfach 11 49 · 94240 Teisnach — –

ROHDE & SCHWARZ GmbH & Co. KG · Werk Köln — +49 22 03 49-0
Graf-Zeppelin-Straße 18 · 51147 Köln — +49 22 03 49-51 3 08
Postfach 98 02 60 · 51130 Köln — –

TOCHTERUNTERNEHMEN/SUBSIDIARIES

ROHDE & SCHWARZ Vertriebs-GmbH — +49 89 4129-120 07
Mühldorfstraße 15 · 81671 München — +49 89 4129-135 67
Postfach 801469 · 81614 München — customersupport@rohde-schwarz.com

ROHDE & SCHWARZ International GmbH — +49 89 4129-120 05
Mühldorfstraße 15 · 81671 München — +49 89 4129-135 97
Postfach 80 14 60 · 81614 München — –

ROHDE & SCHWARZ Engineering and Sales GmbH — +49 89 4129-137 11
Mühldorfstraße 15 · 81671 München — +49 89 4129-137 23
Postfach 80 14 29 · 81614 München — –

R&S BICK Mobilfunk GmbH — +49 50 42 9 98-0
Im Landerfeld 7 · 31848 Bad Münder — +49 50 42 9 98-105
Postfach 20 62 · 31844 Bad Münder — rsbick@rsbick.rohde-schwarz.com

ROHDE & SCHWARZ FTK GmbH — +49 30 6 58 91-122
Wendenschloßstraße 168, Haus 28 — +49 30 65 550-221
12557 Berlin — –

SIT Gesellschaft für Systeme
der Informationstechnik mbH — +49 30 6 58 84-2 22
Wendenschloßstraße 168, Haus 28 — +49 30 6 58 84-1 83
12557 Berlin — sit.info@sit.rohde-schwarz.com

Zweigniederlassungen der Rohde & Schwarz Vertriebs-GmbH/Branch offices of Rohde & Schwarz Vertriebs-GmbH

Zweigniederlassung Berlin — (+49 30) 34 79 48-0
Ernst-Reuter-Platz 10 · 10587 Berlin — (+49 30) 34 79 48-48
Postfach 100620 · 10566 Berlin — customersupport@rohde-schwarz.com

Zweigniederlassung Büro Bonn — (+49 2 28) 918 90-0
Josef-Wirmer-Straße 1–3 · 53123 Bonn — (+49 2 28) 25 50 87
Postfach 140264 · 53057 Bonn — customersupport@rohde-schwarz.com

Zweigniederlassung Hamburg — (+49 40) 63 29 00-0
Steilshooper Allee 47 · 22309 Hamburg — (+49 40) 630 78 70
Postfach 602240 · 22232 Hamburg — customersupport@rohde-schwarz.com

Zweigniederlassung Köln — (+49 22 03) 807-0
Graf-Zeppelin-Straße 18 · 51147 Köln — (+49 22 03) 807-50
Postfach 900149 · 51111 Köln — customersupport@rohde-schwarz.com

Zweigniederlassung Mitte — (+49 61 02) 20 07-0
Siemensstraße 20 — (+49 61 02) 80 00 40
63263 Neu-Isenburg — customersupport@rohde-schwarz.com

Zweigniederlassung München — (+49 89) 41 86 95-0
Mühldorfstraße 15 · 81671 München — (+49 89) 40 47 64
Postfach 801449 · 81614 München — customersupport@rohde-schwarz.com

Zweigniederlassung Nürnberg — (+49 9 11) 64203-0
Donaustraße 36 — (+49 9 11) 64203-33
90451 Nürnberg — customersupport@rohde-schwarz.com

Zweigniederlassung Telekommunikation — (+49 61 02) 20 07-0
Siemensstraße 20 — (+49 61 02) 20 07-12
63263 Neu-Isenburg — customersupport@rohde-schwarz.com

ADRESSEN WELTWEIT/ADDRESSES WORLDWIDE

Algeria
ROHDE & SCHWARZ Bureau d'Alger — (2) 59 24 53
5 B, Place de Laperrine — (2) 69 46 08
16035 Hydra-Alger — –

Argentina
Precisión Electrónica SRL — (14) 331 16 85
Av. Julio A. Roca 710 - Piso 6 — (14) 334 51 11
1067 Buenos Aires — preelctr@satlink.com

Australia
ROHDE & SCHWARZ — Sales (2) 8845 4100
(AUSTRALIA) Pty. Ltd. — (2) 9738 3988
Unit 6, 2-8 South Street — Service (2) 8845 4188
Rydalmere, N.S.W. 2116 — (2) 9638 0832
sales@rsaus.rohde-schwarz.com
service@rsaus. rohde-schwarz.com

Austria
ROHDE & SCHWARZ-ÖSTERREICH — (1) 6 02 61 41
Ges. m. b. H. — (1) 6 02 61 41-14
Sonnleithnergasse 20 — office@rsoe.rohde-schwarz.com
1100 Wien

Azerbaijan
ROHDE & SCHWARZ Azerbaijan — 12 93 31 38
Liaison Office Baku — 12 93 03 14
Azerbaijan Avenue 35 — –
370139 Baku

Baltic Countries
siehe/see Denmark

Bangladesh
Business International Ltd. — (2) 881 06 53
Corporation Office — (2) 882 82 91
House No: 95/A, Block -'F' — –
Road No: 4, Banani
Dhaka - 1213

Belgium
ROHDE & SCHWARZ BELGIUM N.V. — (2) 7 21 50 02
Excelsiorlaan 31 Bus 1 — (2) 7 25 09 36
1930 Zaventem — info@rsb.rohde-schwarz.com

Bolivia
siehe auch/see also Argentina

RIBCO LTDA. — (2) 32 84 03
Av. Mariscal Santa Cruz 1392 — (2) 39 30 47
Ed. Cámara Nacional de Comercio — gibatta@caoba.entelnet.bo
Piso 10, Of.1010-1011
La Paz

Brazil
ROHDE & SCHWARZ DO BRASIL LTDA.
Av. Alfredo Egidio de Souza Aranha, 177 — (11) 56 41 12 00
1° andar - Santo Amaro — (11) 56 41 78 10
04726-170 São Paulo- SP

Adressen/Addresses

Brunei
GKL Equipment PTE. Ltd. 276 06 26
#11-01 BP Tower 276 06 29
396, Alexandra Road gkleqpt@signet.com.sg
Singapore 119954
Republic of Singapore

Bulgaria
ROHDE & SCHWARZ (2) 963 43 34
Representation Office Bulgaria (2) 963 21 97
39, Fridtjof Nansen Blvd. rohdebg@rsoe.com
1000 Sofia

Canada
Kommunikationstechnik/Communications Equipment:
ROHDE & SCHWARZ CANADA Inc. (613) 592 80 00
555 March Rd. (613) 592 80 09
Kanata, Ontario K2K 2M5 –

Messtechnik/T & M Equipment:
TEKTRONIX CANADA, Inc. (416) 747 50 00
3280 Langstaff Road, Unit 1 (905) 760 72 41
Concord, Ontario L4K 5B6 –

Chile
DYMEQ Ltda. (2) 277 50 50
Avenida Larraín 6666 (2) 227 87 75
Santiago dymeq@entelchile.net

China
ROHDE & SCHWARZ (10) 64 31 28 28
Representative Office Beijing (10) 64 37 98 88
Parkview Center, Room 602 –
No. 2 Jiangtai Road,
Chao Yang District
Beijing 100016, P. R. China

Colombia
Ferrostaal de Colombia (1) 415 77 00
Av. Eldorado Nro. 97-03 Interior 2 (1) 413 18 06
Santafé de Bogotá, D.C. mc_fsc@multiphone.net.co

Costa Rica
siehe/see Mexico (EPSA)

Croatia
siehe/see Austria

Republic of Cyprus
HINIS TELECAST LTD. (4) 42 51 78
Agiou Thoma 18 (4) 42 46 21
Kiti
Larnaca 7550

Czech Republic
ROHDE & SCHWARZ – Praha, s.r.o. (2) 24 32 20 14
Pod Kastany 3 (2) 24 31 70 43
160 00 Praha 6 rohdecz@rsoe.com

Denmark
ROHDE & SCHWARZ DANMARK A/S 43 43 66 99
Ejby Industrivej 40 43 43 77 44
2600 Glostrup RSDK@post1.tele.dk

Ecuador
REPRESENTACIONES (2) 25 22 51
MANFRED WEINZIERL (2) 25 22 51
Guanguiltagua 72 (39-93) mweinzierl@accessinter.net
Urbanización Jardines del Batán
Quito

Egypt
U.A.S. Universal Advanced Systems (202) 455 67 44
31 Manshiet El Bakry St., Heliopolis (202) 256 17 40
11341 Cairo uas@intouch.com

El Salvador
siehe/see Mexico (EPSA)

Estonia
ROHDE & SCHWARZ DANMARK A/S (6) 14 31 20
Estonian Branch Office (6) 14 31 21
Narva mnt. 13
10151 Tallinn

Finland
Orbis Oy (9) 47 88 30
P.O. B. 15 (9) 53 16 04
00421 Helsinki info@orbis.fi

France
ROHDE & SCHWARZ FRANCE (1) 41 36 10 00
Immeuble "Le Newton" (1) 41 36 11 10
9-11, rue Jeanne Braconnier –
92366 Meudon-la-Forêt Cédex

Niederlassung/Subsidiary Rennes:
ROHDE & SCHWARZ FRANCE (2) 99 51 97 00
Sigma 1 (2) 99 41 91 31
Rue du Bignon –
35135 Chantepie

Niederlassung/Subsidiary Toulouse:
ROHDE & SCHWARZ FRANCE (5) 61 39 10 69
Technoparc 3 (5) 61 39 99 10
B.P.501 –
31674 Labège Cédex
Büros/Offices:
Aix-en-Provence (4) 94 07 39 94
(4) 94 07 55 11
Lyon (4) 78 29 88 10
(4) 78 29 94 71
Nancy (3) 83 54 51 29
(3) 83 55 39 51

Ghana
KOP Engineering Ltd. (21) 77 99 13
P.O. Box 11012 (21) 22 47 69
3rd Floor Akai House, Osu
Accra

Greece
MERCURY SA. (1) 722 92 13
6, Loukianou Str. (1) 721 51 98
10675 Athens mercury@hol.gr

Guatemala
siehe/see Mexico (EPSA)

Honduras
siehe/see Mexico (EPSA)

Hong Kong
Schmidt & Co. (HK) Ltd. 25 07 03 33
9/F North Somerset House 28 27 56 56
Taikoo Place frankwong@shk.schmidtgroup.com
979 King's Road
Quarry Bay, Hong Kong

Hungary
ROHDE & SCHWARZ (1) 203 02 82
Budapesti Iroda (1) 203 02 82
Etele ut. 68 rohdehu@rsoe.com
1115 Budapest

Iceland
siehe/see Denmark

India
ROHDE & SCHWARZ (11) 683 74 84
India Pvt. Ltd.
244, Okhla Industrial Estate rsindiad@vsnl.com
Phase - III
New Delhi 110 020

Indonesia
P.T. REKANUSA SOLUSI (21) 576 16 02
Menara Rajawali, (21) 576 16 04
24th floor –
Jl Mega Kuningan Lot # 5.1
Kawasan Mega Kuningan
Jakarta 12950

Iran
ROHDE & SCHWARZ IRAN (21) 8 73 02 82
Liaison Office - Reg. N° RFC 1947 (21) 8 73 02 83
Dr. Beheschty Ave., Pakistan Ave., –
12th Street N° 1
Tehran 15317

Adressen/Addresses

Ireland siehe/see Great Britain

Italy
ROHDE & SCHWARZ ITALIA S.p.a. (6) 41 59 81
Via Tiburtina 1182 (6) 41 59 82 70
00156 Roma –

Centro Direzionale Lombardo (2) 95 70 41
Via Roma 108 (2) 95 30 27 72
20060 Cassina de´ Pecchi (MI)

Japan
ADVANTEST Corporation (3) 33 42 75 53
RS Sales Department (3) 53 22 72 70
Shinjuku-NS Building, 4-1 yoshimu@inst.advantest.co.jp
Nishi-Shinjuku
Tokyo 163-08, Japan

Jordan
Middle East Development (6) 465 96 71
c/o Jordan Crown Engineering & Trading Co. (6) 465 96 72
P.O. Box 830414
Amman, 11183

Kazakhstan
ROHDE & SCHWARZ Kazakhstan 32 72 63 55 55
Liaison Office Almaty 32 72 63 46 33
Pl. Respubliki 15 –
480013 Almaty

Kenya
Excel Enterprises Limited (2) 55 80 88
Dunga Road (2) 54 46 79
P.O. Box 42 788
Nairobi

Korea
Hana Technica Corp. (2) 514 45 46
Seoul Kangnam, P.O. Box 1458 (2) 514 45 49
Young Dong Bldg. 4F hanateco@unitel.co.kr
63-16 Nonhyun-Dong, Kang Nam-Ku
Seoul

Kuwait
Group Five Trading & Contracting Co. 244 91 72
P.O. Box 26645 244 95 28
Safat 13127
State of Kuwait

Latvia
Rohde & Schwarz Danmark A/S (7) 50 23 55
Latvian Branch Office (7) 50 23 60
Merkela iela 21-301 rsdk@rsdk.rohde-schwarz.com
1050 Riga

Lebanon
Rohde & Schwarz International (1) 465 64 28 Ext. 303
Liaison Office Riyadh (1) 465 64 28 Ext. 229
PO Box 361
c/o Haji Abdullah Alireza & Co.
Riyadh 11411 – KSA

Liechtenstein siehe/see Switzerland

Lithuania
Rohde & Schwarz Danmark A/S 222 46 62
Lithuanian Office 222 46 62
Lukiskiu 5-228
2600 Vilnius

Luxembourg siehe/see Belgium

Malaysia
DAGANG TEKNIK SDN. BHD. (3) 7035503/7035568
No. 9, Jalan SS 4D/2 (3) 7 03 34 39
Taman People´s Park danik@tm.net.my
47301 Petaling Jaya
Selangor Darul Ehsan

Malta
ITEC – International Technology Ltd. 37 43 00
B'Kara Road 37 43 53
San Gwann itec@keyworld.net

Mexico
Vertrieb Kommunikationstechnik/
Sales of Communications Equipment:
ELECTROINGENIERIA de Precisión (5) 559 76 77
S.A. (EPSA) (5) 575 33 81
Uxmal 520 epsa@compuserve.com
Colonia Vertiz Narvarte
03600 Mexico DF

Vertrieb Messtechnik/Sales of T&M Equipment:
Tektronix S.A. de C.V. (5) 666 63 33
Periférico Sur 5000, 8° Piso (5) 666 63 36
Col. Insurgentes Cuicuilco
Del. Coyoacán
04530 Mexico, D.F.

Nepal
Abishek Trade Links (P) Ltd. (1) 25 69 30
P.O.B. 9700 (1) 24 25 73
Kathmandu Durbar@hotel.mos.com.np

Netherlands
ROHDE & SCHWARZ (30) 600 17 00
NEDERLAND B.V. (30) 600 17 99
Perkinsbaan 1 Rob.DenHartog@rsn.rohde-schwarz.com
3439 ND Nieuwegein

New Zealand
Nichecom (4) 232 32 33
Level 1 Tawa Plaza (4) 232 32 30
210 Main Rd / P.O.B. 56-045 ISDN (4) 237 30 10
Tawa, Wellington robin.hodgson@nichecom.co.nz

Nicaragua siehe/see Mexico (EPSA)

Nigeria
Ferrostaal (Nigeria) Ltd. (1) 262 00 60
27/29 Adeyemo Alkaija Street (1) 262 00 64
P.O. Box 72021
Victoria Island
Lagos

Norway
ROHDE & SCHWARZ NORGE 23 17 22 50
Østensjøveien 36, P.O.B. 103 BRYN 23 17 22 69
0611 Oslo –

Oman
T&M Equipment and Broadcasting:
Mustafa & Jawad Science & Industry Co. Ltd. 60 20 09
P.O. Box 3340 60 70 66
Post Code 112
Ruwi
Sultanate of Oman

Pakistan
TelcoNet Communications & (51) 26 30 72
Engineering (51) 26 32 11
213/D, Ordnance Road tnc@meganet.com.pk
Rawalpindi-Pakistan-46000

Panama siehe auch/see also Mexico (EPSA)

ELECTRONICO BALBOA S.A. 614 93 64
Av. El Paical, Edif. El Dorado 236 18 20
Urb. Los Angeles pdubois@ebsa.com
Panama City

Papua-New Guinea siehe/see Australia

Peru siehe auch/see also Argentina

BMP INGENIEROS S.A. (1) 225 40 30
Av. José Gálvez Barrenechea 645 (1) 475 15 13
Urb. Corpac - San Borja wmelgarejo@bmp.com.pe
Lima 41

Adressen/Addresses

Philippines
MARCOM Industrial Equipment, Inc.
MCC P.O.Box 2307
6-L Mezzanine Suite, Vernida I
Condominium120 Amorsolo St.
Legaspi Village
Makati City/Philippines 3117
(2) 8 13 29 31
(2) 8 17 05 07

Poland
ROHDE & SCHWARZ
Oddzial w Polsce
ul. Stawki 2, Pietro 28
00-193 Warszawa
(22) 860 64 90
(22) 860 64 99
rohdepl@rsoe.com

Portugal
TELERUS
Sistemas de Telecomunicações, S.A.
Rua General Ferreira Martins, Lote 6,2.°B
1495 Algés
(21) 412 35 90
(21) 412 36 00
telerus@mail.telepac.pt

Romania
ROHDE & SCHWARZ
Representation Office Bucharest
Uranus 98
Bloc U8, scara 2, etaj 5, ap. 36
76102 Bucuresti
(1) 410 68 46
(1) 411 20 13
rohdero@rsoe.com

Russian Federation
ROHDE & SCHWARZ
Representative Office Moscow
Kazachy per. 7
109017 Moscow
(095) 234 49 62
(095) 234 49 63
rohderus@rsoe.com

Saudi Arabia
Rohde & Schwarz Liaison Office
c/o Haji Abdullah Alireza Co. Ltd.
P.O.B. 361
Riyadh 11411
(1) 465 64 28
(1) 465 07 82
–

Singapore
Vertrieb/Sales:
INFOTEL TECHNOLOGIES LTD.
19 Tai Seng Drive
Kinergy Building # 06-00
Singapore 535222
287 68 22
284 95 55
general@infotel.com.sg

Service:
Rohde & Schwarz
Support Centre Asia Pte. Ltd.
1 Kaki Bukit View
#04-05/07 Techview
Singapore 415941
846 37 10
846 00 29
rssca@mbox4.singnet.com.sg

Slovak Republic
Specialne systemy a software, a.s.
Svrcic ul
84104 Bratislava
(7) 65 42 25 29
(7) 65 42 07 68
3s@internet.sk

Slovenia
ROHDE & SCHWARZ
Representation Ljubljana
Koprska 92
1000 Ljubljana
(61) 123 46 51
(61) 123 46 11
rohdesi@rsoe.com

South Africa
Protea Data Systems (Pty) Ltd
Communications & Measurement Division
Private Bag X19
Bramley 2018
(11) 786 36 47
(11) 786 58 91
Colin.Forbes@protea.co.za

Spain
ROHDE & SCHWARZ ESPAÑA
Salcedo, 11
28034 Madrid
(91) 334 10 70
(91) 729 05 06
rema@rsd.rohde-schwarz.com

Sri Lanka
LANKA AVIONICS
658/1/1, Negombo Road
Mattumagala
Ragama
(1) 95 66 78
(1) 95 83 11
–

Sudan
SolarMan Co. Ltd.
P.O. Box 11 545
Karthoum
(11) 47 31 08
(11) 78 17 25

Sweden
ROHDE & SCHWARZ SVERIGE AB
Flygfältsgatan 15
12830 Skarpnäck
(8) 605 19 00
(8) 605 19 80
info@rss.rohde-schwarz.com

Switzerland
Roschi Rohde & Schwarz AG
Papiermühlestrasse 145, Postfach
3063 Ittigen
(31) 922 15 22
(31) 921 81 01
–

Syria
Electro Scientific Office
Baghdad Street
Dawara Clinical Lab. Building
P.O.B. 8162
Damascus
(11) 231 59 74
(11) 231 88 75
–

Tanzania
Security Systems (T) Ltd.
P.O. Box 7512
Dar Es Salaam
(22) 2 76 00 37
(22) 276 02 93

Taiwan
Lancer Communication Co., LTD.
16F, No. 30, Pei-Ping East Road
Taipei
(2) 23 91 10 02
(2) 23 95 82 83
rosa.ho@lancercomm.com.tw

Thailand
Vertrieb Kommunikationstechnik/Sales Communications Equipment:
TPP Operation Co., Ltd.
41/5 MoobanTarinee Boromrajchonnee Rd.
Talingchan, Bangkok 10170
(2) 880 93 45
(2) 880 93 47
–

Vertrieb Messtechnik/Sales T & M Equipment:
Schmidt Scientific (Thailand) Ltd.
212 Government Housing Bank Bldg.
Tower II, 19th Floor, Rama 9 Rd.,
Huaykwang, Bangkapi, Bangkok 10320
(2) 643 13 30-9
(2) 643 13 40
–

Turkey
ROHDE & SCHWARZ
Liaison Office Istanbul
Bagdad Cad. 191/3, Ard.
81030 Selamicesme-Istanbul
(216) 385 19 17
(216) 385 19 18
rsturk@superonline.com

Ukraine
ROHDE & SCHWARZ
Representative Office Kiev
ul. Patrisa Loumoumba, 4
252042 Kiev
(044) 268 60 55
(044) 268 83 64
rohdeukr@rsoe.com

United Arab Emirates
Service-Center für den Mittleren Osten/
Service Center for the Middle East:
ROHDE & SCHWARZ Emirates L.L.C.
P.O.B. 31156
Abu Dhabi
(2) 631 20 40
(2) 631 30 40
–

ROHDE & SCHWARZ
Liaison Office Middle East
P.O. Box 311 56
Abu Dhabi
(2) 63 35 670
(2) 63 35 671
–

Vertrieb/Sales:
ROHDE & SCHWARZ Liaison Office Dubai
P.O.B. 53726
Dubai
(4) 39 44 829
(4) 39 44 794
–

R&S BICK Mobile Communication
P.O.B. 17466
JAFZ, LOB 04-028
Dubai
(4) 81 36 75
(4) 81 36 76
–

United Kingdom
ROHDE & SCHWARZ UK Ltd.
Ancells Business Park
Fleet, Hampshire GU 13 8UZ
(12 52) 81 13 77
(12 52) 81 14 47
–

Uruguay
siehe auch/see also Argentina

	AEROMARINE S.A. Cerro Largo 1497 11200 Montevideo	(2) 400 39 62 (2) 401 85 97 aeromar@adinet.com.uy
USA	Kommunikationstechnik/Communications Equipment: ROHDE & SCHWARZ, Inc. 4425 Nicole Drive Lanham, MD 20706	(301) 459 88 00 (301) 459 28 10 –
	Messtechnik/T & M Equipment: TEKTRONIX Inc. P.O.B. 500, M/S 50-216 Beaverton, OR 97076	(800) 835 9433 Ext. 6630 (800) 835 7732 –
Venezuela	EQUILAB TELECOM C.A. Centro Seguros La Paz Piso 6, Local E-61 Ava. Francisco de Miranda Boleita, Caracas 1070	(2) 34 46 26 (2) 239 52 05 r_ramire@equilabtelecom.com.ve
	Military customers only: REPRESENTACIONES BOPIC S.A. Av. Diego Cisneros Centro Empresarial Los Ruices Of. 119, 1er piso Los Ruices Caracas	(2) 985 21 29 (2) 985 39 94 incotr@cantv.net
Vietnam	Schmidt Vietnam Co., Ltd. 8/F, Schmidt Tower, Hanoi Intern. Technology Centre Cau Giay, Tu Liem, IPO Box 89 Hanoi	(4) 834 61 86 (4) 834 61 88 svnhn@schmidt group.com
Yugoslavia	see/siehe Austria	

Nicht aufgeführte Länder/Countries not listed:

ROHDE & SCHWARZ INTERNATIONAL GmbH
P.O.B. 80 14 69
81614 München / Germany
Please fax to +49 89 41 29 136 62

Contents of Manuals for Spectrum Analyzer FSP

Operating Manual FSP

The operating manual describes the following models and options of spectrum analyzer FSP:

- FSP3 9 kHz to 3 GHz
- FSP7 9 kHz to 7 GHz
- FSP13 9 kHz to 13.6 GHz
- FSP30 9 kHz to 30 GHz

- Option FSP B3 audio demodulator
- Option FSP-B4 OCXO - reference oscillator
- Option FSP-B9 tracking generator
- Option FSP-B10 external generator control
- Option FSP-B16 LAN interface
- Option FSP-B25 electronic attenuator

This operating manual contains information about the technical data of the instrument, the setup functions and about how to put the instrument into operation. It informs about the operating concept and controls as well as about the operation of the FSP via the menus and via remote control. Typical measurement tasks for the FSP are explained using the functions offered by the menus and a selection of program examples.

Additionally the operating manual includes information about maintenance of the instrument and about error detection listing the error messages which may be output by the instrument. It is subdivided into 9 chapters:

Chapter 1 describes the control elements and connectors on the front and rear panel as well as all procedures required for putting the FSP into operation and integration into a test system.

Chapter 2 gives an introduction to typical measurement tasks of the FSP which are explained step by step.

Chapter 3 describes the operating principles, the structure of the graphical interface and offers a menu overview.

Chapter 4 forms a reference for manual control of the FSP and contains a detailed description of all instrument functions and their application. The chapter also lists the remote control command corresponding to each instrument function.

Chapter 5 describes the basics for programming the FSP, command processing and the status reporting system.

Chapter 6 lists all the remote-control commands defined for the instrument. At the end of the chapter a alphabetical list of commands and a table of softkeys with command assignment is given.

Chapter 7 contains program examples for a number of typical applications of the FSP.

Chapter 8 describes preventive maintenance and the characteristics of the instrument's interfaces.

Chapter 8 gives a list of error messages that the FSP may generate.

Chapter 9 contains a list of error messages.

Chapter 10 contains an index for the operating manual.

Contents - Chapter 1 " Preparing for Operation "

1 Preparing for Operation 1.1
Description of Front and Rear Panel Views 1.1
Front View 1.1
Rear View 1.9
Getting Started with the instrument 1.12
Preparing the instrument for Operation 1.12
Setting up the Instrument 1.12
Stand-alone Operation 1.12
Rackmounting 1.13
EMI Protection Measures 1.13
Connecting the Instrument to the AC Supply 1.13
Switching the Instrument on/off 1.14
Switching on the Instrument 1.14
Startup Menu and Booting 1.15
Switching off the FSP 1.15
Power-Save Mode 1.15
Battery-Powered Memory 1.16
Functional Test 1.16
Windows NT 1.17
Connecting an External Keyboard 1.18
Connecting a Mouse 1.19
Connecting an External Monitor 1.20
Connecting a Printing Device 1.21
Installation of a Network Printer (with option FSP-B16 only) 1.27
Installing Windows NT Software 1.30

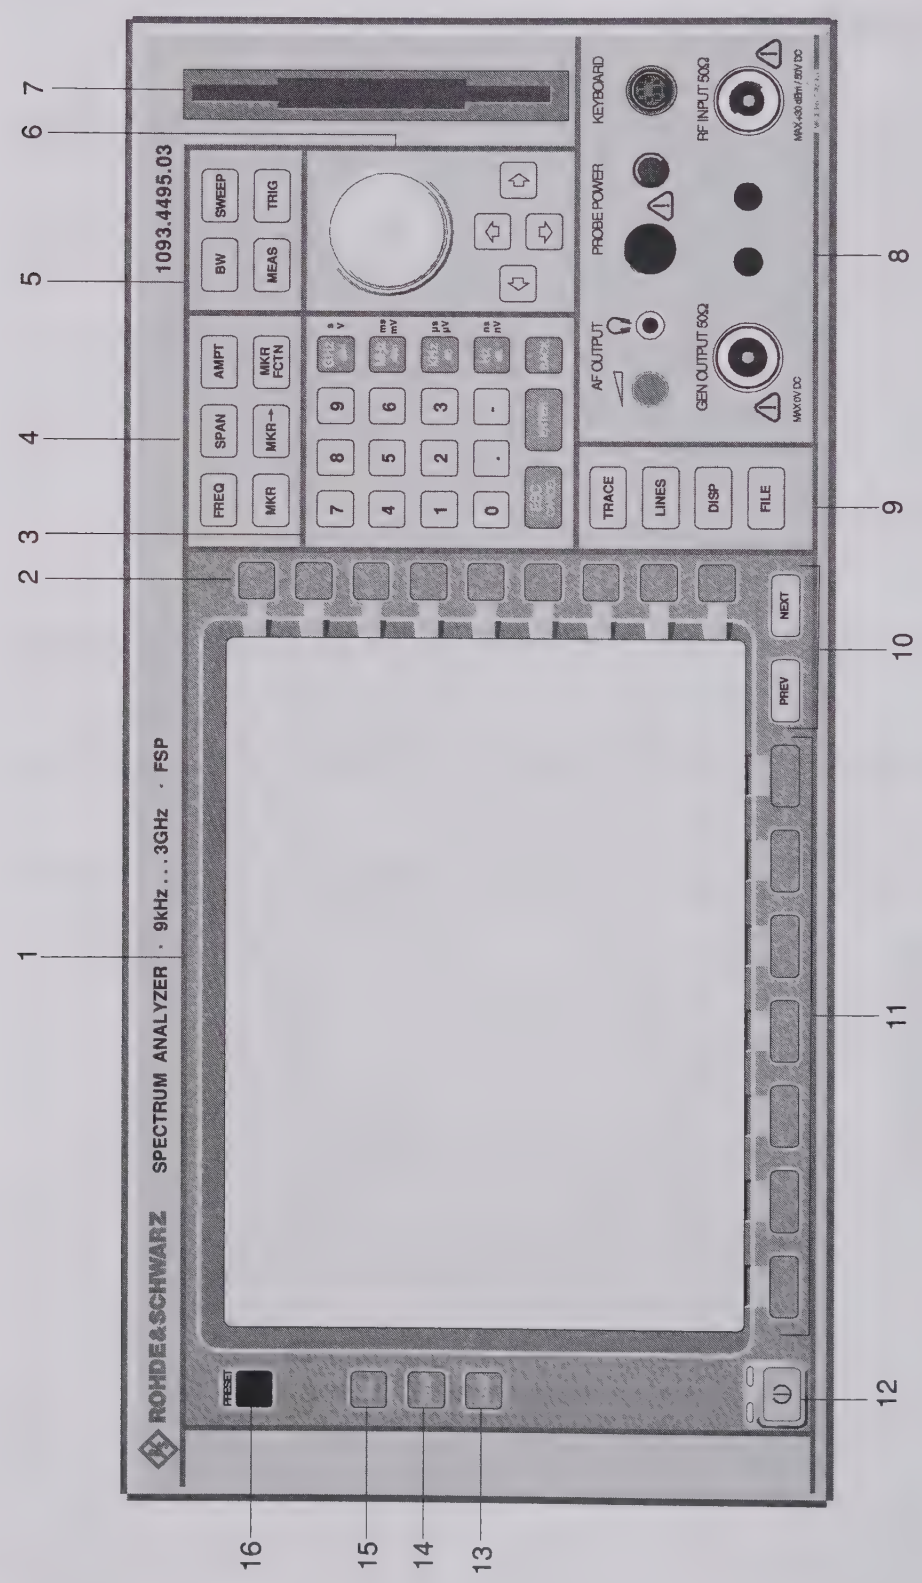

Fig. 1-1 Front View



Keypad for data input

GHz s
-dBm V
MHz ms
dBm mV
kHz µs
dB µV

Hz ns
dB.. nV

The units keys close the data input and define the multiplication factor for each basic unit.
For dimension-less or alphanumeric inputs, the units keys have weight 1.
They behave, in this case, like the ENTER key.

see Chapter 3

4



FREQ	Set frequency axis
SPAN	Set span
AMPT	Set level indication and configure RF input.
MKR	Select and set standard marker and delta marker functions.
MKR->	Change instrument settings via markers
MKR FCTN	Select further marker and delta marker functions

see Chapter 4

5



BW	– Set resolution bandwidth, video bandwidth and sweep time, – Set coupling of these parameters
SWEEP	Select sweep
MEAS	Select and set power measurements
TRIG	Set trigger sources

see Chapter 4

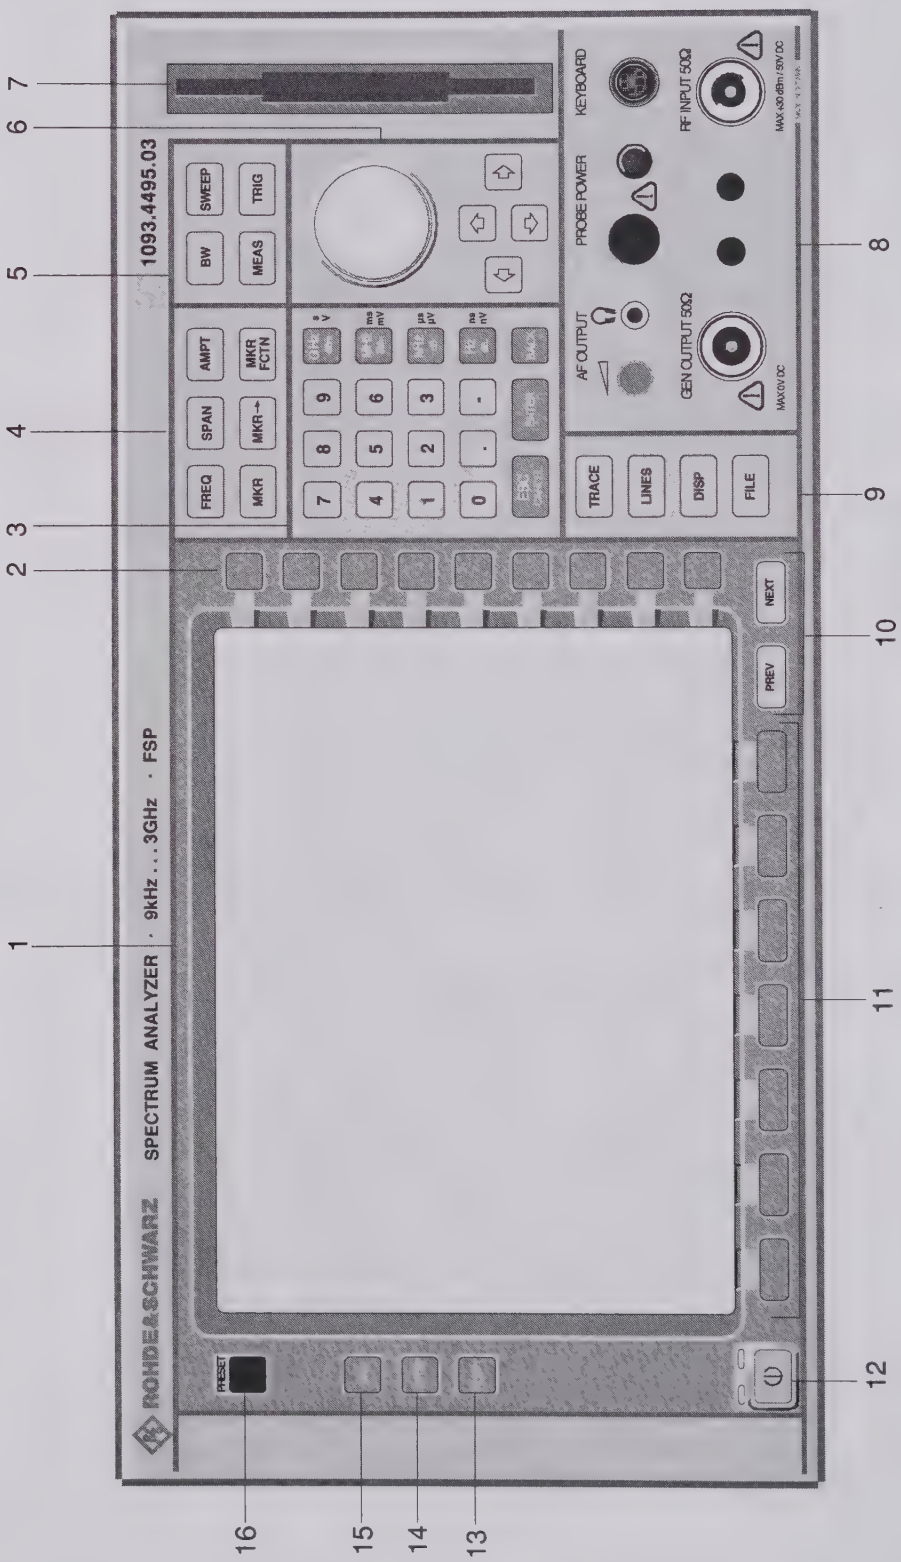

Fig. 1-1 Front View

6



Key group for entering data and for cursor movement — see Chapter 3

Cursor keys
- Move the cursor within the input fields and tables.
- Vary the input value.
- Define the direction of movement for the roll-key.

Roll-key
- Vary input values.
- Move markers and limits.
- Select letters in the help line editor.
- Move cursor in the tables
- Close data input (ENTER)

7

3 1/2" diskette drive; 1.44 MByte

8

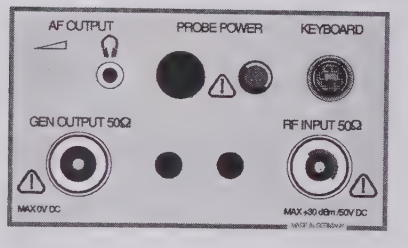

AF OUTPUT (only with option FSP-B3) — see Chapter 8

Volume control

Head phone connector

PROBE POWER — Power supply and coded socket (+15 V/ -12 V) for accessories

KEYBOARD — Connector for an external keyboard

RF INPUT — RF input — see Chapter 8

Caution:

The maximum DC voltage is 50 V, the maximum power is 1 W (≙ 30 dBm) at ≥ 10 dB attenuation.

9



TRACE — Select and activate traces and detectors — see Chapter 4

LINES — Set limit lines

DISP — Configure display

FILE
- Save and recall instrument data
- Configuration of memory media and data

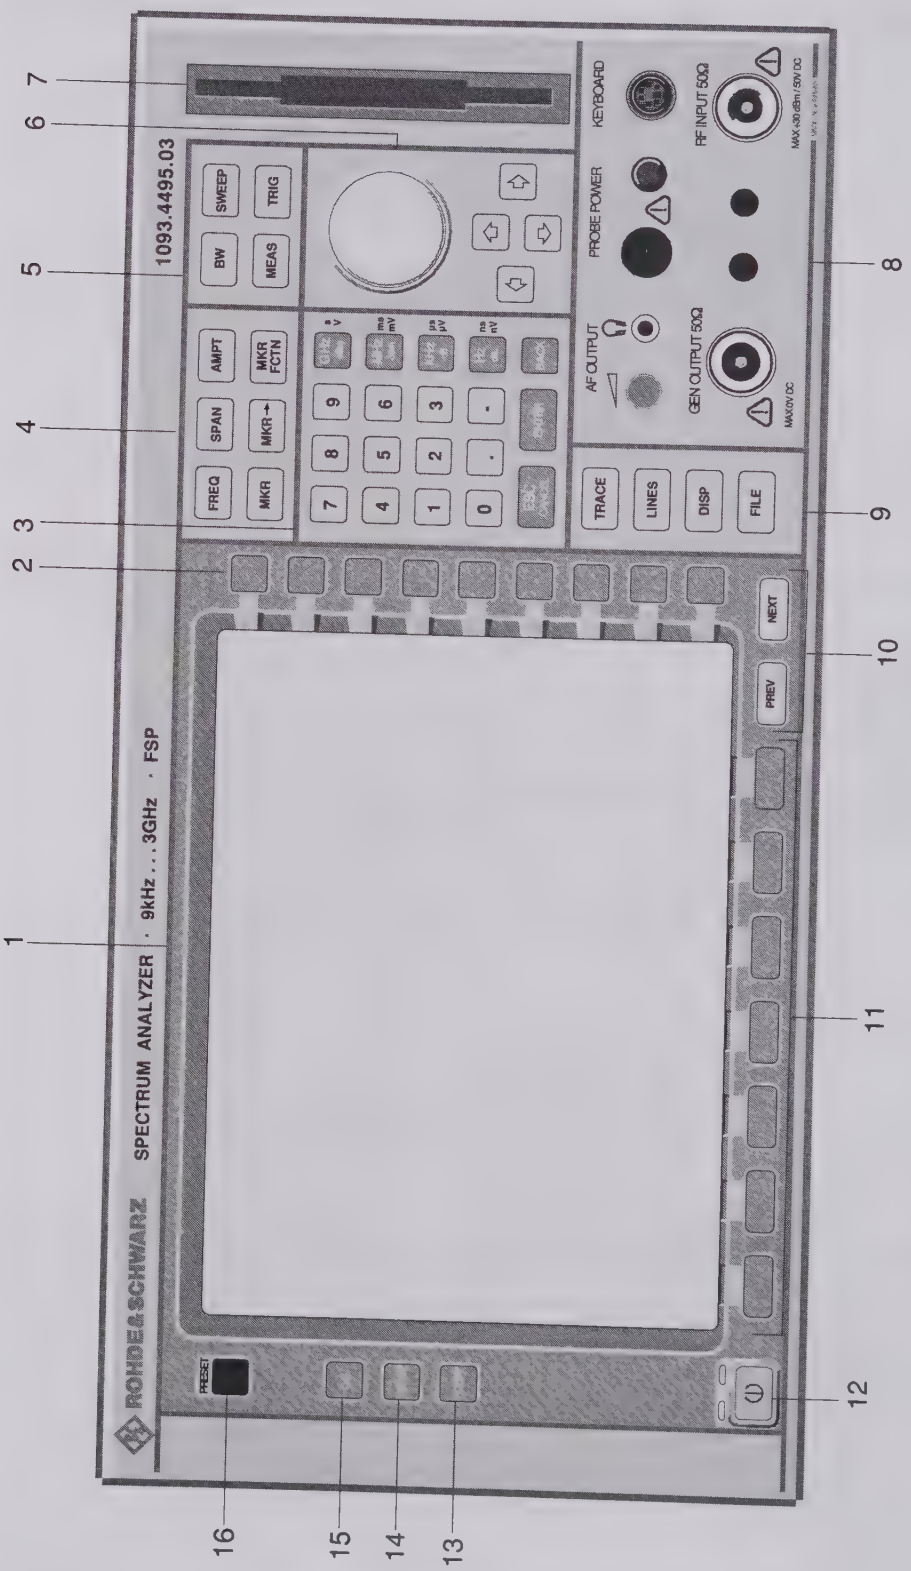

Fig. 1-1 Front View

10



Menu-change keys

NEXT Change to side menu

PREV Call main menu

see Chapter 3

11

Hotkeys

see Chapter 3

12

ON/STANDBY switch

see Chapter 1

13

Configure and start a print job

see Chapters 1 and 4

14

Define general configuration

see Chapter 4

15

Record correction data

see Chapter 4

16

Call default settings

see Chapter 4

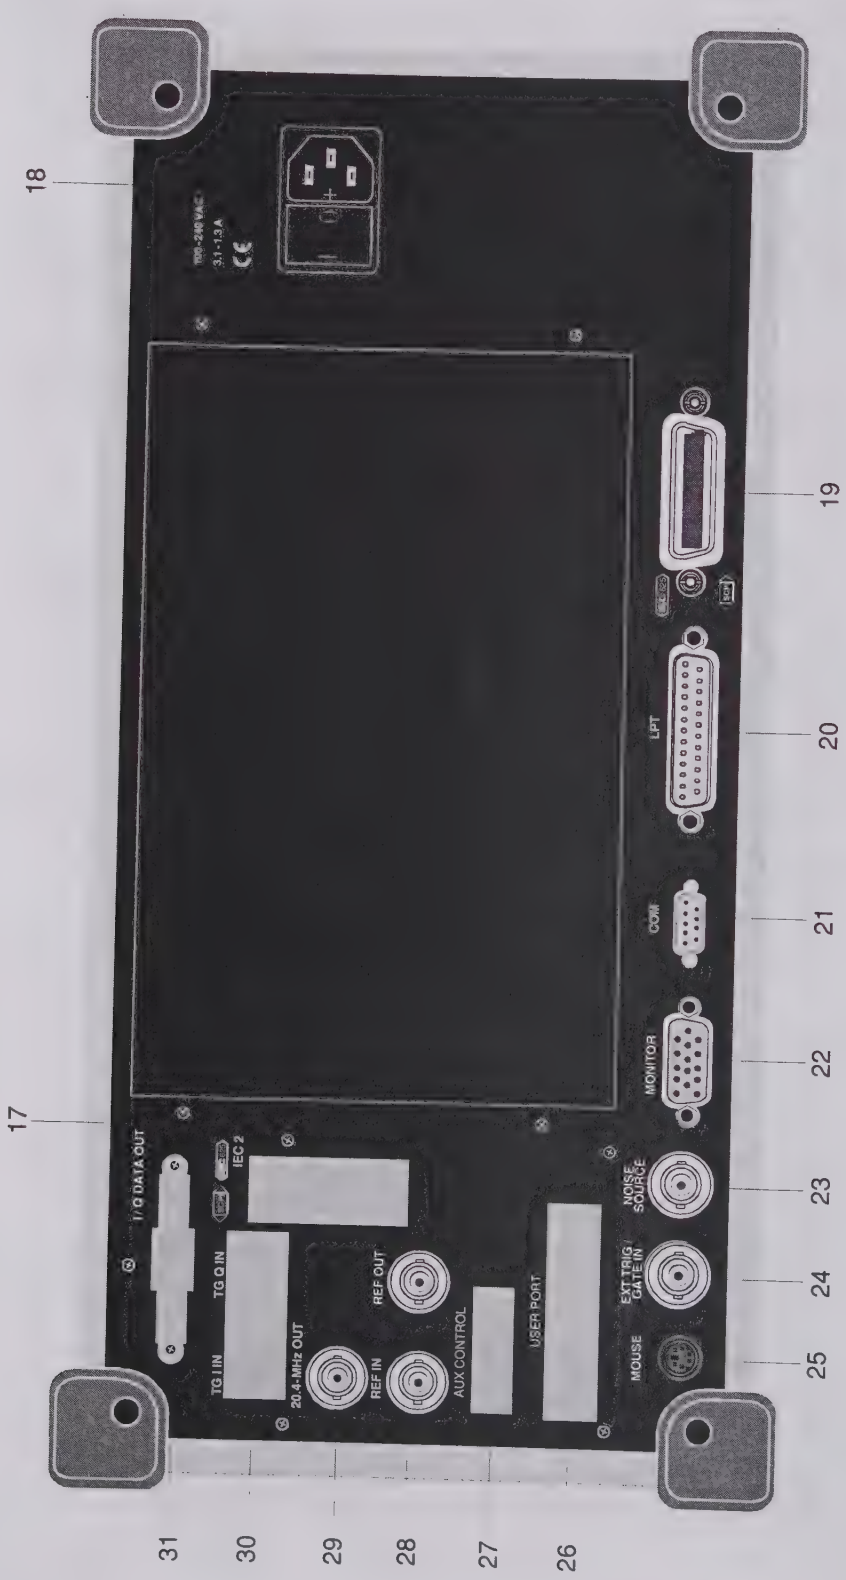

Fig. 1-1 Rear View

Rear View

17

Reserved for options

see Chapter 8

18



Power switch and AC power connector

see Chapter 1

19

IEC/IEEE bus-connector

see Chapter 8

20



Parallel interface connector
(printer connector)

see Chapter 8

21

Connector for a serial interface
(9-pin socket; COM)

see Chapter 8

22

Connector for an external monitor

see Chapter 8

23

Output connector for an external noise source

see Chapter 8

Fig. 1-2 Rear View

24

Input connector for an external trigger or an external gate signal

see Chapter 8

25

Connector for a PS/2 mouse

see Chapter 8

26

Reserved for options

27

Reserved for options

28



REF IN Input connector for an external reference (10 MHz)

REF OUT Output connector for an internal reference (10 MHz)

29

Output connector for 20.4 MHz IF

see Chapter 8

30

Reserved for options

31

Reserved for options

Getting Started with the instrument

The following section describes how to activate the instrument and how to connect external devices like eg printer and monitor.

Chapter 2 explains the operation of the instrument using simple measurement examples.

Important note:

Before turning the instrument on, care should be taken that the following conditions are fulfilled:

- *instrument covers are in place and tightened by the corresponding screws,*
- *fan openings are free from obstructions,*
- *signal levels at the input connectors are all within specified limits,*
- *signal outputs are connected correctly and not overloaded.*

Ignoring these conditions may cause damage to the instrument .

Preparing the instrument for Operation



remove protective caps

- Take the instrument out of the shipping box and check whether the items listed in the packing list and in the lists of accessories are all included.
- Remove the two protective caps from the front and rear of the FSP and carefully check the instrument for damage.
- Should the instrument be damaged, immediately notify the transportation company that shipped the instrument to you and keep the box and packing material.
- For further transport or shipment of the FSP the original packing should also be used. It is recommended to keep at least the two protective caps for front and rear side in order to prevent damage to the controls and connectors.

Setting up the Instrument

Stand-alone Operation

The instrument is designed for use under general laboratory conditions. The ambient conditions required at the operational site are as follows:

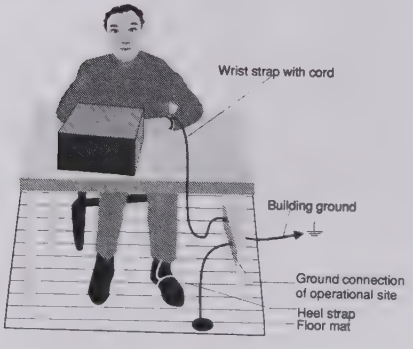

- The ambient temperature must be in the range indicated in the data sheet.
- All fan openings must be unobstructed and the air flow at the rear panel and at the side-panel perforations must not be obstructed. The distance to the wall should be at least 10 cm.
- The mounting surface should be flat.
- In order to avoid damage of electronic components of the device under test due to electrostatic discharge on manual touch, protection of the operational site against electrostatic discharge is recommended.

Rackmounting

Important Note:

For rack installation, ensure that the air flow at the side-panel perforations and the air exhaust at the rear panel are not obstructed.

The instrument may be mounted in a 19" rack by using a rack adapter kit (order number see data sheet). The installation instructions are included in the adapter kit.

EMI Protection Measures

In order to prevent electromagnetic interference (EMI), the instrument may be operated only when all covers are correctly in place. Only adequately shielded signal and control cables may be used (see recommended accessories).

Connecting the Instrument to the AC Supply

The FSP is equipped with an AC voltage selection feature and will automatically adapt itself to the applied AC voltage (range: 100 to 240 VAC, 40 to 400 Hz). External voltage selection or adaptation of the fuses are not necessary. The AC power connector is located on the rear panel (see below).



Power connector

➢ Connect the instrument to the AC power source using the AC power cable delivered with the instrument.

As the instrument is designed according to the regulations for safety class EN61010, it must be connected to a power outlet with earthing contact.

Switching the Instrument on/off

Caution:

Do not power down during booting. *Such a switch-off may lead to corruption of the hard disk files.*

AC power switch on the rear panel

Power switch Power connector

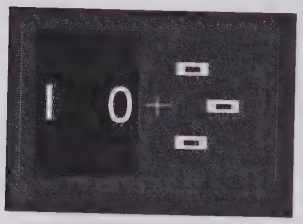

Power switch

Position I = ON

In the I position, the instrument is in standby mode or in operation, depending on the position of the ON/STANDBY key at the front of the instrument.

Note:

The AC power switch may remain ON continuously. Switching to OFF is only required when the instrument must be completely removed from the AC power source.

Position O = OFF

The 0 position implies an all-pole disconnection of the instrument from the AC power source.

ON/STANDBY switch on the front panel

ON STANDBY

Caution:

In standby mode, the AC power voltage is present within the instrument

Standby switch

The ON/STANDBY switch activates two different operating modes indicated by colored LEDs:

Operation ON - ON/STANDBY is depressed

The green LED (ON) is illuminated. The instrument is ready for operation. All modules within the instrument are supplied with power.

STANDBY - ON/STANDBY switch is not pressed.

The yellow LED (STANDBY) is illuminated. Only the power supply is supplied with power and the quartz oven is maintained at normal operating temperature.

Switching on the Instrument

- In order to switch on the FSP, set the power switch on the rear panel to position I.
- Set the FSP to operating mode by pressing the *ON/STANDBY* key on the front panel. The green LED must be illuminated.

Startup Menu and Booting

After switching on the instrument, a message indicating the installed BIOS version (eg Analyzer BIOS Rev. 1.2) appears on the screen for a few seconds.

Subsequently Windows NT is booted first and after that the instrument firmware will boot. As soon as the boot process is finished the instrument will start measuring. The settings used will be the one that was active when the instrument was previously switched off, provided no other device configuration than *FACTORY* had been selected with *STARTUP RECALL* in the *FILE* menu.

Switching off the FSP

- Switch the ON/STANDBY key on the front panel to standby mode by pressing it once. The yellow LED must be illuminated.

Only when removing the FSP completely from the AC power source:

- Set the power switch at the rear panel to position 0.

Power-Save Mode

Display:

The FSP offers the possibility of switching on a power-save mode for the screen display. The screen is blanked out if no entry is made on the front panel (key, softkey or hotkey and rollkey) during the selected response time.

In order to switch on the power-save mode:

1. Call the *DISPLAY - CONFIG DISPLAY* submenu to configure the screen display:
   - Press *DISP* key
   - Press *CONFIG DISPLAY* softkey

2. Activate the save mode
   - Press *DISPLAY PWR SAVE* softkey.
     The softkey is highlighted in colour, thus indicating that the power-save mode is on. At the same time the data entry for the delay time is opened.

3. Define the delay time
   - Enter the required response time in minutes and confirm the entry using the *ENTER* key.
     The screen will be blanked out after the selected time period has elapsed.

Harddisk:

A power-save mode is preset for the built-in harddisk which is automatically closed down 15 minutes after the last access.

Battery-Powered Memory

The FSP is equipped with a battery-powered read/write memory (CMOS-RAM) where instrument settings are saved at power-off. After each power-on, the FSP is reloaded with the operational parameters which were active just prior to the last power-off (STANDBY or AC power OFF) or were set with STARTUP RACALL (see Chapter 4 "Saving and Recalling Data Sets").

A lithium battery is used to supply power to the CMOS-RAM. As soon as the battery is discharged (expected life time is approx. 5 years), any data stored in CMOS-RAM will be lost. In this case, the factory standard setup is loaded at power-on. For changing batteries please contact your local service representative.

Functional Test

After turning on the AC power, the FSP will display the following message on the display screen:

Rohde & Schwarz GmbH & Co. KG
Analyzer BIOS Vx.y

After appearance of the above message, a self-test of the digital hardware is performed. Subsequently, the Windows NT controller boots and the measurement screen will appear.

The system self-alignment is actived via *CAL* key, *CAL TOTAL* softkey. The individual results of the self-alignment (PASSED / FAILED) can be displayed in the *CAL* menu (*CAL RESULTS*).
With the aid of the built-in self-test functions (*SETUP* key, *SERVICE, SELFTEST* soft keys), the functional integrity of the instrument can be verified and/or defective modules can be localized.

Windows NT

Caution:

The drivers and programms used under Windows NT are adapted to the measuring instrument. In order to prevent the instrument functions from damage, the settings should only be modified as described below. Existing software may only be modified using update software released by Rohde&Schwarz. Additionally only programs authorized by Rohde&Schwarz for use on the FSP may be run on the instrument.

Do not power down during booting. *Such a switch-off may lead to corruption of the hard disk files.*

The instrument runs under the operating system Windows NT. The computer can be used to configure and install and configure device drivers that were authorized by Rohde&Schwarz. Any further use of the computer function is only allowed under the conditions described in this operating manual.

Login

Windows NT requires a login process, during which the user is asked for identification by entering his name and password. As a factory default the instrument is configured for *Auto Login*, ie the login is performed automatically and in the background. The user name used for this is "instrument" and the password is also "instrument" (in small letters).

Administrator Level

The NT user account used for the autologin function has administrator access rights.

After a software installation that requires administrator rights (eg the installation of new printer drivers), Service Pack 5 of Windows NT has to be re-installed. The necessity to re-install the service pack is indicated in the corresponding operating manual chapters. The installation of the Service Pack is described in the section "Installing Windows NT Software".

Calling the Windows NT start menu

The Windows NT start menu is called using the key combination <CTRL> <ESC>. It is possible to access the required submenus from the start menu by means of the mouse or the cursor keys. In order to return to the measurement screen the button "R&S Analyzer Interface" in the Windows NT task bar can be used.

Connecting an External Keyboard

Caution:
The keyboard may only be connected when the instrument is switched off (STANDBY). Otherwise, correct operation of the keyboard cannot be guaranteed.

The FSP offers a 6-contact PS/2-connector KEYBOARD on the instrument's front panel for the connection of an external PC. It is recommended to use keyboard PSP-Z2 (Order No. 1091.4100.02, English). This keyboard is equipped with a trackball for mouse control.

During measurement operations, the keyboard simplifies the input of commentary text, filenames, etc.

The section "Instrument Interfaces" in Chapter 8 contains the interface description of the connector.

After connection of the keyboard and subsequent power-on, the keyboard will be automatically recognized. The default language used is "US keyboard". Special settings such as repetition rate etc. can be performed in the Windows NT menu START - SETTINGS - CONTROL PANEL - KEYBOARD.

Connecting a Mouse

Caution:
The mouse may only be connected when the instrument is switched off (STANDBY). Otherwise, correct operation of the mouse and instrument cannot be guaranteed.

In order to ease up operation of Windows NT, the FSP provides an option for connecting a mouse to the PS/2 mouse connector (MOUSE) at the rear panel of the instrument.
The mouse type supported is "Microsoft mouse". It is available as option PS-B1 (order number 1006.6359.02).

Note. *The recommended keyboard PSP-Z2 is equipped with a trackball for mouse control. Connecting an additional mouse will cause interface conflicts and lead to malfunctions of the instrument.*

The section "Instrument Interfaces" in Chapter 8 contains the interface description of the connector.

After connection and subsequent power-on the mouse is automatically recognized. Special settings such as mouse cursor speed etc., can be performed in the Windows NT menu START - SETTINGS - CONTROL PANEL - MOUSE.

Connecting an External Monitor

Caution:
The monitor may only be connected when the instrument is switched off (STANDBY). Otherwise, the monitor may be damaged.

Do not modify the screen driver (display type) and display configuration since this will severely affect instrument operation.

The instrument is equipped with a rear-panel connector MONITOR for the connection of an external monitor.



After connecting the external monitor the instrument needs to be rebooted in order to recognize the monitor. After that the measurement screen is displayed on both the external monitor and the instrument. Further settings are not necessary.

Connecting a Printing Device

Caution:
The printing device may be connected only when the instrument is switched off (STANDBY)

Note: *When installing printer drivers that are not pre-installed on the instrument, the operator is requested to insert the disk with the new driver into drive A.*
After installation the Service Pack needs to be re-installed (see section "Installing Windows NT Software")

The instrument is prepared for connecting printing devices to two different interfaces in order to create hard copies of the display screen. The *DEVICE* table in menu *HCOPY – DEVICE1/2* indicates the available selection of installed printing devices (see also Chapter 4, section "Documentation of Test Results").

The interface connectors are located on the rear panel:

Chapter 8 contains the interface descriptions of the connectors.

After connection of the printing device to the appropriate interface connector, the interface needs to be configured, the printer driver has to be installed and assigned to an interface.

1. Connecting keyboard and mouse

For the installation and configuration of printer drivers on the FSP, it is necessary to connect a keyboard to the front panel and a PS/2 mouse to the rear panel (only in case of using a keyboard without trackball, see sections "Connecting a Mouse" and "Connecting a Keyboard").

2. Switching to Windows NT start menu and opening the system control

The combination of keys <CTRL><ESC> is used to switch to the Windows NT start menu. The system control panel is then opened in the NT start menu using the sequence SETTINGS - CONTROL PANEL.

3. Configuration of the interface

LPT	Interface LPT needs no configuration.
COM	The COM interface must first be assigned to the operating system (owner = OS) in menu SETUP - GENERAL SETUP. The configuration of the serial interface can then be performed either in the Windows NT menu START - SETTINGS - CONTROL PANEL - PORTS or in the FSP SETUP - GENERAL SETUP menu. The parameters *Baud Rate*, *Data Bits*, *Parity*, *Stop Bits*, *Flow Control* determine the transmission parameters of the interface. They must correspond to the specifications of the printing device (see the operating manual for the printer).

Note: *The settings made for the serial interface in the menu SETUP - GENERAL SETUP overwrite the settings in the NT menu.*
However, settings in the Windows NT menu do not overwrite those of the SETUP menu. This means that the settings are only valid as long as the interface is assigned to the operating system.

4. Selection and installation of the printer driver

The selection and installation of the printer driver, the assignment to the interface and the setting of most of the printer-specific parameters (eg paper size) is performed under Windows NT in the START - SETTINGS - PRINTER menu.

5. Configuration of the connected output device

The configuration of the connected output device and the assignment to the interface takes place in the *HCOPY DEVICE1/2* menu (see in Chapter 4, the section "Measurement Documantation"). The instrument supports the configuration of up to two output devices (DEVICE1 and DEVICE2), one of which must be activated for printing.

- The parameter *DEVICE* determines which output device is to be used.
- The parameter *PRINT TO FILE* determines if the output is in the form of a file.
- The parameter *ORIENTATION* sets the page format to horizontal or vertical (portrait).

Selecting the type of printer automatically sets the parameters *PRINT TO FILE* and *ORIENTATION* to values which correspond to a standard operating mode with this output device. Other printer-dependent parameters such as *FORMFEED*, *PAPERFEED* etc., can be modified under Windows NT in the printer properties window (START/SETTINGS/PRINTER/SETTINGS/....).

Table 1-1 shows the standard factory settings for the two output devices.

The factory settings for DEVICE 1 correspond to output format "WMF" (Windows Metafile); printing is performed in a file. WMF is a common format which is used for the import of hardcopies (eg measurement windows) in other Windows applications that support this format (eg WinWord).

The factory settings for DEVICE 2 are "Clipboard". In this setting the printout is copied to the Windows NT clipboard. Most of Windows applications support the clipboard. The clipboard contents can be directly inserted into a document via EDIT - PASTE.

Table 1-1 Factory settings for *DEVICE 1* and *DEVICE 2* in the *HCOPY* menu.

Setting	**Selection in the configuration table**	***DEVICE 1* Settings**	***DEVICE 2* Settings**
Output Device	DEVICE/LANGUAGE	WINDOWS METAFILE	CLIPBOARD
Output	PRINT TO FILE	YES	---
Page Orientation	ORIENTATION	---	---

In the following example, a HP DeskJet 660C printer is connected to the LPT interface and configured as *DEVICE2* for hardcopies of the screen contents.

Switch off the FSP.

Connect the printer to interface LPT.

Switch on both FSP and printer.

Select the printer driver under Windows NT

➢ Press key combination <CTRL> <ESC>

The Windows NT start menu is displayed.

➢ In the Start menu press "Setting" and then "Printers".

The printer window is opened.

➢ Double-click symbol "Add Printer".

The "Add Printer Wizard" window is opened. This window leads through the following printer driver installation.

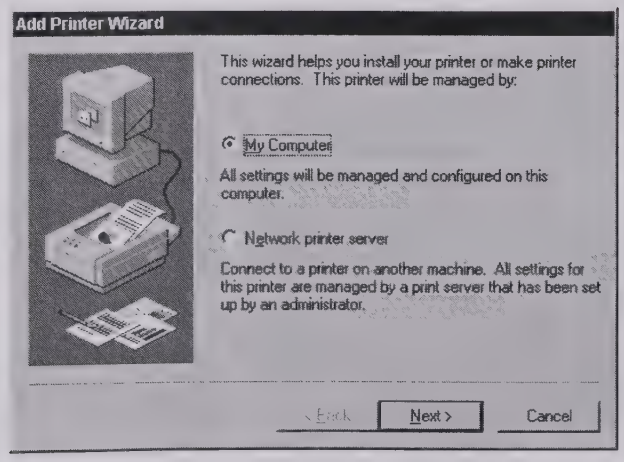
Add Printer Wizard
This wizard helps you install your printer or make printer connections. This printer will be managed by:
My Computer
All settings will be managed and configured on this computer.
Network printer server
Connect to a printer on another machine. All settings for this printer are managed by a print server that has been set up by an administrator.
< Back
Next >
Cancel

➢ Click "My computer" and then "Next".

The available printer ports are displayed.

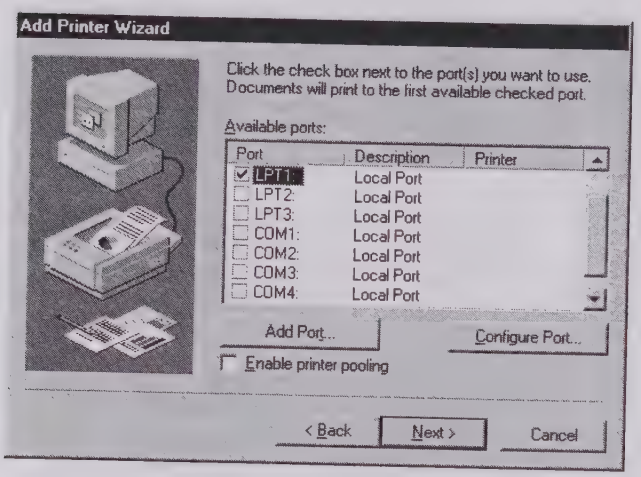

➢ Select LPT1.

The selection is marked by a tick.

➢ "Click "Next".

The available printer drivers are displayed. The left-hand selection table indicates the manufacturers and the right-hand one the available printer drivers.

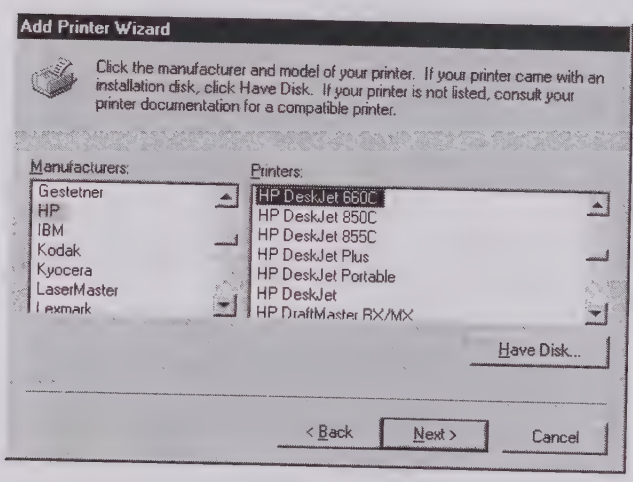

➢ Mark "HP" in selection table "Manufacturers" and "HP DeskJet 660C" in selection table "Printers".

Note:
If the required type of output device is not included in the list, the driver has not yet been installed. In this case click on button "HAVE DISK". A message box requesting to insert a disk with the corresponding printer driver will be displayed. Insert the disk, press OK and select the required printer driver. After installation, Service Pack 5 must be re-installed (see section "Installing Windows NT Software").

➢ Click "Next".

The entry field for the printer name is displayed.

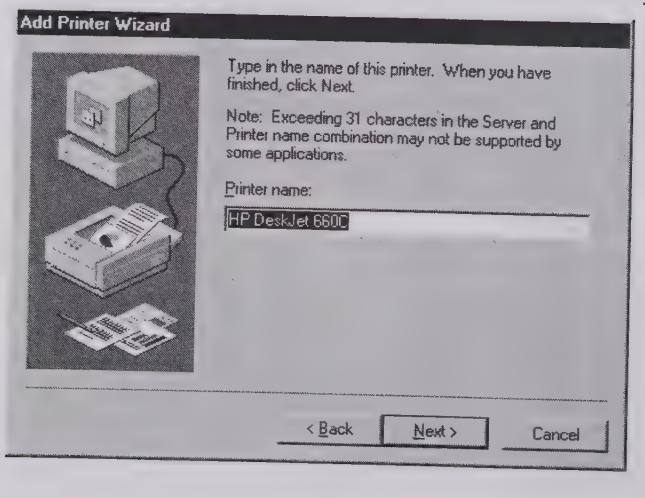
Add Printer Wizard
Type in the name of this printer. When you have finished, click Next.
Note: Exceeding 31 characters in the Server and Printer name combination may not be supported by some applications.
Printer name:
HP DeskJet 660C
< Back
Next >
Cancel

➢ The printer name can be modified in the entry field "Printer name" (max. 60 characters).

If one or more printers are already installed, a query is displayed in this window to ask if the printer last installed as default printer should be selected for the Windows NT applications (Do you want your Windows-based programs to use this printer as default printer?). The default selection is "No".

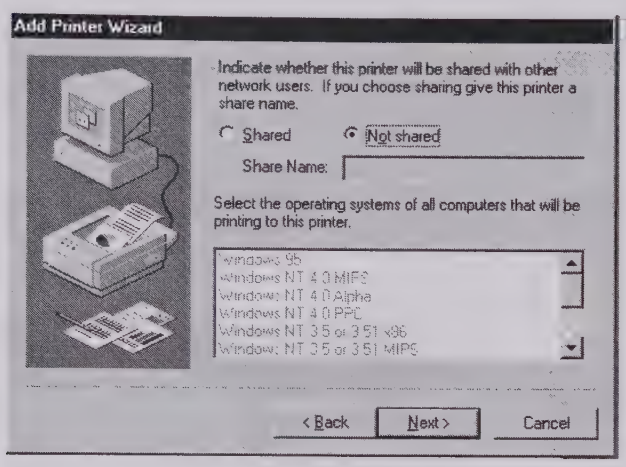
Add Printer Wizard
Indicate whether this printer will be shared with other network users. If you choose sharing give this printer a share name.
Shared
Not shared
Share Name:
Select the operating systems of all computers that will be printing to this printer.
Windows 95
Windows NT 4.0 MIPS
Windows NT 4.0 Alpha
Windows NT 4.0 PPC
Windows NT 3.5 or 3.51 x86
Windows NT 3.5 or 3.51 MIPS
< Back
Next >
Cancel

➢ "Click "Next".

A query is displayed for providing the printer in the network. This query is irrelevant when installing a local printer. The default selection is "Not shared".

➢ Click "Next".

The window for starting a test page print is displayed. The test page is helpful for checking if the installation was successful.

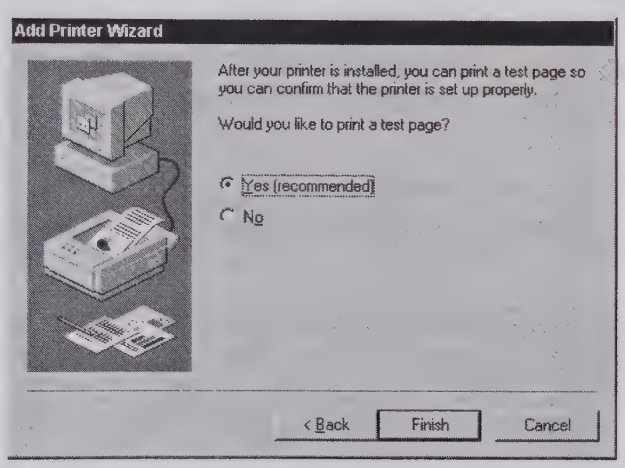
Add Printer Wizard
After your printer is installed, you can print a test page so you can confirm that the printer is set up properly.
Would you like to print a test page?
Yes (recommended)
No
< Back
Finish
Cancel

➢ Click Yes (recommended)".

➢ Click "Finish".

A test page is printed if the installation was successful.
If the test page is not printed or not printed completely, the Windows NT online help offers troubleshooting instructions under the topic "Printer Trouble Shooting".

Note:
If a prompt for the printer driver path appears after pressing "Finish", the Service Pack must be re-installed after this printer installation (see Chapter 1, section "Installing Windows NT Software").

Now the instrument needs to be configured for creating hardcopies of the measurement screen using this printer.

Configuring HP DeskJet 660C.

➢ Click button "R&S Analyzer Interface".

The measurement screen is displayed.

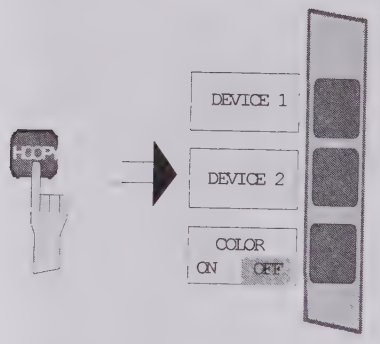

➢ Press the *HCOPY* key.

The *HCOPY* menu is opened.

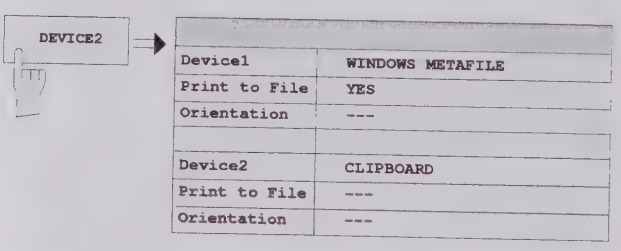

➢ Press softkey *DEVICE2.*

DEVICE 2 is activated as printing device.

The *HARDCOPY DEVICE SETTINGS*-table is opened and the current settings of the two output devices are displayed. The current selection in line DEVICE2 is highlighted by the selection bar.

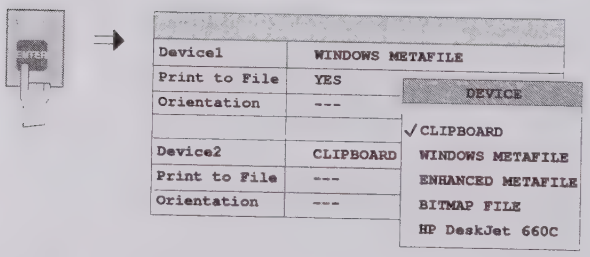

➢ Press the *ENTER* key.

The selection box *DEVICE* is displayed on the screen. The current selection is marked by a tick.

➢ Press cursor key ⓘ until the entry *HP DeskJet 660C* is highlighted by the selection bar.

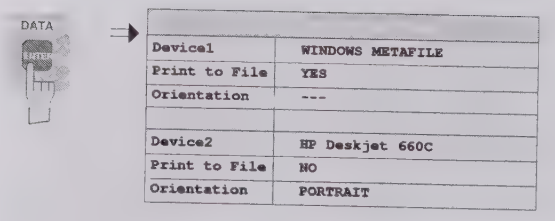

➢ Press the *ENTER* key.

The selection box *DEVICE* is closed and *HP DeskJet 660C* is entered in line *DEVICE2.*

Note:
The selection of the printer type automatically sets the parameters PRINT TO FILE and ORIENTATION to values which correspond to a standard mode with this output device. Other printer-dependent parameters such as PAPERSIZE, can be modified under Windows NT in the printer properties window (START / SETTINGS / PRINTER / SETTINGS).

Start print of measurement results

➢ Press Softkey *PRINT SCREEN* to start the print job.

Installation of a Network Printer (with option FSP-B16 only)

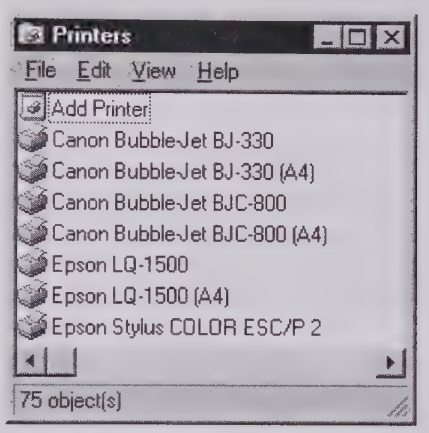

After opening the "Printers" dialog window proceed with the installation as follows:

➢ Double-click the "Add Printer" line.

The "Add Printer Wizard" window is opened. This window guides the user through the printer driver installation.

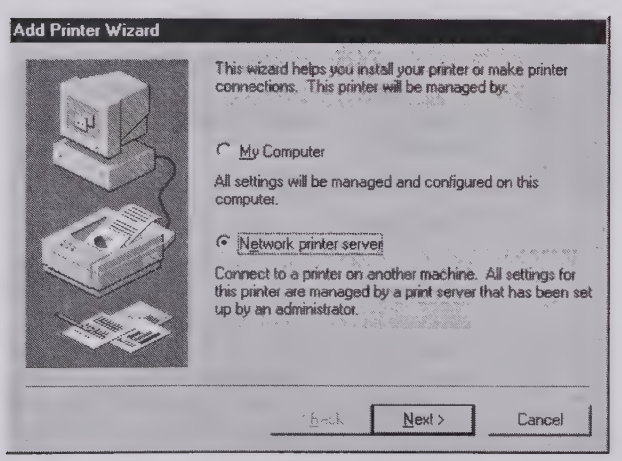
Add Printer Wizard
This wizard helps you install your printer or make printer connections. This printer will be managed by:
My Computer
All settings will be managed and configured on this computer.
Network printer server
Connect to a printer on another machine. All settings for this printer are managed by a print server that has been set up by an administrator.
< Back
Next >
Cancel

➢ Click "Network printer server" and then "Next".

A list of selectable printers is displayed.

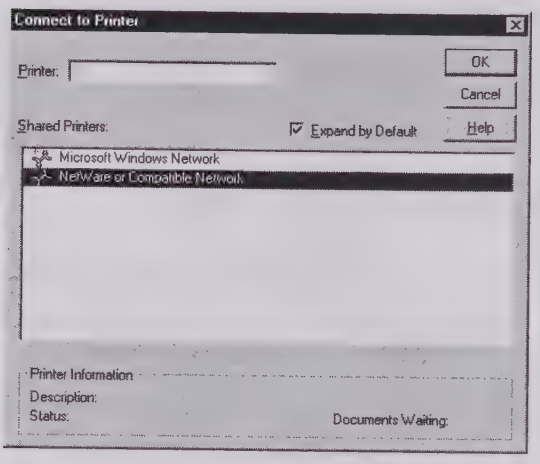

➢ Mark the desired printer and select it with OK.

➢ Confirm the following request for the installation of a suitable printer driver with OK.

The list of printer drivers is displayed. The manufacturers are listed in the window at the left, the available printer drivers at the right.

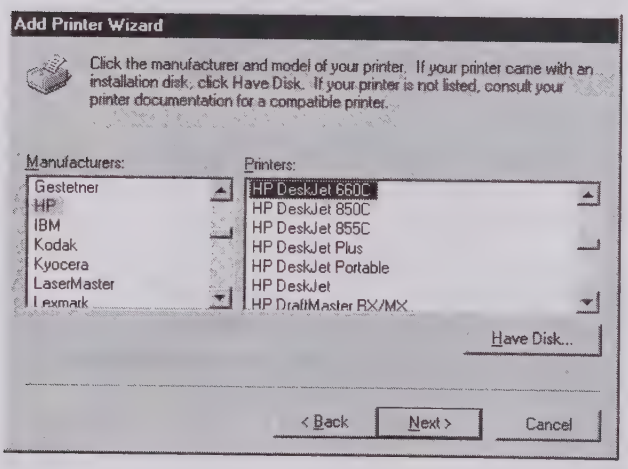

➢ Select the manufacturer in the "Manufacturers" window and then the printer driver in the "Printers" window.

Note:
If the required type of output device is not included in the list, the driver has not yet been installed. In this case click on button "HAVE DISK". A message box requesting to insert a disk with the corresponding printer driver will be displayed. Insert the disk, press OK and select the required printer driver. After installation, Service Pack 5 must be re-installed (see section "Installing Windows NT Software").

➢ Click "Next"

If one or more printers are already installed, a prompt is displayed in this window to ask if the printer last installed as default printer should be selected for the Windows NT applications ("Do you want your Windows-based programs to use this printer as default printer?"). The default selection is "No".

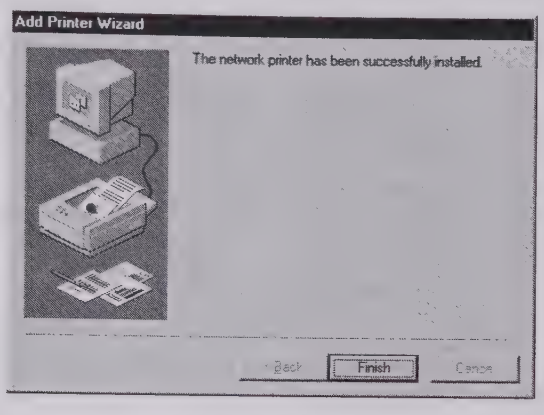

➢ Start the printer driver installation with "Finish".

Note:
If a prompt for the printer driver path appears after pressing "Finish", the Service Pack must be re-installed after this printer installation (see Chapter 1, section "Installing Windows NT Software").

Finally, the instrument has to be configured for printout with this printer using the DEVICE 1 and DEVICE 2 softkeys in the hardcopy menu.

Installing Windows NT Software

The driver software and the system settings of Windows NT are adapted to the measurement functions of the instrument. Correct operation of the instrument can therefore only be guaranteed if the software and hardware used is authorized or offered by Rohde & Schwarz.
The use of other software or hardware may cause failures in the functions of the FSP.
A current list of the software authorized for use on the FSP can be obtained from your nearest Rohde&Schwarz agency (see list of addresses).

After installing any software of other manufacturers from a disk, it is necessary to re-install Service Pack 5 of Windows NT:

Re-installing Service Pack 5

➢ In the Start menu press "Run".

A data entry window is opened.

➢ Enter "C:\SP\SP5I386E.EXE" into the command line and start the installation with "OK".

The following window leads through the installation.

Contents - Chapter 2 "Getting Started"

2 Getting Started 2.1

Level and Frequency Measurements 2.1

Measurement Example 1 – Measuring Frequency and Level using Markers 2.1

Measurement Example 2 – Measuring Frequency with the Frequency Counter 2.3

Measurement of Harmonics 2.5

Measuring Harmonics with Frequency Sweeps 2.7

Measurement Example – Measuring the distance between fundamental wave and the 2nd and 3rd harmonics of the internal reference signal 2.7

High-Sensitivity Harmonics Measurements 2.10

Measurement Example 2.10

Measuring the Spectra of complex Signals 2.13

Separating Signals by Selecting an Appropriate Resolution Bandwidth 2.13

Measurement Example - Resolving two signals with a level of –30 dBm each and a frequency difference of 30 kHz 2.14

Intermodulation Measurements 2.17

Measurement Example – Measuring the FSP's intrinsic intermodulation distance 2.19

Measuring Signals in the Vicinity of Noise 2.23

Measurement example – Measuring the level of the internal reference generator at low S/N ratios 2.25

Noise Measurements 2.28

Measuring noise power density 2.28

Measurement example – Measuring the intrinsic noise power density of the FSP at 1 GHz and calculating the FSP's noise figure. 2.28

Measurement of Noise Power within a Transmission Channel 2.31

Measurement Example – Measuring the intrinsic noise of the FSP at 1 GHz in a 1.23 MHz channel bandwidth with the channel power function 2.31

Measuring Phase Noise 2.35

Measurement Example -
Measuring the phase noise of a signal generator at a carrier offset of 10 kHz. 2.35

Measurements on Modulated Signals 2.37

Measurements on AM signals 2.37

Measurement Example 1 –
Displaying the AF of an AM signal in the time domain. 2.37

Measurement Example 2 - .....

Measuring the modulation depth of an AM carrier in the frequency domain. 2.39

Measurements on FM Signals 2.40

Measurement Example - Displaying the AF of an FM carrier 2.40

Measuring Channel Power and Adjacent Channel Power 2.43

Measurement Example 1 - ACPR measurement on an IS95 CDMA Signal 2.44

Measurement Example 2 – Measuring the adjacent channel power of an IS136 TDMA signal 2.48

Measurement Example 3 - Measuring the Modulation Spectrum in Burst Mode with the Gated Sweep Function 2.51

Measurement Example 4 - Measuring the Transient Spectrum in Burst Mode with the Fast ACP function 2.53

Measurement Example 5 - Measuring adjacent channel power of a W-CDMA uplink signal 2.55

Amplitude distribution measurements 2.58
Measurement Example – Measuring the APD and CCDF of white noise generated by the FSP 2.58
Time Domain Measurements 2.61
Power measurements 2.61
Measurement Example – Measuring the power of a GSM burst during the switch-on phase 2.61
Power Ramping Measurement for Burst Signals 2.63
Measurement Example – Measurements on GSM burst edges using a high time resolution 2.63
Measuring the S/N Ratio of Burst Signals 2.65
Measurement Example - S/N ratio of a GSM signal 2.65

2 Getting Started

Chapter 2 explains how to operate the FSP using typical measurements as examples. Chapter 3 describes the basic operating steps such as selecting the menus and setting parameters, and explains the screen structure and displayed function indicators.
Chapter 4 describes all the menus and FSP functions.

All of the following examples are based on the standard settings of the analyzer. These are set with the *PRESET* key. A complete listing of the standard settings can be found in chapter 4, section "Preset settings of the FSP – *PRESET key*".

Level and Frequency Measurements

Measuring the frequency and level of a signal is one of the most common purposes for the use of a spectrum analyzer. For unknown signals, the spectrum analyzer default settings (PRESET) are a good starting point for the measurement.
If signal levels at the RF input are expected to be above 30 dBm (= 1 W), a power attenuator must be connected to the RF input of the spectrum analyzer. Please note that the total powar of all applied signals must be taken into account concerning this limit. If a power attenuator is not used, signal levels above 30 dBm can destroy the RF attenuator or the input mixer.

Measurement Example 1 – Measuring Frequency and Level using Markers

It is easy to measure the level and frequency of a sinewave carrier with the marker function. At the marker position, the FSP indicates the signal's amplitude and frequency. The accuracy of the frequency measurement is determined by the FSP reference frequency, the resolution of the marker frequency display and the resolution of the screen.

In the example, the frequency of the 128-MHz internal reference generator is displayed using the marker.

1. ***Set the spectrum analyzer to its default settings.***
   - Press the *PRESET* key.
2. ***Connect the test signal to the RF INPUT on the instrument front panel.***
3. ***Switch on the internal reference generator.***
   - Press the *SETUP* key.
     The *SETUP* menu opens.
   - Press the *SERVICE soft*key.
     The *SETUP - SERVICE* menu opens.
   - Press the *INPUT CAL soft*key.
     The internal reference generator is turned on.
     The FSP's RF input is turned off.
4. ***Set the center frequency to 128 MHz.***
   - Press the *FREQ* key.
   - The entry field for the center frequency is displayed on the screen.
   - Enter *128* from the numeric keypad and terminate the entry with the *MHz* key.

5. ***Reduce the measurement frequency range (SPAN) to 1 MHz.***

   ➢ Press the *SPAN* key.

   ➢ Enter *1* from the numeric keypad and terminate the entry with the *MHz* key.

Note:	*If the SPAN is changed, the resolution bandwidth (RES BW), the video bandwidth (VIDEO BW) and the sweep time (SWEEP TIME) are also set to new values because they are defined as coupled functions in the standard PRESET settings.*

6. ***Measure the level and frequency using the marker and read off the results from the screen.***

   ➢ Press the MKR key.
   The marker is switched on and automatically jumps to the trace peak.

Note:	*When a marker is switched on for the first time, it automatically performs the PEAK SEARCH function (as in this example).* *If a marker is already active, the PEAK softkey in the MKR-> menu must be pressed in order to set the currently active marker onto the displayed signal maximum.*

   The level and frequency indicated by the marker are displayed in the marker info field at the upper edge of the screen. These are the measurement results.

   The info-field header indicates the number of the marker (`MARKER 1`) and the number of the trace on which the marker is positioned (`[T1]` = Trace 1).

Increasing the Frequency Resolution During a Frequency Measurement with a Marker

The frequency resolution of the marker is determined by the pixel resolution of the trace. The FSP uses 501 pixels for a trace, i.e. at a frequency span of 1 MHz each pixel corresponds to a frequency range of approx. 2 kHz. This gives a maximum error of 1 kHz.
To increase the pixel resolution of the trace, the frequency span has to be reduced.

7. ***Reduce the frequency span to 10 kHz.***

   ➢ Press the *SPAN* key.

   ➢ Enter *10* from the numeric keypad and terminate the entry with the *kHz* key.

Note:	*If the SPAN is changed, the resolution bandwidth (RES BW), the video bandwidth (VIDEO BW) and the sweep time (SWEEP TIME) are also set to new values because they are defined as coupled functions in the standard PRESET settings.*

   The internal reference signal is measured with a span of 10 kHz. The pixel resolution of the trace is now approx. 20 Hz (10 kHz span / 501 pixel), i.e. the accuracy of the marker frequency display is increased to approx. 10 Hz.

8. ***Switch on the RF input again for normal operation of the analyzer.***

   ➢ Press the *PRESET* key *or* press the *SETUP* key and the *SERVICE* softkey.

   ➢ Press the *INPUT RF* softkey.
   The internal signal path of the FSP is switched back to the RF input in order to resume normal operation.

Measurement Example 2 – Measuring Frequency with the Frequency Counter

With the internal frequency counter, frequencies can be measured more accurately than with the marker. The frequency sweep is stopped at the marker position and the FSP measures the frequency of the corresponding signal. If an analog bandwidth (≥300 kHz) is used, the frequency is measured by counting the zero-crossings of the last IF. With digital resolution bandwidths (10 Hz to 100 kHz), the frequency measurement is performed in the IQ baseband by a special approximation algorithm.

The resolution range for the frequency measurement is 0.1 Hz to 10 kHz. At bandwidths ≥300 kHz, the time required for the FSP to perform the frequency measurement is dependent on the selected counter resolution (1/(frequency resolution in Hz)). The digital frequency approximation takes about 30 ms to perform a frequency measurement irrespective of the selected resolution.
The frequency measurement accuracy is determined by the reference frequency of the FSP and the selected counter resolution.

In the example, the frequency of the 128-MHz internal reference generator is displayed with the marker.

1. ***Set the spectrum analyzer to the default settings.***

   ➢ Press the *PRESET* key.
   The FSP is in its default state.

2. ***Switch on internal reference generator***

   ➢ Press the *SETUP* key.

   ➢ Press the softkeys *SERVICE - INPUT CAL.*
   The internal 128 MHz reference generator is now on. The FSP's RF input is turned off.

3. ***Set the center frequency and the frequency span***

   ➢ Press the *FREQ* key and enter *128 MHz.*
   The FSP center frequency is set to 128 MHz.

   ➢ Press the *SPAN* softkey and enter *1 MHz.*
   The FSP frequency span is set to 1 MHz.

4. ***Switch on the marker***

   ➢ Press the *MKR* key.
   The marker is switched on and set to the signal maximum. The level and the frequency at the marker are displayed in the marker-info field.

5. ***Switch on the frequency counter.***

   ➢ Press the *SIGNAL COUNT* softkey in the marker menu.
   The frequency count is displayed in the marker field at the top of the screen along with the set resolution (1 kHz is the default setting).
   The sweep stops at the marker position and the FSP measures the frequency of the corresponding signal. The frequency is output in the marker info field. To distinguish the signal count result from the normal marker frequency display, the marker is labeled with CNT.

6. Set the resolution of the frequency counter to 1 Hz.

➢ Press the *NEXT* key.

➢ Press the *CNT RESOL 1 Hz* softkey.

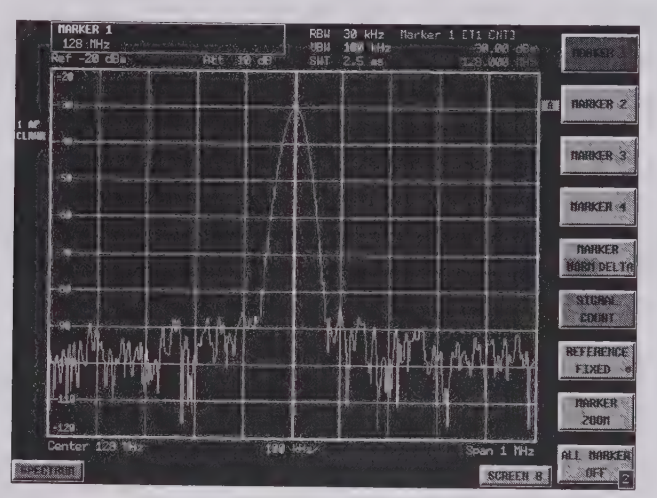

Fig. 2-1 Frequency measurement with a frequency counter

Note:	*The frequency measurement with the integral frequency counter only gives correct results for RF sinewaves or discrete spectral lines. To meet the specified measurement accuracy, the marker should be more than 25 dB above noise.*

7. Switch on the RF input again for normal operation of the analyzer.

➢ Press the *PRESET* key *or* press the *SETUP* key and the *SERVICE* softkey.

➢ Press the *INPUT RF* softkey.
The internal signal path of the FSP is switched back to the RF input in order to resume normal operation.

Hint:	For bandwidths between 300 kHz and 10 MHz, the FSP uses a frequency counter at an IF of 20.4 MHz. The time for measuring the frequency is, therefore, inversely proportional to the selected resolution, i.e. at a resolution of 1 Hz a gate time of 1 second is required for the counter. For digital bandwidths below 300 kHz, the frequency is measured in the baseband by digital frequency approximation. The time required for measuring the frequency is approx. 30 ms irrespective of the selected resolution. When measuring the frequency of a sinewave carrier at a high resolution it is, therefore, best to set a resolution bandwidth of 100 kHz or less. The measurement time will then be reduced to a minimum.

Measurement of Harmonics

Measuring the harmonics of a signal is a frequent problem which can be solved best by means of a spectrum analyzer. In general, every signal contains harmonics which are larger than others. Harmonics are particularly critical regarding high-power transmitters such as transceivers because large harmonics can interfere with other radio services.

Harmonics are produced by nonlinear characteristics. They can often be reduced by lowpass filters. Since the spectrum analyzer has a nonlinear characteristic, e.g. in its first mixer, measures must be taken to ensure that harmonics produced in the analyzer do not cause spurious results. If necessary, the fundamental wave must be selectively attenuated with respect to the other harmonics with a highpass filter.

When harmonics are being measured, the obtainable dynamic range depends on the K2 intercept of the spectrum analyzer. The K2 intercept is the virtual input level at the RF input mixer at which the level of the 2nd harmonic becomes equal to the level of the fundamental wave. In practice, however, applying a level of this magnitude would damage the mixer. Nevertheless the available dynamic range for measuring the harmonic distance of a DUT can be calculated relatively easily using the second harmonic intercept.

As shown in Fig. 2-2, the level of the 2nd harmonic is reduced by 20 dB if the level of the fundamental wave is reduced by 10 dB.

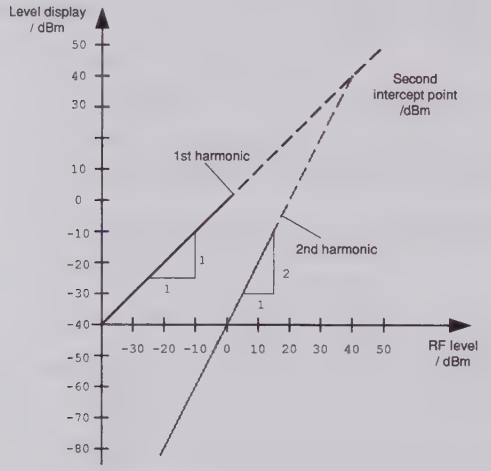

Fig. 2-2 Extrapolation of the 1st and 2nd harmonics to the second harmonic intercept at 40 dBm

The following formula for the obtainable harmonic distortion d_2 in dB is derived from the straight-line equations and the given intercept point:

$$d_2 = S.H.I - P_I \quad (1)$$

d_2 = harmonic distortion
P_I = mixer level/dBm
S.H.I. = second harmonic intercept

Note: *The mixer level is the applied RF level minus the set RF attenuation.*

The formula for the internally generated level P_1 at the 2nd harmonic in dBm is:

$$P_1 = 2 \cdot P_I - S.H.I. \quad (2)$$

The lower measurement limit for the harmonic is the noise floor of the spectrum analyzer. The harmonic of the measured DUT should – if sufficiently averaged by means of a video filter – be at least 4 dB above the noise floor so that the measurement error due to the input noise is less than 1 dB.

The following rules for measuring high harmonic ratios can be derived:

1. Select the smallest possible IF bandwidth for a minimal noise floor.
2. Select an RF attenuation which is high enough to just measure the harmonic ratio.

The maximum harmonic distortion is obtained if the level of the harmonic equals the intrinsic noise level of the receiver. The level applied to the mixer, according to (2), is:

$$P_I = \frac{P_{noise} / dBm + IP2}{2}$$

At a resolution bandwidth of 10 Hz (noise level -143 dBm, S.H.I. = 40 dBm), this level is –51.5 dBm. According to (1) a maximum measurable harmonic distortion of 91.5 dB minus a minimum S/N ratio of 4 dB is obtained.

Hint:	If the harmonic emerges from noise sufficiently (approx. >15 dB), it is easy to check (by changing the RF attenuation) whether the harmonics originate from the DUT or are generated internally by the spectrum analyzer. If a harmonic originates from the DUT , its level remains constant if the RF attenuation is increased by 10 dB. Only the displayed noise is increased by 10 dB due to the additional attenuation. If the harmonic is exclusively generated by the spectrum analyzer, the level of the harmonic is reduced by 20 dB or is lost in noise. If both – the DUT and the spectrum analyzer – contribute to the harmonic, the reduction in the harmonic level is correspondingly smaller.

Measuring Harmonics with Frequency Sweeps

There are advantages in performing harmonic measurements with a single frequency sweep, provided that the harmonic distance is in a way that a resolution bandwidth can be selected which is wide enough to give an acceptably short sweep time.

Measurement Example – Measuring the distance between fundamental wave and the 2nd and 3rd harmonics of the internal reference signal

1. ***Set the spectrum analyzer to the default settings.***

   ➢ Press the *PRESET* key.
   The FSP is in its default state.

2. ***Switch on the internal reference generator***

   ➢ Press the *SETUP* key.
   Press the softkeys *SERVICE - INPUT CAL*.
   The internal 128 MHz reference generator is now on. The FSP's RF input is switched off.

3. ***Set the start frequency to 100 MHz and the stop frequency to 400 MHz***

   ➢ Press the *FREQ* key.

   ➢ Press the *START* softkey and enter *100 MHz*.

   ➢ Press the *STOP* softkey and enter *400 MHz*.
   The FSP displays the fundamental and the 2nd and 3rd harmonics of the input signal.

4. ***Set the RF attenuation to 0 dB to obtain maximum sensitivity***

   ➢ Press the *AMPT* key.

   ➢ Press the *RF ATTEN MANUAL* softkey and enter *0 dB*.

5. ***Reduce the video bandwidth to average (suppress) noise.***

   ➢ Press the *BW* key.

   ➢ Press the *COUPLING RATIO* softkey.

   ➢ Select *RBW/VBW NOISE [10]* using the cursor keys.

   The video bandwidth (VBW) will now always be set to a value which is 10 times smaller than the resolution bandwidth (RBW).

6. ***Switch on the marker***

   ➢ Press the *MKR* key.
   Marker 1 is switched on and is positioned on the signal maximum (fundamental wave at 128 MHz). The level and the frequency of the marker are displayed in the marker info field.

7. Switch on the delta marker and measure the harmonic distance

➢ Press the *MARKER 2* softkey in the marker menu.
Marker 2 is activated as a delta marker (Delta 2 [T1]). It appears automatically on the largest harmonic of the signal. The frequency and level, related to marker 1, are indicated in the marker field at the top of the screen.

➢ Press the *MARKER 3* softkey in the marker menu.
Marker 3 is activated as a delta marker (Delta 3 [T1]). It appears automatically on the next largest harmonic of the signal. The frequency and level, related to marker 1 on the fundamental wave, are displayed in the marker info field at the top of the screen (see Fig. 2-3).

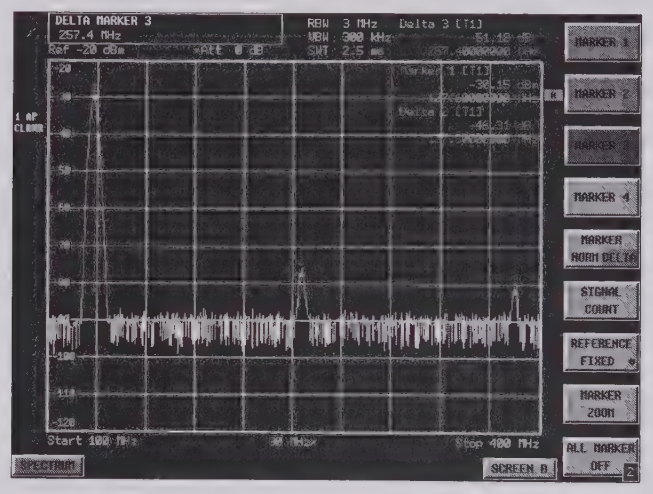

Fig. 2-3 Measuring the harmonic distance of the internal reference generator. Delta marker 2 [T1] and Delta marker 3 [T1] indicate the distance between the fundamental wave and the 2nd and 3rd harmonics.

In order to make the harmonics grow out of the noise, the following things can be done:

- Reducing the video bandwidth
- Averaging the trace
- Reducing the resolution bandwidth

The noise of the analyzer or the DUT (depending on which one is higher) is suppressed by reducing the video bandwidth and by averaging the trace. Especially for low S/N ratios, the measurement uncertainty is reduced using the two averaging methods since the signal under test is also freed from noise.

8. Reduce noise by reducing the video bandwidth

➢ Press the *BW* key.

➢ Press the *VIDEO BW MANUAL* softkey.

➢ Reduce the video bandwidth, e.g. to 10 kHz, using the spinwheel (turn knob counterclockwise), or enter *10 kHz.*

The noise is clearly smoothed and the sweep time is increased to 25 ms, i.e. the measurement lasts longer. The displayed video bandwidth is marked with an asterisk (*VBW) to indicate that it is no longer coupled to the resolution bandwidth (see Fig. 2-4).

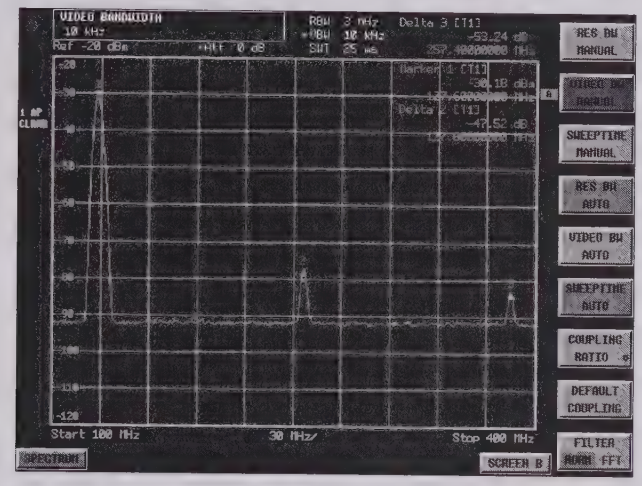

Fig. 2-4 Suppression of noise during harmonic measurement by reducing video bandwidth

9. Coupling the video bandwidth to the resolution bandwidth again.

➢ Press the *VIDEO BW AUTO* softkey.

10. Reduce noise by averaging the trace

➢ Press the *TRACE* key.

➢ Press the *AVERAGE* softkey.
The noise component of the trace is smoothed by averaging 10 consecutive traces.

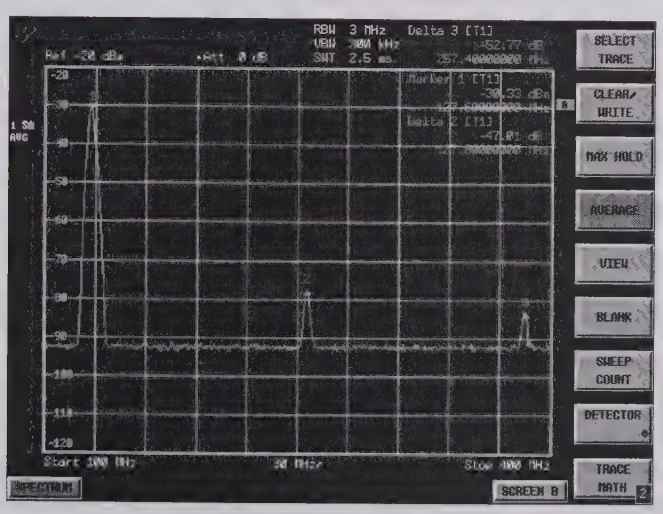

Fig. 2-5 Suppression of noise during harmonic measurements by averaging the trace

11. Switch off trace averaging again.

➢ Press the *CLEAR/WRITE* softkey.

12. Reduce noise by reducing the measurement bandwidth.

If the resolution bandwidth is decreased, noise is reduced proportionally, i.e. if the resolution bandwidth is reduced by a factor of 10, the noise is also reduced by the same factor (corresponds to 10 dB). The amplitude of a sinusoidal signal is not changed by reducing the resolution bandwidth.

13. Set the resolution bandwidth to 10 kHz.

- Press the *BW* key.
- Press the *RES BW MANUAL* softkey and enter *10 kHz*.
  The noise is reduced by approx. 25 dB compared to the previous setting. Since the video bandwidth is coupled to the resolution bandwidth, it is reduced to 1 kHz – the same proportional reduction as the resolution bandwidth. The sweep time is therefore increased to 60 seconds.

14. Reset the resolution bandwidth again (coupling to span).

- Press the *RES BW AUTO* softkey.

If you want to stop the harmonics measurement on the internal reference generator at this point, switch the FSP's RF input on again with the following key sequence.

- Press the *SETUP* key and the softkey sequence *SERVICE - INPUT RF* or press the *PRESET* key.

High-Sensitivity Harmonics Measurements

If harmonics have very small levels, the resolution bandwidth required to measure them must be reduced considerably. The sweep time is, therefore, also increased considerably. In this case, the measurement of individual harmonics is carried out with the spectrum analyzer set to a small span. Only the frequency range around the harmonics will then be measured with a small resolution bandwidth.

Measurement Example

1. Set the spectrum analyzer to its default settings.

- Press the *PRESET* key.
  The FSP is in its default state.

2. Switch on the internal reference generator.

- Press the *SETUP* key.
- Press the softkeys *SERVICE - INPUT CAL*.
  The internal 128 MHz reference generator is now on. The FSP's RF input is switched off.

3. Set the center frequency to 128 MHz and the span to 100 kHz.

- Press the *FREQ* key.
  The frequency menu opens.
- Enter *128* in the entry field from the numeric keypad and terminate with the *MHz* key.
- Press the *SPAN* key.
- Enter *100* in the entry filed from the numeric keypad and terminate with the *kHz* key.
  The FSP displays the reference signal with a span of 100 kHz and resolution bandwidth of 3 kHz.

4. *Switching on the marker.*

➢ Press the *MKR* key.
The marker is positioned on the trace maximum.

5. *Set the measured signal frequency and the measured level as reference values*

➢ Press the *REFERENCE FIXED* softkey.

➢ The position of the marker becomes the reference point. The reference point level is indicated by a horizontal line, the reference point frequency with a vertical line. At the same time, the delta 2 marker is switched on at the marker position.

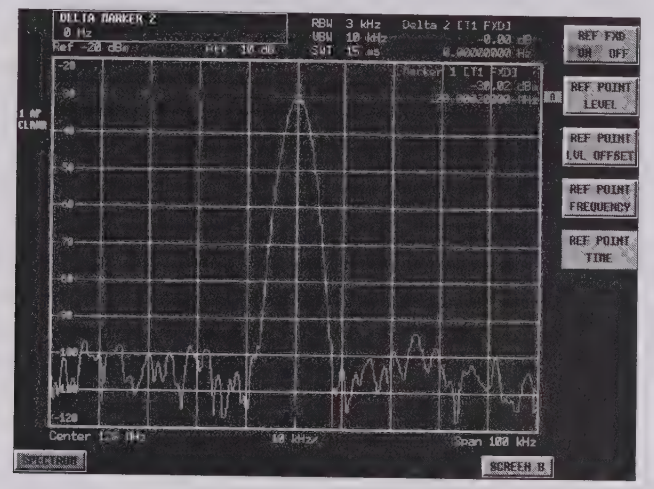

Fig. 2-6 Fundamental wave and the frequency and level reference point

6. *Make the step size for the center frequency equal to the signal frequency*

➢ Press the *FREQ* key.
The frequency menu opens.

➢ Press the *CF STEPSIZE* softkey and press the *=MARKER* softkey in the submenu.
The step size for the center frequency is now equal to the marker frequency.

7. *Set the center frequency to the 2nd harmonic of the signal*

➢ Press the *FREQ* key.
The frequency menu open. s

➢ Press the up cursor key (below the spinwheel) once.
The FSP's center frequency is set to the 2nd harmonic.

8. *Place the delta marker on the 2nd harmonic.*

➢ Press the *MKR →* key.

➢ Press the *PEAK* softkey.
The delta marker jumps to the maximum of the 2nd harmonic. The displayed level result is relative to the reference point level (= fundamental wave level).

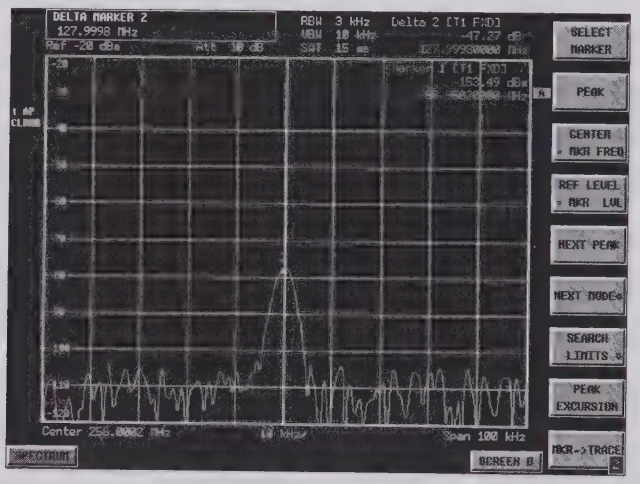

Fig. 2-7 Measuring the level difference between the fundamental wave (= reference point level) and the 2nd harmonic

The other harmonics are measured with steps 6 and 7, the center frequency being incremented or decremented in steps of 128 MHz using the up or down cursor key.

Measuring the Spectra of complex Signals

Separating Signals by Selecting an Appropriate Resolution Bandwidth

One basic characteristics of the spectrum analyzer is that it can separate the spectral components of a composite signal. The resolution with which the individual components are separated is determined by the resolution bandwidth. If the resolution bandwidth is too large, spectral components may no longer be distinct, i.e. they are displayed as a single component.

An RF sinewave signal is displayed on the screen of the spectrum analyzer with the passband characteristics of the set resolution filter (RBW). It is the 3 dB bandwidth of the filter that is displayed.

Two signals with the same amplitude can be resolved if the resolution bandwidth is less than or equal to the signals' frequency difference. If the resolution bandwidth and the frequency difference are equal, a 3 dB level dip can be seen in the middle between the two signals. The smaller the resolution bandwidth, the deeper the level dip and the better the signal resolution.

If there are large level differences between signals, the resolution is determined by selectivity as well as by the resolution bandwidth that has been selected. The measure of selectivity used for spectrum analyzers is the ratio of the 60 dB bandwidth to the 3 dB bandwidth (= shape factor).

For the FSP, the shape factor for bandwidths up to 100 kHz is < 5 and for larger bandwidths < 15, i.e. the 60 dB bandwidth of the 30 kHz filter is < 150 kHz and that of the 300 kHz filter is < 4.5 MHz. Although the 3 dB bandwidths only differ by a factor of 10, the 60 dB bandwidths differ by a factor of 30.

The higher spectral resolution with smaller bandwidths has to be traded off against longer sweep times for the same span. The sweep time required to allow the resolution filters to settle during a sweep at all signal levels and frequencies to be displayed is given by the following formula.

$$SWT = k \bullet Span/RBW^2 \qquad (1)$$

SWT = max. sweep time for correct measurement
k = factor depending on type of resolution filter
= 2.5 for analog IF filter (≥300 kHz)
= 1 for digital IF filters (≤ 100 kHz)
Span = frequency display range
RBW = resolution bandwidth

If the resolution bandwidth is reduced by a factor of 3, the sweep time is increased by a factor of 9.

Note: *The impact of the video bandwidth on the sweep time is not taken into account in (1). For the formula to be valid, the video bandwidth must be ≥ 3 x the resolution bandwidth.*

For bandwidths > 300 kHz, the FSP uses 4pole, single-section filters. They require a k factor of 2.5 to settle during the frequency sweep. Digital filters with a Gaussian characteristic are used below a bandwidth of 300 kHz (up to 100 kHz). These filters settle at a k factor of 1, i.e. the sweep time is 2.5 times shorter than with conventional 4 or 5 pole, single-section filters.

FFT filters can be used for resolution bandwidths up to 30 kHz. Like digital filters, they have a shape factor of less than 5 up to 30 kHz. For FFT filters, however, the sweep time is given by the following formula:

$$SWT = k \cdot span/RBW \qquad (2)$$

i.e. if the resolution bandwidth is reduced by a factor of 3, the sweep time is increased by a factor of 3 only

Measurement Example - Resolving two signals with a level of –30 dBm each and a frequency difference of 30 kHz

Example:

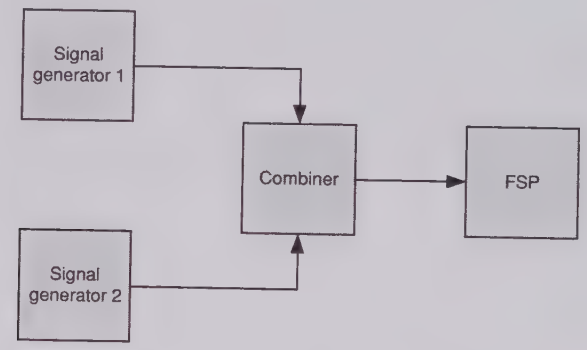

Fig. 2-8 Test setup for generating two signals

Signal generator settings (e.g. SMIQ):

	Level	**Frequency**
Signal generator 1	-30 dBm	100.00 MHz
Signal generator 2	-30 dBm	100.03 MHz

FSP measurement sequence:

1. ***Set the spectrum analyzer to its default settings.***
   - Press the *PRESET* key.
     The FSP is in its default state.
2. ***Set the center frequency to 100.015 MHz and the frequency span to 300 kHz.***
   - Press the *FREQ* key and enter *100.015 MHz*.
   - Press the *SPAN* key and enter *300 kHz*.
3. ***Set the resolution bandwidth is to 30 kHz and the video bandwidth to 1 kHz.***
   - Press the *BW* key.
   - Press the *RES BW MANUAL* softkey and enter *30 kHz*.
   - Press the *VIDEO BW MANUAL* softkey and enter *1 kHz*.
   - The two signals are clearly separated by a 3 dB level dip in the middle of the screen.

> ***Note:*** The video bandwidth is set to 1 kHz to clearly display the level dip in the middle between the two signals. At larger video bandwidths, the video voltage which arises from envelope detection is not sufficiently suppressed. Therefore, additional voltages occur between the two signals and can be seen on the trace.

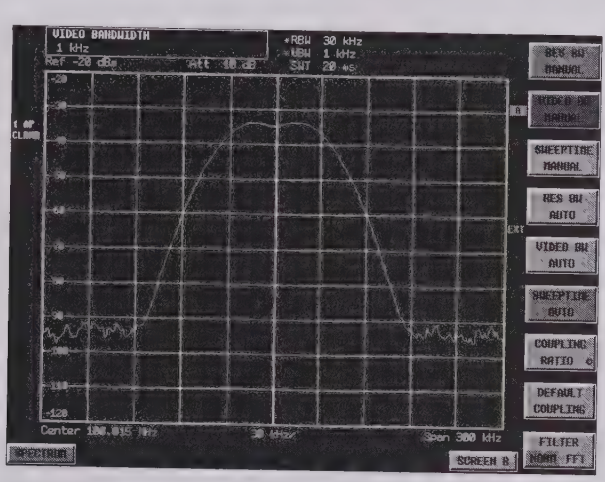

Fig. 2-9 Measurement of two RF sinewave signals with the same level using a resolution bandwidth which corresponds to the frequency difference of the signals.

Note: *The level dip is only exactly in the middle of the screen if the generator frequencies exactly correspond with the frequency display of FSP. To ensure this, the generators and the FSP must have their frequencies synchronized.*

4. *Set the resolution bandwidth to 100 kHz.*

➢ Press the *RES BW MANUAL* softkey and enter *100 kHz*.
The two generator signals can no longer be clearly distinguished.

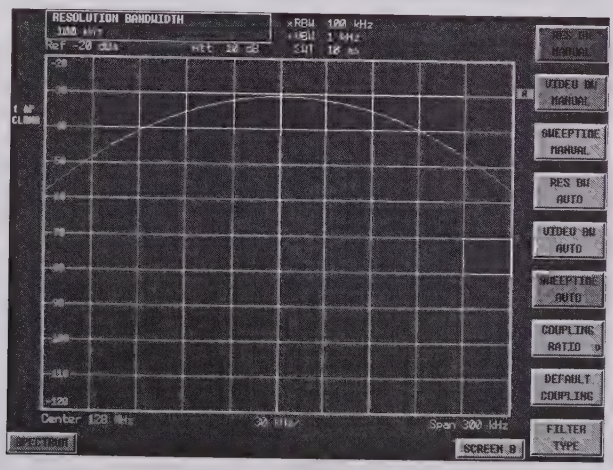

Fig. 2-10 Measurement on two RF sinewave signals with the same level using a resolution bandwidth which is greater than their frequency difference.

The resolution bandwidth (RBW) can be reduced again by turning the spinwheel counterclockwise to obtain a higher frequency resolution.

5. Set the resolution bandwidth to 1 kHz.

➢ Turn the spinwheel counterclockwise until a bandwidth of 1 kHz is displayed.
The two generator signals are displayed at high resolution. The sweep time increases considerably (600 ms) because it increases by 1/ RBW^2. The noise floor also goes down at small resolution bandwidths (10 dB per bandwidth factor of 10).

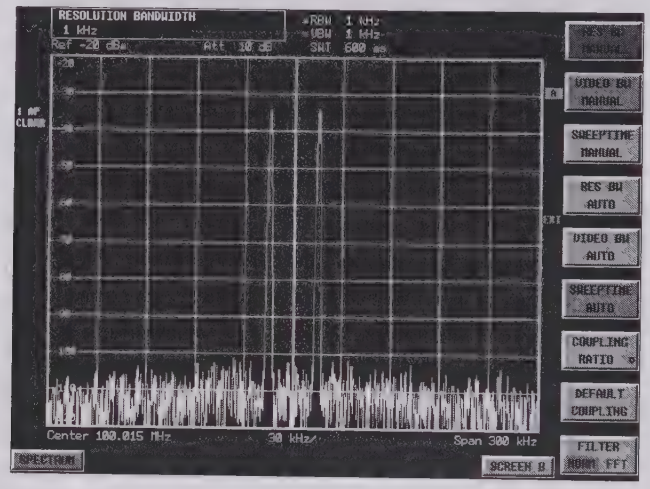

Fig. 2-11 Measurement on two RF sinewave signals with the same level using a resolution bandwidth (1 kHz) which is far below their frequency difference.

6. Switch on the FFT bandwidths.

➢ Set the *FILTER* softkey to *FFT*.
IF filtering is now carried out with the FFT algorithm. The sweep time is considerably reduced from 600 ms to 15 ms (factor of 40). The update rate of the display is increased in almost the same proportion.

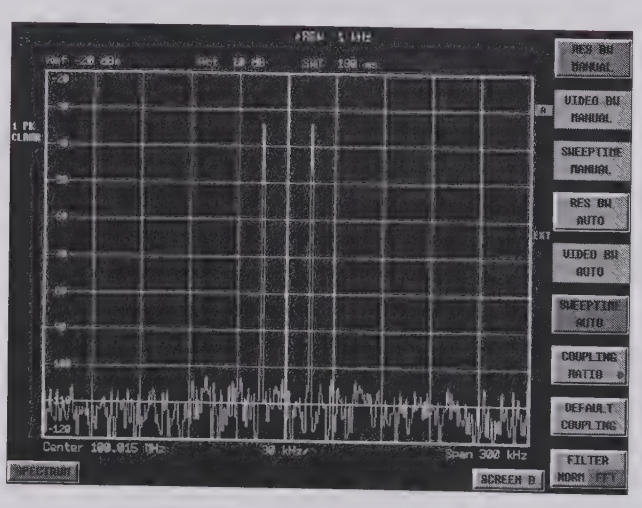

Fig. 2-12 Measurement with FFT filters gives a considerably shorter sweep time and a higher refresh rate.

Intermodulation Measurements

If several signals are applied to a DUT with non-linear characteristics, unwanted mixing products are generated – mostly by active components such as amplifiers or mixers. The products created by 3rd order intermodulation are particularly troublesome as they have frequencies close to the useful signals and, compared with other products, are closest in level to the useful signals. The fundamental wave of one signal is mixed with the 2nd harmonic of the other signal.

$$f_{s1} = 2 \cdot f_{u1} - f_{u2} \quad (1)$$

$$f_{s2} = 2 \cdot f_{u2} - f_{u1} \quad (2)$$

where f_{s1} and f_{s2} are the frequencies of the intermodulation products and f_{u1} and f_{u2} the frequencies of the useful signals.

The following diagram shows the position of the intermodulation products in the frequency domain.

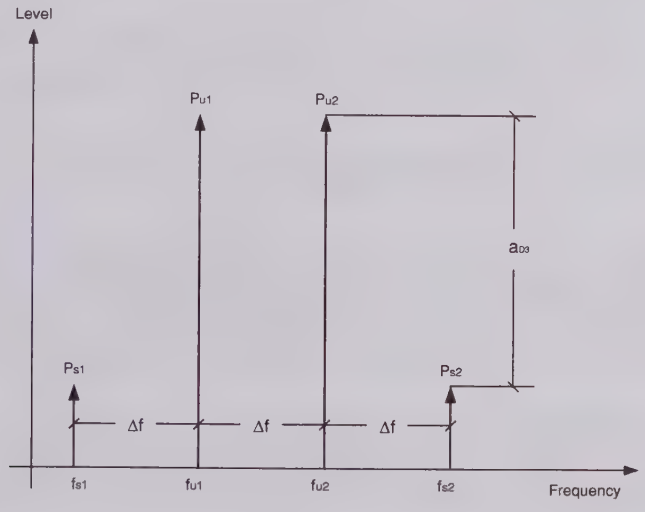

Fig. 2-13 3rd order intermodulation products

Example: f_{u1} = 100 MHz, f_{u2} = 100.03 MHz
$f_{s1} = 2 \cdot f_{u1} - f_{u2} = 2 \cdot 100$ MHz – 100.03 MHz = 99.97 MHz
$f_{s2} = 2 \cdot f_{u2} - f_{u1} = 2 \cdot 100.03$ MHz – 100 MHz = 100.06 MHz

The level of the intermodulation products depends on the level of the useful signals. If the level of the two useful signals is increased by 1 dB, the level of the intermodulation products is increased by 3 dB. The intermodulation distance d_3 is, therefore, reduced by 2 dB. Fig. 2-14 shows how the levels of the useful signals and the 3rd order intermodulation products are related.

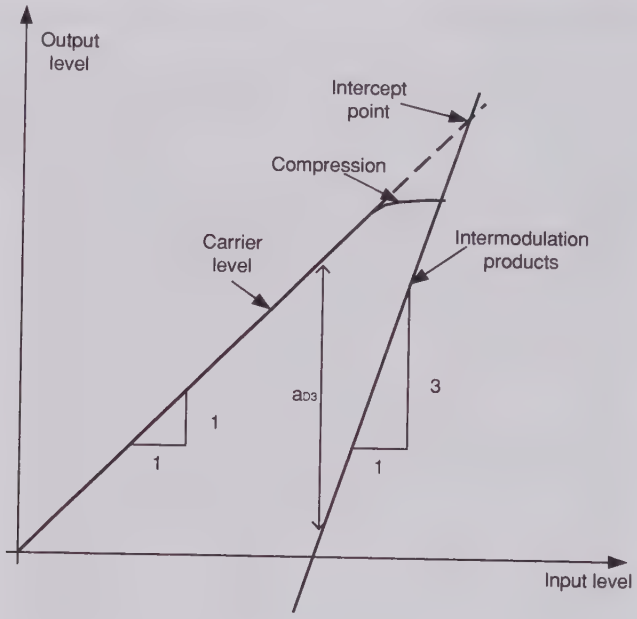

Fig. 2-14 Level of the 3rd order intermodulation products as a function of the level of the useful signals

The behavior of the signals can explained using an amplifier as an example. The change in the level of the useful signals at the output of the amplifier is proportional to the level change at the input of the amplifier as long as the amplifier is operating in linear range. If the level at the amplifier input is changed by 1 dB, there is a 1 dB level change at the amplifier output. At a certain input level, the amplifier enters saturation. The level at the amplifier output does not increase with increasing input level.

The level of the 3rd order intermodulation products increases 3 times faster than the level of the useful signals. The 3rd order intercept is the virtual level at which the level of the useful signals and the level of the spurious products are identical, i.e. the intersection of the two straight lines. This level cannot be measured directly as the amplifier goes into saturation or is damaged before this level is reached.

The 3rd order intercept can be calculated from the known slopes of the lines, the intermodulation distance d_2 and the level of the useful signals.

$$TOI = a_{D3} / 2 + P_n \qquad (3)$$

with TOI (Third Order Intercept) being the 3rd order intercept in dBm and P_n the level of a carrier in dBm.

With an intermodulation distance of 60 dB and an input level, P_w, of –20 dBm, the following 3rd order intercept is obtained:

TOI = 60 dBm / 2 + (-20 dBm) = 10 dBm.

Measurement Example – Measuring the FSP's intrinsic intermodulation distance

To measure the intrinsic intermodulation distance, use the test setup in Fig. 2-8.

Signal generator settings (e.g. SMIQ):

	Level	Frequency
Signal generator 1	-10 dBm	999.9 MHz
Signal generator 2	-10 dBm	1000.1 MHz

Measurement using the FSP:

1. ***Set the spectrum analyzer to its default settings.***
   - Press the *PRESET* key.
     The FSP is in its default state.
2. ***Set center frequency to 1 GHz and the frequency span to 1 MHz.***
   - Press the *FREQ* key and enter 1 GHz.
   - Press the *SPAN* key and enter 1 MHz.
3. ***Set the reference level to –10 dBm and RF attenuation to 0 dB.***
   - Press the *AMPT* key and enter *-10 dBm.*
   - Press the *RF ATTEN MANUAL* softkey and enter 0 dB.
     By reducing the RF attenuation to 0 dB, the level to the FSP input mixer is increased. Therefore, 3rd order intermodulation products are displayed.
4. ***Set the resolution bandwidth to 10 kHz.***
   - Press the *BW* key.
   - Press the *RES BW MANUAL* softkey and enter *10 kHz.*
     By reducing the bandwidth, the noise is further reduced and the intermodulation products can be clearly seen.
5. ***Measuring intermodulation by means of the 3rd order intercept measurement function***
   - Press the *MKR FCTN* key.
   - Press the *TOI* softkey.
     The FSP activates four markers for measuring the intermodulation distance. Two markers are positioned on the useful signals and two on the intermodulation products. The 3rd order intercept is calculated from the level difference between the useful signals and the intermodulation products. It is then displayed on the screen:

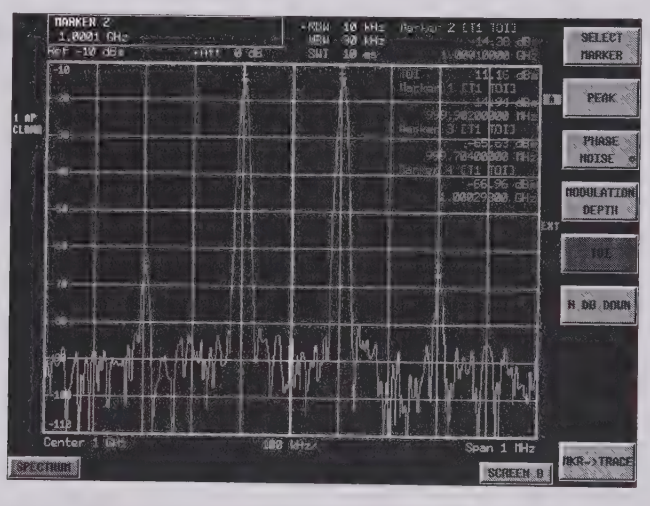

Fig. 2-15 Result of intrinsic intermodulation measurement on the FSP. The 3rd order intercept (TOI) is displayed at the top right corner of the grid

The level of a spectrum analyzer's intrinsic intermodulation products depends on the RF level of the useful signals at the input mixer. When the RF attenuation is added, the mixer level is reduced and the intermodulation distance is increased. With an additional RF attenuation of 10 dB, the levels of the intermodulation products are reduced by 20 dB. The noise level is, however, increased by 10 dB.

6. *Increasing RF attenuation to 10 dB to reduce intermodulation products.*

- Press the *AMPT* key.
- Press the *RF ATTEN MANUAL* softkey and enter *10 dB*.
  The FSP's intrinsic intermodulation products disappear below the noise floor.

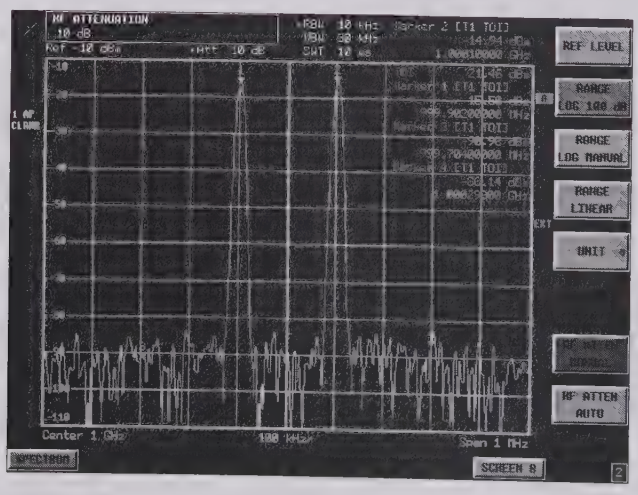

Fig. 2-16 If the RF attenuation is increased, the FSP's intrinsic intermodulation products disappear below the noise floor.

Calculation method:

The method used by the FSP to calculate the intercept point takes the average useful signal level P_u in dBm and calculates the intermodulation d_3 in dB as a function of the average value of the levels of the two intermodulation products. The third order intercept (TOI) is then calculated as follows:

$TOI/dBm = ½\ d_3 + Pu$

Intermodulation- free dynamic range

The **Intermodulation – free dynamic range** , i.e. the level range in which no internal intermodulation products are generated if two-tone signals are measured, is determined by the 3rd order intercept point, the phase noise and the thermal noise of the spectrum analyzer. At high signal levels, the range is determined by intermodulation products. At low signal levels, intermodulation products disappear below the noise floor, i.e. the noise floor and the phase noise of the spectrum analyzer determine the range. The noise floor and the phase noise depend on the resolution bandwidth that has been selected. At the smallest resolution bandwidth, the noise floor and phase noise are at a minimum and so the maximum range is obtained. However, a large increase in sweep time is required for small resolution bandwidths. It is, therefore, best to select the largest resolution bandwidth possible to obtain the range that is required. Since phase noise decreases as the carrier-offset increases, its influence decreases with increasing frequency offset from the useful signals.

The following diagrams illustrate the intermodulation-free dynamic range as a function of the selected bandwidth and of the level at the input mixer (= signal level – set RF attenuation) at different useful signal offsets.

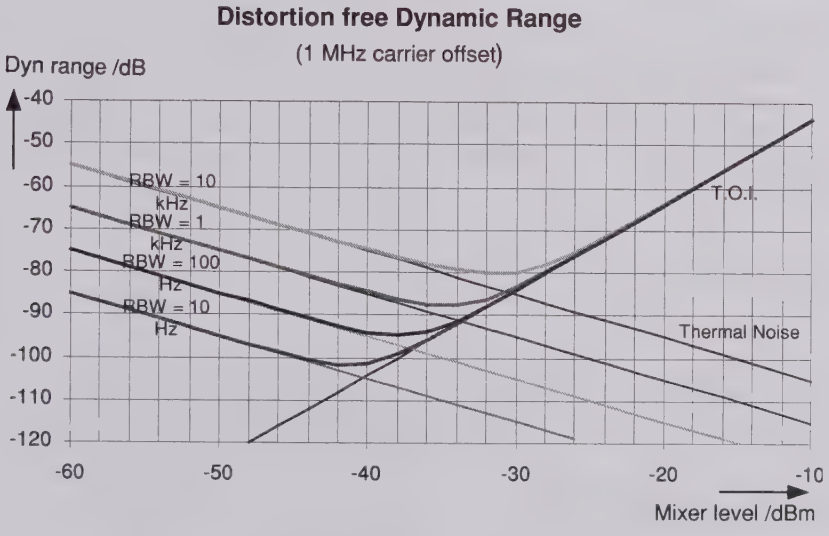

Fig. 2-17 Intermodulation-free range of the FSP3 as a function of level at the input mixer and the set resolution bandwidth (useful signal offset = 1 MHz, DANL = -155 dBm /Hz, TOI = 12 dBm; typ. values at 2 GHz)

The optimum mixer level, i.e. the level at which the intermodulation distance is at its maximum, depends on the bandwidth. At a resolution bandwidth of 10 Hz, it is approx. –42 dBm and at 10 kHz increases to approx. -32 dBm.

Phase noise has a considerable influence on the intermodulation-free range at carrier offsets between 10 and 100 kHz (Fig. 2-18). At greater bandwidths, the influence of the phase noise is greater than it would be with small bandwidths. The optimum mixer level at the bandwidths under consideration becomes almost independent of bandwidth and is approx. –40 dBm.

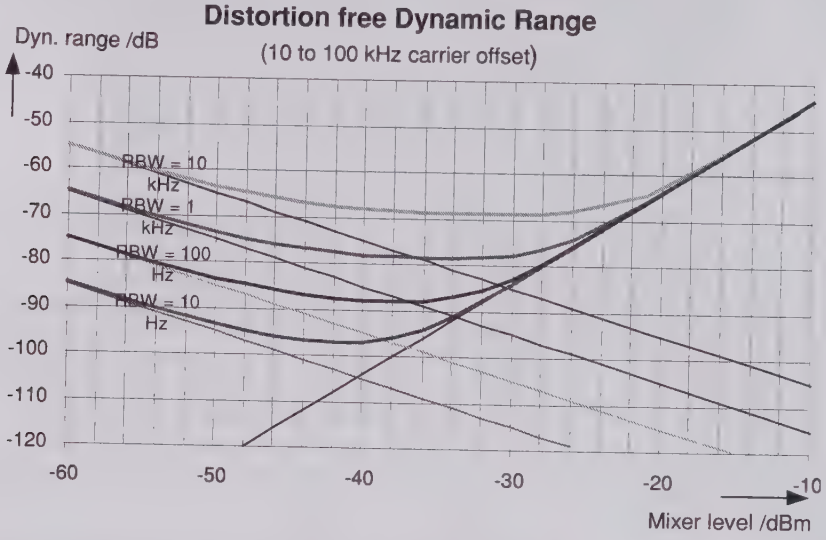

Fig. 2-18 Intermodulation-free dynamic range of the FSP3 as a function of level at the input mixer and of the selected resolution bandwidth (useful signal offset = 10 to 100 kHz, DANL = -155 dBm /Hz, TOI = 12 dBm; typ. values at 2 GHz).

Hint: If the intermodulation products of a DUT with a very high dynamic range are to be measured and the resolution bandwidth to be used is therefore very small, it is best to measure the levels of the useful signals and those of the intermodulation products separately using a small span. The measurement time will be reduced– in particular if the offset of the useful signals is large. To find signals reliably when frequency span is small, it is best to synchronize the signal sources and the FSP.

Measuring Signals in the Vicinity of Noise

The minimum signal level a spectrum analyzer can measure is limited by its intrinsic noise. Small signals can be swamped by noise and therefore cannot be measured. For signals that are just above the intrinsic noise, the accuracy of the level measurement is influenced by the intrinsic noise of the spectrum analyzer.

The displayed noise level of a spectrum analyzer depends on its noise figure, the selected RF attenuation, the selected reference level, the selected resolution and video bandwidth and the detector. The effect of the different parameters is explained in the following.

Impact of the RF attenuation setting
The sensitivity of a spectrum analyzer is directly influenced by the selected RF attenuation. The highest sensitivity is obtained at a RF attenuation of 0 dB. The FSP's RF attenuation can be set in 10 dB steps up to 70 dB (5 dB steps up to 75 dB with option *Electronic Attenuator* FSP-B25. Each additional 10 dB step reduces the FSP's sensitivity by 10 dB, i.e. the displayed noise is increased by 10 dB.

Impact of the reference level setting
If the reference level is changed, the FSP changes the gain on the last IF so that the voltage at the logarithmic amplifier and the A/D converter is always the same for signal levels corresponding to the reference level. This ensures that the dynamic range of the log amp or the A/D converter is fully utilized. Therefore, the total gain of the signal path is low at high reference levels and the noise figure of the IF amplifier makes a substantial contribution to the total noise figure of the FSP. Fig. 2-(21) below shows the change in the displayed noise depending on the set reference level at 10 kHz and 300 kHz resolution bandwidth. With digital bandwidths (≤ 100 kHz) the noise increases sharply at high reference levels because of the dynamic range of the A/D converter.

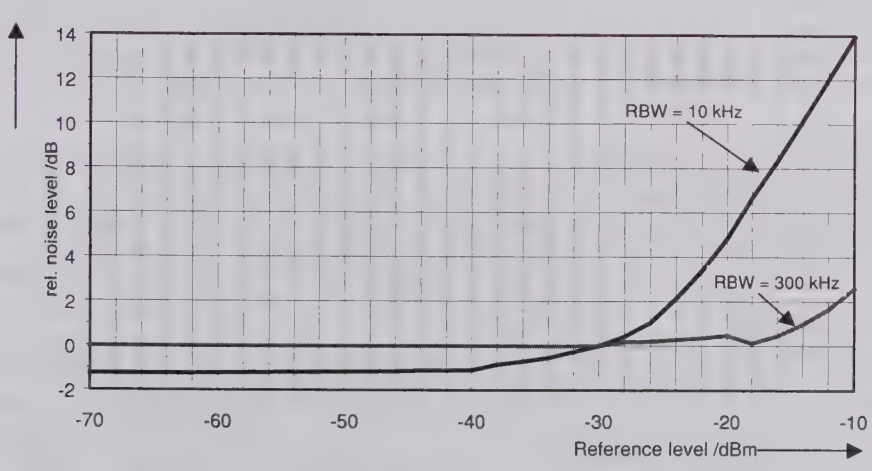

Fig. 2-19 Change in displayed noise as a function of the selected reference level at bandwidths of 10 kHz and 300 kHz (-30 dBm reference level)

Impact of the resolution bandwidth
The sensitivity of a spectrum analyzer also directly depends on the selected bandwidth. The highest sensitivity is obtained at the smallest bandwidth (for the FSP: 10 Hz, for FFT filtering: 1 Hz). If the bandwidth is increased, the reduction in sensitivity is proportional to the change in bandwidth. The FSP has bandwidth settings in 1, 3, 10 sequence. Increasing the bandwidth by a factor of 3 increases the displayed noise by approx. 5 dB (4.77 dB precisely). If the bandwidth is increased by a factor of 10, the displayed noise increases by a factor of 10, i.e. 10 dB. Because of the way the resolution filters are

designed, the sensitivity of spectrum analyzers often depends on the selected resolution bandwidth. In data sheets, the displayed average noise level is often indicated for the smallest available bandwidth (for the FSP: 10 Hz). The extra sensitivity obtained if the bandwidth is reduced may therefore deviate from the values indicated above. The following table illustrates typical deviations from the noise figure for a resolution bandwidth of 10 kHz which is used as a reference value (= 0 dB).

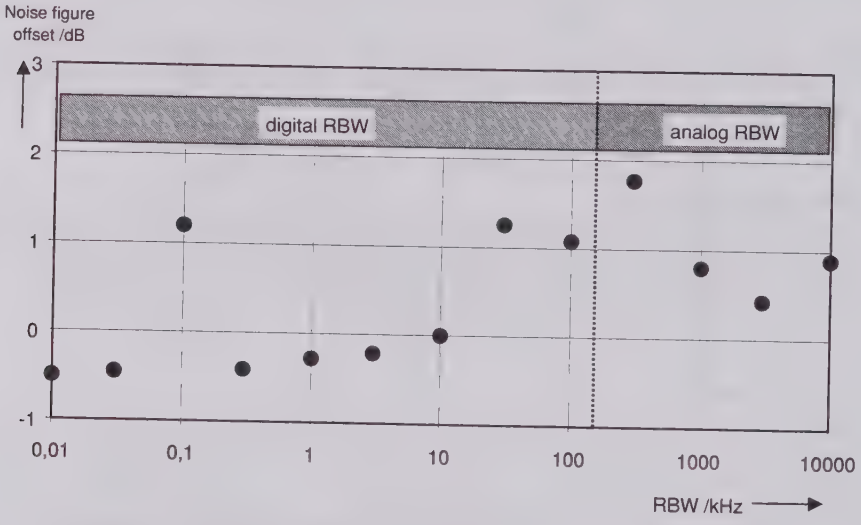

Fig. 2-20 Change in FSP noise figure at various bandwidths. The reference bandwidth is 10 kHz

Impact of the video bandwidth
The displayed noise of a spectrum analyzer is also influenced by the selected video bandwidth. If the video bandwidth is considerably smaller than the resolution bandwidth, noise spikes are suppressed, i.e. the trace becomes much smoother. The level of a sinewave signal is not influenced by the video bandwidth. A sinewave signal can therefore be freed from noise by using a video bandwidth that is small compared with the resolution bandwidth, and thus be measured more accurately.

Impact of the detector
Noise is evaluated differently by the different detectors. The noise display is therefore influenced by the choice of detector. Sinewave signals are weighted in the same way by all detectors, i.e. the level display for a sinewave RF signal does not depend on the selected detector, provided that the signal-to-noise ratio is high enough. The measurement accuracy for signals in the vicinity of intrinsic spectrum analyzer noise is also influenced by the detector which has been selected. The FSP has the following detectors:

Maximum peak detector
If the max. peak detector s selected, the largest noise display is obtained, since the spectrum analyzer displays the highest value of the IF envelope in the frequency range assigned to a pixel at each pixel in the trace. With longer sweep times, the trace indicates higher noise levels since the probability of obtaining a high noise amplitude increases with the dwell time on a pixel. For short sweep times, the display approaches that of the sample detector since the dwell time on a pixel is only sufficient to obtain an instantaneous value.

Minimum peak detector
The min. peak detector indicates the minimum voltage of the IF envelope in the frequency range assigned to a pixel at each pixel in the trace. The noise is strongly suppressed by the minimum peak detector since the lowest noise amplitude that occurs is displayed for each test point. If the signal-to-noise ratio is low, the minimum of the noise overlaying the signal is displayed too low.
At longer sweep times, the trace shows smaller noise levels since the probability of obtaining a low noise amplitude increases with the dwell time on a pixel. For short sweep times, the display approaches that of the sample detector since the dwell time on a pixel is only sufficient to obtain an instantaneous value.

Autopeak detector
The Autopeak detector displays the maximum and minimum peak value at the same time. Both values are measured and their levels are displayed on the screen joint by a vertical line.

Sample detector
The sample detector samples the logarithm of the IF envelope for each pixel of the trace only once and displays the resulting value. If the frequency span of the spectrum analyzer is considerably higher than the resolution bandwidth (span/RBW >500), there is no guarantee that useful signals will be detected. They are lost due to undersampling. This does not happen with noise because in this case it is not the instantaneous amplitude that is relevant but only the probability distribution.

RMS detector
For each pixel of the trace, the RMS detector outputs the RMS value of the IF envelope for the frequency range assigned to each test point. It therefore measures noise power. The display for small signals is, however, the sum of signal power and noise power. For short sweep times, i.e. if only one uncorrelated sample value contributes to the RMS value measurement, the RMS detector is equivalent to the sample detector. If the sweep time is longer, more and more uncorrelated RMS values contribute to the RMS value measurement. The trace is, therefore, smoothed. The level of sinewave signals is only displayed correctly if the selected resolution bandwidth (RBW) is at least as wide as the frequency range which corresponds to a pixel in the trace. At a resolution bandwidth of 1 MHz, this means that the maximum frequency display range is 501 MHz.

Average detector
For each pixel of the trace, the average detector outputs the average value of the linear IF envelope for the frequency range assigned to each test point. It therefore measures the linear average noise. The level of sinewave signals is only displayed correctly if the selected resolution bandwidth (RBW) is at least as wide as the frequency range which corresponds to a pixel in the trace. At a resolution bandwidth of 1 MHz, this means the maximum frequency display range is 501 MHz.

Quasi peak detector
The quasi peak detector is a peak detector for EMI measurements with defined charge and discharge times. These times are defined in CISPR 16, the standard for equipment used to measure EMI emissions.

Measurement example – Measuring the level of the internal reference generator at low S/N ratios

The example shows the different factors influencing the S/N ratio.

1. ***Set the spectrum analyzer to its default state.***

   ➢ Press the *PRESET* key.
   The FSP is in its default state.

2. ***Switch on the internal reference generator***

   ➢ Press the *SETUP* key.

   ➢ Press the softkeys *SERVICE - INPUT CAL.*
   The internal 128 MHz reference generator is on.
   The FSP's RF input is off.

3. ***Set the center frequency to 128 MHz and the frequency span to 100 MHz.***

   ➢ Press the *FREQ* key and enter *128 MHz.*

   ➢ Press the *SPAN* key and enter *100* MHz.

4. Set the RF attenuation to 60 dB to attenuate the input signal or to increase the intrinsic noise.

➢ Press the *AMPT* key.

➢ Press the *RF ATTEN MANUAL* softkey and enter *60 dB*.
The RF attenuation indicator is marked with an asterisk (*Att 60 dB) to show that it is no longer coupled to the reference level. The high input attenuation reduces the reference signal which can no longer be detected in noise.

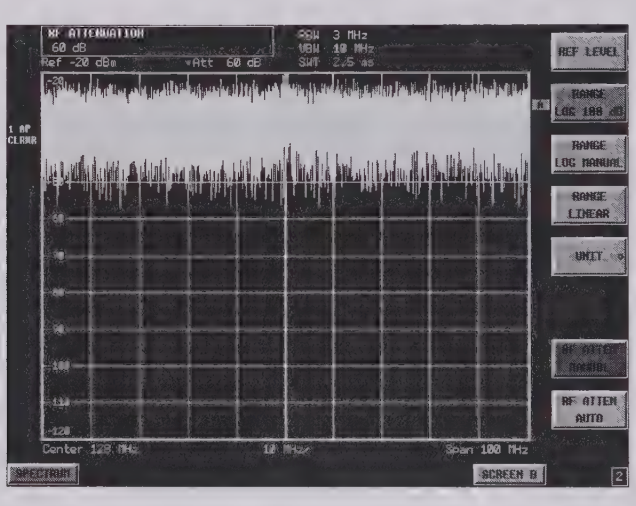

Fig. 2-21 Sinewave signal with low S/N ratio. The signal is measured with the autopeak detector and is completely swamped by the intrinsic noise of the spectrum analyzer.

5. To suppress noise spikes the trace can be averaged.

➢ Press the *TRACE* key.

➢ Press the *AVERAGE* softkey.
The traces of consecutive sweeps are averaged. To perform averaging, the FSP automatically switches on the sample detector. The RF signal, therefore, can be more clearly distinguished from noise.

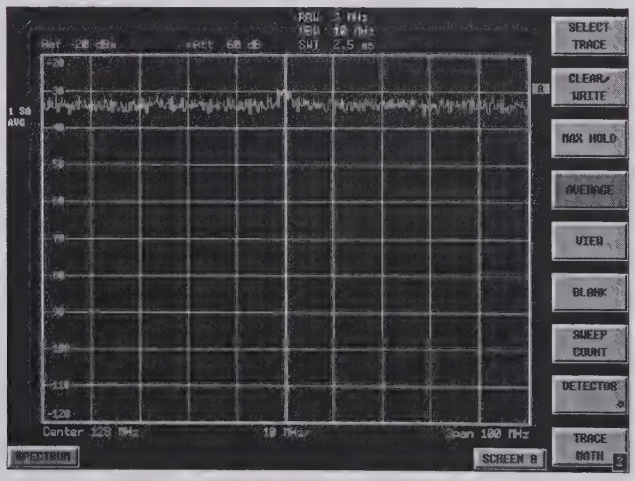

Fig. 2-22 RF sinewave signal with low S/N ratio if the trace is averaged.

6. Instead of trace averaging, a video filter that is narrower than the resolution bandwidth can be selected.

- Press the *CLEAR/WRITE* softkey in the trace menu.
- Press the *BW* key.
- Press the *VIDEO BW MANUAL* softkey and enter *10 kHz*.
  The RF signal can be more clearly distinguished from noise.

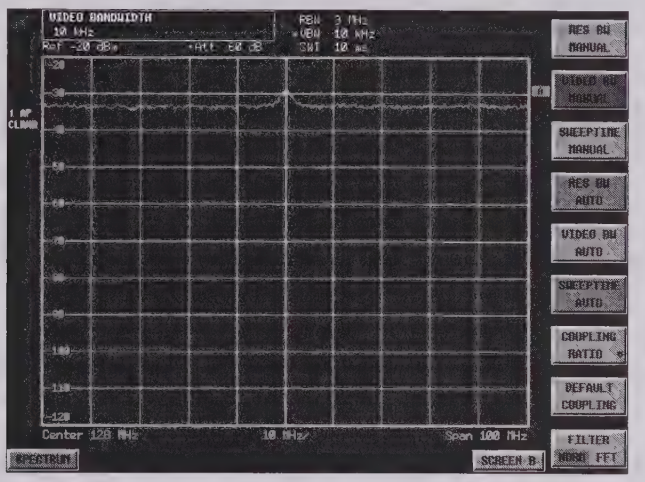

Fig. 2-23 RF sinewave signal with low S/N ratio if a smaller video bandwidth is selected.

7. By reducing the resolution bandwidth by a factor of 10, the noise is reduced by 10 dB.

- Press the *RES BW MANUAL* softkey and enter *300 kHz*.
  The displayed noise is reduced by approx. 10 dB. The signal, therefore, emerges from noise by about 10 dB. Compared to the previous setting, the video bandwidth has remained the same, i.e. it has increased relative to the smaller resolution bandwidth. The averaging effect is, therefore, reduced by the video bandwidth. The trace will be noisier.

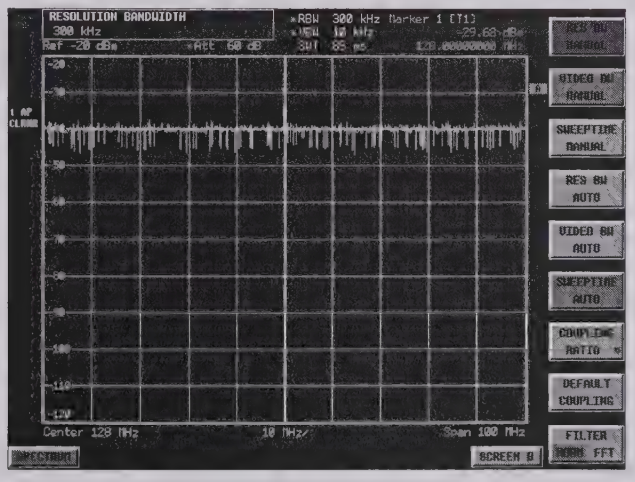

Fig. 2-24 Reference signal at a smaller resolution bandwidth

Noise Measurements

Noise measurements play an important role in spectrum analysis. Noise e.g. affects the sensitivity of radiocommunication systems and their components.

Noise power is specified either as the total power in the transmission channel or as the power referred to a bandwidth of 1 Hz. The sources of noise are, for example, amplifier noise or noise generated by oscillators used for the frequency conversion of useful signals in receivers or transmitters. The noise at the output of an amplifier is determined by its noise figure and gain.

The noise of an oscillator is determined by phase noise near the oscillator frequency and by thermal noise of the active elements far from the oscillator frequency. Phase noise can mask weak signals near the oscillator frequency and make them impossible to detect.

Measuring noise power density

To measure noise power referred to a bandwidth of 1 Hz at a certain frequency, the FSP has an easy-to-use marker function. This marker function calculates the noise power density from the measured marker level.

Measurement example – Measuring the intrinsic noise power density of the FSP at 1 GHz and calculating the FSP's noise figure.

1. ***Set the spectrum analyzer to its default state.***

   ➢ Press the *PRESET* key.
   The FSP is in its default state.

2. ***Set the center frequency to 1 GHz and the span to 1 MHz.***

   ➢ Press the *FREQ* key and enter *1 GHz*.

   ➢ Press the *SPAN* key and enter *1 MHz*.

3. ***Switch on the marker and set the marker frequency to 1 GHz.***

   ➢ Press the *MKR* key and enter *1 GHz*.

4. ***Switch on the noise marker function.***

   ➢ Press the *NOISE MARKER* softkey.
   The FSP displays the noise power at 1 GHz in dBm (1Hz).

   Since noise is random, a sufficiently long measurement time has to be selected to obtain stable measurement results. This can be achieved by averaging the trace or by selecting a very small video bandwidth relative to the resolution bandwidth.

5. ***The measurement result is stabilized by averaging the trace***

   ➢ Press the *TRACE* key.

   ➢ Press the *AVERAGE* softkey.
   The FSP performs sliding averaging over 10 traces from consecutive sweeps. The measurement result becomes more stable.

Conversion to other reference bandwidths

The result of the noise measurement can be referred to other bandwidths by simple conversion. This is done by adding 10 · log (BW) to the measurement result, BW being the new reference bandwidth.

Example:

A noise power of –150 dBm (1 Hz) is to be referred to a bandwidth of 1 kHz.
$P_{[1kHz]}$ = -150 + 10 * log (1000) = -150 +30 = -120 dBm(1 kHz)

Calculation method:

The following method is used to calculate the noise power:

If the noise marker is switched on, the FSP automatically activates the sample detector. The video bandwidth is set to 1/10 of the selected resolution bandwidth (RBW).

To calculate the noise, the FSP takes an average over 17 adjacent pixels (the pixel on which the marker is positioned and 8 pixels to the left, 8 pixels to the right of the marker). The measurement result is stabilized by video filtering and averaging over 17 pixels.

Since both video filtering and averaging over 17 trace points is performed in the log display mode, the result would be 2.51 dB too low (difference between logarithmic noise average and noise power). The FSP, therefore, corrects the noise figure by 2.51 dB.

To standardize the measurement result to a bandwidth of 1 Hz, the result is also corrected by –10 * log (RBW_{noise}), with RBW_{noise} being the power bandwidth of the selected resolution filter (RBW).

Detector selection

The noise power density is measured in the default setting with the sample detector and using averaging. Other detectors that can be used to perform a measurement giving true results are the average detector or the RMS detector. If the average detector is used, the linear video voltage is averaged and displayed as a pixel. If the RMS detector is used, the squared video voltage is averaged and displayed as a pixel. The averaging time depends on the selected sweep time (=SWT/501). An increase in the sweep time gives a longer averaging time per pixel and thus stabilizes the measurement result. The FSP automatically corrects the measurement result of the noise marker display depending on the selected detector (+1.05 dB for the average detector, 0 dB for the RMS detector). It is assumed that the video bandwidth is set to at least three times the resolution bandwidth. While the average or RMS detector is being switched on, the FSP sets the video bandwidth to a suitable value.

The Pos Peak, Neg Peak, Auto Peak and Quasi Peak detectors are not suitable for measuring noise power density.

Determining the noise figure:

The noise figure of amplifiers or of the FSP alone can be obtained from the noise power display. Based on the known thermal noise power of a 50 Ω resistor at room temperature (-174 dBm (1Hz)) and the measured noise power P_{noise} the noise figure (NF) is obtained as follows:

$NF = P_{noise} + 174 - g$,
where g = gain of DUT in dB

Example: The measured internal noise power of the FSP at an attenuation of 0 dB is found to be –153 dBm/1 Hz. The noise figure of the FSP is obtained as follows

$NF = -153 + 174 = 19$ dB

Note: If noise power is measured at the output of an amplifier, for example, the sum of the internal noise power and the noise power at the output of the DUT is measured. The noise power of the DUT can be obtained by subtracting the internal noise power from the total power (subtraction of linear noise powers). By means of the following diagram, the noise level of the DUT can be estimated from the level difference between the total and the internal noise level.

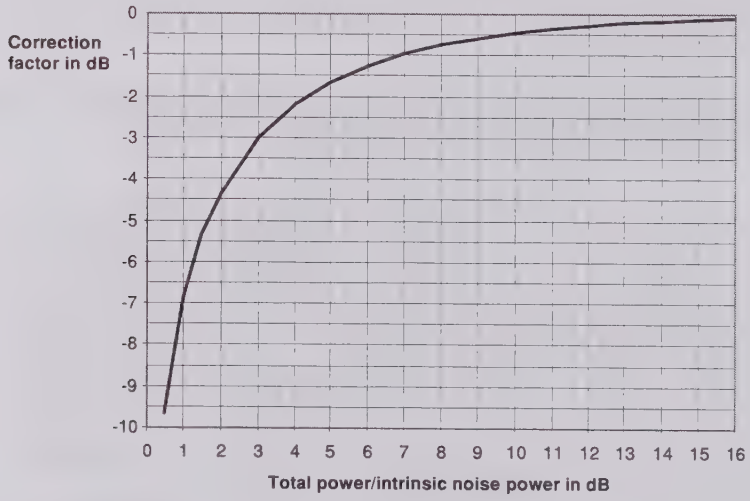

Fig. 2-25 Correction factor for measured noise power as a function of the ratio of total power to the intrinsic noise power of the spectrum analyzer.

Measurement of Noise Power within a Transmission Channel

Noise in any bandwidth can be measured with the channel power measurement functions. Thus the noise power in a communication channel can be determined, for example. If the noise spectrum within the channel bandwidth is flat, the noise marker from the previous example can be used to determine the noise power in the channel by considering the channel bandwidth. If, however, phase noise and noise that normally increases towards the carrier is dominant in the channel to be measured, or if there are discrete spurious signals in the channel, the channel power measurement method must be used to obtain correct measurement results.

Measurement Example – Measuring the intrinsic noise of the FSP at 1 GHz in a 1.23 MHz channel bandwidth with the channel power function

Test setup:

The RF input of the FSP remains open-circuited or is terminated with 50 Ω.

Measurement with the FSP:

1. ***Set the spectrum analyzer to its default state.***
   - Press the *PRESET* key.
     The FSP is in its default state.
2. ***Set the center frequency to 1 GHz and the span to 1 MHz.***
   - Press the *FREQ* key and enter *1 GHz.*
   - Press the *SPAN* key and enter *2 MHz.*
3. ***To obtain maximum sensitivity, set RF attenuation on the FSP to 0 dB.***
   - Press the *AMPT* key.
   - Press the *RF ATTEN MANUAL* softkey and enter *0 dB.*
4. ***Switch on and configure the channel power measurement.***
   - Press the *MEAS* key.
   - Press the *CHAN POWER / ACP* softkey.
     The FSP activates the channel or adjacent channel power measurement according to the currently set configuration.
   - Press the *CP/ACP CONFIG* ⇩ softkey.
     The FSP enters the submenu for configuring the channel.
   - Press the *CHANNEL BANDWIDTH* softkey and enter *1.23 MHz.*
     The FSP displays the 1.23 MHz channel as two vertical lines which are symmetrical to the center frequency.
   - Press the *PREV* key.
     The FSP returns to the main menu for channel and adjacent channel power measurement.
   - Press the *ADJUST SETTINGS* softkey.
     The settings for the frequency span, the bandwidth (RBW and VBW) and the detector are automatically set to the optimum values required for the measurement.

Fig. 2-26 Measurement of the FSP's intrinsic noise power in a 1.23 MHz channel bandwidth.

5. Stabilizing the measurement result by increasing the sweep time

➢ Press the *SWEEP TIME* softkey and enter *1 s*.
By increasing the sweep time to 1 s, the trace becomes much smoother thanks to the RMS detector and the channel power measurement display is much more stable.

6. Referring the measured channel power to a bandwidth of 1 Hz

➢ Press the *CHAN PWR / Hz* softkey.
The channel power is referred to a bandwidth of 1 Hz. The measurement is corrected by -10 * log (ChanBW), with ChanBW being the channel bandwidth that was selected.

Method of calculating the channel power

When measuring the channel power, the FSP integrates the linear power which corresponds to the levels of the pixels within the selected channel. The analyzer uses a resolution bandwidth which is far smaller than the channel bandwidth. When sweeping over the channel, the channel filter is formed by the passband characteristics of the resolution bandwidth (see Fig. 2-27).

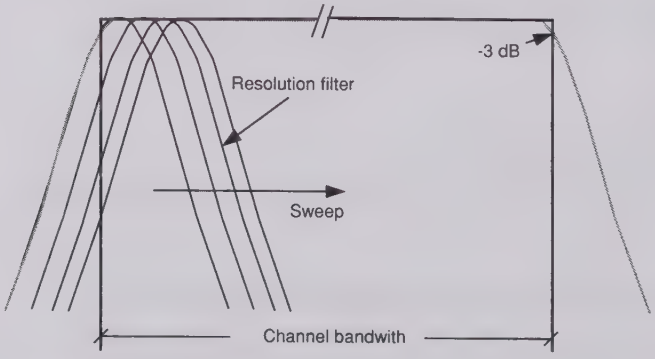

Fig. 2-27 Approximating the channel filter by sweeping with a small resolution bandwidth

The following steps are performed:

- The linear power of all the trace pixels within the channel is calculated.

  $P_i = 10^{(L_i/10)}$

  where P_i = power of the trace pixel i

  L_i = displayed level of trace point i

- The powers of all trace pixels within the channel are summed up and the sum is divided by the number of trace pixels in the channel.
- The result is multiplied by the quotient of the selected channel bandwidth and the noise bandwidth of the resolution filter (RBW).

Since the power calculation is performed by integrating the trace within the channel bandwidth, this method is also called the IBW method (**I**ntegration **B**and**w**idth method).

Bandwidth selection (RBW)

For channel power measurements, the resolution bandwidth (RBW) must be small compared to the channel bandwidth, so that the channel bandwidth can be defined precisely. If the resolution bandwidth which has been selected is too wide, this may have a negative effect on the selectivity of the simulated channel filter and result in the power in the adjacent channel being added to the power in the transmit channel. A resolution bandwidth equal to 1% to 3% of the channel bandwidth should, therefore, be selected. If the resolution bandwidth is too small, the required sweep time becomes too long and the measurement time increases considerably.

Detector selection

Since the power of the trace is measured within the channel bandwidth, only the sample detector and RMS detector can be used. These detectors provide measured values that make it possible to calculate the real power. The peak detectors (Pos Peak, Neg Peak and Auto Peak) are not suitable for noise power measurements as no correlation can be established between the peak value of the video voltage and power.

With the **sample detector,** a value (sample) of the IF envelope voltage is displayed at each trace pixel. Since the frequency spans are very large compared with the resolution bandwidth (span/RBW >501), sinewave signals present in the noise might be lost, i.e. they are not displayed. This is not important for pure noise signals, however, since a single sample in itself is not important - it is the probability distribution of all measured values that counts. The number of samples for power calculation is limited to the number of trace pixels (501 for the FSP).

Note: *To increase the repeatability of measurements, averaging is often carried out over several traces (**AVERAGE** softkey in the **TRACE** menu). This gives spurious results for channel power measurements (max. –2.51 dB for ideal averaging). Trace averaging should, therefore, be avoided.*

With the **RMS detector,** the whole IF envelope is used to calculate the power for each trace pixel. The IF envelope is digitized using a sampling frequency which is at least five times the resolution bandwidth which has been selected. Based on the sample values, the power is calculated for each trace pixel using the following formula:

$$P_{RMS} = \sqrt{\frac{1}{N} \cdot \sum_{i=1}^{N} s_i^2}$$

s_i = linear digitized video voltage at the output of the A/D converter
N = number of A/D converter values per pixel of the trace

P_{RMS} = power represented by a trace pixel

When the power has been calculated, the power units are converted into decibels and the value is displayed as a trace pixel.

The number of A/D converter values, N, used to calculate the power, is defined by the sweep time. The time per trace pixel for power measurements is directly proportional to the selected sweep time. The RMS detector uses far more samples for power measurement than the sample detector, especially if the sweep time is increased. The measurement uncertainty can be reduced considerably. In the default setting, the FSP therefore uses the RMS detector to measure the channel power.

For both detectors (sample and RMS), the video bandwidth (VBW) must at least be three times the resolution bandwidth, so that the peak values of the video voltage are not cut off by the video filter. At smaller video bandwidths, the video signal is averaged and the power readout will be too small.

Sweep time selection

If the sample detector is used, it is best to select the smallest sweep time possible for a given span and resolution bandwidth. The minimum time is obtained if the setting is coupled. This means that the time per measurement is minimal. Extending the measurement time does not have any advantages as the number of samples for calculating the power is defined by the number of trace pixels in the channel.

When using the RMS detector, the repeatability of the measurement results can be influenced by the selection of sweep times. Repeatability is increased at longer sweep times.
Repeatability can be estimated from the following diagram:

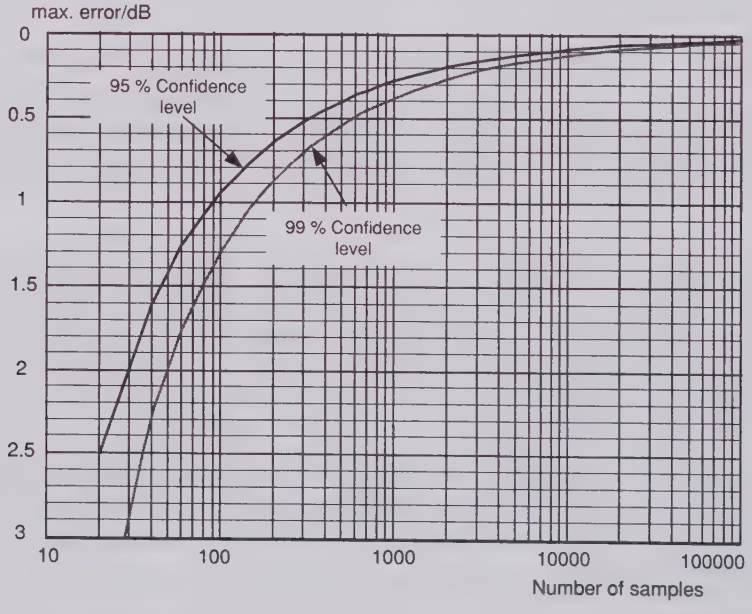

Fig. 2-28 Repeatability of channel power measurements as a function of the number of samples used for power calculation

The curves in Fig. 2-28 indicates the repeatability obtained with a probability of 95% and 99% depending on the number of samples used.
The repeatability with 600 samples is ± 0.5 dB. This means that – if the sample detector and a channel bandwidth over the whole diagram (channel bandwidth = span) is used - the measured value lies within ± 0.5 dB of the true value with a probability of 99%.

If the RMS detector is used, the number of samples can be estimated as follows:

Since only uncorrelated samples contribute to the RMS value, the number of samples can be calculated from the sweep time and the resolution bandwidth.

Samples can be assumed to be uncorrelated if sampling is performed at intervals of 1/RBW. The number of uncorrelated samples (N_{decorr}) is calculated as follows:

$N_{decorr} = SWT \cdot RBW$

The number of uncorrelated samples per trace pixel is obtained by dividing N_{decorr} by 501 (= pixels per trace).

Example:

At a resolution bandwidth of 30 kHz and a sweep time of 100 ms, 3000 uncorrelated samples are obtained. If the channel bandwidth is equal to the frequency display range, i.e. all trace pixels are used for the channel power measurement, a repeatability of 0.2 dB with a confidence level of 99% is the estimate that can be derived from Fig. 2-28.

Measuring Phase Noise

The FSP has an easy-to-use marker function for phase noise measurements. This marker function indicates the phase noise of an RF oscillator at any carrier in dBc in a bandwidth of 1 Hz.

Measurement Example - Measuring the phase noise of a signal generator at a carrier offset of 10 kHz.

Test setup:

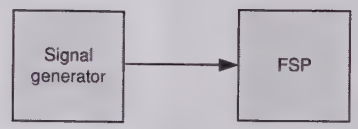

Settings on the signal generator (e.g. R&S SMIQ):
Frequency: 100 MHz
Level: 0 dBm

Measurement using FSP:

1. ***Set the spectrum analyzer to its default state***
   - Press the *PRESET* key.
     FSP is in its default state.
2. ***Set the center frequency to 100 MHz and the span to 50 kHz***
   - Press the *FREQ* key and enter *100 MHz*.
   - Press the *SPAN* key and enter *50 kHz*.
3. ***Set the FSP's reference level to 0 dBm (=signal generator level)***
   - Press the *AMPT* key and enter *0 dBm*.

4. Enable phase noise measurement

➢ Press the *MKR FCTN* key.

➢ Press the *PHASE NOISE* ⇩ softkey.
The FSP activates phase noise measurement. Marker 1 (=main marker) and marker 2 (= delta marker) are positioned on the signal maximum. The position of the marker is the reference (level and frequency) for the phase noise measurement. A horizontal line represents the level of the reference point and a vertical line the frequency of the reference point. Data entry for the delta marker is activated so that the frequency offset at which the phase noise is to be measured can be entered directly.

5. 10 kHz frequency offset for determining phase noise.

➢ Enter *10 kHz*.
The FSP displays the phase noise at a frequency offset of 10 kHz . The magnitude of the phase noise in dBc/Hz is displayed in the delta marker output field at the top right of the screen (delta 2 [T1 PHN]).

6. Stabilize the measurement result by activating trace averaging.

➢ Press the *TRACE* key.

➢ Press the *AVERAGE* softkey.

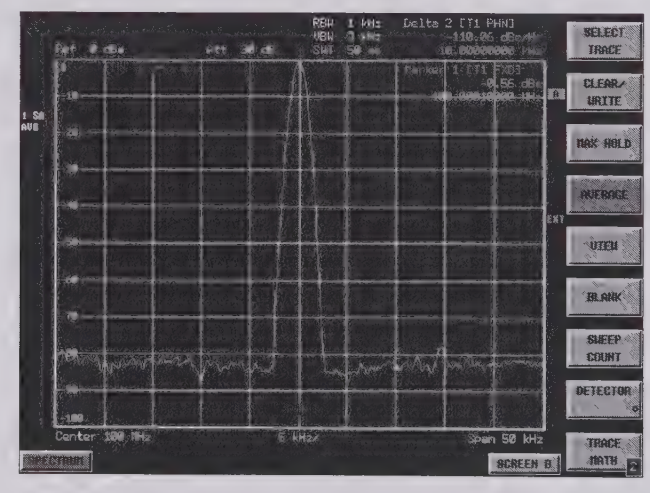

Fig. 2-29 Measuring phase noise with the phase-noise marker function

The frequency offset can be varied by moving the marker with the spinwheel or by entering a new frequency offset as a number.

Measurements on Modulated Signals

If RF signals are used to transmit information, an RF carrier is modulated. Analog modulation methods such as amplitude modulation, frequency modulation and phase modulation have a long history and digital modulation methods are now used for modern systems. Measuring the power and the spectrum of modulated signals is an important task to assure transmission quality and to ensure the integrity of other radio services. This task can be performed easily with a spectrum analyzer. Modern spectrum analyzers also provide the test routines that are essential to simplify complex measurements.

Measurements on AM signals

The spectrum analyzer detects the RF input signal and displays the magnitudes of its components as a spectrum. AM modulated signals are also demodulated by this process. The AF voltage can be displayed in the time domain if the modulation sidebands are within the resolution bandwidth. In the frequency domain, the AM sidebands can be resolved with a small bandwidth and can be measured separately. This means that the modulation depth of a carrier modulated with a sinewave signal can be measured. Since the dynamic range of a spectrum analyzer is very wide, even extremely small modulation depths can be measured accurately. The FSP has a test routine which measures the modulation depth in %.

Measurement Example 1 – Displaying the AF of an AM signal in the time domain.

Test setup:

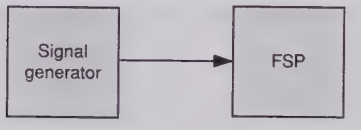

Settings on the signal generator (e.g. R&S SMIQ):
Frequency: 100 MHz
Level: 0 dBm
Modulation: 50 % AM, 1 kHz AF

Measurement with the FSP:

1. ***Set the spectrum analyzer to its default state***

   ➢ Press the *PRESET* key.
   The FSP is in its default state.

2. ***Set the center frequency to 100 MHz and the span to 0 kHz***

   ➢ Press the *FREQ* key and enter *100 MHz*.

   ➢ Press the *SPAN* key and enter *0 Hz*.

3. ***Set the reference level to +6 dBm and the display range to linear***

   ➢ Press the *AMPT* key and enter *6 dBm*.

   ➢ Press the *RANGE LINEAR* softkey.

4. Use the video trigger to trigger on the AF signal in order to obtain a stationary display

➢ Press the *TRIG* key.

➢ Press the *VIDEO* softkey.
The video trigger level is set to 50% if the instrument is switched on for the first time. The trigger level is displayed as a horizontal line across the graph. The FSP displays the 1 kHz AF signal stably in the time domain.

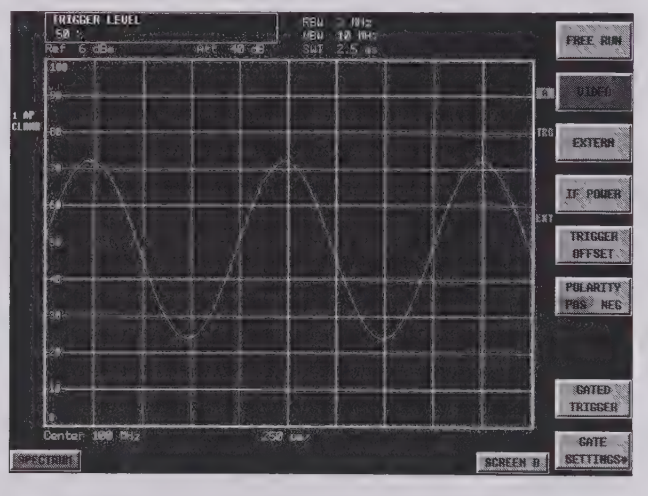

Fig. 2-30 Measuring the AF signal from a 1 kHz AM carrier

If the FSP is equipped with the AM/FM Demodulator option (FSP-B3), the AF can be monitored on the built-in loudspeaker.

5. Switch on the internal AM demodulator

➢ Press the *MKR FCTN* key.

➢ Press the *MKR DEMOD* softkey.
The FSP switches the AM demodulator on automatically.

➢ Turn up volume control.
A 1 kHz tone is output by the built-in loudspeaker.

Measurement Example 2 - Measuring the modulation depth of an AM carrier in the frequency domain.

Test setup:

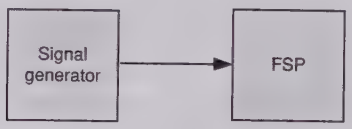

Settings on the signal generator (e.g. R&S SMIQ):
Frequency: 100 MHz
Level: -30 dBm
Modulation: 50 % AM, 1 kHz AF

Measurement with the FSP:

1. ***Set the spectrum analyzer to its default state***

   ➢ Press the PRESET key.
   The FSP is in its default state.

2. ***Set the center frequency to 100 MHz and the span to 0 kHz***

   ➢ Press the *FREQ* key and enter *100 MHz.*

   ➢ Press the *SPAN* key and enter *5 kHz.*

3. ***Activate the marker function for AM depth measurement***

   ➢ Press the *MKR FCTN* key.

   ➢ Press the *MODULATION DEPTH* softkey.
   The FSP automatically positions a marker on the carrier signal in the middle of the graph and one delta marker on each of the lower and upper AM sidebands. The FSP calculates the AM modulation depth from the ratios of the delta marker levels to the main marker level and outputs the numerical value in the marker info field

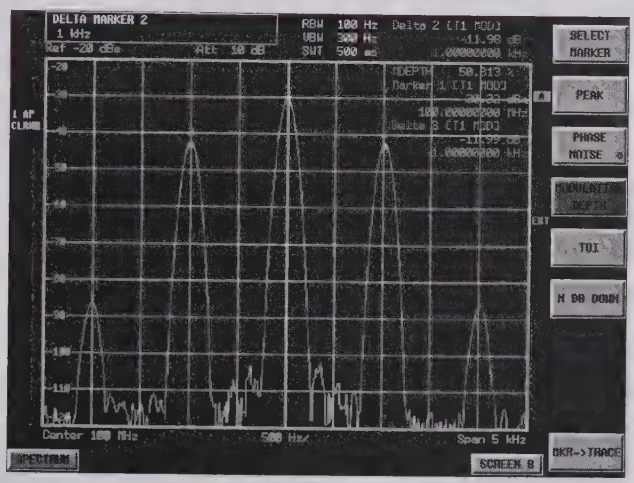

Fig. 2-31 Measurement of AM modulation depth. The modulation depth is indicated by MDEPTH. The frequency of the AF signal is indicated by the delta markers

Measurements on FM Signals

Since spectrum analyzers only display the magnitude of signals by means of the envelope detector, the modulation of FM signals cannot be directly measured as is the case with AM signals. With FM signals, the voltage at the output of the envelope detector is constant as long as the frequency deviation of the signal is within the flat part of the passband characteristic of the resolution filter which has been selected. Amplitude variations can only occur if the current frequency lies on the falling edge of the filter characteristic. This effect can be used to demodulate FM signals. The center frequency of the analyzer is set in a way that the nominal frequency of the test signal is on the filter edge (below or above the center frequency). The resolution bandwidth and the frequency offset are selected in a way that the current frequency is on the linear part of the filter slope. The frequency variation of the FM signal is then transformed into an amplitude variation which can be displayed in the time domain.

The FSP's analog 4^{th} order filters with frequencies from 300 kHz to 3 MHz have a good filter-slope linearity, if the frequency of the FSP is set to 1.2 times the filter bandwidth below or above the frequency of the transmit signal. The useful range for FM demodulation is then almost equal to the resolution bandwidth.

Measurement Example - Displaying the AF of an FM carrier

Test setup:

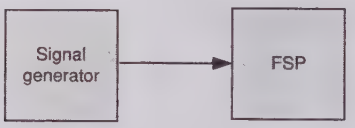

Settings on the signal generator (e.g. R&S SMIQ):
Frequency: 100 MHz
Level: -30 dBm
Modulation: FM 0 kHz deviation (i.e., FM = off), 1 kHz AF

Measurement with the FSP:

1. ***Set the spectrum analyzer to its default state***
   - Press the *PRESET* key.
     The FSP is in its default state.
2. ***Set the center frequency to 99.64 MHz and the span to 300 kHz.***
   - Press the *FREQ* key and enter *99.64 MHz.*
   - Press the *SPAN* key and enter *300 kHz.*
3. ***Set a resolution bandwidth of 300 kHz.***
   - Press the *BW* key.
   - Press the *RES BW MANUAL* softkey and enter *300 kHz.*
4. ***Set a display range of 20 dB and shift the filter characteristics to the middle of the display.***
   - Press the ***AMPT*** key.
   - Press the *RANGE LOG MANUAL* softkey and enter *20 dB.*
   - Press the ***NEXT*** key.
   - Set the *GRID* softkey to *REL.*

➢ Press the *PREV* softkey.

➢ Using the spinwheel, shift the reference level so that the filter edge intersects the - 10 dB level line at the center frequency.

The slope of the 300 kHz filter is displayed. This corresponds to the demodulator characteristics for FM signals with a slope of approx. 5 dB/100 kHz.

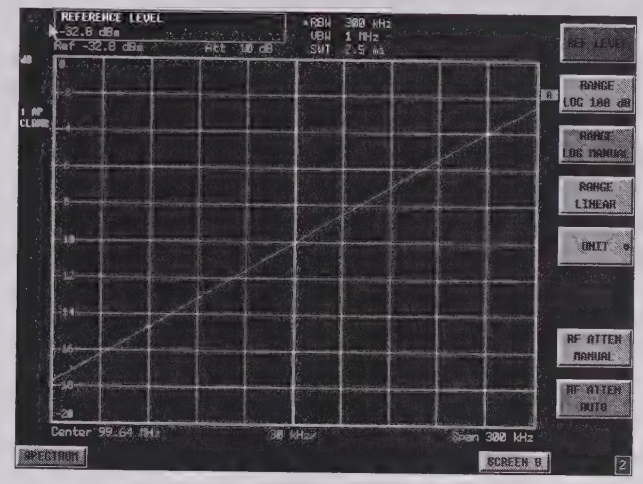

Fig. 2-32 Filter edge of a 300 kHz filter used as an FM-discriminator characteristic

5. Set an FM deviation of 100 kHz and an AF of 1 kHz on the signal generator

6. Set a frequency deviation of 0 Hz on the FSP

➢ Press the SPAN key.

➢ Press the ZERO SPAN.
The demodulated FM signal is displayed. The signal moves across the screen.

7. Creating a stable display by video triggering

➢ Press the TRIG key.

➢ Press the VIDEO softkey.
A stationary display is obtained for the FM AF signal

Result (-10 ± 5) dB; this means that a deviation of 100 kHz is obtained if the demodulator characteristic slope is 5 dB/100 kHz

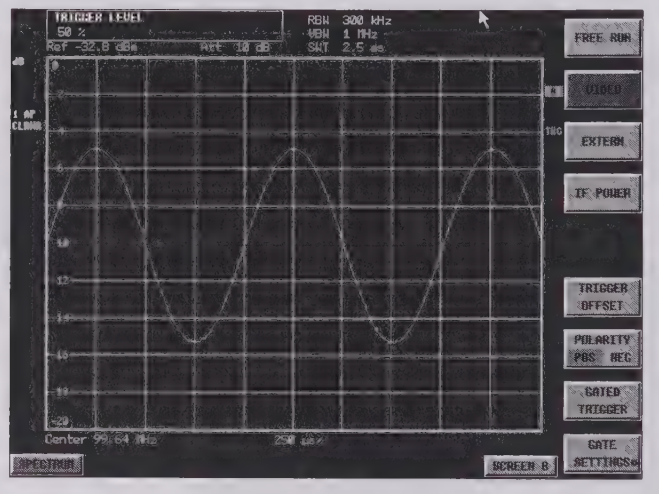

Fig. 2-33 Demodulated FM signal

Measuring Channel Power and Adjacent Channel Power

Measuring channel power and adjacent channel power is one of the most important tasks in the field of digital transmission for a spectrum analyzer with the necessary test routines. While, theoretically, channel power could be measured at highest accuracy with a power meter, its low selectivity means that it is not suitable for measuring adjacent channel power as an absolute value or relative to the transmit channel power. The power in the adjacent channels can only be measured with a selective power meter.

A spectrum analyzer cannot be classified as a true power meter, because it displays the IF envelope voltage. However, it is calibrated such as to correctly display the power of a pure sinewave signal irrespective of the selected detector. This calibration is not valid for non-sinusoidal signals. Assuming that the digitally modulated signal has a Gaussian amplitude distribution, the signal power within the selected resolution bandwidth can be obtained using correction factors. These correction factors are normally used by the spectrum analyzer's internal power measurement routines in order to determine the signal power from IF envelope measurements. These factors are valid if and only if the assumption of a Gaussian amplitude distribution is correct.
Apart from this common method, the FSP also has a true power detector, i.e. an RMS detector. It correctly displays the power of the test signal within the selected resolution bandwidth irrespective of the amplitude distribution, without additional correction factors being required. With an absolute measurement uncertainty of < 0.5 dB and a relative measurement uncertainty of < 0.2 dB (each with a confidence level of 95%), the FSP comes close to being a true power meter.

There are two possible methods for measuring channel and adjacent channel power with a spectrum analyzer:
The IBW method (**I**ntegration **B**andwidth **M**ethod) in which the spectrum analyzer measures with a resolution bandwidth that is less than the channel bandwidth and integrates the level values of the trace versus the channel bandwidth. This method is described in the section on noise measurements.

Measurement using a channel filter.
In this case, the spectrum analyzer makes measurements in the time domain using an IF filter that corresponds to the channel bandwidth. The power is measured at the output of the IF filter. Until now, this method has not been used for spectrum analyzers, because channel filters were not available and the resolution bandwidths, optimized for the sweep, did not have a sufficient selectivity. The method was reserved for special receivers optimized for a particular transmission method.

The FSP has test routines for simple channel and adjacent channel power measurements. These routines give quick results without any complex or tedious setting procedures.

Measurement Example 1 - ACPR measurement on an IS95 CDMA Signal

Test setup:

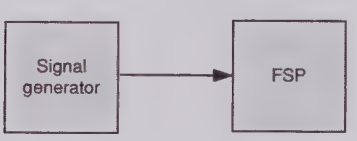

Settings on the signal generator (e.g. R&S SMIQ):
Frequency: 850 MHz
Level: 0 dBm
Modulation: CDMA IS 95

Measurement with the FSP:

1. ***Set the spectrum analyzer to its default state.***

   ➢ Press the *PRESET* key.
   The FSP is in its default state.

2. ***Set the center frequency to 850 MHz and frequency deviation to 4 MHz.***

   ➢ Press the *FREQ* key and enter *850 MHz*.

3. ***Set the reference level to +10 dBm.***

   ➢ Press the *AMPT* key and enter *10 dBm*.

4. ***Configuring the adjacent channel power for the CDMA IS95 reverse link.***

   ➢ Press the *MEAS* key.

   ➢ Press the *CHAN PWR ACP* ⇩ softkey.

   ➢ Press the *CP/ACP STANDARD* softkey.

   From the list of standards, select *CDMA IS95A REV* using the spinwheel or the cursor down key below the spinwheel and press *ENTER*.
   The FSP sets the channel configuration according to the IS95 standard for mobile stations with 2 adjacent channels above and below the transmit channel. The spectrum is displayed in the upper part of the screen, the numeric values of the results and the channel configuration in the lower part of the screen. The various channels are represented by vertical lines on the graph.
   The frequency span, resolution bandwidth, video bandwidth and detector are selected automatically to give correct results. To obtain stable results - especially in the adjacent channels (30 kHz bandwidth) which are narrow in comparison with the transmission channel bandwidth (1.23 MHz) - the RMS detector is used.

5. Set the optimal reference level and RF attenuation for the applied signal level.

➢ Press the *ADJUST REF LVL* softkey.
The FSP sets the optimal RF attenuation and the reference level based on the transmission channel power to obtain the maximum dynamic range. The following figure shows the result of the measurement.

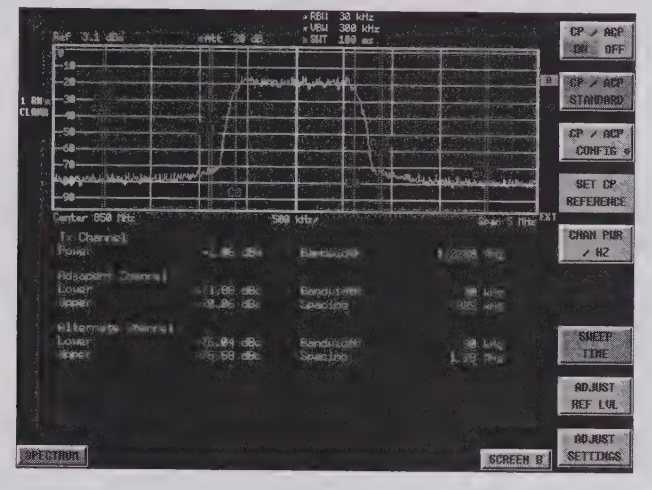

Fig. 2-34 Adjacent channel power measurement on a CDMA IS95 signal

The repeatability of the results, especially in the narrow adjacent channels, strongly depends on the measurement time since the dwell time within the 30 kHz channels is only a fraction of the complete sweep time. A longer sweep time may increase the probability that the measured value converges to the true value of the adjacent channel power, but this increases measurement time.

To avoid long measurement times, the FSP measures the adjacent channel power in the time domain (FAST ACP). In the FAST ACP mode, the FSP measures the power of each channel at the defined channel bandwidth, while being tuned to the center frequency of the channel in question. The digital implementation of the resolution bandwidths makes it possible to select a filter characteristics that is precisely tailored to the signal. In case of CDMA IS95, the power in the useful channel is measured with a bandwidth of 1.23 MHz and that of the adjacent channels with a bandwidth of 30 kHz. Therefore the FSP jumps from one channel to the other and measures the power at a bandwidth of 1.23 MHz or 30 kHz using the RMS detector. The measurement time per channel is set with the sweep time. It is equal to the selected measurement time divided by the selected number of channels. The five channels from the above example and the sweep time of 100 ms give a measurement time per channel of 20 ms.

Compared to the measurement time per channel given by the span (= 5 MHz) and sweep time (= 100 ms, equal to 1.66 ms per 30 kHz channel) used in the example, this is a far longer dwell time on the adjacent channels (factor of 12). In terms of the number of uncorrelated samples this means 20000/33 µs = 606 samples per channel measurement compared to 1667/33µs = 50.5 samples per channel measurement.

Repeatability with a confidence level of 95% is increased from ± 1.4 dB to ± 0.38 dB as shown in Fig. 2-28. For the same repeatability, the sweep time would have to be set to 1.2 s with the integration method. The following figure shows the standard deviation of the results as a function of the sweep time.

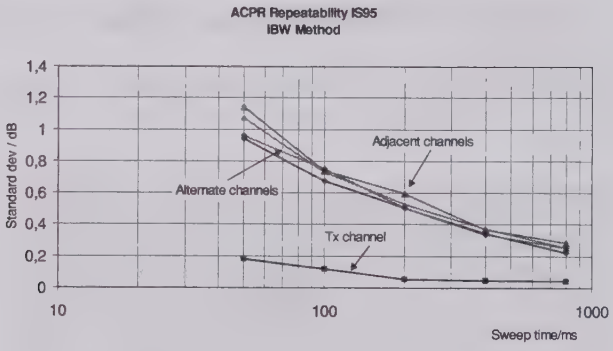

Fig. 2-35 Repeatability of adjacent channel power measurement on IS95-standard signals if the integration bandwidth method is used

6. Switch to Fast ACP to increase the repeatability of results.

- Press the *CP/ACP CONFIG* ⇩ softkey.
- Set the *FAST ACP* softkey to *ON*.
  The FSP measures the power of each channel in the time domain. The trace represents power as a function of time for each channel (see Fig. 2-36). The numerical results over consecutive measurements become much more stable.

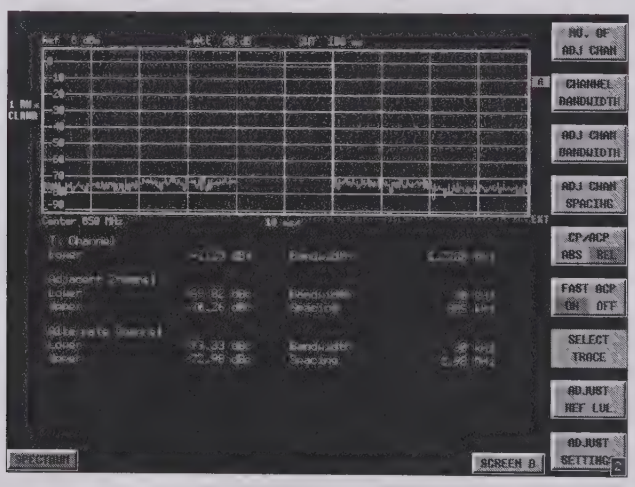

Fig. 2-36 Measuring the channel power and adjacent channel power ratio for IS95 signals in the time domain (Fast ACP)

The following figure shows the repeatability of power measurements in the transmit channel and of relative power measurements in the adjacent channels as a function of sweep time. The standard deviation of measurement results is calculated from 100 consecutive measurements as shown in Fig. 2-35. Take scaling into account if comparing power values.

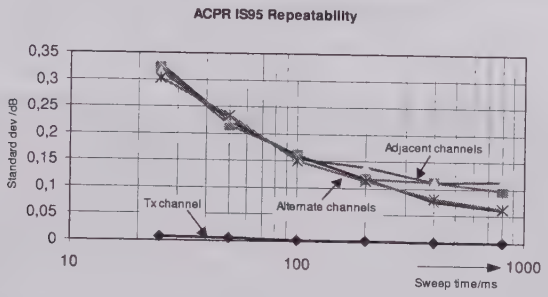

Fig. 2-37 Repeatability of adjacent channel power measurements on IS95 signals in the Fast ACP mode

Note on adjacent channel power measurements on IS95 base-station signals:
When measuring the adjacent channel power of IS95 base-station signals, the frequency spacing of the adjacent channel to the nominal transmit channel is specified as ±750 kHz. The adjacent channels are, therefore, so close to the transmit channel that the power of the transmit signal leaks across and is also measured in the adjacent channel if the usual method using the 30 kHz resolution bandwidth is applied. The reason is the low selectivity of the 30 kHz resolution filter. The resolution bandwidth, therefore, must be reduced considerably, e.g. to 3 kHz to avoid this. This causes very long measurement times (factor of 100 between a 30 kHz and 3 kHz resolution bandwidth).
This effect is avoided with the time domain method which uses steep IF filters. The 30 kHz channel filter implemented in the FSP has a very high selectivity so that even with a ± 750 kHz spacing to the transmit channel the power of the useful modulation spectrum is not measured.

The following figure shows the passband characteristics of the 30 kHz channel filter in the FSP.

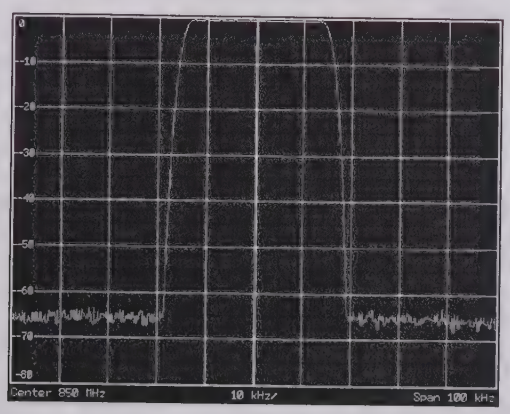

Fig. 2-38 Frequency response of the 30 kHz channel filter for measuring the power in the IS 95 adjacent channel

Measurement Example 2 – Measuring the adjacent channel power of an IS136 TDMA signal

Test setup:

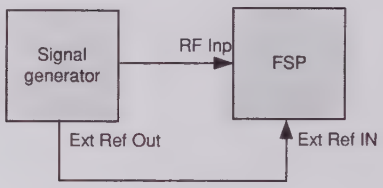

Note: *As the modulation spectrum of the IS136 signal leaks into the adjacent channel, it makes a contribution to the power in the adjacent channel. Exact tuning of the spectrum analyzer to the transmit frequency is therefore critical. If tuning is not precise, the adjacent channel power ratios in the lower and upper adjacent channels become asymmetrical. The FSP's frequency and the generator frequency are therefore synchronized.*

Settings on the signal generator (e.g. R&S SMIQ):
Frequency: 850 MHz
Level: -20 dBm
Modulation: IS136/NADC

Measurement with the FSP

1. ***Set the spectrum analyzer to its default state.***
   - Press the *PRESET* key.
     The FSP is in its default state.
2. ***Set up the FSP for synchronization to an external reference frequency.***
   - Press the *SETUP* key.
   - Set the *REFERENCE* softkey to *EXT.*
3. ***Set the center frequency to 850 MHz-***
   Press the FREQ key and enter *850 MHz.*
4. ***Configure adjacent channel power measurement for IS136 signals.***
   - Press the *MEAS* key.
   - Press the *CHAN PWR ACP* ⇩ softkey.
   - Press the *CP/ACP STANDARD* softkey.
   - Select *NADC IS136* from the list of standards and press *ENTER.*
     The FSP performs the power measurement in 5 channels (in the useful channel and in the two upper and two lower adjacent channels).

5. *Setting the optimum reference level and RF attenuation for the measurement*

➢ Press the *ADJUST REF LEVEL* softkey.
The FSP sets the optimum RF attenuation and the optimum reference level on the basis of the measured channel power.

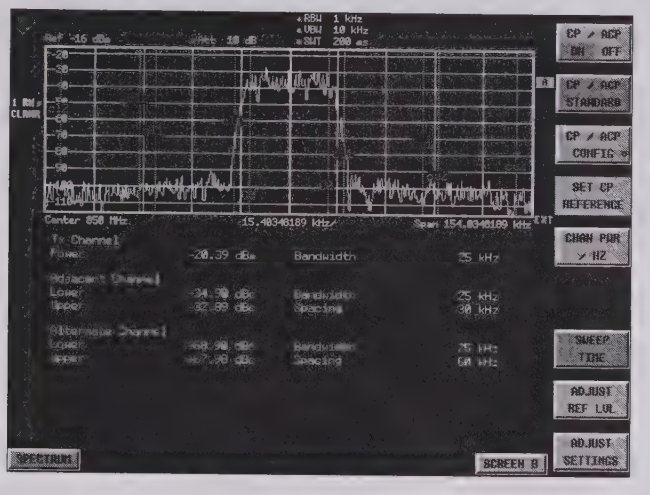

Fig. 2-39 Measuring the relative adjacent channel power of an NADC signal in each of the two adjacent channels below and above the transmit channel.

To increase repeatability - especially in the adjacent channels - the FSP's Fast ACP routine is recommended.

6. *Switching on the Fast ACP routine.*

➢ Press the *CP/ACP CONFIG* ⇩ softkey

➢ Set the *FAST ACP* softkey to *ON*.
The FSP makes consecutive measurements on the 5 channels in the Zero Span mode using the receive filter specified in IS 136 to define the resolution bandwidth. The power in each channel is displayed on the graph as a function of time

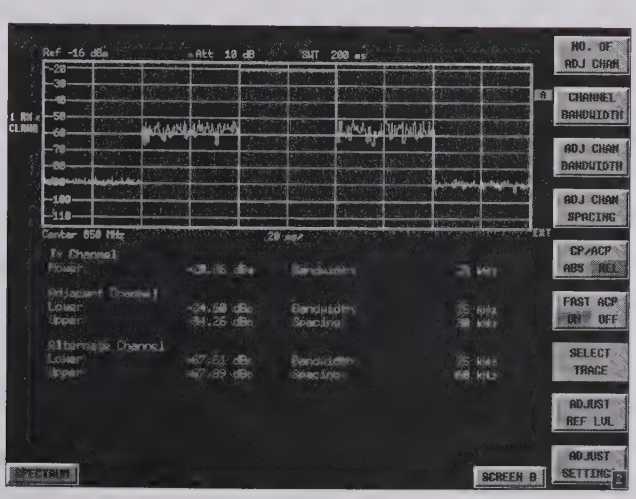

Fig. 2-40 Measuring adjacent channel power in time domain (Fast ACP)

As the resolution bandwidth is much wider than the one used for the integration method, the results are much more stable when compared at the same sweep time.

Repeatability can be influenced by the selected sweep time. The results become much more stable if long sweep times are selected. Since the amplitude distribution is different in different channels (part of the modulation spectrum falls within the first adjacent channel), the repeatability depends on the spacing of the measured channel from the transmit channel.
Fig. 2-41 below shows the standard deviation of results in the different channels as a function of the selected sweep time. The standard deviation for the various sweep times was recorded using a signal generator as a source. With real DUTs the amplitude distributions in adjacent channels may be different so that the standard deviation could differ from that shown in Fig. 2-41. To evaluate the correct measuring time for time-critical measurements at a given standard deviation, the standard deviation of the ACP values at the output of the real DUT must be determined.

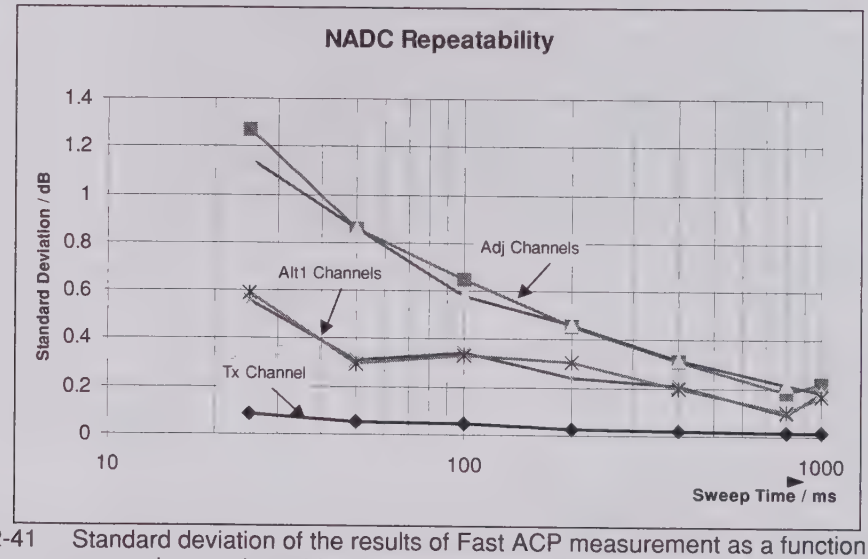

Fig. 2-41 Standard deviation of the results of Fast ACP measurement as a function of selected sweep time evaluated from 100 measurements per sweep time

Measurement Example 3 - Measuring the Modulation Spectrum in Burst Mode with the Gated Sweep Function

Since transmission systems compliant to IS136 use a TDMA method, the adjacent channel power must also be measured in burst mode. An IS136 TDMA frame is divided into 6 time slots. Two of these slots are assigned to a subscriber. This means that the ratio of transmit time to off-time for IS136 mobile phones is only 1:3 (e.g. time slots 1 and 4)

The FSP supports the measurement of the adjacent channel power in the TDMA mode with the Gated Sweep function.

Test setup with the R&S Signal Generator SMIQ:

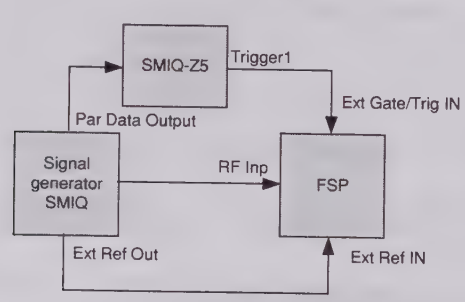

The SMIQ has to be equipped with options SMIQ-B10 or SMIQ-B20 (modulation coder) and SMIQ-B11 (data generator).

Option SMIQ-Z5 is required to trigger the FSP. This option is connected to the SMIQ's parallel output port. The BNC output Trigger 1 of the SMIQ-Z5 provides a TTL trigger signal on the rising edge of the IS136 burst, which is used to start the FSP sweep in the Gated Sweep mode.

Note: *The FSP's IF power trigger is not suitable for IS136. It triggers on every level edge of the input signal. Since the modulation of the IS136 signal causes level dips even during the transmit burst, there is no way of ensuring that the FSP is only triggered on the burst edge.*

Settings on signal generator SMIQ:

Switch the signal generator to the IS136 burst mode (time slots 1 and 4 are switched on, the other time slots are switched off).

The SMIQ is set as follows to generate the signal :

- Press the *PRESET* key.
- Press the *FREQ* key and enter 850 MHz.
- Press the *LEVEL* key and enter -20 dBm.
- Press the *RETURN* key.
- Select *DIGITAL STANDARD* using the spinwheel and press the *SELECT* key.
- Select *NADC* using the spinwheel and press the *SELECT* key.
- Press the *SELECT* key.
- Select *ON* using the spinwheel and press the *SELECT* key.
- Press the *RETURN* key.
- Keep turning the spinwheel until *SAVE/RECALL FRAME* appears in the list and select the menu item *SAVE/RECALL FRAME* using the *SELECT* key.
- The cursor is set to *GET PREDEFINED FRAME*.
- Press the *SELECT* key.

➢ Select *UP1TCH* using the spinwheel and press the *SELECT* key.

In the following operating sequence for the FSP, it is assumed that steps 1 to 6 of the previous example (example no. 2) have already been performed.

1. Configuring the Gated Sweep function on the FSP.

➢ Press the *TRIG* key.

➢ Press the *GATED TRIGGER* softkey.

➢ Press the *EXTERN* softkey.

➢ Press the *GATE SETTINGS* ⇩ softkey.
The FSP switches to time domain measurement so that the setting of the Gated Sweep parameters can be checked visually.

➢ Press the *ZOOM X-AXIS* softkey and enter *10 ms*.
Exactly one TDMA burst will be displayed.

➢ Press the *GATE DELAY* softkey and enter *2 ms* or set the Gate Delay using the spinwheel so that the burst is reliably detected.

➢ Press the *GATE LENGTH* softkey and enter *5 ms* or set the vertical line for the gate length using the spinwheel so that the burst is reliably detected.

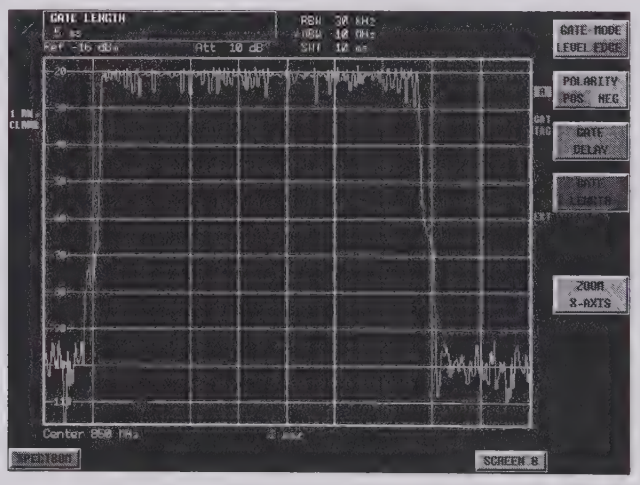

Fig. 2-42 Setting the parameters Gate Delay and Gate Length in time domain. The time interval required to measure the spectrum is indicated by two vertical lines.

➢ Press the *PREV* key.
The FSP now performs the ACP measurement only during the switch-on phase of the TDMA burst. The measurement is stopped during the switch-off phase.

Note:	*The selected sweep time is the net sweep time, i.e. the time during which the FSP is actually measuring. The complete frame of an IS136 signal takes 40 ms. In the above example, measurement only takes place for 2x5 ms within a frame. The FSP is therefore only measuring for 25 % of the frame duration. The total measuring time is therefore four times that for the CW mode.*

Measurement Example 4 - Measuring the Transient Spectrum in Burst Mode with the Fast ACP function

In addition to the modulation spectrum or adjacent channel power from the modulation of the RF carrier, the spectrum or adjacent channel power generated by burst edges is also to be measured in TDMA systems. The spectrum is a pulse spectrum and must be measured with the peak detector. With the usual IBW method, only the power of the continuously modulated signal can be measured properly. Even if the modulation spectrum is transmitted in the TDMA mode, the measurement of the modulation spectrum will work because the burst edges are blanked out for the measurement by means of the Gated Sweep function. The spectrum analyzer performs measurements only if the modulation spectrum is continuous when the burst is on.

However, the IBW method fails for the spectrum created by the burst edges. As the measurement is carried out with resolution bandwidths that are very small compared to the signal bandwidth, a spurious amplitude distribution is obtained in the defined measurement channel because of the resolution bandwidth. The small resolution bandwidth cannot settle to the peak amplitudes of the test signal. This problem is avoided in the FSP by performing time domain measurements with the root raised cosine filter specified in the IS136 standard.

If the peak detector is used instead of the default RMS detector (which is selected when the standard is selected), the true adjacent channel power generated by the burst edges can also be measured.

Test setup: The test setup for this example and the settings for SMIQ are identical to those in the previous example.

Measurement with the FSP:

1. ***Set the spectrum analyzer to its default state.***
   - ➢ Press the *PRESET* key.
     The FSP is in its default state.
2. ***Synchronize the FSP to an external reference frequency.***
   - ➢ Press the *SETUP* key.
   - ➢ Set the *REFERENCE* softkey to *EXT*.
3. ***Set the center frequency to 850 MHz***
   - ➢ Press the *FREQ* key and enter *850 MHz*.
4. ***Configure the adjacent channel power measurement for IS136 signals in Fast ACP mode.***
   - ➢ Press the *MEAS* key.
   - ➢ Press the *CHAN PWR ACP* ⇩ softkey.
   - ➢ Press the *CP/ACP STANDARD* softkey.
   - ➢ Select *NADC IS136* from the list of standards and press *ENTER*.
   - ➢ Press the *CP/ACP CONFIG* ⇩ softkey.
   - ➢ Set the *FAST ACP* softkey to *ON*.
     The FSP performs the power measurement in 5 channels (in the useful channel and in the two upper and lower adjacent channels).
5. ***Set the optimum reference level and RF attenuation for the measurement.***
   - ➢ Press the *ADJUST REF LEVEL* softkey.
     The FSP sets the optimum RF attenuation and the optimum reference level on the basis of the measured channel power.

6. Select the peak detector and increase the sweep time to 10 s.

- Press the *TRACE* key.
- Press the *DETECTOR* softkey.
- Press the *PEAK* softkey.
- Press the *SWEEP* key.
- Press the *SWEEP TIME* softkey and enter *10 s*.
  The FSP measures the adjacent channel power generated by the burst edges and the modulation.

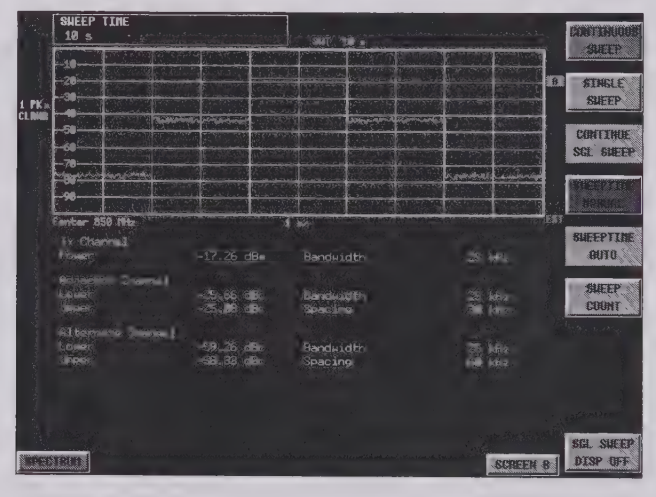

Fig. 2-43 Adjacent channel power due to modulation spectrum and transient spectrum

Note:	*The peak power display depends on the selected sweep time. The longer the sweep time, the higher the probability of measuring the highest peak amplitude of the signal. With shorter sweep times, level dips can be seen in the time domain traces. These level dips come from the burst characterics of the signal. The numerical results, however, indicate the peak amplitudes during the measurement in the corresponding channel.*

Measurement Example 5 - Measuring adjacent channel power of a W-CDMA uplink signal

Test setup:

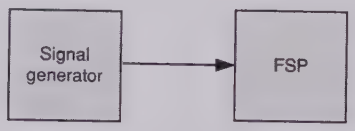

Settings on the signal generator (e.g. R&S SMIQ):
Frequency: 1950 MHz
Level: 4 dBm
Modulation: W-CDMA Reverse Link (NTT-DoCoMo, 4.096 Mcps)

Measurement with the FSP:

1. ***Set the spectrum analyzer to its default state.***

   ➢ Press the *PRESET* key.
   The FSP is in its default state.

2. ***Set the center frequency to 1950 MHz.***

   ➢ Press the *FREQ* key and enter *1950 MHz.*

3. ***Switch on the ACP measurement for W-CDMA.***

   ➢ Press the *MEAS* key.

   ➢ Press the *CHAN PWR ACP* ⇩ softkey.

   ➢ Press the *CP/ACP STANDARD* softkey.

   ➢ From the list of standards, select *W-CDMA 4.096 REV* using the spinwheel or the cursor down key below the spinwheel and press *ENTER.*
   The FSP sets the channel configuration to the W-CDMA standard (NTT-DoCoMo and ARIB, 4.096 Mcps) for mobiles with two adjacent channels above and below the transmit channel. The frequency span, the resolution and video bandwidth and the detector are automatically set to the correct values. The spectrum is displayed in the upper part of the screen and the channel power, the level ratios of the adjacent channel powers and the channel configuration in the lower part of the screen. The individual channels are displayed as vertical lines on the graph.

4. ***Set the optimum reference level and the RF attenuation for the applied signal level.***

   ➢ Press the *ADJUST REF LEVEL* softkey.
   The FSP sets the optimum RF attenuation and the reference level for the power in the transmission channel to obtain the maximum dynamic range. The following figure shows the result of the measurement:

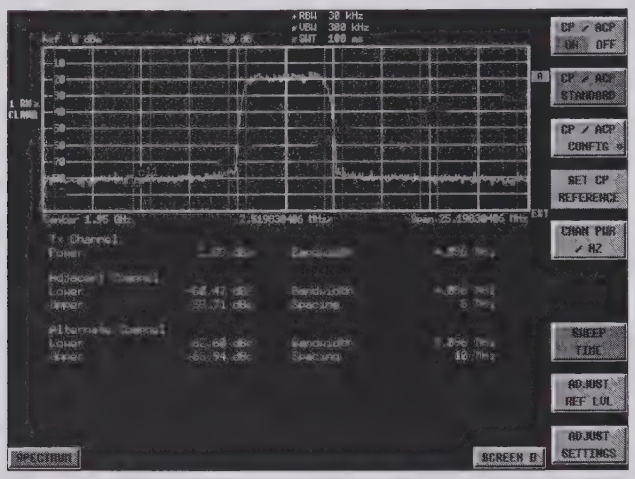

Fig. 2-44 Measuring the relative adjacent channel power on a W-CDMA uplink signal

5. Measuring adjacent channel power with the Fast ACP method.

- Press the *CP/ACP CONFIG* ⇩ softkey.
- Set *FAST ACP* softkey to *ON*.
- Press the ADJUST REF LVL softkey.
  The FSP measures the power of the individual channels in the time domain. A root raised cosine filter with the parameters $\alpha = 0.22$ and chip rate 4.096 Mcps (= receive filter for W-CDMA) is used as the channel filter.

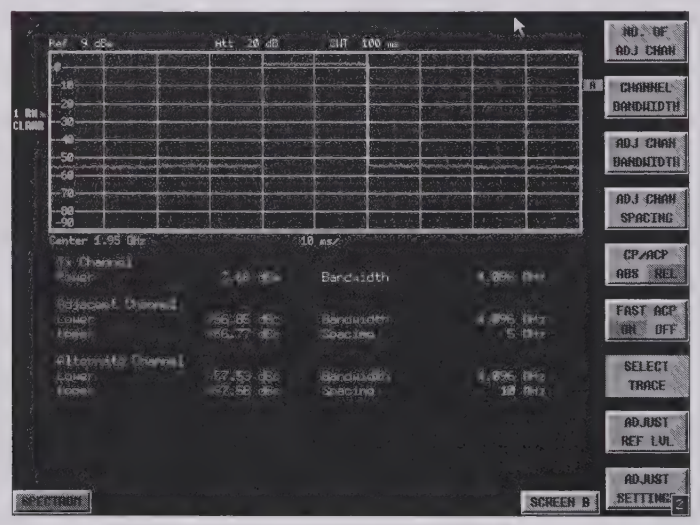

Fig. 2-45 Measuring the adjacent channel power of a W-CDMA signal with the Fast ACP method

Note:	*With W-CDMA, the FSP's dynamic range for adjacent channel measurements is limited by the 12-bit A/D converter. The greatest dynamic range is, therefore, obtained with the IBW method.*

Optimum Level Setting for ACP Measurements on W-CDMA Signals

The dynamic range for ACPR measurements is limited by the thermal noise floor, the phase noise and the intermodulation (spectral regrowth) of the spectrum analyzer. The power values produced by the FSP due to these factors accumulate linearly. They depend on the applied level at the input mixer. The three factors are shown in the figure below for the adjacent channel (5 MHz carrier offset)

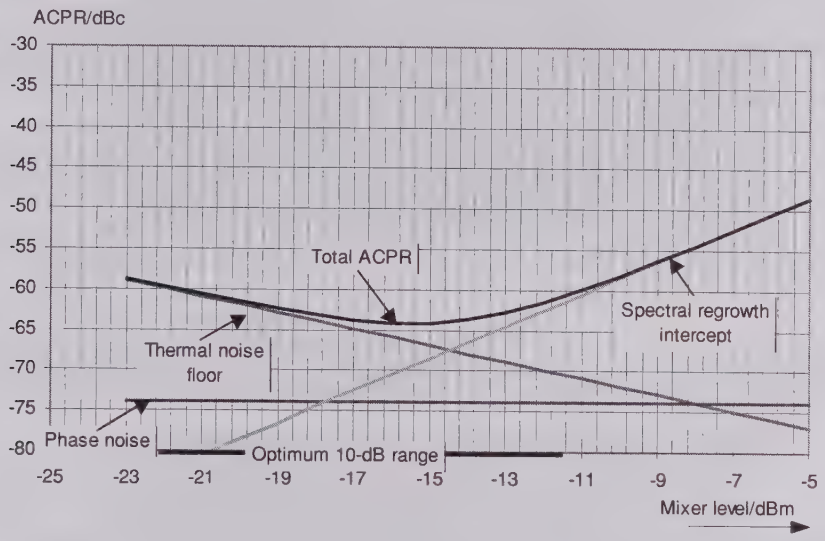

Fig. 2-46 The FSP's dynamic range for adjacent channel power measurements on W-CDMA uplink signals is a function of the mixer level.

The level of the W-CDMA signal at the input mixer is shown on the horizontal axis, i.e. the measured signal level minus the selected RF attenuation. The individual components which contribute to the power in the adjacent channel and the resulting relative level (total ACPR) in the adjacent channel are displayed on the vertical axis. The optimum mixer level is –16 dBm. The relative adjacent channel power (ACPR) at an optimum mixer level is –64 dBc. Since, at a given signal level, the mixer level is set in 10 dB steps with the 10 dB RF attenuator, the optimum 10 dB range is shown in the figure: it spreads from –11 dBm to –21 dBm. The obtainable dynamic range in this range is 60 dB.

To set the attenuation parameter manually, the following method is recommended:

- Set the RF attenuation so that the mixer level (= measured channel power – RF attenuation) is between -11 dBm and -21 dBm.
- Set the reference level so that it is 20 dB less than the RF attenuation which has been set.

This method is automated with the FSP's ADJUST REF LEVEL function. Especially in remote control mode, e.g. in production environments, it is best to correctly set the attenuation parameters prior to the measurement, as the time required for automatic setting can be saved.

Note: *To measure the FSP's intrinsic dynamic range for W-CDMA adjacent channel power measurements, a filter which suppresses the adjacent channel power is required at the output of the transmitter. A SAW filter with a bandwidth of 4 MHz, for example, can be used.*

Amplitude distribution measurements

If modulation types that do not have a constant envelope in the time domain are used, the transmitter has to handle peak amplitudes that are greater than the average power. This includes all modulation types that involve amplitude modulation -QPSK for example. CDMA transmission modes in particular may have power peaks that are large compared to the average power.

For signals of this kind, the transmitter must provide large reserves for the peak power to prevent signal compression and thus an increase of the bit error rate at the receiver.
The peak power, or the crest factor of a signal is therefore an important transmitter design criterion. The crest factor is defined as the peak power / mean power ratio or, logarithmically, as the peak level minus the average level of the signal.

To reduce power consumption and cut costs, transmitters are not designed for the largest power that could ever occur, but for a power that has a specified probability of being exceeded (e.g. 0.01%). .

To measure the amplitude distribution, the FSP has simple measurement functions to determine both the APD[1] = Amplitude Probability Distribution and CCDF = Complementary Cumulative Distribution Function.

In the APD display mode, the probability of occurrence of a certain level is plotted against the level.
In the CCDF display mode, the probability that the mean signal power will be exceeded is shown in percent.

Measurement Example – Measuring the APD and CCDF of white noise generated by the FSP

1. Set the spectrum analyzer to its default state.

- Press the *PRESET* key.
  The FSP is in its default state.

2. Configure the FSP for APD measurement

- Press the *AMPT* key and enter *-60 dBm*.
  The FSP's intrinsic noise is displayed at the top of the screen.
- Press the *MEAS* key.
- Press the *SIGNAL STATISTIC* ⇩ softkey.
- Set the *APD* softkey to *ON*.
  The FSP sets the frequency span to 0 Hz and measures the amplitude probability distribution (APD). The number of uncorrelated level measurements used for the measurement is 100000. The mean power and the peak power are displayed in dBm. The crest factor (peak power – mean power) is output as well (see Fig. 2-47).

[1] In the literature, APD is also used for the probability of amplitude violation. This is the complimentary function to the APD function of FSP. The term PDF (=Probability Density Function) which is frequently used in the literature corresponds to the APD function of FSP.

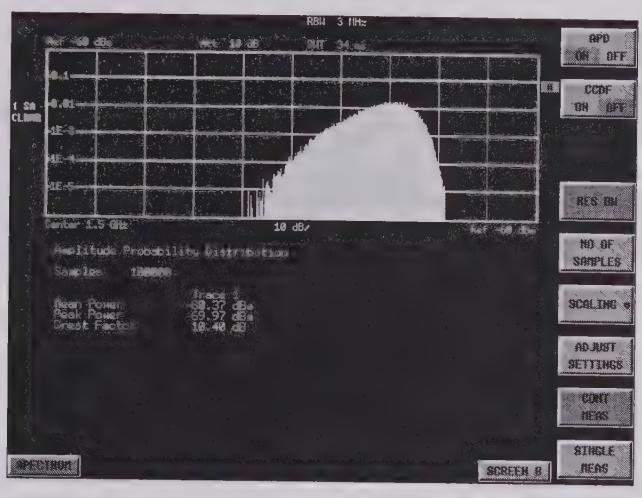

Fig. 2-47 Amplitude probability distribution of white noise

3. *Switch to the CCDF display mode.*

➢ Set the *CCDF* softkey to *ON*
The APD measurement is switched off and the CCDF display mode is switched on.

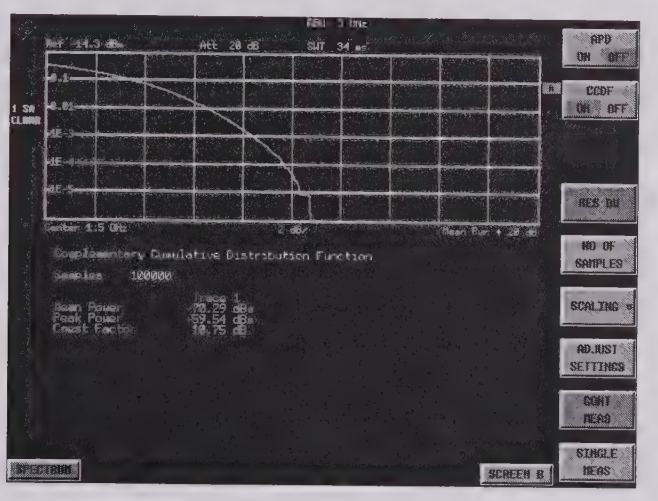

Fig. 2-48 The CCDF of white noise

The CCDF trace indicates the probability that a level will exceed the mean power. The level above the mean power is plotted along the X axis of the graph.The origin of the axis corresponds to the mean power level. The probability that a level will be exceeded is plotted along the Y axis.

4. Bandwidth selection

If the amplitude distribution is measured, the resolution bandwidth must be set in a way that the complete spectrum of the signal to be measured falls within the bandwidth. This is the only way of ensuring that all the amplitudes will pass through the IF filter without being distorted. If the selected resolution bandwidth is too small for a digitally modulated signal, the amplitude distribution at the output of the IF filter becomes a Gaussian distribution according to the central limit theorem and so corresponds to a white noise signal. The true amplitude distribution of the signal therefore cannot be determined.

A video bandwidth which is large in comparison to the resolution bandwidth ($\geq 3 \times$ RBW) must be selected. This ensures that the amplitude peaks of the signal are not smoothed by the lowpass effect of the video filter. The video bandwidth is set automatically during statistics measurements.

Since the video bandwidth of the FSP is limited to 10 MHz, lowpass filtering occurs during measurements with a resolution bandwidth of 10 MHz. Additional band-limiting occurs at a resolution bandwidth of 10 MHz due to the lowpass filtering at the output of the log amplifier. The latter limits the video signal to a bandwidth of 8 MHz in order to obtain sufficient suppression of the 20.4 MHz IF. The level range of the signal amplitudes, e.g. during APD white-noise measurements, is smaller. For broadband-modulated signals such as W-CDMA signals, the effect depends on the bandwidth occupied by the signal. At a signal bandwidth of 4 MHz, the amplitude distribution can be measured correctly with the effective video bandwidth.

5. Selecting the number of samples

For statistics measurements with the FSP, the number of samples $N_{Samples}$ is entered for statistical evaluation instead of the sweep time. Since only statistically independent samples contribute to statistics, the measurement or sweep time is calculated automatically. It is indicated on the FSP display. The samples are statistically independent if the time difference is at least 1/RBW. The sweep time SWT is, therefore, expressed as follows:

$SWT = N_{Samples} / RBW$

Time Domain Measurements

With TDMA radiocommunication systems (e.g. GSM or IS136), the transmission quality is determined not only by the spectral characteristics, but also by the time domain characteristics. Since several users share the same frequency, a time slot is assigned to the each user. Unimpaired operation can only be ensured if each user adheres to his assigned time slot.

In this case, both the power during the transmit phase and the time characteristics such as duration of the TDMA burst as well as rise and fall time of the burst are relevant.

Power measurements

The FSP has easy-to-operate functions for measuring power during a given time interval.

Measurement Example – Measuring the power of a GSM burst during the switch-on phase

Test setup:

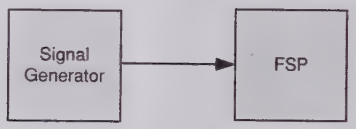

Settings on the signal generator (e.g. R&S SMIQ):
Frequency: 100 MHz
Level: 0 dBm
Modulation: GSM, one time slot is switched on

Measurement using the FSP:

1. ***Set the spectrum analyzer to its default state.***
   - Press the *PRESET* key.
     The FSP is in its default state.
2. ***Set the center frequency to 100 MHz, the span to 0 Hz and the resolution bandwidth to 1 MHz.***
   - Press the *FREQ* key and enter *100 MHz*.
   - Press the *SPAN* key and enter *0 Hz* or press the *ZEROSPAN* softkey.
3. ***Set the FSP reference level to 10 dBm (= signal generator level +10 dB).***
   - Press the *AMPT* key and enter *10 dBm*.
4. ***Set the sweep time to 1 ms***
   - Press the *SWEEP* key and enter 1 ms.
     The FSP shows the GSM burst running across the display.

5. Trigger on the rising edge of the burst using the video trigger.

- Press the *TRIG* key.
- Press the *VIDEO* softkey and enter *70%*.
  The FSP displays a stable curve with the GSM burst at the beginning of the trace. The trigger level is shown as a horizontal line labeled with the absolute level for the trigger threshold.

6. Configure the power measurement in the time domain.

- Press the *MEAS* key.
- Press the *TIME DOM POWER* ⇩ softkey.
- Set the *LIMITS* softkey to *ON*.
- Press the *START LIMIT* softkey.
- Place the vertical line on the start of the burst by turning the spinwheel clockwise.
- Press the *STOP LIMIT* softkey.
- Place the second vertical line on the end of the burst by turning the spinwheel counterclockwise.
  The FSP displays the mean power during the switch-on phase of the burst (see Fig. 2-49).

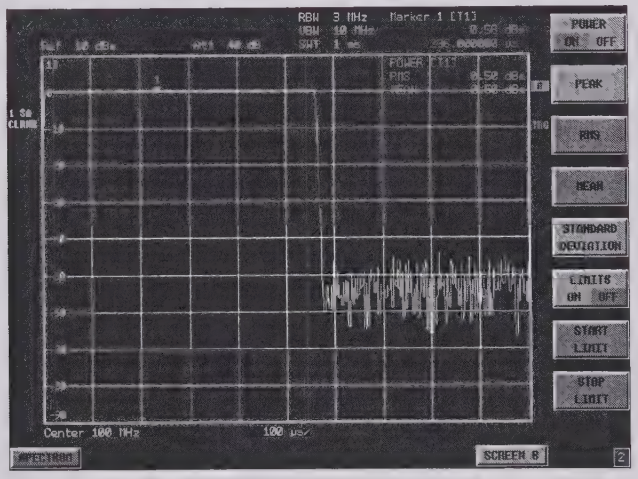

Fig. 2-49 Measuring mean power during the switch-on phase of a GSM burst

Power Ramping Measurement for Burst Signals

Since the FSP has a high time resolution at 0 Hz span, the edges of the TDMA burst can be measured accurately. The use of the trigger offset makes it possible to shift the edges onto the screen.

Measurement Example – Measurements on GSM burst edges using a high time resolution

Test setup:

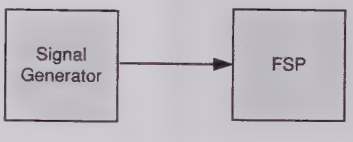

Settings on the signal generator (e.g. R&S SMIQ):
Frequency: 100 MHz
Level: 0 dBm
Modulation: GSM, one time slot is switched on

Measurement using the FSP

The settings of the example above are used to measure GSM burst power during the switch-on phase.

1. ***Switch off power measurement.***
   - ➢ Press the *MEAS* key.
   - ➢ Press the *TIME DOM POWER* ⇩ softkey.
   - ➢ In the submenu, set the *POWER* softkey to *OFF*.
2. ***Increase the time resolution to 100 µs.***
   - ➢ Press the *SWEEP* key and enter *100 µs*.
3. ***Shift the rising edge of the GSM burst to the middle of the screen using the trigger offset.***
   - ➢ Press the *TRIG* key.
   - ➢ Press the *TRIGGER OFFSET* softkey.
   - ➢ Set the trigger offset by turning the spinwheel (counterclockwise) until the burst edge is in the middle of the screen or enter *-50 µs*.
     The FSP displays the rising edge of the GSM burst (see Fig. 2-50)

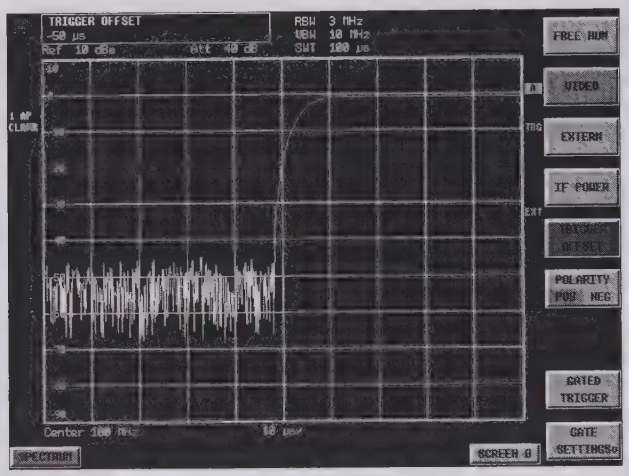

Fig. 2-50 Rising edge of GSM burst at high time-resolution.

4. Shift the falling edge of burst to the middle of the screen using the trigger offset.

➢ Set the *POLARITY* softkey to *NEG*.
The FSP displays the falling edge of the GSM burst (see Fig. 2-51)

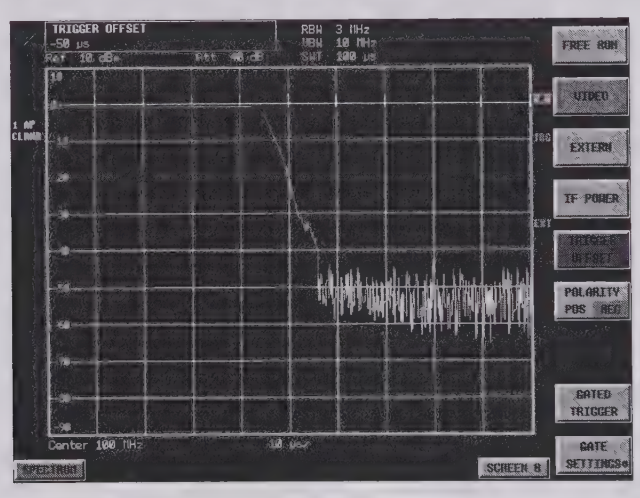

Fig. 2-51 Falling edge of GSM burst at high time resolution

Measuring the S/N Ratio of Burst Signals

For TDMA transmission methods, the S/N ratio or the switch-off range can be measured by comparing the powers during the switch-on and switch-off phase of the transmission burst. The FSP, therefore, has a function to perform absolute and relative power measurements in the time domain. The measurement is carried out as follows, using a GSM burst as an example.

Measurement Example - S/N ratio of a GSM signal

Test setup:

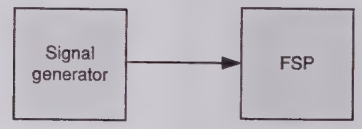

Settings on the signal generator (e.g. R&S SMIQ):
Frequency: 100 MHz
Level: 0 dBm
Modulation: GSM, one time slot is switched on

Measurement using the FSP

1. ***Set the spectrum analyzer to its default state.***
   - Press the *PRESET* key.
     The FSP is in its default state.
2. ***Set the center frequency to 100 MHz, the span to 0 Hz and the resolution bandwidth to 1 MHz.***
   - Press the *FREQ* key and enter *100 MHz*.
   - Press the *SPAN* key and enter *0 Hz*
     or
   - press the *ZEROSPAN* softkey.
   - Press the *BW* key and enter *1 MHz*.
3. ***Set the reference level of the FSP to 0 dBm (= signal generator level) and the RF attenuation to 10 dB for maximum sensitivity.***
   - Press the **AMPT** key and enter 0 **dBm**.
   - Press the *RF ATTEN MANUAL* softkey and enter *10 dB*.
4. ***Set the sweep time to 2 ms.***
   - Press the *SWEEP* key and enter *2 ms*.
     The FSP displays the GSM burst running across the display.

5. Trigger on the rising edge of the burst using the video trigger and shift beginning of burst to the middle of the screen.

- Press the TRIG key.
- Press the VIDEO softkey and enter 70%.
  The FSP displays a stable image with the GSM burst at the start of the trace.
- Press the TRIGGER OFFSET softkey and enter -1 ms.
  The FSP displays the GSM burst in the right half of the graph.

6. Configure the power measurement in the time domain.

- Press the MEAS key.
- Press the TIME DOM POWER ⇩ softkey.
- Set the LIMITS softkey to ON.
- Press the *START LIMIT* softkey.
- Place the vertical line on the start of the burst using the spinwheel.
- Press the *STOP LIMIT* softkey.
- Place the second vertical line on the end of the burst using the spinwheel. .
  The FSP displays the power during the switch-on phase of the burst.

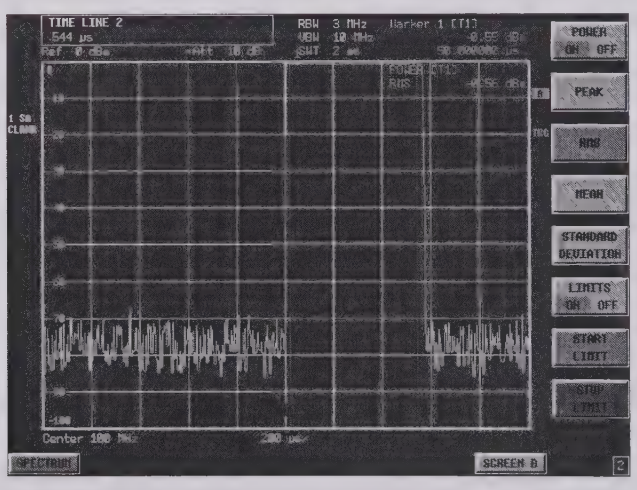

Fig. 2-52 Measuring power during the switch-on phase of the burst

7. Define the measured power as the reference and switch on relative power measurement.

- Press the *NEXT* key.
  The side menu for setting the power measurement is opened.
- Set the *POWER ABS/REL* softkey to *REL*.
- The power relative to the power during the switch-on phase of the burst is displayed.
- Press the *SET REFERENCE* softkey.
  The measured power of the GSM burst is defined as the reference.

8. *Measure the power during the switch-off phase of the burst.*

➢ Press the *TRIG* key.

➢ Set the *POLARITY POS/NEG* softkey to *NEG*.
The FSP triggers on the falling edge of the burst. The burst is then shifted to the left half of the screen. The power is measured in the switch-off phase. The start of the burst is shifted to the middle of the screen and the power is measured during the switch-off phase relative to the reference power (= burst power).

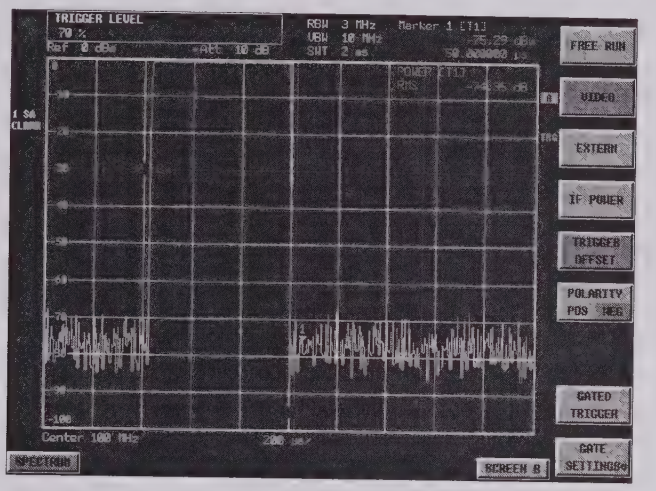

Fig. 2-53 Measuring the S/N ratio of the GSM burst signal in the time domain

Contents - Chapter 3 "Manual Operation"

3 Manual Operation 3.1
The Screen 3.1
Diagram Area 3.2
Indications in the Diagram Area 3.3
Full Screen 3.8
Split Screen 3.8
Softkey Area 3.9
Hotkey Area 3.10
Calling and Changing the Menus 3.10
Setting Parameters 3.11
Numeric Keypad 3.11
Roll-key and Cursor Keys 3.12
Selection and Setting of Parameters via Keys or Softkeys 3.13
Editing of Numeric Parameters 3.16
Entry of Alphanumeric Parameter 3.19
Editing with External Keyboard 3.19
Editing with Help Line Editor 3.20
Selection and Setting of Parameters via Tables 3.21
Menu Overview 3.24
FREQUENCY Key 3.24
SPAN Key 3.25
AMPT Key 3.26
MKR Key 3.27
MKR-> Key 3.28
MKR FCTN Key 3.29
BW Key 3.30
SWEEP Key 3.31
MEAS Key 3.32
TRIG Key 3.33
TRACE Key 3.34
LINES Key 3.35
DISP Key 3.36
FILE Key 3.37
CAL Key 3.38
SETUP Key 3.39
HCOPY Key 3.40
Hotkey Menu 3.41
LOCAL Menu 3.41
Menu Overview Network Mode 3.42
Menu Overview Option Ext. Generator Control 3.43

3 Manual Operation

Chapter 3 provides an overview of the operating concept and the basic steps of manual operation of the FSP. This includes a description of the screen, of the control of menus and of the setting of parameters. An overview of the menus will be listed at the end of this chapter.

The functions of the menus are described in dtail in Chapter 4. Chapter 2 contains a short introduction on step-by-step simple measurements. The remote control of the instrument is described in Chapters 5, 6 and 7

The operation of the spectrum analyzer is menu-controlled via keys, hotkeys and softkeys. The setting of the instrument and test parameters in the menus is made either directly via softkeys or by entry of values in entry fields and by selection in tables. The operating mode and the screen mode is selected via the hotkeys.
If required, data entry windows and tables are superimposed on the screen.

The Screen

The screen informs continuously on the results and parameters of the selected measuring functions. It shows the assignment of the softkeys and menus, which are required for setting the measuring parameters. The display of test results, the softkey labeling and the type of menu depend on the selected measuring function.
The screen is subdivided into three areas:

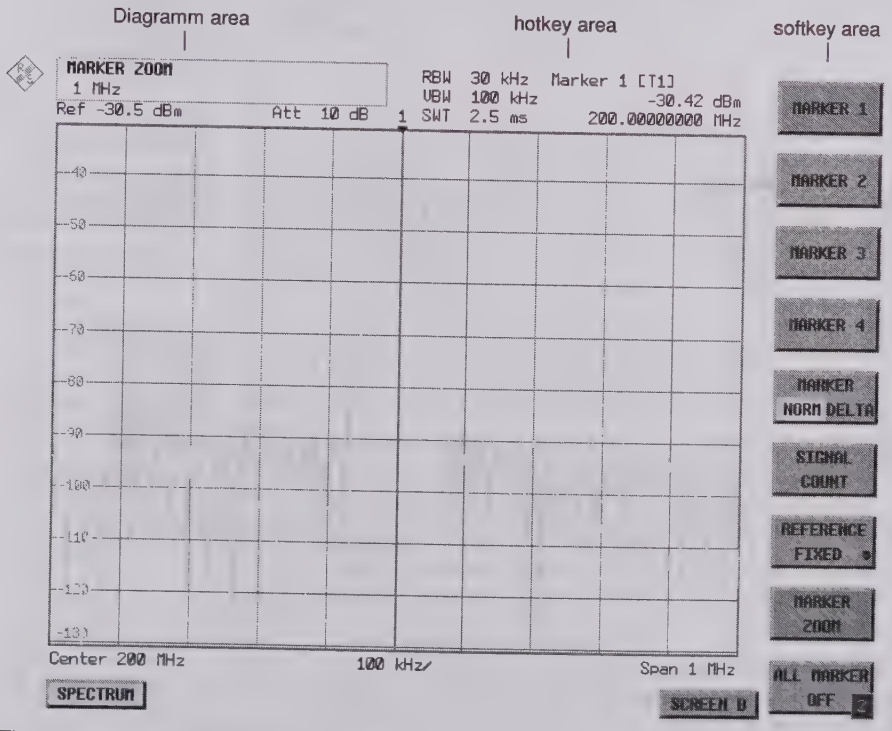

Fig. 3-1 Subdivision of screen

Diagram area This area contains the measuring diagrams and other measured-value information as well as the parameters and status information which are important for analysis of the results.
In addition, message fields, entry windows and tables may be shown in this area.

Softkey area This area contains the instrument functions which can be selected via the softkeys. The softkey area is not superimposed by other graphics.

Hotkey area This area contains the available operating modes and screen modes. The hotkey area is not superimposed by other graphics.

Diagram Area

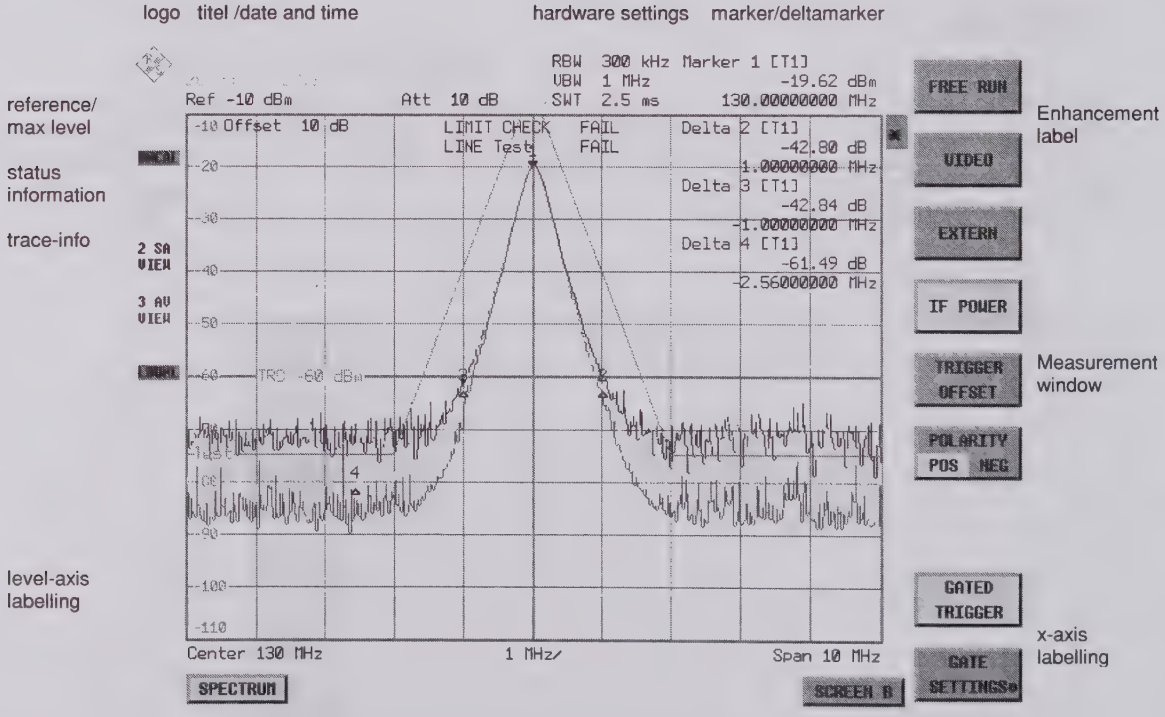

Fig. 3-2 Subdivision of the FSP screen in analyzer mode (without measuring diagram)

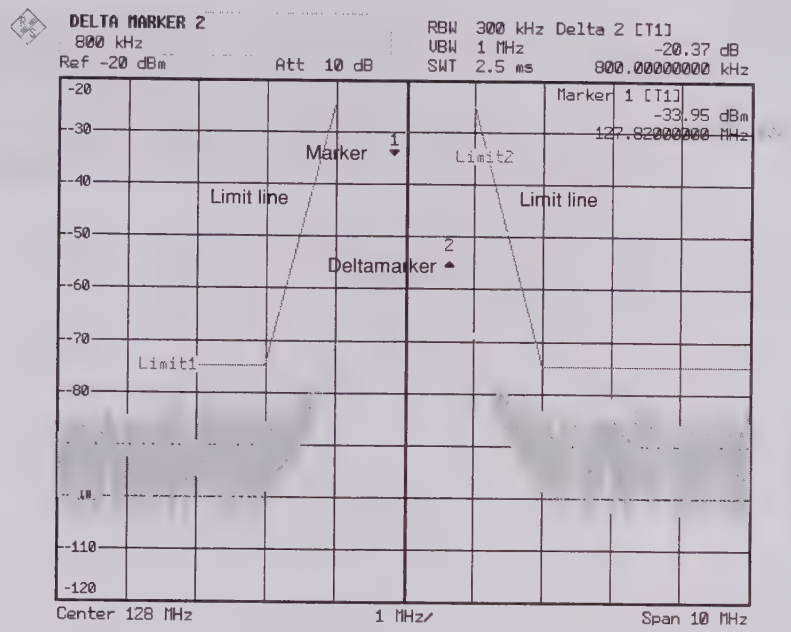

Fig.3-3 Measuring diagram

Indications in the Diagram Area

The following graphic elements are displayed in the diagram area:

General indications Indication of the logo

Logo

Screen title Indication of selected screen title

Date / time Indication of date and time

Hardware settings

Ref Indication of the reference level

Offset Indication of the offset of reference level.

Att Indication of the set RF attenuation.

RBW Indication of the set resolution bandwidth.
If the bandwidth does not correspond to the value of the automatic coupling, a green asterisk "*" is prefixed to the field.

VBW Indication of the set video bandwidth.
If the bandwidth does not correspond to the value of the automatic coupling, a green asterisk "*" is prefixed to the field.

SWT Indication of the set sweep time.
If the sweep time does not correspond to the value of the automatic coupling an asterisk "*" is prefixed to the field. The colour of the asterisk turns red as soon as the sweep time falls below the value of the automatic coupling.

Marker/deltamarker

This label displays the position of the last selected marker or deltamarker in the x and y-directions and the marker/deltamarker index. The square brackets contain the curve which the marker is assigned to and the active measuring function of the marker indicated. The measuring function of the markers in the second field is indicated by the following abbreviations:

FXD	reference fixed active
PHN	phase noise measurement active
CNT	frequency counter active
TRK	signal track active
NOI	noise measurement active
MOD	measurement of AM modulation depth active
TOI	TOI measurement active (3rd order intercept)

Limit check

Indication of the result of the limit check.

X-axis labelling

Display of the x-scaling.

The distance between two grid lines is displayed in this label.





The set center frequency or start frequency is displayed in this label depending on whether the keys FREQ/SPAN or the softkeys START/STOP were last pressed.
If span = 0 Hz, the center frequency is always displayed.







The set frequency range (*SPAN*) or the stop frequency is displayed, depending on whether the keys FREQ/SPAN or the softkeys START/STOP were last pressed.
If span = 0 Hz, the trigger moment (*PRETRIGGER*) is displayed.

Status information

The status information on the left side of the diagram hint at irregularity (e.g. UNCAL)

UNCAL

"UNCAL" is indicated under the following circumstances:

- correction data are switched off (menu CAL, CAL CORR OFF).
  ⇒ switch on CAL CORR ON or PRESET
- no valid correction data. This may occur after a cold start of the instrument following a firmware update.
  ⇒ record correction data
- Sweep time too short for current instrument settings (span, resolution bandwidth, video band width).
  ⇒ increase sweep time

OVLD / IFOVL

OVLD is indicated when the input mixer is overloaded.
⇒ Increase input attenuation

IFOVL is indicated when overload occurs in the IF signal path after the input mixer.
⇒ Increase reference level

MSG / LOUNL

MSG is indicated if a failure has occurred which impair correct measurement. The exact error message can be queried in the menu *SETUP SERVICE INFO*. The display disappears after the cause for the error has been eliminated.

LOUNL is indicated when an error occurs in the frequency processing of the instrument.

OVEN

OVEN is indicated when the crystal oscillator (option FSP-B4) has not yet reached its operating temperature. This indication vanishes after a few minutes after switch on.

Trace info:

Every active measurement curve (trace ≠ BLANK) is allocated a trace info of two or three lines at the left of the diagram. The trace info has the same colour as the measurement curve.

<n> <detector> <*>
<mode>
<trace math>

Example:

```
1 PK *
CLRWR
1-2
```

n = trace number (**1 ... 3**)

detector = selected detector
- **AP:** AUTOPEAK detector
- **PK:** MAX PEAK detector
- **MI:** MIN PEAK detector
- **SA:** SAMPLE detector
- **AV:** AVERAGE detector
- **RM:** RMS detector
- **QP:** QUASIPEAK detector

* = indicates that the selected detector does not correspond to that of the automatic coupling.

mode = indication of sweep mode
- **CLRWR:** CLEAR/WRITE
- **MAXH:** MAX HOLD
- **MINH:** MIN HOLD
- **AVG:** AVERAGE
- **VIEW:** VIEW

Trace math = trace math active
- **1 - 2** trace 1 - trace 2
- **1 - 3:** trace 1 - trace 3

Instrument settings
(Enhancement Labels)

Indication of user instrument settings which influence the measuring result and which are not immediately obvious when viewing the measured values.

***** The current instrument setting does not correspond to the one which applied when one of the displayed curves had been stored. This occurs under the following circumstances:

- The instrument setting is modified while a measurement is being performed.
- The instrument setting is modified in SINGLE SWEEP mode subsequent to the end of the sweep and no new sweep is started.
- The instrument setting is modified after setting the trace to VIEW.

The display is retained until the cause is eliminated by the user. I.e., either a new sweep is started (SINGLE SWEEP mode), or the trace of interest is switched to BLANK.

A / B Identification for screen A / B. When screen A / B is activated for the entry of test parameters, this label is highlighted.

SGL The sweep is set to SINGLE SWEEP.

GAT The frequency sweep is controlled via the *EXT TRIG/GATE* input of the instrument.

TRG The instrument is not triggered in *FREE RUN* mode.

LVL A level offset ≠ 0 dB has been set.

FRQ A frequency offset ≠ 0 Hz has been set.

PRN A printer output is active.

75 Ω The input impedance of the instrument is set to 75 Ω.

EXT The instrument is configured for operation with external reference

Entry fields:

Entry window The data entry window is superimposed in the left upper corner of the diagram area, if required. It covers the display of the title and the time. The field is used to enter numeric or alphanumeric device parameters.

Tables The tables are superimposed in the diagram area, if required. Sie dienen der Anzeige und Konfiguration von Geräteparametern.

Message windows:

Message field

Message fields provide notes on measurements, e.g. results of the limit check (PASS/FAIL).
These notes are no error messages, which are indicated as system messages.

They can be masked out by pressing the *ESC* key.

System messages

System messages indicate warnings and error messages.

Message without action field:
These system messages contain only arbitrary information. They hint at events which are of interest for the user but do not affect the measurement or functioning of the instrument.

They are deleted either automatically after a predefined time has passed (3 seconds) or upon any keystroke or mouse click.

Message with action field:
These system messages require a decision to be taken by the user. They are not deleted until any action has been selected. Deletion of the message initiates the action selected and appropriate measures to be taken. The action field consists of one (OK), two (OK/CANCEL) or three (arbitrary) buttons.
The user may select one of the buttons using the cursor keys and initiate the associated action by means of the unit keys. The ESC key is used to acknowledge the message without releasing any action.

Traces:

1 to 3

Up to 3 traces in each measurement diagram can be displayed simultaneously.

Limit lines

Limit lines are used to mark level curves or spectral distributions which must not be exceeded or dropped below.

The FSP provides two display modes:

- Full Screen: 1 window, the measurement is performed in the active diagram.
- Split Screen: 2 windows, the measurements are performed in both diagrams.

Full Screen

In the full-screen mode, the settings and measurements are performed in the active visible window. All indications on the screen refer to this window. The designation (SCREEN A or SCREEN B) is inserted as enhancement label A or B on the right diagram margin.
Switching between the windows is by means of *SCREEN A/B* hotkey. The current measurement is terminated when its window is blanked out.
Switching from split-screen to full-screen mode is performed in menu *DISP*.

Split Screen

In Split Screen mode, the screen is divided into two halves.

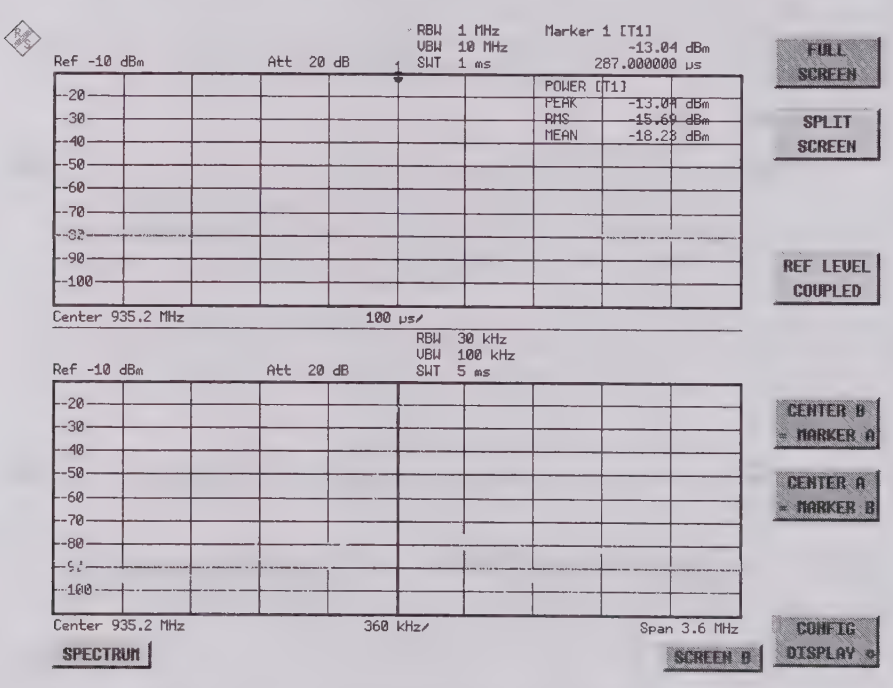

Fig.3-4 Subdivision of the screen in Split Screen mode

The upper half is assigned Screen A, the lower one Screen B. The settings for measurement can be selected independently for both screens. E.g., a spectrum may be displayed in Screen A and a time amplitude in the time range is displayed in Screen B.

The indications which are valid only for one window appear in the margin of the associated diagram. Indications which are valid for the two windows are displayed between the diagrams.

The window for entry of the measuring parameters or the marker operation is selected using the *SCREEN A/B* hotkey. The measurements are simultaneously performed in the two windows irrespective of the currently active one.
Switching from full-screen to split-screen mode is performed in menu *DISP*.

Softkey Area

The softkeys are assigned to the nine keys on the right side of the display
The setup of the softkey area is independent of the operating mode. It consists of the following graphic elements:

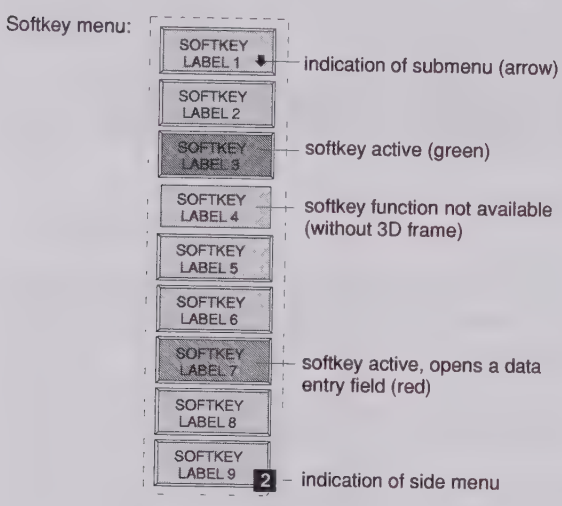

Fig.3-5 Setup of the softkey area

The softkeys have different functions depending on the instrument state. Therefore, their labeling can be varied. The labeling of all softkeys which call a submenu includes a ⇓ arrow.
The function and current state of the softkeys is indicated in the label by different texts and colors. The color assignment is factory-set as follows:

Table 3-1 Factory-set color assignment of soft keys

Softkey color	Meaning
gray	Softkey switched off
green	Softkey switched on
red	Softkey switched on and data entry active

These colors can be changed by the user as desired in the *DISP - CONFIG DISPLAY* menu.

A softkey is switched on or off by pressing the respective hardkey (see following section "Setting the Parameters").

Softkeys are masked out, too, if the functionality which they represent is not available. A distinction has to be made between two cases:

- If an instrument function depends on an option, and if this option is not fitted, the associated softkey is masked out,.
- If the instrument function is not available temporarily due to specific settings, the softkey is displayed without the 3D frame.

The label **2** on the right lower corner of the softkey area indicates that a side menu is available. The side menu is called by pressing the *NEXT* key.

Hotkey Area

Hotkeys are allocated to the eight keys on the bottom margin of the screen. They change between modes and the active diagrams.
The menu only shows the hotkeys which are actually used:

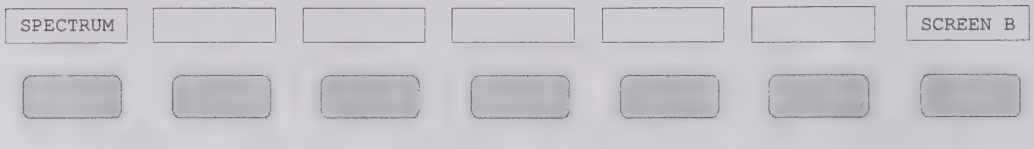

A keystroke activates the associated hotkey. An activated hotkey changes its frame:

Calling and Changing the Menus

The operation of the spectrum analyzer is menu-controlled via keys and softkeys. Various softkey menus are displayed depending on the instrument status. The individual menus constitute the so-called menu tree. The top menu (the root of the menu tree) is always called by means of a keystroke. Arrows at the lower edge of the softkey area indicate whether a supplementary menu can be entered or not.
Softkeys with an arrow allow for branching into further menus (so-called submenus): The field "2" at the lower right side of the softkey area indicates that this menu has a side menu.

The menu change keys on the front panel below the softkey area allow for switching between the main menu and the side menus and submenus.

The *NEXT* key calls the side menu.

The *PREVIOUS* key returns to the next higher menu.

Several menus provide for automatic change, i.e., return to the next higher menu is caused automatically after pressing a softkey.

Selection of a submenu is always effected via a softkey.

The labeling of all softkeys which call a submenu includes a ⇓ arrow.

Setting Parameters

Parameters are set either by simple selection (selection parameters) or by (alpha)numeric entries in data entry windows or tables.

The numeric keypad on the front panel, an external keyboard (optional), a roll-key and the cursor keys are provided for the entry of instrument parameters in an entry window or in a table.

The external keyboard is optional. If it is not fitted, the help line editor is called automatically for entry of alphanumeric parameters. The help line editor provides for selection of individual letters and a number of special characters which are copied into the actual entry window.

Numeric Keypad

The numeric keypad is provided for entry of numeric parameters. It contains the following keys:

- Number keys 0 to 9
- Decimal point
  Inserts a decimal point "." at the cursor position.
- Sign key
  Changes the sign of the mantissa or exponent of a numeric parameter.
  A "-" is inserted at the cursor position in case of an alphanumeric parameter.
- Unit keys (*GHz/-dBm*, *MHz/dBm*, *kHz/dB* and *Hz/dB*)
  - Provide the numeric value entered with the selected unit and terminate the entry.
    The unit keys are all assigned the value "1" for dimensionless quantities or for level entries (e.g., in dB). The unit keys thus assume the function of an *ENTER* key. The same applies for an alphanumeric entry.
  - Open and close the selection windows of tables.
- *BACK* key
  - Deletes the character left to the cursor with numeric entry.
  - Allows for toggling between the current and the previous values subsequent or prior to entry (UNDO function).
- *ESC/CANCEL* key
  - Aborts the entry before it has been terminated. The previous value is restored.
  - Closes the entry field after termination of input.
  - Closes system messages.
- *ENTER* key
  - Terminates the input of dimensionless quantities. The new value is set.

  Note: *The ENTER keys assumes the function of the Hz key for frequency input, and the function of the µs(kHz) key for time input.*

Roll-key and Cursor Keys

The roll-key and the cursor keys are arranged besides the numeric keypad.

The roll-key has various functions:

- With numeric entry, the instrument parameter is incremented (turning clockwise) or decremented (turning counterclockwise) at a defined step size.
- In tables, the roll-key can be used to shift the cursor horizontally or vertically when no entry window is open. The direction (horizontal/ vertical) is switched over using the cursor keys.
- The roll-key is used with the help-line editor to select the individual letters.
- It can be used to shift markers, display lines, limit lines etc.
- Pressing the roll-key terminates the input of parameters.

In tables, the cursor keys are used to shift the cursor between the lines and columns of the table.

The keys ◁ and ▷ are used to shift the cursor inside the entry window to reach a particular position in the string.

The keys △ and ▽

- increase or decrease the value of a parameter for numeric input .
- switch between editing line and help line editor for alphanumeric input.

Selection and Setting of Parameters via Keys or Softkeys

The selection of parameters and their settings is effected by means of a key, a softkey or in a table depending on the hierarchical level of the menu they are assigned to. Selection and setting of parameters in tables is described in section "Selection and Setting of Parameters in Tables" .

Selection via key

Most keys of the network analyzer are used to enter menus where the selection and the settings are made. Few settings can be made directly by means of a keystroke, only.

Example: Call up of preset settings

➢ Press *PRESET* key

The spectrum analyzer is brought into a predefined initial state.

Selection via softkey

In most cases the selection is made by pressing the respective softkey. There are various alternatives of making the selection:

1. The softkey is active or inactive.

Example: Switching on/off the frequency counter

➢ Press *MKR* key.

➢ Press *SIGNAL COUNT* softkey.

Each time the softkey is pressed, the marker info list is switched on or off. If the softkey is active (= marker info list on), it is illuminated.

2. The softkey acts like a toggle switch, each pressing changes the active selection.

Example: Selection of the reference (internal or external)

➢ Press *SETUP* key.

➢ Press *GENERAL SETUP* softkey, the *GENERAL SETUP* submenu is opened.

➢ Press *REFERENCE INT/EXT* softkey.

With each pressing, the checkmark on the softkey changes from INT (internal reference) to EXT (external reference) and vice versa. When in the active setting the softkey menu item is illuminated.

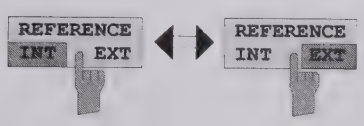

3. Various softkeys act like selection switches. Only one softkey may be active at a time.

Example: sweep setting

➢ Press *SWEEP* key.

➢ Press *CONTINOUS SWEEP* softkey.

The continuous sweep is thus set. The *CONTINOUS SWEEP* softkey is colored (factory-set: green). The second alternative, a series of n sweeps according to the trigger definition, can be selected via the *SINGLE SWEEP* softkey in the same menu. Only one of the two softkeys can be active at a time, the softkeys thus act like selection switches.

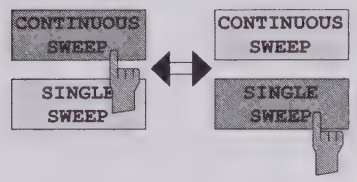

4. The softkey is used to select the parameter, the setting is made in an alphanumeric data entry window.

Example: SWEEP COUNT parameter

➢ Press *SWEEP* key

➢ Press *SWEEP COUNT* softkey.

The window for entering the number of sweeps for the SINGLE SWEEP mode is opened. The softkey is colored (factory-set: red). (Data entry is described in the next section).

4. The softkey is used to select the parameter, the setting is made in an (alpha)numeric data entry window. The softkey function is switched on. To switch off the function, the softkey has to be pressed again.

Example: parameter MARKER

➢ Press *MRK* key.

➢ Press *MARKER 1* softkey.

The window for entering the marker frequency is opened. The softkey is colored (factory set: red).
Marker1 is switched on and the peak search is started.

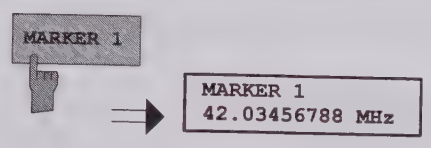

➢ Press *MARKER 2* softkey.

The entry window for the marker frequency of marker 2 is opened. The softkey is colored (red), marker 2 is switched on, and the *MARKER 1* softkey turns green.

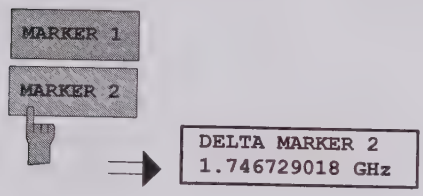

➢ Press *MARKER 1* softkey again.

Marker 1 is switched off.

5. The softkey selects the parameter, the setting is made in a selection table.

Example: Selection of the sorting criteria of a file list

➢ Press *FILE* key.

➢ Press *FILE MANAGER* softkey.

➢ Press *SORT MODE* softkey.

A selection table is displayed. The softkey is colored (factory-set: red). (operation see below).

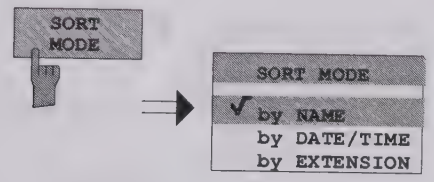

Editing of Numeric Parameters

The entry of numeric values is always made in a data entry window, which is displayed automatically after selection of the parameter.

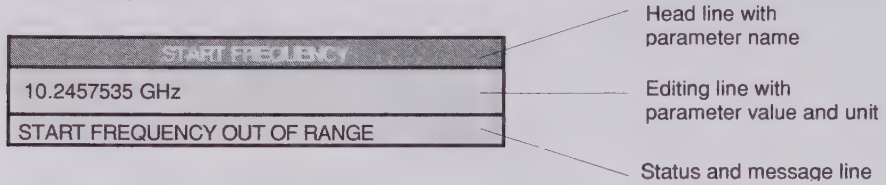
START FREQUENCY
10.2457535 GHz
START FREQUENCY OUT OF RANGE
Head line with parameter name
Editing line with parameter value and unit
Status and message line

The headline indicates the name of the instrument parameter, which has been selected. The entry is made in the editing line. Subsequent to calling the entry window, the current parameter value including the unit is displayed left-justified in the editing line. Status and error messages which refer to the current entry are displayed in the third and (optionally) fourth line.

Note: *Entry windows may be represented transparent (cf. DISPLAY - CONFIG DISPLAY menu)*

Entry of a numeric value

➢ Call data entry window (cf. selection of parameters)
The editing line indicates the current value

Example: center frequency (frequency-sweep mode)

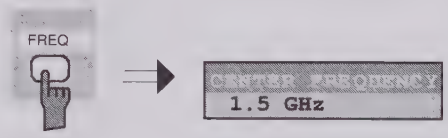

Entry via number keys

➢ Enter required value via number keys.

Example:

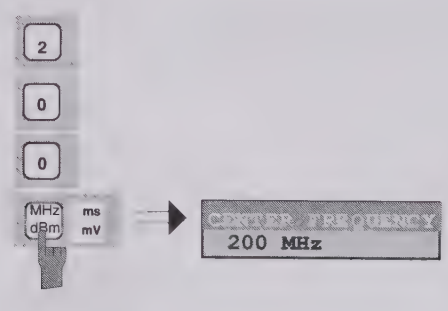

Entry via cursor keys

➢ Cursor ⇦ or ⇨ until obtaining the required value.

Example:

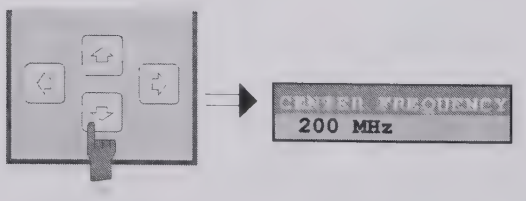

Entry via roll-key

➢ Rotate the roll-key until reaching the required value.

The variation step size increases with increasing rotational speed.

Turning the roll-key clockwise increases the value, turning it counterclockwise decreases the value.

Example:

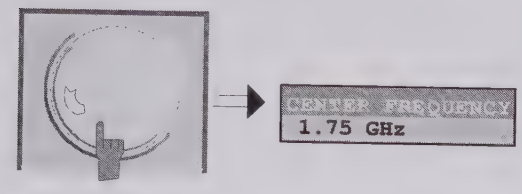

Note: *When the value is modified by means of the roll-key or the cursor keys the new value is immediately set.*

Terminating the entry

➢ Press one of the unit keys

The unit is entered in the entry window and the new setting is accepted by the instrument.

For dimensionless quantities:

➢ Press the ENTER key or the roll-key

The new setting is accepted by the instrument.

A few data entry windows close automatically whereas others like the entry window for the start frequency remain open even after termination of the entry. They can be closed by pressing the *ESC* key.

If an error occurs, a corresponding error message is displayed in the status line of the entry window, e.g., "Out of range", "Value adjusted", etc. In this case, the new value is not accepted for the instrument setting.

Example:

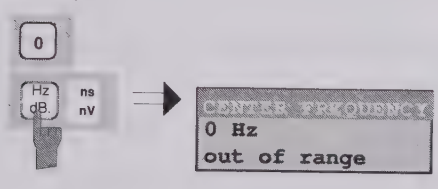

Correcting the entry

Deleting an entry

➢ Position the cursor beside the digit which is to be deleted using the cursor keys ⇦ or ⇨ .

➢ Press the *BACK* key. The entry left to the cursor is deleted.

➢ Enter new numbers. The number is inserted to the left of the cursor, the other numbers are shifted right.

Restoring the original value

➢ Press the *BACK* key

For numerous parameters, the data administration of the instrument stores the previously valid parameter value in addition to the current value. The BACK key can be used to toggle between these two values. This applies for terminated entries as long as the data entry window is displayed.

Aborting the entry

➢ Press *ESC* key

The original parameter value is restored. The new entry is deleted.

➢ Press *ESC* key again

The entry window is closed, the original value remains active.

or

➢ Press any key or any softkey (even the softkey which has opened the entry window).

The entry is aborted and the entry window is closed. The original value remains active.

Entry of Alphanumeric Parameter

A help-line editor or an external keyboard (optional) are provided for the entry of alphanumeric instrument parameters.
The roll-key and the exponent key have no function with alphanumeric entry. All unit keys assume the function of an ENTER key.

The entry is always made in a data entry window which is displayed automatically upon selection of the parameter. The editing line comprises 60 characters. Up to 256 characters may be entered. If a text exceeds 60 characters the contents is shifted automatically 20 characters left or right when the left or right margin of the editing line is touched by the cursor.

Editing with External Keyboard

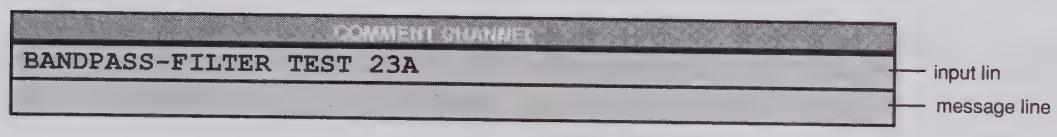

Entry of text

- Select parameter.
  The data entry is active automatically upon calling the data entry window. The cursor is positioned at the beginning of the previous entry.
- Press the required character on the keyboard.
  The character is inserted prior to the cursor.
- Enter further characters

Correcting the entry

- Delete the entry using the *DELETE* key or *BACKSPACE* key.

Terminating the entry

- Press the *ENTER* key of the external keyboard
  The data entry window is closed and the new value is accepted for the instrument.

Aborting the entry

- Press the **ESC** key on the front panel

or

- any softkey.

  The data entry window is closed, the original value is retained.

Editing with Help Line Editor

If the external keyboard is not fitted, the help line editor is called automatically with entry of alphanumeric parameters. The help line editor is an extension of the alphanumeric entry window. It contains the complete alphabet with uppercase and lowercase letters as well as special characters in two lines of 52 characters, each. Individual letters and a series of special characters can be selected in the help line editor and copied into the entry line.

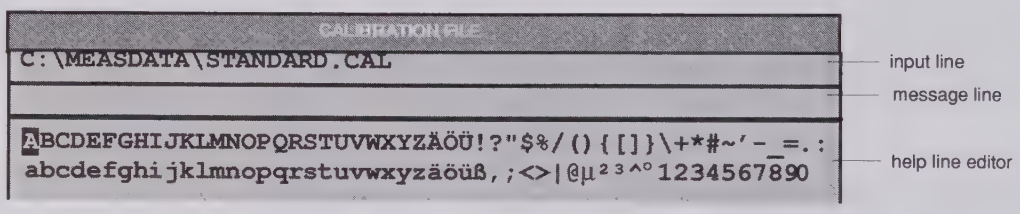

The cursor keys ⇦ or ⇨ toggle between entry in the editing line and selection in the help line editor.

Entry of text

- ➢ Select parameter.
  The data entry is active automatically upon calling the data entry window. The cursor is positioned on the left in the editing line.
- ➢ Position the cursor in the help line editor using the cursor key ⇨.
  The cursor marks the first letter of the editor.
- ➢ Locate the cursor on the character which is to be entered into the editing line using the cursor keys ⇩ or ⇧ or the roll-key.
- ➢ Press the *ENTER* key or the roll-key
  The character is entered in the editing line.

Correcting the entry

- ➢ Locate the cursor in the editing line using the cursor key ⇦.
- ➢ Position the cursor after the character which is to be deleted using the cursor keys ⇩ and ⇧.
- ➢ Press the *BACK* key.
  The entry left to the cursor is deleted.

Terminating the entry

- ➢ Locate the cursor in the editing line using the cursor key ⇨.
- ➢ Press any unit key or the roll-key.
  The data entry window is closed, the new entry is accepted by the instrument.

Aborting the entry

- ➢ Press the *CLR* key.
  The data entry window is closed, the previous entry is retained.

Selection and Setting of Parameters via Tables

The spectrum analyzer uses numerous tables for display and configuration of instrument parameters.

The tables differ considerably in the number of lines, columns and inscriptions. The basic steps of operation for the selection and setting of parameters are, however, the same for all tables. Shown below is the typical entry of parameters into a table.

Note:

Most of the tables are coupled to a softkey menu which provides further functions for editing table entries such as deletion of tables, copying of lines or columns, marking of table elements, restoring default states.

The definition of individual tables and the operation of particular editing functions can be looked up in the description of the corresponding softkey menu.

1. Activating the table

- If the menu has only one table, the latter is activated automatically subsequent to calling this menu in most cases and the marking cursor is positioned to the top field of the left column.
- If the menu contains various tables, the table of interest must be selected using the softkey which is labeled with the title of the table.

2. Selection of the parameter

marking cursor

NAME	COMPATIBLE	LIMIT CHECK	TRACE	MARGIN
GSM22UP	√	off	1	0 dB
√ LP1GHz		on	2	0 dB
√ LP1GHz	√	off	1	0 dB
MIL461A		off	2	-10 dB

Selection of the parameter (or the setting) is made using the marking cursor.

➢ Press the cursor keys to move to the wanted field.

or

➢ Rotate the roll-key until the wanted field is marked. The cursor keys are used to specify the direction of the roll-key movement (horizontal or vertical)

When shifting the cursor, elements may be skipped which can not be edited. Table elements, which can not be selected are indicated by a different color.

➢ Press the *ENTER* key or the roll-key.
The parameter/the setting has been selected.

The selected parameter can be edited the way described below:

3. Editing the marked parameter

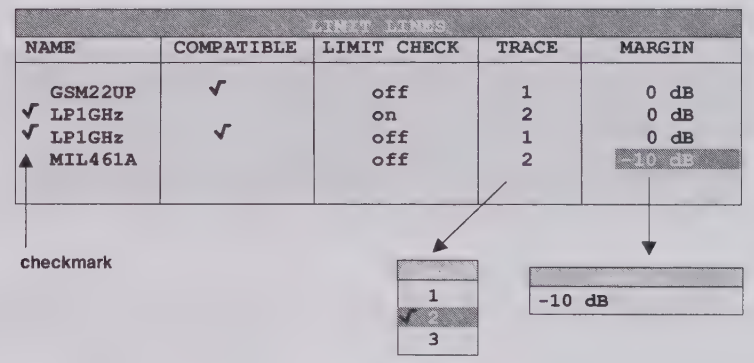

a) Toggling between two states

If an element of a table can be switched on and off only, the unit keys are used to toggle between these two states.

➢ Press one of the unit keys.
The table element is switched on and provided with a checkmark. (√).

➢ Press one of the unit keys once more.
The table element is switched off.

or

➢ Press one of the unit keys.
The table element is switched on, "on" is displayed.

➢ Press one of the unit keys once more.
The table element is switched off, "off" is displayed

b) Opening a data entry window

If a table entry consists of an (alpha-) numeric value, selection of the latter causes the corresponding entry window to be opened.

Note: *For numeric or alphanumeric instrument parameters, the editing operation may be started by entering any number or letter on the front panel or on the external keyboard. In this case, the data entry window is opened automatically.*

c) Opening a selection table

If a table entry may have various states (e.g., colors from a color pallet, fixed filter bandwidths, etc.), a table indicating all possible states is displayed with selection. The current state is and marked by a checkmark and by the cursor.

- ➢ Set the cursor to the desired setting.
- ➢ Press one of the unit keys.
  The setting is switched on and marked (√). The selection table closes and the value is transferred to the original table. The cursor is positioned automatically on the next table element.

Abortion of entry

➢ Press the *ESC* key.

The current entry/selection is aborted and the original setting is restored.

Scrolling

Some tables contain more entries than can be displayed on one screen page. In this case, a **scrollbar** is displayed at the right margin of the table, whose slider shows the current position in the text.

➢ Actuate the *PAGE UP* or *PAGE DOWN* softkeys.

The table is paged forward or back by one page.

➢ Press cursor key ⊡ or ⊡.

The table is scrolled up or down by one line.

Menu Overview

The following section gives a graphical overview of the FSP menus. Side menus are marked by an arrow directed to the left/right, submenus by an arrow showing upwards.
The menus appear in the order corresponding to the arrangement of keys on the front panel. The available hotkeys and the LOCAL menu appearing during the remote control of the instrument are also displayed.

The functions of menus are described in detail in Chapter 4. The IEC/IEEE-bus command associated with each softkey is indicated. In addition, the softkey list at the of Chapter 6 gives the assignment of IEC/IEEE-bus commands to softkeys.

FREQUENCY Key

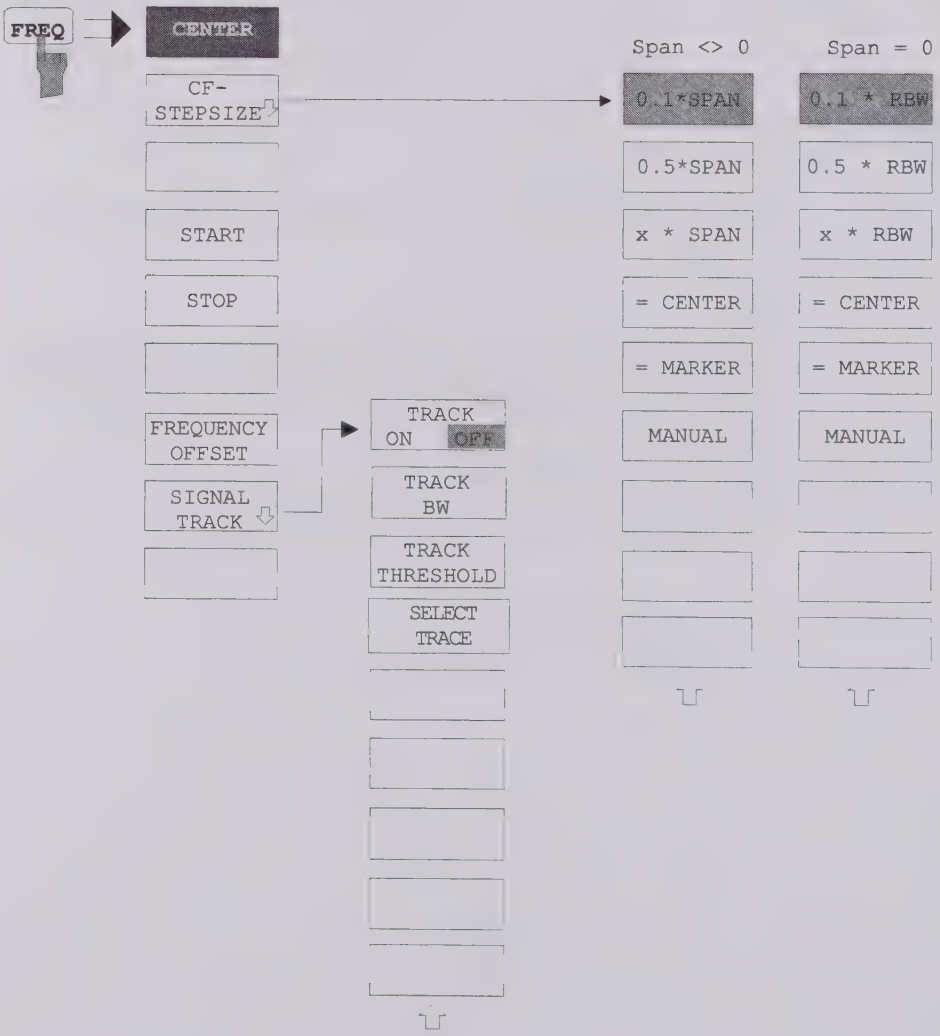

SPAN Key

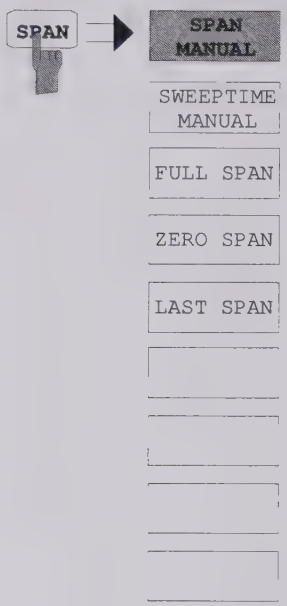
SPAN
SPAN MANUAL
SWEEPTIME MANUAL
FULL SPAN
ZERO SPAN
LAST SPAN

AMPT Key

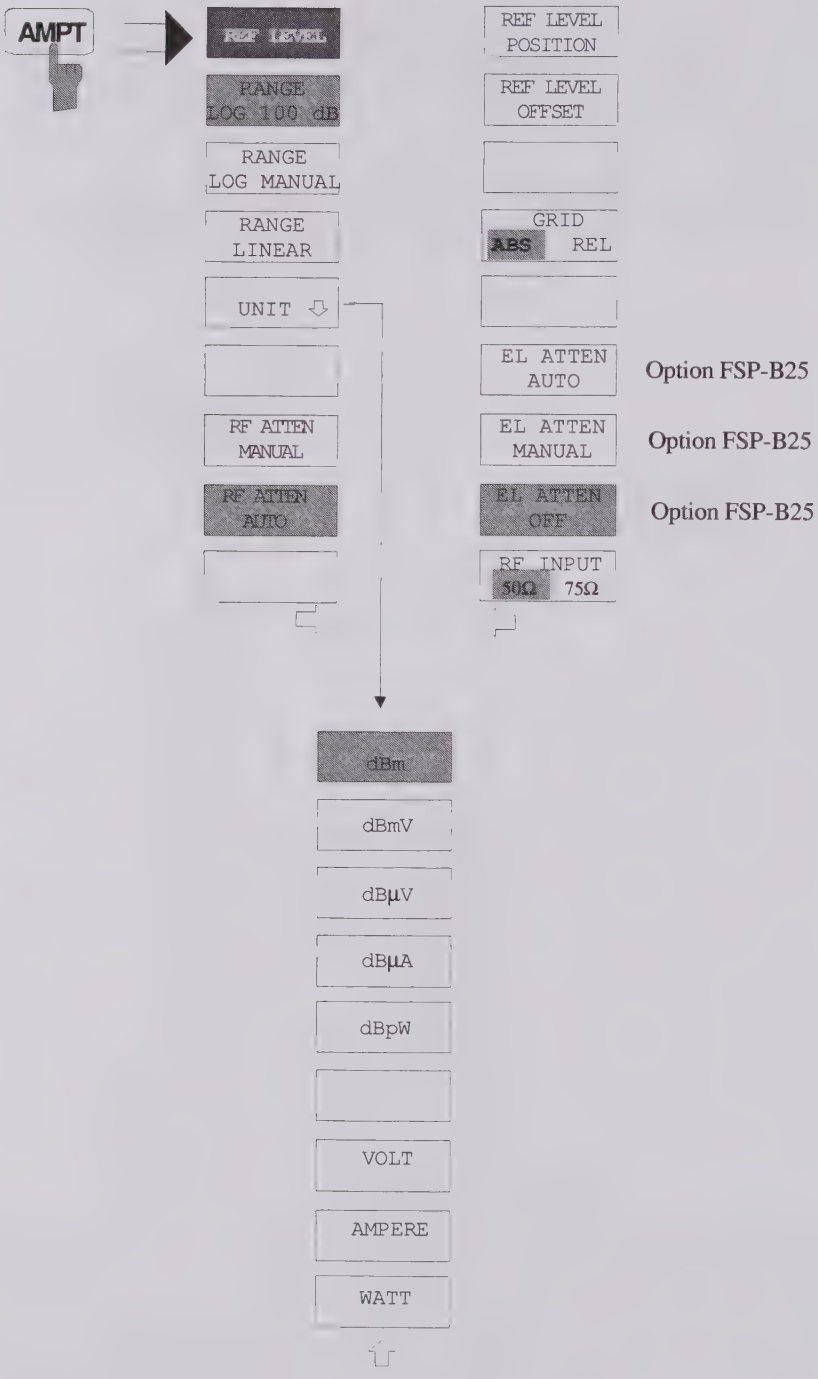
AMPT
REF LEVEL
RANGE
LOG 100 dB
RANGE
LOG MANUAL
RANGE
LINEAR
UNIT
RF ATTEN
MANUAL
RF ATTEN
AUTO
REF LEVEL
POSITION
REF LEVEL
OFFSET
GRID
ABS REL
EL ATTEN
AUTO
Option FSP-B25
EL ATTEN
MANUAL
Option FSP-B25
EL ATTEN
OFF
Option FSP-B25
RF INPUT
50Ω 75Ω
dBm
dBmV
dBµV
dBµA
dBpW
VOLT
AMPERE
WATT

MKR Key

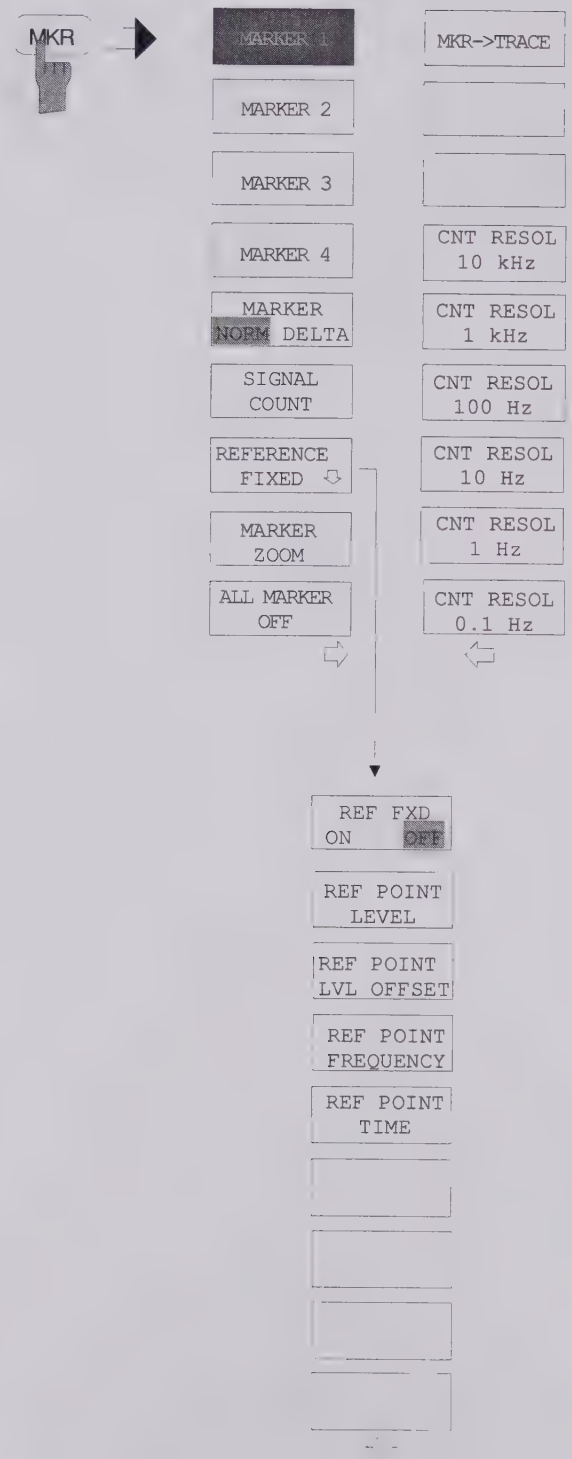
MKR
MARKER 1
MARKER 2
MARKER 3
MARKER 4
MARKER
NORM DELTA
SIGNAL
COUNT
REFERENCE
FIXED
MARKER
ZOOM
ALL MARKER
OFF
MKR->TRACE
CNT RESOL
10 kHz
CNT RESOL
1 kHz
CNT RESOL
100 Hz
CNT RESOL
10 Hz
CNT RESOL
1 Hz
CNT RESOL
0.1 Hz
REF FXD
ON OFF
REF POINT
LEVEL
REF POINT
LVL OFFSET
REF POINT
FREQUENCY
REF POINT
TIME

MKR-> Key

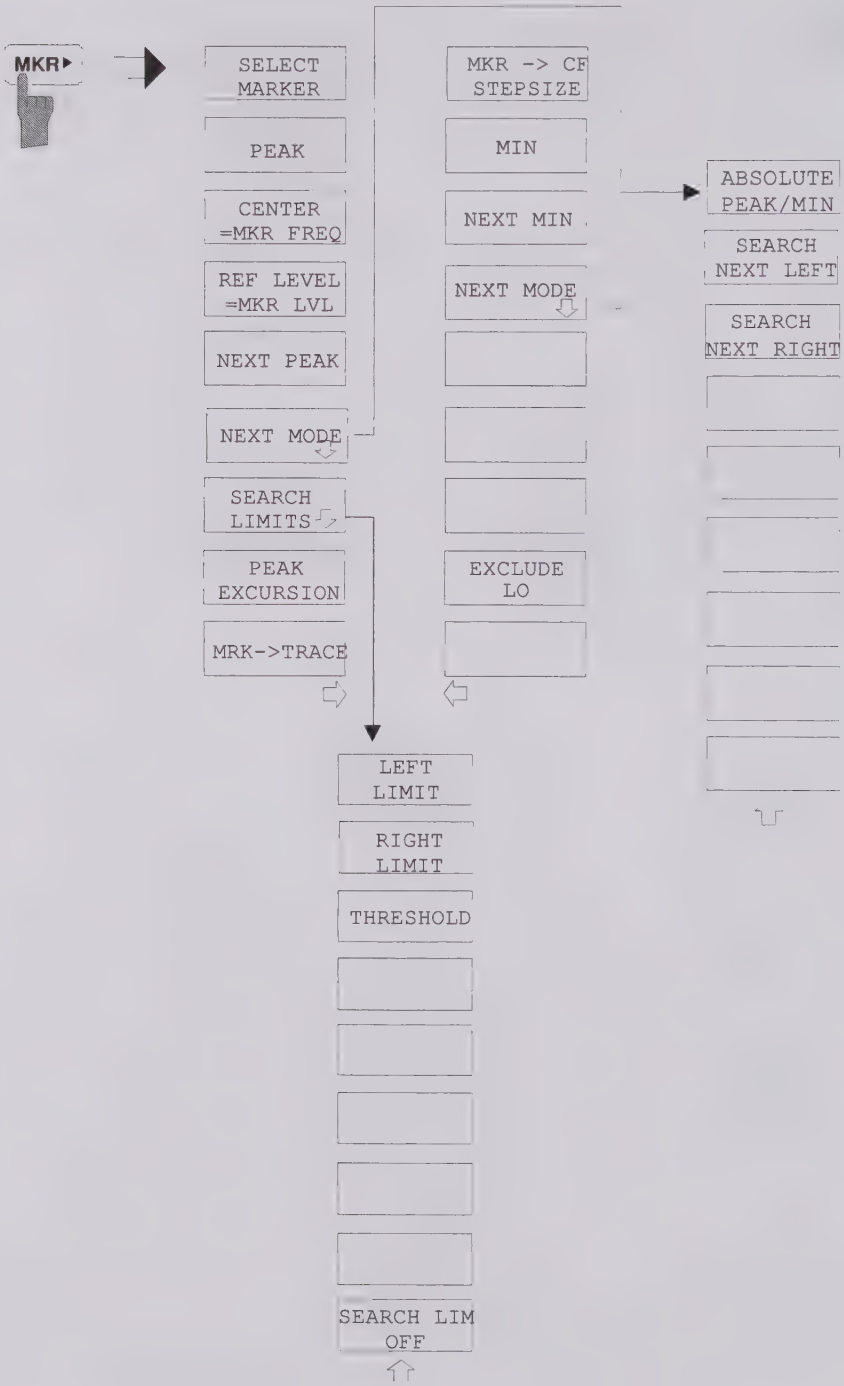
MKR
SELECT MARKER
PEAK
CENTER =MKR FREQ
REF LEVEL =MKR LVL
NEXT PEAK
NEXT MODE
SEARCH LIMITS
PEAK EXCURSION
MRK->TRACE
MKR -> CF STEPSIZE
MIN
NEXT MIN
NEXT MODE
EXCLUDE LO
ABSOLUTE PEAK/MIN
SEARCH NEXT LEFT
SEARCH NEXT RIGHT
LEFT LIMIT
RIGHT LIMIT
THRESHOLD
SEARCH LIM OFF

MKR FCTN Key

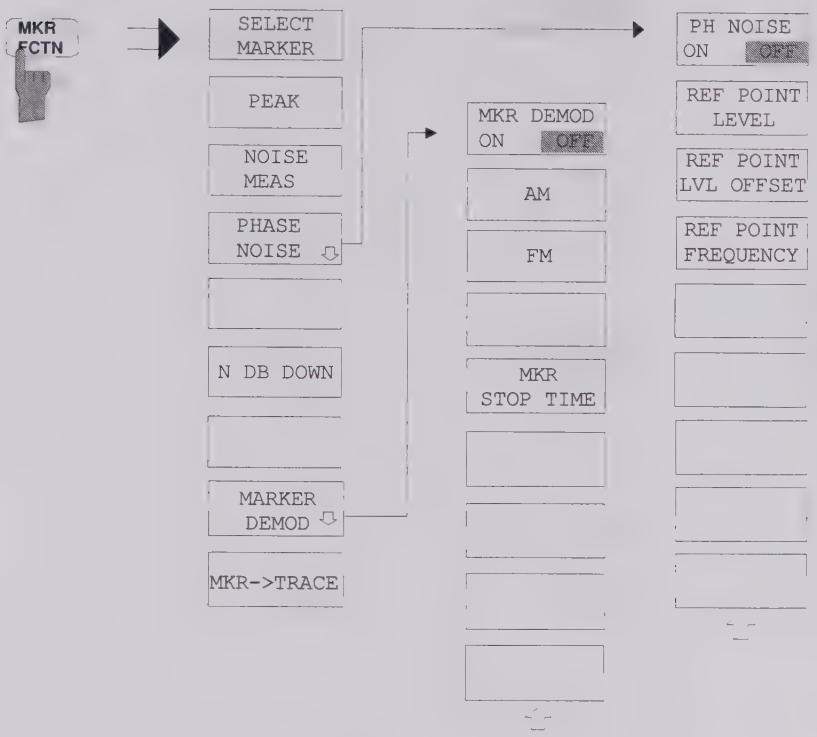
MKR FCTN
SELECT MARKER
PEAK
NOISE MEAS
PHASE NOISE
N DB DOWN
MARKER DEMOD
MKR->TRACE
MKR DEMOD ON OFF
AM
FM
MKR STOP TIME
PH NOISE ON OFF
REF POINT LEVEL
REF POINT LVL OFFSET
REF POINT FREQUENCY

BW Key

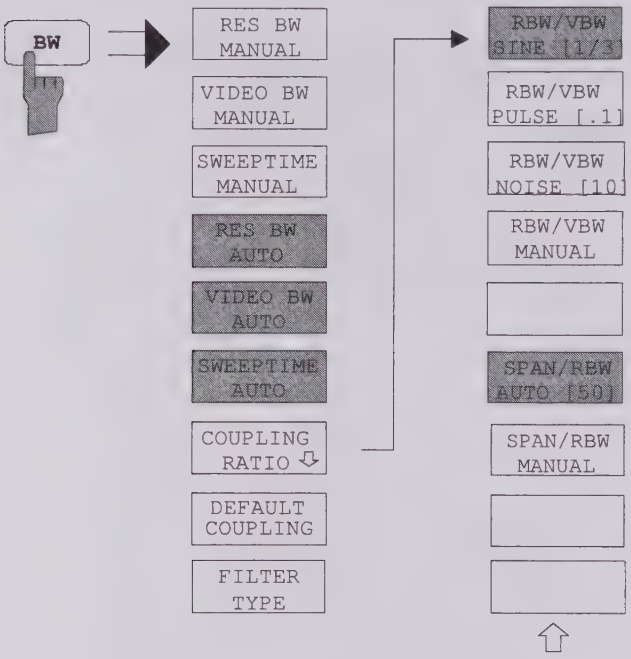
BW
RES BW MANUAL
VIDEO BW MANUAL
SWEEPTIME MANUAL
RES BW AUTO
VIDEO BW AUTO
SWEEPTIME AUTO
COUPLING RATIO
DEFAULT COUPLING
FILTER TYPE
RBW/VBW SINE [1/3]
RBW/VBW PULSE [.1]
RBW/VBW NOISE [10]
RBW/VBW MANUAL
SPAN/RBW AUTO [50]
SPAN/RBW MANUAL

SWEEP Key

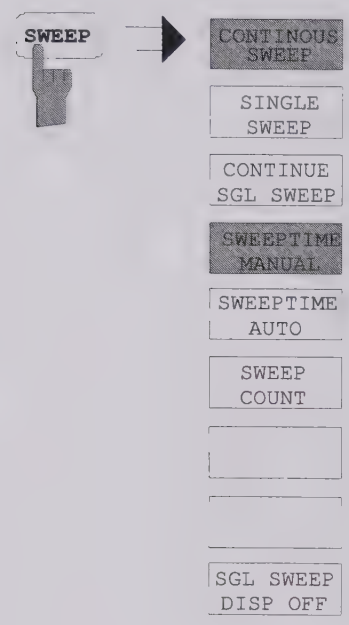
SWEEP
CONTINOUS SWEEP
SINGLE SWEEP
CONTINUE SGL SWEEP
SWEEPTIME MANUAL
SWEEPTIME AUTO
SWEEP COUNT
SGL SWEEP DISP OFF

MEAS Key

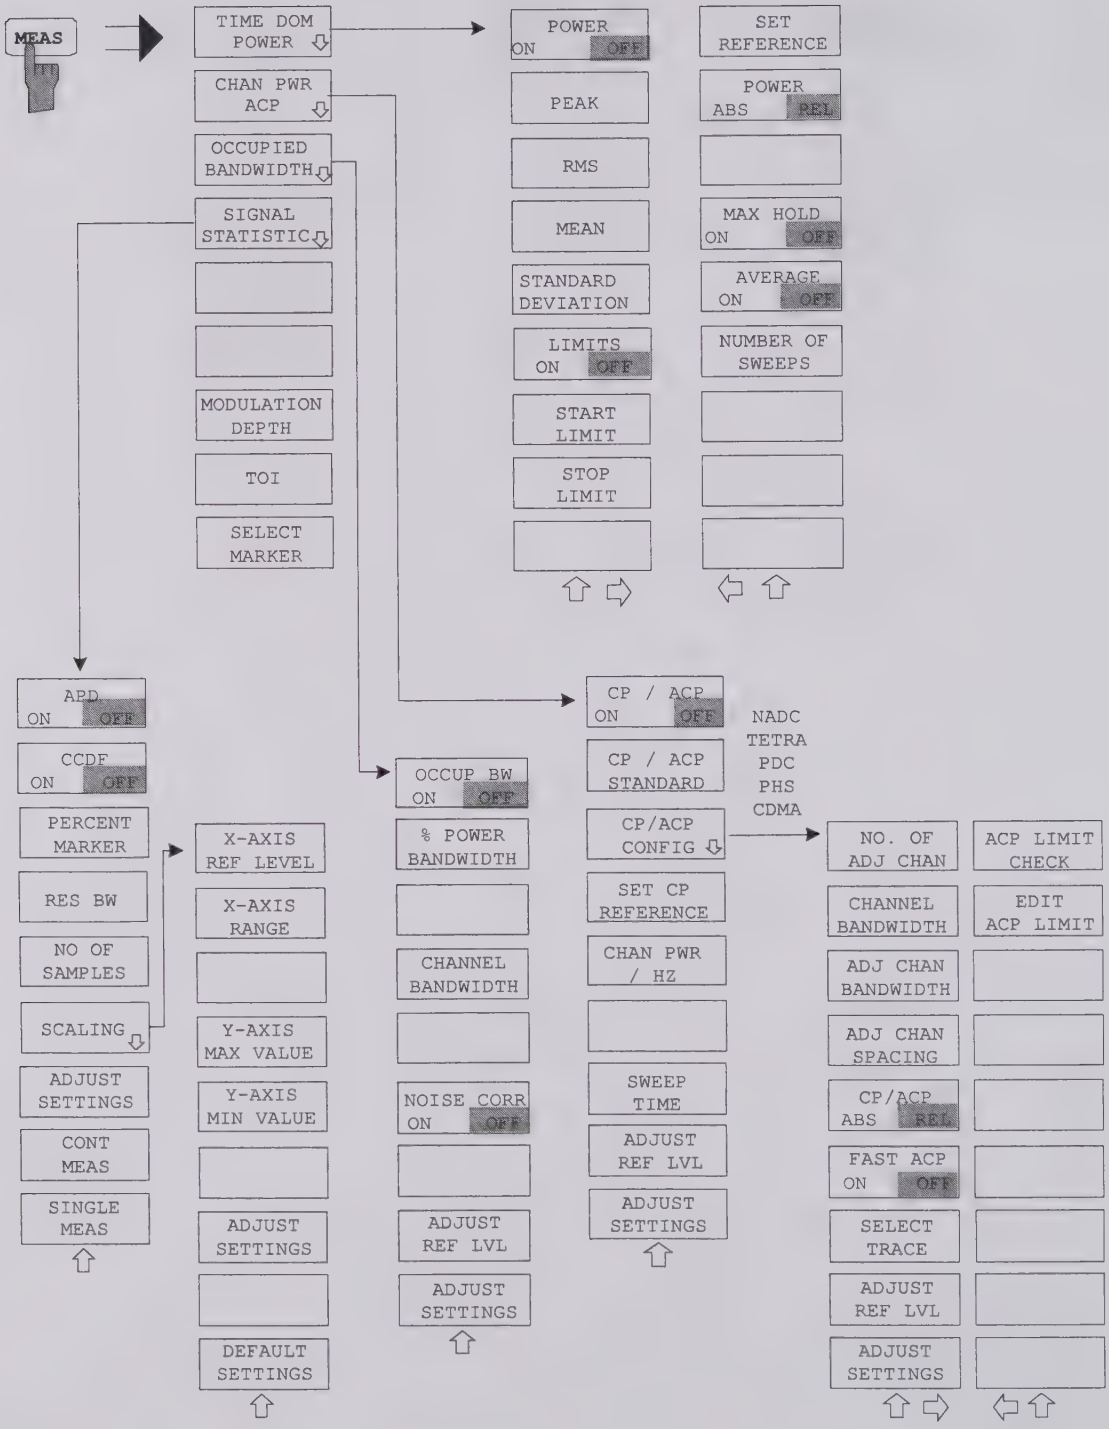
MEAS
TIME DOM POWER
CHAN PWR ACP
OCCUPIED BANDWIDTH
SIGNAL STATISTIC
MODULATION DEPTH
TOI
SELECT MARKER
POWER ON OFF
PEAK
RMS
MEAN
STANDARD DEVIATION
LIMITS ON OFF
START LIMIT
STOP LIMIT
SET REFERENCE
POWER ABS REL
MAX HOLD ON OFF
AVERAGE ON OFF
NUMBER OF SWEEPS
APD ON OFF
CCDF ON OFF
PERCENT MARKER
RES BW
NO OF SAMPLES
SCALING
ADJUST SETTINGS
CONT MEAS
SINGLE MEAS
X-AXIS REF LEVEL
X-AXIS RANGE
Y-AXIS MAX VALUE
Y-AXIS MIN VALUE
ADJUST SETTINGS
DEFAULT SETTINGS
OCCUP BW ON OFF
% POWER BANDWIDTH
CHANNEL BANDWIDTH
NOISE CORR ON OFF
ADJUST REF LVL
ADJUST SETTINGS
CP / ACP ON OFF
CP / ACP STANDARD
CP/ACP CONFIG
SET CP REFERENCE
CHAN PWR / HZ
SWEEP TIME
ADJUST REF LVL
ADJUST SETTINGS
NADC
TETRA
PDC
PHS
CDMA
NO. OF ADJ CHAN
CHANNEL BANDWIDTH
ADJ CHAN BANDWIDTH
ADJ CHAN SPACING
CP/ACP ABS REL
FAST ACP ON OFF
SELECT TRACE
ADJUST REF LVL
ADJUST SETTINGS
ACP LIMIT CHECK
EDIT ACP LIMIT

TRIG Key

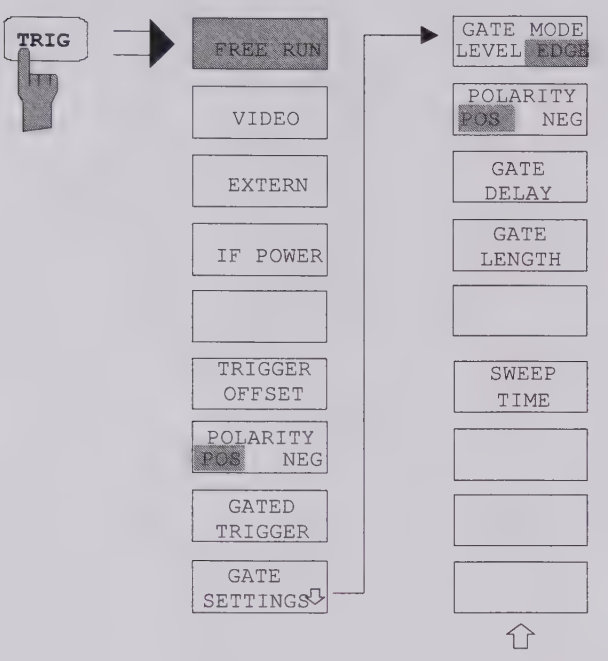
TRIG
FREE RUN
VIDEO
EXTERN
IF POWER
TRIGGER OFFSET
POLARITY POS NEG
GATED TRIGGER
GATE SETTINGS
GATE MODE LEVEL EDGE
POLARITY POS NEG
GATE DELAY
GATE LENGTH
SWEEP TIME

TRACE Key

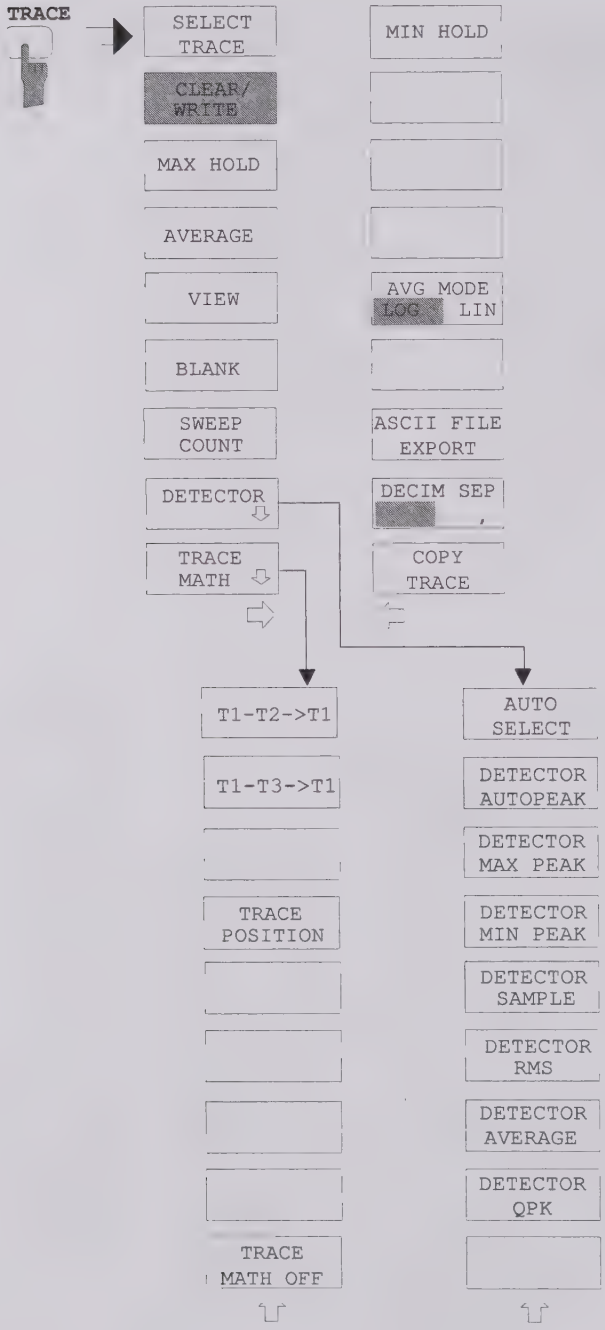
TRACE
SELECT TRACE
CLEAR/ WRITE
MAX HOLD
AVERAGE
VIEW
BLANK
SWEEP COUNT
DETECTOR
TRACE MATH
MIN HOLD
AVG MODE LOG LIN
ASCII FILE EXPORT
DECIM SEP
COPY TRACE
T1-T2->T1
T1-T3->T1
TRACE POSITION
TRACE MATH OFF
AUTO SELECT
DETECTOR AUTOPEAK
DETECTOR MAX PEAK
DETECTOR MIN PEAK
DETECTOR SAMPLE
DETECTOR RMS
DETECTOR AVERAGE
DETECTOR QPK

LINES Key

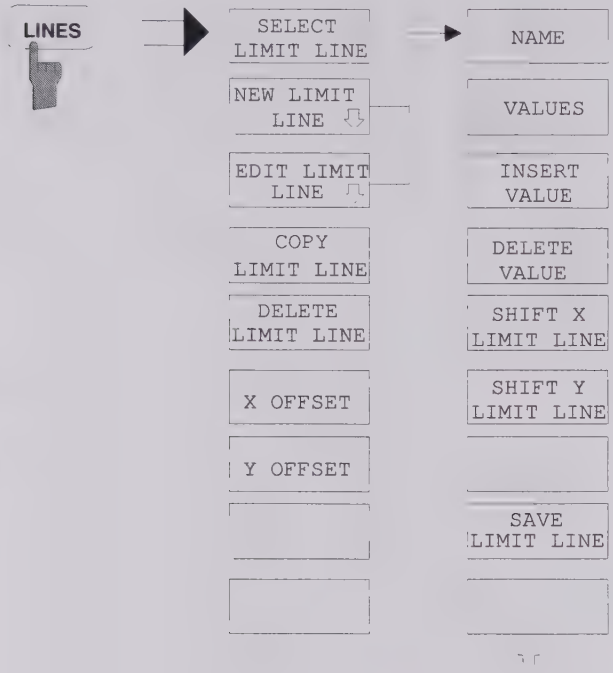
LINES
SELECT LIMIT LINE
NEW LIMIT LINE
EDIT LIMIT LINE
COPY LIMIT LINE
DELETE LIMIT LINE
X OFFSET
Y OFFSET
NAME
VALUES
INSERT VALUE
DELETE VALUE
SHIFT X LIMIT LINE
SHIFT Y LIMIT LINE
SAVE LIMIT LINE

DISP Key

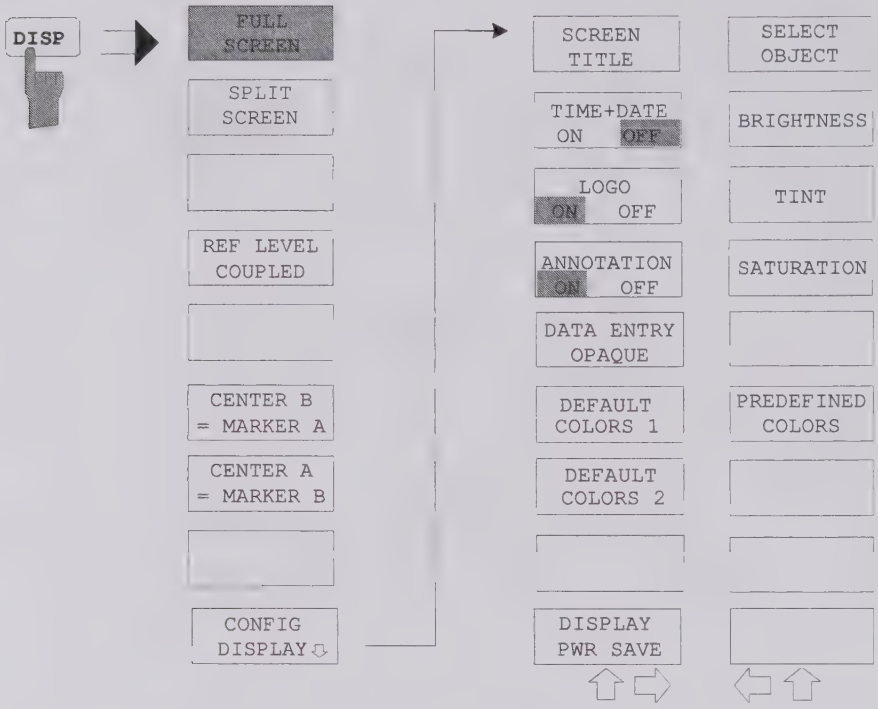
DISP
FULL SCREEN
SPLIT SCREEN
REF LEVEL COUPLED
CENTER B = MARKER A
CENTER A = MARKER B
CONFIG DISPLAY
SCREEN TITLE
TIME+DATE ON OFF
LOGO ON OFF
ANNOTATION ON OFF
DATA ENTRY OPAQUE
DEFAULT COLORS 1
DEFAULT COLORS 2
DISPLAY PWR SAVE
SELECT OBJECT
BRIGHTNESS
TINT
SATURATION
PREDEFINED COLORS

FILE Key

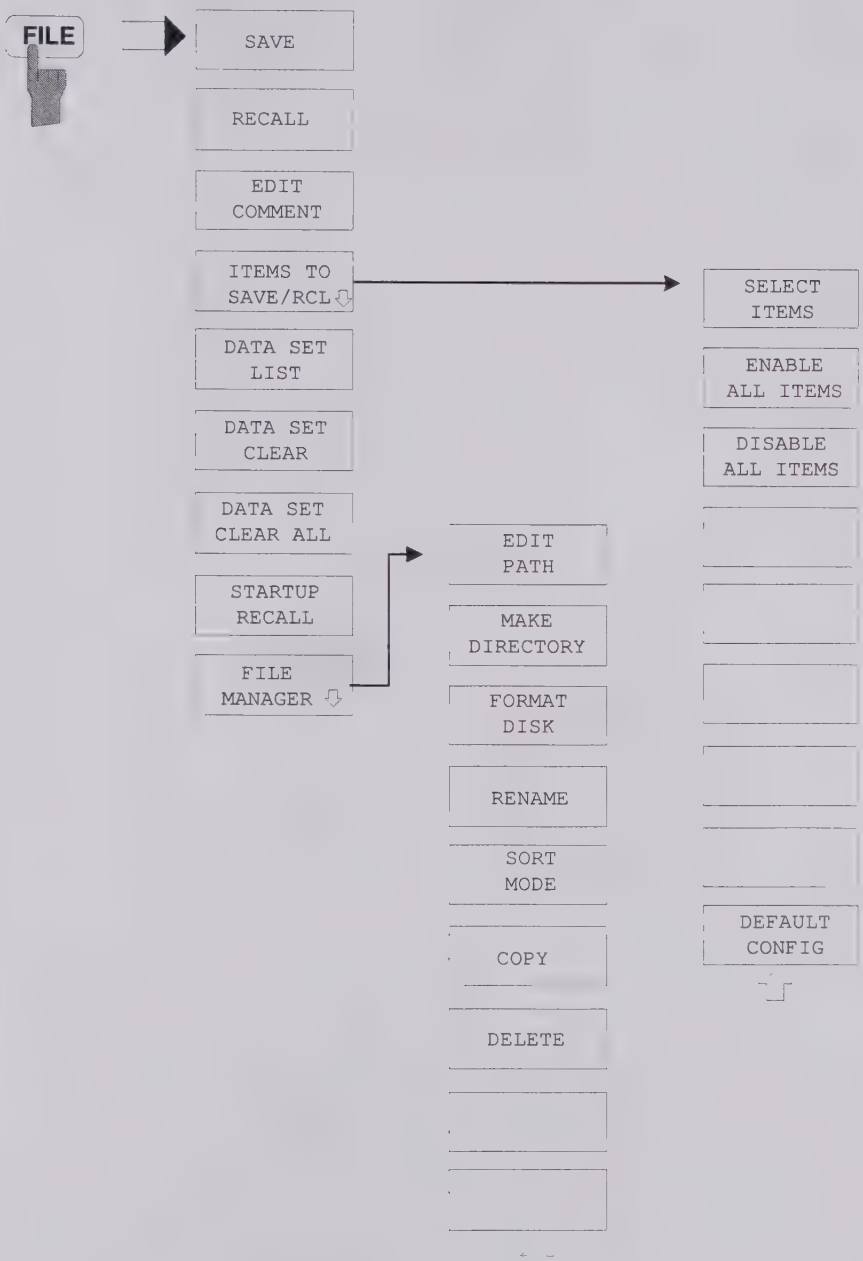
FILE
SAVE
RECALL
EDIT COMMENT
ITEMS TO SAVE/RCL
DATA SET LIST
DATA SET CLEAR
DATA SET CLEAR ALL
STARTUP RECALL
FILE MANAGER
SELECT ITEMS
ENABLE ALL ITEMS
DISABLE ALL ITEMS
EDIT PATH
MAKE DIRECTORY
FORMAT DISK
RENAME
SORT MODE
COPY
DELETE
DEFAULT CONFIG

CAL Key

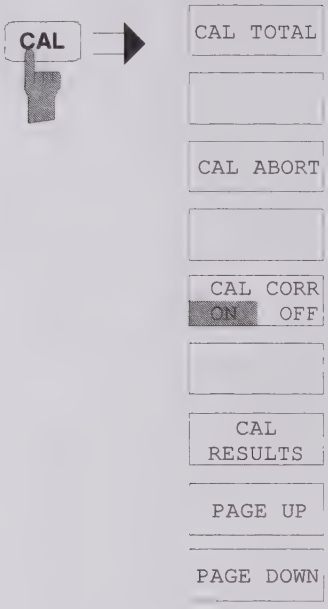
CAL
CAL TOTAL
CAL ABORT
CAL CORR
ON OFF
CAL
RESULTS
PAGE UP
PAGE DOWN

SETUP Key

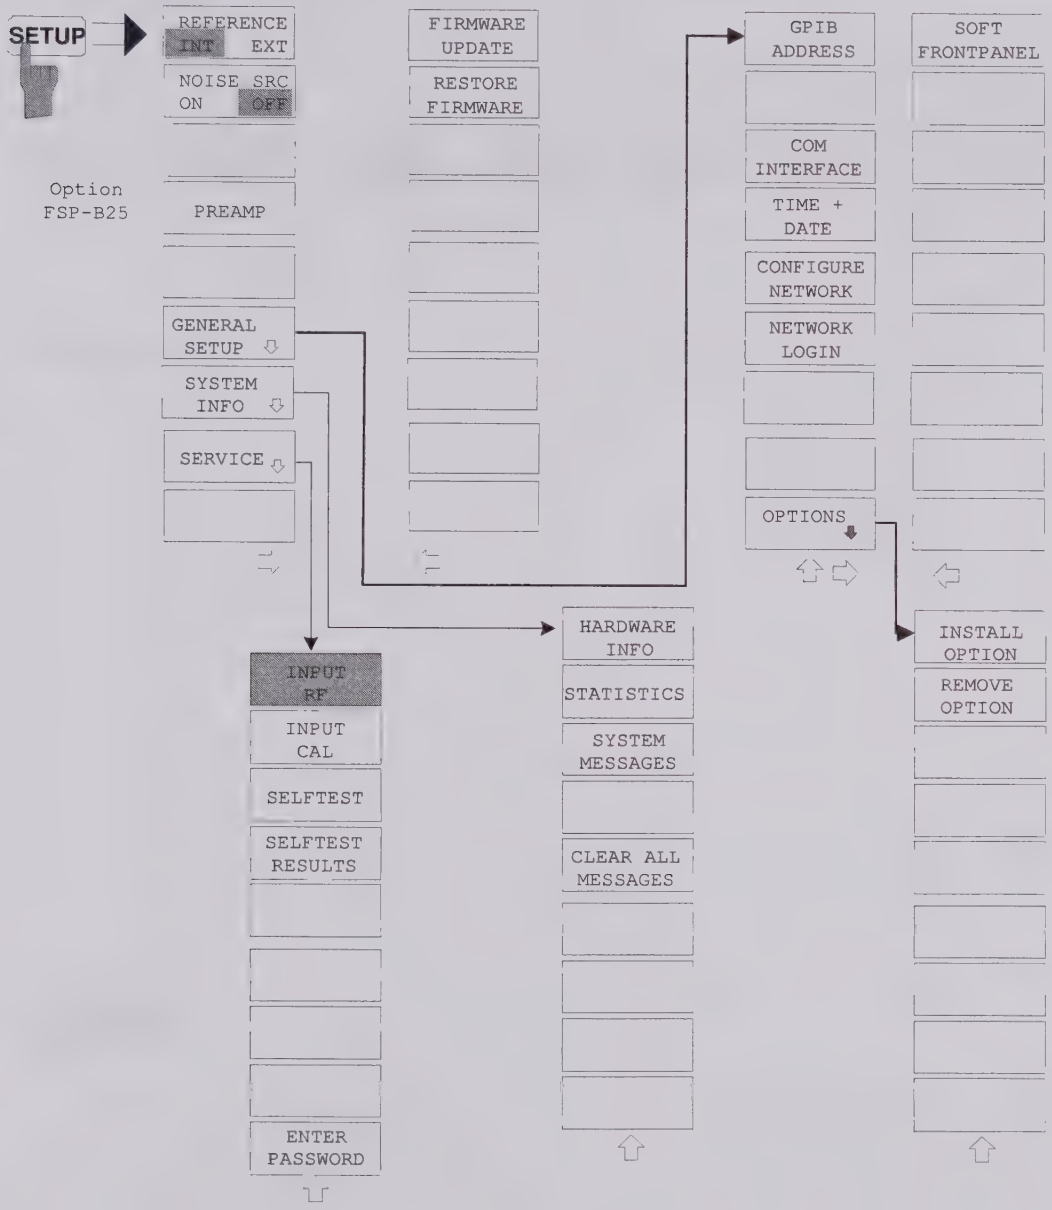
SETUP
REFERENCE INT EXT
NOISE SRC ON OFF
Option FSP-B25
PREAMP
GENERAL SETUP
SYSTEM INFO
SERVICE
FIRMWARE UPDATE
RESTORE FIRMWARE
GPIB ADDRESS
COM INTERFACE
TIME + DATE
CONFIGURE NETWORK
NETWORK LOGIN
OPTIONS
SOFT FRONTPANEL
INSTALL OPTION
REMOVE OPTION
INPUT RF
INPUT CAL
SELFTEST
SELFTEST RESULTS
ENTER PASSWORD
HARDWARE INFO
STATISTICS
SYSTEM MESSAGES
CLEAR ALL MESSAGES

HCOPY Key

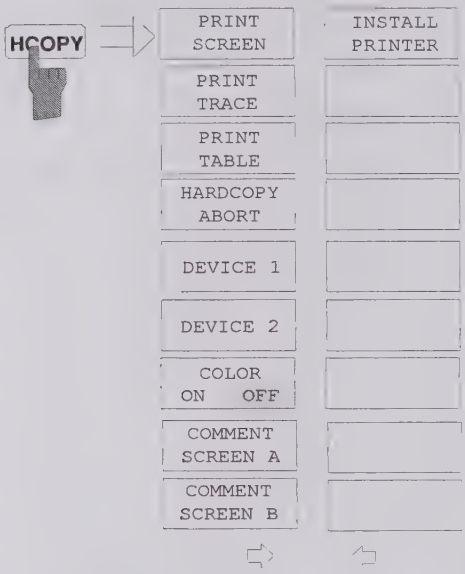
HCOPY
PRINT SCREEN
INSTALL PRINTER
PRINT TRACE
PRINT TABLE
HARDCOPY ABORT
DEVICE 1
DEVICE 2
COLOR ON OFF
COMMENT SCREEN A
COMMENT SCREEN B

Hotkey Menu

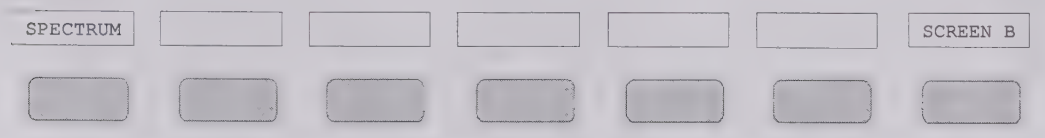

LOCAL Menu

Menu Overview Network Mode

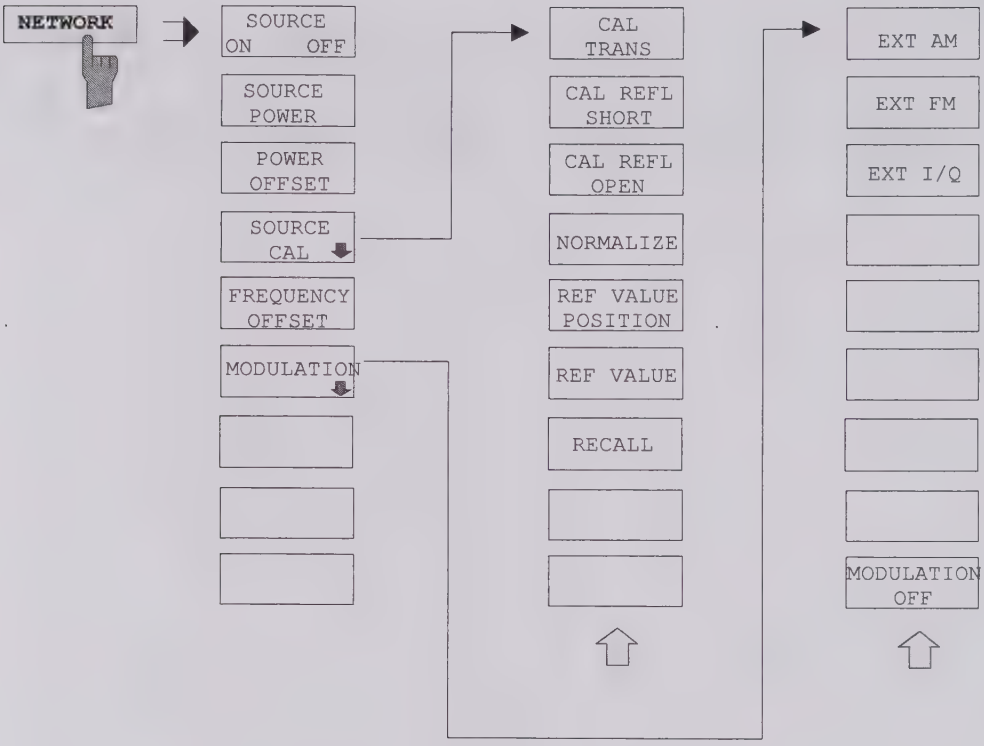

Menu Overview Option Ext. Generator Control

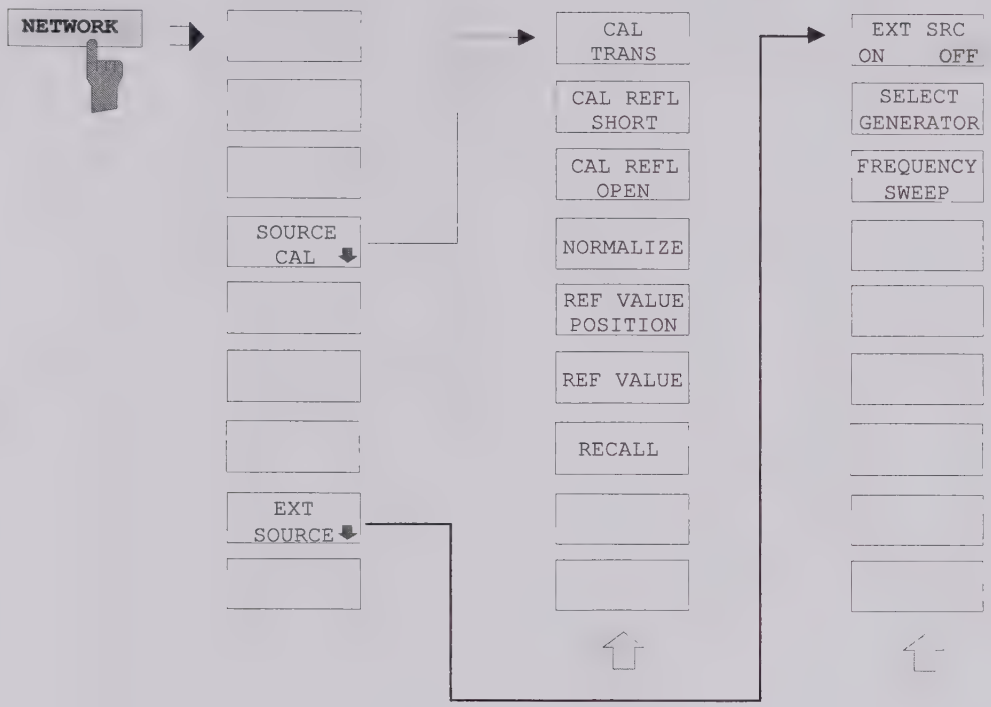

Contents - Chapter 4 "Instrument Functions"

4 Instrument Functions 4.1

FSP Initial Configuration – *PRESET* Key 4.2

Mode Selection – *HOTKEY* Bar 4.3

Return to manual control – *LOCAL* Menu 4.4

Spectrum Analyzer Mode 4.5

Frequency and Span Selection – *FREQ* Key 4.6

Setting the Frequency Span – *SPAN Key* 4.11

Level Display Setting and RF Input Configuration – *AMPT Key* 4.13

Electronic Attenuator 4.16

Setting the Bandwidths and Sweep Time – *BW* Key 4.18

List of available channel filters 4.26

Sweep Settings – *SWEEP* Key 4.27

Triggering the Sweep– *TRIG* Key 4.29

Selection and Setting of Traces –*TRACE* Key 4.36

Selection of Trace Function 4.36

Selection of Detector 4.44

Mathematical Functions for Traces 4.49

Recording the Correction Data of FSP – *CAL* Key 4.50

Markers and Delta Markers – *MKR* Key 4.52

Frequency Measurement with the Frequency Counter 4.54

Marker Functions – *MKR FCTN* Key 4.59

Activating the Markers 4.60

Measurement of noise density 4.60

Phase Noise Measurement 4.62

Measurement of the Filter or Signal Bandwidth 4.64

AF Demodulation 4.65

Selecting the Trace 4.66

Change of Settings via Markers – *MKR* ⇒ Key 4.67

Power Measurements – Hardkey *MEAS* 4.75

Power Measurement in Time Domain 4.76

Channel and Adjacent-Channel Power Measurements 4.81

Setting the Channel Configuration 4.88

Measurement of Signal Amplitude Statistics 4.99

Measurement of the AM Modulation Depth 4.105

Measurement of the Third Order Intercept (TOI) 4.106

Setup of Limit Lines – *LINES* Key 4.109

Limit Line Selection 4.110

Entry and Editing of Limit Lines 4.114

Configuration of Screen Display – *DISP* Key 4.119

Instrument Setup and Interface Configuration – *SETUP* Key 4.125

External Reference Oscillator 4.126

External Noise Source 4.126

RF Preamplifier 4.126

Programming the Interface Configuration and Time Setup 4.127

Selecting the IEC/IEEE-bus address 4.127

Serial Interface Configuration 4.128

Setting Date and Time 4.131
Configuration of network settings (with option FSP-B16 only) 4.132
Emulation of the instrument front panel 4.134
System Information 4.135
Display of Module Data 4.136
Display of Device Statistics 4.137
Display of System Messages 4.138
Service Menu 4.139
General Service Functions 4.139
Selftest 4.140
Hardware Adjustment 4.141
Firmware Update 4.141

Saving and Recalling Data Sets – *FILE* Key 4.142
Saving a Data Set 4.143
Recalling a Data Set: 4.143
FILE Menu 4.144

Measurement Documentation – *HCOPY* Key 4.151
Installation of a local Printer 4.156
Installation of a Network Printer (with option FSP-B16 only) 4.159

Tracking Generator - Option FSP-B9 ..... 4.163
Tracking Generator Settings 4.164
Transmission Measurement 4.166
Calibration of Transmission Measurement 4.166
Normalization 4.168
Reflection Measurement 4.172
Calibration of Reflection Measurement 4.172
Calibration mechanism 4.173
Frequency-Converting Measurements 4.174
External Modulation of the Tracking Generator 4.175

Option External Generator Control - FSP-B10 ..... 4.179
External Generator Settings 4.180
Transmission Measurement 4.181
Calibration of Transmission Measurement 4.181
Normalization: 4.183
Reflection Measurement 4.187
Calibration of Reflection Measurement 4.187
Calibration mechanism 4.188
Frequency-converting Measurements 4.189
Configuration of an External Generator 4.190
List of Generator Types Supported by the FSP 4.192

Option LAN Interface – FSP-B16 ..... 4.195
Connecting the Instrument to the Network 4.195
Installing the Software 4.195
Installation and Configuration of the Driver for the Network Card 4.196
Selection of the Network Protocols 4.198
Selection of the Network Services 4.199
Completion of the Installation 4.199
Examples of Configurations 4.202
Subsequent Changing of the Network Configuration (Computer Name etc.) 4.202
Operating the Instrument on the Network 4.203

Operating the Instrument on the Network 4.205
NOVELL Networks 4.205
MICROSOFT Network 4.205
Defining Users 4.206
Login in the Network 4.207
Using Network Drives 4.207
Printing on a Network Printer 4.209
Remote Data Transfer with TCP/IP Services 4.211
File Transfer via FTP 4.211

RSIB Interface 4.213
Remote Control via RSIB Interface 4.213

RSIB Interface Functions 4.214
Overview of Interface Functions 4.214
Variables ibsta, iberr, ibcntl 4.215
Description of Interface Functions 4.216

Programming via the RSIB Interface 4.221
Visual Basic 4.221
Visual Basic for Applications (Winword and Excel) 4.223
C / C++ 4.225

4 Instrument Functions

All functions of the spectrum analyzer and their application are explained in detail in this chapter. The sequence of the described menu groups depends on the procedure selected for the configuration and start of a measurement:

1. Resetting the instrument - *PRESET* key
2. Setting the mode – hotkey bar and *LOCAL* key
3. Setting the measurement parameters - keys *FREQ*, *SPAN*, *AMPT*, *BW*, *SWEEP*, *TRIG*, *TRACE*, *CAL*
4. Selecting and configuring the measurement function - keys *MKR*, *MKR->*, *MKR FCTN*, *MEAS*, *LINES*

The instrument functions for general settings, printout and data management are described at the end of this chapter – keys *DISP*, *SETUP*, *FILE* and *HCOPY*.

The different softkeys of a menu are described from top to bottom and from the left to the right side menu. The submenus are marked by an indentation or displayed in a separate section. The whole path (key - softkey - ...) is indicated in the line above the menu display.

An overview of the menus is given in chapter 3 which also contains the description of the operating concept.

The IEC/IEEE-bus commands (if any) are indicated for each softkey. For a fast overview a list of softkeys with the associated IEC/IEEE-bus commands is given at the end of Chapter 6.

An index at the end of the handbook serves as further help for the user.

FSP Initial Configuration – *PRESET* Key

Using the *PRESET* key, the FSP can be set to a predefined initial state.

Notes: *The settings are selected in a way that the RF input is always protected against overload, provided that the applied signal levels are in the allowed range for the instrument.*

The initial instrument state set by the PRESET key can be adapted to arbitrary applications using the STARTUP RECALL function. With this function the STARTUP RECALL dataset is loaded upon pressing the PRESET key. For further information refer to section "Saving and Recalling Data Sets".

Pressing the *PRESET* key causes the FSP to enter its initial state according to the following table:

Table 4-1 Initial State of FSP

Parameter	Settings
Mode	Spectrum
Center frequency	1.5 GHz / 3.5 GHz / 6.8 GHz / 15 GHz (FSP3/7/13/30)
Center frequency step size	0.1 * center frequency
Span	3 GHz / 7 GHz / 13.6 GHz / 30 GHz (FSP3/7/13/30)
RF attenuation	auto (10 dB)
Reference level	-20 dBm
Level range	100 dB log
Level unit	dBm
Sweep time	auto
Resolution bandwidth	auto (3 MHz)
Video bandwidth	auto (10 MHz)
FFT filters	off
Span / RBW	50
RBW / VBW	0.33
Sweep	cont
Trigger	free run
Trace 1	clr write
Trace 2/3	blank
Detector	auto peak
Trace math	off
Frequency offset	0 Hz
Reference level offset	0 dB
Reference level position	100 %
Grid	abs
Cal correction	on
Noise source	off
Input	RF
Display	Full screen, active screen A
Tracking Generator (only with option FSP-B9)	off
External Generator 1/2 (only with option FSP-B10)	off
Preamplifier (only with option FSP-B25)	off
El. Attenuator (only with option FSP-B25)	off

Mode Selection – *HOTKEY* Bar

For fast mode selection FSP has seven keys (the so-called *HOTKEY*s) which can be allocated depending on the options installed on the instrument.

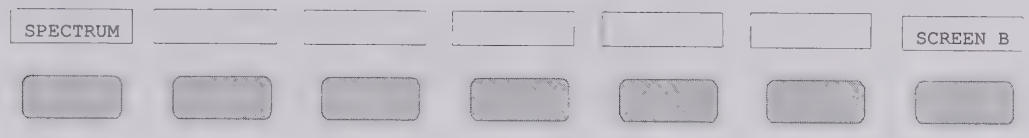

Two keys are reserved for the basic model:



The *SPECTRUM* hotkey sets FSP to spectrum analysis mode.

The spectrum analysis mode is the basic setting of FSP.

IEC/IEEE-bus command: `INST:SEL SAN`

With the *SCREEN A / SCREEN B* hotkey two different settings can be selected on the FSP in the FULL SCREEN mode.

In the SPLIT SCREEN mode the key switches between active diagram A and B.

The key designation indicates the diagram which has been activated by means of the key.

The currently active window is marked by A or B on the right of the diagram.

IEC/IEEE-bus command: `DISP:WIND<1|2>:SEL`

The meaning of the other keys is described in the operating manuals of the various options.

Return to Manual Control – *LOCAL* Menu

The menu LOCAL is displayed on switching the instrument to remote control mode.

At the same time, the *HOTKEY* bar is blanked out and all keys are disabled except the *PRESET* key. The diagram, traces and display fields are then blanked out (they can be activated using the remote control command `SYSTem:DISPlay:UPDate ON`).

The menu contains only one softkey, the *LOCAL* key. The *LOCAL* key switches the instrument from remote to manual control, with the assumption that the remote controller has not previously set the LOCAL LOCKOUT function.

A change in the control mode consists of:

- **Enabling the Front Panel Keys**
  Returning to manual mode enables all inactive keys and turns on the hotkey menu. The soft key menu which is displayed is the main menu of the current mode.

  Inserting the measurement diagrams
  The blanked diagrams, traces and display fields are inserted.

- **Generating the message OPERATION COMPLETE**
  If, at the time of pressing the *LOCAL* softkey, the synchronisation mechanism via *OPC, *OPC? or *WAI is active, the currently running measurement procedure is aborted and synchronisation is achieved by setting the corresponding bits in the registers of the status reporting system.

- **Setting Bit 6 (User Request) of the Event Status Register**
  With a corresponding configuration of the status reporting system, this bit immediately causes the generation of a service request (*SRQ*) which is used to inform the control software that the user wishes to return to front-panel control. This information can be used, e.g., to interrupt the control program so that the user can make necessary manual corrections to instrument settings. This bit is set each time the *LOCAL* softkey is pressed.

Note: *If the LOCAL LOCKOUT function is active in the remote control mode, the front-panel PRESET key is also disabled. The LOCAL LOCKOUT state is left as soon as the process controller de-activates the REN line or the IEC/IEEE-bus cable is disconnected from the instrument.*

Spectrum Analyzer Mode

The analyzer mode is activated by pressing hotkey *SPECTRUM* (see also Section 'Mode Selection')

The *SPECTRUM* hotkey selects the *ANALYZER* mode.

This mode is the default setting of the FSP.

The functions provided correspond to those of a conventional spectrum analyzer. The analyzer measures the frequency spectrum of the test signal over the selected frequency range with the selected resolution and sweep time, or, for a fixed frequency, displays the waveform of the video signal.

Note: *If two displays (screen A and screen B) are opened after switch-on of signal analysis, the analyzer mode is only set for the display activated for entry (marked at the top right corner of diagram). For the other display, the previous settings remain valid.*
Data acquisition and display of measured values is sequential: first in the upper and then in the lower display.

Frequency and Span Selection – *FREQ* Key

The *FREQ* key is used to specify the frequency axis of the active display window. The frequency axis can be defined either by the start and stop frequency or by the center frequency and the span (*SPAN* key). With two windows (*SPLIT SCREEN)* displayed at the same time, the input data always refer to the window selected in the *SYSTEM-DISPLAY* menu.
After pressing one of the *CENTER*, *START* or *STOP* softkeys, the value of the corresponding parameter can be defined in an input window.

FREQ menu:

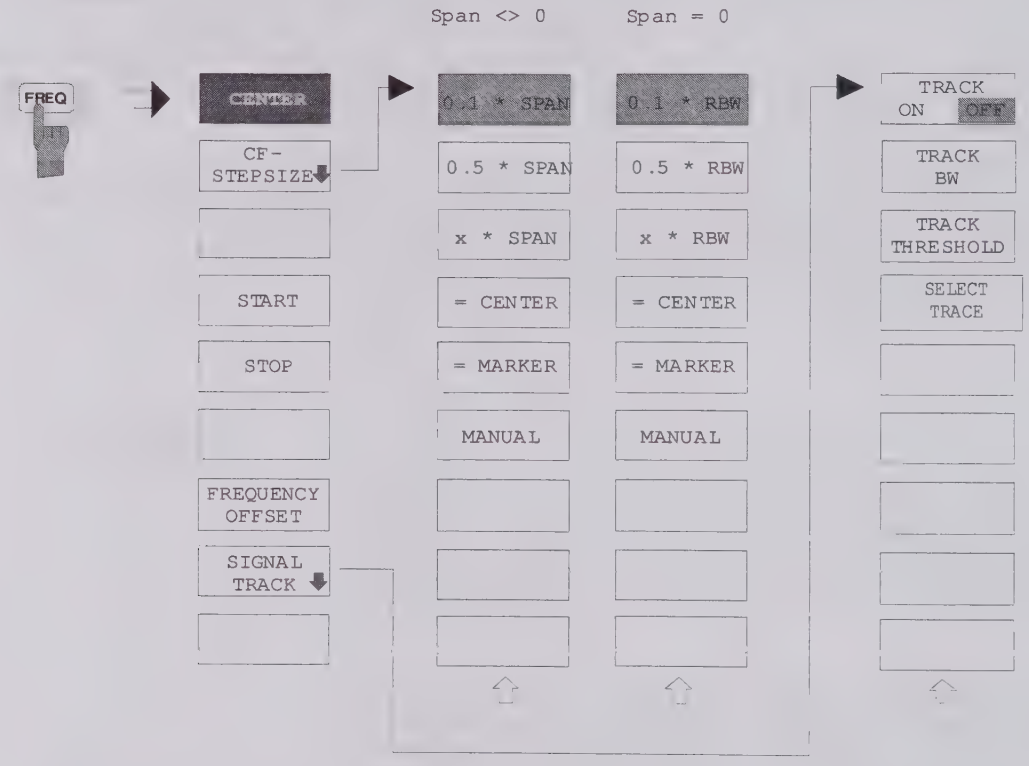



The *CENTER* softkey opens the window for manually entering the center frequency.

The allowed range of values for the center frequency is:

for the frequency domain (span >0):

$$\text{minspan} / 2 \leq f_{center} \leq f_{max} - \text{minspan} / 2$$

and for the time domain (span = 0):

$$0\ \text{Hz} \leq f_{center} \leq f_{max}$$

f_{center}	center frequency
minspan	smallest selectable span > 0 Hz (10 Hz)
f_{max}	max. frequency

IEC/IEEE-bus command: `FREQ:CENT 100MHz`

The CF *STEPSIZE* softkey opens a submenu for setting the step size of the center frequency. The step size can be coupled to the span (frequency domain) or the resolution bandwidth (time domain) or it can be manually set to a fixed value. The softkeys are mutually exclusive selection keys.

The softkeys are presented according to the selected domain (frequency or time).

Softkeys in frequency domain:

The *0.1 * SPAN* softkey sets the step size for the center frequency entry to 10% of the span.

IEC/IEEE-bus command:

```
FREQ:CENT:STEP:LINK SPAN
FREQ:CENT:STEP:LINK:FACT 10PCT
```



The *0.5 * SPAN* softkey sets the step size for the center frequency entry to 50% of the span.

IEC/IEEE-bus command:

```
FREQ:CENT:STEP:LINK SPAN
FREQ:CENT:STEP:LINK:FACT 50PCT
```



The *X * SPAN* softkey allows the factor defining the center frequency step size to be entered as % of the span.

IEC/IEEE-bus command:

```
FREQ:CENT:STEP:LINK SPAN
FREQ:CENT:STEP:LINK:FACT 20PCT
```



The = *CENTER* softkey sets the step size coupling to *MANUAL* and the step size to the value of the center frequency. This function is especially useful during measurements of the signal harmonic content because by entering the center frequency each stroke of the *STEP* key selects the center frequency of another harmonic.

IEC/IEEE-bus command: --

The = *MARKER* softkey sets the step size coupling to *MANUAL* and the step size to the value of the marker. This function is especially useful during measurements of the signal harmonic content at the marker position because by entering the center frequency each stroke of the *STEP* key selects the center frequency of another harmonic.

IEC/IEEE-bus command: --

The *MANUAL* softkey activates the window for entering a fixed step size.

IEC/IEEE-bus command: `FREQ:CENT:STEP 120MHz`

Softkeys in time domain:

The *0.1 * RBW* softkey sets the step size for the center frequency entry to 10% of the resolution bandwidth.

*AUTO 0.1 * RBW* corresponds to the default setting.

IEC/IEEE-bus command:

```
FREQ:CENT:STEP:LINK RBW
FREQ:CENT:STEP:LINK:FACT 10PCT
```

The *0.5 * RBW* softkey sets the step size for the center frequency entry to 50% of the resolution bandwidth.

IEC/IEEE-bus command:

```
FREQ:CENT:STEP:LINK RBW
FREQ:CENT:STEP:LINK:FACT 50PCT
```



The *X * RBW* softkey allows the factor defining the center frequency step size to be entered as % of the resolution bandwidth.

Values between 1 and 100% in steps of 1% are allowed. The default setting is 10%.

IEC/IEEE-bus command:

```
FREQ:CENT:STEP:LINK RBW
FREQ:CENT:STEP:LINK:FACT 20PCT
```

The = *CENTER* softkey sets the step size coupling to *MANUAL* and the step size to the value of the center frequency. This function is especially useful during measurements of the signal harmonic content because by entering the center frequency each stroke of the *STEP* key selects the center frequency of another harmonic.

IEC/IEEE-bus command: --



The = *MARKER* softkey sets the step size coupling to *MANUAL* and the step size to the value of the marker. This function is especially useful during measurements of the signal harmonic content at the marker position because by entering the center frequency each stroke of the *STEP* key selects the center frequency of another harmonic.

IEC/IEEE-bus command: --



The *MANUAL* softkey activates the window for entering a fixed step size.

IEC/IEEE-bus command:

```
FREQ:CENT:STEP 120MHz
```



The *START* softkey activates the window for manually entering the start frequency.

The allowed range of values for the start frequency is:

$0\ Hz \leq f_{start} \leq f_{max} - minspan$

f_{start} start frequency
minspan smallest selectable span (10 Hz)
f_{max} max. frequency

IEC/IEEE-bus command: `FREQ:STAR 20MHz`



The *STOP* softkey activates the window for entering the .

The allowed range of values for the stop frequency is:

$minspan \leq f_{stop} \leq f_{max}$

f_{stop} stop frequency
minspan smallest selectable span (10 Hz)
f_{max} max. frequency

IEC/IEEE-bus command: `FREQ:STOP 2000MHz`

The *FREQUENCY OFFSET* softkey activates the window for entering an arithmetical frequency offset which is added to the frequency axis labelling. The allowed range of values for the offset is -100 GHz to 100 GHz. The default setting is 0 Hz.

IEC/IEEE-bus command: `FREQ:OFFS 10 MHz`

The *SIGNAL TRACK* softkey switches on the tracking of a signal near the center frequency. The signal is tracked as long it is in the search bandwidth around the center frequency defined with *TRACK BW* and above the level threshold defined with *TRACK THRESHOLD*.
For that purpose, the maximum signal is searched (*PEAK SEARCH)* on the screen and the center frequency set to this signal (*MARKER ->CENTER)* after each frequency sweep within the search bandwidth.

If the signal falls below the level threshold or jumps out of the search bandwidth around the center frequency, the center frequency is not varied until a signal is in the search bandwidth above the level threshold. This can be achieved by manually modifying the center frequency, for example.

On switching on, the softkey is highlighted and the search bandwidth and the threshold value are marked on the diagram by two vertical lines and one horizontal line. All these lines are allocated the designation TRK.

At the same time a submenu is opened in which the search bandwidth, the threshold value and the trace can be modified for the maximum search.

The softkey is only available in the frequency domain (span >0).

IEC/IEEE-bus command: `CALC:MARK:FUNC:STR OFF`

The *TRACK ON/OFF* softkey switches on and off signal tracking.

IEC/IEEE-bus command: `CALC:MARK:FUNC:STR OFF`

The *TRACK BW* softkey defines the search bandwidth for signal tracking. The frequency range is symmetrical with respect to the center frequency.

IEC/IEEE-bus command:
`CALC:MARK:FUNC:STR:BAND 10KHZ`

The *TRACK THRESHOLD* softkey defines the threshold value for signal detection. The value is always entered as an absolute level value.

IEC/IEEE-bus command:
`CALC:MARK:FUNC:STR:THR -70DBM`



The *SELECT TRACE* softkey selects the trace on which signal tracking is to be performed.

IEC/IEEE-bus command:
`CALC:MARK:FUNC:STR:TRAC 1`

Setting the Frequency Span – *SPAN Key*

SPAN menu

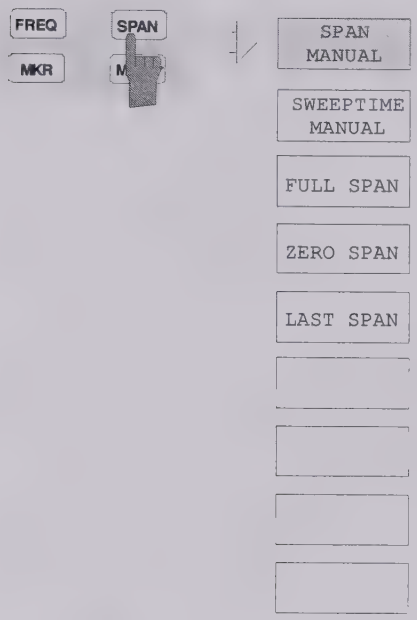

The *SPAN* key opens a menu which offers various options for setting the span.
The entry of the span (*SPAN MANUAL* softkey) is automatically active for span > 0 Hz.
For span = 0 Hz the entry for sweep time (*SWEEPTIME MANUAL*) is automatically active.
With two windows (*SPLIT SCREEN)* displayed at the same time, the input data always refer to the window selected with hotkey *SCREEN A/B.*

The *SPAN MANUAL* softkey activates the window for manually entering the frequency span. The center frequency is kept constant.

The allowed range of span values is:

for the time domain (span = 0): 0 Hz

and for the frequency domain (span >0): minspan $\leq f_{span} \leq f_{max}$

f_{span}	frequency span
minspan	smallest selectable span (10 Hz)
f_{max}	max. frequency

IEC/IEEE-bus command `FREQ:SPAN 2GHz`



The *SWEEPTIME MANUAL* softkey activates the window for entering the sweep time manually with Span = 0 Hz. The softkey is not available for Span > 0 Hz.

IEC/IEEE-bus command: `SWE:TIME 10s`

The *FULL SPAN* softkey sets the span to the full frequency range of FSP.

IEC/IEEE-bus command `FREQ:SPAN:FULL`

The *ZERO SPAN* softkey sets the span to 0 Hz. The x axis becomes the time axis with the grid lines corresponding to 1/10 of the current sweep time (SWT).

IEC/IEEE-bus command `FREQ:SPAN 0Hz`

After changing the span setting the *LAST SPAN* softkey activates the previous setting. With this function a fast change between overview measurement (*FULL SPAN*) and detailed measurement (manually set center frequency and span) is possible.

Note: *Only values > 0 Hz are restored, i.e. a transition between time and frequency domain is not possible.*

IEC/IEEE-bus command `---`

Level Display Setting and RF Input Configuration – *AMPT Key*

The *AMPT* key is used to set the reference level, the maximum level and the display range of the active window as well as the input impedance and the input attenuation of the RF input.

The *AMPT* key opens a menu for setting the reference level and the input attenuation of the active window. The data entry for the reference level (*REF LEVEL* softkey) is opened automatically.

Further settings regarding level display and attenuation can be made in this menu.

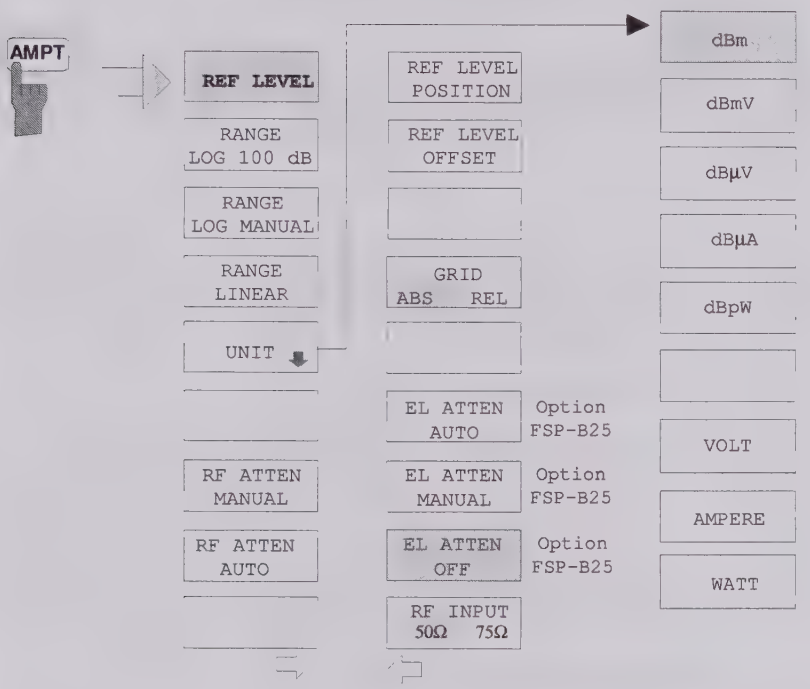



The *REF LEVEL* softkey allows the reference level to be input in the currently active unit (dBm, dBµV, etc).

IEC/IEEE-bus command: `DISP:WIND:TRAC:Y:RLEV -60dBm`

The *RANGE LOG 100 dB* softkey sets the level display range to 100 dB.

IEC/IEEE-bus command:
```
DISP:WIND:TRAC:Y:SPAC LOG
DISP:WIND:TRAC:Y 100DB
```

The *RANGE LOG MANUAL* softkey activates the manual entry of the level display range. Display ranges from 10 to 200 dB are allowed in 10 dB steps. Inputs which are not allowed are rounded to the next valid value.

The default setting is 100 dB.

IEC/IEEE-bus command:
```
DISP:WIND:TRAC:Y:SPAC LOG
DISP:WIND:TRAC:Y 120DB
```

The *RANGE LINEAR* softkey switches the display range of the analyzer to linear scaling. The horizontal lines are labelled in %. The grid has a decadic scaling.

IEC/IEEE-bus command:
```
DISP:WIND:TRAC:Y:SPAC LIN
```

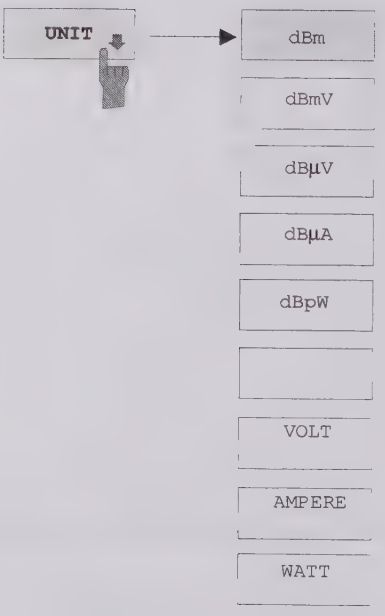

The *UNIT* softkey opens a sub menu allowing to select the unit for the level axis.

The default setting is dBm.

In general, the spectrum analyzer measures the signal voltage at the RF input. The level display is calibrated in rms values of an unmodulated sinewave signal. In the default state, the level is displayed at a power of 1 mW (= dBm). Via the known input resistance of 50 Ω or 75Ω , conversion to other units is possible. The units dBm, dBmV, dBµV, dBµA, dBpW, V, A and W are directly convertible.

IEC/IEEE-bus command:
```
CALC:UNIT:POW DBM
```

The *RF ATTEN MANUAL* softkey allows the attenuation to be entered irrespective of the reference level.

The attenuation can be set in 10 dB steps between 0 and 70 dB (in 5 dB steps between 0 and 75 dB if option FSP-B25, *Electronic Attenuator*, is fitted). Other entries will be rounded to the next lower integer value.

If the defined reference level cannot be set for the given RF attenuation, the reference level will be adjusted accordingly and the warning "Limit reached" will be output.

Note: *The 0-dB value can be entered only via the numeric keypad in order to protect the input mixer against occasional overload.*

IEC/IEEE-bus command: `INP:ATT 40 DB`

The *RF ATTEN AUTO* softkey sets the RF attenuation automatically as a function of the selected reference level.
This ensures that the optimum RF attenuation desired by the user is always used.

RF ATTEN AUTO is the default setting.

IEC/IEEE-bus command: `INP:ATT:AUTO ON`

AMPT – NEXT menu:



The *REF LEVEL POSITION* softkey allows the reference level position to be entered.

The setting range is from -200 to +200%, 0% corresponding to the lower and 100% to the upper limit of the diagram.

IEC/IEEE-bus command: `DISP:WIND:TRAC:RPOS 100PCT`

The *REF LEVEL OFFSET* softkey allows the arithmetic level offset to be entered. This offset is added to the measured level irrespective of the selected unit. The scaling of the Y axis is changed accordingly.

The setting range is ±200 dB in 0.1 dB steps.

IEC/IEEE-bus command: `DISP:WIND:TRAC:RLEV:OFFS -10dB`



The *GRID ABS/REL* softkey switches between absolute and relative scaling of the level axis.

G*RID ABS* is the default setting.

ABS The labelling of the level lines refers to the absolute value of the reference level.

REL The upper line of the grid is always at 0 dB.
The scaling is in dB whereas the reference level is always in the set unit (dBm, dBµV,..).

For setting *RANGE LINEAR* (linear scaling, labelling of axes in %) the softkey is not displayed since the unit % itself implies a relative scale.

IEC/IEEE-bus command: `DISP:WIND:TRAC:Y:MODE ABS`



The *RF INPUT 50 Ω / 75 Ω* softkey switches the input impedance of FSP between 50 Ω (= default setting) and 75 Ω.

The setting 75 Ω should be used if the input impedance (50 Ω) is transformed to 75 Ω using the corresponding adapter unit of type RAZ (= 25 Ω in series to the input impedance of the analyzer). The correction value used for the adaption is 1.76 dB = 10 log (75Ω / 50Ω).

All levels specified in this operating manual refer to the default setting of FSP (50 Ω).

IEC/IEEE-bus command: `INP:IMP 50OHM`

Electronic Attenuator

Besides the mechanical attenuator at the RF input, the FSP also offers an electronic attenuation setting (option *ELECTRONIC ATTENUATOR FSP-B25*). The attenuation range is 0 to 30 dB, with the default attenuation being preset by the mechanical attenuator.

The *EL ATTEN MANUAL* softkey switches the electronic attenuator on and allows the attenuation of the electronic attenuator to be set.

The attenuation can be varied in 5 dB steps from 0 to 30 dB. Other entries are rounded to the next lower integer value.

If the defined reference level cannot be set for the given RF attenuation, the reference level will be adjusted accordingly and the warning "Limit reached" will be output.

IEC/IEEE-bus command:
```
INP:EATT:AUTO OFF
INP:EATT 10 DB
```

This function is only available with option *ELECTRONIC ATTENUATOR FSP-B25*.

The *EL ATTEN AUTO* softkey switches the electronic attenuator on and automatically sets its attenuation to 0 dB.
The allowed setting range of the reference level ranges from the current reference level on switching on the electronic attenuator to over 30 dB. If a reference level is set outside the allowed 30-dB range, setting is performed by means of the mechanical attenuator. From this new reference level to over 30 dB the setting is again performed with the electronic attenuator.

IEC/IEEE-bus command: `INP:EATT:AUTO ON`

This function is only available with option *ELECTRONIC ATTENUATOR FSP-B25*.

The *EL ATTEN OFF* softkey switches the electronic attenuator off.

IEC/IEEE-bus command: `INP:EATT:STAT OFF`

This function is only available with option *ELECTRONIC ATTENUATOR FSP-B25*.

Setting the Bandwidths and Sweep Time – *BW* Key

The *BW* key calls a menu for setting the resolution bandwidth (*RBW*), video bandwidth (*VBW*) and sweep time (*SWT*) for the frequency sweep. The parameters may be coupled dependent on the span (stop minus start frequency) or freely set by the user. When working with a split screen display, the settings always refer to the active window.

FSP offers resolution bandwidths from 10 Hz to 10 MHz in 1, 3, 10 steps:

Resolution bandwidths up to 100 kHz are realized using digital bandpasses with Gaussian characteristics. As far as the attenuation characteristic is concerned they behave like analog filters but have a much higher measurement speed than comparable analog filters. This is due to the fact that the transient response can be compensated as a result of an accurately defined filter behaviour.

Bandwidths above 100 kHz are realized using decoupled 4-circuit LC filters.

As an alternative to the analog filters, FFT filters are available for the bandwidths between 1 Hz and 30 kHz. When working with bandwidths up to 30 kHz, the FFT algorithm offers considerably higher measurement speeds with all the other settings remaining the same. The reason is that with analog filters the sweep time required for a particular span is proportional to (Span/RBW^2). When using the FFT algorithm, however, the sweep time is proportional to (Span/RBW).

The video bandwidths are available in 1, 3, 10 steps between 1 Hz and 10 MHz. They can be set in accordance with the resolution bandwidth. The video filters serve for smoothing the displayed trace. Video bandwidths that are small compared to the resolution bandwidth average out noise peaks and pulsed signals, so that only the signal average is displayed. If pulsed signals are to be measured, it is recommended to use a video bandwidth that is large compared to the resolution bandwidth (VBW $\geq$ 10 x RBW) for the amplitudes of pulses to be measured correctly.

Note:
*For analog and digital filters, FSP has overload reserves of different magnitude above the reference level. Due to the LO breakthrough the overload display OVLD responds with digital filters with RBW < 100 kHz, as soon as the start frequency is selected <6 * resolution bandwidth, for RBW = 100 kHz, as soon as the start frequency is below 3 MHz.*

BW menu:

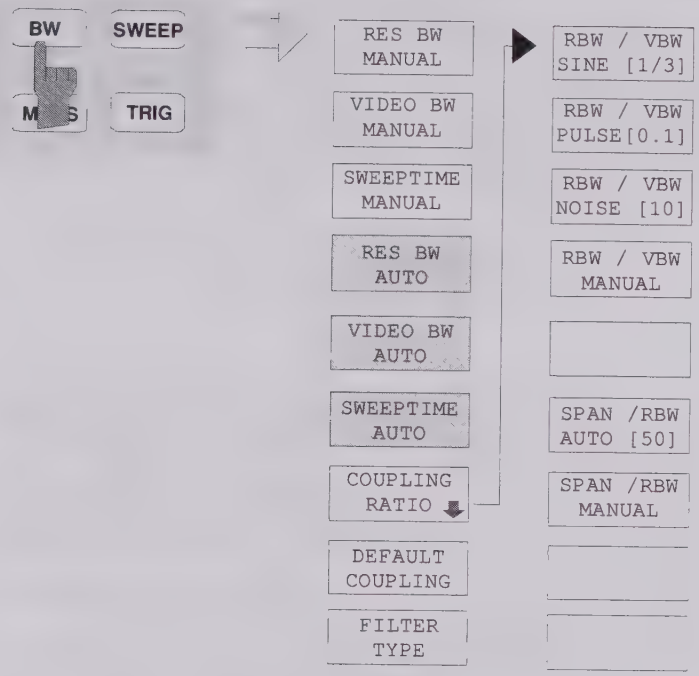

The *BW* key calls a menu for setting the resolution bandwidth, video bandwidth, sweep time and their couplings.

The various .. *BW AUTO* softkeys are used to couple the functions. The coupling ratios are selected by the *COUPLING RATIO* softkey.

The .. *BW MANUAL* softkeys enable the entry of the parameter concerned. This parameter is not coupled to the other parameters.

Note: *With the ... BW AUTO softkeys the resolution bandwidth, the video bandwidth and the sweep time can be entered separately for the frequency domain (span > 0 Hz) and the time domain (span = 0 Hz).*
But with ...BW MANUAL softkeys the selected values apply to both the frequency and time domain.



The *RES BW MANUAL* softkey activates the manual data entry for the resolution bandwidth.

The resolution bandwidth can be selected in 1/3/10 steps in the range between 10 Hz and 10 MHz. The nominal resolution bandwidth is the 3 dB bandwidth. When FFT filters are used, the lower limit of the bandwidth is 1 Hz. FFT filters may be used with bandwidths up to 30 kHz.

For numeric inputs, the values are always rounded to the nearest possible bandwidth. For rollkey or UP/DOWN key inputs, the bandwidth is adjusted in steps either upwards or downwards.

For filter type CHANNEL or RRC the bandwidth is selected from the list of available channel filters given at the end of this chapter. For data entry, the cursor keys ↑ and ↓ scroll through this list.

The manual input mode of the resolution bandwidth is indicated by a green terisk (*) on the display.

IEC/IEEE-bus command:

```
BAND:AUTO OFF;
BAND 1MHz
```



The *VIDEO BW MANUAL* softkey activates the manual data entry for the video bandwidth.

The video bandwidth can be selected in 1/3/10 steps in the range between 1 Hz and 10 MHz.
For numeric inputs, the values are always rounded to the nearest possible allowed bandwidth. For rollkey or UP/DOWN key inputs, the bandwidth is adjusted in steps either downwards or upwards.
The manual input mode of the video bandwidth is indicated by a green terisk (*) on the display.

IEC/IEEE-bus command:
```
BAND:VID:AUTO OFF;
BAND:VID 10 kHz
```



The *SWEEPTIME MANUAL* softkey activates the manual data entry for the sweep time. At the same time, the coupling of the sweep time is cancelled. Other couplings (*VIDEO BW, RES BW*) remain effective.

In the frequency domain (span > 0 Hz) and for resolution bandwidths above 1 kHz, the allowed sweep times for spans > 3.2 kHz range from 2.5 ms through to 16000 s. With spans below 3.2 kHz, the maximum allowed sweep time is reduced to 5 s * span/Hz.
If FFT filters are used, the sweep time is fixed by the span and the bandwidth and therefore cannot be set.
In time domain (span = 0 Hz), the range of sweep times is 1 µs to 16000 s is selectable in steps of max. 5% of the sweep time. For numeric inputs, rounding is made to the nearest possible sweep time. For rollkey or UP/DOWN key inputs, the sweep time is adjusted in steps either downwards or upwards.

The manual input mode of the sweep time is indicated by a green terisk (*) on the display. If the selected sweep time is too short for the selected bandwidth and span, level measurement errors will occur. This happens because the available settling time for the resolution or video filters is too short. In this case, the FSP outputs *UNCAL* on the display and marks the indicated sweep time with a red asterisk (*).

IEC/IEEE-bus command:
```
SWE:TIME:AUTO OFF;
SWE:TIME 10s
```

The *RES BW AUTO* softkey couples the resolution bandwidth to the selected span. Changing the span causes automatic adjustment of the resolution bandwidth.

Automatic coupling of resolution bandwidth to span is always recommended when a favourable setting of the resolution bandwidth in relation to the selected span is desired for the measurement under request.

The coupling ratio is set in the *COUPLING RATIO* submenu.

The *RES BW AUTO* softkey is only available in the frequency domain (span > 0 Hz). The softkey is blanked in the time domain.

IEC/IEEE-bus command:
```
BAND:AUTO ON
```



The *VIDEO BW AUTO* softkey couples the video bandwidth to the resolution bandwidth. If the resolution bandwidth is changed, the video bandwidth is automatically adjusted.

The coupling of the video bandwidth is always recommended when the minimum sweep time is required for a selected resolution bandwidth. Narrower video bandwidths require longer sweep times due to the longer settling time. Wider bandwidths reduce the signal/noise ratio.

The coupling ratio is set in the *COUPLING RATIO* submenu.

The coupling of the video bandwidth to the resolution filter is also permitted for the time domain display (span = 0).

IEC/IEEE-bus command: `BAND:VID:AUTO ON`

The *SWEEPTIME AUTO* softkey couples the sweep time to the span, video bandwidth (VBW) and resolution bandwidth (RBW). The sweep time is automatically adjusted on any change in span, resolution bandwidth or video bandwidth.

The softkey is only available in the frequency domain (span >0 Hz). It is blanked in the time domain.
The FSP always selects the shortest sweep time possible without falsifying the signal. The maximum level error compared to using a longer sweep time is < 0.1 dB. If additional bandwidth and level errors are to be avoided, the sweep time is to be set to three times the time offered in coupled mode.

IEC/IEEE-bus command: `SWE:TIME:AUTO ON`

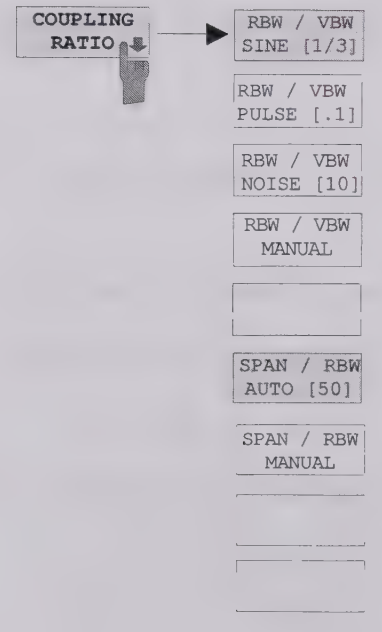

The *COUPLING RATIO* softkey opens a sub menu for selection of the coupling ratios.

When the default setting is active, ie the *COUPLING RATIO* softkey is deactivated (not highlighted), the ratio span/resolution bandwidth (SPAN/RBW) is 50 (this corresponds to SPAN / RBW AUTO [50]) and the ratio resolution bandwidth/video bandwidth (RBW/VBW) is 0.33 (this corresponds to RBW / VBW SINE [1/3]).

If the ratio RBW/VBW or SPAN/RBW is different from the default setting, the *COUPLING RATIO* softkey is highlighted.

The softkeys RBW/VBW... are selection keys. Only one softkey can be enabled at any one time. The softkeys are only effective for the *VBW AUTO* selection in the main menu.

The softkeys SPAN/RBW... are also selection keys. They are only effective for the *RBW AUTO* selection in the main menu.



The *RBW/VBW SINE [1/3]* softkey sets the following coupling ratio:
video bandwidth = 3 x resolution bandwidth.

This is the default setting for the coupling ratio resolution bandwidth/video bandwidth.

This is the coupling ratio recommended if sinusoidal signals are to be measured.

IEC/IEEE-bus command `BAND:VID:RAT 3`

This setting is only effective for the *VBW AUTO* selection in the main menu.



The *RBW/VBW PULSE [.1]* softkey sets the following coupling ratio:
video bandwidth = 10 x resolution bandwidth or
video bandwidth = 10 MHz (= max. VBW).

This coupling ratio is recommended whenever the amplitudes of pulsed signals are to be measured correctly. The IF filter is exclusively responsible for pulse shaping. No additional evaluation is performed by the video filter.

IEC/IEEE-bus command `BAND:VID:RAT 10`

This setting is only effective for the *VBW AUTO* selection in the main menu.



The *RBW/VBW NOISE [10]* softkey sets the following coupling ratio:
video bandwidth = resolution bandwidth/10

At this coupling ratio, noise and pulsed signals are suppressed in the video domain. For noise signals, the average value is displayed.

IEC/IEEE-bus command `BAND:VID:RAT 0.1`

This setting is only effective for the *VBW AUTO* selection in the main menu.



The *RBW/VBW MANUAL* softkey activates the manual input of the coupling ratio.

The resolution bandwidth/video bandwidth ratio can be set in the range 0.001 to 1000.

IEC/IEEE-bus command `BAND:VID:RAT 10`

This setting is only effective for the *VBW AUTO* selection in the main menu.



The *SPAN/RBW AUTO [50]* softkey sets the following coupling ratio:
resolution bandwidth = span/50

This coupling ratio is the default setting of the FSP.

IEC/IEEE-bus command `BAND:RAT 0.02`

This setting is only effective for the *RBW AUTO* selection in the main menu.



The *SPAN/RBW MANUAL* softkey activates the manual input of the coupling ratio.

The span / resolution bandwidth ratio can be set in the range 1 to 10000.

IEC/IEEE-bus command `BAND:RAT 0.1`

This setting is only effective for the *RBW AUTO* selection in the main menu.



The *DEFAULT COUPLING* softkey sets all coupled functions to the default state (*AUTO).* In addition, the ratio *RBW/VBW* is set to *SINE [1/3]* and the ratio *SPAN/RBW* to 50 in the *COUPLING RATIO* submenu (default setting, *COUPLING RATIO* softkey not highlighted).

IEC/IEEE-bus command
```
BAND:AUTO ON
BAND:VID:AUTO ON
SWE:TIME:AUTO ON
```

The *FILTER TYPE* softkey opens the selection list for different filter types. In the range up to 30 kHz digital band filters with Gaussian characteristic and filtering with FFT algorithm can be selected.

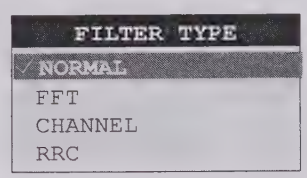

NORMAL For resolution bandwidths up to 30 kHz bandpasses are used.

FFT An FFT is performed. For that purpose, the filtered IF signal is digitized and then transformed into the spectral domain via FFT. The transformation range depends on the selected filter bandwidths and can be set between 4 kHz to 50 kHz. If the span is larger than the transformation range, several transformations are performed and the results are appended to each other in the spectral domain. If the span is smaller than the transformation range, the measurement results are interpolated when the number of measurement points provided by the FFT is smaller than the number of display points in x-direction (501). A flattop window serves as a window in the time domain so that high amplitude precision with good selection is achieved.

Sweep time	Defined by the selected bandwidth and span (reason: FFT filtering is a block transformation). It cannot be changed (softkey deactivated).
Detector	Sample detector and peak detector are available. Peak detector is active when AUTO SELECT is selected.
Video bandwidth	Not defined in case of FFT; therefore cannot be set (softkeys deactivated).

Compared to bandpasses, FFT filters lead to significantly reduced sweep times. For a span of 50 kHz and a bandwidth of 100 Hz, for instance, the sweep time is reduced from 5 s to 40 ms. FFT filters are particularly suitable for stationary signals (sinusoidal signals or signals that are continuously modulated in time). For burst signals (TDMA) or pulsed signals, normal filters are preferable.

Note:

As soon as the FFT filters are active (RBW ≤ 30 kHz) the sweep time display field (SWT) is replaced by the acquisition time (AQT) display field.

FFT is a block transformation so the result depends on the time relation between the dataset to be transformed and the burst or pulsed signal. A gated sweep measurement for TDMA signals is therefore not provided if FFT filters are used.

When the tracking generator (option FSP-B9) is used as signal source for the DUT, filtering with the FFT algorithm is not useful. The selection FFT is thus not available if the tracking generator is switched on.

Additionally, a number of especially steep-edged channel filters are available for power measurement since firmware version 1.10.

A distinction is made between the following filter types:

CHANNEL = general, steep-edged channel filters

RRC = filters with root-raised cosine characteristic (RRC = Root Raised Cosine)

When selecting these filter types, the automatic coupling of the resolution bandwidth to the span is not available. The filters are selected via the *RES BW* softkey.

A list of all available channel filters with their associated applications can be found at the end of this chapter.

IEC/IEEE-bus command: `BAND:TYPE NORM`

List of available channel filters

The channel filters included in the following table are available for firmware version 1.10 or higher. They can be activated via the *FILTER TYPE* softkey and are then available as resolution filters (softkey *RES BW*).

Note:
For filters of type RRC (Root Raised Cosine), the filter bandwidth indicated describes the sampling rate of the filter.
For all other filters (CFILter) the filter bandwidth is the 3 dB bandwidth.

Filter Bandwidth	Filter Type	Application
100 Hz	CFILter	
200 Hz	CFILter	A0
300 Hz	CFILter	
500 Hz	CFILter	
1 kHz	CFILter	
1.5 kHz	CFILter	
2 kHz	CFILter	
2.4 kHz	CFILter	SSB
2.7 kHz	CFILter	
3 kHz	CFILter	
3.4 kHz	CFILter	
4 kHz	CFILter	DAB, Satellite
4.5 kHz	CFILter	
5 kHz	CFILter	
6 kHz	CFILter	
8.5 kHz	CFILter	ETS300 113 (12.5 kHz channels)
9 kHz	CFILter	AM Radio
10 kHz	CFILter	
12.5 kHz	CFILter	CDMAone
14 kHz	CFILter	ETS300 113 (20 kHz channels)
15 kHz	CFILter	
16 kHz	CFILter	ETS300 113 (25 kHz channels)
18 kHz, α=0.35	RRC	TETRA
20 kHz	CFILter	
21 kHz	CFILter	PDC
24.3 kHz, α=0.35	RRC	IS 136
25 kHz	CFILter	
30 kHz	CFILter	CDPD, CDMAone
50 kHz	CFILter	
100 kHz	CFILter	
150 kHz	CFILter	FM Radio
192 kHz	CFILter	PHS
200 kHz	CFILter	
300 kHz	CFILter	
500 kHz	CFILter	J.83 (8-VSB DVB, USA)
1.0 MHz	CFILter	CDMAone
1.2288 MHz	CFILter	CDMAone
1.5 MHz	CFILter	DAB

Sweep Settings – *SWEEP* Key

The SWEEP key serves for configuring the sweep mode.

SWEEP menu

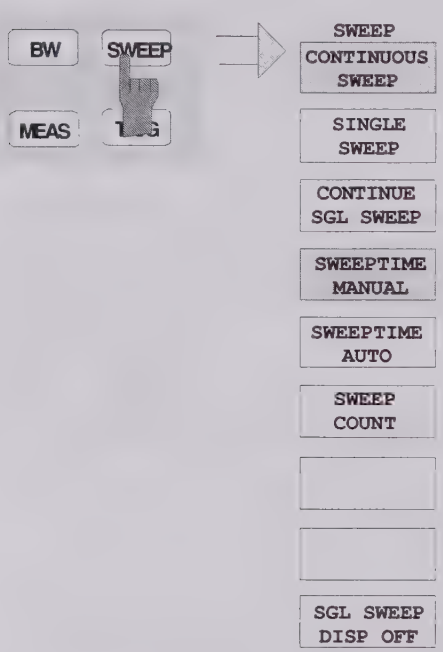

The *SWEEP* key calls a menu in which the sweep mode is defined. In split-screen mode, the entries made are valid for the active window only.

The *CONTINUOUS SWEEP, SINGLE SWEEP* and *SGL SWEEP DISP OFF* softkeys are mutually exclusive selection keys.



The *CONTINUOUS SWEEP* softkey activates the continuous sweep mode, which means that the sweep takes place continuously according to the trigger mode set.

When working in the split-screen mode and with different settings in the two windows, screen A is swept first, followed by screen B. When the softkey is pressed, the sweep is restarted.

CONTINUOUS SWEEP is the default setting of FSP.

IEC/IEEE-bus command: `INIT:CONT ON`

The *SINGLE SWEEP* softkey starts n sweeps after triggering. The number of sweeps is determined by the *SWEEP COUNT* softkey.

When working in the split-screen mode, the frequency ranges of the two windows are swept one after the other.

If a trace is swept using *TRACE AVERAGE* or *MAXHOLD,* the value set via the SWEEP COUNT softkey determines the number of sweeps. If 0 has been entered, one sweep is performed.

IEC/IEEE-bus command: `INIT:CONT OFF`

The *CONTINUE SGL SWEEP* softkey repeats the number of sweeps set under *SWEEP COUNT*, however without first deleting the trace.

This is particularly of interest when using the functions *TRACE AVERAGE* and *MAXHOLD*, if previously recorded measurement results are to be taken into consideration for averaging / maximum search.

If *SGL SWEEP DISP OFF* is active, the screen is switched off also during repeated sweeps.

IEC/IEEE-bus command: `INIT:CONT ONCE`

The *SWEEPTIME MANUAL* softkey activates the window for entering the sweep time manually (see also BW menu).

IEC/IEEE-bus command: `SWE:TIME 10s`

The *SWEEPTIME AUTO* softkey activates the automatic selection of the sweep time as a function of the bandwidth of the resolution and video filters (see also BW menu).

IEC/IEEE-bus command: `SWE:TIME:AUTO ON`

The *SWEEP COUNT* softkey activates the window for the entry of the number of sweeps to be performed by FSP after a single sweep has been started. If Trace Average, Max Hold or Min Hold is activated, this also determines the number of averaging or maximum search procedures.

Example:
[**TRACE1**: *MAX HOLD*]
[**SWEEP**: *SWEEP COUNT*: {10} **ENTER**]
[*SINGLE SWEEP*]

FSP performs the Max Hold function over 10 sweeps.

The allowed range for the sweep count is 0 to 32767. For sweep count = 0 or 1, one sweep is performed. For trace averaging in the continuous-sweep mode, FSP performs running averaging over 10 sweeps if sweep count = 0; if sweep count = 1, no averaging is performed.

The sweep count is valid for all the traces in a diagram.

Note: *The number of sweeps set in the TRACE menu is the same as that in the SWEEP menu.*
If SINGLE SWEEP is selected, the measurement stops after the selected number of sweeps has been performed.

IEC/IEEE-bus command: `SWE:COUN 64`

The *SGL SWEEP DISP OFF* softkey deactivates the display while a single sweep is being performed. Once the sweep has been completed, the trace is shown.

IEC/IEEE-bus command: `INIT:DISP OFF;:INIT.04`

Triggering the Sweep– *TRIG* Key

The *TRIG* key opens a menu for selection of the various trigger sources, trigger polarity and external gate function. The active trigger mode is indicated by highlighting the corresponding softkey.

For video trigger, a trigger threshold can be entered, which is represented in the diagram as a horizontal line.

To indicate that a trigger mode other than *FREE RUN* has been set, the enhancement label **TRG** is displayed on the screen. If two windows are displayed, TRG appears next to the appropriate window.

TRIGGER menu

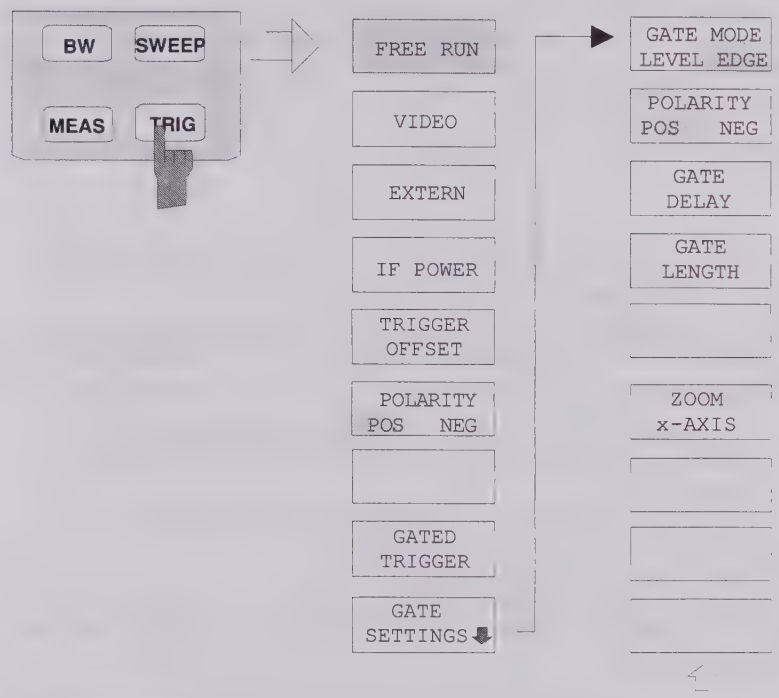



The *FREE RUN* softkey activates the free-run sweep mode, ie start of a sweep is not triggered. Once a measurement is completed, another is started immediately.

FREE RUN is the default setting of FSP.

IEC/IEEE-bus command: `TRIG:SOUR IMM`

The *VIDEO* softkey activates triggering through the displayed voltage.

For the video triggering mode, a horizontal trigger line is shown in the diagram. It may be used to set the trigger threshold between 0% and 100% of the overall diagram height.

IEC/IEEE-bus command:
```
TRIG:SOUR VID
TRIG:LEV:VID 50 PCT
```



The *EXTERN* softkey activates triggering via a TTL signal at the input connector *EXT TRIGGER/GATE* on the rear panel.

IEC/IEEE-bus command:
```
TRIG:SOUR  EXT
SWE:EGAT:SOUR  EXT
```

The *IF POWER* softkey activates triggering of the measurement via signals which are outside the measurement channel.

FSP uses a level detector at the second intermediate frequency. The detector threshold is approximately -20 dBm at the input mixer. This means that the actual trigger level at the RF input is approx. -20 dBm plus the set RF attenuation.
The bandwidth at the intermediate frequency is 10 MHz. Triggering takes place when the trigger threshold is exceeded within a 5 MHz bandwidth about the selected frequency (= start frequency in the frequency sweep). Thus, the measurement of spurious emissions, eg for pulsed carriers, is possible even when the carrier lies outside the selected frequency span.

IEC/IEEE-bus command:
```
TRIG:SOUR  IFP
SWE:EGAT:SOUR  IFP
```

The *TRIGGER OFFSET* softkey activates the window for entering the time offset between the trigger signal and the start of the sweep.

Triggering is delayed by the entered time with respect to the trigger signal (time entered > 0) or is started earlier (time entered < 0). The time may be entered in multiples of 125 ns in the range -100 s to 100 s (default 0 s).

Note: *A negative offset (pretrigger) can be set in the time domain only (SPAN = 0 Hz) provided GATED TRIGGER is not active in that domain.*
The maximum allowed range and the maximum resolution of the pretrigger is limited by the set sweep time:
max. range = - 499/500 x sweep time
max. resolution = sweep time/500.
Pretriggering is not possible when the rms or the average detector is activated.

As a common input signal is used for both trigger and gate when selecting *EXTERN* and *IF POWER,* changes to the gate delay will affect the trigger delay *(TRIGGER OFFSET)* as well.

IEC/IEEE-bus command:
```
TRIG:HOLD  10US
```



The *POLARITY POS/NEG* softkey selects the polarity of the trigger source.

The sweep starts after a positive or negative edge of the trigger signal. The selected setting is highlighted.

The selection is valid for all trigger modes with the exception of *FREE RUN*; in the gate mode, it also applies to the gate polarity.

The default setting is *POLARITY POS.*

IEC/IEEE-bus command:
```
TRIG:SLOP  POS
```

By using a gate in sweep mode and stopping the measurement while the gate signal is inactive, the spectrum for pulsed RF carriers can be displayed without the superposition of frequency components generated during switching. Similarly, the spectrum can also be examined for an inactive carrier. The sweep can be controlled by an external gate or by the internal power trigger.

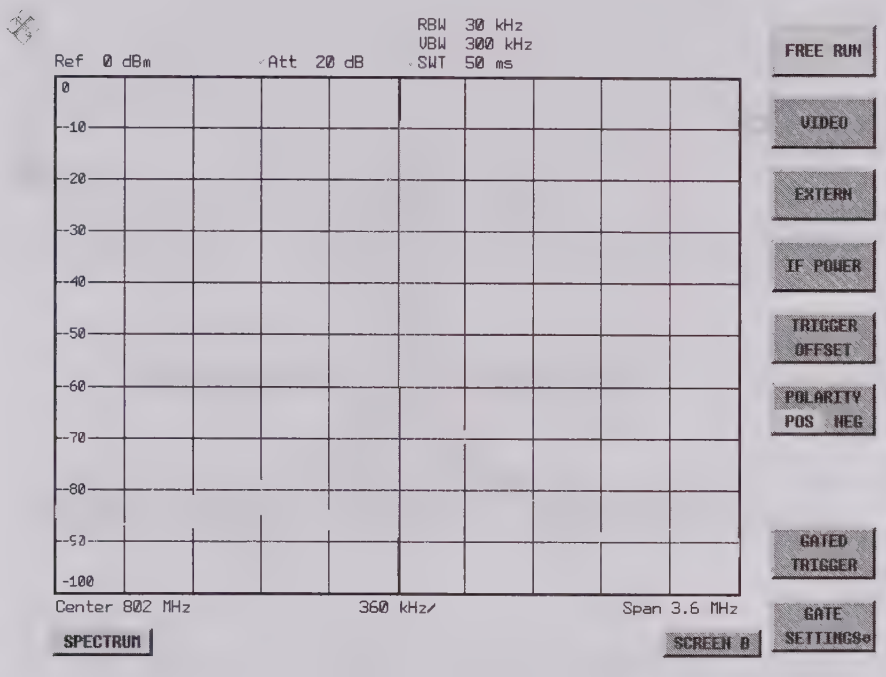

Fig. 4-1 Pulsed signal GATE OFF

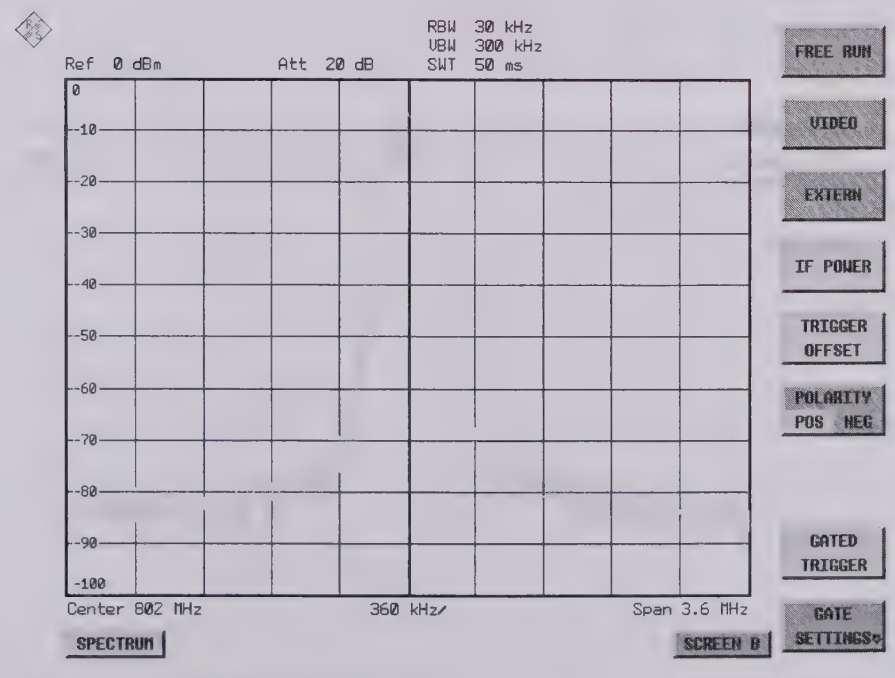

Fig. 4-2 TDMA signal with GATE ON

The gated-sweep mode is activated by the *GATED TRIGGER* softkey. The setting of the mode takes place in the *GATE SETTINGS* submenu.

The *GATED TRIGGER* softkey switches the sweep mode with gate on and off.

When gate is switched on, a gate signal applied to the rear panel connector *EXT TRIGGER/GATE* or the internal IF power detector controls the sweep of the analyzer. This selection is made via the *EXTERN* and *IF POWER* softkeys for trigger and gate.
The length of the gate signal defines when the sweep is to be interrupted. Here a differentiation is made between edge-triggered and level-triggered modes: in case of edge triggering the gate length can be set via the *GATE LENGTH* softkey, while in case of level triggering the gate length depends on the length of the gate signal.

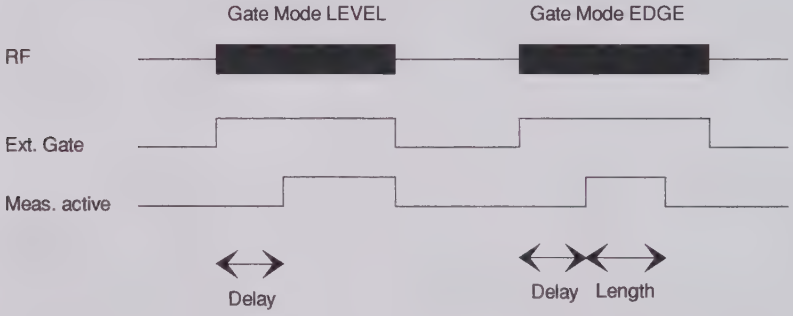

Fig.4-3 Timing diagram for GATE, GATE DELAY and GATE LENGTH

This softkey requires the *EXTERN* or *IF POWER* trigger mode. If a different mode is active, IF POWER is automatically selected.

Gated-sweep operation is also possible in the time domain. This enables - eg in burst signals - level variations of individual slots to be displayed versus time.

To indicate that a gate is used for the sweep, the enhancement label **GAT** is displayed on the screen. This label appears to the right of the window for which the gate is configured.

IEC/IEEE-bus command:

```
SWE:EGAT  ON
SWE:EGAT:SOUR  IFP
or:
SWE:EGAT:SOUR  EXT
```

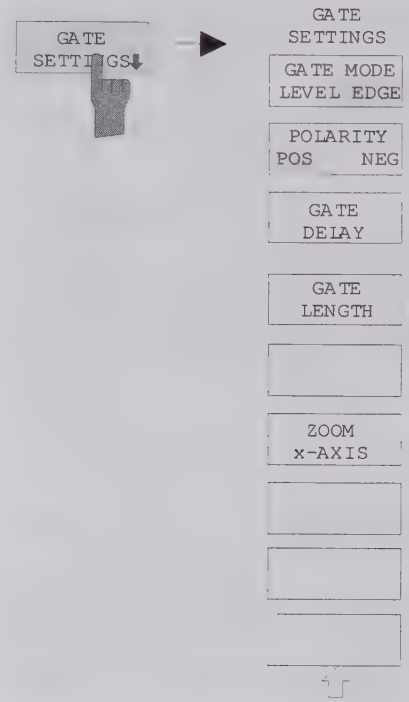

The *GATE SETTINGS* softkey calls a submenu for making all the settings required for gated-sweep operation.

At the same time, a transition is made to the time domain (span = 0) and the time parameters *GATE DELAY* and *GATE LENGTH* are represented as vertical lines. This allows the required gate time parameters to be set easily.

For highly accurate setting of gate delay and gate length, the x axis can be altered using the *ZOOM x-AXIS* softkey in a way that the signal range concerned (eg one full burst) is displayed.

Then the sampling time and duration can be set by *GATE DELAY* and *GATE LENGTH* in a way that the desired portion of the signal is shown.

When quitting the submenu, the program will return to the frequency domain provided it was active before. The original span is restored so the desired measurement can now be performed with the accurately set gate.

IEC/IEEE-bus command: --

The *GATE MODE LEVEL/EDGE* softkey selects the trigger mode. Gated sweep is possible in the level-triggered as well as in the edge-triggered mode.

If level triggering is selected, the *GATE LENGTH* softkey becomes inactive and cannot be operated.

IEC/IEEE-bus command: `SWE:EGAT:TYPE EDGE`

The *POLARITY POS/NEG* softkey controls the polarity of the *EXT TRIGGER/GATE* control line.

In case of level triggering the sweep is stopped by *POLARITY POS* and a logic ´0´ signal; the signal ´1´ will restart the sweep after the *GATE DELAY* time has elapsed.

In case of edge triggering the sweep is continued on a ´0´ to ´1´ transition for the duration of *GATE LENGTH* after a delay (*GATE DELAY)* has elapsed.

Changing the polarity automatically implies a transition of the trigger-edge polarity (*POLARITY* softkey in the higher menu).

IEC/IEEE-bus command: `SWE:EGAT:POL POS`

The *GATE DELAY* softkey activates the window for setting the delay time between the gate signal and the continuation of the sweep.

This may be useful for taking into account a delay between the gate signal and the stabilization of an RF carrier for example.

As gate delay, values between 125 ns and 100 s may be set. The position of the delay on the time axis in relation to the sweep is indicated by the line labelled **GD**.

As there is a common input signal for trigger and gate if *EXTERN* or *IF POWER* is selected, changes to the gate delay will affect the trigger delay (*TRIGGER OFFSET*) as well.

IEC/IEEE-bus command: `SWE:EGAT:HOLD 1US`

The *GATE LENGTH* softkey activates the window for setting the sweep duration of FSP in the edge-triggered mode.

Values between 125 ns and 100 s may be set for the gate length. The length of the gate in relation to the sweep is indicated by the line labelled **GL.**

This softkey is only available if *GATE MODE EDGE* (edge triggering) has been selected.

IEC/IEEE-bus command: `SWE:EGAT:LENG 100US`



The *ZOOM x-AXIS* softkey enables the user to change the time axis to obtain a higher resolution for positioning gate delay and gate length.
When this is to be done, the sweep time temporarily changes; the original value is restored when the menu is quit.

IEC/IEEE-bus command: `--`

Measurement example:

The modulation spectrum of a GSM or PCS1900 signal is to be measured using the gated-sweep function. The signal is generated by a Signal Generator SME03 whose RF output is directly connected to the RF input of FSP.

Settings on SME03:

FREQ:	802 MHz
Level:	0 dBm: Return
Digital Mod:	Select: GMSK: Select
Source:	Select: PRBS: Select: Return
Level Attenuation:	Select: 60 dB: Return

The SME03 supplies a GMSK-modulated TDMA signal (GSM).

Settings on FSP:

Conventions:

[KEY]	Menu called by this key. All information between the brackets refers to this menu.
{Number}	Numeric value to be entered for the parameter on hand.
SOFTKEY	Softkey to be used for making a selection or entering a value.

[PRESET]
[FREQ: *CENTER* {802} **MHz]**
[SPAN {3.6} **MHz]**
[AMPT: *REF LEVEL* {0} **dBm**: *RF ATTEN MANUAL*: {10} **dB]**
[BW: *RES BW MANUAL*: {30} **kHz]**
[TRACE : *TRACE 1* *DETECTOR*: *RMS]*
[SWEEP: *SWEEPTIME MANUAL*: {50} **ms]**
[TRIG: *EXTERN*
GATED TRIGGER;
GATE SETTINGS: *GATE MODE EDGE; POLARITY POS*
SWEEPTIME MANUAL {1} **ms**: *GATE DELAY* {300} **µs**:
GATE LENGTH: {250} **µs]**

The following figure shows the screen display for setting gate parameters. The vertical lines for gate delay (GD) and gate length (GL) can be adjusted to the burst signal by entering numeric values or by means of the rollkey.

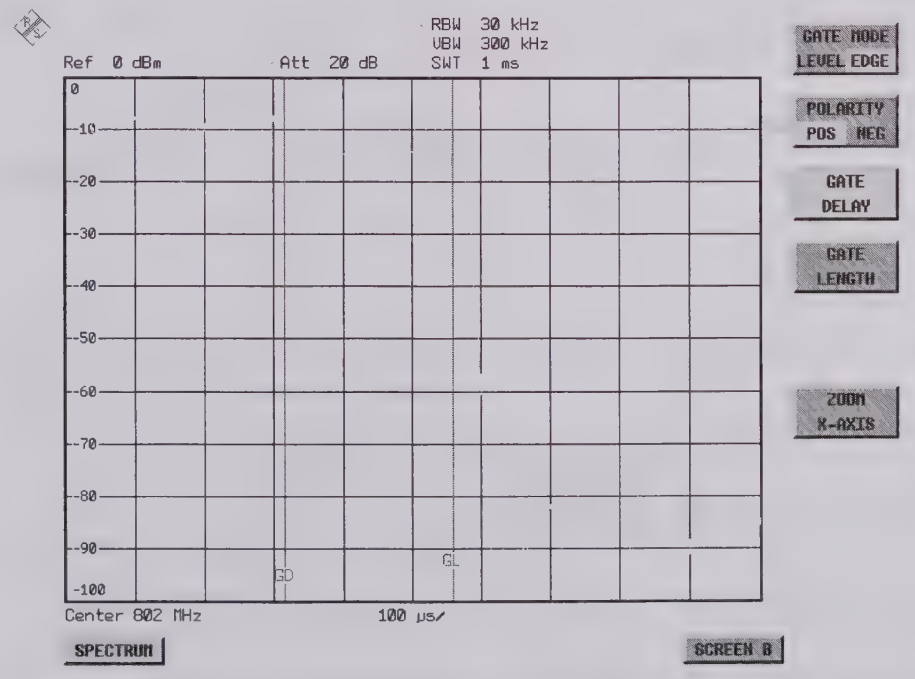

Fig.4-4 Setting GATE DELAY and GATE LENGTH in time domain by means of lines GD and GL

On quitting the *GATE SETTINGS* menu, FSP returns to the previous screen.

Selection and Setting of Traces – *TRACE* Key

The FSP is capable of displaying up to three different traces at a time in a diagram. A trace consists of a maximum of 501 pixels on the horizontal axis (frequency or time). If more measured values than pixels are available, several measured values are combined in one pixel.
The traces are selected using the *SELECT TRACE* softkey in the menu of the *TRACE* key.

The traces can individually be activated for a measurement or frozen after completion of a measurement. Traces that are not activated are blanked.

The display mode can be selected for each trace. Traces can be overwritten in each measurement (CLEAR/WRITE mode), averaged over several measurements (AVERAGE mode), or a maximum or minimum value can be determined from several measurements and displayed (MAX HOLD or MIN HOLD).
Individual detectors can be selected for the various traces. The autopeak detector displays maximum and minimum values connected by a vertical line. The max peak detector and min peak detector display the maximum and minimum value of the level within a pixel. The sample detector displays the instantaneous value of the level at a pixel. The rms detector displays the power (rms value) of the measured values within a pixel, the average detector the average value.

Selection of Trace Function

The trace functions are subdivided as follows:

- Display mode of trace (CLEAR/WRITE, VIEW and BLANK)
- Evaluation of the trace as a whole (AVERAGE, MAX HOLD and MIN HOLD)
- Evaluation of individual pixels of a trace (AUTOPEAK, MAX PEAK, MIN PEAK, SAMPLE, RMS, AVERAGE and QUASIPEAK)

TRACE menu

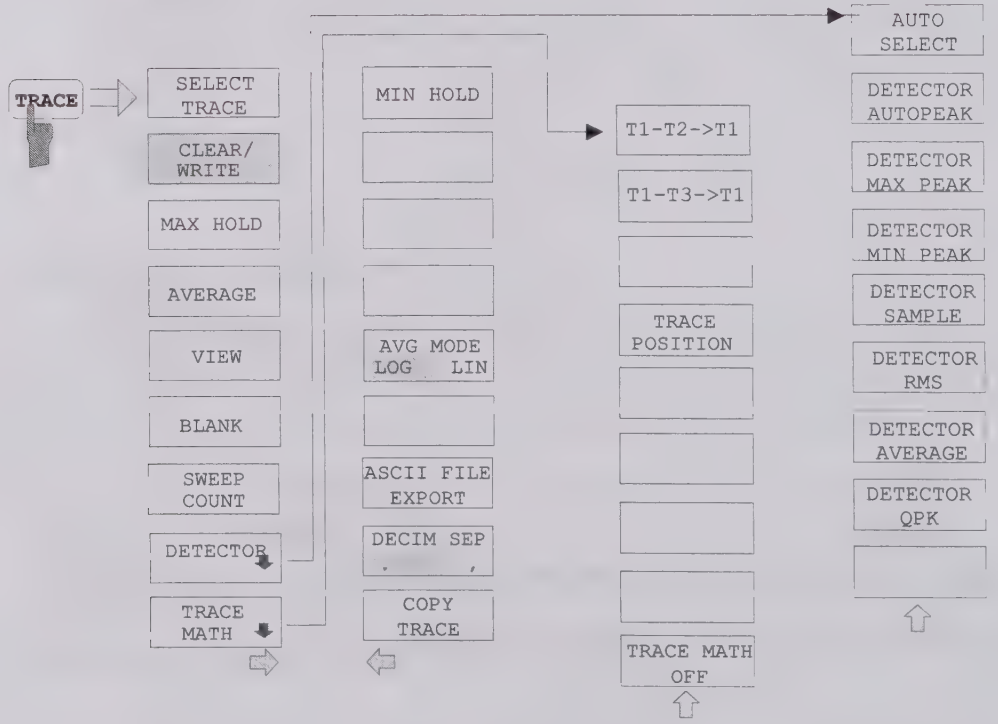

The *TRACE* key opens a menu offering the setting options for the selected trace.

In this menu, the mode of representing the measured data in the frequency or time domain in the 501 pixels of the display is determined. Upon start of the measurement, each trace can be displayed either completely new or based on the previous results.
Traces can be displayed, blanked and copied. Traces can also be corrected with the aid of mathematical functions.
The measurement detector for the individual display modes can be selected directly by the user or set automatically by FSP.

The default setting is trace 1 in the overwrite mode (*CLEAR / WRITE*), the other traces 2 and 3 are switched off (*BLANK*).

The *CLEAR/WRITE, MAX HOLD, MIN HOLD, AVERAGE, VIEW* and *BLANK* softkeys are mutually exclusive selection keys.

The *SELECT TRACE* softkey activates the entry for the active trace (1, 2, 3).

IEC/IEEE-bus command -- (selected via numeric suffix of `:TRACe`)



The *CLEAR/WRITE* softkey activates the overwrite mode for the collected measured values, ie the trace is overwritten by each sweep.

In the *CLEAR/WRITE* display mode all the available detectors can be selected. In the default mode the autopeak detector (setting *AUTO*) is selected.

Each time the *CLEAR/WRITE* softkey is actuated, FSP clears the selected trace memory and starts the measurement anew.

IEC/IEEE-bus command `DISP:WIND:TRAC:MODE WRIT`

The *MAX HOLD* softkey activates the max peak detector.
FSP saves the sweep result in the trace memory only if the new value is greater than the previous one.

The detector is automatically set to *MAX PEAK*. The maximum value of a signal can thus be determined over several sweeps.

This is especially useful with modulated or impulsive signals. The signal spectrum is filled up upon each sweep until all signal components are detected in a kind of envelope.

Pressing the *MAX HOLD* softkey again clears the trace memory and restarts the max hold mode.

IEC/IEEE-bus command `DISP:WIND:TRAC:MODE MAXH`



The *AVERAGE* softkey activates the trace averaging function. The average is formed over several sweeps. Averaging can be performed with any of the detectors available. If the detector is automatically selected by FSP, the sample detector is used.

Depending on the setting of AVG MODE LOG / LIN, the logarithmic level values or the measured power/voltage values are averaged.

Averaging is restarted every time the *AVERAGE* softkey is pressed. The trace memory is always cleared.

IEC/IEEE-bus command `DISP:WIND:TRAC:MODE AVER`

Description of averaging

Averaging is carried out over the pixels derived from the measurement samples. Several measured values may be combined in a pixel. This means that with linear level display the average is formed over linear amplitude values and with logarithmic level display over levels. For this reason the trace must be measured again when changing between *LIN* and *LOG* display mode. The settings *CONT/SINGLE SWEEP* and running averaging apply to the average display analogously.

There are two methods for calculating the average. For a sweep count = 0 , a running average is calculated according to the following formula:

$$\mathrm{TRACE} = \frac{9 * \mathrm{TRACE} + \mathrm{meas.\ value}}{10}$$

Due to the weighting between the new measured value and the trace average, past values have practically no influence on the displayed trace after about ten sweeps. With this setting, signal noise is effectively reduced without need for restarting the averaging process after a change of the signal.

If the sweep count is >1, averaging takes place over the selected number of sweeps. In this case the displayed trace is determined during averaging according to the following formula:

$$\mathrm{Trace}_n = \frac{1}{n}\left[\sum_{i=1}^{n-1}(T_i) + \mathrm{meas.value}_n\right]$$

where n is the number of the current sweep (n = 2 ... SWEEP COUNT). No averaging is carried out for the first sweep but the measured value is stored in the trace memory. With increasing n, the displayed trace is increasingly smoothed since there are more single sweeps for averaging.

After the selected number of sweeps the average trace is saved in the trace memory. Until this number of sweeps is reached, a preliminary average is displayed.

After completion of averaging, ie when the averaging length defined by *SWEEP COUNT* is attained, a running averaging is continued with *CONTINUOUS SWEEP* according to the following formula:

$$\mathrm{Trace} = \frac{(N-1)\cdot \mathrm{Trace}_{old} + \mathrm{meas.value}}{N}$$

where

Trace = new trace
Trace_{old} = old trace
N = SWEEP COUNT

The display "Sweep N of N" does not change any more until a new start is triggered.

In the *SINGLE SWEEP* mode, the number of sweeps is triggered with *SWEEP START*. The sweeps are stopped when the selected number of sweeps is attained. The number of the current sweep and the total number of sweeps are shown on the display: "Sweep 3 of 200".



The *VIEW* softkey freezes the current contents of the trace memory and displays it.

If a trace is frozen by *VIEW*, the instrument settings can be changed without the displayed trace being modified (exception: level display range and reference level, see below). The fact that the trace and the current instrument setting do not agree any more is indicated by an enhancement label "*" at the right edge of the grid.

If in the *VIEW* display mode the level display range (*RANGE*) or the reference level (*REF LEVEL*) are changed, FSP automatically adapts the measured data to the changed display range. This allows an amplitude zoom to be made after the measurement in order to show details of the trace.

IEC/IEEE-bus command `DISP:WIND:TRAC:MODE VIEW`

The *BLANK* softkey activates the blanking of the trace on the screen.

IEC/IEEE-bus command `DISP:WIND:TRAC OFF`

The *SWEEP COUNT* softkey activates the entry of the number of sweeps used for averaging. The allowed range of values is 0 to 30000 and the following should be observed:

- Sweep Count = 0 means running averaging
- Sweep Count = 1 means no averaging being carried out
- Sweep Count > 1 means averaging over the selected number of sweeps; in the continuous sweep mode averaging is performed until the set number of sweeps is attained and is then continued as running averaging.

The default setting is running averaging (Sweep Count = 0). The number of sweeps used for averaging is the same for all active traces in the selected diagram.

Note: *The setting of the sweep count in the trace menu is equivalent to the setting in the sweep menu.*

IEC/IEEE-bus command `SWE:COUN 64`

See following Section "Selection of Detector"



See following Section "Mathematical Functions for Traces"

TRACE - NEXT menu

The *MIN HOLD softkey* activates the min peak detector. FSP saves for each sweep the smallest of the previously stored/currently measured values in the trace memory. The detector is automatically set to *MIN PEAK*. In this way, the minimum value of a signal can be determined over several sweeps.

This function is useful eg for making an unmodulated carrier in a composite signal visible. Noise, interference signals or modulated signals are suppressed by the min hold function whereas a CW signal is recognized by its constant level.

Pressing the *MIN HOLD* softkey again clears the trace memory and restarts the min hold function.

IEC/IEEE-bus command `DISP:WIND:TRAC:MODE MINH`



The *AVG MODE LOG/LIN* softkey selects logarithmic or linear averaging for the logarithmic level display mode.

At the same time the difference calculation is switched between linear and logarithmic in submenu *TRACE MATH*.

IEC/IEEE-bus command `CALC:MATH:AVER:MODE LIN`

With logarithmic averaging, the dB values of the display voltage are averaged or substracted from each other with trace mathematical functions. With linear averaging the level values in dB are converted into linear voltages or powers prior to averaging. Voltage or power values are averaged or offset against each other and reconverted into level values.

For stationary signals the two methods yield the same result.

Logarithmic averaging bzw. Verrechnung is recommended if sinewave signals are to be clearly visible against noise since with this type of averaging noise suppression is improved while the sinewave signals remain unchanged.

For noise or pseudo-noise signals the positive peak amplitudes are decreased in logarithmic averaging due the characteristic involved and the negative peak values are increased relative to the average value. If the distorted amplitude distribution is averaged, a value is obtained that is smaller than the actual average value. The difference is -2.5 dB.

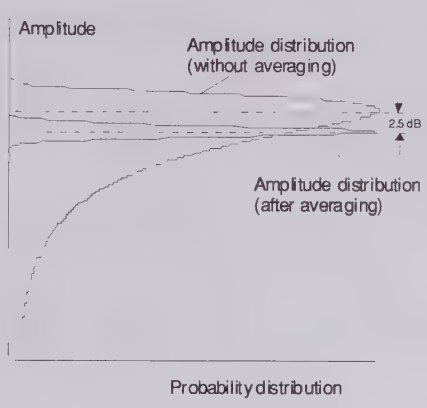

This low average value is usually corrected in noise power measurements by a 2.5 dB factor. Therefore the FSP offers the selection of linear averaging. The trace data are delogarithmized prior to averaging, then averaged and logarithmized again for display on the screen. The average value is always correctly displayed irrespective of the signal characteristic.

The *ASCII FILE EXPORT* softkey stores the active trace in ASCII format on a floppy disk.

IEC/IEEE command
```
FORM ASC;
MMEM:STOR:TRAC 1,'TRACE.DAT'
```

The file consists of the header containing important scaling parameters and a data section containing the trace data.

The data of the file header consist of three columns, each separated by a semicolon:
parameter name; numeric value; basic unit

The data section starts with the keyword " Trace <n> " (<n> = number of stored trace), followed by the measured data in one or several columns (depending on measurement) which are also separated by a semicolon.
This format can be read in from spreadsheet calculation programs, eg MS-Excel. It is necessary to define ';' as a separator.

Note: *Different language versions of evaluation programs may require a different handling of the decimal point. It is therefore possible to select between separators '.' (decimal point) and ',' (comma) using softkey DECIM SEP.*

Example:

	File contents	Description
File header	Type;FSP3;	Instrument model
	Version;1.00;	Firmware version
	Date;01.Jul 1999;	Date of data set storage
	Mode;Spectrum;	Instrument mode
	Center Freq;55000;Hz	Center frequency
	Freq Offset;0;Hz	Frequency offset
	Span;90000;Hz	Frequency range (0 Hz with zero span and statistics measurements)
	x-Axis;LIN;	Scaling of x axis linear (LIN) or logarithmic (LOG)
	Start;10000;Hz Stop;100000;Hz	Start/stop of the display range. Unit: Hz for span > 0, s for span = 0, dBm/dB for statistics measurements
	Ref.Level;-30;dBm	Reference level
	Level Offset;0;dB	Level offset
	Ref Position;75;%	Position of reference level referred to diagram limits (0% = lower edge)
	y-Axis;LOG;	Scaling of y axis linear (LIN) or logarithmic (LOG)
	Level Range;100;dB	Display range in in y direction. Unit: dB with x axis LOG, % with x axis LIN
	RF Att;20;dB	Input attenuation
	RBW;100000;Hz	Resolution bandwidth
	VBW;30000;Hz	Video bandwidth
	SWT;0.005;s	Sweep time
	Trace Mode;AVERAGE;	Display mode of trace: CLR/WRITE,AVERAGE,MAXHOLD,MINHOLD
	Detector;SAMPLE;	Detector set: AUTOPEAK,MAXPEAK,MINPEAK,AVERAGE, RMS,SAMPLE,QUASIPEAK
	Sweep Count;20;	Number of sweeps set
Data section of the file	Trace 1:;;	Selected trace
	x-Unit;Hz;	Unit of x values: Hz with span > 0; s with span = 0; dBm/dB with statistics measurements
	y-Unit;dBm;	Unit of y values: dB*/V/A/W depending on the selected unit with y axis LOG or % with y axis LIN
	Values;501;	Number of test points
	10000;-10.3;-15.7 10180;-11.5;-16.9 10360;-12.0;-17.4 ...;...;	Measured values: <x value>, <y1>, <y2> <y2> being available only with detector AUTOPEAK and containing in this case the smallest of the two measured values for a test point.

The *DECIM SEP* softkey selects the decimal separator between '.' (decimal point) and ',' (comma) with floating-point numerals for the function ASCII FILE EXPORT.
With the selection of the decimal separator different language versions of evaluation programs (eg MS-Excel) can be supported.

IEC/IEEE-bus command `FORM:DEXP:DSEP POIN`



The *COPY TRACE* softkey copies the screen contents of the current trace into another trace memory. The desired memory is selected by entering the number 1, 2 or 3.

Upon copying, the contents of the selected memory is overwritten and the new contents displayed in view mode.

IEC/IEEE-bus command `TRAC:COPY TRACE1,TRACE2`

Selection of Detector

The detectors of the FSP are implemented as pure digital devices. The detectors available are the peak detectors which determine the maximum and/or the minimum value from a number of samples, the rms detector which measures the power within a pixel, the average, the quasipeak and the sample detector. The sample detector routes through the sampled data without any modification or performs a data reduction by suppressing measured values that cannot be displayed.
The peak detectors compare the current level value with the maximum or minimum level from the previously sampled data. When the number of samples defined by the instrument setting is reached, the samples are combined in displayable pixels. Each of the 501 pixels of the display thus represents 1/500 of the sweep range and contains all single measurements (frequency samples) in this subrange in compressed form. For each trace display mode an optimized detector is selected automatically. Since peak detectors and sample detector are connected in parallel, a single sweep is sufficient for collecting all detector values for 3 traces.

Peak detectors
(*MAX PEAK* and *MIN PEAK*)

Peak detectors are implemented by digital comparators. They determine the largest of all positive (max peak) or the smallest of all negative (min peak) peak values of the levels measured at the individual frequencies which are displayed in one of the 501 pixels. This procedure is repeated for each pixel so that for wide frequency spans and despite the limited resolution of the display a large number of measurements can be taken into consideration for the display of the spectrum.

Autopeak detector

The *AUTOPEAK* detector combines the two peak detectors. The max peak detector and the min peak detector simultaneously determine the maximum and the minimum level within a displayed testpoint and display it as a single measured value. The maximum and minimum levels within a frequency point are connected by a vertical line.

Sample detector

The *SAMPLE* detector routes through the sampled data without any further evaluation and either displays them directly or, for reasons of speed in case of short sweep times, first writes them into a memory and processes them subsequently.
There is no data reduction, ie no summing up of measured values of neighbouring frequencies or time samples. If during a frequency sweep more measured values are obtained than can be displayed, measured values will be lost. This means that discrete signals might be lost.
The sample detector therefore can only be recommended for a span-to-resolution bandwidth ratio of up to approx. 250 in order to ensure that no signal will be suppressed (example: span 1 MHz, -> min. bandwidth 5 kHz).

RMS detector

The RMS detector forms the rms value of the measured values within a pixel.
To this effect, FSP uses the linear voltage after envelope detection. The sampled linear values are squared, summed and the sum is divided by the number of samples (= root mean square). For logarithmic display the logarithm is formed from the square sum. For linear display the root mean square value is displayed. Each pixel thus corresponds to the power of the measured values summed up in the pixel.
The rms detector supplies the power of the signal irrespective of the waveform (CW carrier, modulated carrier, white noise or impulsive signal). Correction factors as needed for other detectors for measuring the power of the different signal classes are not required.

Average detector

The average detector forms the average value of the measured values within a pixel.
To this effect, FSP uses the linear voltage after envelope detection. The sampled linear values are summed up and the sum is divided by the number of samples (= linear average value). For logarithmic display the logarithm is formed from the average value. For linear display the average value is displayed. Each pixel thus corresponds to the average of the measured values summed up in the pixel.
The average detector supplies the average value of the signal irrespective of the waveform (CW carrier, modulated carrier, white noise or impulsive signal).

Quasipeak detector

The quasipeak detector similates the behaviour of an analog voltmeter by evaluating the measured values in a pixel.
The quasipeak detector is especially designed for the requirements of EMC measurements and is used for evaluating pulse-shaped spurious.

Note: *During a frequency sweep, FSP increments the 1st local oscillator in steps that are smaller than approximately 1/10 of the bandwidth. This is to ensure that the signal level is correctly measured. For narrow bandwidths and wide frequency spans a very large number of measured values is thus obtained. The number of frequency steps, however, always is a multiple of 501 (= number of pixels that can be displayed). With the sample detector selected, only every n^{th} value is displayed. The value of n depends on the number of measured values, ie on the frequency span, the resolution bandwidth and the measurement rate.*

TRACE-DETECTOR submenu

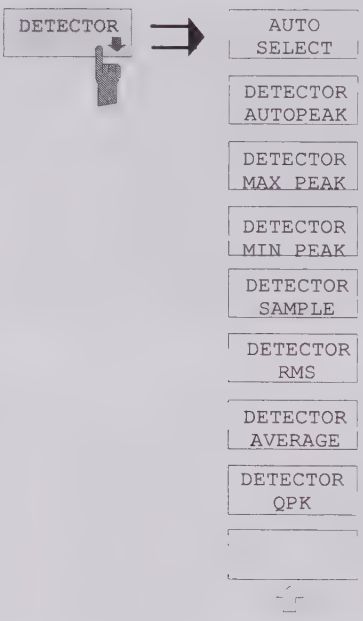

The *DETECTOR* softkey opens a submenu for selecting the detector for the selected trace. The softkey is highlighted if the detector is not selected with *AUTO SELECT*.

The detector can be selected independently for each trace. The *AUTO SELECT* mode selects the optimum detector for each display mode of the trace (Clear/Write, Max Hold or Min Hold).

The softkeys for the detectors are mutually exclusive selection keys.

The *AUTO SELECT* softkey (= default setting) selects the optimum detector for the set display mode of the trace (Clear/Write, Max Hold and Min Hold) and the selected filter mode (bandpass/FFT).

Trace display	**Detector (bandpass)**	**Detector (FFT)**
Clear/Write	Auto Peak	Max Peak
Average	Sample	Sample
Max Hold	Max Peak	Max Peak
Min Hold	Min Peak	Max Peak

The detector activated for the specific trace is identified in the respective trace display field as follows:

Detector	
Auto Peak	AP
Max Peak	PK
Min Peak	MI
Average	AV
RMS	RM
Sample	SA
Quasipeak	QP

IEC/IEEE-bus command `DET:AUTO ON`

The *DETECTOR AUTOPEAK* softkey activates the autopeak detector.

IEC/IEEE-bus command `DET APE`

The *DETECTOR MAX PEAK softkey* activates the max peak detector. It is recommended for measurement of impulsive signals.

IEC/IEEE-bus command `DET POS`

The *DETECTOR MIN PEAK* softkey activates the min peak detector. Weak sinewave signals become clearly visible in noise using this detector. In case of a composite signal made up of sinewave and impulsive signals, the impulsive signals are suppressed.

IEC/IEEE-bus command `DET NEG`

The *DETECTOR SAMPLE* softkey activates the sample detector.

It is used for measuring uncorrelated signals such as noise. The power can be determined with the aid of fixed correction factors for evaluation and the logarithmic function.

IEC/IEEE-bus command `DET SAMP`

The *DETECTOR RMS* softkey activates the rms detector.

The rms detector supplies the power of the signal independent of the waveform. For this effect the root mean square of all sampled level values is formed during the sweep of a pixel. The sweep time thus determines the number of averaged values and with increasing sweep time better averaging is obtained. The rms detector is thus an alternative for averaging over several sweeps (see TRACE AVERAGE).

Since the video bandwidth must be at least 10 times the resolution bandwidth (RBW) to ensure that video filtering does not invalidate the rms values of the signal, this ratio is set automatically upon activating the detector.

IEC/IEEE-bus command `DET RMS`

The *DETECTOR AVERAGE* softkey activates the average detector.

In contrast to the rms detector, the average detector supplies the linear average of all sampled level values during the sweep of a pixel.
The same relations as for the rms detector apply (see above).

IEC/IEEE-bus command `DET AVER`

The *DETECTOR QPK* softkey activates the quasipeak detector.

This detector evaluates the sampled level values during the sweep of a pixel like an analog voltmeter.
On switching the quasipeak detector on the video bandwidth is automatically set to 10 MHz so as to exclude the influence of the video filter on the signal evaluation.

IEC/IEEE-bus command `DET QPE`

Mathematical Functions for Traces

TRACE 1-TRACE MATH submenu:

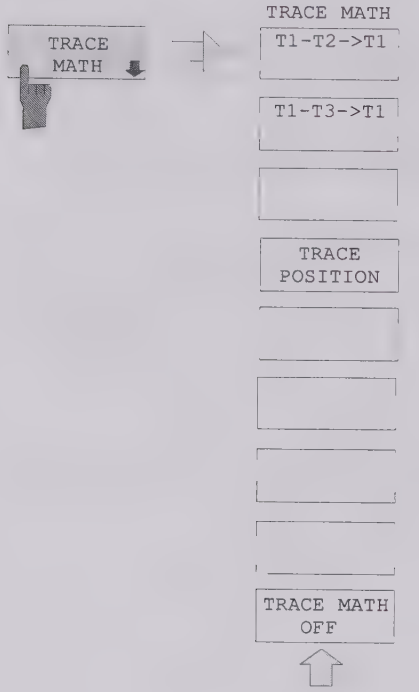

The *TRACE MATH* softkey opens a submenu in which the difference between the selected trace to trace 1 is calculated. The softkey is highlighted if a math function is activated.



The *T1-T2* and *T1-T3* softkeys subtract the corresponding traces. The result displayed is referred to the zero point defined by *TRACE POSITION*.

To indicate that the trace has been obtained by subtraction, the difference "1 - 2" or "1 - 3" is indicated on the trace info of trace 1 and in the *TRACE* main menu the *TRACE MATH* softkey is highlighted.

IEC/IEEE-bus command
```
CALC:MATH (TRACE1-TRACE2)
CALC:MATH (TRACE1-TRACE3)
```

The *TRACE POSITION* softkey activates the entry of the trace position for 0 difference. The position is stated in % of the diagram height.
The range of values extends from -100% to +200%

IEC/IEEE-bus command `DISP:MATH:POS 50PCT`



The *TRACE MATH OFF* softkey switches the math function off.

IEC/IEEE-bus command `CALC:MATH:STAT OFF`

Recording the Correction Data of FSP – *CAL* Key

The FSP obtains its high measurement accuracy through its inbuitl self-alignment method.

The correction data and characteristics required for the alignment are determined by comparison of the results at different settings with the known characteristics of the high-precision calibration signal source of FSP at 128 MHz. The correction data are then available in the instrument as a file and can be displayed by means of the *CAL RESULTS* softkey.
For service purposes the use of correction data can be deactivated by means of the *CAL CORR ON/OFF* softkey. If the correction data recording is aborted, the last complete correction data set is restored.

Note: *The term "Calibration" formerly used for the integrated self alignment was often mistaken for the "true" calibration of the instrument at the test set in production and in service. It is therefore no longer used although it appears in the abbreviated form in the name of keys ("CAL...").*

CAL menu:

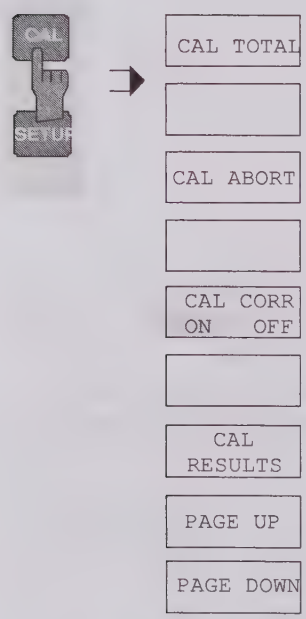

The *CAL* key opens a menu with the available functions for recording, displaying and activating the data for self alignment.



The *CAL TOTAL* softkey starts the recording of correction data of the instrument.

If the correction data recording has failed or if the correction values are deactivated (*CAL CORR = OFF* softkey), the status field indicates

UNCAL.

IEC/IEEE-bus command: `*CAL?`

The *CAL ABORT* softkey interrupts the recording of correction data and restores the last complete correction data set.

IEC/IEEE-bus command: `CAL:ABOR`

The *CAL CORR ON/OFF* softkey switches the calibration data on/off.

ON The status message depends upon the results of the total calibration.

OFF The message *UNCAL* appears in the status line.

IEC/IEEE-bus command: `CAL:STAT ON`



The *CAL RESULTS* softkey calls the *CALIBRATION RESULTS* table, which shows the correction data found during calibration.

The *CALIBRATION RESULTS* table contains the following information:

- date and time of last record of correction valuesKorrekturwertaufnahme
- overall results of correction value record
- list of found correction values according to function/module

The results have the following meaning:

PASSED calibration successful without any restrictions

CHECK deviation of correction value larger than expected, correction could however be performed

FAILED deviations of correction value too large, no correction was possible. The found correction data are not valid.

ABORTED calibration aborted

CALIBRATION RESULTS

```
Calibration: PASSED
Date:        05.Jun 1999 16:24:54

Total GAIN Adjust              PASSED
Calibration of IF Filters      PASSED
Bandwidth:
Filter   Cal Val [Hz] DAC Val State

100kHz    1.804e+03    3698   PASSED
300kHz    8.417e+03    3516   PASSED
  1MHz    2.806e+04    2881   PASSED
  3MHz    1.804e+03    3698   PASSED
 10MHz    8.417e+03    3516   PASSED
```

IEC/IEEE-bus command: `CAL:RES?`





The softkeys *PAGE UP* and *PAGE DOWN* scroll one page forward or backward in the *CALIBRATION RESULTS* table. They have no function when the table is closed.

IEC/IEEE-bus command: --

Markers and Delta Markers – *MKR* Key

The markers are used for marking points on traces, reading out measurement results and for quickly selecting a display section. FSP provides four markers per display window. All markers can be used either as markers or delta markers. The availability of marker functions depends on whether the measurement is performed in the frequency, time or level domain.
The marker that can be moved by the user is defined in the following as the **active marker**.
Examples of marker display:

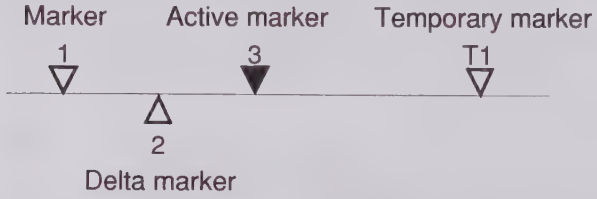

Temporary markers are used in addition to the markers and delta markers to evaluate the measurement results. They disappear when the associated function is deactivated.
The measurement results of the active marker (also called **marker values**) are displayed in the marker field. The marker info field at the upper right of the display shows the marker location (here, frequency), the level and the currently selected trace [T1].



The *MKR* key calls a menu that contains all marker and delta marker standard functions. If no marker is active, *MARKER 1* will be enabled and a peak search on the trace carried out. Otherwise, the data entry for the marker activated last is opened.

MKR menu:

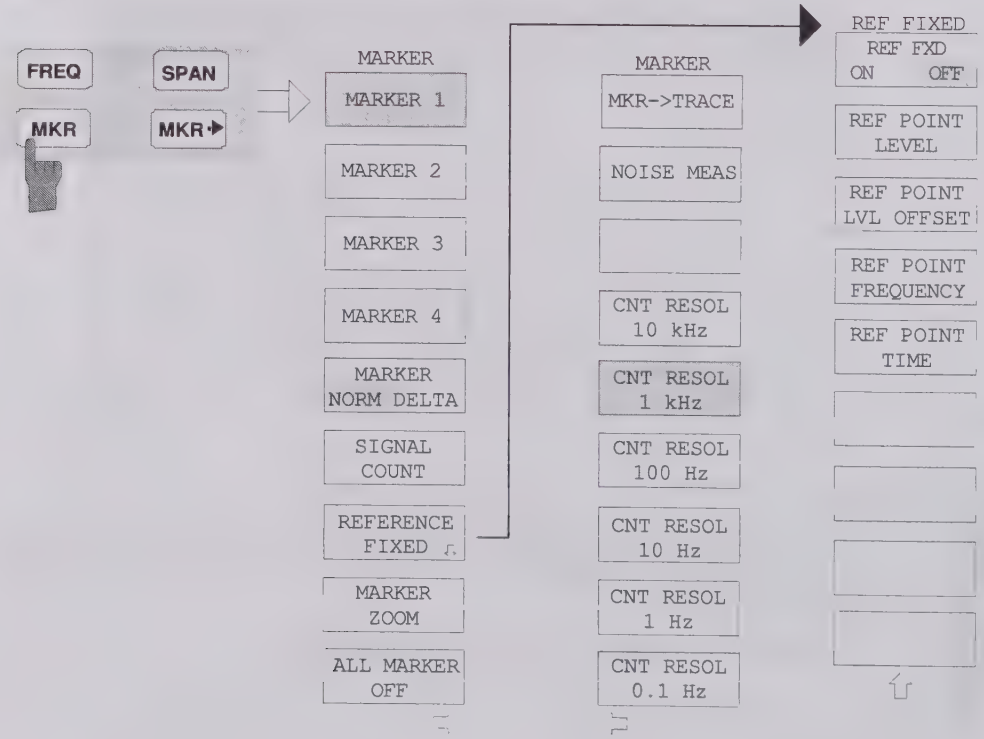



The *MARKER 1/2/3/4* .softkey selects the corresponding marker and activates it.

MARKER 1 is always the normal marker. After they have been switched on, *MARKERS 2 to 4* are delta markers that refer to *MARKER 1*. These markers can be converted into markers with absolute value display by means of the *MARKER NORM DELTA* softkey. When *MARKER 1* is the active marker, pressing the M*ARKER NORM DELTA* softkey switches on an additional delta marker.

Pressing the *MARKER 1 to 4* softkey again switches off the selected marker.

Example:

[PRESET] FSP is set to the default setting.

[MKR] On calling the menu, *MARKER 1* is switched on ('1' highlighted in the softkey) and positioned on the maximum value of the trace. It is a normal marker and the *MARKER NORMAL* softkey is highlighted.

[*MARKER 2*] *MARKER 2* is switched on ('2' highlighted in the softkey). It is automatically defined as a delta marker on switching on so the *DELTA* is is highlighted on softkey *MARKER NORM DELTA*. The frequency and level of *MARKER 2* with reference to *MARKER 1* are output in the marker info field.

[MARKER NORM DELTA] The *MARKER NORM DELTA* softkey is highlighted. *MARKER 2* becomes a normal marker. The frequency and level of *MARKER 2* are output as absolute values in the marker info field.

[MARKER 2] *MARKER 2* is switched off. *MARKER 1* is the active marker for entry. The frequency and level of *MARKER 1* are output in the marker info field.

IEC/IEEE-bus command:

```
CALC:MARK ON;
CALC:MARK:X <value>;
CALC:MARK:Y?

CALC:DELT ON;
CALC:DELT:MODE ABS|REL
CALC:DELT:X <value>;
CALC:DELT:X:REL?
CALC:DELT:Y?
```

When several traces are being displayed, the marker is set to the maximum value (peak) of the active trace which has the lowest number (1 to 3). In case a marker is already located there, it will be set to the frequency of the next lowest level (next peak).

When the split-screen display mode is active, the marker will be placed in the active window. A marker can only be enabled when at least one trace in the corresponding window is visible.

If a trace is turned off, the corresponding markers and marker functions are also deactivated. If the trace is switched on again (*VIEW*, *CLR/WRITE*;..), the markers along with coupled functions will be restored to their original positions provided the markers have not been used on another trace.



The *MKR→TRACE* softkey places the marker on a new trace. The trace is selected via a data entry field. Only those traces can be selected which are visible on the screen in the same window.

Example:
Three traces are presented on the screen. The marker is always on Trace 1 on switching on.

[MKR ->TRACE]
"2"<ENTER> The marker jumps to Trace 2 but remains on the previous frequency or time.

[MKR ->TRACE]
"3"<ENTER> The marker jumps to Trace 3. '

IEC/IEEE-bus command:
```
CALC:MARK1:TRAC 1
CALC:DELT:TRAC 1
```

Frequency Measurement with the Frequency Counter

In order to accurately determine the frequency of a signal, FSP is equipped with a frequency counter which measures the frequency of the RF signal at the intermediate frequency. Using the measured IF, FSP calculates the frequency of the RF input signal by applying the known frequency conversion factors.

The frequency measurement error depends only upon the accuracy of the frequency standard used (external or internal reference). Although FSP always operates synchronously irrespective of the set span, the frequency counter delivers a more exact result than a measurement performed with a marker. This is due to the following:

- The marker measures only the position of the pixel on the trace and infers the frequency of the signal from this value. The trace, however, contains only a limited number of pixels. Depending upon the selected span, each pixel may contain many measurement values, which therefore limits the frequency resolution.
- The resolution with which the frequency can be measured is proportional to the measurement time. For this reason, the bandwidth is normally made as wide as possible and the sweep time as short as possible. This results in a loss of frequency resolution.

For the measurement with the frequency counter, the sweep is stopped at the reference marker, the frequency is counted with the desired resolution and then the sweep is allowed to continue.



The *SIGNAL COUNT* softkey switches the frequency counter on/off.

The frequency is counted at the position of the reference marker (*MARKER* 1). The sweep stops at the reference marker until the frequency counter has delivered a result. The time required for a frequency measurement depends on the selected frequency resolution. The resolution is set in the side menu.

If no marker is enabled when the *SIGNAL COUNT* softkey is pressed, *MARKER 1* is switched on and set at the largest signal.

In addition, the *SIGNAL COUNT* function is displayed in the marker info field on the screen with [Tx CNT].



Switching the *SIGNAL COUNT* function off is accomplished by pressing the softkey again.

IEC/IEEE-bus command:
```
CALC:MARK1:COUN ON;
CALC:MARK:COUN:FREQ?
```

MARKER NEXT menu

The resolution of the frequency counter is set in the *NEXT* menu of the MARKER menu. FSP offers counter resolutions between 0.1 Hz and 10 kHz.

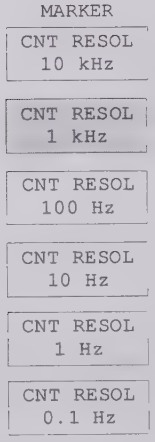

The *CNT RESOL ...* softkeys select the counter resolution. They are selection switches, i.e. only one of the can be active at any one time.
The marker stop time, ie the frequency measurement time, depends on the selected resolution.

IEC/IEEE-bus command:
```
CALC:MARK1:COUN:RES <value>
```

Measurement example:
The frequency of a CW signal is to be determined by means of the frequency counter with a resolution of 10 Hz.

[**PRESET**]	FSP is set to the default setting.
[**MARKER**]	*MARKER 1* is switched on and set to the maximum value of the displayed spectrum.
[*SIGNAL COUNT*]	The frequency counter is switched on. FSP counts the frequency of the signal at the marker position with a resolution of 1 kHz. The counted frequency is indicated in the marker info field.
[*NEXT*]	Changes to the submenu for setting the counter resolution.
[*CNT RESOL 10 Hz*]	The frequency counter resolution is increased to 10 Hz.

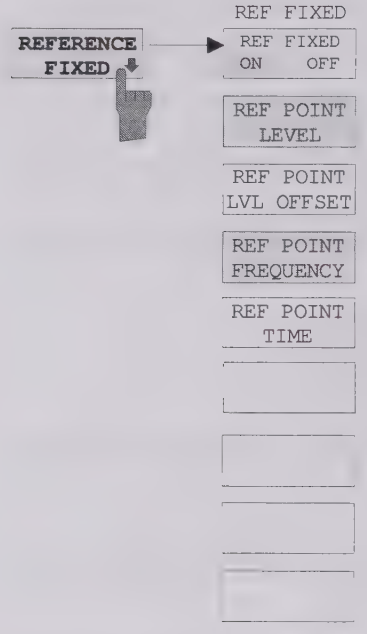

The *REFERENCE FIXED* softkey defines the level and the frequency or time of *MARKER 1* as a reference for one or several delta markers. The measured values for one or several markers displayed in the marker info field are derived from this reference point instead of the current values of the reference marker (*MARKER* 1).

On actuating the softkey, reference fixed is switched on and thus, the level value and the frequency, time or x-level value of *MARKER 1* immediately become the reference point.

Additionally, the *REFERENCE FIXED* softkey opens the submenu where it is possible to determine manually a reference point with level and frequency, time or x-axis level, to define a level offset or deactivate the reference point.

The *REFERENCE FIXED* function is useful for the measurement of the harmonic suppression at small span (fundamental not represented).



The *REF FXD ON/OFF* softkey switches on or off the relative measurement to a fixed reference value (*REFERENCE POINT*) independent of the trace.

IEC/IEEE-bus command: `CALC:DELT2:FUNC:FIX ON`



The *REF POINT LEVEL* softkey enters a reference level independent of the reference marker level. All relative level values of the delta markers refer to this reference level.

IEC/IEEE-bus command:

```
CALC:DELT2:FUNC:FIX:RPO:Y -10dBm
```



The *REF POINT LVL OFFSET* softkey specifies a level offset relevant to the reference level. The relative level values of the delta markers refer to the reference point level plus the level offset.

The level offset is set to 0 dB on enabling the *REFERENCE FIXED* or *PHASE NOISE* function.

IEC/IEEE-bus command:

```
CALC:DELT2:FUNC:FIX:RPO:Y:OFFS 0dB
```



With the *REF POINT FREQUENCY* softkey a reference frequency can be manually activated for the delta markers when the *REFERENCE FIXED* or *PHASE NOISE* function is used.

IEC/IEEE-bus command:

```
CALC:DELT2:FUNC:FIX:RPO:X 10.7MHz
```

The *REF POINT TIME* softkey activates the entry box for the input of a reference time for the *REFERENCE FIXED* function in the time domain (span = 0 Hz).

IEC/IEEE-bus command:

```
CALC:DELT2:FUNC:FIX:RPO:X 5MS
```

For phase noise measurement, input of reference time is not possible.

The *REF POINT x-LEVEL* softkey activates the entry box for the input of a reference level on the x-axis for the *REFERENCE FIXED* function when the power sweep is active.

IEC/IEEE-bus command:

```
CALC:DELT2:FUNC:FIX:RPO:X -5DBM
```

Measurement example:
Small-span harmonics measurement to increase sensitivity
CW signal (eg 100 MHz, 0 dBm) with harmonics at the RF input of FSP.

[**PRESET**]	FSP is set to the default setting.
[**CENTER**: 100 **MHz**]	The center frequency of FSP is set to 100 MHz.
[**SPAN**: 1 **MHz**]	The span is set to 1 MHz.
[**AMPL**: 3 **dBm**]	The reference level is set to 3 dBm (3 dB above the expected RF level).
[**MKR**]	*MARKER* 1 is switched on ('1' highlighted in the softkey) and set to the signal peak.
[*MARKER 2*]	*MARKER 2* is switched on and automatically defined as the delta marker (*DELTA* is highlighted on *MARKER NORM DELTA* softkey).
[*REFERENCE FIXED*]	The frequency and level of *MARKER 1* are a reference for the delta marker.
[**CENTER**: 200 **MHz**]	The center frequency is set to 200 MHz (= frequency of the 2nd harmonic). The reference level may have to be reduced to see the 2nd harmonic from the noise. This does not affect the reference level set with *REFERENCE FIXED*.
[**MKR->**: *PEAK*]	The delta marker jumps to the 2nd harmonic of the signal. The level spacing of the harmonic to the fundamental is displayed in the marker info field.

The *MARKER ZOOM* softkey expands the area around MARKER 1. With the zoom function, more details of the spectrum can be seen. The desired display range can be defined in an entry window.
The following sweep is stopped at the position of the reference marker. The frequency of the signal is counted and the measured frequency becomes the new center frequency. The zoomed display range is then configured and the new settings are used by FSP for further measurements.

As long as switching to the new frequency display range has not yet taken place, pressing the softkey will abort the procedure.

If *MARKER 1* is not active when the softkey is pressed, it is automatically activated and set to the highest peak in the window.

If an instrument setting is changed after selection of *MARKER ZOOM*, the function is aborted.

The *MARKER ZOOM* softkey is only available in the frequency domain (span > 0).

IEC/IEEE-bus command: `CALC:MARK1:FUNC:ZOOM 1kHz`

The *ALL MARKER OFF* softkey switches off all markers (reference and delta markers). It also switches off all functions and displays associated with the markers/delta markers.

IEC/IEEE-bus command: `CALC:MARK:AOFF`

Marker Functions – *MKR FCTN* Key

The MKR FCTN menu offers further measurements with the markers:

- Measurement of noise density (*NOISE MEAS* softkey)
- Measurement of phase noise (*PHASE NOISE* softkey)
- Measurement of filter or signal bandwidth (*N DB DOWN* softkey)
- Activating of AF demodulation (*MARKER DEMOD* softkey)

On calling the menu, the entry for the last active marker is activated (*SELECT MARKER* softkey); if no marker is activated, marker 1 is activated and a maximum search (*PEAK* softkey) is performed. The marker can be set to the desired trace by means of *MKR -> TRACE* softkey.

Menu *MKR FCTN*:

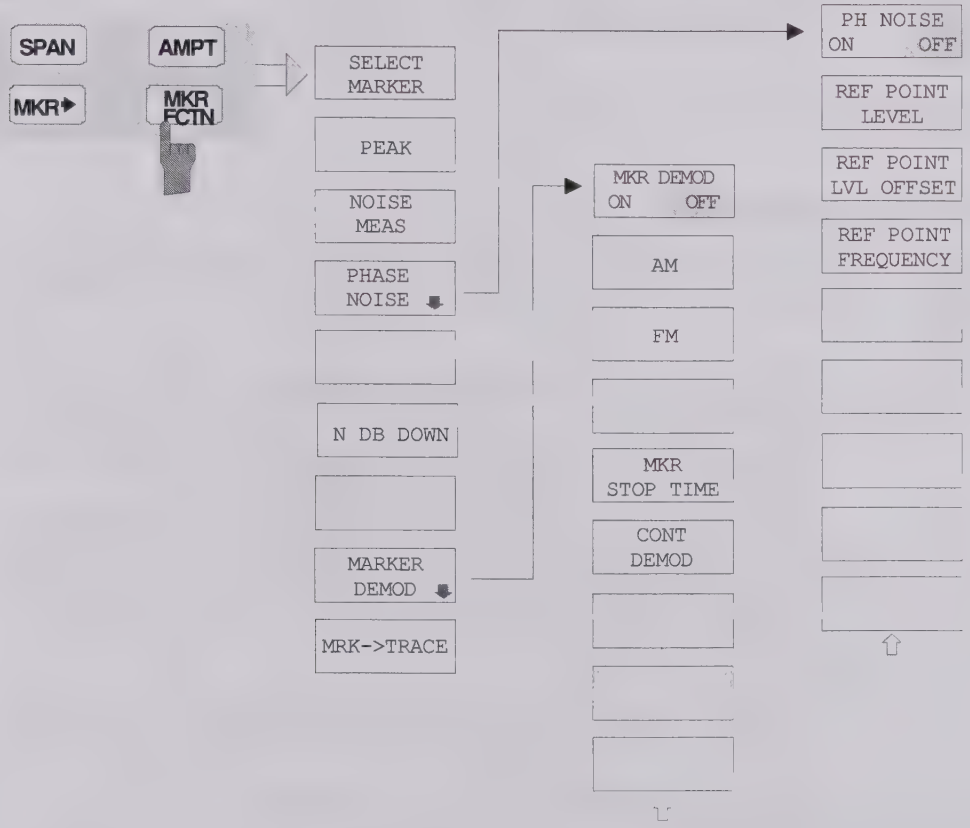

Activating the Markers

Menu *MKR FCTN*:

The *SELECT MARKER* softkey activates the numerical selection of the marker in the data entry field. Delta marker 1 is selected by input of ' 0 '.
If the marker is switched off, then it is switched on and can be moved later on.

IEC/IEEE-bus command:
```
CALC:MARK1 ON;
CALC:MARK1:X <value>;
CALC:MARK1:Y?
```

The *PEAK* softkey sets the active marker/delta marker to the peak of the trace.

IEC/IEEE-bus command:
```
CALC:MARK1:MAX
CALC:DELT1:MAX
```

Measurement of noise density



The *NOISE MEAS* softkey switches the noise measurement for the active marker on or off. The corresponding marker becomes the *NORMAL* marker.

During noise measurement, the noise power density is measured at the position of the marker. In the time domain mode, all points of the trace are used to determine the noise power density. When measurements are performed in the frequency domain, two points to the right and left of the marker are used for the measurement to obtain a stable result.
The noise power density is indicated in the marker field. With a logarithmic amplitude units (dBm, dBmV, dBmµV, dBµA, dBpT) the noise power density is output in dBm/Hz ie as level in 1 Hz bandwidth with reference to 1 mW. With linear amplitude units (V, A, W) the noise voltage density is evaluated in µV/√Hz, the noise current density in µA/√Hz or the noise power density in µW/Hz.

The following settings have to be made to ensure that the power density measurement yields correct values:

Detector: Sample or RMS

Video bandwidth:

≤	0.1	x	resolution bandwidth with sample detector (corresponds to RBW / VBW NOISE)
≥	3	x	resolution bandwidth with RMS detector (corresponds to RBW / VBW SINE)

In the default setting, FSP uses the sample detector for the noise function.

With the sample detector, the trace can additionally be set to AVERAGE to stabilize the measured values. With RMS detector used, trace averaging must not be used since in this case it produces too low noise levels which cannot be corrected. Instead, the sweep time can be increased to obtain stable measurement results.

The FSP uses the following correction factors to evaluate the noise density from the marker level:

- Since the noise power is indicated with reference to 1 Hz bandwidth, the bandwidth correction value is deducted from the marker level. It is 10 x lg (1Hz/BW_{Noise}), where BW_{Noise} is the noise or power bandwidth of the set resolution filter (RBW).

Sample detector:

- As a result of video filter averaging and trace averaging, 1.05 dB is added to the marker level. This is the difference between the average value and the rms value of white noise.
- With a logarithmic level axis, 1.45 dB is added additionally. Logarithmic averaging is thus fully taken into account which yields a value that is 1.45 dB lower than that of linear averaging.

RMS detector:

- With the exception of bandwidth correction, no further corrections are required for the RMS detector since it already indicates the power with every point of the trace.

To allow a more stable noise display the adjacent (symmetric to the measurement frequency) points of the trace are averaged.

In time domain mode, the measured values are averaged versus time (after a sweep).

IEC/IEEE-bus command:
```
CALC:MARK:FUNC:NOIS ON;
CALC:MARK:FUNC:NOIS:RES?
```

Example: Measurement of inherent FSP noise

[**PRESET**] FSP is set to default setting.

[**MARKER**] Marker 1 is switched on and set to the maximum value of the displayed spectrum. Set marker to desired frequency using the rotary knob.

[***NOISE***] The FSP switches the sample detector on and sets the video bandwidth to 300 kHz (0.1 x RBW). The power density level of inherent noise is displayed in dBm/Hz in the marker info field.

Note: *The FSP noise figure can be calculated from the measured power density level. It is calculated by deducting the set RF attenuation (RF Att) from the displayed noise level. 174 is to be added to the result to obtain the FSP noise figure.*

Phase Noise Measurement

Menu MKR FCTN:

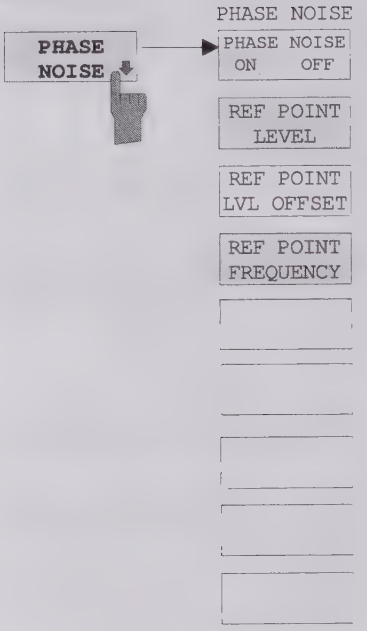

The *PHASE NOISE* softkey switches the *PHASE NOISE* function on/off. Additionally, the softkey opens the submenu for manually setting the reference point. The phase noise measurement can be switched off in the submenu.

MARKER 1 (= reference marker) is used as a reference for the phase noise measurement. The frequency and level of the reference marker are used as fixed reference values, ie the *REFERENCE FIXED* function is activated. After switching on the phase noise measurement the reference level or the center frequency can thus be set in a way that the carrier is outside the displayed frequency range, or, for example, a notch filter is switched on to suppress the carrier.
A noise power density measurement is carried out with the delta marker or delta markers. This measurement corresponds to the NOISE function in the *MARKER* menu (MKR). The result of the phase noise measurement is the difference in level between the reference point and the noise power density.

The following possibilities can be selected on switching on *PHASE NOISE*:

1. No marker enabled:

[**MKR FCTN**]	*MARKER 1* is enabled and set to peak.
[*PHASE NOISE*]	*MARKER 1* becomes the reference marker, *MARKER 2* the delta marker; frequency = frequency of the reference marker. The delta marker is the active marker, ie it can be moved with the rollkey or adjusted by entering numerals. The *PHASE NOISE* function is switched on and the measured value is output.

2. Markers are enabled:

[**MKR FCTN**]	The previous marker configuration remains unchanged.
[*PHASE NOISE*]	*MARKER* 1 becomes the reference marker. If other markers are enabled, they become delta markers and measure the phase noise at their respective positions.

If further markers are enabled during the phase noise measurement, they automatically become delta markers and measure the phase noise at their respective positions.

When the phase noise measurement is switched off, the marker configuration remains unchanged and the delta markers measure the relative level to the reference marker (*MARKER 1*).

The *PHASE NOISE* function measures the noise power at the delta markers referred to 1 Hz bandwidth. The sample detector is automatically used and the video bandwidth set to 0.1 times the resolution bandwidth (RBW). The two settings are taken into account in the correction values used for the noise power measurement.
To obtain stable results, two pixels on the right and the left of the respective delta marker position are taken for the measurement. The procedure for determining the noise power is identical to the method used for the noise power measurement (see NOISE softkey). The measured noise level referred to 1 Hz bandwidth is subtracted from the carrier level at the reference marker (*MARKER 1*). The measured values are displayed in the delta marker field in dBc/Hz (= spacing in dB of the noise power from the carrier level in 1 Hz bandwidth).

If several delta markers are enabled, only the value read by the active marker is shown in the marker field. If several delta markers are active, their measurement results are shown in the marker info field.

The reference value for the phase noise measurement can be defined with *REF POINT LEVEL*, *REF POINT FREQUENCY* and *REF POINT LVL OFFSET* to differ from that of the reference marker.

IEC/IEEE-bus command: --



The *PH NOISE ON/OFF* softkey switches on/off the phase noise measurement. Switching on is performed by means of the *PHASE NOISE* softkey and is only necessary when the phase noise measurement has been switched off in the submenu.

IEC/IEEE-bus command:
```
CALC:DELT1:FUNC:PNO ON
CALC:DELT1:FUNC:PNO:RES?
```



The *REF POINT LEVEL* softkey activates an entry box for the input of a reference level other than the reference marker level. The function is identical to that of the softkey with the same name in the marker menu (MKR).

IEC/IEEE-bus command:
```
CALC:DELT1:FUNC:FIX:RPO:Y -10dB
```



The *REF POINT LVL OFFSET* softkey activates an entry box for the input of an additional level offset for the phase noise calculation.

This level offset is set to 0 dB on when the *REFERENCE FIXED* or *PHASE NOISE* function is enabled.

IEC/IEEE-bus command:
```
CALC:DELT:FUNC:FIX:RPO:Y:OFFS 10dB
```



The *REF POINT FREQUENCY* softkey activates an entry box for the manual input of a reference frequency for the *REFERENCE FIXED* or *PHASE NOISE* function.

IEC/IEEE-bus command:

```
CALC:DELT1:FUNC:FIX:RPO:X 10.7MHz
```

Measurement example:

The phase noise of a CW signal at 100 MHz with 0 dBm level is to be measured at 800 kHz from the carrier

[**PRESET**]	FSP is set to the default setting.
[**CENTER**: 100 **MHz**]	The center frequency is set to 100 MHz.
[**SPAN**: 2 **MHz**]	The span is set to 2 MHz.
[**AMPT**: 0 **dBm**]	The reference level is set to 0 dBm.
[**MKR FCTN**]	*MARKER 1* is switched on and positioned at the maximum of the displayed trace.
[*PHASE NOISE*: 800 **kHz**]	The phase noise measurement is switched on. The delta marker is positioned on the main marker and the measured phase noise value is displayed in the marker info field. The sample detector is used and the video bandwidth is set to 0.1 x RBW. When the phase noise measurement function is enabled, the entry of the delta marker frequency is activated. It can be entered directly.

Measurement of the Filter or Signal Bandwidth

Menu *MKR FCTN*:



The *N dB DOWN* softkey activates the temporary markers T1 and T2 which are n dB below the active reference marker. Marker T1 is placed to the left and marker T2 at the right of the reference marker. The value n can be input in a window.

The default setting is 3 dB.

The frequency spacing of the two temporary markers is indicated in the marker info field.
If, for example, it is not possible to form the frequency spacing for the n dB value because of the noise display, dashes are indicated instead of a measured value.

IEC/IEEE-bus command:

```
CALC:MARK1:FUNC:NDBD:STAT ON
CALC:MARK1:FUNC:NDBD 3dB
CALC:MARK1:FUNC:NDBD:RES?
CALC:MARK1:FUNC:NDBD:FREQ?
```

AF Demodulation

The FSP provides demodulators for AM and FM signals when equipped with Option AF-Demodulator (FSP-B3). With these demodulators, a displayed signal can be identified acoustically through the use of the internal loudspeaker or with headphones. The frequency at which the demodulation is enabled is coupled to the markers. The sweep stops at the frequency determined by the active marker for the selected time and the RF signal is demodulated. During a measurement in the time domain (span = 0 Hz) the demodulation is continuously on.
The threshold line (*MKR->SEARCH LIMITS:THRESHOLD*) performs a squelch function in the demodulator. If the threshold is set, the FSP LF demodulation is switched on only when the signal to be demodulated exceeds the set threshold.

Menu *MKR FCTN*:

The *MARKER DEMOD* softkey switches on the audio demodulator and calls a submenu in which the demodulation mode and the duration of the demodulation can be selected.

IEC/IEEE-bus command: `CALC:MARK1:FUNC:DEM ON`



The *MKR DEMOD ON/OFF* softkey switches the demodulation on/off.

In the frequency range (span >0), the frequency scan is stopped at the frequency of the active marker with demodulation switched on – provided that the level is above the threshold line - and the signal is demodulated during the given stop time.
In the time domain (span = 0) demodulation is continuous, ie not only active at the marker position.

IEC/IEEE-bus command: `CALC:MARK1:FUNC:DEM ON`

The *MKR STOP TIME* softkey defines the stop time for demodulation at the marker or markers.

FSP stops the sweep at the marker or markers for the duration of the defined stop time and then switches the demodulation on (see also *MKR DEMOD ON/OFF*).

IEC/IEEE-bus command: `CALC:MARK1:FUNC:DEM:HOLD 3s`

The softkeys *AM and FM* are selector switches one of which only may be active at a time. They set the desired demodulation mode FM or AM. Default setting is AM.

IEC/IEEE-bus command: `CALC:MARK1:FUNC:DEM:SEL AM`
`CALC:MARK1:FUNC:DEM:SEL FM`

The *MKR STOP TIME* softkey defines the stop time for demodulation at the marker(s).
The FSP interrupts the frequency sweep at the marker position and activates the demodulation for the duration of the stop time (see also *MKR DEMOD ON/OFF*).
In the time domain (span = 0) the demodulation is continuously active irrespective of the stop time set.

IEC/IEEE-bus command: `CALC:MARK1:FUNC:DEM:HOLD 3s`



The *CONT DEMOD* softkey switches on the continuous demodulation in the frequency domain. If the sweep time is long enough, the set frequency range can be monitored acoustically.

IEC/IEEE-bus command: `CALC:MARK1:FUNC:DEM:CONT ON`

Selecting the Trace

Menu *MKR FCTN*:

The *MKR→TRACE* softkey sets the active marker to different traces. Only those traces can be selected which are visible on the screen in the same window.

The function of the softkey is identical to that of the softkey with the same name in the MKR-> menu.

Example:
Three traces are displayed on the screen. The marker is always on Trace 1 on switching on.

[*MKR ->TRACE*]
"1"<ENTER> The marker jumps to Trace 2, but remains at the previous frequency or time.

[*MKR ->TRACE*]
"3"<ENTER> The marker jumps to Trace 3.

IEC/IEEE-bus command: `CALC:MARK:TRAC 2`

Change of Settings via Markers – *MKR* ⇒ Key

The *MKR →* menu offers functions through which instrument parameters can be changed with the aid of the currently active marker. The functions can be used on markers and delta markers.

On opening the menu, the entry for the last active marker is activated; if no marker was enabled, *MARKER 1* is activated and a peak search is performed.

MKR → menu

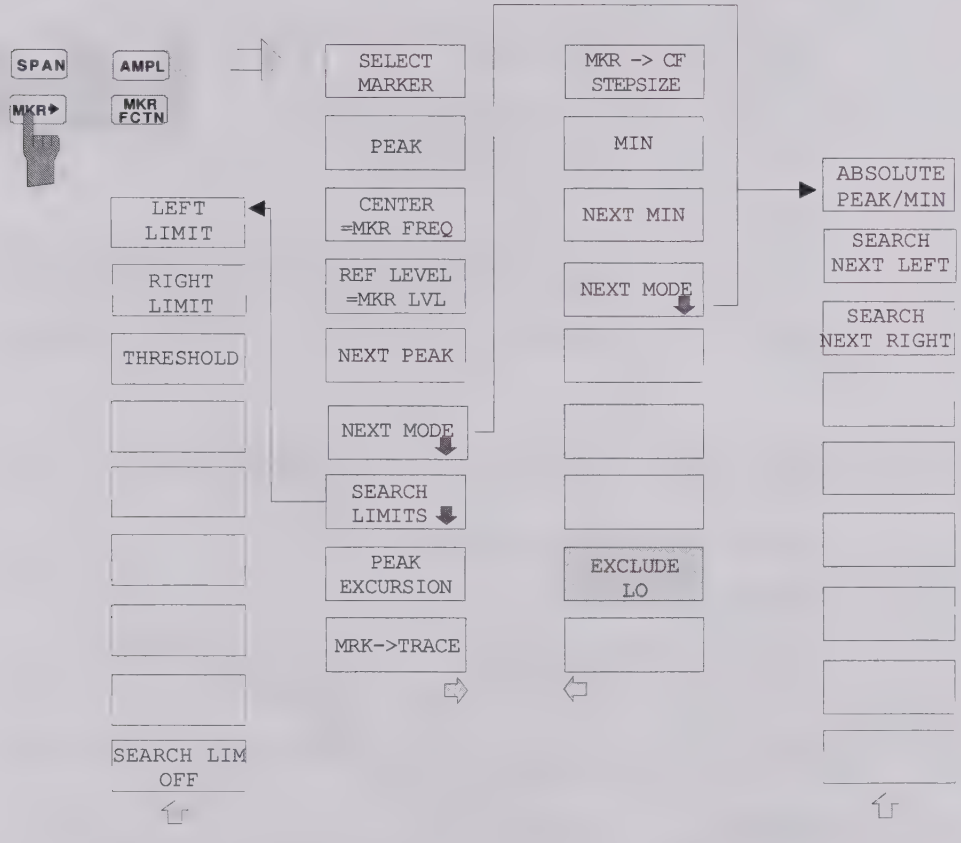

The *SELECT MARKER* softkey activates the numerical selection of the marker in the data entry field. Delta marker 1 is selected by input of ' 0 '.

IEC/IEEE-bus command:
```
CALC:MARK1 ON;
CALC:MARK1:X <value>;
CALC:MARK1:Y?
```



The *PEAK* softkey sets the active marker or delta marker to the peak of the trace.
If no marker is active when **MKR->** menu is called, *MARKER 1* is automatically switched on and the peak search is performed.

IEC/IEEE-bus command:
```
CALC:MARK:MAX
CALC:DELT:MAX
```



The *CENTER = MKR FREQ* softkey sets the center frequency to the current marker or delta marker frequency.
A signal can thus be set to the center of the frequency display range, for example, so that it can then be examined in detail with a smaller span.

The softkey is not available in the time domain (zero span).

IEC/IEEE-bus command: `CALC:MARK:FUNC:CENT`

Example:

A spectrum is displayed with a large span after PRESET. A signal off the center is to be examined in detail:

[**PRESET**]	FSP is set to the default setting.
[**MKR->**]	*MARKER 1* is switched on and automatically jumps to the largest signal of the trace.
[*CENTER =MKR FREQ*]	The center frequency is set to the marker frequency. The span is adapted in such a way that the minimum frequency (= 0 Hz) or the maximum frequency is not exceeded.
[*SPAN*]	The span can, for example, be reduced using the rollkey.

The *REF LEVEL = MKR LVL* softkey sets the reference level to the current marker level.

IEC/IEEE-bus command: `CALC:MARK:FUNC:REF`

Example:

A spectrum is displayed with a large span after PRESET. A signal off the center is to be examined in detail:

[**PRESET**]	FSP is set to the default setting.
[**MKR->**]	*MARKER 1* is switched on and automatically jumps to the largest signal of the trace.
[*CENTER =MKR FREQ*]	The center frequency is set to the marker frequency. The span is adapted in such a way that the minimum frequency (= 0 Hz) or the maximum frequency is not exceeded.
[*REF LEVEL = MKR LVL*]	The reference level is set to the measured marker level.
[**SPAN**]	The span can, for example, be reduced using the rollkey.



The *NEXT PEAK* softkey sets the active marker/delta marker to the next lower peak value on the trace. The search direction is defined in the *NEXT MODE* submenu (see below).

IEC/IEEE-bus command: `CALC:MARK:MAX:NEXT`
`CALC:DELT:MAX:NEXT`

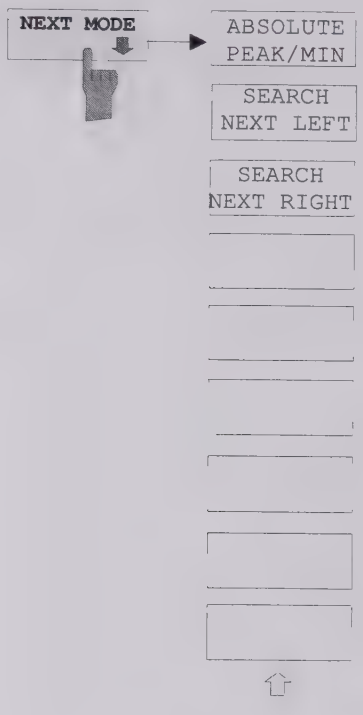

The *NEXT MODE* softkey opens a sub menu for definition of the search direction for *NEXT PEAK and NEXT MIN.*

The softkeys are selection switches, ie only one of them can be active at any one time.

The *ABSOLUTE PEAK/MIN* softkey defines that the next higher maximum or minimum is searched for on the whole trace.

IEC-Bus-Befehle:

```
CALC:MARK:MAX:NEXT
CALC:DELT:MAX:NEXT
CALC:MARK:MIN:NEXT
CALC:DELT:MIN:NEXT
```

The *SEARCH NEXT LEFT* softkey defines that the next higher maximum or minimum on the left of the active marker is searched for, ie only frequencies or time values smaller than the current marker frequency or time are taken into account.

IEC-Bus-Befehle:

```
CALC:MARK:MAX:LEFT
CALC:DELT:MAX:LEFT
CALC:MARK:MIN:LEFT
CALC:DELT:MIN:LEFT
```

The *SEARCH NEXT RIGHT* softkey defines that the the next higher maximum or minimum on the right of the active marker is searched for, ie only frequencies or time values higher than the current marker frequency or time are taken into account.

IEC-Bus-Befehle:

```
CALC:MARK:MAX:RIGH
CALC:DELT:MAX:RIGH
CALC:MARK:MIN:RIGH
CALC:DELT:MIN:RIGH
```

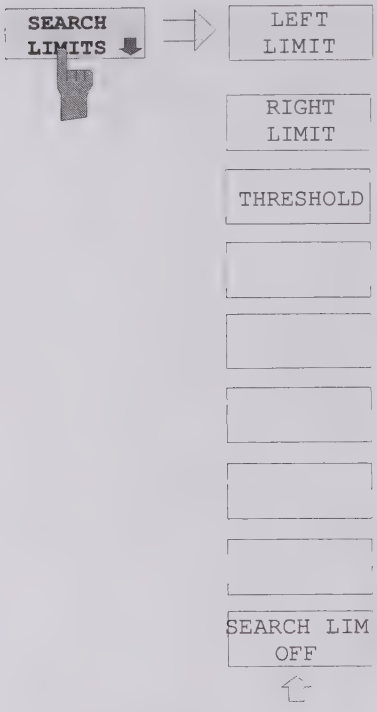

The *SEARCH LIMITS* softkey limits the search range for maximum or minimum search. The softkey switches to a submenu in which the search range limits can be set in the x and y direction.



The *LEFT LIMIT* und *RIGHT LIMIT* softkeys define the two vertical lines SL1 and SL2. The search is performed between these lines in the frequency and time domain
If only one line is enabled, line SL1 is the lower limit and the upper limit corresponds to the stop frequency. If SL2 is also enabled, it determines the upper limit.

IEC/IEEE-bus command:
```
CALC:MARK:X:SLIM:LEFT 1MHZ
CALC:MARK:X:SLIM:RIGH 10MHZ
CALC:MARK:X:SLIM ON
```



The *THRESHOLD* softkey defines the threshold line.
The threshold line represents a limit for the level range of the max. search at the lower end and that of the min. search at the upper end.

IEC/IEEE-bus command:
```
CALC:THR -20dBm
CALC:THR ON
```



The *SEARCH LIMIT OFF* softkey disables all limits of the search range.

IEC/IEEE-bus command:
```
CALC:MARK:X:SLIM OFF
CALC:THR OFF
```

The *PEAK EXCURSION* softkey activates an entry box for selecting the minimum amount by which a signal level must decrease/increase before it is recognized by the *NEXT PEAK* and *NEXT MIN* search functions as a maximum or minimum.

Input values from 0 to 80 dB are allowed, the resolution being 0.1 dB.

IEC/IEEE-bus command: `CALC:MARK:PEXC 10dB`

The peak excursion is preset to 6 dB. This is sufficient for the *NEXT PEAK* (or *NEXT MIN*) functions in the *NEXT MODE ABS* setting as always the next smaller (or larger) signal is searched for.

In the *SEARCH NEXT LEFT* or *SEARCH NEXT RIGHT* setting, functions *NEXT PEAK* and *NEXT MIN* search for the next relative maximum or minimum on the right or left of the current marker position irrespective of the instantaneous signal amplitude. A relative maximum is given when the signal amplitude on both sides of the maximum is reduced by a certain amount, ie the peak excursion.
The preset 6 dB level change can already be reached by the noise indication of the analyzer. Noise maxima are identified as peaks. In this case, *PEAK EXCURSION* has to be selected with a higher value than the difference between the highest and lowest noise indication values.

The following example shows the effect of different *PEAK EXCURSION* settings.

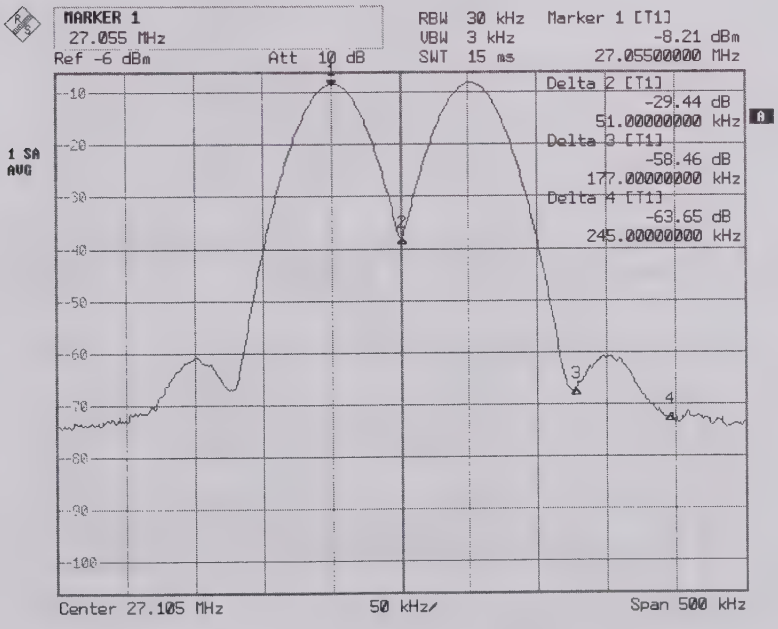

Fig. 4-7 Example for level measurements at different peak excursion settings

Maximum relative level change of the measured signals:

Signal 2:	42 dB
Signal 3	30 dB
Signal 4:	46 dB

The setting **Peak Excursion 40 dB** causes signals 2 and 4 to be detected with *NEXT PEAK* or *NEXT PEAK RIGHT*. Signal 3 is not detected since it only decreases by 30 dB before the level rises again.

Order of signals found:

PEAK:	Signal 1
NEXT PEAK:	Signal 2
NEXT PEAK:	Signal 4

or

PEAK:	Signal 1
NEXT PEAK RIGHT:	Signal 2
NEXT PEAK RIGHT:	Signal 4

The setting **Peak Excursion 20 dB** causes signal 3 to be detected as well since its highest level change of 30 dB is now higher than the set peak excursion.

Order of signals found:

PEAK:	Signal 1
NEXT PEAK:	Signal 2
NEXT PEAK:	Signal 4
NEXT PEAK:	Signal 3

or

PEAK:	Signal 1
NEXT PEAK RIGHT:	Signal 2
NEXT PEAK RIGHT:	Signal 3
NEXT PEAK RIGHT:	Signal 4

The setting **Peak Excursion 6 dB** detects all the signals, *NEXT PEAK RIGHT* does not work as required.

Order of signals found:

PEAK:	Signal 1
NEXT PEAK:	Signal 2
NEXT PEAK:	Signal 4
NEXT PEAK:	Signal 3

or

PEAK:	Signal 1
NEXT PEAK RIGHT:	Marker in noise between signal 1 and signal 2
NEXT PEAK RIGHT:	Marker in noise between signal 1 and signal 2

The *MKR→TRACE* softkey sets the active marker to a new trace. If only one trace is available on the screen, the softkey does not appear. If several traces are available on the screen, only these are offered.

IEC/IEEE-bus command: `CALC:MARK:TRAC 2`

Example:

Three traces are displayed on the screen. The marker is always on Trace 1 after switching on.

[*MKR ->TRACE] "2" <ENTER>* The marker jumps to Trace 2 but remains at the previous frequency or time.

[*MKR ->TRACE*] "3" *<ENTER>* The marker jumps to Trace 3.

The *MKR→CF STEPSIZE* softkey sets the step size for the center frequency variation to the current marker frequency, and also sets step size adaptation to *MANUAL*. *CF STEPSIZE* remains at this value until the center frequency entry mode in the STEP menu is switched from *MANUAL* to *AUTO* again.

The *MKR→CF STEPSIZE* function is, above all, useful in the measurement of harmonics with large dynamic range (narrow bandwidth and narrow span).

The softkey is not available in the time domain (span = 0 Hz).

IEC/IEEE-bus command: `CALC:MARK:FUNC:CST`

Example:

The harmonics levels of a CW carrier are to be measured at 100 MHz.

[**PRESET**]	FSP is set to the default setting.
[**CENTER**: 100 **MHz**]	FSP sets the center frequency to 100 MHz. The span is set to 200 MHz.
[**SPAN**: 1 **MHz**]	The span is set to 100 MHz.
[**MKR->**]	*MARKER 1* is switched on and set to the maximum value of the signal.
[**NEXT**]	FSP switches to the submenu.
[*MKR->CF STEPSIZE*]	The step size of the center frequency setting equals the marker frequency (100 MHz).
[**CENTER**]	The center frequency entry mode is activated.
[**Right key**]	The center frequency is set to 200 MHz. The first harmonic of the test signal is displayed.
[**MKR->:** *PEAK*]	The marker is set to the harmonic and the level of the latter is output in the marker info field.

The *MIN* softkey sets the active marker to the minimum value on the corresponding trace.

IEC/IEEE-bus command: `CALC:MARK:MIN`
`CALC:DELT:MIN`



The *NEXT MIN* softkey sets the active marker to the next higher minimum value on the corresponding trace. The search direction is defined in the *NEXT MODE* submenu (see above).

IEC/IEEE-bus command: `CALC:MARK:MIN:NEXT`
`CALC:DELT:MIN:NEXT`



The *EXCLUDE LO* softkey limits the frequency range for the marker search functions or disables the limit.

activated Because of the feedthrough of the first local oscillator to the first intermediate frequency at the input mixer, the LO is represented as a signal at 0 Hz. To avoid the marker jumping to the LO at 0 Hz with the peak function when setting the display range, this frequency is excluded. The minimum frequency to which the marker jumps, is ≥ 6 × resolution bandwidth (RBW).

deactivated No restriction to the search range. The frequency 0 Hz is included in the marker search functions.

IEC/IEEE-bus command: `CALC:MARK:LOEX ON`

Power Measurements – Hardkey *MEAS*

With its power measurement functions the FSP is able to measure all the necessary parameters with high accuracy in a wide dynamic range.

A modulated carrier is almost always used (except eg: SSB-AM) for high-frequency transmission of information. Due to the information modulated upon the carrier, the latter covers a spectrum which is defined by the modulation, the transmission data rate and the signal filtering. Within a transmission band each carrier is assigned a channel taking into account these parameters. In order to ensure error-free transmission, each transmitter must be conforming to the specified parameters. These include among others:

- the output power,
- the occupied bandwidth, ie the bandwidth which must contain a defined percentage of the power and
- the power dissipation allowed in the adjacent channels.

Additionally the menu contains functions to determine the modulation depth of AM modulated signals and to measure the 3rd order intercept point.

The measurements and the corresponding settings are selected in the *MEAS* menu.

MEAS menu:

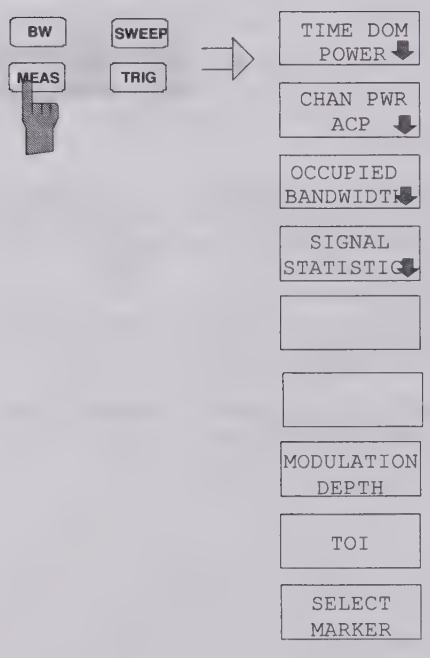

The *MEAS* key opens the menu to select and set the power measurement.

The following measurements can be selected:

- Power in time domain (*TIME DOM POWER*)
- Channel power and adjacent-channel power in frequency domain (*CHAN PWR /ACP*)
- Occupied bandwidth (*OCCUPIED BANDWIDTH*)
- Amplitude probability distribution (*SIGNAL STATISTICS*)
- Modulation depth (*MODULATION DEPTH*)
- 3rd order intercept (*TOI*)

The above measurements are carried out alternatively.

Power Measurement in Time Domain

With the aid of the power measurement function the FSP determines the power of the signal in the time domain (SPAN = 0 Hz) by summing up the power at the individual pixels and dividing the result by the number of pixels. In this way it is possible to measure for example the power of TDMA signals during transmission or during the muting phase. Both the mean power and the rms power can be measured by means of the individual power values.
The result is displayed in the marker info field.

The measured values are updated after each sweep or averaged over a user-defined number of sweeps (*AVERAGE ON/OFF* and *NUMBER OF SWEEPS*) in order to determine eg the mean power over several bursts. For determination of the peak value (*PEAK HOLD ON*) the maximum value from several sweeps is displayed.

Example:
Marker info field for: *MEAN* selected, *AVERAGE ON* and *PEAK HOLD ON*:

```
MEAN HOLD      -2.33 dBm
MEAN AV        -2.39 dBm
```

If both the on and off phase of a burst signal are displayed, the measurement range can be limited to the transmission or to the muting phase with the aid of vertical lines. The ratio between signal and noise power of a TDMA signal for instance can be measured by using a measurement as a reference value and after that varying the measurement range.

Upon switching on power measurement the sample detector is activated (*TRACE-DETECTOR-SAMPLE).*

Submenu *MEAS - TIME DOM POWER*:

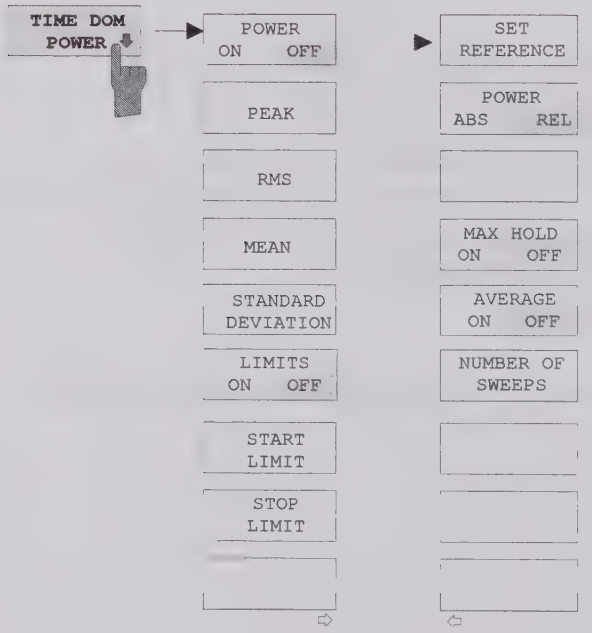

The *TIME DOM POWER* softkey activates the power measurement in the time domain and opens a submenu for configuration of the power measurement.

The submenu allows selection of the type of power measurement (rms or mean power), the settings for max hold and averaging as well as the definition of limits.

The power evaluation range can be limited by input of limit values.

Note: *This softkey is only available in time domain (SPAN = 0).*



The *POWER ON/OFF* softkey switches the power measurement on and off. When entering the submenu it is *ON* since the power measurement is already switched on with the *TIME DOM POWER* softkey in the main menu.

Note: *The measurement is performed on the trace on which marker 1 is placed. To evaluate another trace, marker 1 should be set on another trace using the SELECT TRACE softkey in menu MKR.*

IEC/IEEE-bus command:

```
CALC:MARK:FUNC:SUMM:PPE ON
CALC:MARK:FUNC:SUMM:PPE:RES?
CALC:MARK:FUNC:SUMM:RMS ON
CALC:MARK:FUNC:SUMM:RMS:RES?
CALC:MARK:FUNC:SUMM:MEAN ON
CALC:MARK:FUNC:SUMM:MEAN:RES?
CALC:MARK:FUNC:SUMM:SDEV ON
CALC:MARK:FUNC:SUMM:SDEV:RES?
```

The *PEAK* softkey switches on the calculation of the peak value from the points of the displayed trace or a segment thereof.

For the maximum peak, the largest peak value obtained since the activation of *MAX HOLD ON* is displayed.

With *AVERAGE ON*, the peak values of a trace are averaged over several sweeps and displayed.

The number of sweeps over which the average or the maximum value is calculated is set with the *NUMBER OF SWEEPS* softkey.

IEC/IEEE-bus command:

```
CALC:MARK:FUNC:SUMM:PPE ON
CALC:MARK:FUNC:SUMM:PPE:RES?
```

The *RMS* softkey switches on the calculation of the rms value from the points of the displayed trace or a segment of it.

For the maximum peak, the largest rms value obtained since the activation of *MAX HOLD ON* is displayed.

With *AVERAGE ON*, the rms values of a trace are averaged over several sweeps and displayed.

The number of sweeps over which the average or the maximum value is calculated is set with the *NUMBER OF SWEEPS* softkey.

IEC/IEEE-bus command:

```
CALC:MARK:FUNC:SUMM:RMS ON
CALC:MARK:FUNC:SUMM:RMS:RES?
```



The *MEAN* softkey switches on the calculation of the mean value from the points of the displayed trace or a segment of it. The linear mean value of the equivalent voltages is calculated.

This can be used for instance to measure the mean power during a GSM burst.

For the maximum peak, the largest mean value obtained since the activation of *MAX HOLD ON* is displayed.

With *AVERAGE ON*, the mean values of a trace are averaged over several sweeps and displayed.

The number of sweeps over which the average or the maximum value is calculated is set with the *NUMBER OF SWEEPS* softkey.

IEC/IEEE-bus command:
```
CALC:MARK:FUNC:SUMM:MEAN ON
CALC:MARK:FUNC:SUMM:MEAN:RES?
```

The *STANDARD DEVIATION* softkey switches on the calculation of the standard deviation of trace points from the mean value and outputs them as measured value. The measurement of the mean power is automatically switched on at the same time.

For the maximum peak, the largest standard deviation obtained since the activation of *MAX HOLD ON* is displayed.

With *AVERAGE ON*, the standard deviations of a trace are averaged over several sweeps and displayed.

The number of sweeps over which the average or the maximum value is calculated is set with the *NUMBER OF SWEEPS* softkey.

IEC/IEEE-bus command:
```
CALC:MARK:FUNC:SUMM:SDEV ON
CALC:MARK:FUNC:SUMM:SDEV:RES?
```



The *LIMIT ON/OFF* softkey selects the limited (*ON*) or non-limited (*OFF*) evaluation range.

The evaluation range is defined by the *START LIMIT* and *STOP LIMIT* softkeys. If *LIMIT = ON*, signals are only searched between the two lines.

If only one limit line is switched on, time line 1 is the lower limit and the upper limit corresponds to the stop frequency. If time line 2 is also switched on, it defines the upper limit.

If no limit line is switched on, the evaluation range is not limited.

The default setting is *LIMIT = OFF*.

IEC/IEEE-bus command:
```
CALC:MARK:X:SLIM OFF
```

The *START LIMIT* softkey activates the entry of the lower limit of the evaluation range.

IEC/IEEE-bus command:
```
CALC:MARK:X:SLIM:LEFT <value>
```

The *STOP LIMIT* softkey activates the entry of the upper limit of the evaluation range.

IEC/IEEE-bus command:
```
CALC:MARK:X:SLIM:RIGH <value>
```



The *SET REFERENCE* softkey sets the power values currently measured as reference values for the calculation of the mean value (*MEAN)* and the rms value (*RMS)*. The reference values are used to perform relative measurements.

If the calculation of the mean value (*MEAN)* and rms value (*RMS)* is not switched on, 0 dBM is used as a reference value.

If the average value (*AVERAGE)* or maximum value (*MAX HOLD*) is calculated over several sweeps, the current value is the measured value summed up at the actual time.

IEC/IEEE-bus command: `CALC:MARK:FUNC:SUMM:REF:AUTO ONCE`



The *POWER ABS/REL* softkey selects the absolute power measurement (default setting) or relative power measurement. The reference value for the relative power is defined by *SET REFERENCE*.

The value 0 dBm is used if the reference value is not defined.

IEC/IEEE-bus command: `CALC:MARK:FUNC:SUMM:MODE ABS`

The *MAX HOLD ON/OFF* softkey switches the display of the maximum peak obtained from measurements at successive sweeps on and off.

The displayed maximum peak is only updated at the end of a sweep if a higher value has occurred.

The maximum value can be reset by switching the *MAX HOLD ON / OFF* softkey off and on again.

IEC/IEEE-bus command:
```
CALC:MARK:FUNC:SUMM:PHOL ON
CALC:MARK:FUNC:SUMM:PPE:PHOL:RES?
CALC:MARK:FUNC:SUMM:RMS:PHOL:RES?
CALC:MARK:FUNC:SUMM:MEAN:PHOL:RES?
CALC:MARK:FUNC:SUMM:SDEV:PHOL:RES?
```

The *AVERAGE ON/OFF* softkey switches averaging over successive sweep measurements on and off.

The measured values can be reset by switching the *AVERAGE ON / OFF* softkey off and on again.

IEC/IEEE-bus command:
```
CALC:MARK:FUNC:SUMM:AVER ON
CALC:MARK:FUNC:SUMM:PPE:AVER:RES?
CALC:MARK:FUNC:SUMM:RMS:AVER:RES?
CALC:MARK:FUNC:SUMM:MEAN:AVER:RES?
CALC:MARK:FUNC:SUMM:SDEV:AVER:RES?
```



The *NUMBER OF SWEEPS* softkey activates the entry of the number of sweeps for maximum or average value calculation.

SINGLE SWEEP mode	The FSP performs sweeps until the selected number of sweeps is reached and stops then.
CONTINUOUS SWEEP mode	Averaging is carried out until the selected number of sweeps is reached. After that, averaging is performed in continuous mode. and is then continued as running averaging. Calculation of the maximum peak (*MAX HOLD*) is performed continuously irrespective of the selected number of sweeps.

The valid range values is 0 to 32767.

Depending on the specified number of sweeps, averaging is carried out according to the following rules:

NUMBER OF SWEEPS = 0	Continuous averaging is carried out over 10 measured values.
NUMBER OF SWEEPS = 1	No averaging is carried out.
NUMBER OF SWEEPS > 1	Averaging is carried out over the set number of measured values.

Note: *This setting is equivalent to the setting of the sweep count in the TRACE menu.*

IEC/IEEE-bus command: `SWE:COUN <value>`

Example:

The mean power of a GSM burst with 0 dBm nominal power at 800 MHz is to be measured.

[**PRESET**]	Set the FSP to the default setting.
[**FREQ:** *CENTER*: 800 **MHz**]	Set the center frequency to 800 MHz.
[**SPAN**: *ZERO SPAN*]	Select time domain display (span = 0 Hz).
[**AMPT**: 0 **dBm**]	Set the reference level to 0 dBm.
[**BW**: *RES BW MANUAL*: 30 **kHz**]	Set the resolution bandwidth to 30 kHz in line with the requirements of the GSM standard.
[**SWEEP**: *SWEEPTIME MANUAL* 600 µs]	Set the sweep time to 600 µs.
[**TRIG**: *VIDEO*: 50 **%**]	Use the video signal as trigger source.
[**MEAS**]	Call the menu for the measurement functions.
[*TIME DOM POWER*]	Select power measurement in the time domain. The FSP calculates the mean power from the points of the whole trace. The submenu for configuration of the power measurement is opened. *MEAN* is already switched on.
[*LIMITS ON*]	Activate the limitation of the time domain of the power measurement .
[*START LIMIT*: 250 **µs**]	Set the start of the power measurement at 250 µs.
[*STOP LIMIT*: 500 **µs**]	Set the end of the power measurement at 500 µs.

Note: *The GSM specifications require the power to be measured between 50% and 90% of the TDMA burst. The time limits set above approximately correspond to the required time domain.*

Channel and Adjacent-Channel Power Measurements

For all channel and adjacent-channel power measurements a specified channel configuration is assumed which is for instance based on a specific radiocommunication system.
This configuration is defined by the nominal channel frequency (= center frequency of the FSP), channel bandwidth, adjacent-channel bandwidth and adjacent-channel spacing. The FSP is able to simultaneously measure the power in up to three adjacent channels (7 channels: transmission channel, 3 lower and 3 upper adjacent channels).
It offers two methods for channel and adjacent-channel power measurement:

- The integrated bandwidth method (IBW method), ie the integration of trace pixels within the bandwidth of the channel to be measured to the total power of the channel,
- The measurement in time domain (Fast ACP) by means of steep resolution filters simulating the channel.

The two measurements yield the same results. The measurement in time domain can be performed much faster since the complete signal is measured within a channel at the same time. With the IBW method, the channel is divided into subspectra. This is done by means of a bandwidth which is small compared to the channel bandwidth. These subspectra are then combined by integration of the trace pixels.

With the IBW method, the transmission channel or adjacent channels are marked by vertical lines at a distance of half the channel bandwidth to the left and to the right of the corresponding channel center frequency. (see Fig. 4-6).
In the time-domain method, the power trace in the different channels is shown. (see Bild 4-7).
For both methods, the results are listed in tables in the lower half of the screen.
The FSP offers predefined standard settings which can be selected from a table for the common mobile radio standards. Thus, channel configuration is performed automatically without the need to enter the corresponding parameters manually.
For some standards, the channel power and the adjacent-channel power are to be weighted by means of a root-raised cosine filter corresponding to a receive filter. This type of filtering is switched on automatically for both methods on selecting the standard (eg NADC, TETRA or 3GPP W-CDMA).

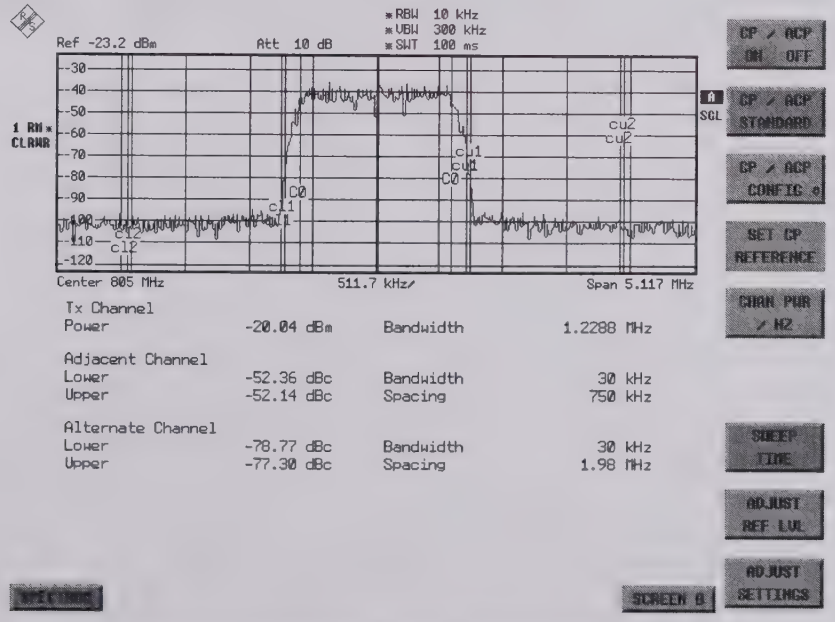

Fig. 4-6 Screen display of adjacent-channel power measurement using the IBW method

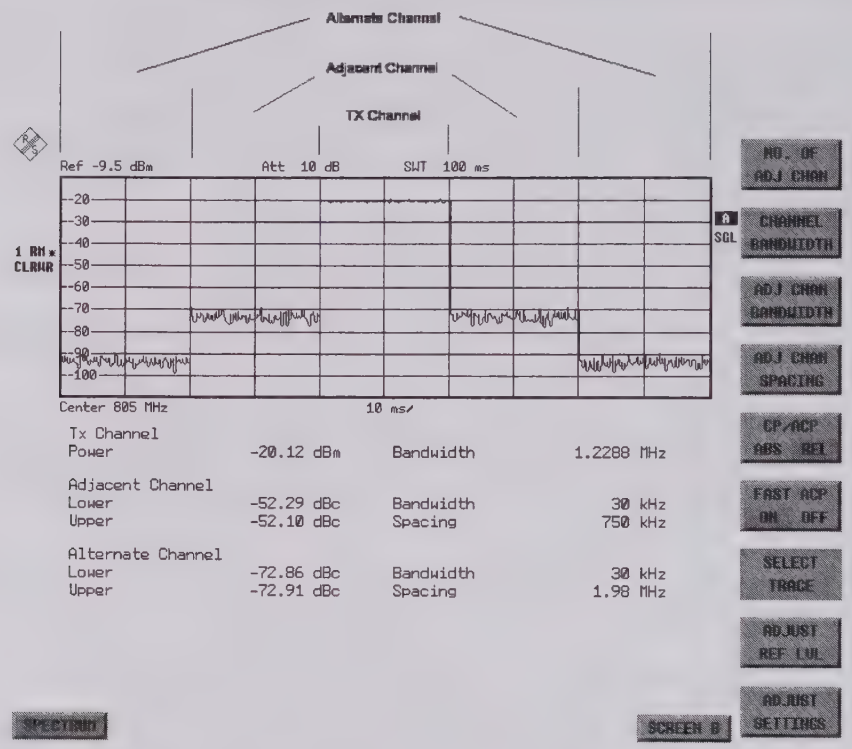

Fig. 4-7 Screen display of adjacent-channel power measurement using the time-domain method

Limit values for the adjacent-channel power can be defined for the measurement. If limit checking is switched on, a pass/fail information indicating that the power has been exceeded is displayed during the measurement in the table in the lower half of the screen.

Note: *With the CP/ACP measurement switched on the functions SPLIT SCREEN and FULL SCREEN are inhibited.*

The channel configuration is defined in the *MEAS CHAN POWER/ACP* menu.

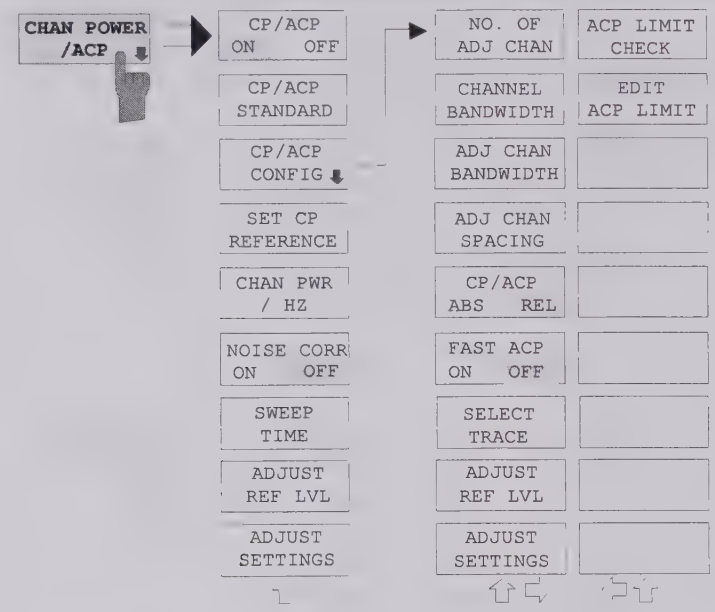

The *CHAN POWER /ACP* softkey switches on the channel power measurement or adjacent-channel power measurement according to the current configuration. At the same time it opens the submenu for defining the channel power measurement. The softkey is highlighted to show that channel or adjacent-channel power measurement is on.

Note: *This softkey can only be operated in frequency domain (SPAN > 0).*



The *CP/ACP ON/OFF* softkey switches the calculation of the channel power or adjacent-channel power on or off.

With default settings the measurement is performed by integrating the powers at the display points within the specified channels (IBW method).

The adjacent-channel power can be either absolute or relative related to the transmission channel power. The default setting is relative measurement (see softkey *CP/ACP ABS/ REL*).

IEC/IEEE-bus command:

```
CALC:MARK:FUNC:POW:SEL CPOW|ACP
CALC:MARK:FUNC:POW:RES? CPOW|ACP
CALC:MARK:FUNC:POW OFF
```



The *CP/ACP STANDARD* softkey opens a table for the selection of the settings according to predefined standards. The test parameters for the channel and adjacent-channel measurements are set according to the mobile radio standard.

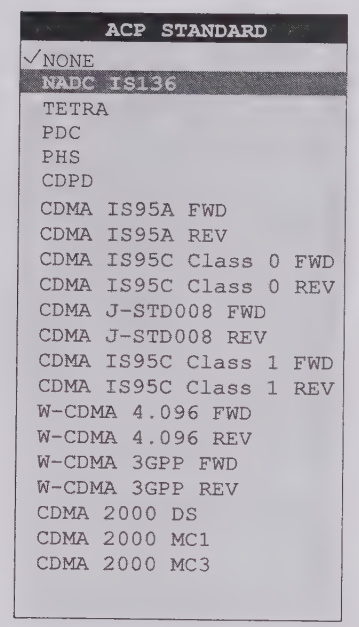

The standards available are listed in the table on the left.

Note: *For the FSP, the channel spacing is defined as the distance between the center frequency of the adjacent channel and the center frequency of the transmission channel. The definition of the adjacent-channel spacing in standards IS95 B and C, IS97 B and C and IS98 B and C is different. These standards define the adjacent-channel spacing from the center of the transmission channel to the closest border of the adjacent channel. This definition is also used for the FSP when the following standard settings are selected:*
CDMA IS95 Class 0 FWD
CDMA IS95 Class 0 REV
CDMA IS95 Class 1 FWD
CDMA IS95 Class 1 REV

The selection of the standard influences the following parameters:
- channel spacing
- channel bandwidth and type of filtering
- resolution bandwidth
- video bandwidth
- detector
- # of adjacent channels

Trace mathematics and trace averaging are switched off.
The reference level is not influenced by the selection of a standard. To achieve an optimum dynamic range, the reference level has to be set in a way that places the signal maximum close to the reference level without forcing an overload message.

The default setting is CP/*ACP STANDARD NONE*.

IEC/IEEE-bus command: `CALC:MARK:FUNC:POW:PRES <standard>`



See following section "Setting the Channel Configuration"



With channel power measurement activated, the *SET CP REFERENCE* softkey defines the currently measured channel power as the reference value. The reference value is displayed in the *CH PWR REF* field; the default value is 0 dBm.

During the adjacent-channel power measurement the power in the transmission channel becomes the reference value. The display *CH PWR REF* is not required.

IEC/IEEE-bus command: `POW:ACH:REF:AUTO ONCE`



The *CHAN PWR / HZ* softkey selects the measurement of the total channel power or the measurement of the channel power referred to 1 Hz bandwidth. The conversion factor is $10 \cdot \lg \frac{1}{\text{Channel} \cdot \text{Bandwidth}}$.

This function allows for instance measurement of the noise power density or, in conjunction with the *CP/ACP REL* and *SET CP REFERENCE* functions, measurement of the signal-to-noise ratio.

□□Ç¹´´â«¢ł □□□□□□□□đ□□□□□□□□□□ъ□ъ□□□□□Ĉđ□□□□□□□˝□□□□□□□□□đ
□□□□□

The *SWEEP TIME* softkey activates the entry of the sweep time. With the RMS detector, a longer sweep time increases the stability of the measurement results. The function of the softkey is identical to the softkey *SWEEP TIME MANUAL* in the menu *BW*.

IEC/IEEE-bus command: `SWE:TIM <value>`

The *ADJUST REF LVL* softkey adjusts the reference level of the FSP to the measured channel power. This ensures that the settings of the RF attenuation and the reference level are optimally adjusted to the signal level without overloading the FSP or limiting the dynamic range by a too small S/N ratio.
Since the measurement bandwidth for channel power measurements is significantly lower than the signal bandwidth, the signal path may be overloaded although the trace is still significantly below the reference level.

IEC/IEEE-bus command: `SENS:POW:ACH:PRES:RLEV`

The *ADJUST SETTINGS* softkey automatically optimizes the analyzer settings for the selected power measurement (see below).
All analyzer settings relevant for a power measurement within a specific frequency range (channel bandwidth) are optimized for the selected channel configuration (channel bandwidth, channel spacing):

- Frequency span:

  The frequency span has to cover at least all channels to be considered. When measuring the channel power, 2 x channel bandwidth is set as span.
  The setting of the span during adjacent-channel power measurement is dependent on the channel spacing and channel bandwidth of the adjacent channel ADJ, ALT1 or ALT2 with the largest distance from the transmission channel.

- Resolution bandwidth RBW $\leq$ 1/40 of channel bandwidth
- Video bandwidth VBW $\geq 3 \times$ RBW
- Detector RMS detector

Trace math and trace averaging functions are switched off.
The reference level is not influenced by *ADJUST SETTINGS*. It can be separately adjusted with *ADJUST REF LVL*.

The adjustment is carried out only once; if necessary, the instrument settings can be changed later.

IEC/IEEE-bus command: `SENS:POW:ACH:PRES ACP|CPOW|OBW`

For manual setting of the test parameters different from the settings made with *ADJUST SETTINGS* the following should be observed:

Frequency span

The frequency span has to cover at least all channels to be measured.
For channel power measurement this is the channel bandwidth.
If the frequency span is large compared to the frequency section (or frequency sections) under test, only a few pixels are available to be measured.

Resolution bandwidth (RBW)

To ensure both an acceptable measurement speed and the required selection (to suppress spectral components outside the channel to be measured, especially of the adjacent channels), the resolution bandwidth must not be selected too small or too large. As a general approach, the resolution bandwidth is to be set to values between 1% and 4% of the channel bandwidth. A larger resolution bandwidth can be selected if the spectrum within the channel to be measured and around it has a flat characteristic. In the standard setting, eg for standard IS95A REV at an adjacent channel bandwidth of 30 kHz, a resolution bandwidth of 30 kHz is used. This yields correct results since the spectrum in the neighbourhood of the adjacent channels normally has a constant level. For standard NADC/IS136 this is not possible for example, since the spectrum of the transmit signal penetrates into the adjacent channels and a too large resolution bandwidth causes a too low selection of the channel filter. The adjacent-channel power would thus be measured too high.

With the exception of the IS95 CDMA standards, the *ADJUST SETTINGS* softkey sets the resolution bandwidth (RBW) as a function of the channel bandwidth:

RBW $\leq$ 1/40 of channel bandwidth.

The maximum possible resolution bandwidth (with respect to the requirement RBW $\leq$ 1/40) resulting from the available RBW steps (1, 3) is selected .

Video bandwidth (VBW)

For a correct power measurement, the video signal must not be limited in bandwidth. A restricted bandwidth of the logarithmic video signal would cause signal averaging and thus result in a too low indication of the power (-2.51 dB at very low video bandwidths). The video bandwidth should therefore be selected at least three times the resolution bandwidth.

The *ADJUST SETTINGS* softkey sets the video bandwidth (VBW) as a function of the channel bandwidth as follows:

VBW $\geq 3 \times$ RBW.

The smallest possible VBW with regard to the available step size (1, 3) will be selected.

Detector

The *ADJUST SETTINGS* softkey selects the RMS detector.
The RMS detector is selected since it correctly indicates the power irrespective of the characteristics of the signal to be measured. In principle, the sample detector would be possible as well. Due to the limited number of trace pixels used to calculate the power in the channel, the sample detector would yield less stable results. Averaging, which is often performed to stabilize the measurement results, leads to a too low level indication and should therefore be avoided. The reduction in the displayed power depends on the number of averages and the signal characteristics in the channel to be measured.

Setting the Channel Configuration

MEAS - CP/ACP CONFIG submenu:

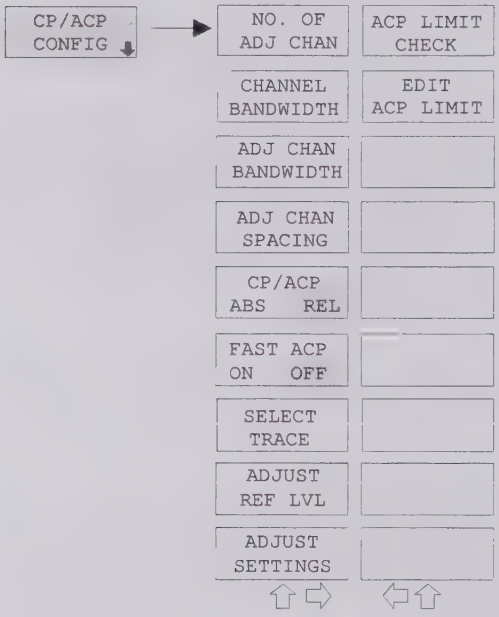

The *CP/ACP CONFIG* softkey opens a submenu for configuration of the channel power and adjacent channel power measurement independent from the offered standards.

The channel configuration consists of the number of adjacent channels to be measured, the channel bandwidth (*CHANNEL BANDWIDTH*), the bandwidth of the adjacent channels (*ADJ CHANNEL BANDWIDTH*) and the distance of the adjacent channels from the center frequency of the transmission channel (*ADJ CHANNEL SPACING*).

Limit values can additionally be specified for the adjacent-channel power (*ACP LIMIT CHECK* and *EDIT ACP LIMITS*) which are checked for compliance during the measurement.



The *NO. OF ADJ CHAN* softkey activates the entry of the number ±n of adjacent channels to be considered in the adjacent-channel power measurement.
Numbers from 0 to 3 can be entered.

The following measurements are performed depending on the number of the channels.

0 Only the channel power is measured.

1 The channel power and the power of the upper and lower adjacent channel are measured.

2 The channel power, the power of the upper and lower adjacent channel and of the next higher and lower channel (alternate channel 1) are measured.

3 The channel power, the power of the upper and lower adjacent channel, the power of the next higher and lower channel (alternate channel 1) and of the next but one higher and lower adjacent channel (alternate channel 2) are measured.

IEC/IEEE-bus command: `POW:ACH:ACP 1`

CHANNEL BANDWIDTH

The *CHANNEL BANDWIDTH* softkey activates the entry of the channel bandwidth for the transmission channel.

The useful channel bandwidth is generally defined by the transmission method. It is automatically adjusted correctly on measurements according to a given standard (see *CP/ACP STANDARD* softkey).

When measuring according to the IBW method (*FAST ACP OFF)* the channel bandwidth is displayed by two vertical lines to the left and right of the screen center. It can thus be visually checked whether the whole power of the signal to be measured is within the selected channel bandwidth.

With the time domain method (*FAST ACP ON)* the measurement is performed in zero span. The channel limits are not marked in this case. The FSP offers all available channel filters for selection of the channel bandwidth. Deviating channel bandwidths cannot be set. If deviating channel bandwidths are required, the IBW method should be used.

The list of available channel filters is included in section "Setting of Bandwidths and Sweep Time – *BW key".*

The default setting is 14 kHz.

IEC/IEEE-bus command: `SENS:POW:ACH:BWID 14kHz`

ADJ CHAN BANDWIDTH

The ADJ *CHAN BANDWIDTH* softkey opens a table for defining the channel bandwidths for the adjacent channels.

ACP CHANNEL BW	
CHAN	BANDWIDTH
ADJ	30 kHz
ALT1	30 kHz
ALT2	30 kHz

When measuring according to the IBW method (FAST ACP OFF) the bandwidths of the different adjacent channels are to be entered numerically. Since all adjacent channels often have the same bandwidth, the other channels Alt1 and Alt2 are set to the bandwidth of the adjacent channel on entering the adjacent-channel bandwidth (ADJ). Thus only one value needs to be entered in case of equal adjacent channel bandwidths. The same holds true for the ALT2 channels (alternate channels 2) when the bandwidth of the ALT1 channel (alternate channel 1) is entered.

Note: *The bandwidths can be selected independent from each other by overwriting the table from top to bottom.*

With the time domain method (FAST ACP ON), the adjacent-channel bandwidths are selected from the list of available channel filters. For deviating adjacent-channel bandwidths the IBW method should be used.

IEC/IEEE-bus command:
```
SENS:POW:ACH:BWID:ACH 1kHz
SENS:POW:ACH:BWID:ALT1 14kHz
SENS:POW:ACH:BWID:ALT2 14kHz
```

The ADJ *CHAN SPACING* softkey opens a table for defining the channel spacings.

ACP CHANNEL SPACING	
CHAN	SPACING
ADJ	800 kHz
ALT1	1.60 MHz
ALT2	2.40 MHz

Since all the adjacent channels often have the same distance to each other, the entry of the adjacent-channel spacing (ADJ) causes channel spacing ALT1 to be set to twice and channel spacing ALT2 to three times the adjacent-channel spacing. Thus only one value needs to be entered in case of equal channel spacing. The same holds true for the ALT2 channels when the bandwidth of the ALT1 channel is entered.

Note: *The channel spacings can be set separately by overwriting the table from top to bottom.*

IEC/IEEE-bus command:
```
SENS:POW:ACH:SPAC:ACH 20kHz
SENS:POW:ACH:SPAC:ALT1 40kHz
SENS:POW:ACH:SPAC:ALT2 60kHz
```

The *CP/ACP ABS/REL* softkey (channel power absolute/relative) switches between absolute and relative power measurement in the channel.

CP/ACP ABS The absolute power in the transmission channel and in the adjacent channels is displayed in the unit of the Y axis, eg in dBm, dBµV.

CP/ACP REL In case of adjacent-channel power measurement (*NO. OF ADJ CHAN* > 0) the level of the adjacent channels is displayed relative to the level of the transmission channel in dBc.

In case of channel power measurement (*NO. OF ADJ CHAN* = 0) the power of a transmission channel is displayed relative to the power of a reference channel defined by *SET CP REFERENCE*. This means:

1. Declare the power of the currently measured channel as the reference value, using the *SET CP REFERENCE* softkey.
2. Select the channel of interest by varying the channel frequency (FSP center frequency).

With linear scaling of the Y axis, the power of the new channel relative to the reference channel (CP/CP_{ref}) is displayed. With dB scaling, the logarithmic ratio $10lg\ (CP/CP_{ref})$ is displayed.

The relative channel power measurement can thus also be used for universal adjacent-channel power measurements. Each channel can be measured individually.

IEC/IEEE-bus command:
```
SENS:POW:ACH:MODE ABS
```

The *FAST ACP* softkey switches between the IBW method (FAST ACP OFF) and the time domain method (FAST ACP ON).

With FAST ACP ON the power measurement is performed in the different channels in time domain. The FSP sets the center frequency consecutively to the different channel center frequencies and measures the power with the selected measurement time (= sweep time/number of channels). The RBW filter suitable for the selected standard and frequency offset are automatically used (eg root raised cos with IS 136). The list of available channel filters is included in section "Setting of Bandwidths and Sweep Time – *BW key*".

The RMS detector is used for obtaining correct power measurement results. Therefore this requires no software correction factors.

The measured values are displayed in a table, the power in the useful channel being displayed in dBm and the power in the adjacent channels in dBm (CP/ACP ABS) or dB (CP/ACP REL).

The sweep time is selected depending on the desired reproducibility of results. Reproducibility increases with sweep time since power measurement is then performed over a longer time period.

As a general approach, it can be assumed that approx. 500 non-correlated measured values are required for a reproducibility of 0.5 dB (99% of the measurements are within 0.5 dB of the true measured value). This holds true for white noise. The measured values are considered as non-correlated when their time interval corresponds to the reciprocal of the measured bandwidth.

With IS 136 the measurement bandwidth is approx. 25 Hz, ie measured values at an interval of 40 µs are considered as non-correlated. A measurement time of 10 ms is thus required per channel for 1000 measured values. This is the default sweep time which the FSP sets in coupled mode. Approx. 5000 measured values are required for a reproducibility of 0.1 dB (99%), ie the measurement time is to be increased to 200 ms.

IEC/IEEE-bus command `SENS:POW:HSP ON`



The *SELECT TRACE* softkey selects the trace, on which the CP/ACP measurement is performed. Only traces can be selected, which are switched on (= not set to BLANK).

IEC/IEEE-bus command: `SENS:POW:TRAC 1`



See main menu *CHAN PWR ACP.*

See main menu *CHAN PWR ACP.*

The *ACP LIMIT CHECK* softkey switches the limit check for the ACP measurement on and off.

IEC/IEEE-bus command:

```
CALC:LIM:ACP ON
CALC:LIM:ACP:ACH:RES?
CALC:LIM:ACP:ALT:RES?
```



The *EDIT ACP LIMITS* softkey opens a table for defining the limits for the ACP measurement.

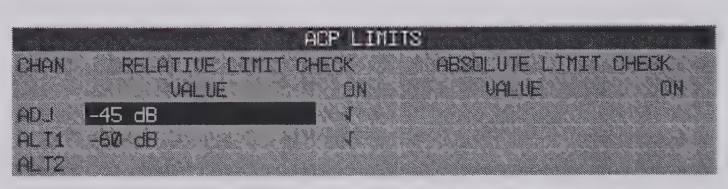

The following rules apply for the limits:

- A separate limit can be defined for each adjacent channel. The limit applies to both the upper and the lower adjacent channel.
- A relative and/or absolute limit can be defined. The check of both limit values can be activated independently.
- The FSP checks adherence to the limits irrespective of whether the limits are absolute or relative or wether the measurement is carried out with absolute or relative levels. If both limits are active and if the higher of both limit values is exceeded, the measured value is marked accordingly.

Note: *Measured values exceeding the limit are marked by a preceding asterisk.*

IEC/IEEE-bus command:

```
CALC:LIM:ACP ON
CALC:LIM:ACP:ACH 0dB,0dB
CALC:LIM:ACP:ACH:STAT ON
CALC:LIM:ACP:ACH:ABS -10dBm,-10dBm
CALC:LIM:ACP:ACH:ABS:STAT ON
CALC:LIM:ACP:ALT1 0dB,0dB
CALC:LIM:ACP:ALT1:STAT ON
CALC:LIM:ACP:ALT1:ABS -10dBm,-10dBm
CALC:LIM:ACP:ALT1:ABS:STAT ON
CALC:LIM:ACP:ALT2 0dB,0dB
CALC:LIM:ACP:ALT2:STAT ON
CALC:LIM:ACP:ALT2:ABS -10dBm,-10dBm
CALC:LIM:ACP:ALT2:ABS:STAT ON
```

Examples:

1. Measurement of adjacent-channel power for a specific standard:

The adjacent-channel power is to be measured for a signal at 800 MHz with 0 dBm level in line with IS136.

[**PRESET**]	Set the FSP to the default setting.
[**FREQ**: *CENTER*: 800 **MHz**]	Set the center frequency to 800 MHz.
[**AMPT**: 0 **dBm**]	Set the reference level to 0 dBm.
[**MEAS**]	Call the menu for the measurement functions.
[*CHAN PWR / ACP*]	Select the channel and adjacent-channel power measurement function. The measurement is performed with the default settings or a previously defined setting. The submenu for setting the desired new configuration is opened.
[*CP/ACP STANDARD*: select IS136: **ENTER**]	Select the NADC (IS136) standard.
[*CP/ACP CONFIG*]	Call the submenu for configuration of the adjacent-channel power measurement.
[*NO. OF ADJ CHAN*: 2 **ENTER**]	Select two adjacent channels for the measurement, ie the adjacent channel and the alternate channel are measured.
PREV	Change to the main menu for channel power measurement.
[*ADJUST SETTINGS*]	Set the optimum span, resolution bandwidth (RBW), video bandwidth (VBW) and detector automatically for the measurement. The absolute channel power and the relative power of the adjacent channels are displayed on the screen.
[*ADJUST REF LVL*]	Set the reference level equal to the channel power measured.

2. Measurement with user-specific channel configuration:

Measurement of the adjacent-channel power ratio (ACPR) of an IS95 CDMA signal at 800 MHz, level 0 dBm. Similar to example 1, the setting can be simplified by using *CP/ACP STANDARD*.

[**PRESET**] Set the FSP to the default setting.

[**FREQ:** *CENTER*: 800 **MHz**] Set the center frequency to 800 MHz.

[**AMPT**: 0 **dBm**] Set the reference level to 0 dBm.

[**MEAS**] Call the menu for the measurement functions.

[*CHAN PWR / ACP*] Select the channel and adjacent-channel power measurement function. The measurement is carried out with the default settings or a previously defined setting. The submenu for setting the desired new configuration is opened.

[*CP/ACP CONFIG*] Call the submenu for defining the channel configuration.

[*NO. OF ADJ CHAN*: 2 **ENTER**] Select two adjacent channels for the measurement, ie the adjacent channel and the alternate channel are measured.

[*CHANNEL BANDWIDTH*: 1.23 **MHz**] Set the channel bandwidth to 1.23 MHz according to IS95.

[*ADJ CHAN BANDWIDTH*: 30 **kHz**] Open the list for setting the bandwidth of the adjacent channels.

ACP CHANNEL BW	
CHAN	BANDWIDTH
ADJ	30 kHz
ALT1	30 kHz
ALT2	30 kHz

Upon entry of 30 kHz for the adjacent channel the alternate channels are also set to 30 kHz.

[*ADJ CHAN SPACING*: 885 **kHz:** : 1.98 **MHz**] Open the list for entering the adjacent-channel spacings.

ACP CHANNEL SPACING	
CHAN	SPACING
ADJ	885 kHz
ALT1	1.98 MHz
ALT2	2.97 MHz

Upon entry of 885 kHz for the adjacent channel the channels ALT1 and ALT2 are set to 1770 kHz and 2655 kHz. Upon entry of 1.98 MHz for the alternate channel 1 the alternate channel 2 is set to 2.97 MHz.

PREV In dasHauptmenü für die Kanalleistungsmessung wechseln.

[*ADJUST SETTINGS*] Automatically set the optimum span (= 5 MHz), resolution bandwidth (RBW = 30 kHz), video bandwidth (VBW = 300 kHz) and detector (RMS) for the measurement. The absolute channel power and the relative power of the adjacent channels and alternate channels are displayed on the screen.

[*ADJUST REF LVL*] Set the reference level equal to the channel power measured.

3. Measurement of signal/noise power density (C/No) of an IS95 CDMA signal (frequency 800 MHz, level 0 dBm)

[**PRESET**]	Set the FSP to the default setting.
[**FREQ:** *CENTER*: 800 **MHz**]	Set the center frequency to 800 MHz.
[**AMPT**: 0 **dBm**]	Set the reference level to 0 dBm.
MEAS]	Call the menu for the measurement functions.
[*CHAN PWR / ACP*]	Select the channel and adjacent-channel power measurement. The measurement is performed with the default setting or a previously defined setting. The submenu for setting the desired new configuration is opened.
[*CP/ACP CONFIG*]	Call the submenu for defining the channel configuration.
[*NO. OF ADJ CHAN*: 0 **ENTER**]	Do not select an adjacent channel for the measurement, ie the measurement is carried out in one channel only.
[*CHANNEL BANDWIDTH*: 1.23 **MHz**]	Set the channel bandwidth to 1.23 MHz in line with IS95.
PREV	Change to the main menu for channel power measurement
[*ADJUST SETTINGS*]	Set the optimum span (= 5 MHz), resolution bandwidth (RBW = 30 kHz), video bandwidth (VBW = 300 kHz) and detector (RMS) for the measurement automatically. The absolute channel power and the relative power of the adjacent channels and alternate channels are displayed on the screen.
[*ADJUST REF LVL*]	Set the reference level equal to the channel power measured.
[*SET CP REFERENCE*]	Set the measured channel power as a reference for the subsequent measurements.
[*CP/ACP ABS / REL*]	Select relative measurement related to the reference power set with *SET REFERENCE* (result 0 dB).
[*CHAN PWR / HZ*]	Select power measurement related to 1 Hz bandwidth (result -60.9 dB).
[**FREQ:** *CENTER*: 805 **MHz**]	Set the center frequency to 805 MHz. The FSP measures the channel power at 1.23 MHz bandwidth and outputs the result in dB relative to the reference power and 1 Hz bandwidth.

Measurement of Occupied Bandwidth

An important characteristics of a modulated signal is its occupied bandwidth. In a radio communications system for instance the occupied bandwidth must be limited to enable distortion-free transmission in adjacent channels. The occupied bandwidth is defined as the bandwidth containing a defined percentage of the total transmitted power. A percentage between 10% and 99.9% can be set on the FSP.

MEAS OCCUPIED BANDWIDTH menu:

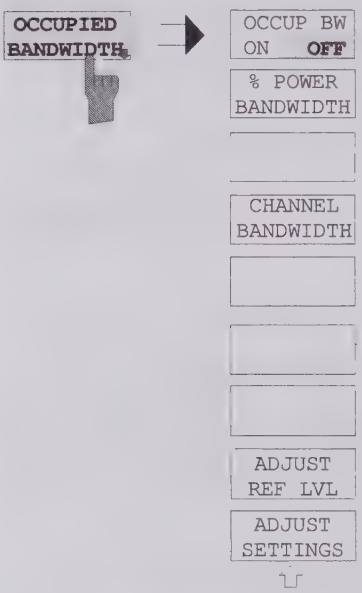

The *OCCUPIED BANDWIDTH* softkey activates measurement of the occupied bandwidth according to the current configuration and opens the submenu for configuring the measurement. The softkey is available only in frequency domain (span > 0) and is highlighted when the measurement is switched on.

In the spectrum display mode, this measurement determines the bandwidth that contains a predefined percentage of the power of the displayed frequency range (*% POWER BANDWIDTH* softkey). The occupied bandwidth is output in the marker display field and marked on the trace by temporary markers.

Note:
- *The softkey is only available in frequency domain (span > 0).*
- *The measurement is performed on the trace with marker 1. In order to evaluate another trace, marker 1 must be placed on another trace by means of SELECT TRACE in the MKR menu*



The *OCCUP BW ON/OFF* softkey switches measurement of the occupied bandwidth on or off.

IEC/IEEE-bus command:
```
CALC:MARK:FUNC:POW:SEL OBW
CALC:MARK:FUNC:POW:RES? OBW
CALC:MARK:FUNC:POW OFF
```



The *% POWER BANDWIDTH* softkey opens the entry of the percentage of power related to the total power in the displayed frequency range which defines the occupied bandwidth (percentage of total power).
The valid range of values is 10% to 99.9%.

IEC/IEEE-bus command:
```
SENS:POW:BWID 99PCT
```

The *CHANNEL BANDWIDTH* softkey opens an input window for defining the channel bandwidth for the transmission channel. For measurements in line with a specific transmission standard, the bandwidth specified by the standard for the transmission channel must be entered.
The default setting is 14 kHz.
The specified channel bandwidth is used for optimization of the test parameters of the FSP with *ADJUST SETTINGS*.

IEC/IEEE-bus command: `SENS:POW:ACH:BWID 14kHz`

The *ADJUST REF LVL* softkey adjusts the reference level of the FSP to the measured total power of the signal. The softkey is activated after the first sweep with the measurement of the occupied bandwidth has been completed and the total power of the signal is thus known.
Adjusting the reference level ensures that the signal path of the FSP will not be overloaded and the dynamic range not limited by too low a reference level.
Since the measurement bandwidth for channel power measurements is significantly lower than the signal bandwidth, the signal path may be overloaded although the trace is distinctly below the reference level. If the measured channel power is equal to the reference level, the signal path cannot be overloaded.

IEC/IEEE-bus command: `SENS:POW:ACH:PRES:RLEV`

The *ADJUST SETTINGS* softkey optimizes the analyzer settings for the measurement of the occupied bandwidth according to the specified channel bandwidth.
All analyzer settings relevant for power measurement within a specific frequency range, such as

- frequency span — 3 x channel bandwidth
- resolution bandwidth — RBW ≤ 1/40 of channel bandwidth
- video bandwidth — VBW ≥ 3 × RBW
- detector — RMS

are optimized.

The reference level is not influenced by *ADJUST SETTINGS*. For an optimum dynamic range it should be selected in a way that the signal maximum is close to the reference level.

The adjustment is carried out only once; if necessary, the instrument settings may be changed later.

IEC/IEEE-bus command: `SENS:POW:PRES OBW`

Measurement principle:

For example, the bandwidth containing 99% of the signal power is to be determined. The routine first calculates the total power of all displayed points of the trace. In the next step, the points from the right edge of the trace are summed up until 0.5% of the total power is reached. Auxiliary marker 1 is positioned at the corresponding frequency. Then the FSP sums up the points from the left edge of the trace until 0.5% of the power is reached. Auxiliary marker 2 is positioned at this point. 99% of the power is now between the two markers. The distance between the two frequency markers is the occupied bandwidth which is displayed in the marker info field.
A prerequisite for correct measurement is that only the signal to be measured is visible on the screen of the FSP. An additional signal would invalidate the measurement.

To ensure correct power measurement especially for noise signals and to obtain the correct occupied bandwidth, the following settings should be selected:

RBW	<< occupied bandwidth (approx. 1/20 of occupied bandwidth, for voice communication type. 300 Hz or 1 kHz)
VBW	≥ 3 x RBW
Detector	RMS or sample
Span	≥2 to 3 x occupied bandwidth

Some of the measurement specifications (eg PDC, RCR STD-27B) require measurement of the occupied bandwidth using a peak detector. The detector setting of the FSP has to be changed accordingly then.

Example:
Measurement of occupied bandwidth of a PDC signal at 800 MHz, level 0 dBm

[**PRESET**]	Set the FSP to the default setting.
[**FREQ**: *CENTER*: 800 MHz]	Set the center frequency to 800 MHz.
[**AMPT**: 0 dBm]	Set the reference level to 0 dBm.
[**MEAS**]	Call the menu for the measurement functions.
[*OCCUPIED BANDWIDTH*]	Select measurement of the occupied bandwidth and open the submenu for configuring the measurement.
[% POWER BANDWIDTH: 99 **%**]	Select 99% for the bandwidth to be measured.
[*CHANNEL BANDWIDTH*: 21 **kHz**]	Enter the channel bandwidth of 21 kHz specified by PDC.
[*ADJUST SETTINGS*]	Optimize the measurement parameters for the specified channel bandwidth. Allow for a complete frequency sweep so that the FSP can determine the total signal power.
[*ADJUST REF LVL*]	Adjust the reference level to the measured signal power.
[**TRACE**: *DETECTOR*: *DETECTOR MAX PEAK*]	PDC requires measurement of the occupied bandwidth using a peak detector. Therefore, switch on the peak detector instead of the RMS detector selected by *ADJUST SETTINGS*.

Measurement of Signal Amplitude Statistics

Digital modulated signals are similar to white noise within the transmit channel, but are different in their amplitude distribution. In order to transmit the modulated signal without distortion all amplitudes of the signal have to be transmitted linearly, e. g. from the output power amplifier. Most critical are the peak amplitude values, of course.
Degradation in transmit quality caused by a transmitter two port network is dependent on the amplitude of the peak values as well as on their probability.
The probability of amplitude values can be measured with the APD function (Amplitude Probability Distribution). During a selectable measurement time all occurring amplitude values are assigned to an amplitude range. The number of amplitude values in the specific ranges is counted and the result is displayed as a histogram. Each bar of the histogram represents the percentage of measured amplitudes within the specific amplitude range.

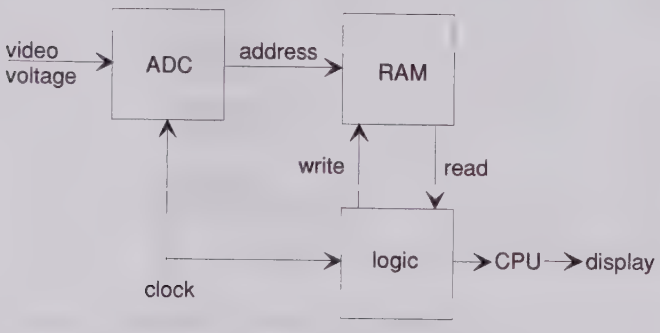

Fig. 4-8 Simplified block diagram for APD measurement

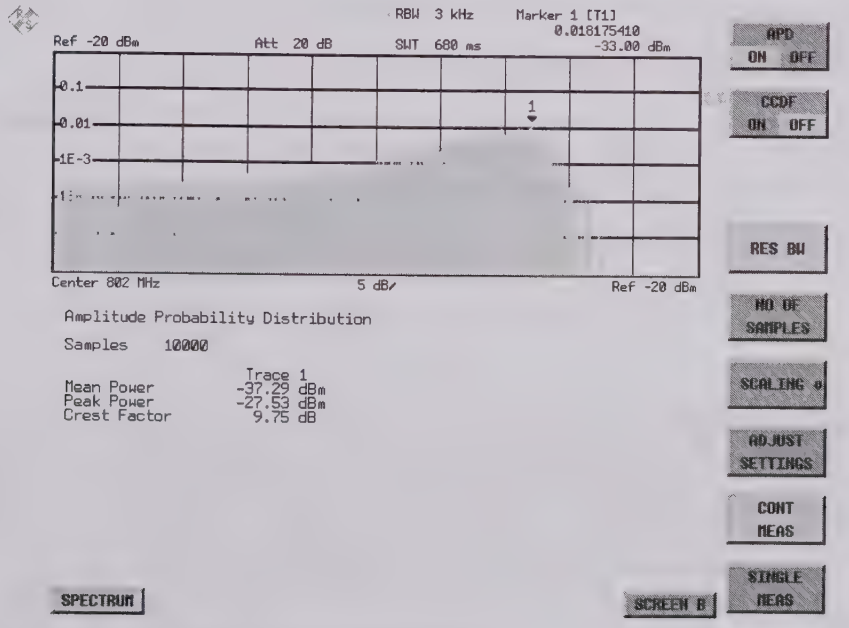

Fig. 4-9 Display of the amplitude probability distribution

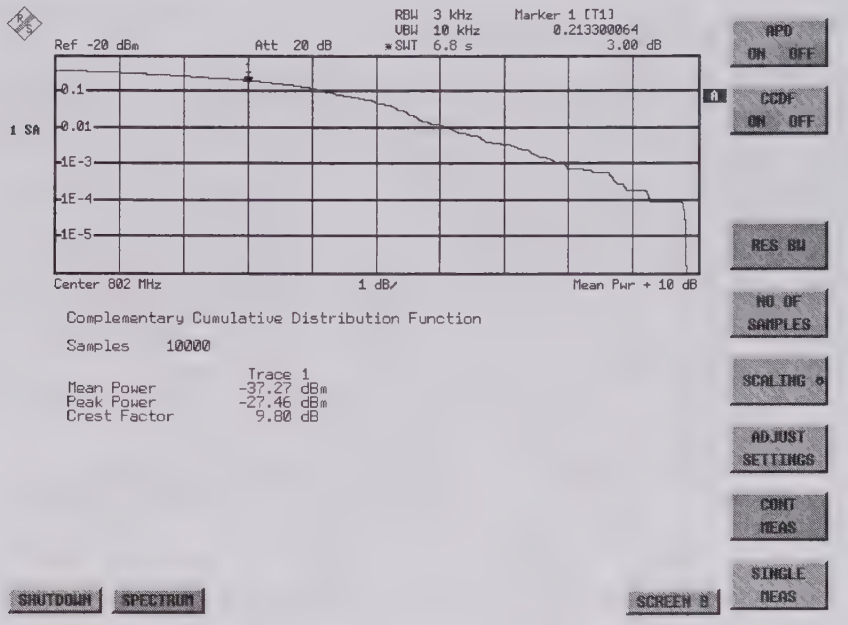

Fig. 4-10 Display of the complementary cumulative distribution function (CCDF)

Alternate to the histogram display of the APD the Complementary Cumulative Distribution Function (CCDF) can be displayed. It shows the probability of an amplitude exceeding a specific value.
For the APD function the x-axis is scaled in absolute values in dBm, whereas for the CCDF function the x-axis is scaled relative to the MEAN POWER measured.

Definitions:
Crest Factor = Peak Voltage to rms
CCDF: Complementary Cumulative Distribution Function

***Note**: During an active statistic measurement the functions FULL SCREEN, SPLIT SCREEN and selection of the active diagram via SCREEN A / SCREEN B are disabled.*

MEAS SIGNAL STATISTIC submenu :

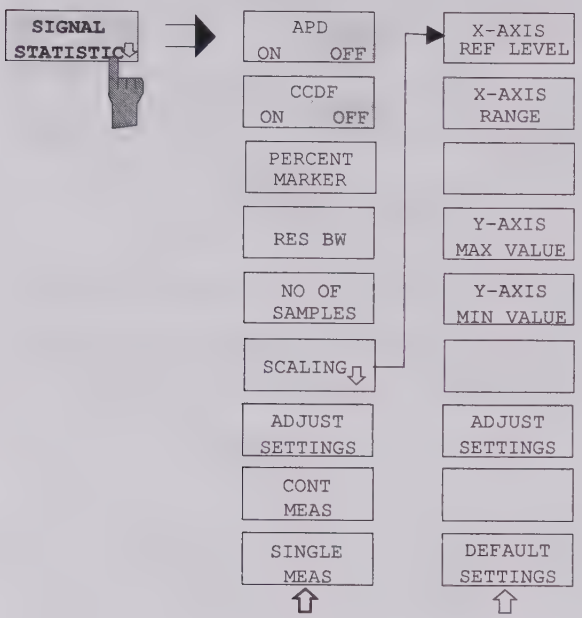

The *SIGNAL STATISTIC* softkey opens a submenu for measurement of signal statistics.
In the submenu measurement of amplitude probability density (*APD*) and complementary cumulative distribution (*CCDF*) can be selected alternately. Only one of the signal statistic functions can be switched on at a time.

In default mode all statistic functions are switched off.
With a statistic function switched on the FSP is set into zero span mode automatically.

The FSP measures the statistics of the signal applied to the RF input with the resolution bandwidth set. In order not to influence the peak amplitudes the video bandwidth is automatically set to 10 times the resolution bandwidth. The sample detector is used for detecting the video voltage.



The *APD ON/OFF* softkey switches on or off the amplitude probability distribution function.
When the APD function is switched on, the CCDF function is switched off automatically.

IEC/IEEE-bus command: `CALC:STAT:APD ON`



The *CCDF ON/OFF* softkey switches on or off the complementary cumulative distribution function.
When the CCDF function is switched on, the APD function is switched off automatically.

IEC/IEEE-bus command: `CALC:STAT:CCDF ON`



If the CCDF function is active, the *PERCENT MARKER* softkey allows to position marker 1 by entering a probability value. Thus, the power which is exceeded with a given probability can be determined very easily.
If marker 1 is in the switched-off state, it will be switched on automatically.

IEC/IEEE-bus command: `CALC:MARK:Y:PERC 0...100%`



The *RES BW* softkey sets the resolution bandwidth in the menu *STATISTIC FUNCTION* directly without switching to the corresponding menu (BW). The function of the softkey is identical to the softkey *RES BW MANUAL* in the menu *BW*.
For correct measurement of the signal statistics the resolution bandwidth has to be wider than the signal bandwidth in order to transmit the actual peaks of the signal amplitude correctly. Video bandwidth is set to 10 MHz automatically with a statistic function switched on.

IEC/IEEE-bus command: `BAND 3 MHz`

The *NO OF SAMPLES* softkey sets the number of power measurements taken into account for the statistics.
Please note that the overall measurement time is influenced by the number of samples selected as well as by the resolution bandwidth set up for the measurement as the resolution bandwidth directly influences the sampling rate.

IEC/IEEE-bus command: `CALC:STAT:NSAM <value>`

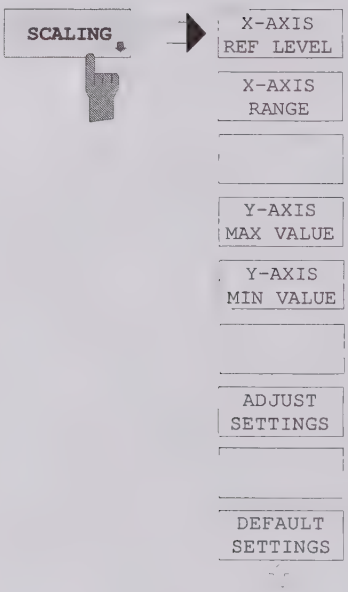

The *SCALING* softkey opens a sub menu that allows changing the scaling parameters for both the x- and the y-axis.

The *X-AXIS REF LEVEL* softkey changes the level settings of the instrument and sets the maximum power to be measured.
The function is identical to softkey *REF LEVEL* in menu *AMPT*.
For the *APD* function this value is mapped to the right diagram border. For the *CCDF* function there is no direct representation of this value on the diagram as the x-axis is scaled relatively to the *MEAN POWER* measured.

IEC/IEEE command: `CALC:STAT:SCAL:X:RLEV <value>`

The *X-AXIS RANGE* softkey changes the level range to be covered by the statistics measurement selected.
The function is identical to softkey *RANGE LOG MANUAL* in menu *AMPT*.

IEC/IEEE command: `CALC:STAT:SCAL:X:RANG <value>`

The *Y-AXIS MAX VALUE* softkey defines the upper limit of the displayed probability range.
Values on the y-axis are normalized which means that the maximum value is 1.0. As the y-axis scaling has a logarithmic axis the distance between max and min value must be at least one decade.

IEC/IEEE command: `CALC:STAT:SCAL:Y:UPP <value>`

The *Y-AXIS MIN VALUE* softkey defines the lower limit of the displayed probability range.
As the y-axis scaling has a logarithmic axis the distance between max and min value must be at least one decade. Valid values are in the range 0 < value < 1.

IEC/IEEE command: `CALC:STAT:SCAL:Y:LOW <value>`

see below

The *DEFAULT SETTINGS* softkey resets the x- and y-axis scalings to their PRESET values.

x-axis ref level:	-20 dBm
x-axis range APD:	100 dB
x-axis range CCDF:	20 dB
y-axis upper limit:	1.0
y-axis lower limit:	1E-6

IEC/IEEE-bus command: `CALC:STAT:PRES`

The *ADJUST SETTINGS* softkey optimizes the level settings of the FSP according to the measured peak power in order to gain maximum sensitivity of the instrument.
The level range is adjusted according to the measured difference between peak and minimum power for APD measurement and peak and mean power for CCDF measurement in order to obtain maximum power resolution.
Additionally the probability scale is adapted to the selected number of samples.

IEC/IEEE-bus command: `CALC:STAT:SCAL:AUTO ONCE`

The *CONT MEAS* softkey starts collecting a new sequence of sample data and calculating the APD or CCDF curve depending on the selected measurement. The next measurement is started automatically as soon as the indicated number of samples has been reached ("CONTinuous MEASurement").

IEC/IEEE-bus command:
```
INIT:CONT ON;
INIT:IMM
```

The *SINGLE MEAS* softkey starts collecting a new sequence of sample data and calculating the APD or CCDF curve depending on the selected measurement. At the beginning of the measurement previously obtained measurement results are discarded.

IEC/IEEE-bus command:
```
INIT:CONT OFF;
INIT:IMM
```

Hint for usage of the marker functions with measurement of signal statistics:

With the signal statistic measurement level always is displayed on x-axis. Y-axis always is a normalized value between 0 and 1. In contrary to use of marker in frequency or time domain marker is input in level values and the output is in percentage values.

Example:

Measurement of CCDF of a IS95 BTS signal, level 0 dBm, frequency 800 MHz

[**PRESET**]	Switch on preset settings.
[**FREQ**: *CENTER*: 800 MHz]	Set center frequency to 800 MHz.
[**AMPT**: 10 dBm]	Set reference level to 10 dBm.
[**BW**: 3 MHz]	Set resolution bandwidth to 3 MHz (resolution bandwidth shall be wider then signal bandwidth (1.25 MHz) in order to have the complete signal within the resolution bandwidth).
[**MEAS**]	Call the menu for measurement functions.
[*SIGNAL STATISTIC*]	Call the menu for signal statistics measurement.
[*CCDF ON /OFF*]	Switch on measurement of the complementary cumulative distribution function. The FSP switches to zero span mode. The power of the signal and the CCDF is calculated for the number of samples selected. With the CCDF function sample detector and video bandwidth are set automatically.
[NO OF SAMPLES: 10000]	Set the number of measurement samples to 10000.
[SINGLE MEAS]	Start the measurement sequence. At the end the resulting trace will display the CCDF for the measured 10000 samples.

Measurement of the AM Modulation Depth

The *MODULATION DEPTH* softkey switches on the measurement of the AM modulation depth. An AM-modulated carrier is required on the screen for ensuring correct operation.
The level value of *MARKER 1* is taken as the carrier level. When this function is activated, *MARKER 2* and *MARKER 3* are automatically set symmetrically to the carrier on the adjacent peak values of the trace as delta markers and *MARKER 2* is activated for the entry.
When the position of *MARKER 2* (delta) is changed, *MARKER 3* (delta) is moved symmetrically with respect to the reference marker (*MARKER 1*).
If the data entry is activated for *MARKER 3* (*MARKER 1 2 3 4* softkey), the latter can be moved for fine adjustment irrespective of *MARKER 2*.

The FSP calculates the power at the marker positions from the measured levels. The AM modulation depth is calculated from the ratio between the power values at the reference marker and at the delta markers. When the powers of the two AM side bands are unequal, the mean value of the two power values is used for AM modulation depth calculation.

Measurement example:

The AM modulation depth of a carrier modulated with 1 kHz is to be measured at 100 MHz.

[**PRESET**]	The FSP is set to the default setting.
[**CENTER**: 100 **MHz**]	The center frequency is set to 100 MHz.
[**SPAN**: 5 **kHz**]	The span is set to 5 kHz.
[**AMPT**: 0 **dBm**]	The reference level is set to 0 dBm.
[**MKR FCTN**]	*MARKER 1* is switched on and positioned at the maximum of the displayed trace.
[*MODULATION DEPTH*: 1 **kHz**]	The measurement of the AM modulation depth is switched on. *MARKERS 2* and *3* (delta markers) are set to the adjacent peak values of the trace and are activated for the frequency entry. The AM modulation depth is output in % in the marker info field. When 1 kHz is entered, *MARKER 2* can be exactly positioned on 1 kHz and *MARKER 3* at -1 kHz from the reference marker.

IEC/IEEE-bus command:

```
CALC:MARK:FUNC:MDEP ON;
CALC:MARK:FUNC:MDEP:RES?
```

Measurement of the Third Order Intercept (TOI)

If several signals are applied to a transmission twoport with nonlinear characteristic, intermodulation products appear at its output by the sums and differences of the signals. The nonlinear characteristic produces harmonics of the useful signals which intermodulate at the characteristic. The intermodulation products of lower order have a special effect since their level is largest and they are near the useful signals. The intermodulation product of third order causes the highest interference. It is the intermodulation product generated from one of the useful signals and the 2nd harmonic of the second useful signal in case of two-tone modulation.
The frequencies of the intermodulation products are above and below the useful signals. Fig. 4-11 shows intermodulation products P_{I1} and P_{I2} generated by the two useful signals P_{U1} and P_{U2}.

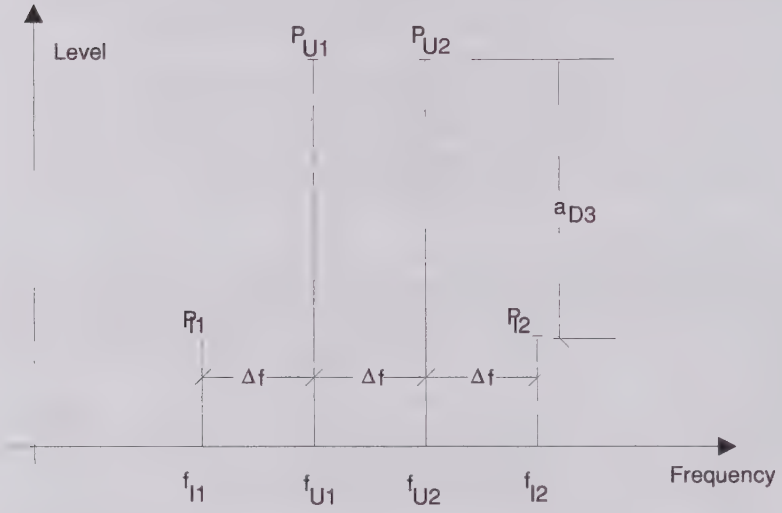

Fig. 4-11 Intermodulation products P_{U1} and P_{U2}

The intermodulation product at f_{I2} is generated by mixing the 2nd harmonic of useful signal P_{U2} and signal P_{U1}, the intermodulation product at f_{I1} by mixing the 2nd harmonic of useful signal P_{U1} and signal P_{U2}.

$f_{i1} = 2 \times f_{u1} - f_{u2}$ (1)

$f_{i2} = 2 \times f_{u2} - f_{u1}$ (2)

The level of the intermodulation products depends on the level of the useful signals. If the two useful signals are increased by 1 dB, the level of the intermodulation products increases by 3 dB, which means that spacing a_{D3} between intermodulation signals and useful signals is reduced by 2 dB. This is illustrated in Fig. 4-12.

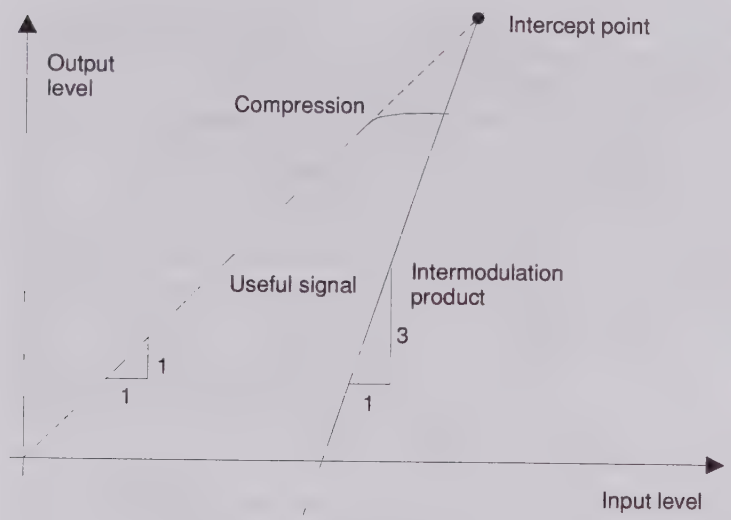

Fig. 4-12 Dependence of intermodulation level on useful signal level

The useful signals at the twoport output increase proportionally with the input level as long as the twoport is in the linear range. A level change of 1 dB at the input causes a level change of 1 dB at the output. Beyond a certain input level, the twoport goes into compression and the output level stops increasing. The intermodulation products of the third order increase three times as much as the useful signals. The intercept point is the fictitious level where the two lines intersect. It cannot be measured directly since the useful level is previously limited by the maximum twoport output power.
It can be calculated from the known line slopes and the measured spacing a_{D3} at a given level according to the following formula.

$$IP3 = \frac{a_{D3}}{2} + P_N \qquad (3)$$

The 3rd order intercept point IP3, for example, is calculated for an intermodulation of 60 dB and an input level P_U of -20 dBm according to the following formula:

$$IP3 = \frac{60}{2} + (-20dBm) = 10dBm. \qquad (4)$$



The *TOI* softkey enables the measurement of the 3rd order intercept point.
A two-tone signal with equal carrier levels is expected at the FSP input. *MARKER 1* and *MARKER 2* (both normal markers) are set to the maximum of the two signals. *MARKER 3* and *MARKER 4* (both delta markers) are placed on the intermodulation products. When the function is enabled, the frequency entry is activated for the delta markers. They can be set manually. The FSP calculates the third order intercept from the level spacing between normal markers and delta markers and outputs it in the marker info field.

IEC/IEEE-bus command:
```
CALC:MARK:FUNC:TOI ON;
CALC:MARK:FUNC:TOI:RES?
```

Example:
A two-tone signal with frequencies of 100 MHz and 101 MHz is applied to the RF input of the FSP. The level of the two signals is -10 dBm.

[**PRESET**]	The FSP is set to the default setting.
[**CENTER**: 100.5 **MHz**]	The center frequency is set to 100.5 MHz.
[**SPAN**: 3 **MHz**]	The span is set to 3 MHz.
[**AMPT**: -10 **dBm**]	The reference level is set to -10 dBm.
[*MKR FCTN*]	*MARKER 1* is switched on and set to the signal peak.
[*TOI*]	The FSP sets the 4 markers to the useful signals and the intermodulation products and calculates the third order intercept. The result is output in the marker info field.

The *SELECT MARKER* softkey activates the selection of a marker for functions *MODULATION DEPTH* and *TOI*. Thus, the markers can be fine-adjusted for these functions.
The markers are numerically selected in a data entry field. Delta marker 1 is selected by entering '0'.
If the marker is in the switch-off state, it will be switched on and can thus be shifted.

IEC/IEEE-bus command:

```
CALC:MARK1 ON;
CALC:MARK1:X <value>;
CALC:MARK1:Y?
```

Setup of Limit Lines – *LINES* Key

Limit lines are used to define amplitude curves or spectral distribution boundaries on the display screen which are not to be exceeded. They indicate, for example, the upper limits for interference radiation or spurious waves which are allowed from a Unit Under Test (UUT). For transmission of information in TDMA (e.g., GSM), the amplitude of the bursts in a time slot must adhere to a curve which must fall within a specified tolerance band. The lower and upper limits may each be specified by a limit line. Then, the amplitude curve can be controlled either visually or automatically for any violations of the upper or lower limits (GO/NOGO test).
The instrument supports limit lines with a maximum of 50 data points. 8 of the limit lines stored in the instrument can be used simultaneously and activated in the split-screen mode either in Screen A, Screen B or in the two windows. The number of limit lines stored in the instrument is only limited by the capacity of the flashdisk used.

For each limit line, the following characteristics must be defined:

- The name of the limit line. The limit line data are stored under this name and can be examined in the table *LIMIT LINES.*
- The domain in which the limit line is to be used. Here, a distinction is made between the time domain (span = 0 Hz) and the frequency domain (span > 0 Hz).
- The reference of the interpolation points to the X-axis. The limit line may be specified either for absolute frequencies or times or for frequencies which are related to the set center frequency and times related to the time on the left edge of the diagram.
- The reference of the interpolation points to the Y-axis. The limit line can be selected either for absolute levels or voltages or referred to the set maximum level (Ref Lvl). The position on the display depends on the REF LEVEL POSITION.
- With relative reference values for the Y axis, it is possible to enter an absolute threshold (THRESHOLD) which lowers the relative limit values (see below).
- The type of limit line (upper or lower limit). With this information and the active limit checking function (Table LIMIT LINES, column *LIMIT CHECK*), the FSP checks for compliance with each limit.
- The limit line units to be used. The units of the limit line must be compatible with the level axis in the active measurement window.
- The measurement curve (trace) to which the limit line is assigned. For the FSP, this defines the curve to which the limit is to be applied when several traces are simultaneously displayed.
- For each limit line, a margin can be defined which serves as a threshold for automatic evaluation.
- In addition, commentary can be written for each limit line, e.g., a description of the application.

LINES menu

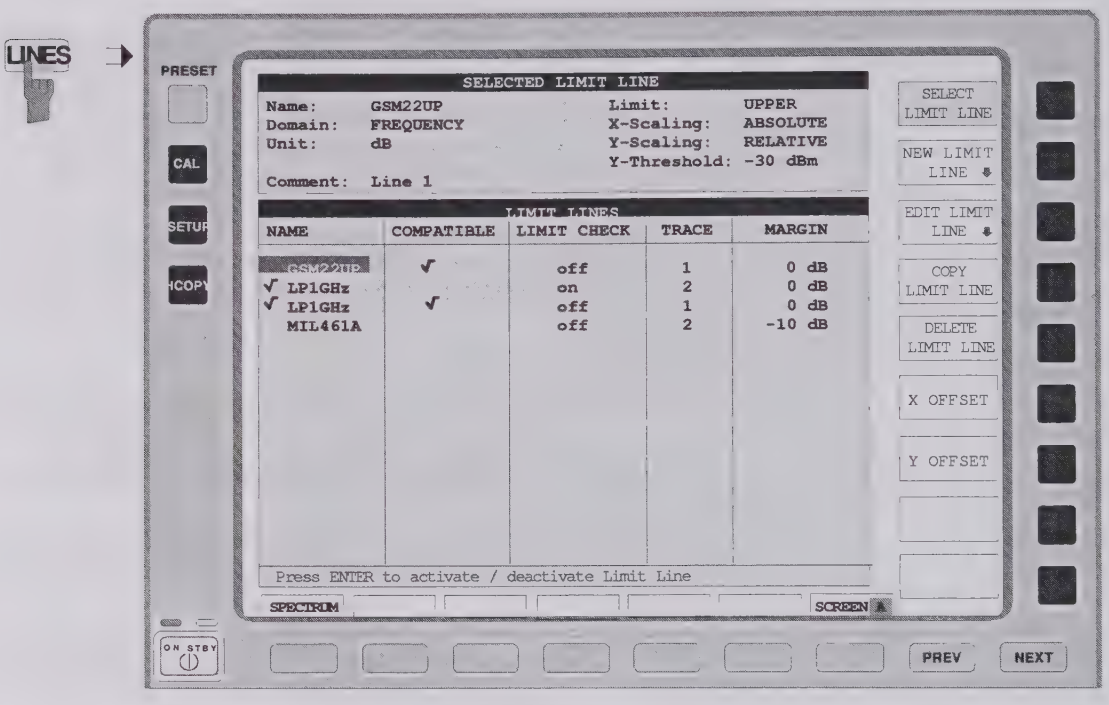

The *LINES* key calls up the menu for setup of the limit lines.

The *SELECTED LIMIT LINE* display field provides information concerning the characteristics of the marked limit lines.

In the *LIMIT LINES* table, the limit lines compatible to the settings of the active screen can be enabled.

New limit lines can be specified and edited in the *NEW LIMIT LINE and EDIT LIMIT LINE* sub-menus, respectively.

Limit Line Selection

LINES menu

The *SELECTED LIMIT LINES* table provides information about the characteristics of the marked limit line :

Name	name
Domain	frequency or time
Unit	vertical scale
Limit	upper/lower limit
X-Scaling	absolute or relative frequencies/times
Y-Scaling	absolute or relative Y-units
Threshold	absolute limit with relative Y-units
Comment	commentary

The characteristics of the limit line are set in the *EDIT LIMIT LINE (=NEW LIMIT LINE)* sub-menu.



The *SELECT LIMIT LINE* softkey activates the *LIMIT LINES* table and the selection bar jumps to the uppermost name in the table.

The following information is offered in the columns of the table:

Name	Enable the limit line.
Compatible	Indicates if the limit line is compatible with the measurement window of the given trace.
Limit Check	Activate automatic violation check for upper/lower limits.
Trace	Select the measurement curve to which the limit is assigned.
Margin	Define margin.

Name and Compatible - Enabling limit lines

A maximum of 8 limit lines can be enabled at any one time. In split screen mode, they may be assigned to screen A, screen B or to both screens. A check mark at the left edge of a cell indicates that this limit line is enabled.
A limit line can only be enabled when it has a check mark in the *Compatible* column, i.e., only when the horizontal display (time or frequency) and vertical scales are ***identical*** to those of the display in the measurement window.
Lines with the unit dB are compatible to all dB(..) settings of the Y-axis.

If the scale of the y-axis or the domain (frequency or time axis) are changed, all non-compatible limit lines are automatically switched off in order to avoid misinterpretation. The limit lines must be enabled anew when the original display is re-displayed.

IEC/IEEE-bus command:

```
CALC:LIM3:NAME "GSM1"
CALC:LIM3:UPP:STAT ON
CALC:LIM4:LOW:STAT ON
```

***Limit Check* - Activate automatic limit violation check**

When *LIMIT CHECK ON* is activated, a GO/NOGO test is performed in the active screen. In the center of the diagram, a display window appears which indicates the results of the limit check test:

LIMIT CHECK: PASSED — No violations of active limits.

LIMIT CHECK: FAILED — One or more active limit lines were violated. The message contains the names of the limit lines which were violated or whose margins were not complied with.

LIMIT CHECK: MARGIN — The margin of at least one active limit lines was not complied with, however, no limit line was violated. The message contains the names of the limit lines whose margins were not complied with.

The following example shows two active limit lines:

```
LIMIT CHECK: FAILED

LINE VHF_MASK: Failed
LINE UHF2MASK: Margin
```

A check for violations of limit lines takes place only if the limit line of the assigned measurement curve (trace) is enabled.
If *LIM CHECK* is set to *OFF* for all active limit lines, then the limit line check is not executed and the display window is activated.

IEC/IEEE-bus command:

```
CALC:LIM:STAT ON
INIT;*WAI
CALC:LIM:FAIL?
```

***Trace* - Select the measurement curve to which the limit line is assigned.**

The selection of the measurement curve (trace) takes place in an entry window. Allowed are the integer entries 1, 2 or 3. The default setting is trace 1. If the selected limit line is not compatible with the assigned measurement curve, then the limit line is disabled (display and limit check).

IEC/IEEE-bus command:

```
CALC:LIM:TRAC 1
```



See following Section "Entry and Editing of Limit Lines".



The *COPY LIMIT LINE* softkey copies the data file describing the marked limit line and saves it under a new name. In this way, a new limit line can be easily generated by parallel translation or editing of an existing limit line. The name can be arbitrarily chosen and input via an entry window (max. of 8 characters).

IEC/IEEE-bus command: `CALC:LIM3:COPY 2` or
`CALC:LIM3:COPY "GSM2"`



The *DELETE LIMIT LINE* softkey erases the selected limit line. Before deletion, a message appears requesting confirmation.

IEC/IEEE-bus command: `CALC:LIM3:DEL`



The *X OFFSET* softkey horizontally shifts a limit line, which has been specified for relative frequencies or times (X-axis). The softkey opens an entry window, where the value for shifting may be entered numerically or via the roll-key.

Note: *When changing the start or stop frequencies, the line on the display is only retained, if SPAN FIXED is set.*

IEC/IEEE-bus command: `CALC:LIM3:CONT:OFFS 10kHz`



The *Y OFFSET* softkey vertically shifts a limit line, which has relative values for the Y-axis (levels or linear units such as volt). The softkey opens an entry window where the value for shifting may be entered numerically or via the roll-key.

IEC/IEEE-bus command: `CALC:LIM3:LOW:OFFS 3dB`
`CALC:LIM3:UPP:OFFS 3dB`

Entry and Editing of Limit Lines

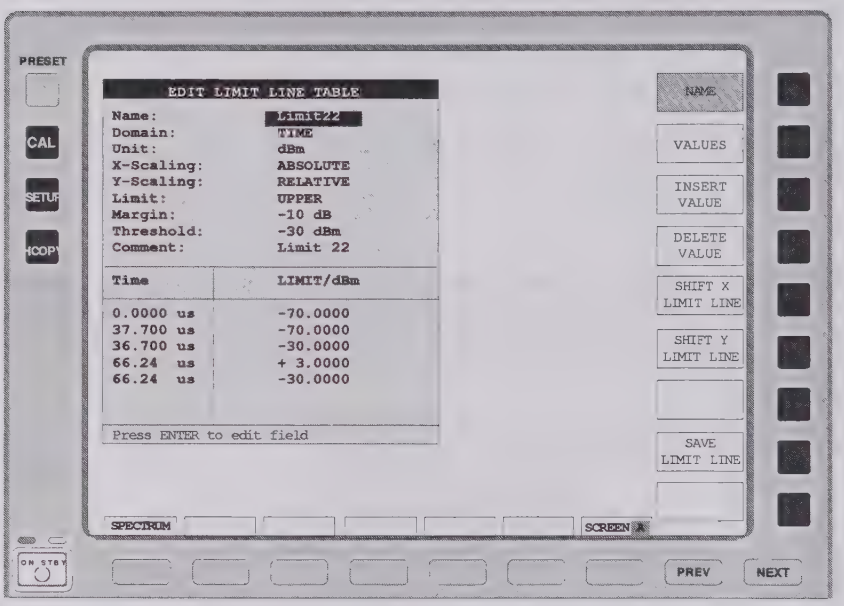

A limit line is characterized by

- its name
- the assignment of domain (frequency or time)
- the scaling in absolute or relative times or frequencies
- the vertical unit
- the vertical scaling
- the vertical threshold (only with relative vertical scaling)
- the margin
- the definition of the limit line as either upper or lower limit.
- the data points for frequency/time and level

At the time of entry, the FSP immediately checks that all limit lines are in accordance with certain guidelines. These guidelines must be observed if specified operation is to be guaranteed.

- The frequencies/times for each data point must be entered in ascending order, however, for any single frequency/time, two data points may be input (vertical segment of a limit line).

  The data points are allocated in order of ascending frequency/time. Gaps are not allowed. If gaps are desired, two separate limit lines must be defined and then both enabled.

- The entered frequencies/times must not necessarily be selectable in FSP. A limit line may also exceed the specified frequency or time domains. The minimum frequency for a data point is -200 GHz, the maximum frequency is 200 GHz. For the time domain representation, negative times may also be entered. The allowable range is -1000 s to +1000 s.

- The minimum/maximum value for a limit line is -200 dB to +200 dB for the logarithmic or 10^{-20} to 10^{+20} or -99.9% to + 999.9% for the linear amplitude scales.

LINES - EDIT LIMIT LINE menu

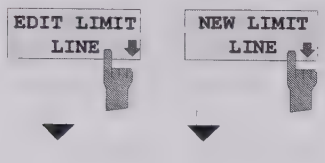

The *EDIT LIMIT LINE* and *NEW LIMIT LINE* softkeys both call the *EDIT LIMIT LINE* sub-menu used for editing limit lines. In the table heading, the characteristics of the limit line can be entered. The data points for frequency/time and level values are entered in the columns.

Name	Enter name.
Domain	Select domain.
Unit	Select units.
Limit	Select upper and lower limit value.
X-Scaling	Entry of absolute or relative values for the X-axis
Y-Scaling	Entry of absolute or relative values for the Y-axis
Margin	Entry of margin.
Threshold	Entry of vertical threshold (only with relative vertical scaling)
Comment	Enter comments.
Time/Frequency	Enter time/frequency for the data points.
Limit/dBm	Enter magnitudes for the data points.

Note: *Domain, unit, X scaling and Y scaling cannot be modified as soon as reference values have been entered in the data section of the table.*



The *NAME* softkey enables the entry of characteristics in the table heading.

***Name* - Enter name**

A maximum of 8 characters is permitted for each name. All names must be compatible with the MS DOS conventions for file names. The instrument stores all limit lines with the .LIM extension.

IEC/IEEE-bus command: `CALC:LIM3:NAME "GSM1"`

***Domain* - Select time or frequency domain**

The default setting is frequency.
A change in domain (frequency/time) is only permitted when the data point table is empty.

IEC/IEEE-bus command: `CALC:LIM3:CONT:DOM FREQ`

***Scaling* - selection of absolute or relative scaling**

The limit line can either be scaled in absolute (frequency or time) or relative units. Any of the unit keys may be used to toggle between *ABSOLUTE* and *RELATIVE*, the cursor must be positioned in the X-*Scaling* or the *Y-Scaling* line

X-Scaling ABSOLUTE The frequencies or times are interpreted as absolute physical units.

X-Scaling RELATIVE In the data point table, the frequencies are referred to the currently set center frequency. In time domain mode, the left boundary of the diagram constitutes the reference.

Y-Scaling ABSOLUTE The limit values refer to absolute levels or voltages.

Y-Scaling RELATIVE The limit values refer to the reference level (Ref Level) or, in case a reference line is set, to the reference line.
Limit values with the unit dB are always relative values.

The *RELATIVE* scaling is always suitable, if masks for bursts are to be defined in the time domain, or if masks for modulated signals are required in the frequency domain.
An X-offset with half the sweep time may be entered in order to shift the mask in the time domain into the center of screen.

IEC/IEEE-bus command:
```
CALC:LIM3:CONT:MODE ABS
CALC:LIM3:UPP:MODE ABS
CALC:LIM3:LOW:MODE ABS
```

***Unit* - Select the vertical scale units for the limit line**

The selection of units takes place in a selection box. The default setting is dBm.

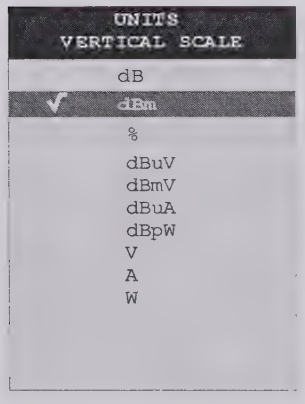

IEC/IEEE-bus command: `CALC:LIM3:UNIT DBM`

***Limit* - Select upper/lower limit**

A limit line can be defined as either an upper or lower limit.

IEC/IEEE-bus command: --
`(defined by key words :UPPer or :LOWer)`

***Margin* - Setting a margin.**

The margin is defined as the signal-level distance to the limit line . When the limit line is defined as an upper limit, the margin means that the level is below the limit line. When the limit line is defined as a lower limit, the margin means that the level is above the limit line. The default setting is 0 dB (i.e., no margin).

IEC/IEEE-bus command:
```
CALC:LIM3:UPP:MARG 10dB
CALC:LIM3:LOW:MARG 10dB
```

***Threshold* – Selection of the threshold value with relative Y scaling**

With relative Y scaling, an absolute threshold value can be defined which lowers the relative limit values. The function is useful especially for mobile radio applications provided the limit values are defined in relatíon to the carrier power as long as they are above an absolute limit value.

Example:

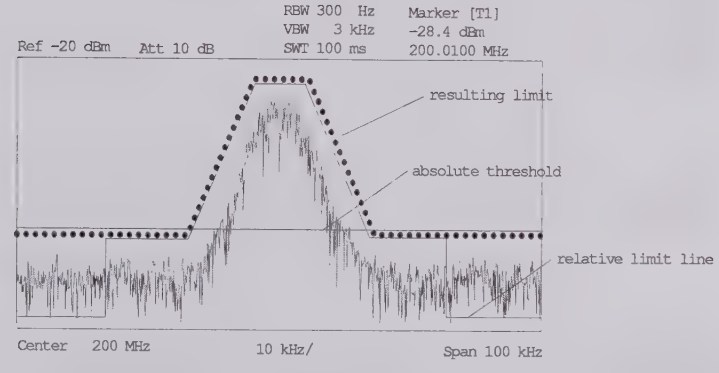

The preset value is at -200 dBm. The field is displayed if the value RELATIVE is entered in the field Y-SCALING.

IEC/IEEE-bus command:
```
CALC:LIM3:UPP:THR -30 dBm
or
CALC:LIM3:LOW:THR -30 dBm
```

***Comment* - Enter comments**

Comments are arbitrary, however, they must be less than 41 characters long.

IEC/IEEE-bus command:
```
CALC:LIM3:COMM "Upper limit"
```

The *VALUES* softkey activates the entry of the data points in the table columns *Time/Frequency* and *Limit/dB*. Which table columns appear depends upon the *Domain* selection in the table heading.

The desired frequency/time data points are entered in ascending order (two repeated frequencies/time values are permitted).

IEC/IEEE-bus command:
```
CALC:LIM3:CONT:DATA 1MHz,3MHz,30MHz
CALC:LIM3:UPP:DATA -10,0,0
CALC:LIM3:LOW:DATA -30,-40,-40
```

The *INSERT VALUE* softkey creates an empty line above the current cursor position where a new data point may be entered. However, during the entry of new values, it is necessary to observe an ascending order for frequency/time.

IEC/IEEE-bus command: `--`

The *DELETE VALUE* softkey erases the data point (complete line) at the cursor position. All succeeding data points are shifted down accordingly.

IEC/IEEE-bus command: `--`

The *SHIFT X LIMIT LINE* softkey calls an entry window where the complete limit line may be shifted parallel in the horizontal direction.

The shift takes place according to the horizontal scale:

– in the frequency domain in Hz, kHz, MHz or GHz

– in the time domain in ns, µs, ms or s

In this manner, a new limit line can be easily generated based upon an existing limit line which has been shifted horizontally and stored (*SAVE LIMIT LINE* softkey) under a new name (*NAME* softkey).

IEC/IEEE-bus command: `CALC:LIM3:CONT:SHIF 50KHz`



The *SHIFT Y LIMIT LINE* softkey calls an entry window where the complete limit line may be shifted parallel in the vertical direction.

The shift takes place according to the vertical scale:

– for logarithmic units, relative, in dB

– for linear units, as a factor

In this manner, a new limit line can be easily generated based upon an existing limit line which has been shifted vertically and stored (*SAVE LIMIT LINE* softkey) under a new name (*NAME* softkey).

IEC/IEEE-bus command:
```
CALC:LIM3:CONT:UPP:SHIF 20dB
CALC:LIM3:CONT:LOW:SHIF 20dB
```



The *SAVE LIMIT LINE* softkey stores the currently edited limit line . The name can be entered in an input window (max. 8 characters)

IEC/IEEE-bus command: `--`

Configuration of Screen Display – *DISP* Key

The *DISPLAY* menu allows the configuration of the diagram display on the screen and also the selection of the display elements and colors. The *POWER SAVE* mode is also configured in this menu for the display.

The test results are displayed on the screen of the FSP either in a full-screen window or in two overlapping windows. The two windows are called diagram A and diagram B.

In the default setting, the two windows are completely decoupled from each other, ie they behave like two separate instruments. This is very useful, for example with harmonics measurements or measurements on frequency-converting DUTs, since the input signal and the output signal lie in different frequency ranges.

However, specific settings of the two windows (reference level, center frequency) can be coupled, if required, so that with *CENTER B = MARKER A* for example, the shift of the marker in diagram A causes the frequency range (zoomed in some cases) to be shifted along diagram B.

New setttings are performed in the diagram selected via hotkey SCREEN A or SCREEN B. If only one window is displayed, it is the diagram in which the measurements are performed; the diagram not displayed is not active for measurements.

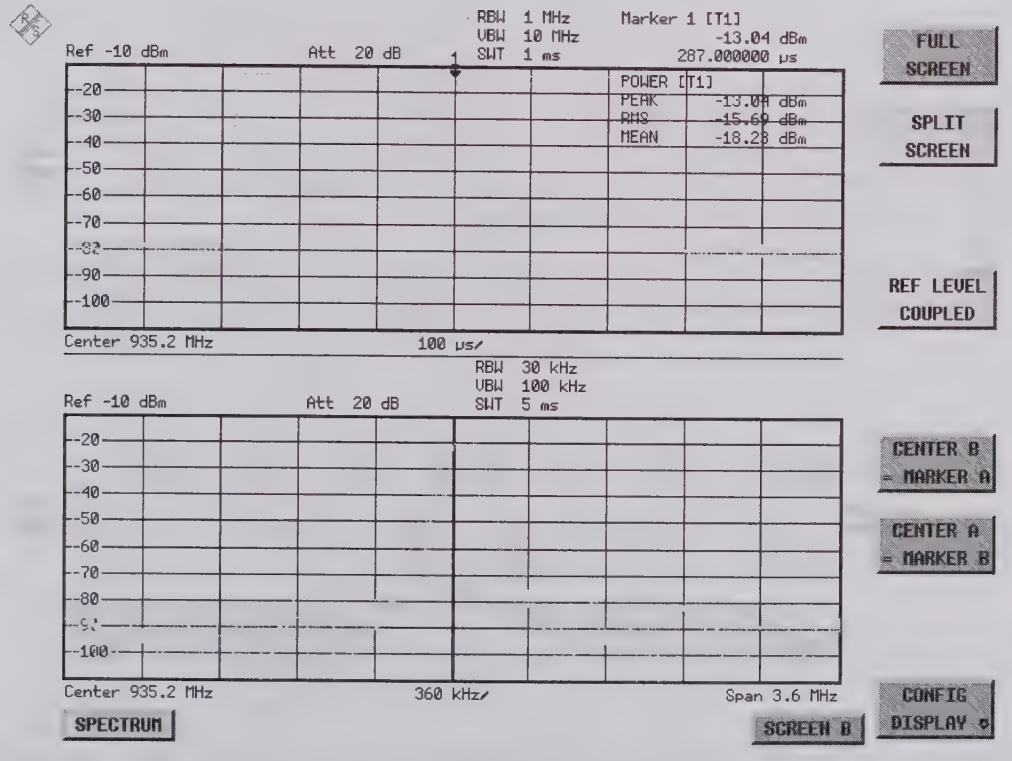

Fig. 4-12 Typical split-screen display, settings are uncoupled

The *DISP* key opens the menu for configuring the screen display and selecting the active diagram in SPLIT SCREEN mode.

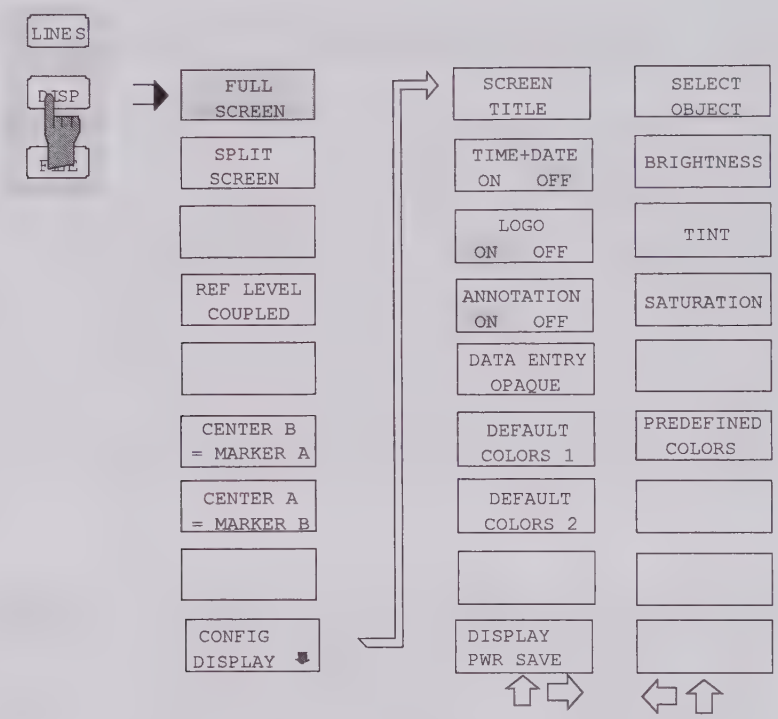



The *FULL SCREEN* softkey selects the display of one diagram. This corresponds to the default setting of FSP.

In the *FULL SCREEN* mode it is possible to switch between two different device settings by selecting the active window (screen A or screen B).
Switching between *SCREEN A* and *SCREEN B* is performed by means of the corresponding key in the *HOTKEY bar*.

It should be noted that the measurements in the FULL SCREEN mode are performed only in the visible (active) window.

The active window is marked by **A** or **B** on the right of the diagram.

IEC/IEEE-bus command:
```
DISP:FORM SING
DISP:WIND<1|2>:SEL
```



The *SPLIT SCREEN* softkey selects the display of two diagrams. The upper diagram is designated *SCREEN A*, the lower diagram *SCREEN B*.

Switching between *SCREEN A* and *SCREEN B* is performed via the corresponding key in the *HOTKEY* bar. The active window is marked by highlighting fields **A** and **B** on the right of the diagram.

IEC/IEEE-bus command:
```
DISP:FORM SPL
```

The *REF LEVEL COUPLED* softkey switches the coupling of the reference level on and off. In addition to the reference level, the mixer level and input attenuation are coupled with one another.

For the level measurement, the same reference level and input attenuation must be set for the two diagrams.

IEC/IEEE-bus command `INST:COUP RLEV`



The *CENTER B = MARKER A and CENTER A = MARKER B* softkeys couple the center frequency in diagram B with the frequency of marker 1 in diagram A and the center frequency in diagram B with the frequency of marker 1 in diagram B. The two softkeys are mutually exclusive.
This coupling is useful, eg for viewing the signal at the marker position in diagram A with higher frequency resolution or in the time domain in diagram B.
If marker 1 is off, it is switched on and set to the maximum of the trace in the active diagram.

IEC/IEEE-bus command:
```
INST:COUP CF_B
INST:COUP CF_A
```

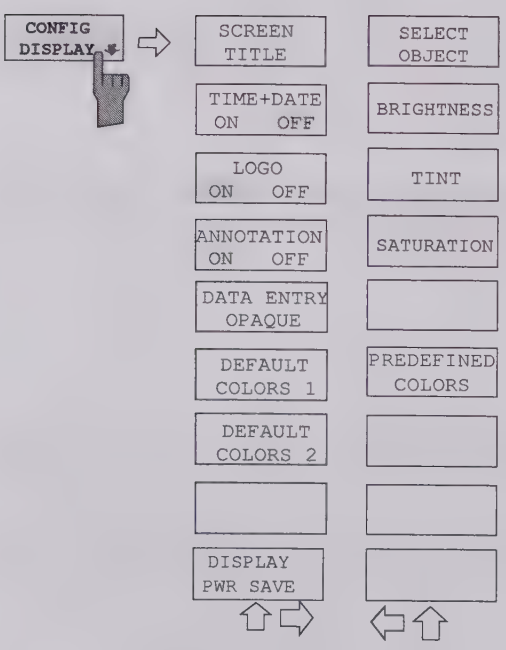

The CONFIG DISPLAY softkey opens a submenu allowing additional display items to be added to the screen. In addition, the display power-save mode (*DISPLAY PWR SAVE*) and the colors of the display elements can be set here.

The *SCREEN TITLE* softkey activates the entry of a title for the active diagram A or B. It switches on or off a title that is already input. The length of the title is limited to max. 20 characters.

IEC/IEEE-bus command:
```
DISP:WIND1:TEXT 'Noise Meas'
DISP:WIND1:TEXT:STATe ON
```

The *TIME+DATE ON/OFF* softkey switches on or off the display of date and time above the diagram.

IEC/IEEE-bus command:
```
DISP:TIME OFF
```

The *LOGO ON/OFF* softkey switches the Rohde & Schwarz company logo displayed in the upper left corner of the display screen on or off.

IEC/IEEE-bus command:
```
DISP:LOGO ON
```

The *ANNOTATION ON/OFF* softkey switches the displaying of frequency information on the screen on and off.

ON Frequency information is displayed.

OFF Frequency information is not outputted to the display. This can be used for example to protect confidential data.

IEC/IEEE-bus command:
```
DISP:ANN:FREQ ON
```

The *DATAENTRY OPAQUE* softkey sets the data entry windows to opaque. This means that entry windows are underlayed with the background color for tables.

IEC/IEEE-bus command: `--`



The *DEFAULT COLORS 1 and 2* softkey restores the default settings for brightness, color tint and color saturation for all display screen elements.
The color schemes have been selected to give optimum visibility of all picture elements at an angle of vision from above or below. *DEFAULT COLORS 1* is active in the default setting of the instrument.

IEC/IEEE-bus command:
```
DISP:CMAP:DEF1
DISP:CMAP:DEF2
```

The *DISPLAY PWR SAVE* softkey is used to switch on/off the power-save mode for the display and to enter the time for the power-save fuction to respond. After the elapse of this time the display is completely switched off, ie including backlighting.

Note: *This mode is recommended for saving the TFT display especially when the instrument is exclusively operated in remote control.*

The power-save mode is configured as follows:

- The first keystroke activates the power-save mode and opens the editor for the response time (*POWER SAVE TIMEOUT*). The response time is entered in minutes between 1 and 6 minutes and is confirmed by *ENTER*.
- The power-save mode is deactivated by pressing the key again.

On leaving the menu with the power-save mode in the activated state, the softkey is highlighted in color on returning to the menu and opens again the editor for the response time. Pressing again the key switches off the power-save mode.

IEC/IEEE-bus command: `DISP:PSAV ON`
`DISP:PSAV:HOLD 15`

The *SELECT OBJECT* softkey activates the *SELECT DISPLAY* OBJECT table, with which a graphics element can be selected. After selection, the brightness, tint and saturation of the selected element can be changed using the softkeys of the same name. The color changes by means of the *PREDEFINED COLORS* softkey can be seen immediately on the display screen.

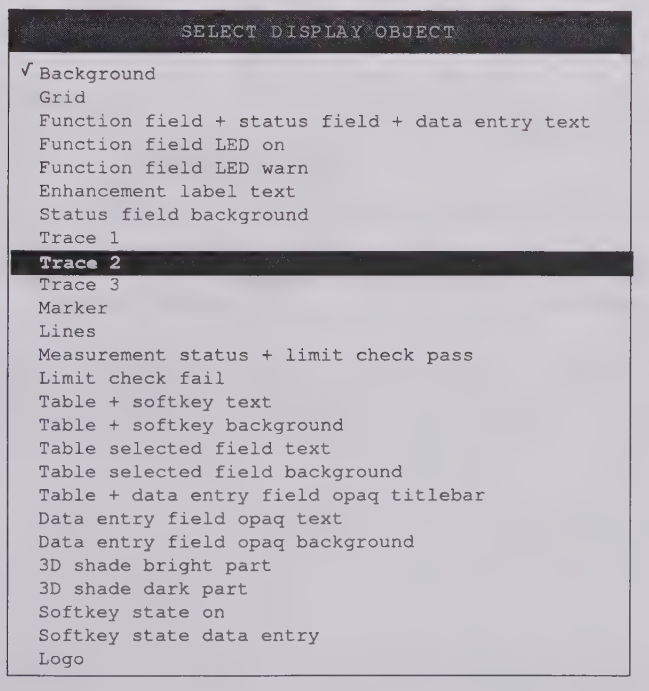

The *BRIGHTNESS* softkey activates entry of the brightness of the selected graphics element.

Values between 0 and 100% can be entered.

IEC/IEEE-bus: `DISP:CMAP3:HSL< hue>,<sat>,<lum>`

The *TINT* softkey activates the entry of the color tint of the selected element. The entered value is related to a continuous color spectrum ranging from red (0%) to blue (100%).

IEC/IEEE-bus: `DISP:CMAP3:HSL <hue>,<sat>,<lum>`

The *SATURATION* softkey activates the entry of the color saturation for the selected element.

The range of inputs is from 0 to 100%.

IEC/IEEE-bus: `DISP:CMAP3:HSL <hue>,<sat>,<lum>`

The *PREDEFINED COLORS* softkey activates a table, with which the predefined colors for the diplay screen elements can be selected.

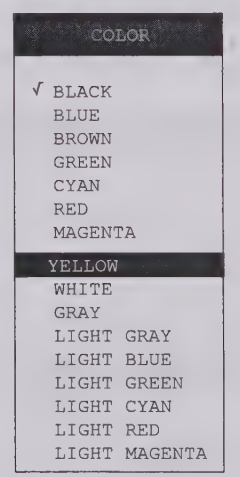

IEC/IEEE-bus command: `DISP:CMAP1 to 26:PDEF <color>`

Instrument Setup and Interface Configuration – *SETUP* Key

The *SETUP* key opens the menu for configuration of the FSP:

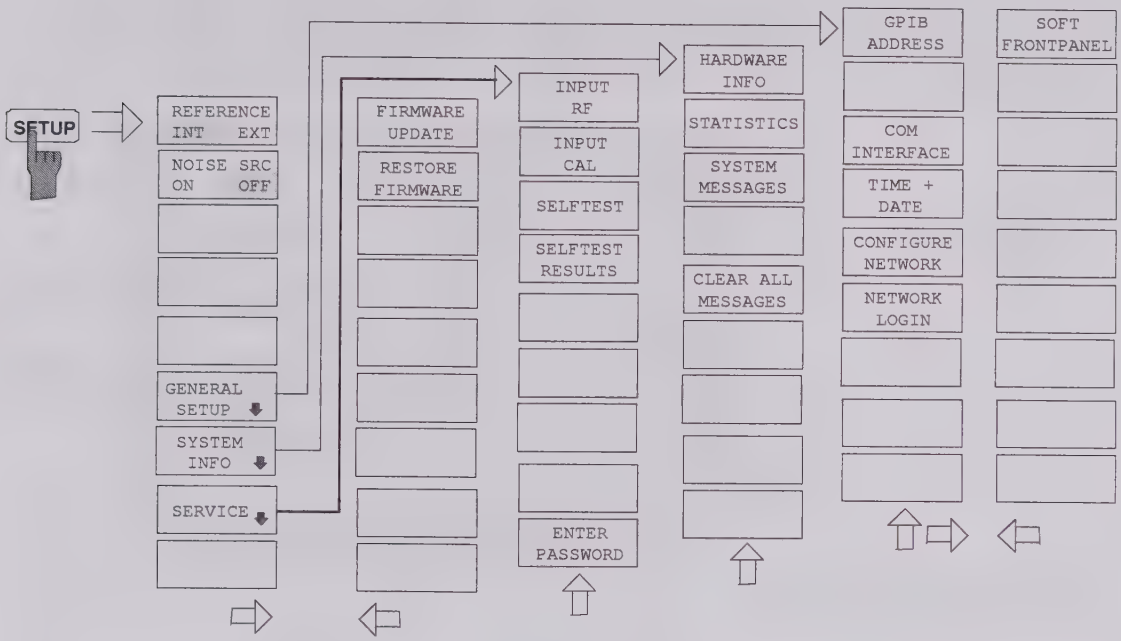

The following settings can be modified here:

- The *REFERENCE INT/EXT* softkey determines the source of the reference
- The *NOISE SRC ON/OFF* softkey switches on and off the voltage supply for an external noise source.
- The *GENERAL SETUP* softkey opens a submenu for all the general settings such as IEC/IEEE-bus address, date and time as well as the configuration of the device interfaces. *FIRMWARE OPTIONS* can be installed under this menu item.
- The *SYSTEM INFO* softkey opens a submenu for displaying the hardware configuration of the instrument, the switching cycle statistics and system messages.
- The *SERVICE* softkey opens a submenu in which special device functions and system information can be selected for servicing. The password required for service functions can be entered in this submenu.
- The *SERVICE FUNCTIONS* softkey enables additional special settings for servicing and troubleshooting. It is available after entering the corresponding password under the *SERVICE* softkey.

External Reference Oscillator

The FSP can use the internal reference source or an external reference source as frequency standard from which all internal oscillators are derived. A 10 MHz crystal oscillator is used as internal reference source. In the default setting (internal reference), this frequency is available as output signal at rear-panel connector REF OUT, eg to synchronize other instruments to the reference of the FSP.
In the setting *REFERENCE EXT*, the connector REF IN is used as input connector for an external frequency standard. In this case all internal oscillators of the FSP are synchronized to the external reference frequency (also 10 MHz).

SETUP menu:

The *REFERENCE INT / EXT* softkey switches between the internal and external reference.

Note: *If the reference signal is missing when switching to external reference, the message "LOUNL" appears after a while to indicate that there is no synchronization.*
On switching to internal reference ensure that the external reference signal is de-activated to avoid interactions with the internal reference signal.

IEC/IEEE-bus command: `ROSC:SOUR INT`

External Noise Source

SETUP menu:

The *NOISE SRC ON/OFF* softkey switches on or off the supply voltage for an external noise source which is connected to the *NOISE SOURCE* connector on the rear panel of the instrument.

IEC/IEEE-bus command: `DIAG:SERV:NSO ON`

RF Preamplifier

To improve the noise figure, a low-noise preamplifier with variable gain at the RF input can be switched into the signal path.
SETUP menu:



The *PREAMP* softkey switches the preamplifier on and activates the entry of the preamplifier gain. The preamplifier is switched off by pressing the softkey again.
The only possible value with option el. attenuator is 20 dB.

IEC/IEEE-bus command: `INP:GAIN 0DB`

Note: The PREAMP softkey is only available with option *EL. ATTENUATOR FSP-B25.*

Programming the Interface Configuration and Time Setup

The *GENERAL SETUP* softkey opens a sub-menu in which the general instrument parameters can be set up. In addition to the configuration of the digital interfaces (*IECBUS, COM*), the date and time may be entered.

The current settings are displayed in tabular form on the display screen where they may be edited.

SETUP - GENERAL SETUP submenu:

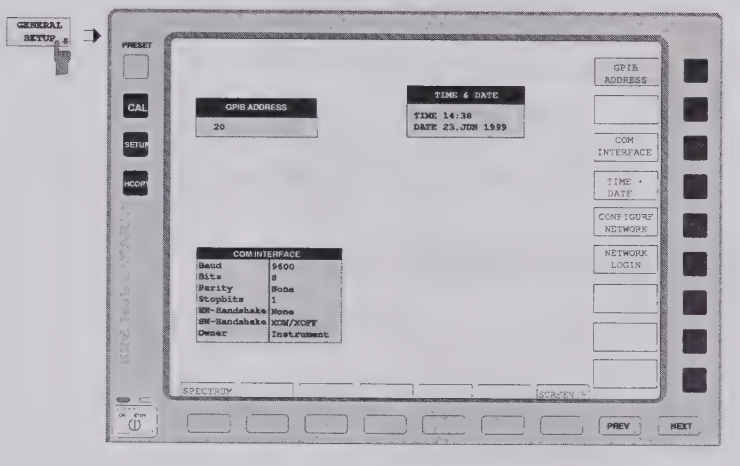

Selecting the IEC/IEEE-bus address

SETUP - GENERAL SETUP submenu:



The *GPIB ADDRESS* softkey activates the entry of the IEC Bus address.

Valid addresses are 0 through 30. The default setting is address 20.

IEC/IEEE-bus command: `SYST:COMM:GPIB:ADDR 20`

Serial Interface Configuration

SETUP-GENERAL SETUP submenu:

The *COM INTERFACE* softkey activates the *COM INTERFACE* table for entry of the serial interface parameters.

The following parameters can be configured in the table:

Baud rate	data transmission rate
Bits	number of data bits
Parity	bit parity check
Stop bits	number of stop bits
HW-Handshake	hardware handshake protocol
SW-Handshake	software handshake protocol
Owner	assignment to the measuring instrument or computer

COM INTERFACE	
Baud	9600
Bits	8
Parity	None
Stopbits	1
HW-Handshake	None
SW-Handshake	XON/XOFF
Owner	Instrument

Baud – Data transmission rate

The FSP supports baud rates between 110 and 19200 baud. The default setting is 9600 baud.



IEC/IEEE-bus command: `SYST:COMM:SER:BAUD 9600`

Bits – Number of data bits per word

For the transmission of text without special characters, 7 bits are adequate. For binary data as well as for text with special characters, 8 bits must be selected (default setting).



IEC/IEEE-bus command: `SYST:COMM:SER:BITS 7`

***Parity* – Bit parity check**

NONE	no parity check (default setting)
EVEN	even parity check
ODD	odd parity check

IEC/IEEE-bus command: `SYST:COMM:SER:PAR NONE`

***Stop bits* – Number of stop bits**

Available are 1 and 2. The default setting is 1 stop bit.



IEC/IEEE-bus command: `SYST:COMM:SER:SBIT 1`

***HW-Handshake* – Hardware handshake protocol**

The integrity of data transmission can be improved by the use of a hardware handshake mechanism, which effectively prevents uncontrolled transmission of data and the resulting loss of data bytes. For hardware handshake additional interface lines are used to transmit acknowledge signals with which the data transmission can be controlled and, if necessary, stopped until the receiver is ready to receive data again.

A prerequisite for using hardware handshaking is, however, that the interface lines (DTR and RTS) are connected on both transmitter and receiver. For a simple 3-wire connection, this is not the case and hardware handshake cannot be used here.

Default setting is *NONE*.



IEC/IEEE-bus command:
`SYST:COMM:SER:CONT:DTR OFF`
`SYST:COMM:SER:CONT:RTS OFF`

***SW-Handshake* – Software handshake protocol**

Besides the hardware handshake mechanism using interface lines, it is also possible to achieve the same effect by using a software handshake protocol. Here, control bytes are transmitted in addition to the normal data bytes. These control bytes can be used, as necessary, to stop data transmission until the receiver is ready to receive data again.

In contrast to hardware handshaking, software handshaking can be realized even for a simple 3-wire connection.

One limitation is, however, that software handshaking cannot be used for the transmission of binary data, since the control characters XON and XOFF require bit combinations that are also used for binary data transmission.

Default setting is *NONE*.

IEC/IEEE-bus command: `SYST:COMM:SER:PACE NONE`

***Owner* – Assignment of the interface**

The serial interface can be assigned alternatively to the measuring instrument section or to the computer section

If the interface is assigned to one section of the instrument, it is not available to the other section.

INSTRUMENT The interface is assigned to the measuring instrument section. Outputs to the interface from the computer section are not possible will get lost.

OS The interface is assigned to the computer section. It cannot be used by the measuring instrument section. This means that remote control of the instrument via the interface is not possible.



IEC/IEEE-bus command: `--`

Setting Date and Time

SETUP-GENERAL SETUP submenu:

The *TIME+DATE* softkey activates the entry of time and date for the internal real time clock.



Time - Input of time

In the corresponding dialog box, the time is partitioned into two input fields so that hours and minutes can be entered independently.

IEC/IEEE-bus command: `SYST:TIME 21,59`

Date - Input of Date

In the corresponding dialog box, the date is partitioned into 3 input fields so that day, month and year can be input separately.

For the selection of the month, pressing a unit key opens a list of abbreviations wherein the desired month can be selected.

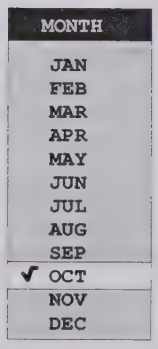

IEC/IEEE-bus command: `SYST:DATE 1999,10,01`

Configuration of network settings (with option FSP-B16 only)

The instrument can be connected to an Ethernet LAN (local area network) by means of the LAN Interface Option FSP-B16. This allows data transmission via the network and the use of network printers. The network card is able to handle both 10 MHz Ethernet IEEE 802.3 and 100 MHz Ethernet IEEE 802.3u.
For more details see section 'LAN Interface - Option FSP-B16'.

SETUP - GENERAL SETUP - menu:

The *CONFIGURE NETWORK* softkey opens the dialog box with the network settings.

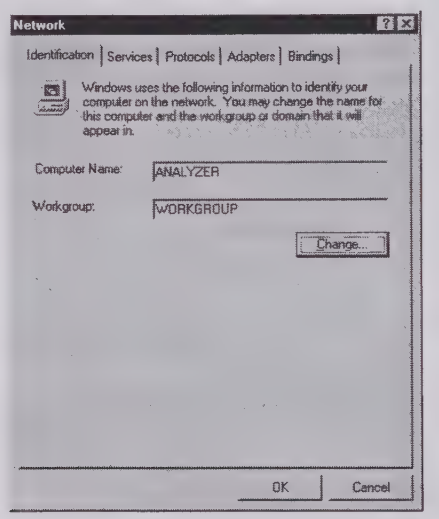

Pressing the key for the first time installs the Windows NT network support (see section 'Installation and Configuration of the Driver for the Network Card' in the manual for LAN Interface FSP-B16) .

If the softkey is pressed again later, the existing network configuration can be changed after selecting the corresponding configuration folder. After pressing the 'Change' button the computer name and the work group on the 'Identification' folder can be adapted to network requirements.

Note:
A PC keyboard with trackball (or mouse instead) is required for the installation/configuration of the network support.
The softkey is only available with built-in LAN interface option (FSP-B16).

IEC/IEEE-bus command: -

The *NETWORK LOGIN* softkey opens the dialog box with the auto login settings.

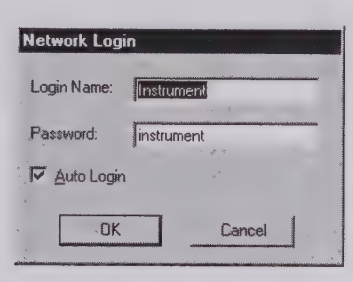

When a network is installed, the preset user name 'Instrument' and the password 'instrument' can be adapted to a new user (see section 'Defining Users' in the LAN interface manual).
With the 'Auto Login' option active, an automatic registration is performed during booting with the specified user name and password. Otherwise the Windows NT login request is displayed during booting.

Note:
A PC keyboard with trackball (or additional mouse instead) is required for the installation/configuration of the network support.

The softkey is only available with built-in LAN interface option (FSP-B16).

IEC/IEEE-bus command: –

Emulation of the instrument front panel

SETUP - GENERAL SETUP – NEXT menu:

The *SOFT FRONTPANEL* softkey switches the display of the front-panel keys on and off.

When the front-panel keys are displayed on the screen, the instrument can be controlled by clicking the respective button with the mouse. This is especially useful when the instrument in a different site is controlled via a remote-control program, like for instance PCANYWHERE, and the screen contents are transferred to the controller via remote link.

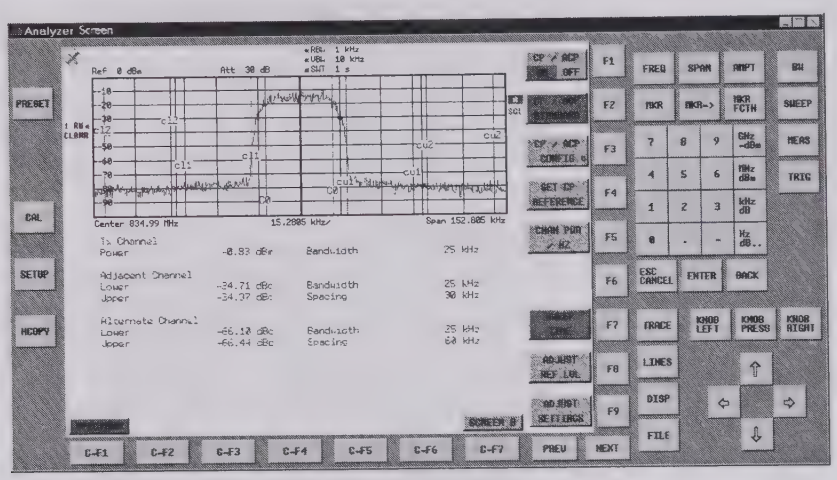

Note:

Display resolution:

When the display of the front-panel keys is switched on, the screen resolution of the instrument changes to 1024x768 pixels. Only a section of the total screen is then displayed on the LC display, which will automatically be shifted on mouse moves.

In order to obtain a complete display of the user interface, an external monitor is to be plugged into the corresponding connector at the rear panel. Prior to performing the resolution change the user is prompted for confirmation whether the required monitor is connected.

Switching off the front-panel display restores the original screen resolution.

Key assignment:

Button labels largely correspond to those of the front-panel keys. The rotation function of the rotary knob is assigned to the 'KNOB LEFT' and 'KNOB RIGHT' buttons, the press function (<ENTER>) to 'KNOB PRESS'.

The labels of the softkey buttons (F1 to F9) and of the hotkey buttons (C-F1 to C-F7) indicate that the keys can be operated directly by means of the corresponding function keys F1 to F9 or <CTRL>F1 to <CTRL>F7 of a PS/2 keyboard.

IEC/IEEE-bus command: `SYST:DISP:FPAN ON`

System Information

The *SYSTEM INFO* softkey opens a submenu in which detailed information on module data, device statistics and system messages is displayed.

SETUP menu:

Display of Module Data

SETUP SYSTEM INFO submenu:

The *HARDWARE INFO* softkey opens a table in which the modules (INSTALLED COMPONENTS) installed in the instrument are listed together with the corresponding hardware revisions.

Table *HARDWARE INFO* consists of six columns:

SERIAL #	serial number
COMPONENT	name of module
ORDER #	order number
MODEL	model number of the module
REV	main modification index of the module
SUB REV	secondary modification index of the module

HARDWARE INFO

COMPONENT	SERIAL #	ORDER #	MODEL	REV	SUB REV
RF_ATTEN_7	688557/005	1067.7684	00	21	00
FRONTEND1	833387/003	1093.5540	03	07	11
FRONTEND2	683346/053	1093.5791	03	05	12
IF-FILTER/REF	689712/002	1093.7242	02	04	04
DETECTOR	683999/035	1093.6998	02	03	04
AF_DEMOD	665087/002	1093.7620	02	03	03
CPU-Board	991025/687	1091.2489	00	04	11
MOTHERBOARD	675631/022	1093.7494	02	05	04
FSP	833387/026	1093.4495	03	00	00
LAN Interface	821818/018	1093.9080	00	00	80

Note:
The screenshot lists the components of an FSP 7 with options FSP-B3 (AF demodulator) and FSP-B16 (LAN interface).

Display of Device Statistics

SETUP SYSTEM INFO submenu:

The *STATISTICS* softkey opens the table *STATISTICS*. This table contains the model information, serial number and firmware version, and a list in which the operating time of the instrument, the power-on cycles as well as attenuator switching cycles are displayed.

STATISTICS	
Model	FSP3
Serial #	123456/789
Firmware Rev	1.23
BIOS Rev.	1.00
Operating time (hours)	375
Power On Cycles	786
Attenuator Cycles	
Input RF/Cal	57
10dB	1786
20dB	1473
40dB	675

IEC/IEEE-bus command: --

Display of System Messages

SETUP SYSTEM INFO submenu:



The *SYSTEM MESSAGES* softkey opens a submenu including a table in which the generated system messages are displayed in the order of their occurrance. The most recent messages are placed at the top of the list.
The following information is available:

No	Device specific error code
MESSAGE	Brief description of the message
COMPONENT	On hardware messages: name of the affected module On Software messages: if needed, the name of the affected software components
DATE/TIME	Date and time of the occurrence of the message

Messages that have occurred since the last call to the *SYSTEM MESSAGES* menu are marked with an asterisk '*'.
The CLEAR ALL MESSAGES softkey is activated and allows clearing of the error buffer.

If the number of error messages exceeds the capacity of the error buffer, the message appearing first is "Message buffer overflow".

SYSTEM INFO

No	MESSAGE	COMPONENT	DATE/TIME
01	No of cycles	Attenuator	05.Jan.99 10:02:00
02	VCO unlock	Frontend	05.Jan.99 10:01:30
03	Calamp range	IF Filter	05.Jan.99 10:00:50
04	3.3V: Voltage	Detector	04.Jan.99 15:58:10
05	I2C-Bus failed	CPU	04.Jan.99 15:58:05

IEC/IEEE-bus command: `SYST:ERR?`

The *CLEAR ALL MESSAGES* softkey deletes all messages in the table.
The softkey is only available when table *SYSTEM INFO* is active.

IEC/IEEE-bus command: `SYST:ERR?`

Service Menu

The service menu offers a variety of additional functions which are used for maintenance and/or trouble shooting.

Caution:

The service functions are not necessary for normal measurement operation. However, incorrect use can affect correct operation and/or data integrity of the FSP. Therefore, many of the functions can only be used after entering a password. They are described in the instrument service manual.

SETUP menu:

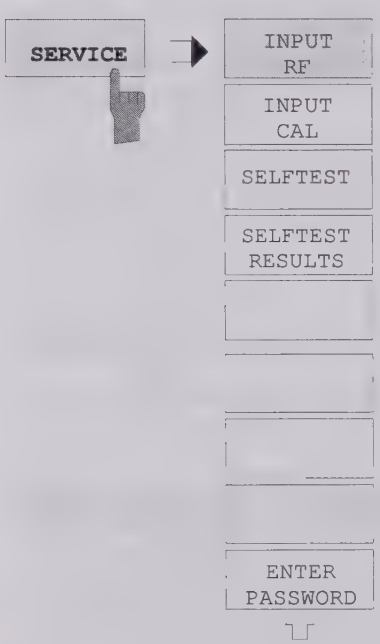

The *SERVICE* softkey opens a submenu for selection of the service function.

The *INPUT RF* and *INPUT CAL* softkeys are mutually exclusive selection switches. Only one switch can be active at any one time.

General Service Functions

SETUP SERVICE submenu:



The *INPUT RF* softkey switches the input of the FSP to the input connector (normal position).

After *PRESET*, *RECALL* or FSP power on, the *INPUT RF* is always selected.

IEC/IEEE-bus command: `DIAG:SERV:INP RF`

The *INPUT CAL* softkey switches the input of the FSP to the internal calibration source (128 MHz) and activates the data entry of the output level of the calibration source. Possible values are 0 dB and –30 dB.

IEC/IEEE-bus command:
```
DIAG:SERV:INP CAL;
DIAG:SERV:INP:CSO 0 DBM
```

The *ENTER PASSWORD* softkey allows the entry of a password.

The FSP contains a variety of service functions which, if incorrectly used, can affect correct operation of the analyzer. These functions are normally not accessible and are only usable after the entry of a password (see instrument service manual).

IEC/IEEE-bus command: `SYST:PASS "Password"`

Selftest

SETUP SERVICE submenu:

The *SELFTEST* softkey initiates the selftest of the instrument modules.

With this function the instrument is capable of identifying a defective module in case of failure.
During the selftest a message box appears in which the current test and its result is shown. The test sequence can be aborted by pressing ENTER ABORT.
All modules are checked consecutively and the test result (selftest PASSED or FAILED) is output in the message box.

IEC/IEEE-bus command: `*TST?`

The *SELFTEST RESULTS* softkey calls the *SELFTEST* table in which the results of the module test are displayed.
In case of failure a short description of the failed test, the defective module, the associated value range and the corresponding test results are indicated.

SELFTEST

SELFTEST: FAILED **24.APR.1999 14:25**
Service level: 0

TEST	RESULT	VALID RANGE	VALUE
Voltages	OK		
Pretune DAC	OK		
Synthesizer	FAIL		
Frontend2 128MHz Ref unlock	FAIL	1.25V...3.5V	1.14V
Frontend1 384MHz Ref Input	OK	0.5...0.6V	0V
Signal Path	OK		

IEC/IEEE-bus command: `DIAG:SERV:STE:RES?`





The *PAGE UP* or *PAGE DOWN* softkey sets the *SELFTEST RESULTS* table to the next or previous page.

IEC/IEEE-bus command --

Hardware Adjustment

Some of the FSP modules can be re-aligned. This re-alignment can become necessary after calibration due to temperature drift or aging of components (see service manual instrument).

Caution:

The re-alignment should be carried out by qualified personnel since the changes considerably influence the measurement accuracy of the instrument. This is the reason why the softkeys REF FREQUENCY, CAL SIGNAL POWER and SAVE CHANGES can only be accessed after entering a password.

Firmware Update

The installation of a new firmware version can be performed using the built-in diskette drive. The firmware update kit contains several diskettes.
The installation program is called in the *SETUP* menu.

SETUP side menu:



The *FIRMWARE UPDATE* softkey starts the installation program and leads the user through the remaining steps of the update

IEC/IEEE-bus command: --

The firmware update is started as follows:

Insert disk 1 into the floppy drive.

Call *SETUP* side menu via ***[SETUP][NEXT]***

Start the update via ***[FIRMWARE UPDATE]***

The *RESTORE FIRMWARE* softkey restores the previous firmware version

IEC/IEEE-bus command: --

Saving and Recalling Data Sets – *FILE* Key

The *FILE* key calls the following functions:

- Storage/loading functions for storing (*SAVE*) instrument settings such as instrument configurations (measurement/display settings, etc.) and measurement results from working memory to permanent storage media, or to load (*RECALL*) stored data into working memory.
- Functions for management of storage media (*FILE MANAGER*). Included are among others functions for listing files, formatting storage media, copying, and deleting/renaming files.

The FSP is capable of internally storing complete instrument settings with instrument configurations and measurement data in the form of data sets. The respective data are stored on the internal hard disk or, if selected, on a floppy. The hard-disk and floppy-disk drives have the following names:

floppy disk	A:
hard disk	D: (hard disk C: is reserved for instrument software)

In addition to the saving and recalling of complete instrument settings, it is also possible to save/recall subsets of settings. Configuration data and measurement values are stored in separate files. These files have the same name as the data set but however have a different extension. A data set thus consists of several files which have the same name but different extensions (see Table 4-2). Default setting for storing the data sets is directory D:\USER\CONFIG.

When saving or loading a data set, the subsets which are to be saved or loaded can be selected in the corresponding tables. This makes it easy to reconstruct specific instrument settings beside the default setting of the instrument.

When saving and loading data, data subsets are selected in table *SEL ITEMS TO SAVE/RECALL*.

The saved files of the data sets can be copied from one storage medium (e.g. drive C:) to another storage medium (e.g. drive A:) or to another directory using the functions found in the *FILE MANAGER* sub menu. File names and extensions must however not be changed. The relationship between the data subsets and the extensions is shown in Table 4-2.

Table 4-2 Relationship between extensions, contents and designations of data subsets

	Designation in the table SEL ITEMS TO SAVE/RECALL	**Contents**	**Extension**
Configuration data:	CURRENTSETTINGS	current settings of the measurement hardware and the related title, if present	.SET
		active limit lines	.LIN
		current configuration of general instrument parameters	.CFG
		configuration for hardcopy output	.HCS
Additional configuration data	ALL LIMIT LINES	all limit lines	.LIA
Measurement results:	ALL TRACES	measurement data trace 1 to trace 3, screen A	.TR1 to TR3
		measurement data trace 1 to trace 3, screen B	.TR4 to TR6

Saving a Data Set

- Select the data subsets to be saved (sub-menu *ITEMS TO SAVE/RCL* (configurations, measurement and calibration data) (softkey *ITEMS TO SAVE/RCL)* .
- Possibly enter a comment (softkey *EDIT COMMENT*)
- Enter the directory in which the data set should be saved in table *SAVE DATA SET* (softkey *SAVE*).
- Enter the name of the data set which should be saved (softkey *SAVE*) and save the data set by pressing the *ENTER* key.

  Data set names may contain both letters and numbers, in the simplest case only numbers.

  If required, the desired directory can be given a prefix to the data set name (the directory is then automatically set for further SAVE and RECALL operations).

  The simplest example for the input of a data set name is illustrated by the following key strokes:

  <SAVE> <1> <units key>

Note: *If the current instrument configuration is to be stored under an existing name, a selection list is available via the DATA SET LIST softkey. The storage is performed as follows.*

- *Press a units key after selecting a data set in table DATA SET LIST*

  The name and the selection of the data subsets for the currently selected data set will be placed in the SAVE DATA SET table.
- *Press the SAVE softkey.*

  The entry field EDIT NAME with the name of the selected data set is opened.
- *Press a units key.*
  The current instrument configuration is saved as a data set under this name.

Recalling a Data Set:

The data set can be loaded in two ways:

1. **Direct entry of the data name:**
   - Select data subsets which should be loaded (configurations, measurement and calibration data) with softkey *ITEMS TO SAVE/RCL* in sub menu *ITEMS TO SAVE/RCL).*
   - Enter the name of the data set to be saved (softkey *RECALL*) and recall the data set by pressing the *ENTER* key*).*

     Data set names may contain both letters and numbers, in the simplest case only numbers. If required, the desired directory can be prefixed to the data set name (the directory is then automatically set for further SAVE and RECALL operations).

     The simplest example for the input of a data set name is illustrated by the following key strokes: <RECALL> <1> <units key>

2. **Selecting the data set from a selection list:**
   - Select from submenu *ITEMS TO SAVE/RCL* the data subsets which should be loaded (configurations, measurement and calibration data) (softkey *ITEMS TO SAVE/RCL).*
   - Select the data set which should be loaded (Softkey *DATA SET LIST*) and confirm with *ENTER*. The data set is taken over in the *RECALL DATA SET* table.
   - Press the RECALL softkey. The entry field for the data set name is opened and contains the desired data set.
   - Initiate the loading of the selected data set by pressing the *ENTER* key.

Note: *If the set directory does not correspond to the required directory for loading, it can be changed as follows:*

- *Press the RECALL softkey.*
- *Close the entry field for the data set name with ESC.*
- *Select the PATH filed with the cursor keys.*
- *Open the entry field for the directory name with ENTER.*
- *Enter the directory name and confirm with ENTER.*

Then proceed with the selection list as described above.

Any settings not restored when data subsets are loaded will remain unchanged in the instrument. During recall operations, the FSP recognises which subsets are present in the recalled data set and ignores selected data subsets that are not available.

FILE Menu

FILE menu

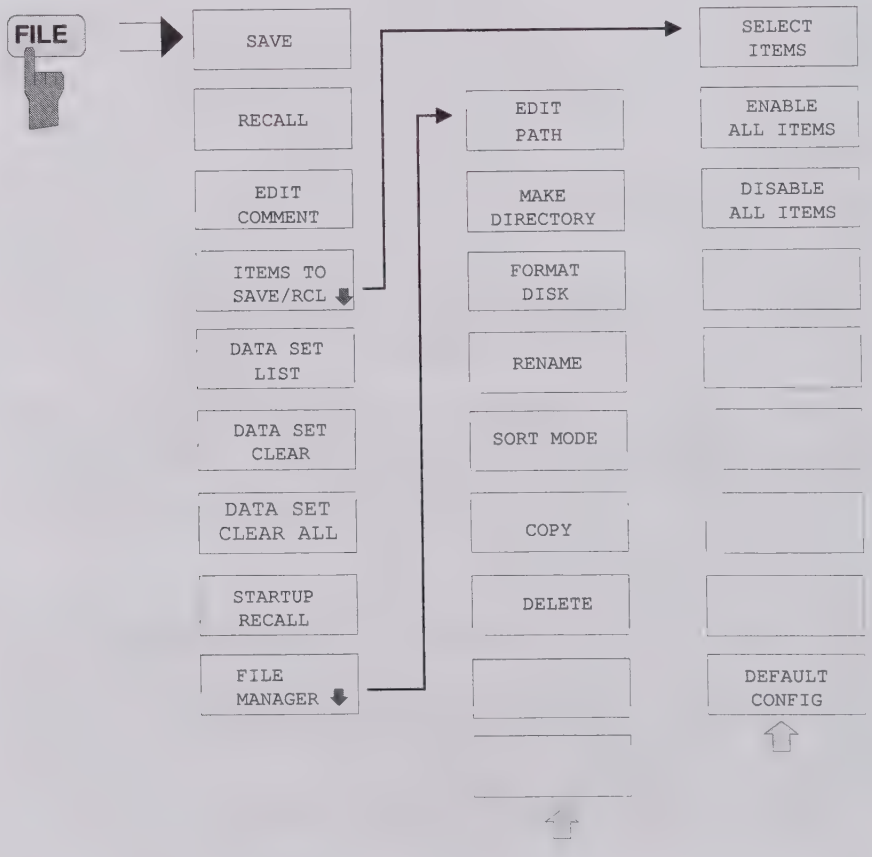

The *SAVE* softkey activates table *SAVE DATA SET*. The data set is stored by pressing the *ENTER* key.

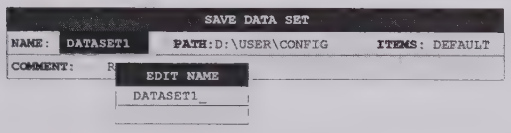

The *SAVE DATA SET* table contains the entry fields for editing the data set:

Name — name of data set
The name can be entered with or without drive name and directory; the drive name and directory, if available, are then taken over in the PATH field. The extension of the data name is ignored.

Path — directory in which the data set will be saved

Items — indicates whether the default selection of the data subset (DEFAULT) or a user-defined selection (SELECTED) will be saved

Comment — Commentary regarding the data set

IEC/IEEE command: `MMEM:STOR:STAT 1,"a:\test02"`

The *RECALL* softkey activates the entry of the path in which the data set is located. The data set is recalled by pressing the *ENTER* key.

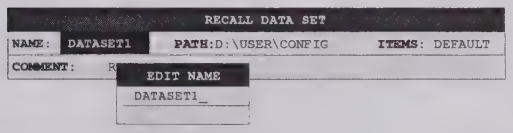

The *RECALL DATA SET* table shows the current settings regarding the data set:

Name — name of data set

Path — directory in which the data set is located

Items — indicates whether the default selection of the data subset (DEFAULT) or a user-defined selection (SELECTED) will be recalled

Comment — Commentary regarding the data set

IEC/IEEE command: `MMEM:LOAD:STAT 1,"a:\test02"`

The *EDIT COMMENT* softkey activates the entry of commentary concerning the current data set. A total of 60 characters are available for this purpose.

IEC/IEEE command: `MMEM:COMM "Setup fuer GSM Messung"`

The *SEL ITEMS TO SAVE/RCL* softkey opens a sub-menu for selection of the data subsets.

FILE - ITEMS TO SAVE/RCL sub-menu:

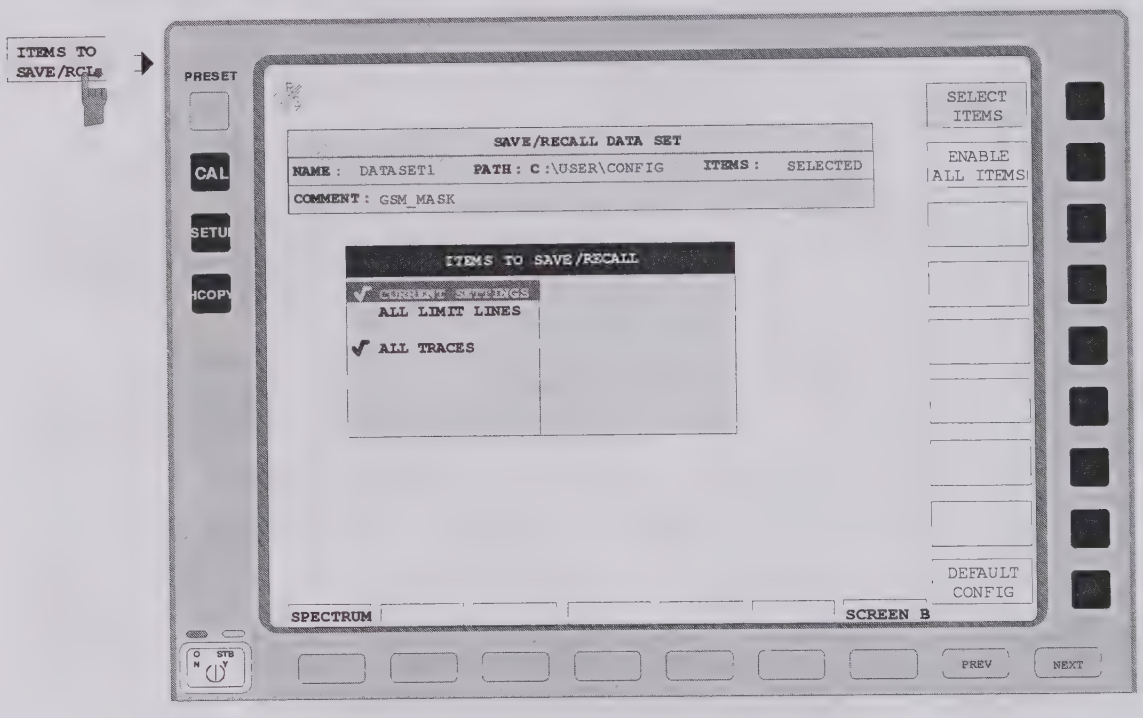

The *ITEMS TO SAVE/RECALL* table offers the following selectable data subsets:

Current Settings these settings include:

- current configuration of general instrument parameters
- current measurement hardware settings
- active limit lines:
  A data set may contain maximum 8 limit lines for each window. It always contain the activated limit lines and the de-activated limit lines used last, if any.
  Consequently, the combination of the restored de-activated limit lines depends on the sequence of use with command `MMEM:LOAD`.
- user-defined color settings
- configuration for hardcopy output
- active transducer*All Limit Lines* all limit lines

All Traces all traces which are not blanked

The *SELECT ITEMS* softkey moves the selection bar to the first line, left column of the table. An entry is selected by pressing the *ENTER* key in the desired line. The selection is cleared by pressing the key again.

IEC/IEEE command:

Current Settings:	`MMEM:SEL:HWS ON`
All Limit Lines:	`MMEM:SEL:LIN:ALL ON`
All Traces:	`MMEM:SEL:TRAC ON`

ENABLE ALL ITEMS

The *ENABLE ALL ITEMS* softkey marks all entries in the table.

IEC/IEEE command: `MMEM:SEL:ALL`

DEFAULT CONFIG

The *DEFAULT CONFIG* softkey establishes the default selection of the data subset to be saved and outputs *DEFAULT* in the *ITEMS* field of the *SAVE/RECALL DATA SET* table.

IEC/IEEE command: `MMEM:SEL:DEF`

DATA SET LIST

The *DATA SET LIST* softkey opens the *DATA SET LIST/CONTENTS* table. In addition, the *DATA SET CLEAR* and *DATA SET CLEAR ALL* softkeys are displayed.

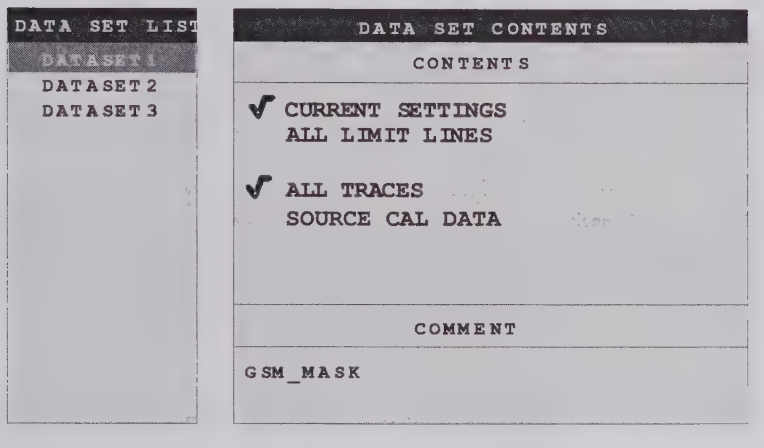

The *DATA SET LIST* column lists all of the data sets which are stored in the selected directory.

The *CONTENTS* and *COMMENT* lines in the *DATA SET CONTENTS* column indicate the saved data subsets and the comment for the currently selected data set. A '-' prefixed to a data subset means that the latter is available in the instrument but that it has not been selected (see *SELECT ITEMS* softkey).

IEC/IEEE command: `---`

DATA SET CLEAR

The *DATA SET CLEAR* softkey deletes the selected data set

IEC/IEEE command: `MMEM:CLE:STAT 1, "test03"`

DATA SET CLEAR ALL

The *DATA SET CLEAR ALL* softkey deletes all data sets in the current directory.

Since, in this case, all available data sets are lost, confirmation by the user is required.

IEC/IEEE command: `MMEM:CLE:ALL`

The *STARTUP RECALL* softkey activates the selection of a data set which is automatically loaded when the instrument is powered on. For that purpose the table *DATA SET LIST/CONTENT* is opened (analog to *DATA SET LIST).*

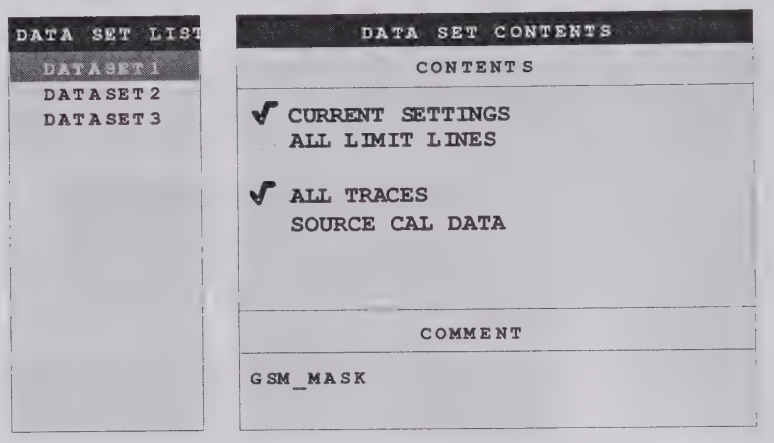

The *DATA SET LIST* column displays all data sets present in the selected directory

The *CONTENTS* and *COMMENT* lines in the *STARTUP RECALL* column indicate the saved data subsets and the commentary for the currently selected data set.

In addition to the data sets stored by the user, the data set *FACTORY*, which specifies the settings of the instrument before it was last switched off (Standby), is always present.

If a data set other than *FACTORY* is chosen then, at the time of instrument power on, the available data subsets of the selected data set are recalled. The data subsets which are not present in this data set are taken from the *FACTORY* data set.

Note: *The specified data set is also loaded upon PRESET if STARTUP RECALL is active. The preset settiongs can thus be arbitrarily modified.*

IEC/IEEE command: `MMEM:LOAD:AUTO 1,"D:\user\config\test02"`

The *FILE MANAGER* softkey opens a menu for managing storage media and files.

FILE - FILE MANAGER sub-menu:

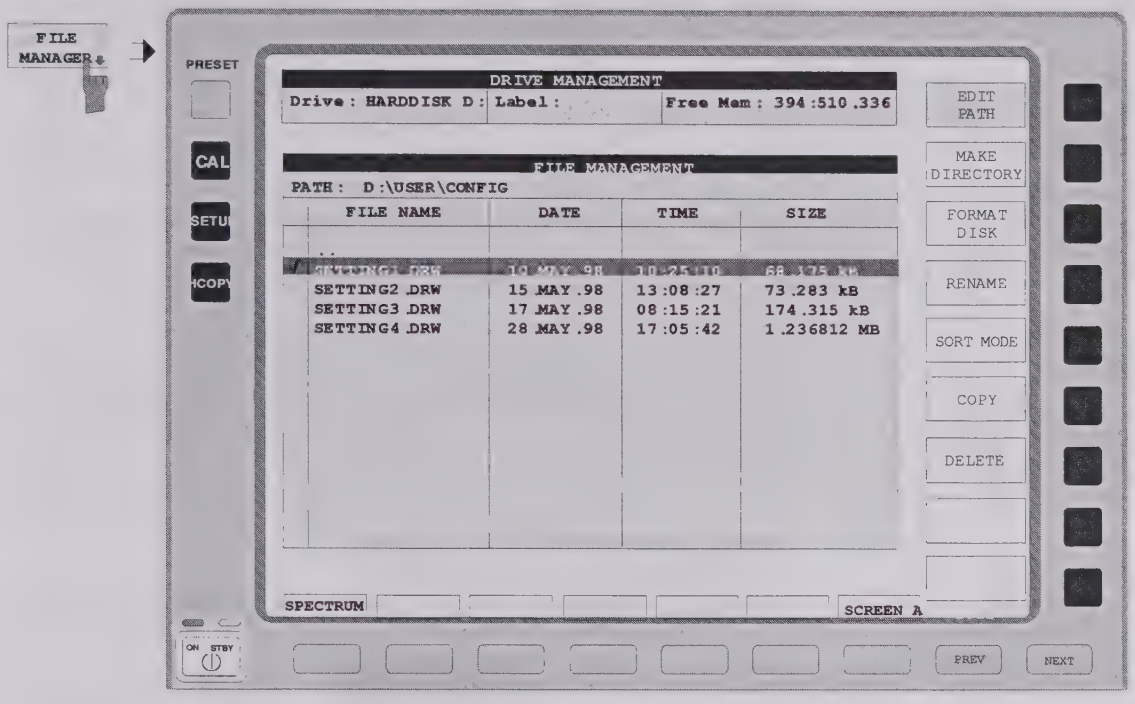

Table *Drive Management* displays the name and label of the storage medium as well as the available storage area.

Table *File Management* displays the files of the current directory and indicates if any subdirectories are present.

If a directory name is selected, the FSP automatically changes to this directory. Selection of the entry '..' moves the FSP to the next higher directory level.

Note: *It is not possible to change menus as long as a file operation is running.*

The *EDIT PATH* softkey activates the input of the directory which will be used in subsequent file operations.

The new path is included in the *FILE MANAGEMENT* table.

IEC/IEEE command:
```
MMEM:MSIS "a:"
MMEM:CDIR "D:\user "
```

The *MAKE DIRECTORY* softkey creates directories/sub-directories. Sub-directories are recommended for sorting files on the storage medium so that the structure is easier to comprehend.

The entry of an absolute path name (e.g.; "\USER\MEAS") as well as the path relative to the current directory (e.g., "..\MEAS") is possible.

IEC/IEEE command: `MMEM:MDIR "D:\user\test"`

The *FORMAT DISK* softkey formats diskettes located in drive A:.
To prevent accidental destruction of diskette data, confirmation by the user is requested.

IEC/IEEE command: `MMEM:INIT "a:"`

The *RENAME* softkey activates the entry of a new name for the selected file or directory.

IEC/IEEE command: `MMEM:MOVE "test02.cfg","set2.cfg"`



The *SORT MODE* softkey activates the selection of the criteria according to which the files listed in the *FILE MANAGEMENT* table may be sorted.



Directory names are located at the top of the list after the entry for the next higher directory level ("..").

IEC/IEEE command: `--`



The *COPY* softkey activates the input of the destination of the copy operation.

By entering a predefined disk drive (e.g. C:), a file can also be copied to another storage medium. The files/directories selected by the cursor are copied after the input is confirmed by pressing the *ENTER* key.

IEC/IEEE command: `MMEM:COPY "D:\user\set.cfg","a:"`

The *DELETE* softkey deletes the selected files.
To prevent accidental deletion of data, confirmation by the user is requested.

IEC/IEEE command:
```
MMEM:DEL "test01.hcp"
MMEM:RDIR "D:\user\test"
```

Measurement Documentation – *HCOPY* Key

Note: *The installation of additional printers is described in chapter 1, section "Installation and Configuration of Printers".*

Pressing one of the softkeys *PRINT...* in the *HCOPY* menu initiates the print job. The printer parameters defined in the *DEVICE SETTINGS* menu are used for setting up the printer configuration. All of the display items to be printed are written to the printer buffer. Since the printer runs in the background, the instrument may be operated immediately after pressing the *PRINT...* softkey.

With *PRINT SCREEN* selected, all the diagrams with traces and status displays are printed as they occur on the screen. Softkeys, open tables and data entry fields are not printed out. Function *PRINT TRACE* allows printing out individual traces. With *PRINT TABLE* tables can be printed out.

If the *PRINT TO FILE* option in the *DEVICE SETTINGS* table is selected the printout is directed to a file. Upon pressing one of the softkeys *PRINT...*, the file name to which the output data are to be written is requested. For this an entry field is opened for entering the file name.

While a print job is in progress, problems may occur in the output device. If, while printing, the output device issues a PAPER OUT message, i.e., no more paper is available, the user will be prompted by the following message



to load paper into the output device. The print job will then be either continued (CONTINUE selected) or aborted (ABORT selected).

Similar *SYSTEM MESSAGES* appear if the printer is offline, etc.

Selection between b/w and colored printouts is possible with softkey *COLOR ON/OFF* provided that the printer connected is able to output such prints. The colors of the printout correspond to those of the screen, i.e. a yellow trace will be output in yellow.
To change the colors of the objects on the printout, the screen colors have to be changed correspondingly in menu *DISPLAY*, submenu *CONFIG DISPLAY*. One exception is the color of the background and of the grid. The output background is always white irrespective of the screen color and the grid is always black.

The *HARDCOPY ABORT* softkey aborts a print job in progress.

HCOPY menu:

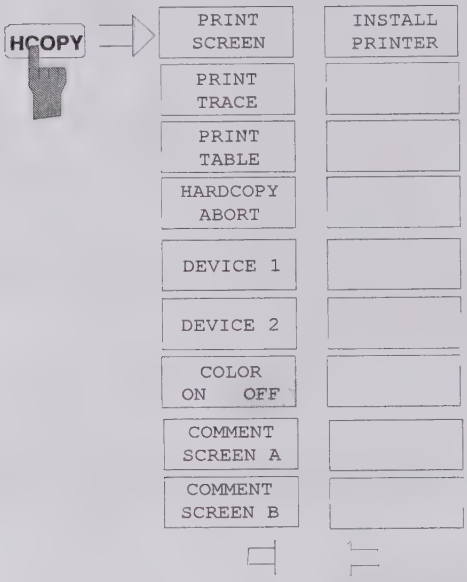

The *HCOPY* key opens the *HARDCOPY* menu for starting and configuring the printout.

The *PRINT SCREEN, PRINT TRACE and PRINT TABLE* softkeys start the desired printout, which can be aborted with HARDCOPY ABORT.

Selection and configuration of the output interface is performed via the DEVICE 1 and 2 softkeys.

The *COMMENT SCREEN A* and *COMMENT SCREEN B softkeys are available for adding comments to the hardcopy* (date and time are automatically added).

With the *INSTALL PRINTER* softkey other printer drivers can be installed.

The *PRINT SCREEN* softkey starts the output of test results.

All the diagrams, traces, markers, marker lists, limit lines etc. are printed out as long as they are displayed on the screen. All the softkeys, tables and open data entry fields are not printed out. Moreover, comments, title, date, and time are output at the bottom margin of the printout .

IEC/IEEE-bus command:
```
HCOP:ITEM:ALL
HCOP:IMM
```

The *PRINT TRACE* softkey starts the output of all curves visible on the display screen without auxiliary information. Specifically, no markers or display lines are printed.

IEC/IEEE-bus command:
```
HCOP:ITEM:WIND:TRAC:STAT ON
HCOP:IMM
```

The *PRINT TABLE* softkey starts the output of all tables and info lists visible on the display screen without the measurement diagrams and other information lying behind.

IEC/IEEE-bus command:
```
HCOP:ITEM:WIND:TABL:STAT ON
HCOP:IMM
```

The *HARDCOPY ABORT* softkey aborts the printout.

IEC/IEEE-bus command: `ABOR`



The *DEVICE 1/DEVICE 2* softkey determines the active output device. Table *HARDCOPY DEVICE SETTINGS* is simultaneously opened for the configuration of the two possible devices. The selection bar marks the selected line of the table.



HARDCOPY DEVICE SETTINGS	
Device1	WINDOWS METAFILE
Print to File	YES
Orientation	---
Device2	CLIPBOARD
Print to File	---
Orientation	---

Device 1/2 In this lines, the selection of the output device/language for Device1 or Device2 is made.

Print to File selects printout to file or printer

Orientation selects the print format of the output page

Device 1/ Device 2

The selection of the output device/language for *Device 1* and *Device 2* is made in this line.
After pressing the *ENTER* key, the list of all installed printers is displayed. Three file formats and the Windows NT clipboard are also available:

CLIPBOARD	output in Windows NT clipboard.
WINDOWS METAFILE or BITMAP FILE	output in file
ENHANCED METAFILE	output in file or Windows NT clipboard.

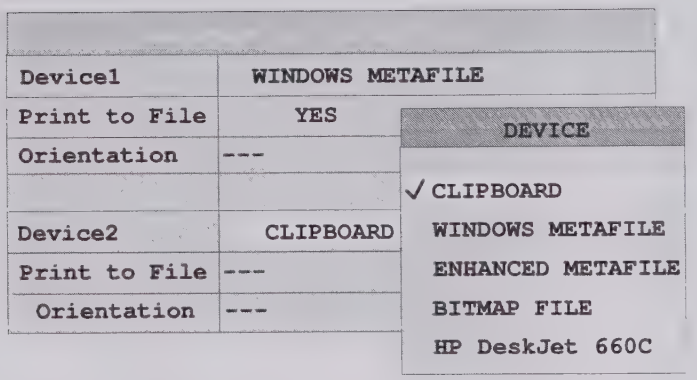

The installation of additional printers is described in chapter 1, section "Installation and Configuration of Printers".

Notes: *Selecting the type of printer automatically sets the parameters PRINT TO FILE and ORIENTATION to values which correspond to a standard mode with this output device. Other printer-dependent parameters, such as PAPERSIZE, can be modified under Windows NT in the printer properties window (START/SETTINGS/PRINTER/ SETTINGS). For operation of Windows NT, a mouse and an external keyboard have to be connected to instrument (see also Section "Installation and Configuration of Printers")*

IEC/IEEE-bus command:

```
HCOP:DEV:LANG GDI;
SYST:COMM:PRIN:ENUM:FIRS?;
SYST:COMM:PRIN:ENUM:NEXT?;
SYST:COMM:PRIN:SEL 'HP Deskjet 660 on LPT1';
HCOP:DEST "SYST:COMM:PRIN"
```

Print to File

In this line, directing the printout to the printer (OFF) or to a file (ON) is selected. For printout to a file, the user is prompted to enter a file name on starting the print.

Selecting the type of printer automatically sets this parameter to the value which corresponds to a standard mode with this output device.

IEC/IEEE-bus command: `HCOP:DEST "SYST:COMM:PRIN" or`
`HCOP:DEST "SYST:COMM:MMEM"`

Orientation

In this line, the print format of the output page is set to either vertical (= PORTRAIT) or horizontal (= LANDSCAPE).

IEC/IEEE-bus command: `HCOP:PAGE:ORI PORT`



The *COLOR ON/ OFF* softkey selects a colored or b/w printout.

Colored background is printed white and colored lines are printed black in order to improve the contrast of the printout.
Default setting is *COLOR OFF*.

IEC/IEEE-bus command: `HCOP:DEV:COL ON`





The *COMMENT SCREEN A* or *B* softkey opens an entry field in which a comment of two lines (60 characters per line) can be entered for screen A or B.

If the user enters more than 60 characters, the excess characters appear on the second line on the print-out. At any point, a manual line-feed can be forced by entering the @ character.

The comment is printed below the corresponding diagram. The comment text appears on the print-out, but does not appear on the display screen.

If a comment is not to appear on the printout, it has to be deleted.
By pressing *PRESET*, all comments will be deleted.

IEC/IEEE-bus command: `HCOP:ITEM:WIND2:TEXT 'Comment'`

HCOPY side menu:

A certain number of printer drivers is already installed on the FSP.
The *INSTALL PRINTER* softkey opens the "Printers" window where further printer drivers can be installed (see section "Installation of a local printer" and "Installation of Network Printer").

IEC/IEC-bus command: -

Installation of a local Printer

Note:
For an easy operation of the subsequent dialogs connection of a PS/2 keyboard including trackball to the front panel is recommended. If no trackball is available, a PS/2 mouse should be connected additionally to the rear panel (see section "Connecting a Mouse" and "Connecting a Keyboard").

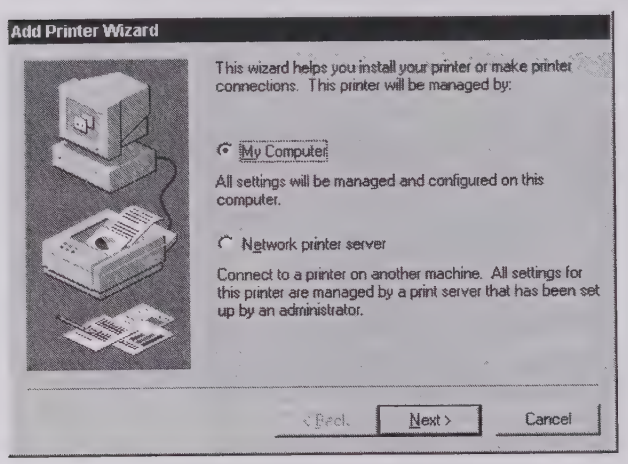
Add Printer Wizard
This wizard helps you install your printer or make printer connections. This printer will be managed by:
My Computer
All settings will be managed and configured on this computer.
Network printer server
Connect to a printer on another machine. All settings for this printer are managed by a print server that has been set up by an administrator.
< Back
Next >
Cancel

➢ Click on "My Computer" and then "Next".

The selection of printer ports appears.

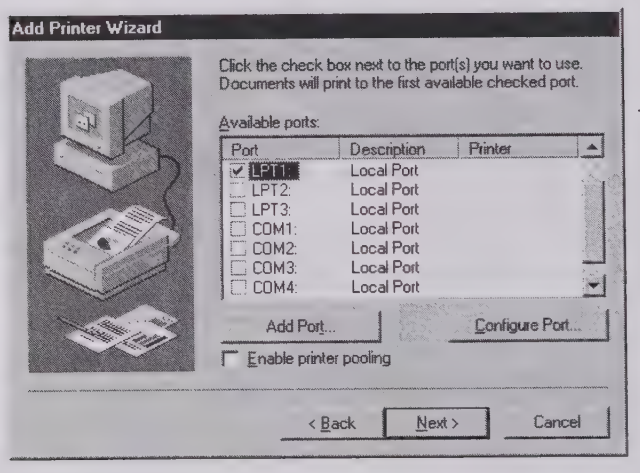

➢ Select port LPT1.

The selection will be marked with a tick.

➢ Click on "Next".

The selection of the printer drivers appears. The left table contains the manufacturers, the right on the available printer drivers.

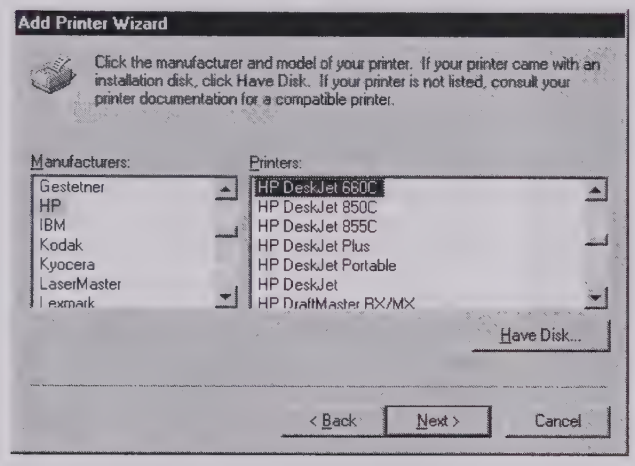

➢ Select the desired manufacturer and the corresponding printer driver.

Note:
If the desired printer type does not appear in the list, then the corresponding driver has not been installed on the instrument so far. In this case click on button "HAVE DISK". This will open a prompt for inserting a disk with the corresponding driver into the floppy drive. Press "OK" and select the desired printer driver.
After the installation the "Service Pack 5" must be re-installed (see section "Installing Windows-NT software").

➢ Click on "Next".

The data entry field for the printer name appears.

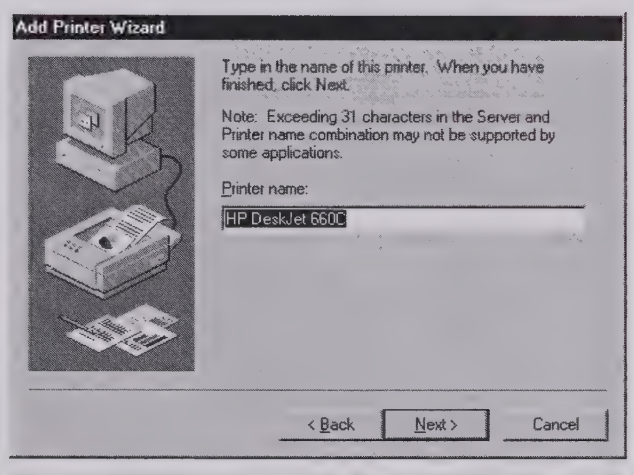
Add Printer Wizard
Type in the name of this printer. When you have finished, click Next.
Note: Exceeding 31 characters in the Server and Printer name combination may not be supported by some applications.
Printer name:
HP DeskJet 660C
< Back
Next >
Cancel

➢ The name of the printer can be modified in the edit field "Printer name" (max. 60 characters).

If there are already installed printers in the system, there will be a prompt for whether the new printer should be used as the standard printer for Windows NT applications (Do you want your Windows-based programs to use this printer as default printer?). The pre-selection is "No".

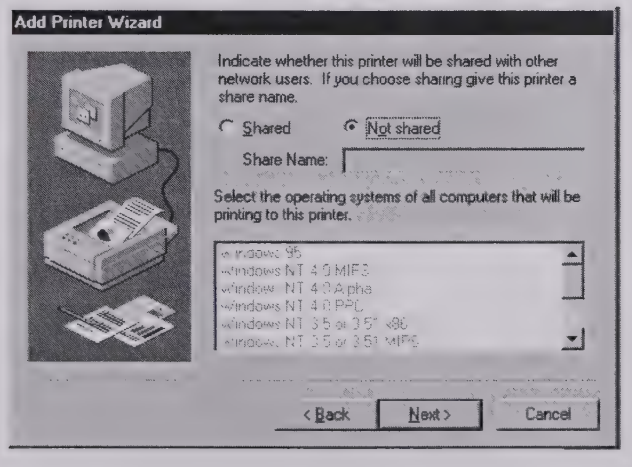
Add Printer Wizard
Indicate whether this printer will be shared with other network users. If you choose sharing give this printer a share name.
Shared
Not shared
Share Name:
Select the operating systems of all computers that will be printing to this printer.
Windows 95
Windows NT 4.0 MIPS
Windows NT 4.0 Alpha
Windows NT 4.0 PPC
Windows NT 3.5 or 3.5" x86
Windows NT 3.5 or 3.51 MIPS
< Back
Next >
Cancel

➢ Click on "Next".

A prompt will appear querying the availability of the printer in a network. This query is irrelevant for the installation of a local printer. The answer "Not shared" is pre-selected.

➢ Click on "Next".

The window for printing a test page appears. This allows testing whether the installation was successful.

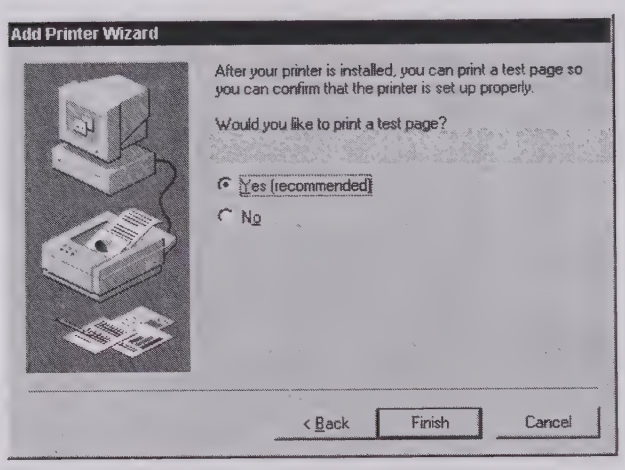
Add Printer Wizard
After your printer is installed, you can print a test page so you can confirm that the printer is set up properly.
Would you like to print a test page?
Yes (recommended)
No
< Back
Finish
Cancel

- Click on "Yes (recommended)".
- Click on "Finish".

  If the installation was successful, a test page will be printed.
  If the test page is not printed or printed incorrectly, the Windows NT online help will supply additional support in chapter "Printer - Trouble Shooting".

Note:
If you are prompted to indicate the printer driver path after clicking on "Finish", the Service Pack must be re-installed after this printer installation (see chapter 1, section "Installing Windows NT software").

Finally the instrument must be configured for printouts of the measurement screen with this printer. For details please refer to softkey *DEVICE 1* and *DEVICE 2* in the hardcopy menu.

Installation of a Network Printer (with option FSP-B16 only)

After opening the "Printer" dialog window proceed with the installation as follows:

➢ Double-click "Add Printer" line.

The "Add Printer Wizard" window is opened. This window guides the user through the printer driver installation.

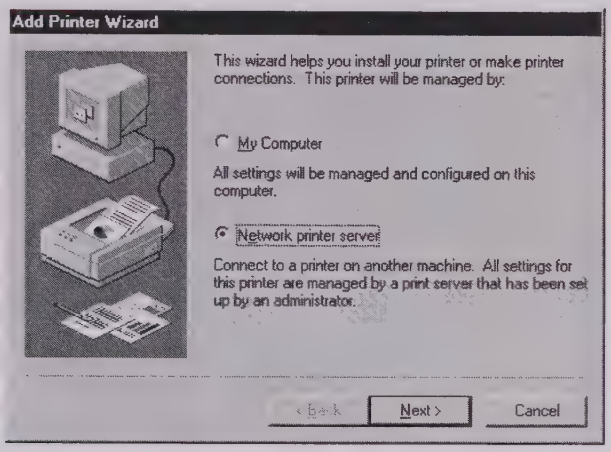
Add Printer Wizard
This wizard helps you install your printer or make printer connections. This printer will be managed by:
My Computer
All settings will be managed and configured on this computer.
Network printer server
Connect to a printer on another machine. All settings for this printer are managed by a print server that has been set up by an administrator.
< Back
Next >
Cancel

➢ Click "Network printer server" and then "Next".

A list of selectable printers is displayed.

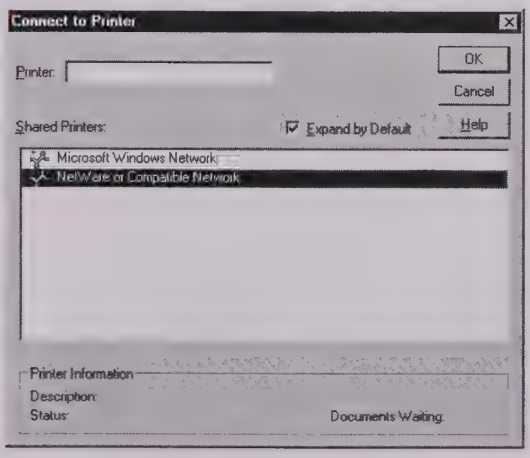

➢ Mark printer and select it with OK.

➢ Confirm the following request for the installation of a suitable printer driver with OK.

The list of printer drivers is displayed. The manufacturers are listed in the window at the left, the available printer drivers at the right.

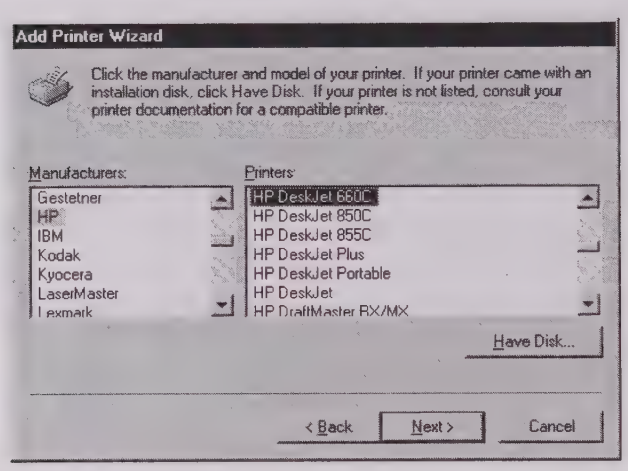

➢ Select the manufacturer in the "Manufacturers" window and then the printer driver in the "Printers" window.

Note:
If the desired printer type is not listed, the driver has not been installed. In this case click HAVE DISK. You are requested to insert a floppy with the respective printer driver. Subsequently press OK and select the desired driver. After this the "Service Pack 5" has to be newly installed (see chapter "Install Windows-NT Software)

➢ Click "Next"

If one or more printers have been installed, a query is displayed in this window, whether the printer you have just instelled should be used as the standard printer for Windows NT applications. (Do you want your Windows-based programs to use this printer as default printer?). Default setting is "No".

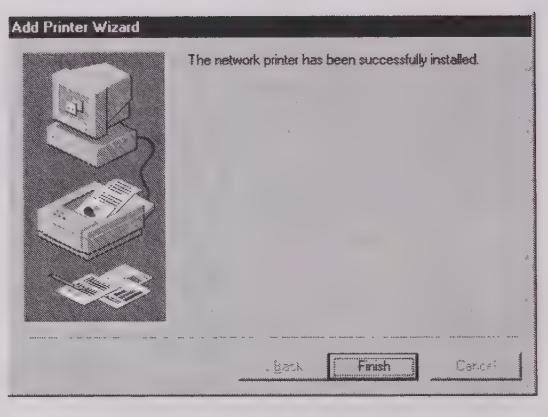

➢ Start the printer driver installation with "Finish".

Note:
If after clicking on "Finish" you are requested to enter the printer driver path, the Service Pack has to be re-installed after the printer installation (see chapter 1, Installing Windows NT Software).

Finally the instrument must be configured for printouts of the measurement screen with this printer. For details please refer to softkey *DEVICE 1* and *DEVICE 2* in the hardcopy menu.

Tracking Generator - Option FSP-B9

During normal operation (without a frequency offset), the tracking generator emits a signal exactly at the input frequency of the analyzer.

For frequency-converting measurements it is possible to set a constant frequency offset of ±150 MHz between the receive frequency of the analyzer and the output signal of the tracking generator.
Moreover, an I/Q modulation or AM and FM modulation of the output signal can be provided using two analog input signals.

The output power is level-controlled and can be set in 0.1 dB steps in a range from -30 dBm to 0 dBm.

The tracking generator can be used in all operating modes. Acquisition of test setup calibration values (SOURCE CAL) and normalization using these correction values (*NORMALIZE*) is only possible in the *NETWORK* operating mode.

Note:
The RF characteristics of some DUTs is especially sensitive concerning the input VSWR. In such cases insertion of 20 dB attenuation between the DUT and the tracking generator output is highly recommended.

The tracking generator is activated by means of the NETWORK hotkey in the hotkey bar at the bottom of the screen:

Tracking Generator Settings

The *NETWORK* hotkey opens a menu for selecting the functions of the tracking generator.

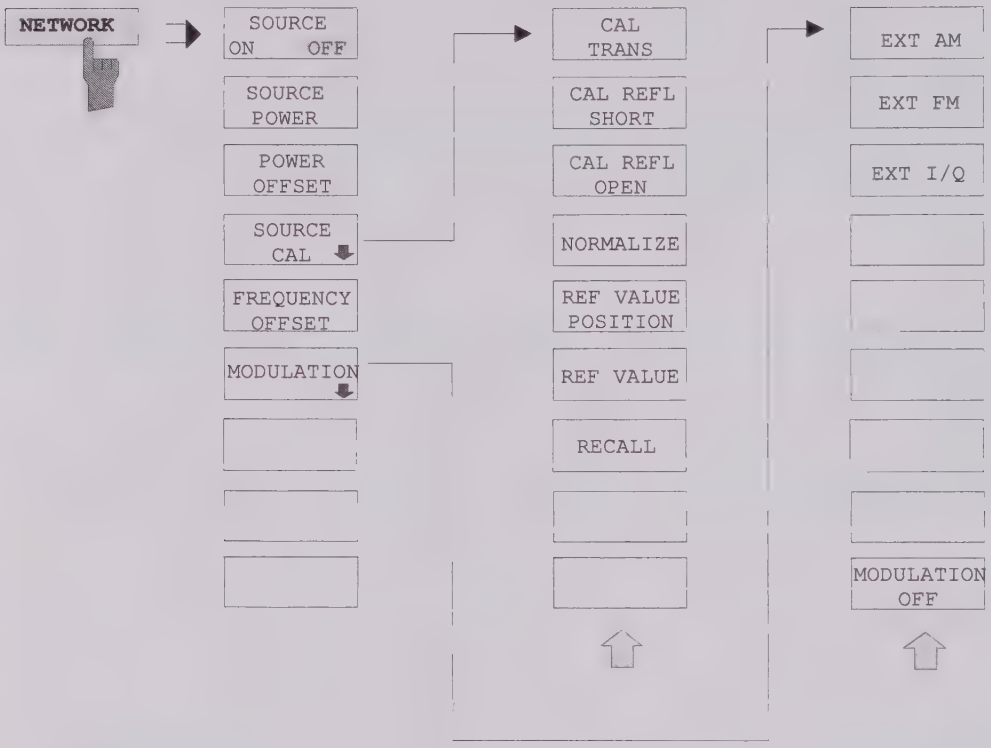

Note: *Additional softkeys are available in the displayed menus for controlling an external generator if option External Generator Control FSP-B10 is fitted. For detailed information see section 'External Generator Control Option FSP-B10'.*



The *SOURCE ON/OFF* softkey switches the tracking generator on or off. Default setting is *OFF*

Note:

- *When the tracking generator is switched on the maximum stop frequency is limited to 3 GHz. This upper limit is automatically reduced by a frequency offset set up for the tracking generator.*
- *In order to meet the data sheet accuracy for measurements with active tracing generetor the start frequency must be set to ≥ 3 x Resolution Bandwidth.*
- *The minimum sweeptime for measurements with data sheet accuracy is 100 ms in frequency domain (span > 0 Hz). Selecting a sweeptime below this limit will result in the sweeptime indicator field SWT being supplied with a red asterisc and the message UNCAL being displayed.*
- *FFT filters (FILTER TYPE FFT in BW menu) are not available when the tracking generator is active.*

IEC/IEEE-bus command: `OUTP:STAT ON`



The *SOURCE POWER* softkey allows the tracking generator output power to be selected.
The output level can be set in 0.1 dB steps from -30 dBm to 0 dBm.

If the tracking generator is off, it is automatically switched on when an output power value is entered.

The default output power is -20 dBm.

IEC/IEEE-bus command: `SOUR:POW -20dBm`



The *POWER OFFSET* softkey allows selection of a constant level offset for the tracking generator.

With this offset for example attenuators or amplifiers at the output connector of the tracking generator can be taken into account for the displayed output power values on screen or during data entry.

The valid range is -200 dB to +200 dB in 0.1 dB steps. Positive offsets apply to an amplifier and negative offsets to an attenuator subsequent to the tracking generator.
The default setting is 0 dB. Offsets <> 0 will display the enhancement label **LVL**.

IEC/IEEE-bus command: `SOUR:POW:OFFS -10dB`

Transmission Measurement

This measurement will yield the transmission characteristics of a two-port network. The built-in tracking generator serves as a signal source. It is connected to the input connector of the DUT. The input of the analyzer is fed from the output of the DUT.

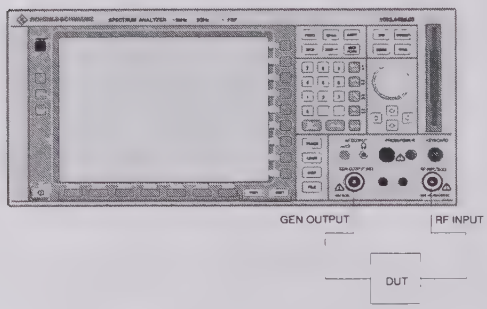

Fig.: 4-13 Test setup for transmission measurement

A calibration can be carried out to compensate for the effects of the test setup (eg frequency response of connecting cables).

Calibration of Transmission Measurement

NETWORK menu:

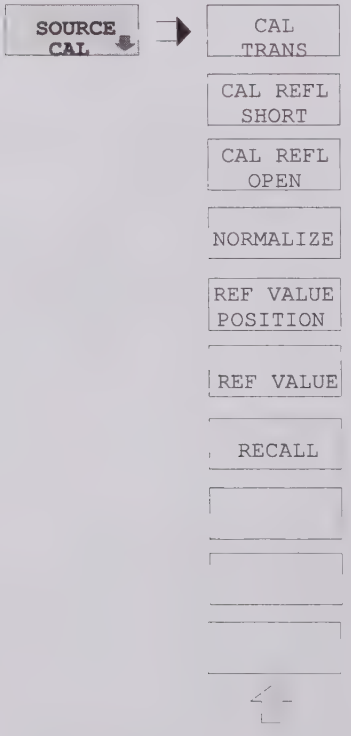

The *SOURCE CAL* softkey opens a submenu comprising of the calibration functions for the transmission and reflection measurement.

The calibration of the reflection measurement (*CAL REFL...*) and its mechanisms are described in separate sections.

To carry out a calibration for transmission measurements the whole test setup is through-connected (THRU).

The *CAL TRANS* softkey triggers the calibration of the transmission measurement.

It starts a sweep that records a reference trace. This trace is then used to calculate the difference for the normalized values.

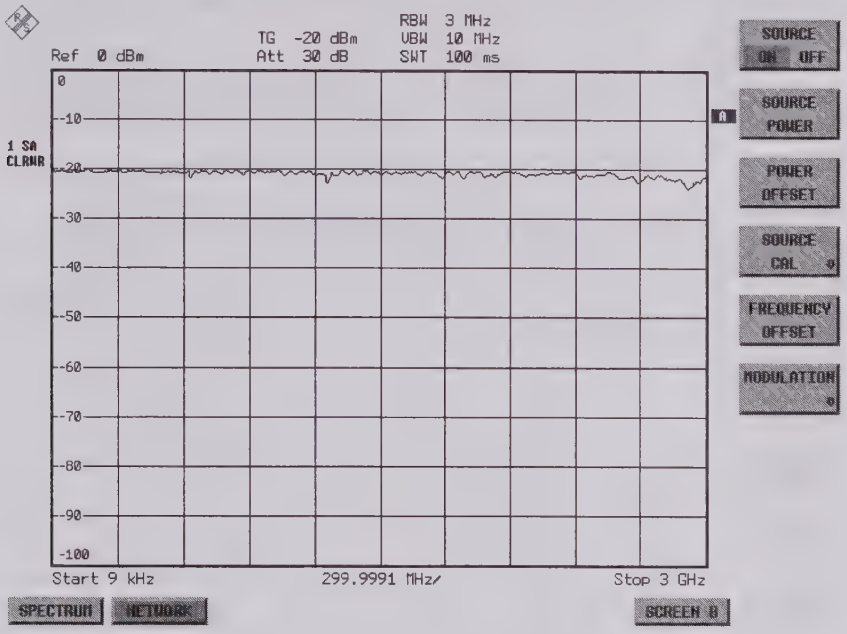

Fig.: 4-14 Calibration curve for transmission measurement

During the calibration the following message is displayed:



After the calibration the following message is displayed:

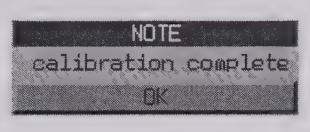

This message will be cleared automatically after approx. 3 seconds.

IEC/IEEE-bus command: `CORR:METH TRAN`

Normalization

NETWORK-SOURCE CAL menu:



The *NORMALIZE* softkey switches the normalization on or off. The softkey is only available if the memory contains a correction trace.

It is possible to shift the relative reference point within the grid using the *REF VALUE POSITION* softkey. Thus, the trace can be shifted from the upper border of the grid to the vertical center of the grid:

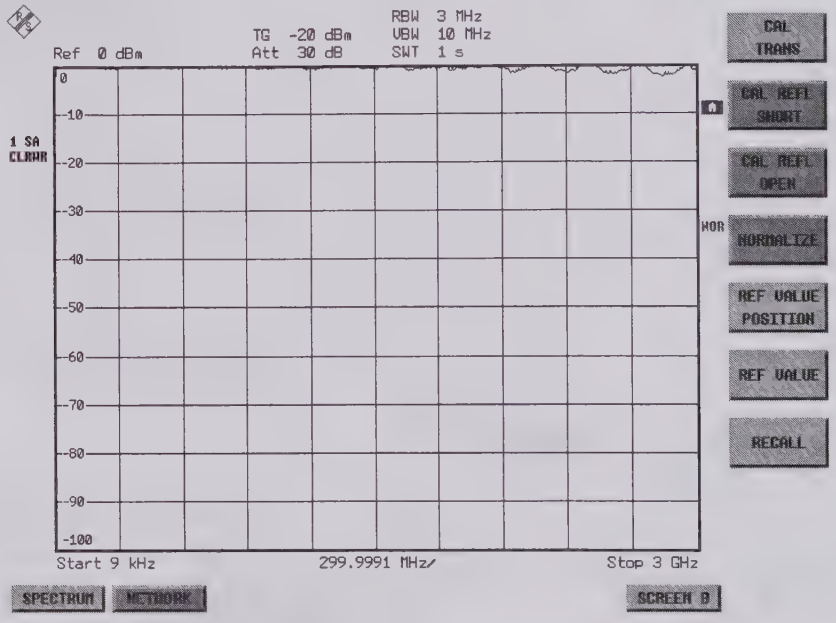

Fig.: 4-15 Normalized display

In *SPLIT SCREEN* operation, the normalization is switched on in the currently active window. Different types of normalization can be active in the two windows.

Normalization is aborted when the *NETWORK* operating mode is quit.

IEC/IEEE-bus command: `CORR ON`

REF VALUE POSITION

The *REF VALUE POSITION* softkey marks a reference position in the active window at which the normalization result (calculated difference with a reference trace) is displayed.

If no reference line is active, the softkey switches on a reference line and activates the input of its position. The line can be moved within the grid boundaries.
The reference line is switched off by pressing the softkey again.

The function of the reference line is explained in the section "Calibration mechanisms".

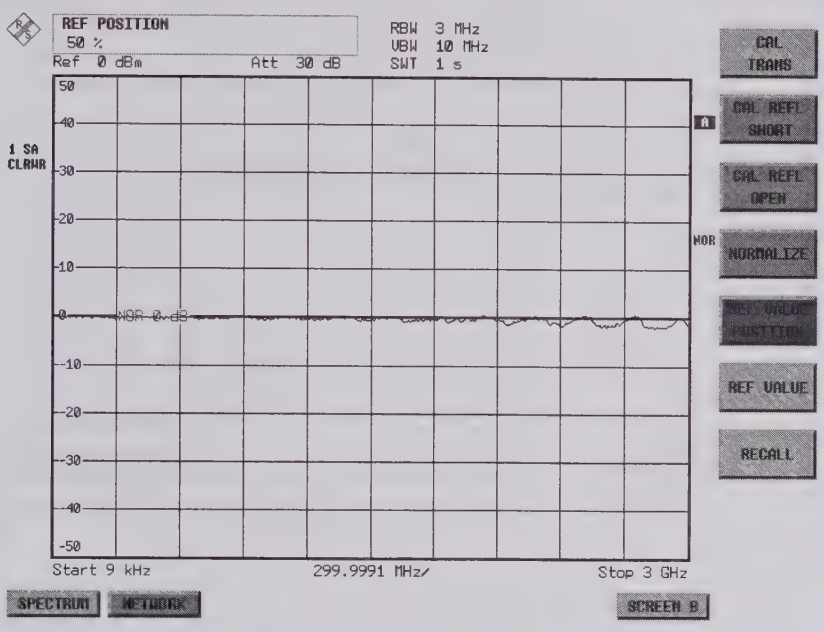

Fig.: 4-16 Normalized measurement, shifted with *REF VALUE POSITION* 50 %

IEC/IEEE-bus command: `DISP:WIND:TRAC:Y:RPOS 10PCT`



The *REF VALUE* softkey activates the input of a value which is assigned to the reference line.

With default settings the reference line corresponds to a difference of 0 dB between the currently measured trace and the reference trace. Setting the *REF VALUE* to a different value helps to compensate for changes to the level conditions in the signal path after the calibration data have been recorded. If eg after a source calibration a 10 dB attenuation is inserted into the signal path between DUT and analyzer input, the measurement trace will be moved by 10 dB down. Entering a *REF VALUE* of –10 dB will then result in the reference line for difference calculation being moved by 10 dB down as well. This means that the measured trace will be placed on it, as displayed in figure 4-17.

REF VALUE always refers to the active window.

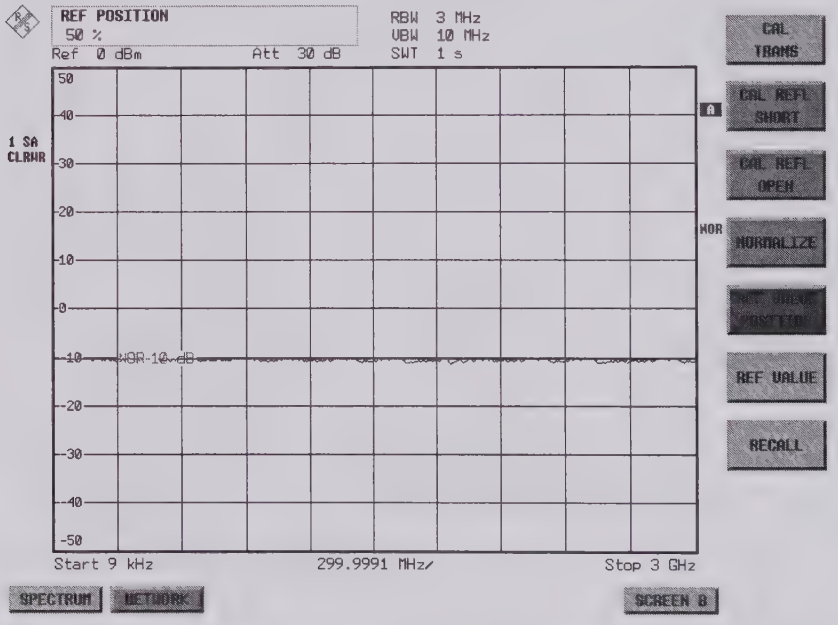

Fig.: 4-17 Measurement with REF VALUE -10 dB and REF VALUE POSITION 50%

After the reference line has been moved by entering a *REF VALUE* of –10 dB the deviation from the nominal power level can be displayed with high resolution (eg 1 dB/div). The power is still displayed in absolute values, which means that in the above example 1 dB below the nominal power (reference line) = 11 dB attenuation.

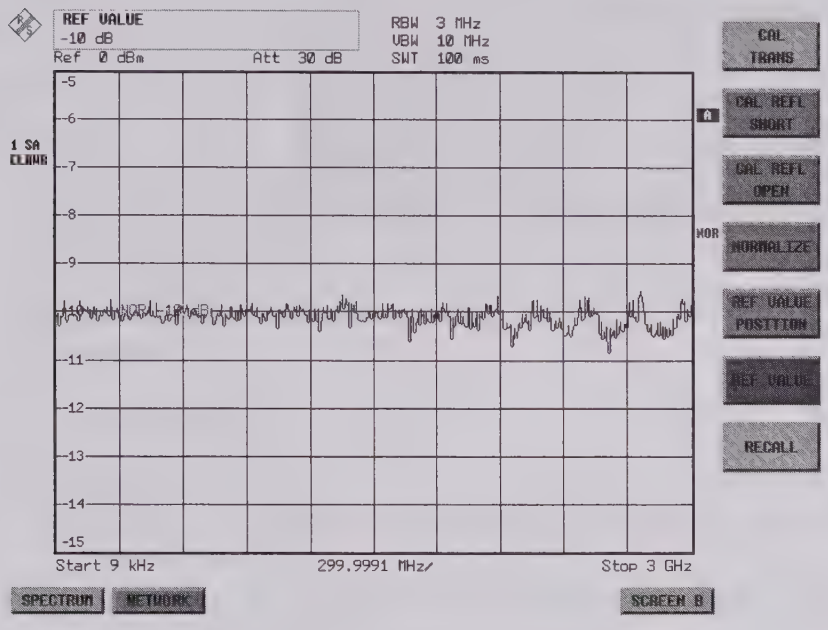

Fig.: 4-18 Measurement of a 10dB attenuator pad with 1dB/DIV

IEC/IEEE-bus command: `DISP:WIND:TRAC:Y:RVAL -10dB`

The *RECALL* softkey restores the analyzer settings that were used during source calibration.
This can be useful if device settings were changed after calibration (eg center frequency, frequency deviation, reference level, etc).

The softkey is only available if:

- the NETWORK mode has been selected
- the memory contains a calibration dataset.

IEC/IEEE-bus command: `CORR:REC`

Reflection Measurement

Scalar reflection measurements can be carried out by means of a reflection-coefficient measurement bridge.

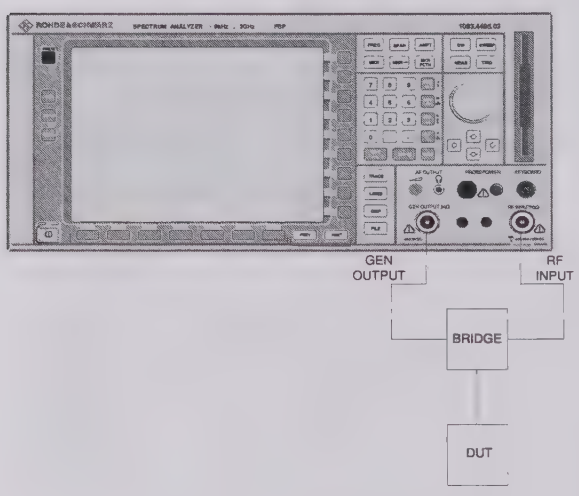

Fig.: 4-19 Test Setup for Reflection Measurement

Calibration of Reflection Measurement

The calibration mechanism for reflection measurement is basically the same as the one used for transmission measurement.

NETWORK-SOURCE CAL submenu

The *CAL REFL OPEN* softkey starts the open-circuit calibration. During calibration the following message is displayed:



IEC/IEEE-bus command:
```
CORR:METH REFL
CORR:COLL OPEN
```

The *CAL REFL SHORT* softkey starts the short-circuit calibration.

If both calibrations (open circuit, short circuit) are carried out, the calibration curve is calculated by averaging the two measurements and stored in the memory. The order of the two calibration measurements is free.

After the calibration the following message is displayed:



The message is cleared after approx. 3 seconds.

IEC/IEEE-bus command:
```
CORR:METH REFL
CORR:COLL THR
```

Calibration mechanism

Calibration means a calculation of the difference between the currently measured power and a reference curve, independent of the selected type of measurement (transmission/reflection). The hardware settings used for measuring the reference curve are included in the reference dataset.

Even with normalization switched on, the device settings can be changed in a wide area without stopping the normalization. This reduces the necessity to carry out a new normalization to a minimum.

For this purpose the reference dataset (trace with 501 measured values) is stored internally as a table of 501 points (frequency/level).
Differences in level settings between the reference curve and the current device settings are taken into account automatically. If the span is reduced, a linear interpolation of the intermediate values is applied. If the span increases, the values at the left or right border of the reference dataset are extrapolated to the current start or stop frequency, ie the reference dataset is extended by constant values.
An enhancement label is used to mark the different levels of measurement accuracy. This enhancement label is displayed at the right diagram border when normalization is switched on and a deviation from the reference setting occurs. Three accuracy levels are defined:

Table 4-3 Measurement accuracy levels

Accuracy	Enhancement label	Reason/Limitation
High	NOR	No difference between reference setting and measurement
Medium	APX (approximation)	Change of the following settings: • coupling (RBW, VBW, SWT) • reference level, RF attenuation • start or stop frequency • output level of tracking generator • frequency offset of tracking generator • detector (max. peak, min. peak, sample, etc.) Change of frequency: • max. 501 points within the set sweep limits (corresponds to a doubling of the span)
-	Aborted normalization	• more than 500 extrapolated points within the current sweep limits (in case of span doubling)

Note: *At a reference level (REF LEVEL) of -10 dBm and at a tracking generator output level of the same value the analyzer operates without overrange reserve, ie the analyzer is in danger of being overloaded if a signal is applied whose amplitude is higher than the reference line. In this case, either the message "OVLD" for overload is displayed in the status line or the display range is exceeded (clipping of the trace at the upper diagram border = Overrange).*

Overloading can be avoided as follows:

- *Reducing the output level of the tracking generator (SOURCE POWER, NETWORK menu)*
- *Increasing the reference level (REF LEVEL, AMPT menu)*

Frequency-Converting Measurements

For frequency-converting measurements (eg on converter units) the tracking generator is able to set a constant frequency offset between the output frequency of the tracking generator and the receive frequency of the analyzer. Up to an output frequency of 150 MHz the measurement can be carried out in both inverted and normal positions.

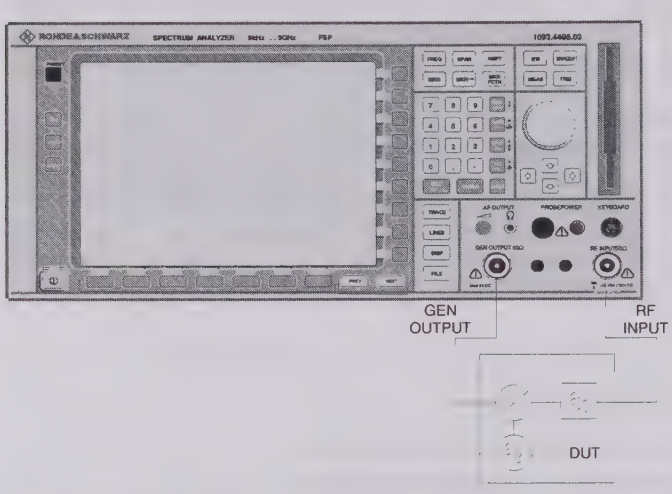

Fig.: 4-20 Test setup for frequency converting measurements

NETWORK menu

The *FREQUENCY OFFSET* softkey activates the input of the frequency offset between the output signal of the tracking generator and the input frequency of the analyzer. Possible offsets are in a range of ±150 MHz in 0.1 Hz steps.
The default setting is 0 Hz. Offsets <> 0 Hz are marked with the enhancement label **FRQ**.

If a positive frequency offset is entered, the tracking generator generates an output signal above the receive frequency of the analyzer. In case of a negative frequency offset it generates a signal below the receive frequency of the analyzer. The output frequency of the tracking generator is calculated as follows:

Tracking generator frequency = receive frequency + frequency offset.

IEC/IEEE-bus command: `SOUR:FREQ:OFFS 50MHz`

External Modulation of the Tracking Generator

NETWORK menu:

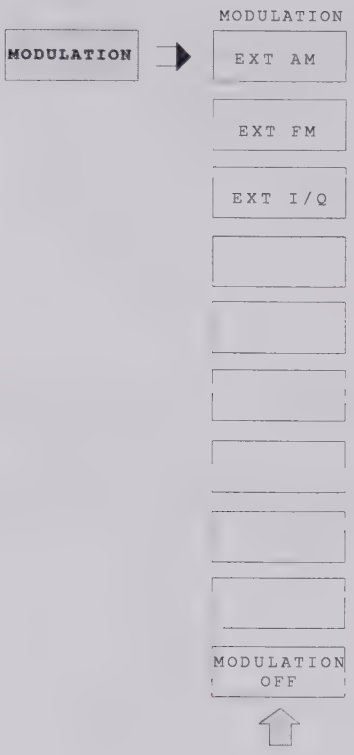

The *MODULATION* softkey opens a submenu for selecting different modulation modes.

The time characteristics of the tracking generator output signal can be influenced by means of external signals (input voltage range -1 V to +1 V).

Two BNC connectors at the rear panel are available as signal inputs. Their function changes depending on the selected modulation:

TG IN I / AM and

TG IN Q / FM

The modulation modes can be combined with each other and with the frequency offset function up to a certain degree. The following table shows which modulation modes are possible at the same time and which ones can be combined with the frequency offset function.

Table 4-4 Simultaneous modes of modulation (tracking generator)

Modulation	Frequency offset	EXT AM	EXT FM	EXT I/Q
Frequency offset		•	•	•
EXT AM	•		•	
EXT FM	•	•		
EXT I/Q	•			

• = can be combined



The *EXT AM* softkey activates an AM modulation of the tracking generator output signal.

The modulation signal is applied to the *TG IN I / AM* connector. An input voltage of 1 V corresponds to 100% amplitude modulation.

Switching on an external AM disables the following function:

– active I/Q modulation.

IEC/IEEE-bus command: `SOUR:AM:STAT ON`

The *EXT FM* softkey activates the FM modulation of the tracking generator output signal.

The modulation frequency range is 1 kHz to 100 kHz, the deviation can be set in 1-decade steps in the range of 100 Hz to 10 MHz at an input voltage of 1 V. The phase deviation η should not exceed the value 100.

Phase deviation η = deviation / modulation frequency

The modulation signal is applied to the TG IN Q / FM connector.

Switching on an external FM disables the following function:

– active I/Q modulation.

IEC/IEEE-bus command:
```
SOUR:FM:STAT ON
SOUR:FM:DEV  10MHz
```



The *EXT I/Q* softkey activates the external I/Q modulation of the tracking generator.

The signals for modulation are applied to the two input connectors *TG IN I* and *TG IN Q* at the rear panel of the unit. The input voltage range is ±1 V into 50 Ω.

Switching on an external I/Q modulation disables the following functions:

- active external AM
- active external FM

Functional description of the quadrature modulator:

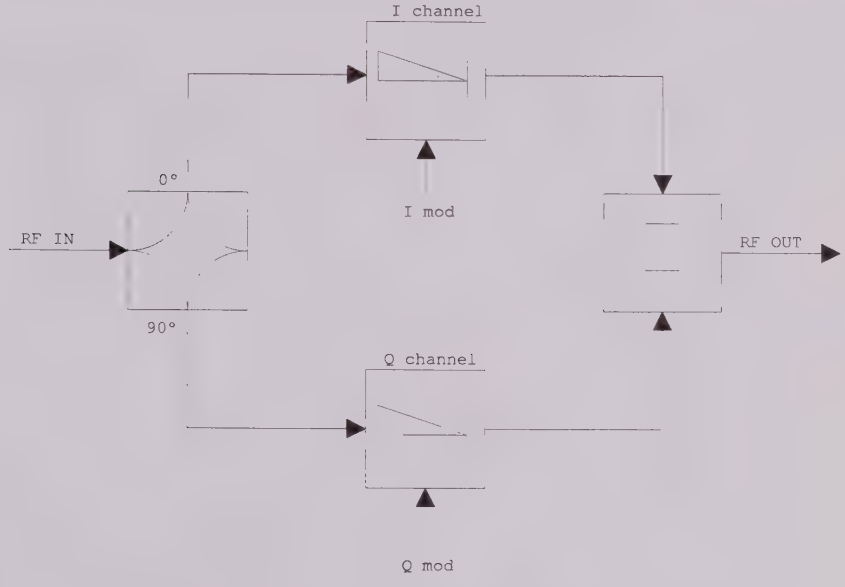

Fig.: 4-21 I/Q modulation

I/Q modulation is performed by means of the built-in quadrature modulator. The RF signal is divided into two orthogonal I and Q components (inphase and quadrature phase). Amplitude and phase are controlled in each path by the I and Q modulation signal. By adding the two components an RF output signal is generated that can be controlled in amplitude and phase.

IEC/IEEE-bus command: `SOUR:DM:STAT ON`



The *MODULATION OFF* softkey switches off the modulation of the tracking generator.

IEC/IEEE-bus command: `SOUR:MOD:STAT OFF`

Option External Generator Control - FSP-B10

The external generator control option permits to operate a number of commercially available generators as tracking generator on the FSP. Thus, scalar network analysis with the FSP is also possible outside the frequency range of the internal tracking generator when the appropriate generators are used.

The FSP also permits to set a frequency offset for frequency-converting measurements when external generators are used. For harmonics measurements or frequency-converting measurements, it is also possible to enter a factor, by which the generator frequency is increased or reduced compared with the receive frequency of the FSP. Only make sure that the resulting generator frequencies do not exceed the allowed setting range of the generator.

The settable level range also depends on the generator used.
The generator is controlled via the – optional – second IECBUS interface of the FSP (= IEC2, supplied with the option) and, with some Rohde & Schwarz generators, additionally via the TTL synchronization interface included in the AUX interface of the FSP.

Note: *The use of the TTL interface enables considerably higher measurement rates as pure IECBUS control, because the frequency stepping of the FSP is directly coupled with the frequency stepping of the generator.*

Therefore, the frequency sweep differs according to the capabilities of the generator used:

- In the case of generators without TTL interface, the generator frequency is first set for each frequency point via IECBUS, then the setting procedure has to be completed before recording of measured values is possible.

- In the case of generators with TTL interface, a list of the frequencies to be set is entered into the generator before the beginning of the first sweep. Then the sweep is started and the next frequency point selected by means of the TTL handshake line TRIGGER. The recording of measured values is only enabled when the generator signals the end of the setting procedure via the BLANK signal. This method is considerably faster than pure IECBUS control.

With the "SELECT GENERATOR" softkey, a list of the supported generators with the frequency and level range as well as the capabilities used is included.

The external generator can be used in all operating modes. Recording of test setup calibration values (*SOURCE CAL*) and normalization with the correction values (*NORMALIZE*) are only possible in the *NETWORK* mode.

Note: *In order to enhance measurement accuracy a common reference frequency should be used for both the FSP and the generator. If no independent 10 MHz reference frequency is available, it is recommended to connect the reference output of the generator with the reference input of the FSP and to enable usage of the external Reference on the FSP via SETUP – REFERENCE EXT.*

Like the internal tracking generator, the external generator is activated by means of the *NETWORK* hotkey in the hotkey bar at the screen bottom:

External Generator Settings

The *NETWORK* hotkey opens the menu for setting the functions of the external generator.

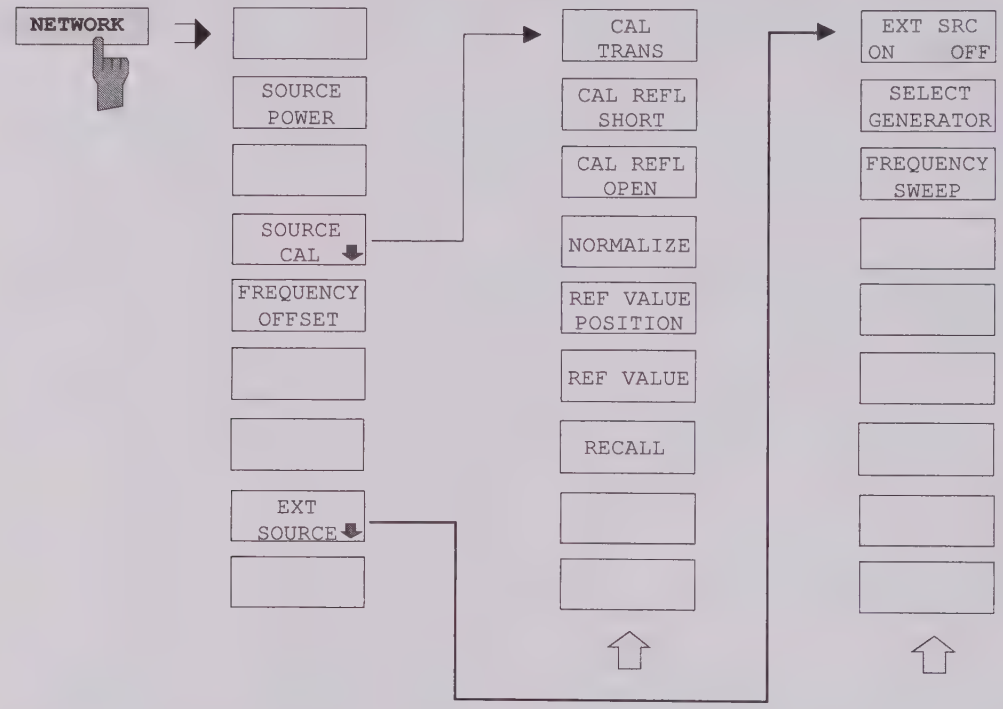

Note: *Other softkeys are available in the displayed menus for controlling the internal tracking generator when option Tracking Generator FSP-B9 is fitted. For detailed information see section "Option Tracking Generator FSP-B9".*



The *SOURCE POWER* softkey allows the generator output level to be entered. The allowed value range depends on the generator selected. For more details see the table in the section "Configuration of External Generator".

If, in addition to the option *External Generator Control FSP-B10* the option *Tracking Generator FSP-B9* is also installed, the softkey will change the output level of the internal tracking generator or of the external generator, depending on which generator is currently switched on.
The default output level is -20dBm.

IEC-bus command `SOUR:EXT:POW -20dBm`

Transmission Measurement

The transmission characteristic of a two-port network is measured . The external generator serves as a signal source. It is connected to the input connector of the DUT. The input of the analyser is fed from the output of the DUT.

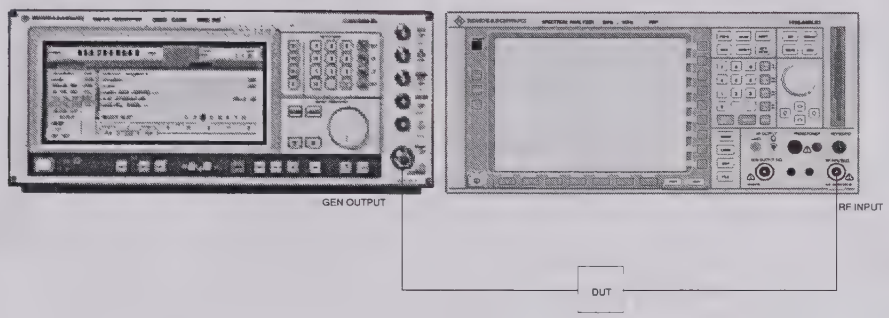

Fig. 4-13 Test setup for transmission measurement

A calibration can be carried out to compensate for the effects of the test setup (eg frequency response of connecting cables).

Calibration of Transmission Measurement

NETWORK menu:

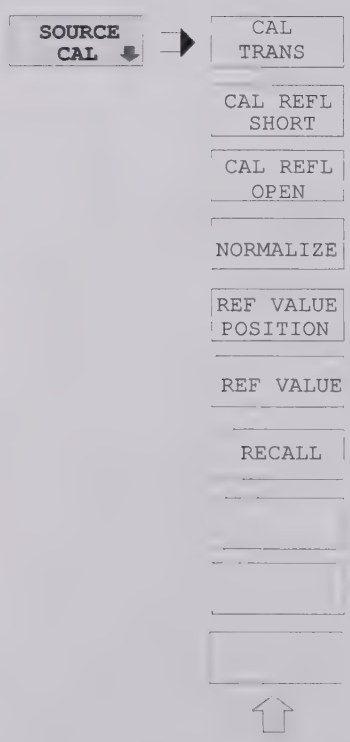

The *SOURCE CAL* softkey opens a submenu comprising the calibration functions for the transmission and reflection measurement.

The calibration of the reflection measurement (*CAL REFL...*) and its functioning are described in separate sections.

To carry out a calibration for transmission measurements the whole test setup is through-connected (THRU).

The *CAL TRANS* softkey triggers the calibration of the transmission measurement.

It starts a sweep that records a reference trace. This trace is then used to obtain the differences to the normalized values.

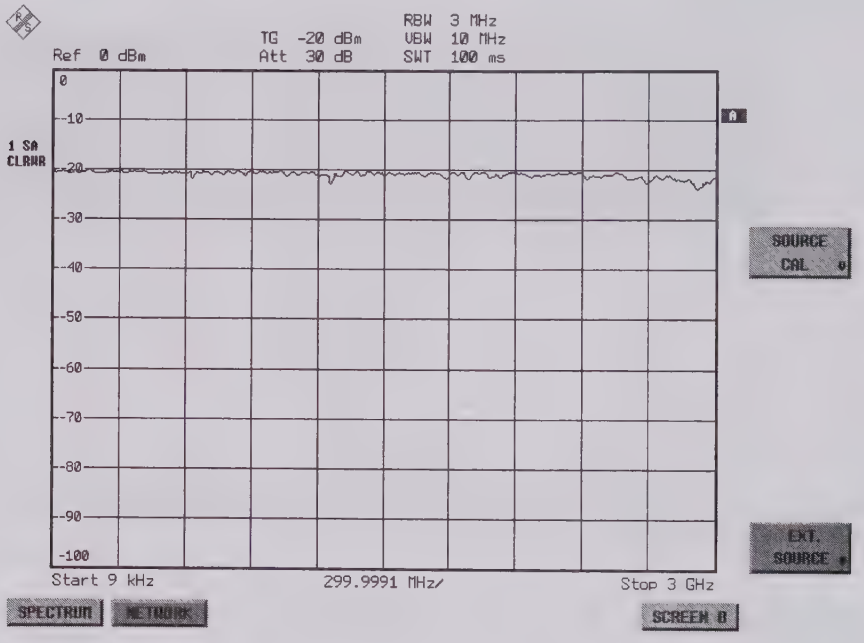

Fig. 4-14 Calibration curve for transmission measurement

During the calibration the following message is displayed:



After the calibration sweep the following message is displayed:



This message is cleared after approx. 3 seconds.

IEC-bus command `CORR:METH TRAN`

Normalization:

NETWORK - SOURCE CAL menu:



The *NORMALIZE* softkey switches normalization on or off. The softkey is only available if the memory contains a correction trace.

It is possible to shift the relative reference point within the grid using the *REF VALUE POSITION* softkey. Thus, the trace can be shifted from the top grid margin to the middle of the grid:

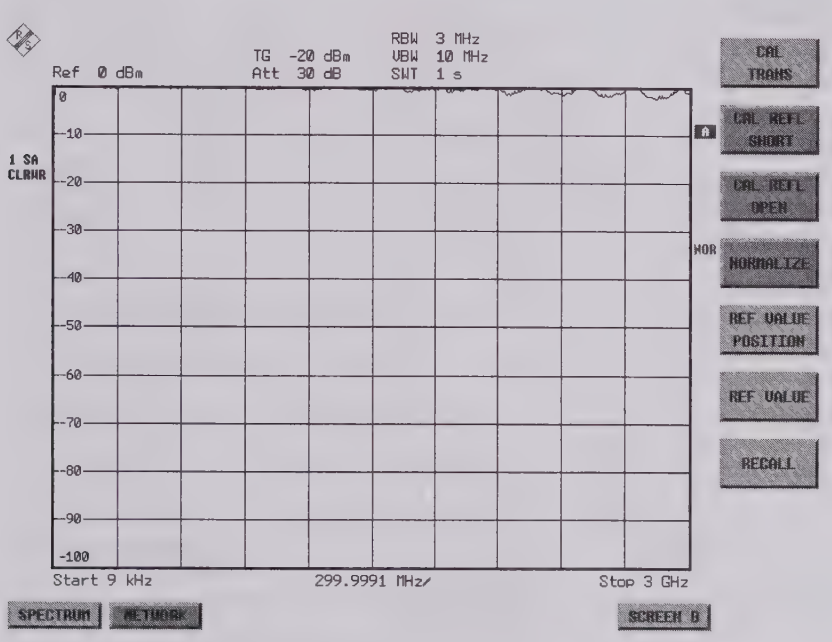

Fig. 4-15 Normalized display

In the *SPLIT SCREEN* setting, the normalization is switched on in the current window. Different normalizations can be active in the two windows.

Normalization is aborted when the *NETWORK* mode is quit.

IEC/IEEE-bus command: `CORR ON`

The *REF VALUE POSITION* softkey (reference position) marks a reference position in the active window on which the normalization (difference formation with a reference curve) is performed.

When pressed for the first time, the softkey switches on the reference line and activates the input of its position. The line can be shifted within the grid limits.

The reference line is switched off by pressing the softkey again.

The function of the reference line is explained in the section "Functioning of Calibration".

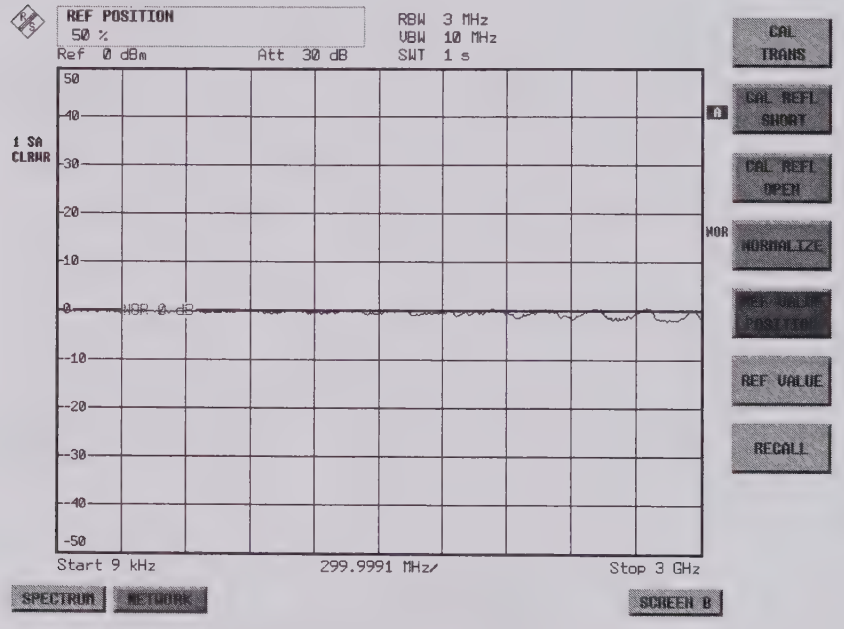

Fig. 4-16 Normalized measurement, shifted with *REF VALUE POSITION* 50 %

IEC-bus command `DISP:WIND:TRAC:Y:RPOS 10PCT`



The *REF VALUE* softkey activates the input of a level difference which is assigned to the reference line.

In the default setting, the reference line corresponds to a level difference of 0 dB. If e.g. a 10-dB attenuator pad is inserted between DUT and analyzer input between recording of the calibration data and normalization, the trace will be shifted down by 10 dB. By entering a *REF VALUE* of –10 dB the reference line for difference formation can also be shifted down by 10 dB so that it will again coincide with the trace (see Fig. 4-17).

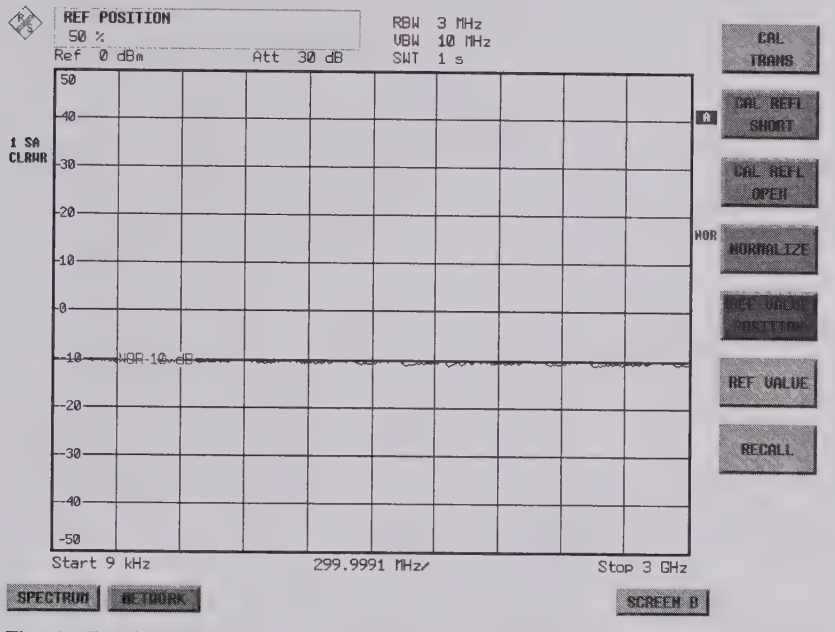

Fig. 4-17 Measurement with REF VALUE -10dB and REF VALUE POSITION 50%

After the reference line has been shifted by entering *REF VALUE* –10 dB, departures from the nominal value can be displayed with high resolution (e.g. 1 dB / Div.). The absolute measured values are still displayed, in the above example, 1 dB below nominal value (reference line) = 11 dB attenuation.

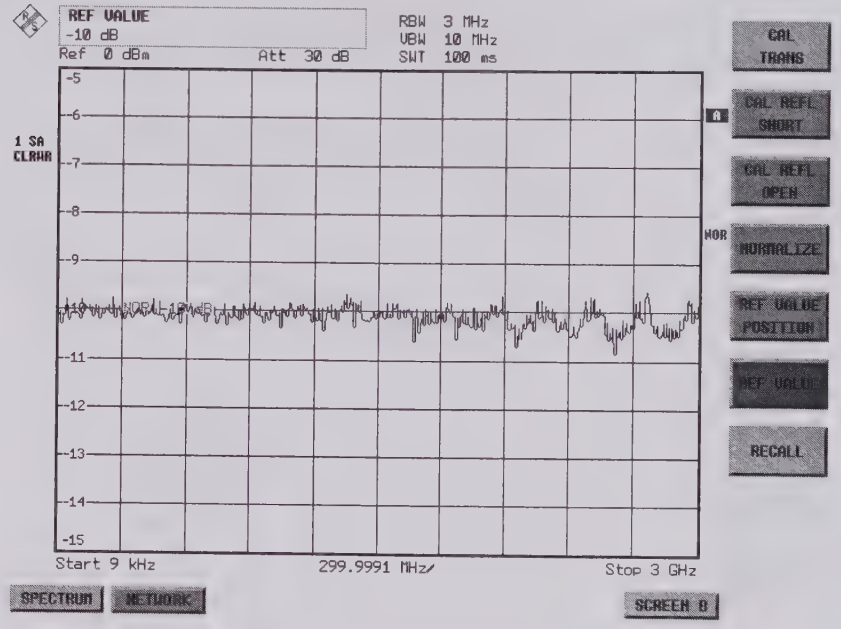

Fig. 4-18 Measurement of a 10-dB attenuator pad with 1dB/DIV

IEC-bus command `DISP:WIND:TRAC:Y:RVAL -10dB`

The *RECALL* softkey restores the analyzer setting with which the calibration was carried out.
This can be useful if the device setting was changed after calibration (eg center frequency setting, frequency deviation, reference level, etc).

The softkey is only available if:

- the *NETWORK* mode has been selected
- the memory contains a calibration data set.

IEC/IEEE-bus command `CORR:REC`

Reflection Measurement

Scalar reflection measurements can be carried out by means of a reflection-coefficient bridge.

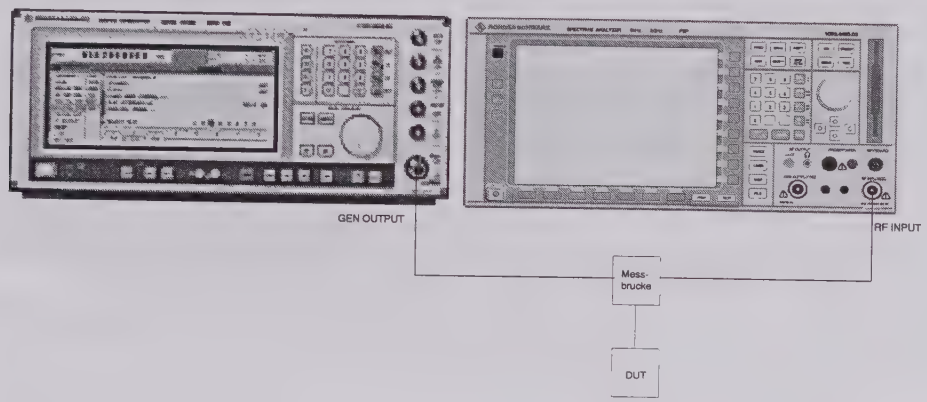

Fig. 4-19 Test setup for reflection measurement

Calibration of Reflection Measurement

The calibration mechanism essentially corresponds to that of the transmission measurement.

NETWORK-SOURCE CAL submenu

The *CAL REFL OPEN* softkey starts the open-circuit calibration. During calibration the following message is displayed:



IEC-bus command
```
CORR:METH REFL
CORR:COLL OPEN
```

The *CAL REFL SHORT* softkey starts the short-circuit calibration.

If both calibrations (open circuit, short circuit) are carried out, the calibration curve is formed by averaging the two measurements and stored in the memory. The order of measurements is optional.

After the calibration the following message is displayed:



The display is cleared after approx. 3 seconds.

IEC-bus command
```
CORR:METH REFL
CORR:COLL THR
```

Calibration mechanism

Calibration means a calculation of the difference between the currently measured power and a reference curve, independent of the selected type of measurement (transmission/reflection). The hardware settings used for measuring the reference curve are included in the reference dataset.

Even with normalization switched on, the device settings can be changed in a wide area without stopping the normalization. This reduces the necessity to carry out a new normalization to a minimum.

For this purpose the reference dataset (trace with 501 measured values) is stored internally as a table of 501 points (frequency/level).
Differences in level settings between the reference curve and the current device settings are taken into account automatically. If the span is reduced, a linear interpolation of the intermediate values is applied. If the span increases, the values at the left or right border of the reference dataset are extrapolated to the current start or stop frequency, ie the reference dataset is extended by constant values.
An enhancement label is used to mark the different levels of measurement accuracy. This enhancement label is displayed at the right diagram border when normalization is switched on and a deviation from the reference setting occurs. Three accuracy levels are defined:

Table 4-3 Measurement accuracy levels

Accuracy	Enhancement label	Reason/Limitation
High	NOR	No difference between reference setting and measurement
Medium	APX (approximation)	Change of the following settings: • coupling (RBW, VBW, SWT) • reference level, RF attenuation • start or stop frequency • output level of tracking generator • frequency offset of tracking generator • detector (max. peak, min. peak, sample, etc.) Change of frequency: • max. 501 points within the set sweep limits (corresponds to a doubling of the span)
-	Aborted normalization	• more than 500 extrapolated points within the current sweep limits (in case of span doubling)

Note: *At a reference level (REF LEVEL) of -10 dBm and at a tracking generator output level of the same value the analyzer operates without overrange reserve, ie the analyzer is in danger of being overloaded if a signal is applied whose amplitude is higher than the reference line. In this case, either the message "OVLD" for overload is displayed in the status line or the display range is exceeded (clipping of the trace at the upper diagram border = Overrange).*

Overloading can be avoided as follows:

- *Reducing the output level of the tracking generator (SOURCE POWER, NETWORK menu)*
- *Increasing the reference level (REF LEVEL, AMPT menu)*

Frequency-converting Measurements

For frequency-converting measurements (e.g. on converters) the external generator is able to set a constant frequency offset between the output frequency of the generator and the receive frequency of the analyzer and, in addition, the generator frequency as a multiple of the analyzer.

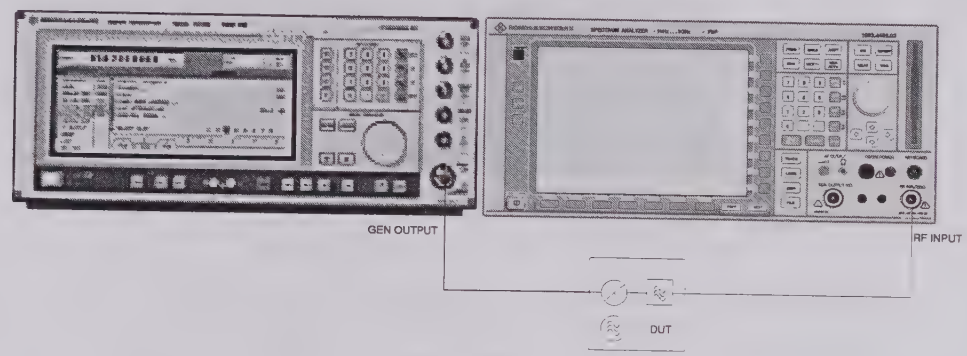

Fig. 4-20 Test setup for frequency-converting measurements

NETWORK menu



The *FREQUENCY OFFSET* softkey activates the input of the frequency offset between the output signal of the generator and the input frequency of the analyzer. The allowed setting range depends on the frequency range of the generator selected.
The default setting is 0 Hz; offsets <> 0 Hz are assigned the enhancement label **FRQ**.

If a positive frequency offset is entered, the generator generates an output signal above the receive frequency of the analyzer. In case of a negative frequency offset it generates a signal below the receive frequency of the analyzer. The output frequency of the generator is calculated as follows:

Generator frequency = receive frequency + frequency offset.

IEC-bus command `SOUR:EXT:FREQ:OFFS 1GHZ`

Configuration of an External Generator

NETWORK menu:

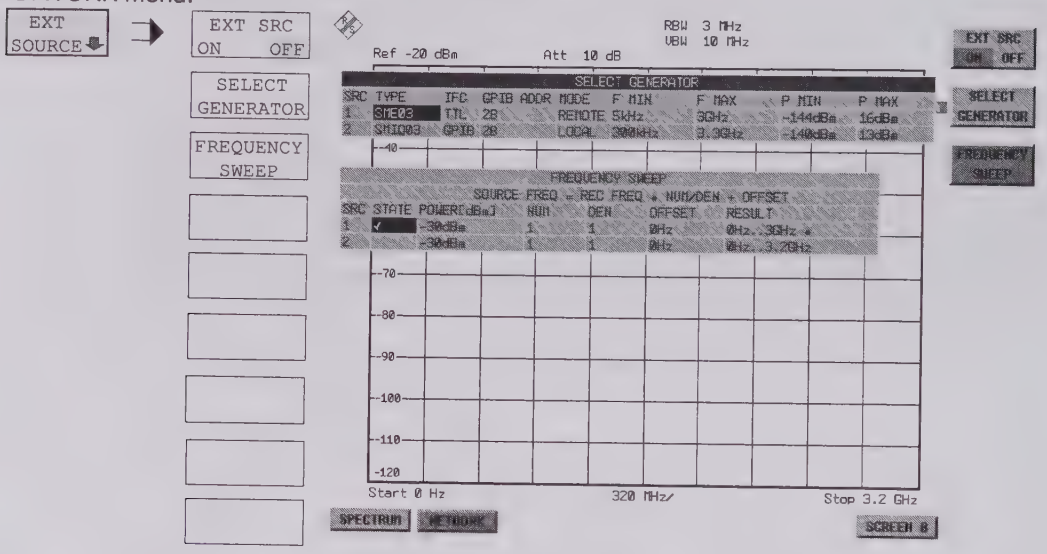

The *EXT SOURCE* softkey opens a submenu for configuration of the external generator.
The FSP is able to manage two generators, one of which can be active at the time.

The *EXT SRC ON / OFF* softkey switches the external generator on or off.
It can only be switched on successfully if the generator has been selected by means of *SELECT GENERATOR* and configured correctly by means of *FREQUENCY SWEEP*.
If one of these conditions is not fulfilled, an error message will be output.

Notes:

When switching on the external generator, the FSP switches off the internal tracking generator and starts programming the generator settings via the IECBUS.

At the same time, the maximum stop frequency is limited to the maximum generator frequency. This upper limit is automatically reduced by the set frequency offset of the generator and a set multiplication factor.

With the external generator switched on, the FFT filters (FILTER TYPE FFT in the menu BW) are not available.

If there is an error on the IECBUS during programming of the external generator, the generator is automatically switched off and the following error message output:

IEC-bus command `SOUR:EXT ON`



The *SELECT GENERATOR* softkey opens a table for selection of the generator and definition of IECBUS address and control interface.
The table permits configuration of two generators so that switching between two different configurations is easily possible.

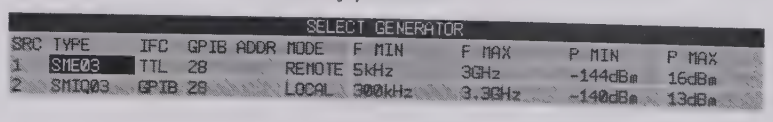
SELECT GENERATOR
SRC TYPE IFC GPIB ADDR MODE F MIN F MAX P MIN P MAX
1 SME03 TTL 28 REMOTE 5kHz 3GHz -144dBm 16dBm
2 SMIQ03 GPIB 28 LOCAL 300kHz 3.3GHz -140dBm 13dBm

The individual fields contain the following settings:

SRC Index of generator selected

TYPE The field opens the list with the available generators:



After completion of the selection, the remaining fields of the table are filled with the generator characteristics.
A list of generator types supported by the FSP is to be found at the end of section "Softkey *SELECT GENERATOR*".

IFC This field selects the interface type of external generator 1or 2. The following types are available:

GPIB IECBUS only, suitable for all generators of other manufacturers and some Rohde & Schwarz instruments

or

TTL IECBUS and TTL interface for synchronization, for most of the Rohde & Schwarz generators, see table above.

The two operating modes differ in the speed of the control: Whereas, with pure IECBUS operation, each frequency to be set must be individually transferred to the generator, additional use of the TTL interface permits to program a total frequency list at once and subsequently perform the frequency stepping via TTL handshake, which is a big advantage in terms of speed.

Note:
Generators equipped with the TTL interface can also be operated with IECBUS (= GPIB) only.
Only one of the two generators can be operated with TTL interface at a time. The other generator must be configured for IECBUS (GPIB).

GPIB ADDR IECBUS address of the respective generator. Addresses from 0 to 30 are possible.

MODE Operating mode of generator. The generator activated using the FREQUENCY SWEEP softkey is automatically set to remote mode (REMOTE), the other to manual mode (LOCAL).

F MIN F MAX Frequency range of generator. Select the start and stop frequency of the FSP in a way that the specified range is not exceeded.
If the start frequency lies below F MIN, the generator is only switched on when F MIN is reached.
If the stop frequency lies above F MAX, it is limited to F MAX when the generator is switched on using the EXT SRC ON/OFF softkey.

P MIN P MAX Level range of generator. This field defines the allowed input range for the *POWER* column in the *FREQUENCY SWEEP* table.

IEC-bus commands
```
SYST:COMM:RDEV:GEN2:TYPE 'SME02'
SYST:COMM:RDEV:GEN:LINK TTL
SYST:COMM:GPIB:RDEV:GEN1:ADDR 28
```

List of Generator Types Supported by the FSP

Generator	Interface Type	Generator Min Freq	Generator Max Freq	Generator Min Power dBm	Generator Max Power dBm
SME02	TTL	5 kHz	1.5 GHz	-144	+16
SME03	TTL	5 kHz	3.0 GHz	-144	+16
SME06	TTL	5 kHz	6.0 GHz	-144	+16
SMG	GPIB	100 kHz	1.0 GHz	-137	+13
SMGL	GPIB	9 kHz	1.0 GHz	-118	+30
SMGU	GPIB	100 kHz	2.16 GHz	-140	+13
SMH	GPIB	100 kHz	2.0 GHz	-140	+13
SMHU	GPIB	100 kHz	4.32 GHz	-140	+13
SMIQ02B	TTL	300 kHz	2.2 GHz	-144	+13
SMIQ02E	GPIB	300 kHz	2.2 GHz	-144	+13
SMIQ03B	TTL	300 kHz	3.3 GHz	-144	+13
SMIQ03E	GPIB	300 kHz	3.3 GHz	-144	+13
SMIQ04B	TTL	300 kHz	4.4 GHz	-144	+10
SMIQ06B	TTL	300 kHz	6.4 GHz	-144	+10
SML01	GPIB	9 kHz	1.1 GHz	-140	+13
SMR20	GPIB	1 GHz	20 GHz	-130 [2]	+11 [2]
SMR20B11 [1]	GPIB	10 MHz	20 GHz	-130 [2]	+13 [2]
SMR27	GPIB	1 GHz	27 GHz	-130 [2]	+11 [2]
SMR27B11 [1]	GPIB	10 MHz	27 GHz	-130 [2]	+12 [2]
SMR30	GPIB	1 GHz	30 GHz	-130 [2]	+11 [2]
SMR30B11 [1]	GPIB	10 MHz	30 GHz	-130 [2]	+12 [2]
SMR40	GPIB	1 GHz	40 GHz	-130 [2]	+9 [2]
SMR40B11 [1]	GPIB	10 MHz	40 GHz	-130 [2]	+12 [2]
SMP02	TTL	10 MHz	20 GHz	-130 [3]	+17 [3]
SMP03	TTL	10 MHz	27 GHz	-130 [3]	+13 [3]
SMP04	TTL	10 MHz	40 GHz	-130 [3]	+12 [3]
SMP22	TTL	10 MHz	20 GHz	-130 [3]	+20 [3]
SMT02	GPIB	5.0 kHz	1.5 GHz	-144	+13
SMT03	GPIB	5.0 kHz	3.0 GHz	-144	+13
SMT06	GPIB	5.0 kHz	6.0 GHz	-144	+13
SMX	GPIB	100 kHz	1.0 GHz	-137	+13
SMY01	GPIB	9 kHz	1.04 GHz	-140	+13
SMY02	GPIB	9 kHz	2.08 GHz	-140	+13
HP8340A	GPIB	10 MHz	26.5 GHz	-110	10
HP ESG-A Series 1000A, 2000A, 3000A, 4000A	GPIB	250 kHz	4 GHz	-136	20
HP ESG-D SERIES E4432B	GPIB	250 kHz	3 GHz	-136	+10

1) Requires the option SMR-B11 to be fitted.
2) Maximum/minimum power depends on presence of Option SMR-B15/-B17 and set frequency range. For more details see SMR data sheet.
3) Maximum/minimum power depends on presence of Option SMP-B15/-B17 and set frequency range. For more details see SMP data sheet.

FREQUENCY SWEEP

The *FREQUENCY SWEEP* softkey opens a table for setting the generator level as well as the multiplier and the offset used to derive the generator frequency from the analyzer frequency.

This table also permits configuration of two generators so that switching between two different configurations is easily possible.

FREQUENCY SWEEP

	SOURCE	FREQ = REC FREQ * NUM/DEN + OFFSET			
SRC	STATE POWER[dBm]	NUM	DEN	OFFSET	RESULT
1	✓ -30dBm	1	1	0Hz	0Hz..3GHz *
2	-30dBm	1	1	0Hz	0Hz..3.2GHz

SRC Index of selected generator

STATE Selects the active generator. Only one generator can be active at a time. The operating mode of the active generator is set to remote control in the SELECT GENERATOR table.

POWER Permits to enter the generator level within the limits P MIN to P MAX of the *SELECT GENERATOR* table.

NUM Numerator,

DEN Denominator,

OFFSET Offset, used to derive the generator frequency from the current frequency of the FSP according to the following formula:

$$F_{Generator} = F_{Analyzer} * \frac{Numerator}{Denominator} + F_{Offset}$$

Note that the frequencies resulting from start and stop frequency of the FSP do not exceed the allowed generator range:

- If the start frequency lies below F MIN, the generator is only switched on when F MIN is reached.
- If the stop frequency lies above F MAX, the generator is switched off. When the generator is subsequently switched on using the *EXT SRC ON/OFF* softkey, the stop frequency is limited to F MAX.
- If the stop frequency lies below F MIN, the generator is switched off and the following error message output:

ERROR
GENERATOR RANGES EXEEDED; EXT GEN SWITCHED OFF.

- In the time domain (Span = 0 Hz) the generator frequency is derived from the set receive frequency of the FSP using the calculation formula.

For the sake of clarity, the formula is also displayed in the table.

RESULT The frequency range of the generator resulting from the calculation formula. An asterisk (*) after the upper limit indicates that the stop frequency of the FSP must be adapted when the generator is switched on in order not to exceed its maximum frequency. In the following illustration, this is true for the upper generator at a stop frequency of 3.2 GHz of the FSP, whereas the lower generator does not yet require an adaptation:



IEC-bus commands

```
SOUR:EXT:POW -30dBm
SOUR:EXT:FREQ:NUM 4
SOUR:EXT:FREQ:DEN 3
SOUR:EXT:FREQ:OFFS 100MHZ
```

Option LAN Interface – FSP-B16

Using the option FSP-B16 LAN Interface, the instrument can be connected to an Ethernet LAN (Local Area Network). Thus it is possible to transfer data via the network and use network printers. The network card allows both for a 10-MHz Ethernet IEEE 802.3 and a 100-MHz Ethernet IEEE 802.3u. The selection between 10 Mbit/s and 100Mbit/s can take place either automatically or via manual setting.

Connecting the Instrument to the Network

Caution:
Before connecting the instrument to the network it is recommended to contact the network administrator, in particular larger LAN installations are affected. Faults in the connection may have a negative effect on the entire network.

The instrument is connected to a network hub of the desired LAN segment via a commercially-available RJ45 cable (not supplied with the instrument) at the instrument rear panel. Since RJ45 provides no bus but a star network topology, no other precautions need to be taken for the connection.

The connection procedure does not produce any disturbances in the network traffic. Disconnection from the network is easily possible provided that there is no more data traffic from and to the instrument.

Installing the Software

The data transfer in the network takes place in data blocks, the so-called packets. In addition to the useful data, further information on the operation, ie the so-called protocol data (transmitter, receiver, type of data, sequence), is transferred in the packets. For processing the protocol information, suitable drivers must be installed. For the network services (file transfer, directory services, printing in the network) a network operating system needs to be installed.

Installation and Configuration of the Driver for the Network Card

Notes:

- *The WINDOWS NT files required for the installation of network drivers, protocols or services are included in the directory "C:\I386".*
- *For the installation, a PC keyboard with trackball (or an additional mouse instead) is required.*

➢ Press the *SETUP* key.

The *SETUP* menu opens.

➢ Press the *GENERAL SETUP* key.

The *GENERAL SETUP* menu opens.

➢ Press the CONFIGURE NETWORK softkey.

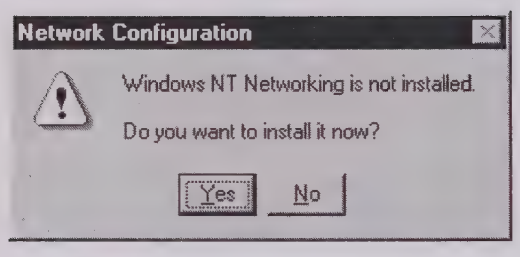

➢ Answer the prompt "Do you want to install it now?" with "Yes".

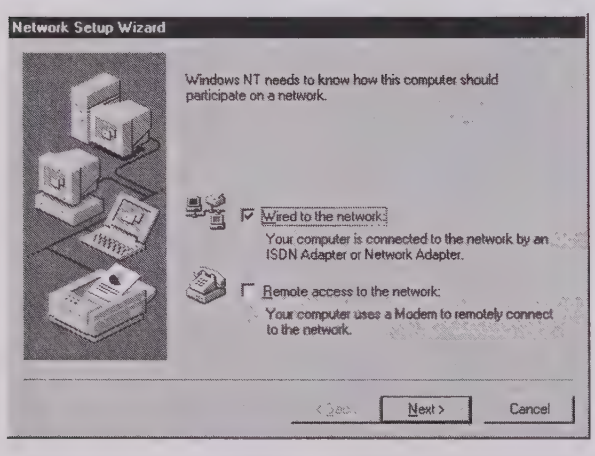
Network Setup Wizard
Windows NT needs to know how this computer should participate on a network.
Wired to the network:
Your computer is connected to the network by an ISDN Adapter or Network Adapter.
Remote access to the network:
Your computer uses a Modem to remotely connect to the network.
Next >
Cancel

➢ Leave the default setting "Wired to the network" unchanged and confirm by means of "NEXT".

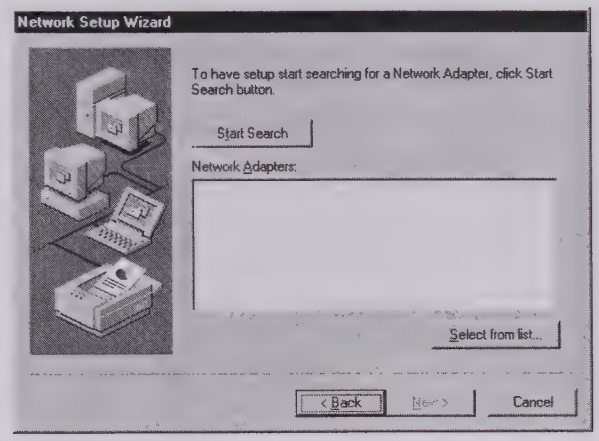
Network Setup Wizard
To have setup start searching for a Network Adapter, click Start Search button.
Start Search
Network Adapters:
Select from list...
< Back
Next >
Cancel

➢ To select the appropriate network card click on "Select from list".

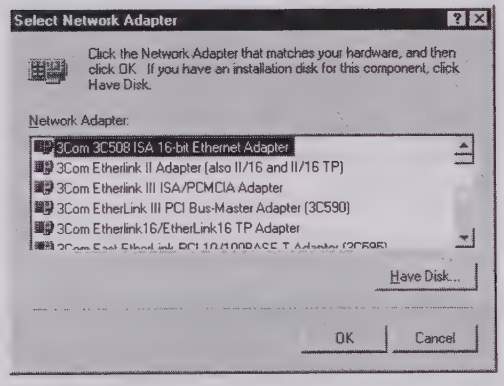
Select Network Adapter
Click the Network Adapter that matches your hardware, and then click OK. If you have an installation disk for this component, click Have Disk.
Network Adapter:
3Com 3C508 ISA 16-bit Ethernet Adapter
3Com Etherlink II Adapter (also II/16 and II/16 TP)
3Com Etherlink III ISA/PCMCIA Adapter
3Com EtherLink III PCI Bus-Master Adapter (3C590)
3Com Etherlink16/EtherLink16 TP Adapter
Have Disk...
OK
Cancel

➢ Click on "Have Disk".

A prompt to insert the disk into the floppy drive will appear.

➢ Insert the driver disk and click on "OK".

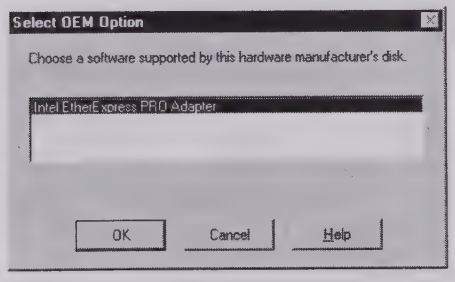

➢ Confirm "Intel EtherExpress PRO Adapter" with "OK".

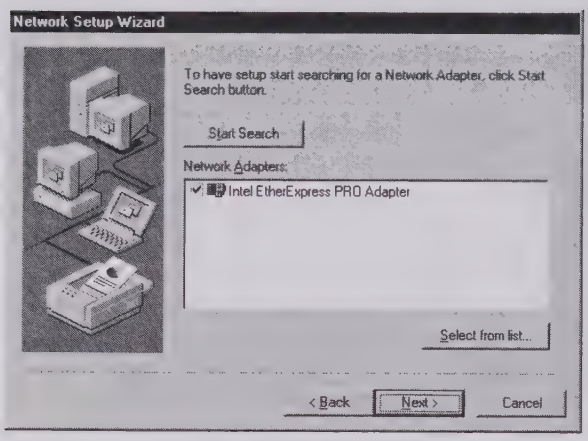
Network Setup Wizard
To have setup start searching for a Network Adapter, click Start Search button.
Start Search
Network Adapters:
Intel EtherExpress PRO Adapter
Select from list...
< Back
Next >
Cancel

➢ Close the dialog by means of "NEXT" after selecting "Intel EtherExpress PRO Adapter" once again.

Selection of the Network Protocols

Note: *The network administrator knows the protocols to be used. For the RSIB interface, the TCP/IP protocol must be installed in any case.*

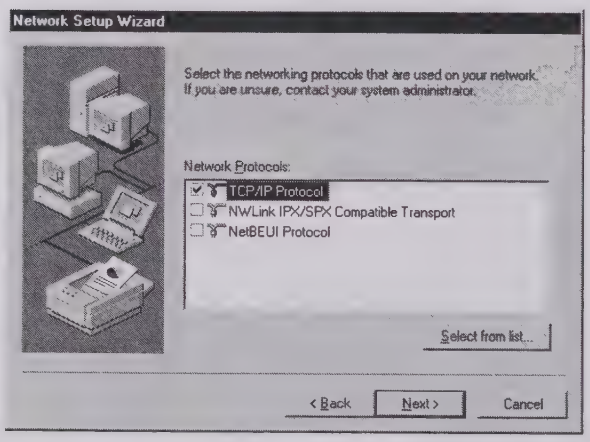
Network Setup Wizard
Select the networking protocols that are used on your network. If you are unsure, contact your system administrator.
Network Protocols:
TCP/IP Protocol
NWLink IPX/SPX Compatible Transport
NetBEUI Protocol
Select from list...
< Back
Next >
Cancel

➢ Select the desired protocols and confirm using "NEXT".

Selection of the Network Services

To be able to utilize the resources in the network, it is necessary to install the respective services.

Note: *The network administrator knows the services to be used.*

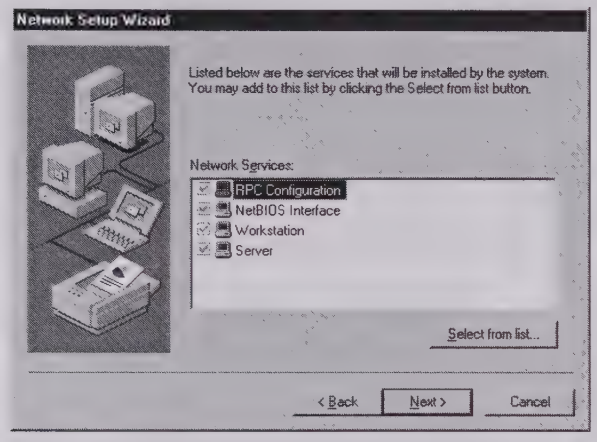
Network Setup Wizard
Listed below are the services that will be installed by the system. You may add to this list by clicking the Select from list button.
Network Services:
RPC Configuration
NetBIOS Interface
Workstation
Server
Select from list...
< Back
Next >
Cancel

➢ During the first installation, the selected services cannot be changed.

Further services can be added after completion of the installation.

Completion of the Installation

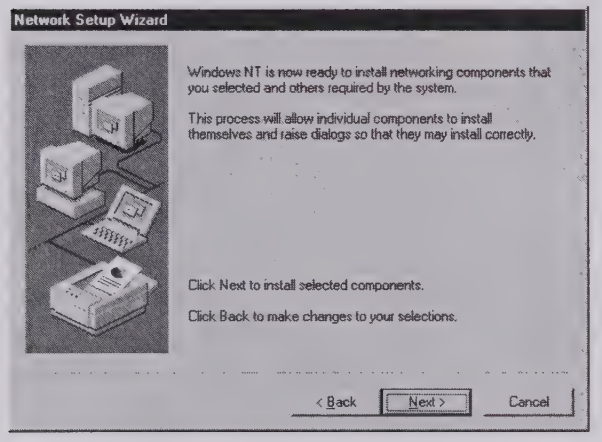
Network Setup Wizard
Windows NT is now ready to install networking components that you selected and others required by the system.
This process will allow individual components to install themselves and raise dialogs so that they may install correctly.
Click Next to install selected components.
Click Back to make changes to your selections.
< Back
Next >
Cancel

➢ Start the installation by clicking on "NEXT" .

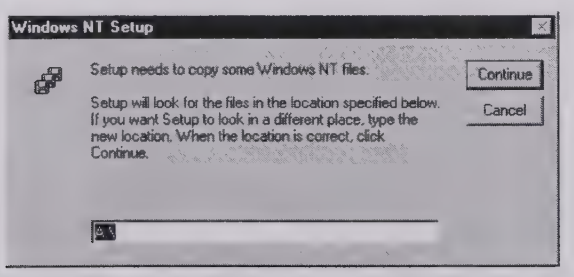
Windows NT Setup
Setup needs to copy some Windows NT files.
Setup will look for the files in the location specified below. If you want Setup to look in a different place, type the new location. When the location is correct, click Continue.
Continue
Cancel

➢ Enter drive "C:\I386" and click on "Continue".

After a couple of files have been copied, there is a message indicating that the driver for the network card has been installed.

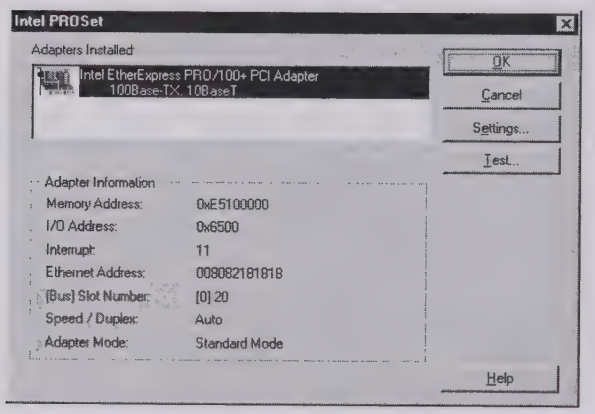

➢ If required, the network speed and the duplex mode can be set manually using the "Settings" button.

➢ Click on "OK".

The settings are checked and processed. Missing information on the installed network protocols (e.g. the TCP/IP address) is queried.

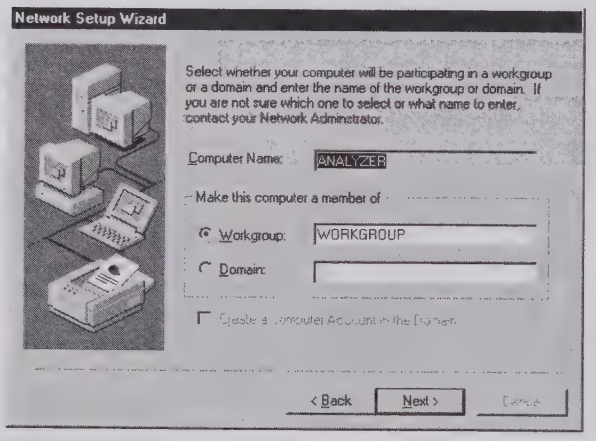
Network Setup Wizard
Select whether your computer will be participating in a workgroup or a domain and enter the name of the workgroup or domain. If you are not sure which one to select or what name to enter, contact your Network Administrator.
Computer Name: ANALYZER
Make this computer a member of
Workgroup: WORKGROUP
Domain:
< Back
Next >

➢ The preselected computer and workgroup names "ANALYZER" and "WORKGROUP" can be confirmed using "NEXT".

Note:
In Windows networks, the computer name must be unique.

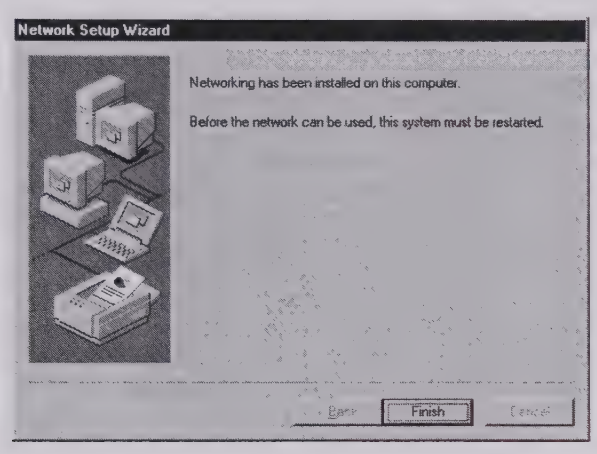
Network Setup Wizard
Networking has been installed on this computer.
Before the network can be used, this system must be restarted.
Back
Finish
Cancel

➢ Terminate the installation by clicking on "Finish".

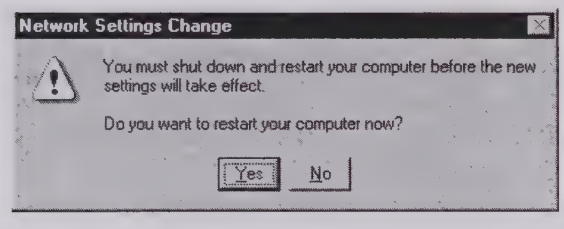
Network Settings Change
You must shut down and restart your computer before the new settings will take effect.
Do you want to restart your computer now?
Yes
No

➢ Answer the prompt "You must shutdown..." with "No", since the "Service Pack 5" of Windows NT must be reinstalled after the installation of the driver software. (see chapter 1, section "Computer Function - "Installing the Windows NT Software ")

Examples of Configurations

Network	Protocols	Services	Notes
NOVELL Netware	NWLink IPX/SPX Compatible Transport	Client Service for NetWare	In folder "Protocols - Properties", the frame type used in the network is to be set.
IP Networks (FTP, TELNET, WWW, GOPHER, etc.)	TCP/IP Protocol	Simple TCP/IP Services	In folder "Protocols - Properties", an IP address that is unique in the network is to be set.
MICROSOFT Network	NetBEUI Protocol or TCP/IP Protocol	Workstation Server	In folder "Identification - Computer Name", a name that is unique in the network is to be entered.

Subsequent Changing of the Network Configuration (Computer Name etc.)

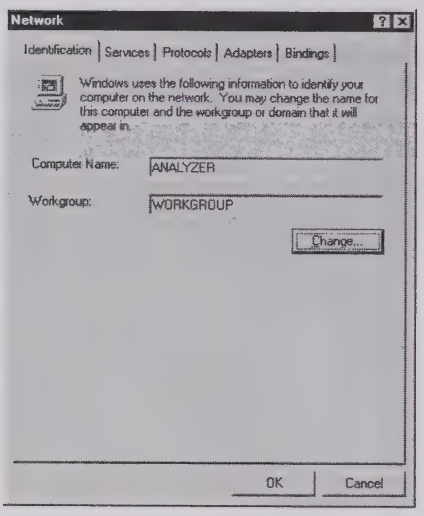

After completion of the installation, the computer name can be adapted as follows:

- Press the *SETUP* key.

  The *SETUP* menu opens.

- Press softkey *GENERAL SETUP.*

  The *GENERAL SETUP* menu opens.

- Press softkey *CONFIGURE NETWORK.*

  The configuration menu "Network" for the network settings opens.

- Select folder "Identification".

  Both entries can be changed in the submenu "Change".

The other settings can be changed after selecting the other folders. However, it is recommended to contact the network administrator before any changes.

Operating the Instrument on the Network

After the network support has been installed, it is possible to exchange data between the instrument and other computers and to use printers in the network.
A prerequisite to the network operation is the appropriate access rights for the required network resources. Resources may be file directories of other computers or also central printers.
Access rights can be obtained from the network or server administrator. In that respect it is necessary to obtain the network name of the resource as well as the corresponding access rights.
In order to avoid misuse, the resources are protected by passwords. Normally, every entitled user of the resources is assigned a user name that is also protected by a password. Resources can then be assigned to this user. It is possible to determine the type of data access, ie whether data can only be read or also written, as well as shared data access. Depending on the network operating system, different types of usage are possible.

NOVELL Networks

The operating system NETWARE from NOVELL is a server based system. Data cannot be exchanged between individual workstations; the data transfer takes place between the PC and a server. This server provides memory space and the connection to network printers. On a server, data are organized in directories as under DOS and mapped to the workstation as virtual drives. A virtual drive behaves like an additional hard disk on the workstation, and the data can be edited accordingly. Network printers can also be addressed like normal printers.

There are two versions of the NOVELL network operating system: NETWARE 3 and NETWARE 4 NDS. In the case of the older version, NETWARE 3, each server manages its resources on its own and is independent. A user must be managed on each server separately. In the case of NOVELL 4 NDS, all resources in the network are managed together in the NDS (NOVELL DIRECTORY SERVICE). The user must log into the network only once and is given access to the resources according to his access rights. The individual resources and users are managed as objects in a hierarchical tree (NDS TREE). The position of the object in the tree is referred to as "CONTEXT" with NETWARE and must be known for access to the resources.

MICROSOFT Network

In case of a MICROSOFT network, data can be exchanged both between workstations (peer to peer) and between workstations and servers. The latter can supply access to files and connection to the printers. On a server, data are organized in directories as under DOS and mapped to the workstation as virtual drives. A virtual drive behaves like an additional hard disk on the workstation, and the data can be edited accordingly. Network printers can also be addressed like normal printers. A connection is possible to DOS, WINDOWS FOR WORKGROUPS, WINDOWS95, WINDOWS NT.

Defining Users

After the network driver software has been installed, the instrument will output an error message on the next power-on, as there is no user called "Instrument" (= user name for NT autologin) in the network. It is therefore necessary to define a common user for Windows NT and the network.
The definition of new users in the network is done by the network administrator. For definition of a new user on the instrument, the User Manager is required:

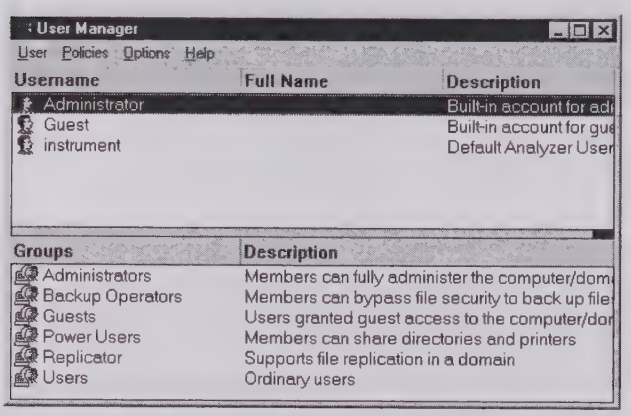

- Use the key combination <CTRL> <ESC> to call the Windows-NT start menu.
- Click on "Programs", "Administrative Tools (Common)" and "User Manager" one after the other.

  The "User Manager" menu opens.

- Select User "instrument".
- Click on the "User" menu and select "Copy...".

  The menu for entering the user data will appear.

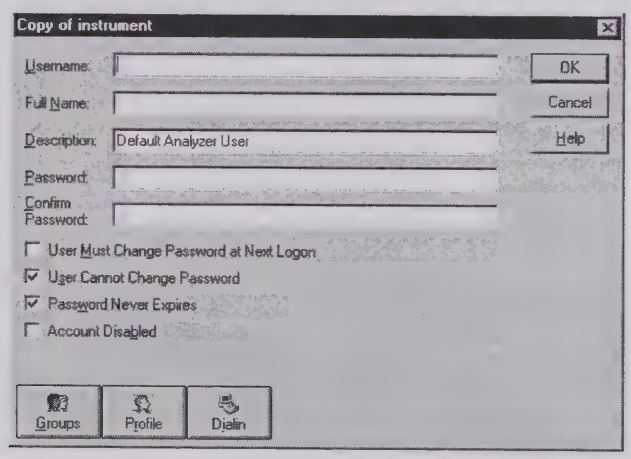

- Fill in the lines
  - "Username"
  - "Password and
  - "Confirm Password"

  and terminate the data entry with "OK".

  The user data must comply with the settings on the network.

Only NOVELL network:
Configure NOVELL Client

- Use the key combination <CTRL> <ESC> to call the Windows NT start menu.
- Click on "Settings", "Control Panel" and "CSNW" one after the other.

NOVELL 3.x

- Click on "Preferred Server".
- Select the NOVELL server where the user is configured using "Select Preferred Server".

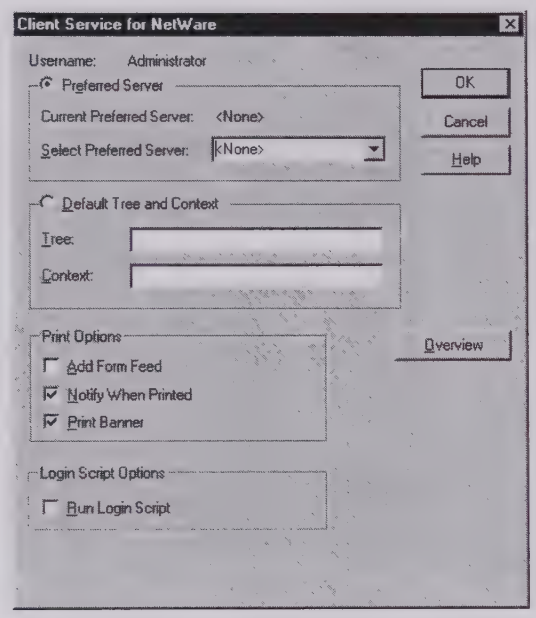

NOVELL 4.x

- Click on "Default Tree and Context".
- Enter the NDS Tree under "Tree" and the hierarchical path where the user is defined under "Context".

Note: *This data can be obtained from the network administrator.*

Login in the Network

The user automatically logs into the network with the registration in the operating system. As a prerequisite, the user name and the password must be identical under Windows NT and on the network.

Using Network Drives

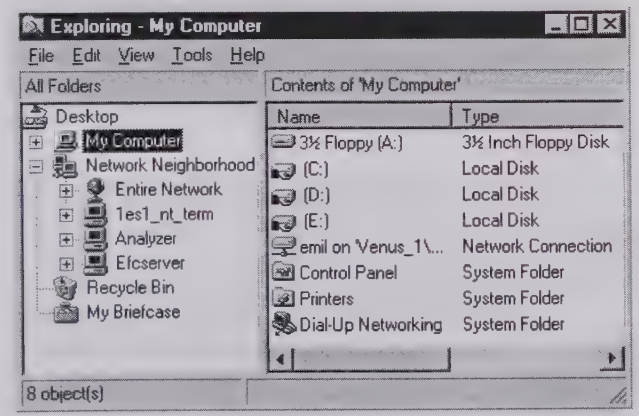

Mapping a network drive:

- Use the key combination <CTRL> <ESC> to call the Windows NT start menu.
- Click on "Programs", "Windows NT Explorer" one after the other.
- Click on the line "Network Neighborhood" in the overview "All Directories".

  An overview of the available network drives is displayed.

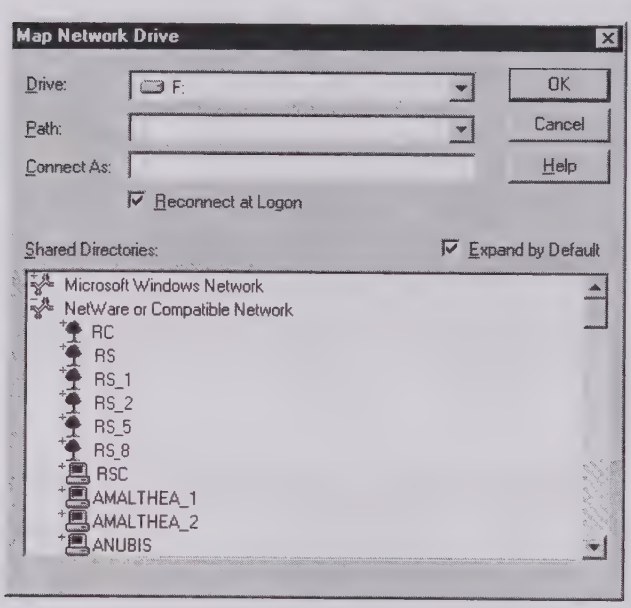

➢ Click on "Tools" and then "Map Network Drive".

The network paths available in the network are displayed in the overview "Shared Directories:".

➢ Mark the desired network path.

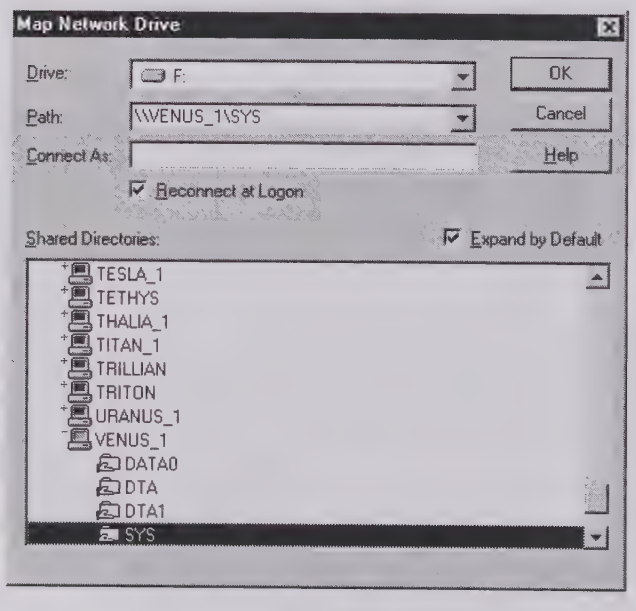

➢ Select the appropriate drive under "Drive:".

➢ Activate "Reconnect at Logon:" if the connection is to be set up automatically each time the instrument is started.

➢ Use "OK" to connect the network path with the selected drive.

The user name and the password are queried. Then the drive will appear in the overview "All Directories" of the explorer.

Note: *Only drives in the network can be connected that the user has the appropriate access rights for.*

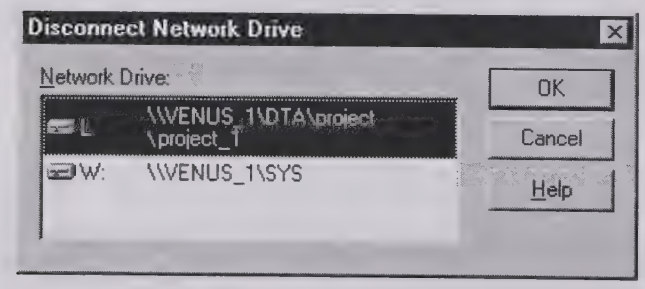

Disconnecting a network drive:

➢ Click on "Tools" in the Explorer and then "Disconnect Network Drive".

➢ Select the drive to be disconnected under "Network Drive:".

➢ Disconnect the drive using "OK". The security prompt must be answered with "Yes".

Printing on a Network Printer

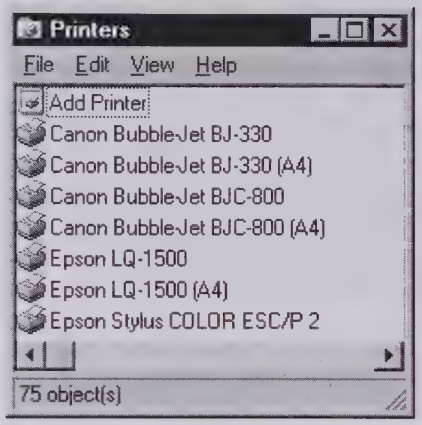

- Press the *HCOPY* key.

  The *HCOPY* menu opens.
- Press the *NEXT* key.

  The *HCOPY* submenu opens.
- Press the *INSTALL PRINTER* softkey.

  The printer window opens.
- Double-click on the line "Add Printer".

  The "Add Printer Wizard" window opens. It guides through the following printer driver installation.

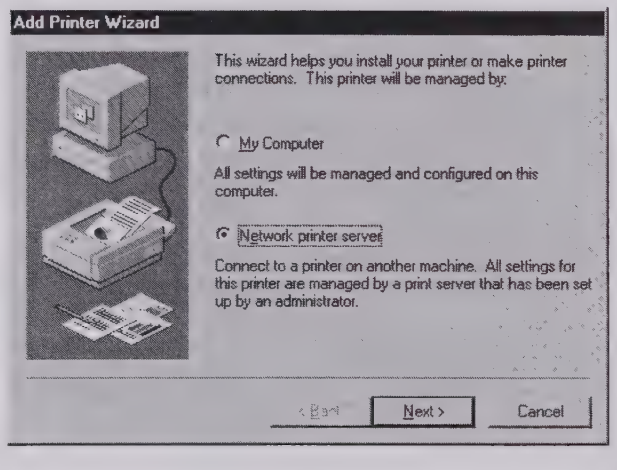
Add Printer Wizard
This wizard helps you install your printer or make printer connections. This printer will be managed by:
My Computer
All settings will be managed and configured on this computer.
Network printer server
Connect to a printer on another machine. All settings for this printer are managed by a print server that has been set up by an administrator.
< Back
Next >
Cancel

- Click on "Network Printer server" first and then on "Next".

  The choice of enabled printers appears.

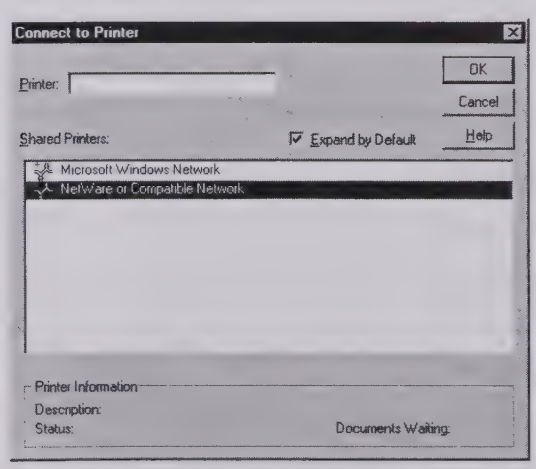

- Mark the printer and select using "OK".
- Confirm the following prompt to install a suitable printer driver using "OK".

  The choice of printer drivers appears. The left table shows the manufacturers, the right one the available printer drivers.

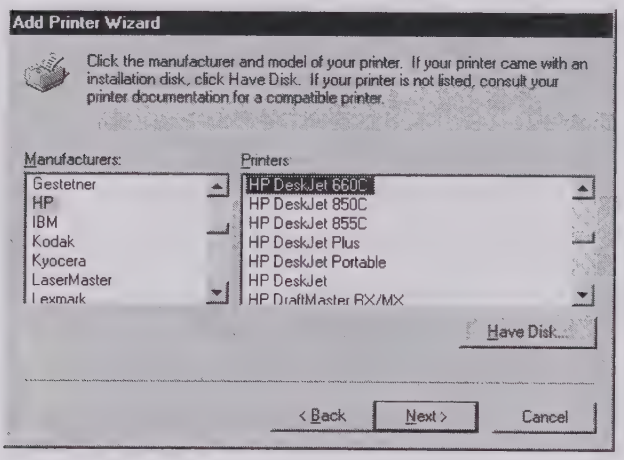

➢ Mark the manufacturer in the "Manufacturers" table and then the printer driver in the "Printers" table.

Note:
If the desired type of the output device does not appear in the list, the driver has not yet been installed on the instrument. In this case, click on the "HAVE DISK" button. A prompt appears, requesting the user to insert a disk with the respective printer driver. Then press "OK" and select the desired printer driver. After the installation, "Service Pack 5" must be reinstalled (see section "Installing the Windows NT Software")

➢ Click on "Next".

If one or more printers are already installed, this window will ask whether the just installed printer is to be selected as standard printer for the Windows NT applications (Do you want your Windows-based programs to use this printer as default printer?). "No" is set as default.

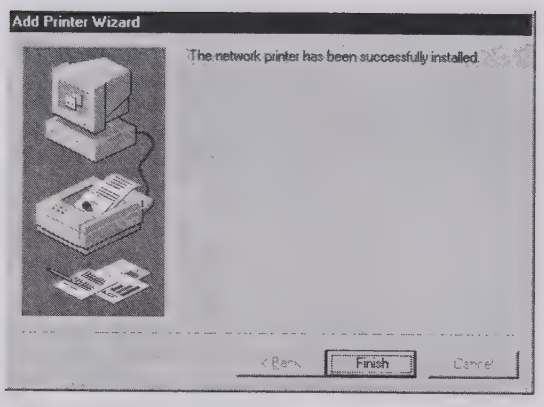

➢ Complete the installation of the printer driver by means of "Finish".

Note:
If the prompt to specify the path to the printer driver appears after clicking on "Finish", the Service Pack must be reinstalled after this printer installation (see Chapter 1, section "Computer Function - Installing the Windows NT Software").

Finally the instrument needs to be configured for use of the installed network printer using softkeys DEVICE 1 and DEVICE 2 in the Hardcopy Main Menu.

Remote Data Transfer with TCP/IP Services

The protocol TCP/IP allows the transfer of files between different computer systems. This requires a program running on the two computers that controls this data transfer. It is not necessary that the same operating or file system is used by both computers. For example, a file transfer between DOS/WINDOWS and UNIX is possible. One of the two partners must be configured as Host and the other one as Client. However, they may as well change their roles. Usually, the system which is able to perform several processes at the same time will play the host role. The file transfer program usually used under TCP/IP is FTP (File Transfer Protocol). An FTP host is installed as standard on the majority of UNIX systems.

If the TCP/IP services are installed, a terminal connection is possible using "Start" - "Programs" - "Accessories" - "Telnet" or a data transfer via FTP by means of "Start" - "Run" "ftp" - "OK". Thus all computer systems supporting these universal protocols can be addressed (UNIX, VMS, ...).

For further information please refer to the corresponding NT literature.

File Transfer via FTP

The total scope of functions and commands is described in the FTP literature. The following table therefore only contains the major functions:

Setting up the connection

Click on "Start" and then "Run" in the task bar

The DOS command
`FTP`
starts the program.

The command
`OPEN <xx.xx.xx.xx>`
sets up the connection.

xx.xx.xx.xx = IP address e.g. 89.0.0.13

Data transfer

The command
`PUT <dateiname>`
transfers the data to the target system.

The command
`GET <dateiname>`
transfers the data from the target system.

The command
`TYPE B`
transfers the data in BINARY format, no conversion takes place.

The command
`TYPE A`
transfers the data in ASCII format, converting control characters so that text files can also be read on the target system.

Examples:
`PUT C:\AUTOEXEC.BAT`
sends the file `AUTOEXEC.BAT` to the target system.
`LCD DATA`
changes the current directory on the local machine to subdirectory `DATA`
`CD SETTING`

changes to the subdirectory `SETTING` on the target system

dateiname= File name e.g. DATA.TXT

Changing the directories

The command

```
LCD <path>
```

changes the directory on the local machine as with `DOS`.

The command

```
LDIR
```

shows the directory contents on the local machine.

These commands refer to the file system of the FSP. If the `L` is omitted ahead of the commands, they apply to the target system.

RSIB Interface

The instrument is equipped with an RSIB interface as standard, which enables controlling of the instrument by means of Visual C++ and Visual Basic programs, but also by using the Windows applications WinWord and Excel. The control applications run on an external computer in the network.

Remote Control via RSIB Interface

In order to be able to access the measuring instruments via the RSIB interface, the file `RSIB32.DLL` must be copied into the Windows `system32` directory or into the directory of the control applications. For 16-bit applications, the file `RSIB.DLL` must be additionally copied into the directories mentioned. The files RSIB.DLL and RSIB32.DLL are included on the instrument in directory D:\R_S\Instr\RSIB.

For the different programming languages there are files available that contain the declarations of the DLL functions and the definition of the error codes.

Visual Basic (16 bit):	`'RSIB.BAS'`	`(D:\R_S\Instr\RSIB)`
Visual Basic (32 bit):	`'RSIB32.BAS'`	`(D:\R_S\Instr\RSIB)`
C:	`'RSIB.H'`	`(D:\R_S\Instr\RSIB)`

For C programs, import libraries are additionally available.

Import library for RSIB.DLL:	`RSIB.LIB'`	`(D:\R_S\Instr\RSIB)`
Import library for RSIB32.DLL:	`RSIB32.LIB'`	`(D:\R_S\Instr\RSIB)`

The control is performed using the Visual C++ or Visual Basic programs or one of the Windows applications WinWord or Excel. The programs use the IP address of the instrument to set up the connection.

Via VisualBasic: ud = RSDLLibfind ("82.1.1.200", ibsta, iberr, ibcntl)

Return to manual operation is possible via the front panel (*LOCAL* key) or via the RSIB interface:

Via RSIB: ud = RSDLLibloc (ud, ibsta, iberr, ibcntl);
or
ud = RSDLLibonl (ud, 0, ibsta, iberr, ibcntl);

RSIB Interface Functions

This chapter lists all functions of the DLL `"RSIB.DLL" or "RSIB32.DLL"`, which allow to produce control applications.

Overview of Interface Functions

The DLL functions are adapted to the interface functions of National Instruments for GPIB programming. The functions supported by the DLL are listed in the following table.

Function	Description
RSDLLibfind()	Provides a handle for access to a device.
RSDLLibwrt()	Sends a zero-terminated string to a device.
RSDLLilwrt()	Sends a certain number of bytes to a device.
RSDLLibwrtf()	Sends the contents of a file to a device.
RSDLLibrd()	Reads data from a device into a string.
RSDLLilrd()	Reads a certain number of bytes from a device.
RSDLLibrdf()	Reads data from a device into a file.
RSDLLibtmo()	Sets timeout for RSIB functions
RSDLLibsre()	Switches a device into the local or remote state
RSDLLibloc()	Temporarily switches a device into the local state
RSDLLibeot()	Enables/disables the END message for write operations.
RSDLLibrsp()	Performs a serial poll and provides the status byte.
RSDLLibonl()	Sets the device On/Offline.
RSDLLTestSrq()	Checks whether a device has generated an SRQ.
RSDLLWaitSrq()	Waits until a device generates an SRQ.

Variables ibsta, iberr, ibcntl

As with the National Instrument interface, the successful execution of a command can be checked by means of the variables `ibsta`, `iberr` and `ibcntl`. For this purpose, all RSIB functions are assigned references to these three variables.

Status word - ibsta

The status word ibsta provides information on the status of the RSIB interface. The following bits are defined:

Bit designation	Bit	Hex code	Description
ERR	15	8000	Is set when an error has occurred on calling a function. If this bit is set, `iberr` contains an error code which specifies the error in greater detail.
TIMO	14	4000	Is set when a timeout has occurred on calling a function.
CMPL	8	0100	Is set if the response of the GPIB parser has been read out completely. If a parser response is read out with the function `RSDLLilrd()` and the length of the buffer is insufficient for the answer, the bit will be cleared.

Error variable - iberr

If the ERR bit (8000h) is set in the status word, `iberr` contains an error code which allows to specify the error in greater detail. Extra error codes are defined for the RSIB interface, independent of the National Instruments interface.

Error	Error code	Description
IBERR_CONNECT	2	Setup of the connection to the measuring instrument has failed.
IBERR_NO_DEVICE	3	A function of the interface has been called with an illegal device handle.
IBERR_MEM	4	No empty memory available
IBERR_TIMEOUT	5	Timeout has occurred.
IBERR_BUSY	6	The RSIB interface is blocked by a still running function.
IBERR_FILE	7	Error when reading or writing to a file.

Count variable - ibcntl

The variable `ibcntl` is updated with the number of transferred bytes each time a read or write function is called.

Description of Interface Functions

RSDLLibfind()

The function provides a handle for access to the device with the name `udName`.

VB format:
```
Function RSDLLibfind (ByVal udName$, ibsta%, iberr%, ibcntl&)
As Integer
```

C-format:
```
short FAR PASCAL RSDLLibfind( char far *udName, short far
*ibsta, short far *iberr, unsigned long far *ibcntl)
```

Parameter: `udName` IP address of device

Example:
```
ud = RSDLLibfind ("89.10.38.97", ibsta, iberr, ibcntl)
```

The function must be called prior to all other functions of the interface.

As return value, the function provides a handle that must be indicated in all functions for access to the device. If the device with the name `udName` is not found, the handle has a negative value.

RSDLLibwrt

This function sends data to the device with the handle `ud`.

VB format:
```
Function RSDLLibwrt (ByVal ud%, ByVal Wrt$, ibsta%, iberr%,
ibcntl&) As Integer
```

C format:
```
short FAR PASCAL RSDLLibwrt( short ud, char far *Wrt, short
far *ibsta, short far *iberr, unsigned long far *ibcntl )
```

Parameter:
`ud` Device handle
`Wrt` String sent to the device.

Example:
```
RSDLLibwrt(ud, "SENS:FREQ:STAR?", ibsta, iberr, ibcntl)
```

This function allows to send setting and query commands to the measuring instruments. Whether the data is interpreted as a complete command can be set using the function `RSDLLibeot()`.

RSDLLilwrt

This function sends `Cnt` bytes to a device with the handle `ud`.

VB format:
```
Function RSDLLilwrt (ByVal ud%, ByVal Wrt$, ByVal Cnt&,
ibsta%, iberr%, ibcntl&) As Integer
```

C format:
```
short FAR PASCAL RSDLLilwrt( short ud, char far *Wrt,
unsigned long Cnt, short far *ibsta, short far *iberr,
unsigned long far *ibcntl)
```

Parameter:
`ud` Device handle
`Wrt` String sent to the GPIB parser.
`Cnt` Number of bytes sent to the device.

Example:
```
RSDLLilwrt (ud, '......', 100, ibsta, iberr, ibcntl)
```

Like `RSDLLibwrt()` this function sends data to a device. The only difference is that binary data can be sent as well. The length of the data is not determined by a zero-terminated string, but by the indication of `Cnt` bytes. If the data is to be terminated with EOS (0Ah), the EOS byte must be appended to the string.

RSDLLibwrtf

This function sends the contents of a file `file$` to the device with the handle `ud`.

VB format: `Function RSDLLibwrtf (ByVal ud%, ByVal file$, ibsta%, iberr%, ibcntl&) As Integer`

C format: `short FAR PASCAL RSDLLibwrt( short ud, char far *Wrt, short far *ibsta, short far *iberr, unsigned long far *ibcntl )`

Parameter:

`ud`	Device handle
`file`	File the contents of which are sent to the device.

Example: `RSDLLibwrtf(ud, "C:\db.sav", ibsta, iberr, ibcntl)`

This function allows to send setting and query commands to the measuring instruments. Whether the data is interpreted as complete command can be set using the function `RSDLLibeot()`.

RSDLLibrd()

The function reads data from the device with the handle `ud` into the string `Rd`.

VB format: `Function RSDLLibrd (ByVal ud%, ByVal Rd$, ibsta%, iberr%, ibcntl&) As Integer`

C format: `short FAR PASCAL RSDLLibrd( short ud, char far *Rd, short far *ibsta, short far *iberr, unsigned long far *ibcntl )`

Parameter:

`ud`	Device handle
`Rd`	String into which the read data is copied.

Example: `RSDLLibrd (ud, Rd, ibsta, iberr, ibcntl)`

This function fetches the responses of the GPIB parser to a query.

In the case of Visual Basic programming, a string of sufficient length must be generated before. This can be done during the definition of the string or using the command `Space$()`.

Generation of a string of the length 100:

- `Dim Rd as String * 100`
- ```
  Dim Rd as String
  Rd = Space$(100)
  ```

RSDLLilrd

This function reads `Cnt` bytes from the device with the handle `ud`.

VB format: `Function RSDLLilrd (ByVal ud%, ByVal Rd$, ByVal Cnt&, ibsta%, iberr%, ibcntl&) As Integer`

C format: `short FAR PASCAL RSDLLilrd( short ud, char far *Rd, unsigned long Cnt, short far *ibsta, short far *iberr, unsigned long far *ibcntl )`

Parameter:

`ud`	Device handle
`cnt`	Maximum number of bytes copied from the DLL into the target string `Rd`.

Example: `RSDLLilrd (ud, RD, 100, ibsta, iberr, ibcntl)`

Like the function `RSDLLibrd()`, this function reads data from a device. The only difference is that in this case the maximum number of bytes to be copied into the target string `Rd` can be indicated by means of `Cnt`. This function prevents writing beyond the end of the string.
  ```

RSDLLibrdf()

Reads data from the device with the handle `ud` into the file `file`.

VB format:
```
Function RSDLLibrdf (ByVal ud%, ByVal file$, ibsta%, iberr%,
ibcntl&) As Integer
```

C format:
```
short FAR PASCAL RSDLLibrd( short ud, char far *file, short
far *ibsta, short far *iberr, unsigned long far *ibcntl )
```

Parameter:

`ud`	Device handle
`file`	File into which the read data is written.

Example:
```
RSDLLibrdf (ud, "c:\db.sav", ibsta, iberr, ibcntl)
```

The file name may as well include a drive or path specification.

RSDLLibtmo

This function defines the timeout for a device. The default value for the timeout is set to 5 seconds.

VB format:
```
Function RSDLLibtmo (ByVal ud%, ByVal tmo%, ibsta%, iberr%,
ibcntl&) As Integer
```

C format:
```
void FAR PASCAL RSDLLibtmo( short ud, short tmo, short far
*ibsta, short far *iberr, unsigned long far *ibcntl )
```

Parameter:

`ud`	Device handle
`tmo`	Timeout in seconds

Example:
```
RSDLLibtmo (ud, 10, ibsta, iberr, ibcntl)
```

RSDLLibsre

This function sets the device to the 'LOCAL' or 'REMOTE' state.

VB format:
```
Function RSDLLibsre (ByVal ud%, ByVal v%, ibsta%, iberr%,
ibcntl&) As Integer
```

C format:
```
void FAR PASCAL RSDLLibsre( short ud, short v, short far
*ibsta, short far *iberr, unsigned long far *ibcntl)
```

Parameter:

`ud`	Device handle
`v`	State of device
	0 - local
	1 - remote

Example:
```
RSDLLibsre (ud, 0, ibsta, iberr, ibcntl)
```

RSDLLibloc

This function temporarily switches the device to the 'LOCAL' state.

VB format:
```
Function RSDLLibloc (ByVal ud%, ibsta%, iberr%, ibcntl&) As
Integer
```

C format:
```
void FAR PASCAL RSDLLibloc( short ud, short far *ibsta, short
far *iberr, unsigned long far *ibcntl)
```

Parameter:
`ud` Device handle

Example:
```
RSDLLibloc (ud, ibsta, iberr, ibcntl)
```

Having reached LOCAl state, the device can be manually operated via the front panel. With the next access to the device with one of the functions of the RSIB.DLL, the device is set back to the 'REMOTE' state again.

RSDLLibeot

This function enables or disables the END message after write operations.

VB format:
```
Function RSDLLibeot (ByVal ud%, ByVal v%, ibsta%, iberr%,
ibcntl&) As Integer
```

C format:
```
void FAR PASCAL RSDLLibsre( short ud, short v, short far
*ibsta, short far *iberr, unsigned long far *ibcntl)
```

Parameter:
`ud` Device handle.
`v` 0 - no END message
1 – send END message

Example:
```
RSDLLibeot (ud, 1, ibsta, iberr, ibcntl)
```

If the END message is disabled, the data of a command can be sent with several successive calls of write functions. The END message must be enabled again before sending the last data block.

RSDLLibrsp

This function performs a serial poll and provides the status byte of the device.

VB format:
```
Function RSDLLibrsp(ByVal ud%, spr%, ibsta%, iberr%, ibcntl&)
As Integer
```

C format:
```
void FAR PASCAL RSDLLibrsp( short ud, char far* spr, short far
*ibsta, short far *iberr, unsigned long far *ibcntl)
```

Parameter:
`ud` Device handle
`spr` Pointer to status byte

Example:
```
RSDLLibrsp(ud, spr, ibsta, iberr, ibcntl)
```

RSDLLibonl

This function switches the device to 'online' or 'offline' mode. When it is switched to 'offline' mode, the interface is released and the device handle becomes invalid. By calling RSDLLibfind again, the communication is set up again.

VB format:
```
Function RSDLLibonl (ByVal ud%, ByVal v%, ibsta%, iberr%,
ibcntl&) As Integer
```

C format:
```
void FAR PASCAL RSDLLibonl( short ud, short v, short far
*ibsta, short far *iberr, unsigned long far *ibcntl)
```

Parameter:

`ud`	Device handle
`v`	Device state 0 - local 1 - remote

Example:
```
RSDLLibonl(ud, 0, ibsta, iberr, ibcntl)
```

RSDLLTestSRQ

This function checks the status of the SRQ bit.

VB format:
```
Function RSDLLTestSrq (ByVal ud%, Result%, ibsta%, iberr%,
ibcntl&) As Integer
```

C format:
```
void FAR PASCAL RSDLLTestSrq( short ud, short far *result,
short far *ibsta, short far *iberr, unsigned long far *ibcntl)
```

Parameter:

`ud`	Device handle
`result`	Reference to an integer value in which the library returns the status of the SRQ bit. 0 - no SRQ 1 - SRQ active, device requests service

Example:
```
RSDLLTestSrq (ud, result%, ibsta, iberr, ibcntl)
```

This function corresponds to the function `RSDLLWaitSrq`. The only difference is that `RSDLLTestSRQ` immediately returns the current status of the SRQ bit, whereas `RSDLLWaitSrq` waits for an SRQ to occur.

RSDLLWaitSrq

This function waits until the device triggers an SRQ with the handle `ud`.

VB format:
```
Function RSDLLWaitSrq (ByVal ud%, Result%, ibsta%, iberr%,
ibcntl&) As Integer
```

C format:
```
void FAR PASCAL RSDLLWaitSrq( short ud, short far *result,
short far *ibsta, short far *iberr, unsigned long far *ibcntl)
```

Parameter:

`ud`	Device handle
`result`	Reference to an integer value in which the library returns the status of the SRQ bit. 0 - No SRQ has occurred during the timeout 1 - SRQ has occurred during the timeout

Parameter:
```
RSDLLWaitSrq( ud, result, ibsta, iberr, ibcntl );
```

The function waits until one of the following two events occurs.

- The measuring instrument triggers an SRQ
- No SRQ occurs during the timeout defined with `RSDLLibtmo()`

Programming via the RSIB Interface

Visual Basic

Programming hints:

- Access to the functions of the RSIB.DLL

  To create Visual Basic control applications, the file RSIB.BAS must be added to a project for 16-bit Basic programs and the file RSIB32.BAS for 32-bit Basic programs (D:\R_S\INSTR\RSIB) so that the functions of the RSIB.DLL or RSIB32.DLL can be accessed.

- Generating a response buffer

  Prior to calling the functions `RSDLLibrd()` and `RSDLLilrd()`, a string of sufficient length must be generated. This is possible either by defining the string or using the command `Space$()`.
  Generating a string of the length 100:

  - `Dim Response as String * 100`
  - ```
    Dim Response as String
    Response = Space$(100)
    ```

  If a response is to be output as a string from the measuring instrument, the appended blanks can be removed using the Visual Basic Function RTrim().

  Example:

  ```
  Response = Space$(100)
  Call RSDLLibrd(ud, Response, ibsta, iberr, ibcntl)
  Response = RTrim(Response)
  ' Output of Response
  ```

- Reading out trace data in real format

  Using the function declarations in the file RSIB.BAS or RSIB32.BAS the responses of the device can be assigned to one string only. If the data are to be read into an array with float values, the header and the useful data must be read out with separate function calls.

  Example of a header

  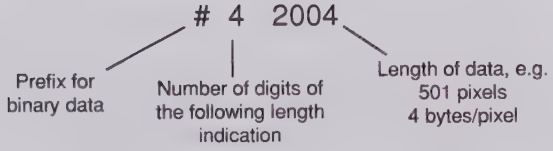
  # 4 2004
  Prefix for binary data
  Number of digits of the following length indication
  Length of data, e.g. 501 pixels 4 bytes/pixel

  In order to enable the trace data to be directly read into a float array, a special function declaration must be created.

  ```
  Declare Function RSDLLilrdTraceReal Lib "rsib32.dll" Alias "RSDLLilrd"
  (ByVal ud%, Rd As Single, ByVal Cnt&, ibsta%, iberr%, ibcntl&) As Integer
  ```
  ```

Example:

```
Dim ibsta As Integer            ' Status variable
Dim iberr As Integer            ' Error variable
Dim ibcntl As Long              ' Count variable
Dim ud As Integer               ' Handle for measuring instrument
Dim Result As String            ' Buffer for simple results
Dim Digits As Byte              ' Number of digits of length indication
Dim TraceBytes As Long          ' Length of trace data in bytes
Dim TraceData(501) As Single    ' Buffer for floating point
                                ' Binary data

' Set up connection to instrument
ud = RSDLLibfind("89.10.38.97", ibsta, iberr, ibcntl)

' Query trace data in real format
Call RSDLLibwrt(ud, "FORM:DATA REAL,32", ibsta, iberr, ibcntl)
Call RSDLLibwrt(ud, "TRACE? TRACE1", ibsta, iberr, ibcntl)

'Read number of digits of length indication
Result = Space$(20)
Call RSDLLilrd(ud, Result, 2, ibsta, iberr, ibcntl)
Digits = Val(Mid$(Result, 2, 1))

'Read length indication
Result = Space$(20)
Call RSDLLilrd(ud, Result, Digits, ibsta, iberr, ibcntl)
TraceBytes = Val(Left$(Result, Digits))    'and store

' Read out trace data
Call RSDLLilrdTraceReal(ud, TraceData(0), TraceBytes, ibsta, iberr,ibcntl)
```

Programming examples:

- In this example, the start frequency of the instrument is queried.

```
Dim ibsta As Integer    ' Status variable
Dim iberr As Integer    ' Error variable
Dim ibcntl As Long      ' Count variable
Dim ud As Integer       ' Handle for measuring instrument
Dim Response As String  ' Response string

' Set up connection to measuring instrument
ud = RSDLLibfind("89.10.38.97", ibsta, iberr, ibcntl)
If (ud < 0) Then
   ' Error treatment
End If

' Send query command
Call RSDLLibwrt(ud, "FREQ:START?", ibsta, iberr, ibcntl)

' Provide space for response
Response = Space$(100)

' Read response from measuring instrument
Call RSDLLibrd(ud, Response, ibsta, iberr, ibcntl)
```

- In this example, a Save/Recall of the instrument setups is performed.

```
Dim ibsta As Integer     ' Status variable
Dim iberr As Integer     ' Error variable
Dim ibcntl As Long       ' Count variable
Dim ud As Integer        ' Handle for measuring instrument
Dim Cmd As String        ' Command string

' Set up connection to measuring instrument
ud = RSDLLibfind("89.10.38.97", ibsta, iberr, ibcntl)
If (ud < 0) Then
   ' Error treatment
End If

' Request instrument settings
Cmd = "SYST:SET?"
Call RSDLLibwrt(ud, Cmd, ibsta, iberr, ibcntl)

' Store instrument response in file
Call RSDLLibrdf(ud, "C:\db.sav", ibsta, iberr, ibcntl)

' Reset instrument
Call RSDLLibwrt(ud, "*RST", ibsta, iberr, ibcntl)

' and restore the previous settings
' to this end disable the END message
Call RSDLLibeot(ud, 0, ibsta, iberr, ibcntl)
' first send off command
Call RSDLLibwrt(ud, "SYST:SET ", ibsta, iberr, ibcntl)
' enable the END message again
Call RSDLLibeot(ud, 1, ibsta, iberr, ibcntl)
' and send the data
Call RSDLLibwrtf(ud, "C:\db.sav", ibsta, iberr, ibcntl)
```

Visual Basic for Applications (Winword and Excel)

Programming hints:

The programming language Visual Basic for Applications (VBA) is supported as a macro language by various manufacturers. The programs Winword and Excel use this language for the versions Winword 97 or Excel 5.0 and higher.
For macros created with Visual Basic for Applications, the same hints are valid as for Visual Basic Applications.

Programming example:

- Using the macro `QueryMaxPeak` a single sweep with subsequent query of the maximum peak is performed. The result is entered in a Winword or Excel document.

```
Sub QueryMaxPeak()

    Dim ibsta As Integer     ' Status variable
    Dim iberr As Integer     ' Error variable
    Dim ibcntl As Long       ' transferred characters
    Dim ud As Integer        ' Unit Descriptor (handle)for instrument
    Dim Response As String   ' Response string

    ' Set up connection to measuring instrument
    ud = RSDLLibfind("89.10.38.97", ibsta, iberr, ibcntl)
    If (ud < 0) Then
      Call MsgBox("Device with address 89.10.38.97 could" & _
                  "not be found", vbExclamation)
      End
    End If

    ' Determine maximum peak in the range 1-2MHZ
    Call RSDLLibwrt(ud, "*RST", ibsta, iberr, ibcntl)
    Call RSDLLibwrt(ud, "INIT:CONT OFF", ibsta, iberr, ibcntl)
    Call RSDLLibwrt(ud, "FREQ:START 1MHZ", ibsta, iberr, ibcntl)
    Call RSDLLibwrt(ud, "FREQ:STOP 2MHZ", ibsta, iberr, ibcntl)
    Call RSDLLibwrt(ud, "INIT:IMM;*WAI", ibsta, iberr, ibcntl)
    Call RSDLLibwrt(ud, "CALC:MARK:MAX;Y?", ibsta, iberr, ibcntl)
    Response = Space$(100)
    Call RSDLLibrd(ud, Response, ibsta, iberr, ibcntl)
    Response = RTrim(Response) ' Cut off space

    ' Insert value in current document (Winword)
    Selection.InsertBefore (Response)
    Selection.Collapse (wdCollapseEnd)

    ' Terminate connection to measuring instrument
    Call RSDLLibonl(ud, 0, ibsta, iberr, ibcntl)

End Sub
```

The entry of the peak value in the Winword document can be replaced as follows for Excel:

```
    ' Insert value in current document (Excel)
    ActiveCell.FormulaR1C1 = Response
```

C / C++

Programming hints:

- Access to the functions of the RSIB32.DLL

  The functions of the `RSIB32.DLL` are declared in the header file `RSIB.H`. The DLL functions can be linked to a C/C++ program in different ways.

  1. Enter one of the supplied import libraries (`RSIB.LIB or RSIB32.LIB`) into the linker options.
  2. Load the library using the function `LoadLibrary()` during runtime and determine the function pointers of the DLL functions using `GetProcAddress()`. Before the end of the program, the `RSIB.DLL` must be unloaded again using the function `FreeLibrary()`.

  When import libraries are used, the DLL is automatically loaded immediately before the application is started. At the end of the program, the DLL is unloaded again unless it is still used by other applications.

- Query of strings

  If instrument responses are to be further processed as strings, a zero termination must be appended.

  Example:

```
char buffer[100];
...
RSDLLibrd( ud, buffer, &ibsta, &iberr, &ibcntl );
buffer[ibcntl] = 0;
```

Programming example:

In the following C program example, a single sweep is started on the device with the IP address 89.10.38.97 and subsequently a marker is set to maximum level. Prior to the search for maximum, a synchronization to the end of the sweep is performed. For this purpose the command `"*OPC"` (Operation complete) is used to create a service request at the end of the sweep, for which the control program waits with the function `RSDLLWaitSrq()`. Then the maximum is determined (`"CALC:MARK:MAX"`) and the level read out (`"Y?"`).

```
#define MAX_RESP_LEN 100

short           ibsta, iberr;
unsigned long   ibcntl;
short           ud;
short           srq;
char            MaxPegel[MAX_RESP_LEN];
char            spr;

// Determine handle for instrument
ud = RSDLLibfind( "89.10.38.97", &ibsta, &iberr, &ibcntl );

// if instrument exists
if ( ud >= 0 )
{
  // Set timeout for RSDLLWaitSrq() to 10 seconds
  RSDLLibtmo( ud, 10, &ibsta, &iberr, &ibcntl );

  // Activate SRQ generation via event status register (ESR)
  // and enable ESB bit in SRE register
  RSDLLibwrt( ud, "*ESE 1;*SRE 32", &ibsta, &iberr, &ibcntl );

  // Set single sweep, trigger sweep and use "*OPC" to cause
  // the generation of a service request at the end of the sweep
  RSDLLibwrt( ud, "INIT:CONT off;INIT;*OPC", &ibsta, &iberr, &ibcntl );

  // Wait for SRQ (end of sweep)
  RSDLLWaitSrq( ud, &srq, &ibsta, &iberr, &ibcntl );

  // Clear RQS/MSS bit
  RSDLLibrsp( ud, &spr, &ibsta, &iberr, &ibcntl );

  // if sweep is terminated
  if (srq)
  {
    // then set marker to first maximum and query the level
    RSDLLibwrt( ud, "CALC:MARK:MAX;Y?", &ibsta, &iberr, &ibcntl );
    RSDLLilrd( ud, MaxPegel, MAX_RESP_LEN, &ibsta, &iberr, &ibcntl );
    MaxPegel[ibcntl] = 0;
  }
  // End connection to instrument
  RSDLLibonl (ud, 0, &ibsta, &iberr, &ibcntl ) ;
}
else
{
  ; // Error Instrument not found
}
```

Contents - Chapter 5 "Remote Control - "Basics"

5 Remote Control - Basics 5.1

Introduction 5.1

Getting Started 5.2

Starting Remote Control Operation 5.3

Display Contents during Remote Control 5.3

Remote Control via IEC/IEEE Bus 5.4

Setting the Device Address 5.4

Return to Manual Operation 5.4

Remote Control via RS-232-Interface 5.5

Setting the Transmission Parameters 5.5

Return to Manual Operation 5.5

Limitations 5.5

Messages 5.6

IEC/IEEE-Bus Interface Messages 5.6

Device Messages (Commands and Device Responses) 5.6

Structure and Syntax of the Device Messages 5.7

SCPI Introduction 5.7

Structure of a Command 5.7

Structure of a Command Line 5.10

Responses to Queries 5.10

Parameters 5.11

Overview of Syntax Elements 5.12

Instrument Model and Command Processing 5.13

Input Unit 5.13

Command Recognition 5.14

Instrument Data Base and Instrument Hardware 5.14

Output Unit 5.15

Command Sequence and Command Synchronization 5.15

Status Reporting System 5.16

Structure of an SCPI Status Register 5.16

Overview of the Status Registers 5.18

Description of the Status Registers 5.19

Status Byte (STB) and Service Request Enable Register (SRE) 5.19

IST Flag and Parallel Poll Enable Register (PPE) 5.20

Event-Status Register (ESR) and Event-Status-Enable Register (ESE) 5.20

STATus:OPERation Register 5.21

STATus:QUEStionable Register 5.22

STATus QUEStionable:ACPLimit Register 5.23

STATus QUEStionable:FREQuency Register 5.24

STATus QUEStionable:LIMit<1|2> Register 5.25

STATus QUEStionable:LMARgin<1|2> Register 5.26

STATus QUEStionable:POWer Register 5.27

Application of the Status Reporting Systems 5.28

Service Request, Making Use of the Hierarchy Structure 5.28

Serial Poll 5.28

Parallel Poll 5.29
Query by Means of Commands 5.29
Error-Queue Query 5.29
Resetting Values of the Status Reporting System 5.30

5 Remote Control - Basics

In this chapter you'll find:

- instructions on how to put the FSP into operation via remote control,
- a general introduction to remote control of programmable instruments. This includes the description of the command structure and syntax according to the SCPI standard, the description of command execution and of the status registers,
- diagrams and tables describing the status registers used in the FSP.

In chapter 6, all remote control functions are described in detail. The subsystems are listed by alphabetical order according to SCPI. All commands and their parameters are listed by alphabetical order in the command list at the end of chapter 6.

Program examples for the FSP can be found in chapter 7.

The remote control interfaces and their interface functions are described in Chapter 8.

Introduction

The instrument is equipped with an IEC-bus interface according to standard IEC 625.1/IEEE 488.2 and a RS-232 interface. The connectors are located at the rear of the instrument and permits to connect a controller for remote control.

The instrument supports the SCPI:version 1997.0 (Standard Commands for Programmable Instruments). The SCPI standard is based on standard IEEE 488.2 and aims at the standardization of device-specific commands, error handling and the status registers (see Section "SCPI Introduction").
The tutorial "Automatic Measurement Control – A tutorial on SCPI and IEEE 488.2" from John M. Pieper (R&S order number 0002.3536.00) offers detailed information on concepts and definitions of SCPI.

This section assumes basic knowledge of IEC/IEEE bus programming and operation of the controller. A description of the interface commands can be obtained from the relevant manuals.

The requirements of the SCPI standard placed on command syntax, error handling and configuration of the status registers are explained in detail in the following sections. Tables provide a fast overview of the bit assignment in the status registers. The tables are supplemented by a comprehensive description of the status registers.

The program examples for IEC-bus programming are all written in VISUAL BASIC.

Getting Started

The short and simple operating sequence given below permits fast putting into operation of the instrument and setting of its basic functions. As a prerequisite, the IEC/IEEE-bus address, which is factory-set to 20, must not have been changed.

1. Connect instrument and controller using IEC/IEEE-bus cable.
2. Write and start the following program on the controller:

```
CALL IBFIND("DEV1", analyzer%)                  'Open port to the instrument
CALL IBPAD(analyzer%, 20)                       'Inform controller about instrument address
CALL IBWRT(analyzer%, '*RST;*CLS')              "Reset instrument

CALL IBWRT(analyzer%, 'FREQ:CENT 100MHz')       ' Set center frequency to 100 MHz
CALL IBWRT(analyzer%, 'FREQ:SPAN 10MHz')        ' Set span to 10 MHz
CALL IBWRT(analyzer%, 'DISP:TRAC:Y:RLEV -10dBm')
                                                ' Set reference level to -10 dBm
```

The instrument now performs a sweep in the frequency range of 95 MHz to 105 MHz.

3. To return to manual control, press the *LOCAL* key at the front panel

Starting Remote Control Operation

On power-on, the instrument is always in the manual operating state ("LOCAL" state) and can be operated via the front panel.
It is switched to remote control ("REMOTE" state)

IEC/IEEE-bus as soon as it receives an addressed command from a controller.

RS-232 as soon as it receives the command "@REM" from a controller.

During remote control, operation via the front panel is disabled. The instrument remains in the remote state until it is reset to the manual state via the front panel or via remote control interfaces. Switching from manual operation to remote control and vice versa does not affect the remaining instrument settings.

Display Contents during Remote Control

During remote control, only the LOCAL softkey appears, with which it is possible to return to manual operation.

In addition, the display of diagrams and results can be blanked out with the command "SYSTem:DISPlay:UPDate OFF" (default in remote control) to obtain optimum performance during remote control operation.

During program execution it is recommended to activate the display of results by means of "SYSTem:DISPlay:UPDate ON" so that it is possible to follow the changes in the device settings and the recorded measurement curves on the screen.

Note: *If the instrument is exclusively operated in remote control, it is recommended to switch on the power-save mode (POWER SAVE). In this mode, the required display is completely switched off after a preset time.*

Remote Control via IEC/IEEE Bus

Setting the Device Address

In order to operate the instrument via the IEC-bus, it must be addressed using the set IEC/IEEE bus address. The IEC/IEEE bus address of the instrument is factory-set to 20. It can be changed manually in the *SETUP - GENERAL SETUP* menu or via IEC bus. Addresses 0 to 30 are allowed.

Manually:

- Call *SETUP - GENERAL SETUP* menu
- Enter desired address in table *GPIB-ADDRESS*
- Terminate input using the *ENTER* key

Via IEC/IEEE bus:

```
CALL IBFIND("DEV1", analyzer%)                    'Open port to the instrument
CALL IBPAD(analyzer%, 20)                         'Inform controller about old address
CALL IBWRT(analyzer%, "SYST:COMM:GPIB:ADDR 18") 'Set instrument to new address
CALL IBPAD(analyzer%, 18)                         'Inform controller about new address
```

Return to Manual Operation

Return to manual operation is possible via the front panel or the IEC/IEEE bus.

Manually:

- Press the *LOCAL* softkey or the *PRESET* key

Notes:

- *Before switchover, command processing must be completed as otherwise transition to remote control is effected immediately.*
- *The keys can be disabled by the universal command LLO (see Chapter 8) in order to prevent unintentional switchover. In this case, switchover to manual mode is only possible via the IEC/IEEE bus.*
- *The keys can be enabled again by deactivating the REN line of the IEC/IEEE bus (see Chapter 8).*

Via IEC bus:

```
...
CALL IBLOC(analyzer%)          'Set instrument to manual operation
...
```

Remote Control via RS-232-Interface

Setting the Transmission Parameters

To enable an error-free and correct data transmission, the parameters of the unit and the controller should have the same setting.
Parameters can be manually changed in menu *SETUP-GENERAL SETUP* in table *COM PORT* or via remote control using the command `SYSTem:COMMunicate:SERial:...`.

The transmission parameters of the COM interface are factory-set to the following values:
baudrate = 9600, data bits = 8, stop bits = 1, parity = NONE and owner = INSTRUMENT.
For remote control operation, the interface should be allocated to the operating system (owner = OS) so that the control characters including @ can be recognized by the interface.

Manually: Setting the COM interface

- ➢ Call *SETUP-GENERAL SETUP* menu
- ➢ Select desired baudrate, bits, stopbit, parity in table *COM PORT.*
- ➢ Set owner to OS in table *COM PORT.*
- ➢ Terminate input using the *ENTER* key.

Return to Manual Operation

Return to manual operation is possible via the front panel or via RS-232 interface.

Manually:

- ➢ Press the *LOCAL* softkey or the *PRESET* key.

Notes:

- *Before switchover, command processing must be completed as otherwise transition to remote control is effected immediately*
- *The keys can be enabled again by sending the control string "@LOC" via RS-232 (see Chapter 8).*

Via RS-232:

```
...
v24puts(port,"@LOC");     Set instrument to manual operation..
...
```

Limitations

The following limitations apply if the unit is remote-controlled via the RS-232-C interface:

- No interface messages, only control strings.
- Only the Common Commands *OPC? can be used for command synchronization, *WAI and *OPC are not available.
- Block data cannot be transmitted.

Messages

The messages transferred via the data lines of the IEC bus can be divided into two groups:

- **interface messages and**
- **device messages.**

IEC/IEEE-Bus Interface Messages

Interface messages are transferred on the data lines of the IEC bus, the "ATN" control line being active. They are used for communication between controller and instrument and can only be sent by a controller which has the IEC/IEEE bus control. Interface commands can be subdivided into

- **universal commands and**
- **addressed commands.**

Universal commands act on all devices connected to the IEC/IEEE bus without previous addressing, addressed commands only act on devices previously addressed as listeners. The interface messages relevant to the instrument are listed in chapter 8.

Device Messages (Commands and Device Responses)

Device messages are transferred on the data lines of the IEC bus, the "ATN" control line not being active. ASCII code is used.
A distinction is made according to the direction in which they are sent on the IEC/IEEE bus:

- **Commands** are messages the controller sends to the instrument. They operate the device functions and request informations.
  The commands are subdivided according to two criteria::

  1. According to the effect they have on the instrument:

     Setting commands cause instrument settings such as reset of the instrument or setting the center frequency.

     Queries cause data to be provided for output on the IEC/IEEE bus, e.g. for identification of the device or polling the marker.

  2. According to their definition in standard IEEE 488.2:

     Common Commands are exactly defined as to their function and notation in standard IEEE 488.2. They refer to functions such as management of the standar-dized status registers, reset and selftest.

     Device-specific commands refer to functions depending on the features of the instrument such as frequency setting. A majority of these commands has also been standardized by the SCPI committee (cf. Section "SCPI Introduction")).

- **Device responses** are messages the instrument sends to the controller after a query. They can contain measurement results, instrument settings and information on the instrument status (cf. Section "Responses to Queries").

Structure and syntax of the device messages are described in the following Section.

Structure and Syntax of the Device Messages

SCPI Introduction

SCPI (Standard Commands for Programmable Instruments) describes a standard command set for programming instruments, irrespective of the type of instrument or manufacturer. The goal of the SCPI consortium is to standardize the device-specific commands to a large extent. For this purpose, a model was developed which defines the same functions inside a device or for different devices. Command systems were generated which are assigned to these functions. Thus it is possible to address the same functions with identical commands. The command systems are of a hierarchical structure.
Fig. 5-1 illustrates this tree structure using a section of command system SENSe, which controls the device-specific settings, that do not refer to the signal characteristics of the measurement signal.
SCPI is based on standard IEEE 488.2, i.e. it uses the same syntactic basic elements as well as the common commands defined in this standard. Part of the syntax of the device responses is defined with greater restrictions than in standard IEEE 488.2 (see Section "Responses to Queries").

Structure of a Command

The commands consist of a so-called header and, in most cases, one or more parameters. Header and parameter are separated by a "white space" (ASCII code 0 to 9, 11 to 32 decimal, e.g. blank). The headers may consist of several key words. Queries are formed by directly appending a question mark to the header.

Note: *The commands used in the following examples are not in every case implemented in the instrument.*

Common commands

Common commands consist of a header preceded by an asterisk "*" and one or several parameters, if any.

Examples:

`*RST`	RESET, resets the device
`*ESE 253`	EVENT STATUS ENABLE, sets the bits of the event status enable register
`*ESR?`	EVENT STATUS QUERY, queries the contents of the event status register.

Device-specific commands

Hierarchy: Device-specific commands are of hierarchical structure (see Fig. 5-1). The different levels are represented by combined headers. Headers of the highest level (root level) have only one key word. This key word denotes a complete command system.

Example: `SENSe` This key word denotes the command system `SENSe`.

For commands of lower levels, the complete path has to be specified, starting on the left with the highest level, the individual key words being separated by a colon ":".

Example: `SENSe:FREQuency:SPAN 10MHZ`

This command lies in the third level of the SENSe system. It set the frequency span.

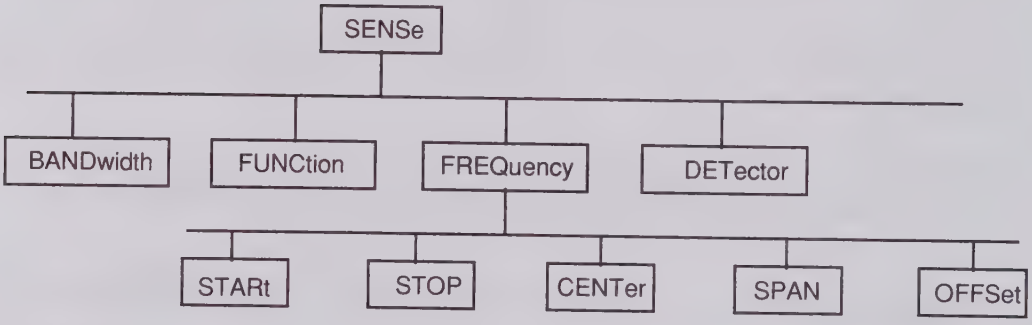

Fig. 5-1 Tree structure the SCPI command systems using the SENSe system by way of example

Some key words occur in several levels within one command system. Their effect depends on the structure of the command, that is to say, at which position in the header of a command they are inserted.

Example: `SOURce:FM:POLarity NORMal`
This command contains key word POLarity in the third command level. It defines the polarity between modulator and modulation signal.

`SOURce:FM:EXTernal:POLarity NORMal`
This command contains key word POLarity in the fourth command level. It defines the polarity between modulation voltage and the resulting direction of the modulation only for the external signal source indicated.

Optional key words: Some command systems permit certain key words to be optionally inserted into the header or omitted. These key words are marked by square brackets in the description. The full command length must be recognized by the instrument for reasons of compatibility with the SCPI standard. Some commands are considerably shortened by these optional key words.

Example: `[SENSe]:BANDwidth[:RESolution]:AUTO`
This command couples the resolution bandwidth of the instrument to other parameters. The following command has the same effect:
BANDwidth`:AUTO`

Note: *An optional key word must not be omitted if its effect is specified in detail by a numeric suffix.*

Long and short form: The key words feature a long form and a short form. Either the short form or the long form can be entered, other abbreviations are not allowed.

Beispiel: `STATus:QUEStionable:ENABle 1= STAT:QUES:ENAB 1`

Note: *The short form is marked by upper-case letters, the long form corresponds to the complete word. Upper-case and lower-case notation only serve the above purpose, the instrument itself does not make any difference between upper-case and lower-case letters.*

Parameter: The parameter must be separated from the header by a "white space". If several parameters are specified in a command, they are separated by a comma ",". A few queries permit the parameters MINimum, MAXimum and DEFault to be entered. For a description of the types of parameter, refer to Section "Parameters".

Example: `SENSe:FREQuency:STOP? MAXimum` Response: 3.5E9
This query requests the maximal value for the stop frequency.

Numeric suffix: If a device features several functions or features of the same kind, e.g. inputs, the desired function can be selected by a suffix added to the command. Entries without suffix are interpreted like entries with the suffix 1.

Example:. `SYSTem:COMMunicate:SERial2:BAUD 9600`
This command sets the baudrate of a second serial interface.

Structure of a Command Line

A command line may consist of one or several commands. It is terminated by a <New Line>, a <New Line> with EOI or an EOI together with the last data byte. The IEC/IEEE driver of the controller usually produces automatically an EOI together with the last data byte.

Several commands in a command line are separated by a semicolon ";". If the next command belongs to a different command system, the semicolon is followed by a colon.

Example:
```
CALL IBWRT(analyzer%,"SENSe:FREQuency:CENTer 100MHz;:INPut:ATTenuation 10")
```

This command line contains two commands. The first one is part of the SENSe command system and is used to determine the center frequency of the analyzer. The second one is part of the INPut command system and sets the input signal attenuation.

If the successive commands belong to the same system, having one or several levels in common, the command line can be abbreviated. To this end, the second command after the semicolon starts with the level that lies below the common levels (see also Fig. 5-1). The colon following the semicolon must be omitted in this case.

Example:
```
CALL IBWRT(analyzer%, "SENSe:FREQuency:STARt 1E6;:SENSe:FREQuency:STOP 1E9")
```

This command line is represented in its full length and contains two commands separated from each other by the semicolon. Both commands are part of the SENSe command system, subsystem FREQuency, i.e. they have two common levels.
When abbreviating the command line, the second command begins with the level below SENSe:FREQuency. The colon after the semicolon is omitted.

The abbreviated form of the command line reads as follows:

```
CALL IBWRT(analyzer%,  "SENSe:FREQuency:STARt 1E6;STOP 1E9")
```

However, a new command line always begins with the complete path.

Example:
```
CALL IBWRT(analyzer,  "SENSe:FREQuency:STARt 1E6")
CALL IBWRT(analyzer%,  "SENSe:FREQuency:STOP 1E9")
```

Responses to Queries

A query is defined for each setting command unless explicitly specified otherwise. It is formed by adding a question mark to the associated setting command. According to SCPI, the responses to queries are partly subject to stricter rules than in standard IEEE 488.2.

1. The requested parameter is transmitted without header.
   Example: `INPut:COUPling?` Response: `DC`
2. Maximum values, minimum values and all further quantities, which are requested via a special text parameter are returned as numerical values.
   Example: `SENSe:FREQuency:STOP? MAX` Response: `3.5E9`
3. Numerical values are output without a unit. Physical quantities are referred to the basic units or to the units set using the Unit command.
   Example: `SENSe:FREQuency:CENTer?` Response: `1E6` for 1 MHz
4. Truth values <Boolean values> are returned as 0 (for OFF) and 1 (for ON).
   Example: `SENSe:BANDwidth:AUTO?` Response: `1` for ON
5. Text (character data) is returned in a short form (see also Section 3.5.5).
   Example: `SYSTem:COMMunicate:SERial:CONTrol:RTS?` Response(for standard): `STAN`

Parameters

Most commands require a parameter to be specified. The parameters must be separated from the header by a "white space". Allowed parameters are numerical values, Boolean parameters, text, character strings and block data. The type of parameter required for the respective command and the allowed range of values are specified in the command description

Numerical values

Numerical values can be entered in any form, i.e. with sign, decimal point and exponent. Values exceeding the resolution of the instrument are rounded up or down. The mantissa may comprise up to 255 characters, the exponent must lie inside the value range -32000 to 32000. The exponent is introduced by an "E" or "e". Entry of the exponent alone is not allowed. In the case of physical quantities, the unit can be entered. Allowed unit prefixes are G (giga), MA (mega), MOHM and MHZ are also allowed), K (kilo), M (milli), U (micro) and N (nano). It the unit is missing, the basic unit is used.

Example:
`SENSe:FREQuency:STOP 1.5GHz = SENSe:FREQuency:STOP 1.5E9`

Special numerical

The texts MINimum, MAXimum, DEFault, UP and DOWN are interpreted as valuesspecial numerical values.

In the case of a query, the numerical value is provided.

Example: Setting command: `SENSe:FREQuency:STOP MAXimum`
Query: `SENSe:FREQuency:STOP?` Response: `3.5E9`

MIN/MAX — MINimum and MAXimum denote the minimum and maximum value.

DEF — DEFault denotes a preset value which has been stored in the EPROM. This value conforms to the default setting, as it is called by the *RST command

UP/DOWN — UP, DOWN increases or reduces the numerical value by one step. The step width can be specified via an allocated step command (see annex C, List of Commands) for each parameter which can be set via UP, DOWN.

INF/NINF — INFinity, Negative INFinity (NINF) Negative INFinity (NINF) represent the numerical values -9.9E37 or 9.9E37, respectively. INF and NINF are only sent as device reponses.

NAN — Not A Number (NAN) represents the value 9.91E37. NAN is only sent as device response. This value is not defined. Possible causes are the division of zero by zero, the subtraction of infinite from infinite and the representation of missing values.

Boolean Parameters

Boolean parameters represent two states. The ON state (logically true) is represented by ON or a numerical value unequal to 0. The OFF state (logically untrue) is represented by OFF or the numerical value 0. 0 or 1 is provided in a query.

Example: Setting command: `DISPlay:WINDow:STATe ON`
Query: `DISPlay:WINDow:STATe?` Response: `1`

Text

Text parameters observe the syntactic rules for key words, i.e. they can be entered using a short or long form. Like any parameter, they have to be separated from the header by a white space. In the case of a query, the short form of the text is provided.

Example: Setting command: `INPut:COUPling GROund`
Query: `INPut:COUPling?` Response `GRO`

Strings

Strings must always be entered in quotation marks (' or ").

Example: `SYSTem:LANGuage "SCPI"` or
`SYSTem:LANGuage 'SCPI'`

Block data

Block data are a transmission format which is suitable for the transmission of large amounts of data. A command using a block data parameter has the following structure:

Example: `HEADer:HEADer #45168xxxxxxxx`

ASCII character # introduces the data block. The next number indicates how many of the following digits describe the length of the data block. In the example the 4 following digits indicate the length to be 5168 bytes. The data bytes follow. During the transmission of these data bytes all End or other control signs are ignored until all bytes are transmitted..

Overview of Syntax Elements

The following survey offers an overview of the syntax elements.

:	The colon separates the key words of a command. In a command line the colon after the separating semicolon marks the uppermost command level.
;	The semicolon separates two commands of a command line. It does not alter the path.
,	The comma separates several parameters of a command.
?	The question mark forms a query.
*	The asterix marks a common command.
"	Quotation marks introduce a string and terminate it.
#	The double dagger (#) introduces block data
	A "white space (ASCII-Code 0 to 9, 11 to 32 decimal, e.g.blank) separates header and parameter.

Instrument Model and Command Processing

The instrument model shown in Fig. 5-2 has been made viewed from the standpoint of the servicing of IEC-bus commands. The individual components work independently of each other and simultaneously. They communicate by means of so-called "messages".

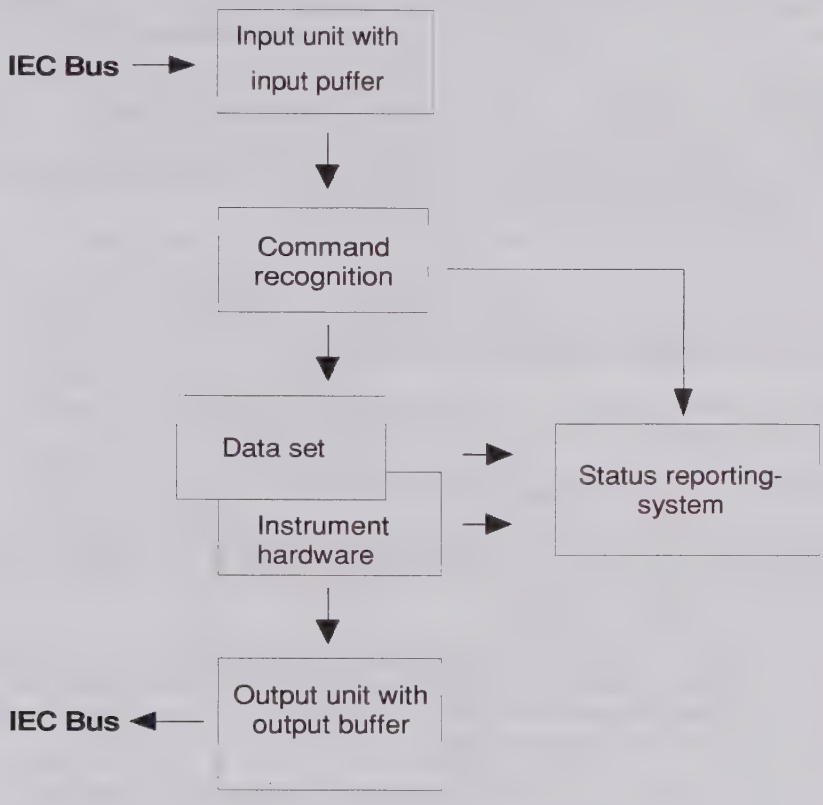

Fig. 5-2 Instrument model in the case of remote control by means of the IEC bus

Input Unit

The input unit receives commands character by character from the IEC bus and collects them in the input buffer. The input unit sends a message to the command recognition as soon as the input buffer is full or as soon as it receives a delimiter, <PROGRAM MESSAGE TERMINATOR>, as defined in IEEE 488.2, or the interface message DCL.
If the input buffer is full, the IEC-bus traffic is stopped and the data received up to then are processed. Subsequently the IEC-bus traffic is continued. If, however, the buffer is not yet full when receiving the delimiter, the input unit can already receive the next command during command recognition and execution. The receipt of a DCL clears the input buffer and immediately initiates a message to the command recognition.

Command Recognition

The command recognition analyses the data received from the input unit. It proceeds in the order in which it receives the data. Only a DCL is serviced with priority, a GET (Group Execute Trigger), e.g., is only executed after the commands received before as well. Each recognized command is immediately transferred to the instrument data base but without being executed there at once.
Syntactical errors in the command are recognized in the command recognition and supplied to the status reporting system. The rest of a command line after a syntax error is analysed further if possible and serviced.
If the command recognition recognizes a delimiter (<PROGRAM MESSAGE SEPARATOR> or <PROGRAM MESSAGE TERMINATOR>) or a DCL, it requests the instrument data base to set the commands in the instrument hardware as well now. Subsequently it is immediately prepared to process commands again. This means for the command servicing that further commands can already be serviced while the hardware is still being set ("overlapping execution").

Instrument Data Base and Instrument Hardware

Here the expression "instrument hardware" denotes the part of the instrument fulfilling the actual instrument function - signal generation, measurement etc. The controller is not included.

The instrument data base is a detailed reproduction of the instrument hardware in the software.

IEC-bus setting commands lead to an alteration in the data set. The data base management enters the new values (e.g. frequency) into the data base, however, only passes them on to the hardware when requested by the command recognition.

The data are only checked for their compatibility among each other and with the instrument hardware immediately before they are transmitted to the instrument hardware. If the detection is made that an execution is not possible, an "execution error" is signalled to the status reporting system. The alteration of the data base are cancelled, the instrument hardware is not reset.

IEC-bus queries induce the data base management to send the desired data to the output unit.

Status Reporting System

The status reporting system collects information on the instrument state and makes it available to the output unit on request. The exact structure and function are described in Section 3.8

Output Unit

The output unit collects the information requested by the controller, which it receives from the data base management. It processes it according to the SCPI rules and makes it available in the output buffer.
If the instrument is addressed as a talker without the output buffer containing data or awaiting data from the data base management, the output unit sends error message "Query UNTERMINATED" to the status reporting system. No data are sent on the IEC bus, the controller waits until it has reached its time limit. This behaviour is specified by SCPI.

Command Sequence and Command Synchronization

What has been said above makes clear that all commands can potentially be carried out overlapping.

In order to prevent an overlapping execution of commands, one of commands *OPC, *OPC? or *WAI must be used. All three commands cause a certain action only to be carried out after the hardware has been set and has settled. By a suitable programming, the controller can be forced to wait for the respective action to occur (cf. Table 5-1).

Table 5-1 Synchronisation using *OPC, *OPC? and *WAI

Command	Action after the hardware has settled	Programming the controller
*OPC	Setting the opteration-complete bit in the ESR	- Setting bit 0 in the ESE - Setting bit 5 in the SRE - Waiting for service request (SRQ)
*OPC?	Writing a "1" into the output buffer	Addressing the instrument as a talker
*WAI	Continuing the IEC-bus handshake	Sending the next command

An example as to command synchronization can be found in Chapter "Program Examples".

Status Reporting System

The status reporting system (cf. Fig. 5-4) stores all information on the present operating state of the instrument, e.g. that the instrument presently carries out a calibration and on errors which have occurred. This information is stored in the status registers and in the error queue. The status registers and the error queue can be queried via IEC bus.

The information is of a hierarchical structure. The register status byte (STB) defined in IEEE 488.2 and its associated mask register service request enable (SRE) form the uppermost level. The STB receives its information from the standard event status register (ESR) which is also defined in IEEE 488.2 with the associated mask register standard event status enable (ESE) and registers STATus:OPERation and STATus:QUEStionable which are defined by SCPI and contain detailed information on the instrument.

The IST flag ("Individual STatus") and the parallel poll enable register (PPE) allocated to it are also part of the status reporting system. The IST flag, like the SRQ, combines the entire instrument status in a single bit. The PPE fulfills the same function for the IST flag as the SRE for the service request.

The output buffer contains the messages the instrument returns to the controller. It is not part of the status reporting system but determines the value of the MAV bit in the STB and thus is represented in Fig. 5-4.

Structure of an SCPI Status Register

Each SCPI register consists of 5 parts which each have a width of 16 bits and have different functions (cf. Fig. 5-3). The individual bits are independent of each other, i.e. each hardware status is assigned a bit number which is valid for all five parts. For example, bit 3 of the STATus:OPERation register is assigned to the hardware status "wait for trigger" in all five parts. Bit 15 (the most significant bit) is set to zero for all parts. Thus the contents of the register parts can be processed by the controller as positive integer.

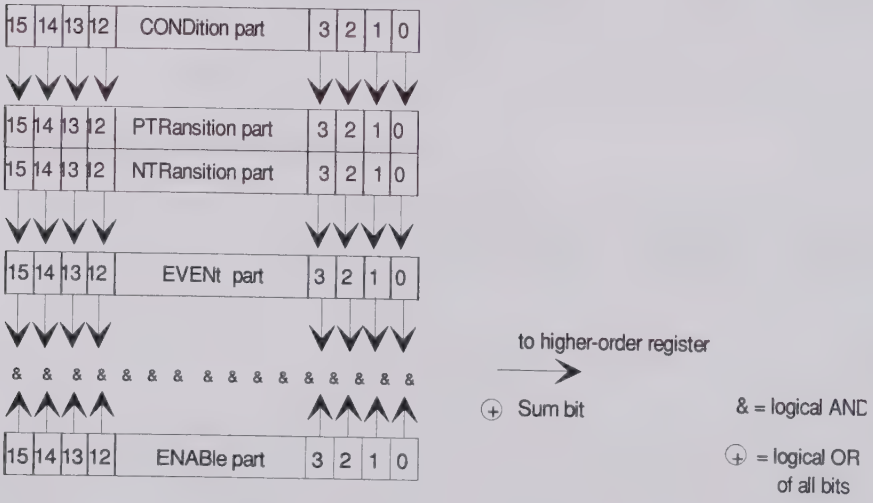
15 14 13 12 CONDition part 3 2 1 0
15 14 13 12 PTRansition part 3 2 1 0
15 14 13 12 NTRansition part 3 2 1 0
15 14 13 12 EVENt part 3 2 1 0
& & & & & & & & & & & & & &
15 14 13 12 ENABle part 3 2 1 0
to higher-order register
⊕ Sum bit
& = logical AND
⊕ = logical OR of all bits

Fig. 5-3 The status-register model

CONDition part

The CONDition part is directly written into by the hardware or the sum bit of the next lower register. Its contents reflects the current instrument status. This register part can only be read, but not written into or cleared. Its contents is not affected by reading.

PTRansition part

The Positive-TRansition part acts as an edge detector. When a bit of the CONDition part is changed from 0 to 1, the associated PTR bit decides whether the EVENt bit is set to 1.
PTR bit =1: the EVENt bit is set.
PTR bit =0: the EVENt bit is not set.
This part can be written into and read at will. Its contents is not affected by reading.

NTRansition part

The Negative-TRansition part also acts as an edge detector. When a bit of the CONDition part is changed from 1 to 0, the associated NTR bit decides whether the EVENt bit is set to 1.
NTR-Bit = 1: the EVENt bit is set.
NTR-Bit = 0: the EVENt bit is not set.
This part can be written into and read at will. Its contents is not affected by reading.

With these two edge register parts the user can define which state transition of the condition part (none, 0 to 1, 1 to 0 or both) is stored in the EVENt part.

EVENt part

The EVENt part indicates whether an event has occurred since the last reading, it is the "memory" of the condition part. It only indicates events passed on by the edge filters. It is permanently updated by the instrument. This part can only be read by the user. During reading, its contents is set to zero. In linguistic usage this part is often equated with the entire register.

ENABle part

The ENABle part determines whether the associated EVENt bit contributes to the sum bit (cf. below). Each bit of the EVENt part is ANDed with the associated ENABle bit (symbol '&'). The results of all logical operations of this part are passed on to the sum bit via an OR function (symbol '+').
ENABle-Bit = 0: the associated EVENt bit does not contribute to the sum bit
ENABle-Bit = 1: if the associated EVENT bit is "1", the sum bit is set to "1" as well.
This part can be written into and read by the user at will. Its contents is not affected by reading.

Sum bit

As indicated above, the sum bit is obtained from the EVENt and ENABle part for each register. The result is then entered into a bit of the CONDition part of the higher-order register.
The instrument automatically generates the sum bit for each register. Thus an event, e.g. a PLL that has not locked, can lead to a service request throughout all levels of the hierarchy.

Note: *The service request enable register SRE defined in IEEE 488.2 can be taken as ENABle part of the STB if the STB is structured according to SCPI. By analogy, the ESE can be taken as the ENABle part of the ESR.*

Overview of the Status Registers

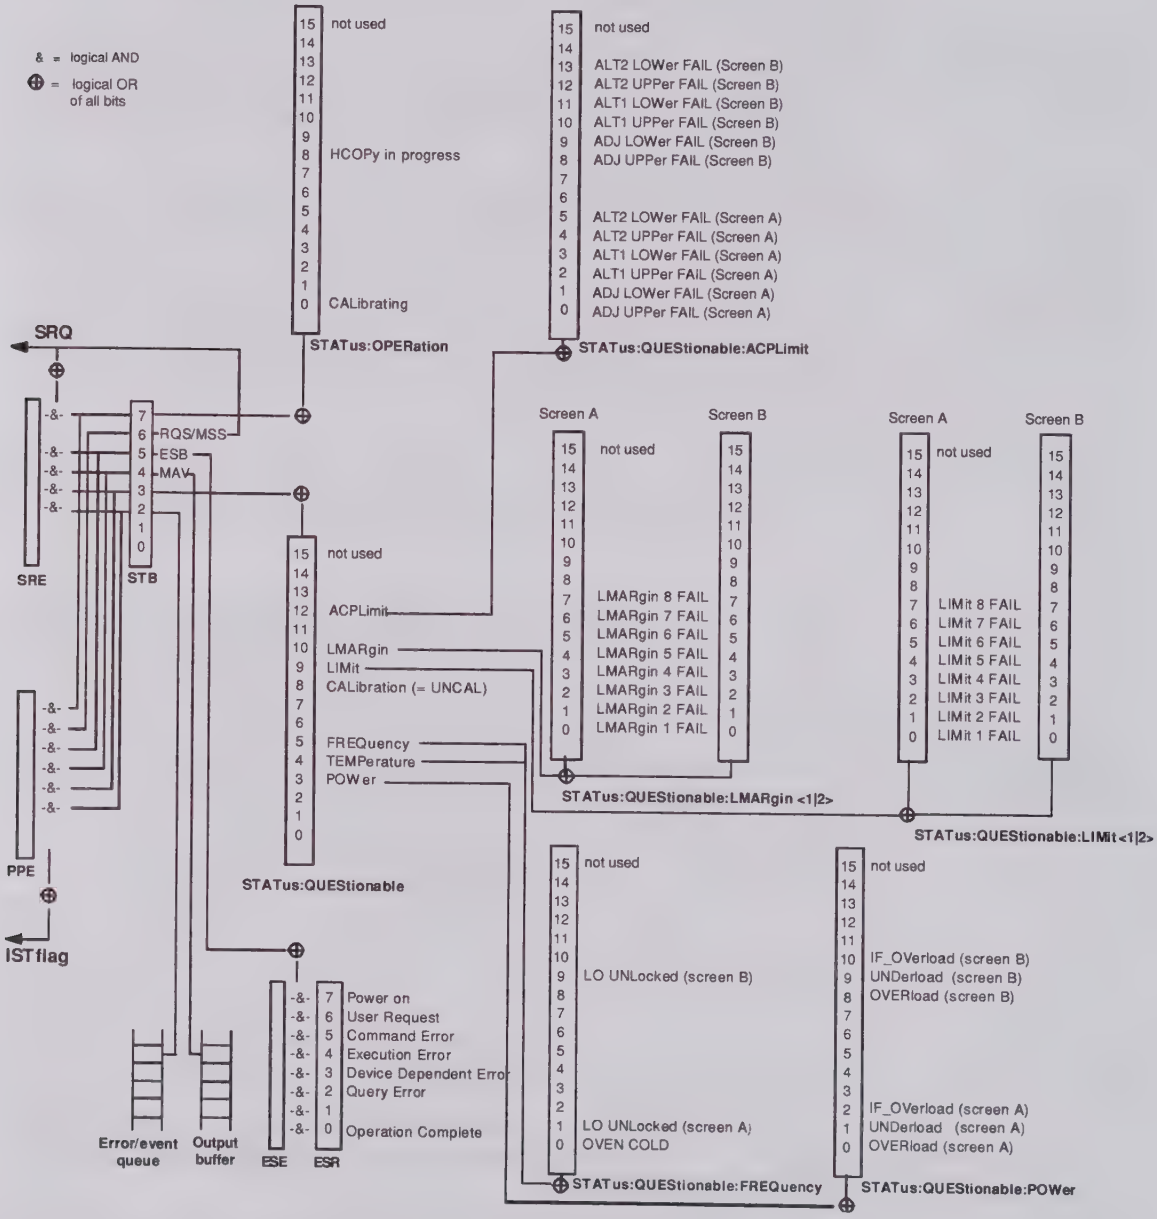

Fig. 5-4 Overview of the status registers

Description of the Status Registers

Status Byte (STB) and Service Request Enable Register (SRE)

The STB is already defined in IEEE 488.2. It provides a rough overview of the instrument status by collecting the pieces of information of the lower registers. It can thus be compared with the CONDition part of an SCPI register and assumes the highest level within the SCPI hierarchy. A special feature is that bit 6 acts as the sum bit of the remaining bits of the status byte.
The STATUS BYTE is read out using the command "*STB?" or a serial poll.

The STB implies the SRE. It corresponds to the ENABle part of the SCPI registers as to its function. Each bit of the STB is assigned a bit in the SRE. Bit 6 of the SRE is ignored. If a bit is set in the SRE and the associated bit in the STB changes from 0 to 1, a Service Request (SRQ) is generated on the IEC bus, which triggers an interrupt in the controller if this is appropriately configured and can be further processed there.
The SRE can be set using command "*SRE" and read using "*SRE?".

Table 5-2 Meaning of the bits in the status byte

Bit No.	Meaning
2	**Error Queue not empty** The bit is set when an entry is made in the error queue. If this bit is enabled by the SRE, each entry of the error queue generates a Service Request. Thus an error can be recognized and specified in greater detail by polling the error queue. The poll provides an informative error message. This procedure is to be recommended since it considerably reduces the problems involved with IEC-bus control.
3	**QUEStionable status sum bit** The bit is set if an EVENt bit is set in the QUEStionable: status register and the associated ENABle bit is set to 1. A set bit indicates a questionable instrument status, which can be specified in greater detail by polling the QUEStionable status register.
4	**MAV bit** (message available) The bit is set if a message is available in the output buffer which can be read. This bit can be used to enable data to be automatically read from the instrument to the controller (cf. annex D, program examples).
5	**ESB bit** Sum bit of the event status register. It is set if one of the bits in the event status register is set and enabled in the event status enable register. Setting of this bit implies an error or an event which can be specified in greater detail by polling the event status register.
6	**MSS bit** (master status summary bit) The bit is set if the instrument triggers a service request. This is the case if one of the other bits of this registers is set together with its mask bit in the service request enable register SRE.
7	**OPERation status register sum bit** The bit is set if an EVENt bit is set in the OPERation-Status register and the associated ENABle bit is set to 1. A set bit indicates that the instrument is just performing an action. The type of action can be determined by polling the OPERation-status register.

IST Flag and Parallel Poll Enable Register (PPE)

By analogy with the SRQ, the IST flag combines the entire status information in a single bit. It can be queried by means of a parallel poll (cf. Section 3.8.4.3) or using command "*IST?".

The parallel poll enable register (PPE) determines which bits of the STB contribute to the IST flag. The bits of the STB are ANDed with the corresponding bits of the PPE, with bit 6 being used as well in contrast to the SRE. The Ist flag results from the ORing of all results. The PPE can be set using commands "*PRE" and read using command "*PRE?".

Event-Status Register (ESR) and Event-Status-Enable Register (ESE)

The ESR is already defined in IEEE 488.2. It can be compared with the EVENt part of an SCPI register. The event status register can be read out using command "*ESR?".
The ESE is the associated ENABle part. It can be set using command "*ESE" and read using command "*ESE?".

Table 5-3 Meaning of the bits in the event status register

Bit No.	Meaning
0	**Operation Complete** This bit is set on receipt of the command *OPC exactly when all previous commands have been executed.
1	This bit is not used
2	**Query Error** This bit is set if either the controller wants to read data from the instrument without having send a query, or if it does not fetch requested data and sends new instructions to the instrument instead. The cause is often a query which is faulty and hence cannot be executed.
3	**Device-dependent Error** This bit is set if a device-dependent error occurs. An error message with a number between -300 and -399 or a positive error number, which denotes the error in greater detail, is entered into the error queue (cf. annex B, Error Messages).
4	**Execution Error** This bit is set if a received command is syntactically correct, however, cannot be performed for other reasons. An error message with a number between -200 and -300, which denotes the error in greater detail, is entered into the error queue (cf. annex B, Error Messages).
5	**Command Error** This bit is set if a command which is undefined or syntactically incorrect is received. An error message with a number between -100 and -200, which denotes the error in greater detail, is entered into the error queue (cf. Section "Error Messages").
6	**User Request** This bit is set on pressing the *LOCAL* key.
7	**Power On** (supply voltage on) This bit is set on switching on the instrument.

STATus:OPERation Register

In the CONDition part, this register contains information on which actions the instrument is being executing or, in the EVENt part, information on which actions the instrument has executed since the last reading. It can be read using commands `"STATus:OPERation:CONDition?"` or `"STATus:OPERation[:EVENt]?"`.

Table 5-4 Meaning of the bits in the STATus.OPERation register

Bit No.	Meaning
0	**CALibrating** This bit is set as long as the instrument is performing a calibration.
1 to 7	These bits are not used
8	**HardCOPy in progress** This bit is set while the instrument is printing a hardcopy.
9 to 14	These bits are not used
15	This bit is always 0

STATus:QUEStionable Register

This register comprises information about indefinite states which may occur if the unit is operated without meeting the specifications. It can be queried by commands `STATus:QUEStionable:CONDition?` and `STATus:QUEStionable[:EVENt]?`.

Table 5-5 Meaning of bits in STATus:QUEStionable register

Bit No.	Meaning
0 to 2	These bits are not used
3	**POWer** This bit is set if a questionable power occurs (cf. also section "STATus:QUEStionable:POWer Register")
4	**TEMPerature** This bit is set if a questionable temperature occurs.
5	**FREQuency** The bit is set if a frequency is questionable (cf. section "STATus:QUEStionable:FREQuency Register")
6 to 7	These bits are not used
8	**CALibration** The bit is set if a measurement is performed uncalibrated (≙ label "UNCAL")
9	**LIMit** (device-specific) This bit is set if a limit value is violated (see also section STATus:QUEStionable:LIMit Register)
10	**LMARgin** (device-specific) This bit is set if a margin is violated (see also section STATus:QUEStionable:LMARgin Register)
11	Device specific- not used
12	**ACPLimit** (device-specific) This bit is set if a limit for the adjacent channel power measurement is violated (see also section "STATus:QUEStionable:ACPLimit Register")
13 to 14	These bits are not used
15	This bit is always 0.

STATus QUEStionable:ACPLimit Register

This register comprises information about the observance of limits during adjacent power measurements. It can be queried with commands 'STATus:QUEStionable:ACPLimit :CONDition?' and 'STATus:QUEStionable:ACPLimit[:EVENt]?'

Table 5-6 Meaning of bits in STATus:QUEStionable:ACPLimit register

Bit No.	Meaning
0	**ADJ UPPer FAIL(Screen A)** This bit is set if in screen A. the limit is exceeded in the upper adjacent channel
1	**ADJ LOWer FAIL (Screen A)** This bit is set if in screen A the limit is exceeded in the lower adjacent channel.
2	**ALT1 UPPer FAIL (Screen A)** This bit is set if in screen A the limit is exceeded in the upper 1st alternate channel.
3	**ALT1 LOWer FAIL (Screen A)** This bit is set if in screen A the limit is exceeded in the lower 1st alternate channel.
4	**ALT2 UPPer FAIL (Screen A)** This bit is set if in screen A the limit is exceeded in the upper 2nd alternate channel.
5	**ALT2 LOWer FAIL (Screen A)** This bit is set if in screen A the limit is exceeded in the lower 2nd alternate channel.
6 to 7	not used
8	**ADJ UPPer FAIL (Screen B)** This bit is set if in screen B the limit is exceeded in the upper adjacent channel.
9	**ADJ LOWer FAIL (Screen B)** This bit is set if in screen B the limit is exceeded in the lower adjacent channel.
10	**ALT1 UPPer FAIL (Screen B)** This bit is set if in screen B the limit is exceeded in the upper 1st alternate channel.
11	**ALT1 LOWer FAIL (Screen B)** This bit is set if in screen B the limit is exceeded in the lower 1st alternate channel.
12	**ALT2 UPPer FAIL (Screen B)** This bit is set if in screen B the limit is exceeded in the upper 2nd alternate channel.
13	**ALT2 LOWer FAIL (Screen B)** This bit is set if in screen B the limit is exceeded in the lower 2nd alternate channel.
14	not used
15	This bit is always set to 0.

STATus QUEStionable:FREQuency Register

This register comprises information aboutthe reference and local oscillator.
It can be queried with commands `STATus:QUEStionable:FREQuency:CONDition?` and "`STATus:QUEStionable:FREQuency[:EVENt]?`.

Table 5-7 Meaning of bits in STATus:QUEStionable:FREQuency register

Bit No.	Meaning
0	**OVEN COLD** This bit is set if the reference oscillator has not yet attained its operating temperature. 'OCXO' will then be displayed.
1	**LO UNLocked** (Screen A) This bit is set if the local oscillator no longer locks. 'LOUNL will then be displayed.
2 to 8	not used
9	**LO UNLocked** (Screen B) This bit is set if the local oscillator no longer locks.' LOUNL' will then be displayed.
10 to 14	not used
15	This bit is always 0.

STATus QUEStionable:LIMit<1|2> Register

This register comprises information about the observance of limit lines in the corresponding measurement window (LIMit 1 corresponds to Screen A, LIMit 2 to Screen B). It can be queried with commands `STATus:QUEStionable:LIMit<1|2>:CONDition?` and `STATus:QUEStionable:LIMit<1|2>[:EVENt]?`.

Table 5-8 Meaning of bits in STATus:QUEStionable:LIMit<1|2> register

Bit No.	Meaning
0	**LIMit 1 FAIL** This bit is set if limit line 1 is violated.
1	**LIMit 2 FAIL** This bit is set if limit line 2 is violated.
2	**LIMit 3 FAIL** This bit is set if limit line 3 is violated.
3	**LIMit 4 FAIL** This bit is set if limit line 4 is violated.
4	**LIMit 5 FAIL** This bit is set if limit line 5 is violated.
5	**LIMit 6 FAIL** This bit is set if limit line 6 is violated.
6	**LIMit 7 FAIL** This bit is set if limit line 7 is violated.
7	**LIMit 8 FAIL** This bit is set if limit line 8 is violated.
8 to 14	not used
15	This bit is always 0.

STATus QUEStionable:LMARgin<1|2> Register

This register comprises information about the observance of limit margins in the corresponding measurement window (LMARgin1 corresponds to Screen A, LMARgin2 corresponds to Screen B). It can be queried with commands `STATus:QUEStionable:LMARgin<1|2>:CONDition?` and "`STATus :QUEStionable:LMARgin<1|2>[:EVENt]?`.

Table 5-9 Meaning of bits in STATus:QUEStionable:LMARgin<1|2> register

Bit No.	Meaning
0	**LMARgin 1 FAIL** This bit is set if limit margin 1 is violated.
1	**LMARgin 2 FAIL** This bit is set if limit margin 2 is violated.
2	**LMARgin 3 FAIL** This bit is set if limit margin 3 is violated.
3	**LMARgin 4 FAIL** This bit is set if limit margin 4 is violated.
4	**LMARgin 5 FAIL** This bit is set if limit margin 5 is violated.
5	**LMARgin 6 FAIL** This bit is set if limit margin 1 is violated.
6	**LMARgin 7 FAIL** This bit is set if limit margin 7 is violated.
7	**LMARgin 8 FAIL** This bit is set if limit margin 8 is violated.
8 to 14	not used
15	This bit is always 0.

STATus QUEStionable:POWer Register

This register comprises all information about possible overloads of the unit.
It can be queried with commands `STATus:QUEStionable:POWer:CONDition?` and `"STATus:QUEStionable:POWer[:EVENt]?`.

Table 5-10 Meaning of bits in STATus:QUEStionable:POWer register

Bit No.	Meaning
0	**OVERload** (Screen A) This bit is set if the RF input is overloaded. 'OVLD' will then be displayed.
1	**UNDerload** (Screen A) This bit is set if, during measurements in vector analyzer mode without capture buffer used, the lower level limit in the IF path is violated.
2	**IF_OVerload** (Screen A) This bit is set if the IF path is overloaded. 'IFOVL' will then be displayed.
3 to 7	not used
8	**OVERload** (Screen B) This bit is set if the RF input is overloaded. 'OVLD' will then be displayed.
9	**UNDerload** (Screen B) This bit is set if, during measurements without capture buffer used, the lower level limit in the IF path is violated.
10	**IF_OVerload** (Screen B) This bit is set if the IF path is overloaded. 'IFOVL' will then be displayed.
11 to 14	not used
15	This bit is always 0.

Application of the Status Reporting Systems

In order to be able to effectively use the status reporting system, the information contained there must be transmitted to the controller and further processed there. There are several methods which are represented in the following. Detailed program examples are to be found in annex D, Program Examples.

Service Request, Making Use of the Hierarchy Structure

Under certain circumstances, the instrument can send a service request (SRQ) to the controller. Usually this service request initiates an interrupt at the controller, to which the control program can react with corresponding actions. As evident from Fig. 5-4, an SRQ is always initiated if one or several of bits 2, 3, 4, 5 or 7 of the status byte are set and enabled in the SRE. Each of these bits combines the information of a further register, the error queue or the output buffer. The corresponding setting of the ENABle parts of the status registers can achieve that arbitrary bits in an arbitrary status register initiate an SRQ. In order to make use of the possibilities of the service request, all bits should be set to "1" in enable registers SRE and ESE.

Examples (cf. Fig. 5-4 and annex D, Program Examples, as well):

Use of command "*OPC" to generate an SRQ at the end of a sweep.

- `CALL IBWRT(analyzer%, "*ESE 1")` Set bit 0 in the ESE (Operation Complete)
- `CALL IBWRT(analyzer%, "*SRE 32")` Set bit 5 in the SRE (ESB)?

  After its settings have been completed, the instrument generates an SRQ.

The SRQ is the only possibility for the instrument to become active on its own. Each controller program should set the instrument in a way that a service request is initiated in the case of malfunction. The program should react appropriately to the service request. A detailed example for a service request routine is to be found in annex D, Program Examples.

Serial Poll

In a serial poll, just as with command "*STB", the status byte of an instrument is queried. However, the query is realized via interface messages and is thus clearly faster. The serial-poll method has already been defined in IEEE 488.1 and used to be the only standard possibility for different instruments to poll the status byte. The method also works with instruments which do not adhere to SCPI or IEEE 488.2.

The VISUAL BASIC command for executing a serial poll is "IBRSP()". Serial poll is mainly used to obtain a fast overview of the state of several instruments connected to the IEC bus.

Parallel Poll

In a parallel poll, up to eight instruments are simultaneously requested by the controller by means of a single command to transmit 1 bit of information each on the data lines, i.e., to set the data line allocated to each instrument to logically "0" or "1". By analogy to the SRE register which determines under which conditions an SRQ is generated, there is a parallel poll enable register (PPE) which is ANDed with the STB bit by bit as well considering bit 6. The results are ORed, the result is then sent (possibly inverted) as a response in the parallel poll of the controller. The result can also be queried without parallel poll by means of command "*IST".

The instrument first has to be set for the parallel poll using quick-BASIC command "IBPPC()". This command allocates a data line to the instrument and determines whether the response is to be inverted. The parallel poll itself is executed using "IBRPP()".

The parallel-poll method is mainly used in order to quickly find out after an SRQ which instrument has sent the service request if there are many instruments connected to the IEC bus. To this effect, SRE and PPE must be set to the same value. A detailed example as to the parallel poll is to be found in annex D, Program Examples.

Query by Means of Commands

Each part of every status register can be read by means of queries. The individual commands are indicated in the detailed description of the registers in Section 3.8.3. What is returned is always a number which represents the bit pattern of the register queried. Evaluating this number is effected by the controller program.

Queries are usually used after an SRQ in order to obtain more detailed information on the cause of the SRQ.

Error-Queue Query

Each error state in the instrument leads to an entry in the error queue. The entries of the error queue are detailed plain-text error messages which can be looked at in the ERROR menu via manual control or queried via the IEC bus using command "SYSTem:ERRor?". Each call of "SYSTem:ERRor?" provides an entry from the error queue. If no error messages are stored there any more, the instrument responds with 0, "No error".

The error queue should be queried after every SRQ in the controller program as the entries describe the cause of an error more precisely than the status registers. Especially in the test phase of a controller program the error queue should be queried regularly since faulty commands from the controller to the instrument are recorded there as well.

Resetting Values of the Status Reporting System

Table 5-11 comprises the different commands and events causing the status reporting system to be reset. None of the commands, except for *RST and SYSTem:PRESet influences the functional instrument settings. In particular, DCL does not change the instrument settings.

Table 5-11 Resettting instrument functions

Event / Effect	Switching on supply voltage: Power-On-Status-Clear 0	Switching on supply voltage: Power-On-Status-Clear 1	DCL,SDC (Device Clear, Selected Device Clear)	*RST or SYSTem:PRESet	STATus:PRESet	*CLS
Clear STB,ESR	—	yes	—	—	—	yes
Clear SRE,ESE	—	yes	—	—	—	—
Clear PPE	—	yes	—	—	—	—
Clear EVENTt parts of the registers	—	yes	—	—	—	yes
Clear Enable parts of all OPERation and QUEStionable registers, Fill Enable parts of all other registers with "1".	—	yes	—	—	yes	—
Fill PTRansition parts with "1" , Clear NTRansition parts	—	yes	—	—	yes	—
Clear error queue	yes	yes	—	—	—	yes
Clear output buffer	yes	yes	yes	1)	1)	1)
Clear command processing and input buffer	yes	yes	yes	—	—	—

1) Every command being the first in a command line, i.e., immediately following a <PROGRAM MESSAGE TERMINATOR> clears the output buffer.

Contents - Chapter 6
"Remote Control - Description of Commands"

6 Remote Control - Description of Commands 6.1

Notation 6.1

Common Commands 6.4

ABORt Subsystem 6.8

CALCulate Subsystem 6.8

CALCulate:DELTamarker Subsystem 6.9

CALCulate:LIMit Subsystem 6.17

CALCulate:LIMit:ACPower Subsystem 6.21

CALCulate:LIMit:CONTrol Subsystem 6.32

CALCulate:LIMit:LOWer Subsystem 6.34

CALCulate:LIMit:UPPer Subsystem 6.37

CALCulate:MARKer Subsystem 6.40

CALCulate:MARKer:FUNCtion Subsystem 6.49

CALCulate:MARKer:FUNCtion:POWer Subsystem 6.56

CALCulate:MARKer:FUNCtion:STRack Subsystem 6.61

CALCulate:MARKer:FUNCtion:SUMMary Subsystem 6.63

CALCulate:MATH Subsystem 6.74

CALCulate:STATistics Subsystem 6.76

CALCulate:THReshold Subsystem 6.80

CALCulate:UNIT Subsystem 6.81

CALibration Subsystem 6.82

DIAGnostic Subsystem 6.84

DISPlay Subsystem 6.86

FORMat Subsystem 6.94

HCOPy Subsystem 6.95

INITiate Subsystem 6.100

INPut Subsystem 6.102

INSTrument Subsystem 6.105

MMEMory Subsystem 6.107

OUTPut Subsystem 6.119

SENSe Subsystem 6.120

SENSe:AVERage Subsystem 6.120

SENSe:BANDwidth Subsystem 6.122

SENSe:CORRection Subsystem 6.125

SENSe:DETector Subsystem 6.127

SENSe:FREQuency Subsystem 6.128

SENSe:LIST Subsystem 6.131

SENSe:MPOWer – Subsystem 6.137

SENSe:POWer Subsystem 6.141

SENSe:ROSCillator Subsystem 6.146

SENSe:SWEep Subsystem 6.147
SOURce Subsystem 6.150
Internal Tracking Generator 6.150
SOURce:EXTernal Subsystem 6.153
STATus Subsystem 6.156
SYSTem Subsystem 6.165
TRACe Subsystem 6.174
General Trace Commands 6.174
TRACe:IQ-Subsystem 6.176
TRIGger Subsystem 6.182
UNIT Subsystem 6.184
Supported GPIB Commands of the HP 8590 Series 6-185
Supported Command Subset 6-185
Differences in Status Reporting 6-191
Differences in GPIB behavior between the FSP and the FSE families of instruments 6.192
Alphabetical List of Commands 6.216

Table of Softkeys with IEC/IEEE-Bus Command Assignment **6.226**
FREQUENCY Key 6.226
SPAN Key 6.227
AMPT Key 6.228
MKR Key 6.229
MKR-> Key 6.230
MKR FCTN Key 6.231
BW Key 6.232
SWEEP Key 6.233
MEAS Key 6.234
TRIG Key 6.237
TRACE Key 6.238
LINES Key 6.240
DISP Key 6.241
FILE Key 6.242
CAL Key 6.243
SETUP Key 6.244
HCOPY Key 6.245
Hotkeys 6.246
Hotkey NETWORK 6.247

6 Remote Control - Description of Commands

Notation

In the following sections, all commands implemented in the instrument are first listed in tables and then described in detail, arranged according to the command subsystems. The notation is adapted to the SCPI standard. The SCPI conformity information is included in the individual description of the commands.

Table of Commands

Command: In the command column, the table provides an overview of the commands and their hierarchical arrangement (see indentations).

Parameter: The parameter column indicates the requested parameters together with their specified range.

Unit: The unit column indicates the basic unit of the physical parameters.

Comment: In the comment column an indication is made on:
- whether the command does not have a query form,
- whether the command has only one query form
- whether the command is implemented only with a certain option of the instrument

Indentations

The different levels of the SCPI command hierarchy are represented in the table by means of indentations to the right. The lower the level, the further the indentation to the right. Please note that the complete notation of the command always includes the higher levels as well.

Example: `SENSe:FREQuency:CENTer` is represented in the table as follows:

`SENSe`	first level
`:FREQuency`	second level
`:CENTer`	third level

Individual description The individual description contains the complete notation of the command. An example for each command, the *RST value and the SCPI information are included as well.
The operating modes for which a command can be used are indicated by the following abbreviations:

A	Spectrum analysis
A-F	Spectrum analysis - frequency domain only
A-T	Spectrum analysis - time domain only (zero span)

Upper/lower case notation Upper/lower case letters are used to mark the long or short form of the key words of a command in the description (see Section 3.5.2). The instrument itself does not distinguish between upper and lower case letters.

Special characters

| A selection of key words with an identical effect exists for several commands. These keywords are indicated in the same line; they are separated by a vertical stroke. Only one of these keywords needs to be included in the header of the command. The effect of the command is independent of which of the keywords is used.

Example: `SENSe:FREQuency:CW|:FIXed`

The two following commands with identical meaning can be created. They set the frequency of the fixed frequency signal to 1 kHz:

`SENSe:FREQuency:CW 1E3` = `SENSe:FREQuency:FIXed 1E3`

A vertical stroke in parameter indications marks alternative possibilities in the sense of "or". The effect of the command is different, depending on which parameter is used.

Example: Selection of the parameters for the command

`DISPlay:FORMat FULL | SPLit`

If parameter FULL is selected, full screen is displayed, in the case of SPLit, split screen is displayed.

[ ] Key words in square brackets can be omitted when composing the header (cf. Section 3.5.2, Optional Keywords). The full command length must be accepted by the instrument for reasons of compatibility with the SCPI standards.
Parameters in square brackets can be incorporated optionally in the command or omitted as well.

{ } Parameters in braces can be incorporated optionally in the command, either not at all, once or several times.

Description of parameters Due to the standardization, the parameter section of SCPI commands consists always of the same syntactical elements. SCPI has therefore specified a series of definitions, which are used in the tables of commands. In the tables, these established definitions are indicated in angled brackets (<...>) and will be briefly explained in the following (see also Section 3.5.5, "Parameters").

<Boolean> This keyword refers to parameters which can adopt two states, "on" and "off". The "off" state may either be indicated by the keyword **OFF** or by the numeric value 0, the "on" state is indicated by **ON** or any numeric value other than zero. Parameter queries are always returned the numeric value 0 or 1.

<numeric_value>
<num>

These keywords mark parameters which may be entered as numeric values or be set using specific keywords (character data).

The following keywords given below are permitted:

MINimum	This keyword sets the parameter to the smallest possible value.
MAXimum	This keyword sets the parameter to the largest possible value.
DEFault	This keyword is used to reset the parameter to its default value.
UP	This keyword increments the parameter value.
DOWN	This keyword decrements the parameter value.

The numeric values associated to MAXimum/MINimum/DEFault can be queried by adding the corresponding keywords to the command. They must be entered following the quotation mark.

Example: `SENSe:FREQuency:CENTer? MAXimum`

returns the maximum possible numeric value of the center frequency as result.

<arbitrary block program data>

This keyword is provided for commands the parameters of which consist of a binary data block.

Common Commands

The common commands are taken from the IEEE 488.2 (IEC 625-2) standard. A particular command has the same effect on different devices. The headers of these commands consist of an asterisk "*" followed by three letters. Many common commands refer to the status reporting system which is described in detail in Section 3.8.

Command	Parameter	Function	Comment
*CAL?		Calibration Query	query only
*CLS		Clear Status	no query
*ESE	0 to 255	Event Status Enable	
*ESR?		Standard Event Status Query	query only
*IDN?		Identification Query	query only
*IST?		Individual Status Query	query only
*OPC		Operation Complete	
*OPT?		Option Identification Query	query only
*PCB	0 to 30	Pass Control Back	no query
*PRE	0 to 255	Parallel Poll Register Enable	
*PSC	0 | 1	Power On Status Clear	
*RST		Reset	no query
*SRE	0 to 255	Service Request Enable	
*STB?		Status Byte Query	query only
*TRG		Trigger	no query
*TST?		Self Test Query	query only
*WAI		Wait to continue	no query

***CAL?**

CALIBRATION QUERY initiates a calibration of the instrument and subsequently queries the calibration status. Any responses > 0 indicate errors.

***CLS**

CLEAR STATUS sets the status byte (STB), the standard event register (ESR) and the EVENt-part of the QUEStionable and the OPERation register to zero. The command does not alter the mask and transition parts of the registers. It clears the output buffer.

***ESE 0 to 255**

EVENT STATUS ENABLE sets the event status enable register to the value indicated. The query form *ESE? returns the contents of the event status enable register in decimal form.

***ESR?**

STANDARD EVENT STATUS QUERY returns the contents of the event status register in decimal form (0 to 255) and subsequently sets the register to zero.

***IDN?**

IDENTIFICATION QUERY queries the instrument identification.
Example: " Rohde&Schwarz, FSP-3, 123456/789, 1.03"
FSP-3 = Device name
123456/789 = Serial number of the instrument
1.03 = Firmware version number

***IST?**

INDIVIDUAL STATUS QUERY returns the contents of the IST flag in decimal form (0 | 1). The IST flag is the status bit which is sent during a parallel poll (cf. Section 3.8.3.2).

***OPC**

OPERATION COMPLETE sets bit 0 in the event status register when all preceding commands have been executed. This bit can be used to initiate a service request (cf. Section 3.7).

***OPC?**

OPERATION COMPLETE QUERY writes message "1" into the output buffer as soon as all preceding commands have been executed (cf. Section 3.7).

***OPT?**

OPTION IDENTIFICATION QUERY queries the options included in the instrument and returns a list of the options installed. The options are separated from each other by means of commas.

Position	Option	
1	FSP-B3	Audio Demodulator
2	FSP-B4	OCXO
3		reserved
4		reserved
5		reserved
6		reserved
7	FSP-B9	Tracking Generator 3 GHz / can be I/Q-modulated
8	FSP-B10	Ext. Generator Control
9...13		reserved
14	FSP-B16	LAN Interface
15...18		reserved
19		reserved
20...22		reserved
23	FSP-B25	Electronic Attenuator + 5dB Attenuator Steps
24...40		reserved

Example:
B3, B4, 0, 0, 0, 0, B9, B10, 0, 0, 0, 0, 0, B16, 0, 0, 0, 0, 0, 0, 0, 0, B25, 0, 0, 0, 0, 0, 0, 0, 0, 0, 0, 0, 0, 0, 0, 0, 0, 0

***PCB 0 to 30**

PASS CONTROL BACK indicates the controller address which the IEC-bus control is to be returned to after termination of the triggered action.

***PRE 0 to 255**

PARALLEL POLL REGISTER ENABLE sets the parallel poll enable register to the indicated value. The query form *PRE? returns the contents of the parallel poll enable register in decimal form.

***PSC 0 | 1**

POWER ON STATUS CLEAR determines whether the contents of the ENABle registers are preserved or reset during power-up.

*PSC = 0 causes the contents of the status registers to be preserved. Thus a service request can be generated when switching on the instrument, if the status registers ESE and SRE are suitably configured.

*PSC ≠ 0 resets the registers.

The query form *PSC? reads out the contents of the power-on-status-clear flag. The response can be 0 or 1.

***RST**

RESET sets the instrument to a defined default status. The command essentially corresponds to pressing the *PRESET* key. The default setting is indicated in the description of the commands.

***SRE 0 to 255**

SERVICE REQUEST ENABLE sets the service request enable register to the indicated value. Bit 6 (MSS mask bit) remains 0. This command determines under which conditions a service request is generated. The query form *SRE? reads the contents of the service request enable register in decimal form. Bit 6 is always 0.

***STB?**
READ STATUS BYTE QUERY reads out the contents of the status byte in decimal form.

***TRG**
TRIGGER initiates all actions in the currently active test screen expecting a trigger event. This command corresponds to `INITiate:IMMediate` (cf. Section "TRIGger subsystem").

***TST?**
SELF TEST QUERY initiates the selftest of the instrument and outputs an error code in decimal form (0 = no error).

***WAI**
WAIT-to-CONTINUE permits servicing of subsequent commands only after all preceding commands have been executed and all signals have settled (cf. Section 3.7 and "*OPC" as well).

ABORt Subsystem

The ABORt subsystem contains the commands for aborting triggered actions. An action can be triggered again immediately after being aborted. All commands trigger events, and therefore they have no *RST value.

COMMAND	PARAMETERS	UNIT	COMMENT
ABORt		--	no query

ABORt

This command aborts a current measurement and resets the trigger system.

Example: "ABOR;INIT:IMM"

Characteristics: *RST value: 0
SCPI: conforming

Mode: A

CALCulate Subsystem

The CALCulate subsystem contains commands for converting instrument data, transforming and carrying out corrections. These functions are carried out subsequent to data acquistion, ie following the SENSe subsystem.

The numeric suffix is used in CALCulate to make the distinction between the two measurement windows SCREEN A and SCREEN B:

CALCulate1 = Screen A
CALCulate2 = Screen B.

For commands without suffix, screen A is selected automatically.

Full Screen — The settings are valid for the measurement window selected with the numeric suffix. They become effective as soon as the corresponding measurement window has been selected as active measurement window using the command DISPLay[:WINDow<1|2>]:SELect. Triggering measurements and querying measured values is possible only in the active measurement window.

Split Screen — The settings are valid for the measurement window selected by means of the numeric suffix and become effective immediately.

CALCulate:DELTamarker Subsystem

The CALCulate:DELTamarker subsystem controls the delta-marker functions in the instrument. The measurement windows are selected via CALCulate1 (screen A) or 2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:DELTamarker<1 to 4>			
[:STATe]	<Boolean>	--	
:MODE	ABSolute|RELative		
:AOFF			no query
:TRACe	<numeric_value>	--	
:X	<numeric_value>	HZ | S | DBM | DB	
:RELative?	--	--	query only
:Y?	--	--	query only
:MAXimum			
[:PEAK]	--	--	no query
:NEXT	--	--	no query
:RIGHt	--	--	no query
:LEFT	--	--	no query
:MINimum			
[:PEAK]	--	--	no query
:NEXT	--	--	no query
:RIGHt	--	--	no query
:LEFT	--	--	no query
:FUNCtion			
:FIXed			
[:STATe]	<Boolean>		
:RPOint			
:Y	<numeric_value>	DBM	
:OFFSet	<numeric_value>	DB	
:X	<numeric_value>	HZ | S	
:PNOise			
[:STATe]	<Boolean>		
:RESult?	--	--	query only

CALCulate<1|2>:DELTamarker<1 to 4>[:STATe] ON | OFF

This command switches on and off the delta marker when delta marker 1 is selected. The corresponding marker becomes the delta marker when delta marker 2 to 4 is selected. If the corresponding marker is not activated, it will be activated and positioned on the maximum of the measurement curve.
If no numeric suffix is indicated, delta marker 1 is selected automatically.

Example: "CALC:DELT3 ON" Switches marker 3 in screen A to delta marker mode.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:MODE ABSolute | RELative

This command switches between relative and absolute frequency input of the delta marker (or time with span = 0). It affects all delta markers independent of the measurement window.

Example: `"CALC:DELT:MODE ABS"` Switches the frequency/time indication for all delta markers to absolute values.

`"CALC:DELT:MODE REL"` Switches the frequency/time indication for all delta markers to relative to marker 1.

Characteristics: *RST value: REL
SCPI: device-specific

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:AOFF

This command switches off all active delta markers in the selected measurement window (screen A or screen B).

Example: `"CALC2:DELT:AOFF"` Switches off all delta markers in screen B.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and therefore it has no *RST-value and no query form.

CALCulate<1|2>:DELTamarker<1 to 4>:TRACe 1 to 3

This command assigns the selected delta marker to the indicated measurement curve in the indicated measurement window. The selected measurement curve must be active, ie its state must be different from "BLANK".

Example: `"CALC:DELT3:TRAC 2"` Assigns deltamarker 3 to trace 2 in screen A.
`"CALC:DELT:TRAC 3"` Assigns deltamarker 1 to trace 3 in screen B.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:X 0 to MAX (frequency | sweep time)

This command positions the selected delta marker in the indicated measurement window to the indicated frequency (span > 0), time (span = 0) or level (APD measurement = ON or CCDFmeasurement = ON). The input is in absolute values or relative to marker 1 depending on the command `CALCulate:DELTamarker:MODE`. If Reference Fixed measurement (`CALCulate:DELTamarker:FUNCtion:FIXed:STATe ON`) is active, relative values refer to the reference position are entered. The query always returns absolute values.

Example:

`"CALC:DELT:MOD REL"`	Switches the input for all delta markers to relative to marker 1.
`"CALC:DELT2:X 10.7MHz"`	Positions delta marker 2 in screen A 10.7 MHz to the right of marker 1.
`"CALC2:DELT:X?"`	Outputs the absolute frequency/time of delta marker 1 in screen B
`"CALC2:DELT:X:REL?"`	Outputs the relative frequency/time/level of delta marker 1 in screen B

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:X:RELative?

This command queries the frequency (span > 0) or time (span = 0) of the selected delta marker relative to marker 1 or to the reference position (for `CALCulate:DELTamarker:FUNCtion :FIXed:STATe ON`). The command activates the corresponding delta marker, if necessary.

Example:

`"CALC:DELT:X:REL?"`	Outputs the frequency of delta marker 3 in screen B relative to marker 1 or relative to the reference position.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:Y?

This command queries the measured value of the selected delta marker in the indicated measurement window. The corresponding delta marker will be activated, if necessary. The output is always a relative value referred to marker 1 or to the reference position (reference fixed active).

To obtain a valid query result, a complete sweep with synchronization to the sweep end must be performed between the activation of the delta marker and the query of the y-value. This is only possible in single sweep mode.

Depending on the unit defined with `CALC:UNIT` or on the activated statistics functions, the query result is output in the units below:

- DBM | DBPW | DBUV | DBMV | DBUA: Output unit DB
- WATT | VOLT | AMPere: Output unit W | V | A
- Statistics function (APD or CCDF) on: Dimensionless output

Example:
```
"INIT:CONT OFF"
"CALC:DELT2 ON"
"INIT;*WAI"
"CALC:DELT2:Y?"
```
Switches to single-sweep mode.
Switches on delta marker 2 in screen A.
Starts a sweep and waits for its end.
Outputs measurement value of delta marker 2 in screen A.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:MAXimum[:PEAK]

This command positions the delta marker to the current maximum value on the measured curve. If necessary, the corresponding delta marker will be activated first.

Example: `"CALC2:DELT3:MAX"` Sets delta marker 3 in screen B to the maximum value of the associated trace.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:DELTamarker<1 to 4>:MAXimum:NEXT

This command positions the delta marker to the next smaller maximum value on the measured curve. The corresponding delta marker will be activated first, if necessary.

Example: `"CALC1:DELT2:MAX:NEXT"` Sets delta marker 2 in screen A to the next smaller maximum value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:DELTamarker<1 to 4>:MAXimum:RIGHt

This command positions the delta marker to the next smaller maximum value to the right of the current value (ie ascending X values). The corresponding delta marker is activated first, if necessary.

Example: `"CALC2:DELT:MAX:RIGH"` Sets delta marker 1 in screen B to the next smaller maximum value to the right of the current value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:DELTamarker<1 to 4>:MAXimum:LEFT

This command positions the delta marker to the next smaller maximum value to the left of the current value (ie descending X values). The corresponding delta marker will be activated first, if necessary.

Example: `"CALC:DELT:MAX:LEFT"` Sets delta marker 1 in screen A to the next smaller maximum value to the left of the current value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:DELTamarker<1 to 4>:MINimum[:PEAK]

This command positions the delta marker to the current minimum value on the measured crve. The corresponding delta marker will be activated first, if necessary.

Example: `"CALC2:DELT3:MIN"` Sets delta marker 3 in screen B to the minimum value of the associated trace.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:DELTamarker<1 to 4>:MINimum:NEXT

This command positions the delta marker to the next higher minimum value of the measured curve. The corresponding delta marker will be activated first, if necessary.

Example: `"CALC1:DELT2:MIN:NEXT"` Sets delta marker 2 in screen A to the next higher minimum value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:DELTamarker<1 to 4>:MINimum:RIGHt

This command positions the delta marker to the next higher minimum value to the right of the current value (ie ascending X values). The corresponding delta marker will be activated first, if necessary.

Example: `"CALC2:DELT:MIN:RIGH"` Sets delta marker 1 in screen B to the next higher minimum value to the right of the current value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:DELTamarker<1 to 4>:MINimum:LEFT

This command positions the delta marker to the next higher minimum value to the left of the current value (ie descending X values). The corresponding delta marker will be activated first, if necessary.

Example: `"CALC:DELT:MIN:LEFT"` Sets delta marker 1 in screen A to the next higher minimum to the left of the current value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:DELTamarker<1 to 4>:FUNCtion:FIXed[:STATe] ON | OFF

This command switches the relative measurement to a fixed reference value on or off. Marker 1 will be activated previously and a peak search will be performed, if necessary. If marker 1 is activated, its position becomes the reference point for the measurement. The reference point can then be modified with commands `CALCulate:DELTamarker:FUNCtion:FIXed:RPOint:X` and `...:RPOint:Y` independently of the position of marker 1 and of a trace. It is valid for all delta markers in the selected measurement window as long as the function is active.

Example: `"CALC2:DELT:FUNC:FIX ON"` Switches on the measurement with fixed reference value for all delta markers in screen B.

`"CALC2:DELT:FUNC:FIX:RPO:X 128 MHZ"` Sets the reference frequency in screen B to 128 MHz.

`"CALC2:DELT:FUNC:FIX:RPO:Y 30 DBM"` Sets the reference level in screen B to +30 dBm

Characteristics: *RST value: OFF
SCPI: device-specific.

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:FUNCtion:FIXed:RPOint:Y <numeric_value>

This command defines a new reference point level for all delta markers in the selected measurement window for a measurement with fixed reference point. (CALCulate:DELTamarker:FUNCtion:FIXed:STATe ON).

For phase-noise measurements (CALCulate:DELTamarker:FUNCtion:PNOise:STATe ON), the command defines a new reference point level for delta marker 2 in the selected measurement window.

Example: "CALC:DELT:FUNC:FIX:RPO:Y -10dBm" Sets the reference point level for delta markers in screen A to -10 dBm.

Characteristics: *RST value: - (FUNCtion:FIXed[:STATe] is set to OFF)
SCPI: device-specific

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:FUNCtion:FIXed:RPOint:Y:OFFSet <numeric_value>

This command defines an additional level offset for the measurement with fixed reference value (CALCulate:DELTamarker:FUNCtion:FIXed:STATe ON). For this measurement, the offset is included in the display of all delta markers of the selected measurement window.

For phase-noise measurements (CALCulate:DELTamarker:FUNCtion:PNOise:STATe ON), the command defines an additional level offset which is included in the display of delta marker 2 in the selected measurement window.

Example: "CALC:DELT:FUNC:FIX:RPO:Y:OFFS 10dB"
sets the level offset for the measurement with fixed reference value or the phase-noise measurement in screen A to 10 dB.

Characteristics: *RST value: 0 dB
SCPI: device-specific

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:FUNCtion:FIXed:RPOint:X <numeric_value>

This command defines a new reference frequency (span > 0) or time (span = 0) for all delta markers in the selected measurement window for a measurement with fixed reference value (CALCulate:DELTamarker:FUNCtion:FIXed:STATe ON).

For phase-noise measurements (CALCulate:DELTamarker:FUNCtion:PNOise:STATe ON), the command defines a new reference frequency or time for delta marker 2 in the selected measurement window.

Example: "CALC2:DELT:FUNC:FIX:RPO:X 128MHz" Sets the reference frequency in screen B to 128 MHz.

Characteristics: *RST value: - (FUNCtion:FIXed[:STATe] is set to OFF)
SCPI: device-specific

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:FUNCtion:PNOise[:STATe] ON | OFF

This command switches on or off the phase-noise measurement with all actíve delta markers in the selected measurement window. The correction values for the bandwidth and the log amplifier are taken into account in the measurement.

Marker 1 will be activated, if necessary, and a peak search will be performed. If marker 1 is activated, its position becomes the reference point for the measurement.

The reference point can then be modified with commands `CALCulate:DELTamarker :FUNCtion:FIXed:RPOint:X` and `...:RPOint:Y` independently of the position of marker 1 and of a trace (the same commands used for the measurment with fixed reference point).

The numeric suffix <1 to 4> with `DELTamarker` is not relevant for this command.

Example:

`"CALC:DELT:FUNC:PNO ON"`	Switches on the phase-noise measurement with all delta markers in screen A.
`"CALC:DELT:FUNC:FIX:RPO:X 128 MHZ"`	Sets the reference frequency to 128 MHz.
`"CALC:DELT:FUNC:FIX:RPO:Y 30 DBM"`	Sets the reference level to +30 dBm

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:DELTamarker<1 to 4>:FUNCtion:PNOise:RESult?

This command queries the result of the phase-noise measurement in the selected measurement window.The measurement will be switched on, if necessary.

Example: `"CALC:DELT:FUNC:PNO:RES?"` Outputs the result of phase-noise measurement of the selected delta marker in screen A.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is only a query and is therefore not assigned an *RST value.

CALCulate:LIMit Subsystem

The CALCulate:LIMit subsystem consists of the limit lines and the corresponding limit checks. Limit lines can be defined as upper or lower limit lines. The individual Y values of the limit lines correspond to the values of the X-axis (CONTrol). The number of X- and Y-values must be identical.

8 limit lines can be active at the same time (marked by LIMIT1 to LIMIT8) in screen A and/or screen B. The measurement windows is selected via CALCulate 1 (screen A) or 2 (screen B).

The limit check can be switched on separately for each measurement screen and limit line. WINDow1 corresponds to screen A, WINDow2 to screen B.

Each limit line can be assigned a name (max. 8 letters) under which the line is stored in the instrument. An explanatory comment can also be given for each line (max. 40 characters).

Example:
Definition and use of a new limit line 5 for trace 2 in screen A and trace 1 in screen B with the following features:

- upper limit line
- absolute X-axis in the frequency domain
- 5 ref. values: 126 MHz/-40 dB, 127 MHz/-40 dB, 128 MHz/-20 dB, 129 MHz/-40 dB, 130 MHz/-40 dB
- relative Y-axis with unit dB
- absolute threshold value at -35 dBm ,
- no safety margin

Definition of the line:

1. Defining the name:	`CALC:LIM5:NAME 'TEST1'`
2. Entering the comment:	`CALC:LIM5:COMM 'Upper limit line'`
3. Associated trace in screen A:	`CALC1:LIM5:TRAC 2`
4. Associated trace in screen B:	`CALC2:LIM5:TRAC 1`
5. Defining the X-axis range:	`CALC:LIM5:CONT:DOM FREQ`
6. Defining the X-axis scaling:	`CALC:LIM5:CONT:MODE ABS`
7. Defining the Y-axis unit:	`CALC:LIM5:UNIT DB`
8. Defining the Y-axis scaling:	`CALC:LIM5:UPP:MODE REL`
9. Defining the X-axis values:	`CALC:LIM5:CONT 126MHZ, 127MHZ, 128MHZ, 129 MHZ, 130MHZ`
10. Defining the y values:	`CALC:LIM5:UPP -40, -40, -30, -40, -40`
11. Defining the y threshold value:	`CALC:LIM5:UPP:THR -35DBM`

The definition of the safety margin and shifting in X- and/or Y-direction can take place as from here (see commands below).

Switching on and evaluating the line in screen A:

1. Switching on the line in screen A:	`CALC1:LIM5:UPP:STAT ON`
2. Switching on the limit check in screen A:	`CALC1:LIM5:STAT ON`
3. Starting a new measurement with synchronization:	`INIT;*WAI`
4. Querying the limit check result:	`CALC1:LIM5:FAIL?`

Switching on and evaluating the line in screen B is performed in the same way by using `CALC2` instead of `CALC1`.

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:LIMit<1 to 8>			
:TRACe	<numeric_value>		
:STATe	<Boolean>	--	
:UNIT	DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | DB | DBUV_M | DBUA_M | DEG | RAD | S | HZ | PCT | UNITLESS		
:FAIL?		--	query only
:CLEar			
[:IMMediate]	--	--	no query
:COMMent	<string>	--	
:COPY	1 to 8 | < name>	--	
:NAME	<string>		
:DELete	--		

CALCulate<1|2>:LIMit<1 to 8>:TRACe 1 to 3

This command assigns a limit line to a trace in the indicated measurement window.

Examples: `"CALC:LIM2:TRAC 3"` Assigns limit line 2 to trace 3 in screen A.

`"CALC2:LIM2:TRAC 1"` Assigns limit line 2 to trace 1 in screen B at the same time.

Characteristics: *RST value: 1
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:STATe ON | OFF

This command switches on or off the limit check for the selected limit line in the selected measurement window.

The result of the limit check can be queried with `CALCulate:LIMit<1 to 8>:FAIL?`.

Example: `"CALC:LIM:STAT ON"` Switches on the limit check for limit line 1 in screen A.

`"CALC2:LIM:STAT OFF"` Switches off the limit check for limit line 1 in screen B.

Characteristics: *RST value: OFF
SCPI: conforming

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:UNIT DBM | DBPW | WATT | DBUV | DBMV | VOLT |DBUA | AMPere | DB | DBUV_M | DBUA_M | DEG | RAD | S | HZ | PCT | UNITLESS

This command defines the unit of the selected limit line.

The definition is valid independently of the measurement window.

Upon selection of the unit DB the limit line is automatically switched to the relative mode. For units different from DB the limit line is automatically switched to absolute mode.

The units DEG, RAD, S, HZ, PCT are not available in spectrum analysis mode.

Example: "CALC:LIM4:UNIT DBUV" Sets the unit of limit line 4 to dBµV.

Characteristics: *RST value: DBM
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:FAIL?

This command queries the result of the limit check of the limit line indicated in the selected measurement window. It should be noted that a complete sweep must have been performed for obtaining a valid result. A synchronization with *OPC, *OPC? or *WAI should therefore be provided.

The result of the limit check responds with 0 for PASS, 1 for FAIL, and 2 for MARGIN.

Example: "INIT;*WAI" Starts a new sweep and waits for its end.

"CALC2:LIM3:FAIL?" Queries the result of the check for limit line 3 in screen B.

Characteristics: *RST value: -
SCPI: conforming

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:CLEar[:IMMediate]

This command deletes the result of the current limit check for all limit lines in the selected measurement window.

Example: "CALC:LIM:CLE" Deletes the result of the limit check in screen A

Characteristics: *RST value: -
SCPI: conforming

Mode: A

This command is an event and is therefore not assigned an *RST value.

CALCulate<1|2>:LIMit<1 to 8>:COMMent <string>

This command defines a comment for the limit line selected (max. 40 characters). The comment is independent from the measurement window.

Example: "CALC:LIM5:COMM 'Upper limit for spectrum'"
Defines the comment for limit line 5.

Characteristics: *RST value: blank comment
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:COPY 1 to 8 | <name>

This command copies one limit line onto another one. It is independent of the measurement window.

The name of the limit line may consist of max 8 characters.

Parameter: 1 to 8 ::= number of the new limit line or:
<name> ::= name of the new limit line given as a string

Example: "CALC:LIM1:COPY 2" Copies limit line 1 to line 2.

"CALC:LIM1:COPY 'GSM2'" Copies limit line 1 to a new line named 'GSM2'.

Characteristics: *RST value: --
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:LIMit<1 to 8>:NAME <name of limit line>

This command assigns a name to a limit line numbered 1 to 8. If it does not exist already, a limit line with this name is created. The command is independent of the measurement window.

The name of the limit line may contain a maximum of 8 characters.

Example: "CALC:LIM1:NAME 'GSM1'" Assigns the name 'GSM1' to limit line 1.

Characteristics: *RST value: 'REM1' to 'REM8' for lines 1 to 8
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:DELete

This command deletes the selected limit line. The command is independent of the measurement window.

Example: "CALC:LIM1:DEL" Deletes limit line 1.

Characteristics: *RST value: --
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate:LIMit:ACPower Subsystem

The CALCulate:LIMit:ACPower subsystem defines the limit check for adjacent channel power measurement.

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
LIMit<1 to 8>			
:ACPower			
[:STATe]	<Boolean>		
:ACHannel			
[:RELative]	<numeric_value>, <numeric_value>	DB, DB	
:STATe	<Boolean>		
:ABSolute	<numeric_value>, <numeric_value>	DBM, DBM	
:STATe	<Boolean>		
:RESult?	--		query only
:ALTernate<1|2>			
[:RELative]	<numeric_value>, <numeric_value>	DB, DB	
:STATe	<Boolean>		
:ABSolute	<numeric_value>, <numeric_value>	DBM, DBM	
:STATe	<Boolean>		
:RESult?	--		query only

CALCulate<1|2>:LIMit<1 to 8>:ACPower[:STATe] ON | OFF

This command switches on and off the limit check for adjacent channel power measurements in the selected measurement window. The commands `CALCulate:LIMit:ACPower:ACHannel:STATe` or `CALCulate:LIMit:ACPower:ALTernate:STATe` must be used in addition to specify whether the limit check is to be performed for the upper/lower adjacent channel or for the alternate adjacent channels.

The numeric suffixes <1 to 8> are irrelevant for this command.

Example: `"CALC:LIM:ACP ON"` Switches on the ACP limit check in screen A.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:ACPower:ACHannel[:RELative] 0 to 100dB, 0 to 100dB

This command defines the relative limit of the upper/lower adjacent channel for adjacent channel power measurements in the selected measurement window. The reference value for the relative limit value is the measured channel power.

It should be noted that the relative limit value has no effect on the limit check as soon as it is below the absolute limit value defined with `CALCulate:LIMit:ACPower:ACHannel:ABSolute`. This mechanism allows automatic checking of the absolute basic values of adjacent channel power as defined in mobile radio standards.

The numeric suffixes <1 to 8> are irrelevant for this command.

Parameter: The first numeric value is the limit for the upper (lower) adjacent channel. The second value is ignored but must be indicated for reasons of compatibility with the FSE family.

Example: `"CALC:LIM:ACP:ACH 30DB, 30DB"` Sets the relative limit value in screen A for the power in the lower and upper adjacent channel to 30 dB below the channel power.

Characteristics: *RST value: 0 dB
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:ACPower:ACHannel[:RELative]:STATe ON | OFF

This command activates the limit check for the relative limit value of the adjacent channel when adjacent channel power measurement is performed. Before the command, the limit check must be activated using `CALCulate:LIMit:ACPower:STATe ON`.

The result can be queried with `CALCulate:LIMit:ACPower:ACHannel:RESult?`. It should be noted that a complete measurement must be performed between switching on the limit check and the result query, since otherwise no valid results are available.

The numeric suffixes <1 to 8> are irrelevant for this command.

Example:

`"CALC:LIM:ACP:ACH 30DB, 30DB"`
Sets the relative limit value in screen A for the power in the lower and upper adjacent channel to 30 dB below the channel power.

`"CALC:LIM:ACP:ACH:ABS -35DBM, -35DBM"`
Sets the absolute limit value in screen A for the power in the lower and upper adjacent channel to -35 dB.

`"CALC:LIM:ACP ON"`
Switches on globally the limit check for the channel/adjacent channel measurement in screen A.

`"CALC:LIM:ACP:ACH:REL:STAT ON"` Switches on the check of the relative limit values for adjacent channels in screen A.

`"CALC:LIM:ACP:ACH:ABS:STAT ON"` Switches on the check of absolute limit values for the adjacent channels in screen A.

`"INIT;*WAI"`
Starts a new measurement and waits for the sweep end.

`"CALC:LIM:ACP:ACH:RES?"`
Queries the limit check result in the adjacent channels in screen A.

Characteristics:

*RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:ACPower:ACHannel:ABSolute -200DBM to 200DBM, -200 to 200DBM

This command defines the absolute limit value for the lower/upper adjacent channel during adjacent-channel power measurement (Adjacent Channel Power) in the selected measurement window.

It should be noted that the absolute limit value has no effect on the limit check as soon as it is below the relative limit value defined with `CALCulate:LIMit:ACPower:ACHannel:RELative`. This mechanism allows automatic checking of the absolute basic values of adjacent channel power as defined in mobile radio standards.

The numeric suffixes <1 to 8> in LIMIt are irrelevant for this command.

Parameter: The first value is the limit for the lower and the upper adjacent channel. The second limit value is ignored but must be indicated for reasons of compatibiltiy with the FSE family.

Example: `"CALC:LIM:ACP:ACH:ABS -35DBM, -35DBM"`

Sets the absolute limit value in screen A for the power in the lower and upper adjacent channel to -35 dBm.

Characteristics: *RST value: -200DBM
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:ACPower:ACHannel:ABSolute:STATe ON | OFF

This command activates the limit check for the adjacent channel when adjacent-channel power measurement (Adjacent Channel Power) is performed. Before the command, the limit check for the channel/adjacent-channel measurement must be globally switched on using `CALC:LIM:ACP ON`.

The result can be queried with `CALCulate:LIMit:ACPower:ACHannel:RESult?`. It should be noted that a complete measurement must be performed between switching on the limit check and the result query, since otherwise no valid results are available.

The numeric suffixes <1 to 8> in LIMIt are irrelevant for this command.

Example:

`"CALC:LIM:ACP:ACH 30DB, 30DB"`
Sets the relative limit value in screen A for the power in the lower and upper adjacent channel to 30 dB below the channel power.

`"CALC:LIM:ACP:ACH:ABS -35DBM, -35DBM"`
Sets the absolute limit value in screen A for the power in the lower and upper adjacent channel to -35 dB.

`"CALC:LIM:ACP ON"`
Switches on globally the limit check for the channel/adjacent channel measurement in screen A.

`"CALC:LIM:ACP:ACH:REL:STAT ON"`
Switches on the check of the relative limit values for adjacent channels in screen A.

`"CALC:LIM:ACP:ACH:ABS:STAT ON"`
Switches on the check of absolute limit values for the adjacent channels in screen A.

`"INIT;*WAI"`
Starts a new measurement and waits for the sweep end.

`"CALC:LIM:ACP:ACH:RES?"`
Queries the limit check result in the adjacent channels in screen A.

Characteristics:

*RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:ACPower:ACHannel:RESult?

This command queries the result of the limit check for the upper/lower adjacent channel in the selected measurement window when adjacent channel power measurement is performed.

If the power measurement of the adjacent channel is switched off, the command produces a query error.
The numeric suffixes <1 to 8> are irrelevant for this command.

Parameter: The result is returned in the form <result>, <result> where <result> = PASSED | FAILED, and where the first returned value denotes the lower, the second denotes the upper adjacent channel.

Example:

`"CALC:LIM:ACP:ACH 30DB, 30DB"`
Sets the relative limit value in screen A for the power in the lower and upper adjacent channel to 30 dB below the channel power.

`"CALC:LIM:ACP:ACH:ABS -35DBM, -35DBM"`
Sets the absolute limit value in screen A for the power in the lower and upper adjacent channel to -35 dB.

`"CALC:LIM:ACP ON"` Switches on globally the limit check for the channel/adjacent channel measurement in screen A.

`"CALC:LIM:ACP:ACH:STAT ON"` Switches on the limit check for the adjacent channels in screen A.

`"INIT;*WAI"` Starts a new measurement and waits for the sweep end.

`"CALC:LIM:ACP:ACH:RES?"` Queries the limit check result in the adjacent channels in screen A.

Characteristics: *RST value: --
SCPI: device-specific

Mode: A

This command is a query and therefore not assigned an *RST value.

CALCulate<1|2>:LIMit<1 to 8>:ACPower:ALTernate<1|2>[:RELative] 0 to 100dB, 0 to 100dB.

This command defines the limit for the first/second alternate adjacent channel in the selected measurement window for adjacent channel power measurements. The reference value for the relative limit value is the measured channel power.

The numeric suffix after `ALTernate<1|2>` denotes the first or the second alternate channel. The numeric suffixes <1 to 8> are irrelevant for this command.

It should be noted that the relative limit value has no effect on the limit check as soon as it is below th absolute limit defined with `CALCulate:LIMit:ACPower:ALTernate<1|2>:ABSolute`. This mechanism allows automatic checking of the absolute basic values of adjacent channel power as defined in mobile radio standards.

Parameter: The first value is the limit for the lower and the upper alternate adjacent channel. The second limit value is ignored but must be indicated for reasons of compatibility with the FSE family.

Example: `"CALC:LIM:ACP:ALT2 30DB, 30DB"` Sets the relative limit value in screen A for the power in the lower and upper alternate adjacent channel to 30 dB below the channel power.

Characteristics: *RST value: 0DB
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:ACPower:ALTernate<1|2>[:RELative]:STATe ON | OFF

This command activates the limit check for the first/second alternate adjacent channel in the selected measurement window for adjacent channel power measurements. Before the command, the limit check must be activated using `CALCulate:LIMit:ACPower:STATe ON`.

The numeric suffix after `ALTernate<1|2>` denotes the first or the second alternate channel. The numeric suffixes <1 to 8> are irrelevant for this command.

The result can be queried with `CALCulate:LIMit:ACPower:ALTernate<1|2>:RESult?`. It should be noted that a complete measurement must be performed between switching on the limit check and the result query, since otherwise no valid results are obtained.

Example:

`"CALC:LIM:ACP:ALT2 30DB, 30DB"`
Sets the relative limit value in screen A for the power in the lower and upper second alternate adjacent channel to 30 dB below the channel power.

`"CALC:LIM:ACP:ALT2:ABS -35DBM, -35DBM"`
Sets the absolute limit value in screen A for the power in the lower and upper second alternate adjacent channel to -35 dBm.

`"CALC:LIM:ACP ON"`
Switches on globally the limit check for the channel/adjacent channel measurement in screen A.

`"CALC:LIM:ACP:ACH:REL:STAT ON"`
Switches on the check of the relative limit values for the alternate adjacent channels in screen A.

`"CALC:LIM:ACP:ACH:ABS:STAT ON"`
Switches on the check of absolute limit values for the alternate adjacent channels in screen A.

`"INIT;*WAI"`
Starts a new measurement and waits for the sweep end.

`"CALC:LIM:ACP:ACH:RES?"`
Queries the limit check result in the second alternate adjacent channels in screen A.

Characteristics:

*RST value:	OFF
SCPI:	device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:ACPower:ALTernate<1|2>:ABSolute -200DBM to 200DBM, -200DBM to .200DBM

This command defines the absolute limit value for the lower/upper alternate adjacent channel power measurement (Adjacent Channel Power) in the selected measurement window.

The numeric suffix after `ALTernate<1|2>` denotes the first or the second alternate channel. The numeric suffixes <1 to 8> are irrelevant for this command.

It should be noted that the absolute limit value for the limit check has no effect as soon as it is below the relative limit value defined with `CALCulate:LIMit:ACPower:ALTernate<1|2>:RELative`. This mechanism allows automatic checking of the absolute basic values defined in mobile radio standards for the power in adjacent channels.

Parameter: The first value is the limit for the lower and the upper alternate adjacent channel. The second limit value is ignored but must be indicated for reasons of compatibility with the FSE family.

Example: `"CALC:LIM:ACP:ALT2:ABS -35DBM, -35DBM"`

Sets the absolute limit value in screen A for the power in the lower and upper second alternate adjacent channel to -35 dBm.

Characteristics: *RST value: -200DBM
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:ACPower:ALTernate<1|2>:ABSolute:STATe ON | OFF

This command activates the limit check for the first/second alternate adjacent channel in the selected measurement window for adjacent channel power measurement (Adjacent Channel Power).

Before the command, the limit check must be globally switched on for the channel/adjacent channel power with the command `CALCulate:LIMit:ACPower:STATe ON`.

The numeric suffix after `ALTernate<1|2>` denotes the first or the second alternate channel. The numeric suffixes <1 to 8> are irrelevant for this command.

The result can be queried with `CALCulate:LIMit:ACPower:ALTernate<1|2>:RESult?`. It should be noted that a complete measurement must be performed between switching on the limit check and the result query, since otherwise no valid results are available.

Example:

`"CALC:LIM:ACP:ALT2 30DB, 30DB"`
Sets the relative limit value in screen A for the power in the lower and upper second alternate adjacent channel to 30 dB below the channel power.

`"CALC:LIM:ACP:ALT2:ABS -35DBM, -35DBM"`
Sets the absolute limit value in screen A for the power in the lower and upper second alternate adjacent channel to -35 dBm.

`"CALC:LIM:ACP ON"`
Switches on globally the limit check for the channel/adjacent channel measurement in screen A.

`"CALC:LIM:ACP:ACH:REL:STAT ON"`
Switches on the check of the relative limit values for the alternative adjacent channels in screen A.

`"CALC:LIM:ACP:ACH:ABS:STAT ON"`
Switches on the check of absolute limit values for the alternative adjacent channels in screen A.

`"INIT;*WAI"`
Starts a new measurement and waits for the sweep end.

`"CALC:LIM:ACP:ACH:RES?"`
Queries the limit check result in the second alternate adjacent channels in screen A.

Characteristics:

*RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:ACPower:ALTernate<1|2>:RESult?

This command queries the result of the limit check for the first/second alternate adjacent channel in the selected measurement window for adjacent channel power measurements.

The numeric suffix after `ALTernate<1|2>` denotes the first or the second alternate channel. The numeric suffixes <1 to 8> are irrelevant for this command.

If the power measurement of the adjacent channel is switched off, the command produces a query error.

Parameter: The result is returned in the form <result>, <result> where <result> = PASSED | FAILED and where the first (second) returned value denotes the lower (upper) alternate adjacent channel.

Example:

`"CALC:LIM:ACP:ALT2 30DB, 30DB"`
Sets the relative limit value in screen A for the power in the lower and upper second alternate adjacent channel to 30 dB below the channel power.

`"CALC:LIM:ACP:ALT2:ABS -35DBM, -35DBM"`
Sets the absolute limit value in screen A for the power in the lower and upper second alternate adjacent channel to -35 dBm.

`"CALC:LIM:ACP ON"`
Switches on globally the limit check for the channel/adjacent channel measurement in screen A.

`"CALC:LIM:ACP:ALT:STAT ON"`
Switches on the limit check for the adjacent channels in screen A.

`"INIT;*WAI"`
Starts a new measurement and waits for the sweep end.

`"CALC:LIM:ACP:ALT:RES?"`
Queries the limit check result in the second alternate adjacent channels in screen A.

Characteristics: *RST value: --
SCPI: device-specific

Mode: A

This command is a query and therefore not assigned an *RST value.

CALCulate:LIMit:CONTrol Subsystem

The CALCulate:LIMit:CONTrol subsystem defines the x-axis (CONTrol-axis).

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:LIMit<1 to 8>			
:CONTrol			
[:DATA]	<numeric_value>,<numeric_value>..	HZ | S	
:DOMain	FREQuency|TIME		
:OFFSet	<numeric_value>	HZ | S	
:MODE	RELative|ABSolute		
:SHIFt	<numeric_value>	HZ | S	

CALCulate<1|2>:LIMit<1 to 8>:CONTrol[:DATA] <numeric_value>,<numeric_value>..

This command defines the X-axis values (frequencies or times) of the upper or lower limit lines.The values are defined independently of the measurement window.

The number of values for the CONTrol axis and for the corresponding UPPer and/or LOWer limit lines have to be identical. Otherwise default values are entered for missing values or not required values are deleted.

The unit of values depends on the frequency or time domain of the X-axis, ie it is `HZ` with `CALC:LIM:CONT:DOM FREQ` und `S` bei `CALC:LIM:CONT:DOM TIME`.

Example: `"CALC:LIM2:CONT 1MHz,30MHz,100MHz, 300MHz,1GHz"`
Defines 5 reference values for the X-axis of limit line 2

`"CALC:LIM2:CONT?"` Outputs the reference values for the X-axis of limit line 2 separated by a comma.

Characteristics: *RST value: - (LIMit:STATe is set to OFF)
SCPI: conforming

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:CONTrol:DOMain FREQuency | TIME

This command defines the frequency or time domain for the x-axis values.

Example: `"CALC:LIM2:CONT:DOM TIME"` Defines the time domain for the X-axis of limit line 2.

Characteristics: *RST value: FREQuency
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:CONTrol:OFFSet <numeric_value>

This command defines an offset for the X-axis value of the selected relative limit line in the frequency or time domain.

The unit of values depends on the frequency or time domain of the X-axis, ie it is HZ with CALC:LIM:CONT:DOM FREQ und S bei CALC:LIM:CONT:DOM TIME.

Example: "CALC:LIM2:CONT:OFFS 100us" Sets the X offset for limit line 2 (defined in the time domain) to 100us.

Characteristics: *RST value: 0
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:CONTrol:MODE RELative | ABSolute

This command selects the relative or absolute scaling for the X-axis of the selected limit line. The definition is independent of the measurement window.

Example: "CALC:LIM2:CONT:MODE REL" Defines the X-axis of limit line 2 as relatively scaled.

Characteristics: *RST value: ABSolute
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:CONTrol:SHIFt <numeric_value>

This command moves a limit line by the indicated value in x direction. In contrast to CALC:LIM:CONT:OFFS, the line is shifted by modifying the individual x values and not by means of an additive offset. The shift is independent of the measurement window.

The unit of values depends on the frequency or time domain of the X-axis, ie it is HZ with CALC:LIM:CONT:DOM FREQ und S bei CALC:LIM:CONT:DOM TIME.

Example: "CALC:LIM2:CONT:SHIF 50KHZ" Shifts all reference values of limit line 2 by 50 kHz.

Characteristics: *RST value: --
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate:LIMit:LOWer Subsystem

The CALCulate:LIMit:LOWer subsystem defines the lower limit line.

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:LIMit<1 to 8>			
:LOWer			
[:DATA]	<numeric_value>,<numeric_value>..	DBM | DB | DEG | RAD | S | HZ | PCT	
:STATe	<Boolean>	--	
:OFFSet	<numeric_value>	DB| DEG| RAD| S | HZ | PCT	
:MARGin	<numeric_value>	DB| DEG| RAD| S | HZ | PCT	
:MODE	RELative|ABSolute	--	
:SHIFt	<numeric_value>	DB| DEG| RAD| S | HZ | PCT	
:THReshold	<numeric_value>	DBM | DB | DEG | RAD | S | HZ | PCT	

CALCulate<1|2>:LIMit<1 to 8>:LOWer[:DATA] <numeric_value>,<numeric_value>..

This command defines the values for the selected lower limit line independently of the measurement window.

The number of values for the CONTrol axis and for the corresponding LOWer limit line has to be identical. Otherwise default values are entered for missing values or not necessary values are deleted.

The unit must be identical with the unit selected by `CALC:LIM:UNIT`. If no unit is indicated, the unit defined with `CALC:LIM:UNIT` is automatically used.

If the measured values are smaller than the LOWer limit line, the limit check signals errors.

The units DEG, RAD, S, HZ, PCT are not available in the spectrum analysis mode.

Example: `"CALC:LIM2:LOW -30,-40,-10,-40,-30"`
Defines 5 lower limit values for limit line 2 in the preset unit.

`"CALC:LIM2:LOW?"`
Outputs the lower limit values of limit line 2 separated by a comma.

Characteristics: *RST value: - (LIMit:STATe is set to OFF)
SCPI: conforming

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:LOWer:STATe ON | OFF

This command switches on or off the indicated limit line in the selected measurement window. The limit check is activated separately with `CALC:LIM:STAT ON`.

The result of the limit check can be queried with `CALCulate:LIMit<1 to 8>:FAIL?`.

Example: `"CALC:LIM4:LOW:STAT ON"` Switches on limit line 4 (lower limit) in screen A.

`"CALC2:LIM4:LOW:STAT ON"` Switches on limit line 4 (lower limit) also in screen B.

Characteristics: *RST value: OFF
SCPI: conforming

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:LOWer:OFFSet <numeric_value>

This command defines an offset for the Y-axis of the selected relative lower limit line. In contrast to `CALC:LIM:LOW:SHIFt`, the line is not shifted by modifying the individual Y values but by means of an additive offset. The offset is independent of the measurement window.

Example: `"CALC:LIM2:LOW:OFFS 3dB"` Shifts limit line 2 in the corresponding measurement windows by 3 dB upwards.

Characteristics: *RST value: 0
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:LOWer:MARGin <numeric_value>

This command defines a margin to a lower limit line, at which out-of-limit values are signalled (if the limit check is active), but not handled as a violation of the limit value. The margin is independent of the measurement window.

Only the unit dB is available in spectrum analysis mode.

Example: `"CALC:LIM:LOW:MARG 10dB"`

Characteristics: *RST value: 0
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:LOWer:MODE RELative | ABSolute

This command selects the relative or absolute scaling for the Y-axis of the selected lower limit line. The setting is independent of the measurement window.

Selecting RELative causes the unit to be switched to DB.

Example: `"CALC:LIM:LOW:MODE REL"` Defines the Y-axis of limit line 2 as relative scaled.

Characteristics: *RST value: ABSolute
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:LOWer:SHIFt <numeric_value>

This command shifts a limit line by the indicated value in Y-direction. In contrast to CALC:LIM:LOW:OFFS, the line is shifted by modifying the individual Y values but not by means of an additive offset. The shift is independent of the measurement window.

Example: "CALC:LIM3:LOW:SHIF 20DB" Shifts all Y values of limit line 3 by 20 dB.

Characteristics: *RST value: --
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:LIMit<1 to 8>:LOWer:THReshold <numeric_value>

This command defines an absolute threshold value for limit lines with relative Y-axis scaling independently of the measurement window. The absolute threshold value is used in the limit check as soon as it exceeds the relative limit value.

The unit must correspond to the unit selected with CALC:LIM:UNIT (except dB which is not allowed). If no unit is indicated, the unit defined with CALC:LIM:UNIT is automatically used (exception: dBm instead of dB).

The units DEG, RAD, S, HZ, PCT are not available in the spectrum analysis mode.

Example: "CALC:LIM2:LOW:THR -35DBM" Defines an absolute threshold value for limit line 2.

Characteristics: *RST value: -200 dBm
SCPI: device-specific

Mode: A

CALCulate:LIMit:UPPer Subsystem

The CALCulate:LIMit:UPPer subsystem defines the upper limit line.

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:LIMit<1 to 8>			
:UPPer			
[:DATA]	<numeric_value>,<numeric_value>..	DBM | DB | DEG | RAD | S | HZ | PCT	
:STATe	<Boolean>	--	
:OFFSet	<numeric_value>	DB| DEG| RAD| S | HZ | PCT	
:MARGin	<numeric_value>	DB| DEG| RAD| S | HZ | PCT	
:MODE	RELative|ABSolute	--	
:SHIFt	<numeric_value>	DB |DEG| RAD| S | HZ | PCT	
:THReshold	<numeric_value>	DBM | DB | DEG | RAD | S | HZ | PCT	

CALCulate<1|2>:LIMit<1 to 8>:UPPer[:DATA] <numeric_value>,<numeric_value>..

This command defines the values for the upper limit lines independently of the measurement window.

The number of values for the CONTrol axis and for the corresponding UPPer and/or LOWer limit line have to be identical. Otherwise default values are entered for missing values or not necessary values are deleted.

The unit must be identical with the unit selected by `CALC:LIM:UNIT`. If no unit is indicated, the unit defined with `CALC:LIM:UNIT` is automatically used.

The units DEG, RAD, S, HZ, PCT are not available in spectrum analysis mode.

If the measured values exceed the UPPer limit line, the limit check signals errors.

Example: `"CALC:LIM2:UPP -10,0,0,-10,-5"` Defines 5 upper limit values for limit line 2 in the preset unit.

`"CALC:LIM2:UPP?"` Outputs the upper limit values for limit line 2 separated by a comma.

Characteristics: *RST value: - (LIMit:STATe is set to OFF)
SCPI: conforming

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:UPPer:STATe ON | OFF

This command switches on or off the indicated limit line in the selected measurement window. The limit check is activated separately with `CALC:LIM:STAT ON`.

The result of the limit check can be queried with `CALCulate:LIMit<1 to 8>:FAIL?`.

Example: `"CALC1:LIM4:UPP:STAT ON"` Switches on limit line 4 (upper limit) in screen A.

`"CALC2:LIM4:UPP:STAT ON"` Switches on limit line 4 (upper limit) in screen B.

Characteristics: *RST value: OFF
SCPI: conforming

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:UPPer:OFFSet <numeric_value>

This command defines an offset for the Y-axis of the selected relative upper limit line. In contrast to `CALC:LIM:UPP:SHIFt`, the line is not shifted by modifying the individual Y values but by means of an additive offset. The offset is independent of the measurement window.

Only the unit dB is available in the spectrum analysis mode.

Example: `"CALC:LIM2:UPP:OFFS 3dB"` Shifts limit line 2 by 3 dB upwards in the corresponding measurement windows.

Characteristics: *RST value: 0
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:UPPer:MARGin <numeric_value>

This command defines a margin to an upper limit line, at which out-of-limit values are signalled (if the limit check is active), but not handled as a violation of the limit value. The margin is independent of the measurement window.

Only the unit dB is available in spectrum analysis mode.

Example: `"CALC:LIM2:UPP:MARG 10dB"` Defines the margin of limit line 2 to 10 dB below the limit value.

Characteristics: *RST value: 0
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:UPPer:MODE RELative | ABSolute

This command selects the relative or absolute scaling for the Y-axis of the selected upper limit line. The setting is independent of the measurement window.

Selecting RELative causes the unit to be switched to DB.

Example: "CALC:LIM2:UPP:MODE REL" Defines the Y-axis of limit line 2 as relative scaled.

Characteristics: *RST value: ABSolute
SCPI: device-specific

Mode: A

CALCulate<1|2>:LIMit<1 to 8>:UPPer:SHIFt <numeric_value>

This command moves a limit line by the indicated value in Y-direction. In contrast to CALC:LIM:UPP:OFFS, the line is shifted by modifying the individual Y values and not by means of an additive offset. The shift is independent of the measurement window.

Only the unit dB is available in the spectrum analysis mode.

Example: "CALC:LIM3:UPP:SHIF 20DB" Shifts all Y values of limit line 3 by 20 dB.

Characteristics: *RST value: --
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:LIMit<1 to 8>:UPPer:THReshold <numeric_value>

This command defines an absolute threshold value for limit lines with relative Y-axis scaling independently of the measurement window. The absolute threshold value is used in the limit check as soon as it exceeds the relative limit value.

The unit must correspond to the unit selected with CALC:LIM:UNIT (except dB which is not possible). If no unit is indicated, the unit defined with CALC:LIM:UNIT is automatically used (exception: dBm instead of dB).

The units DEG, RAD, S, HZ, PCT are not available in the spectrum analysis mode.

Example: "CALC:LIM2:UPP:THR -35DBM" Defines an absolute threshold value for limit line 2.

Characteristics: *RST value: -200 dBm
SCPI: device-specific

Mode: A

CALCulate:MARKer Subsystem

The CALCulate:MARKer subsystem checks the marker functions in the instrument. The measurement windows are assigned to CALCulate 1 (screen A) or 2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:MARKer<1 to 4>			
[:STATe]	<Boolean>	--	
:AOFF			no query
:TRACe	<numeric_value>	--	
:X	<numeric_value>	HZ | S | DBM | DB	
:SLIMits			
[:STATe]	<Boolean>		
:LEFT	<numeric_value>	HZ | S	
:RIGHt	<numeric_value>	HZ | S	
:COUNt	<Boolean>	--	
:RESolution	<numeric_value>	HZ	
:FREQuency?	--	--	query only
:LOEXclude	<Boolean>		
:Y?	--	--	query only
:PERCent	<numeric_value>	PCT	
:MAXimum		--	
[:PEAK]	--	--	no query
:NEXT	--	--	no query
:RIGHt	--	--	no query
:LEFT	--	--	no query
:MINimum			
[:PEAK]	--	--	no query
:NEXT	--	--	no query
:RIGHt	--	--	no query
:LEFT	--	--	no query
:PEXCursion	<numeric_value>	DB	

CALCulate<1|2>:MARKer<1 to 4>[:STATe] ON | OFF

This command switches on or off the currently selected marker in the selected measurement window. If no indication is made, marker 1 is selected automatically. If marker 2, 3 or 4 is selected and used as a delta marker, it is switched to marker mode.

Example: `"CALC:MARK3 ON"` Switches marker 3 in screen A on or to marker mode.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:AOFF

This command switches off all active markers in the selected measurement window. All delta markers and active marker/delta marker measurement functions are switched off.

Example: "CALC:MARK:AOFF" Switches off all markers in screen A.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:TRACe 1 to 3

This command assigns the selected marker (1 to 4) to the indicated measurement curve in the selected measurement window. The corresponding trace must be active, ie its status must be different from "BLANK".

If necessary the corresponding marker is switched on prior to the assignment.

Example: "CALC:MARK3:TRAC 2" Assigns marker 3 in screen A to trace 2.

"CALC2:MARK:TRAC 3" Assigns marker 1 in screen B to trace 3.

Characteristics: *RST value -
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:X 0 to MAX (frequency | sweep time)

This command positions the selected marker to the indicated frequency (span > 0), time (span = 0) or level (APD measurement or CCDF measurement ON) in the selected measurement window. If marker 2, 3 or 4 is selected and used as delta marker, it is switched to marker mode.

Example: "CALC1:MARK2:X 10.7MHz" Positions marker 2 in screen A to frequency 10.7 MHz.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:X:SLIMits[:STATe] ON | OFF

This command switches between a limited (ON) and unlimited (OFF) search range in the selected measurement window. The function is independent of the selection of a marker, ie the numeric suffix MARKer<1 to 4> is irrelevant.

If the time domain power measurement is active, this command limits the evaluation range on the trace.

Example: "CALC:MARK:X:SLIM ON" Switches on search limitation in screen A.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:X:SLIMits:LEFT 0 to MAX (frequency | sweep time)

This command sets the left limit of the search range for markers and delta markers in the selected measurement window. Depending on the x-axis domain the indicated value defines a frequency (span > 0) or time (span = 0). The function is independent of the selection of a marker, ie the numeric suffix in MARKer<1 to 4> is irrelevant.

If the time domain power measurement is active, this command limits the evaluation range to the trace.

Note: *The function is only available if the search limit for marker and delta marker is switched on* `(CALC:MARK:X:SLIM ON)`.

Example:

`"CALC:MARK:X:SLIM ON"`	Switches the search limit function on for screen A.
`"CALC:MARK:X:SLIM:LEFT 10MHz"`	Sets the left limit of the search range in screen A to 10 MHz.

Characteristics: *RST value: - (is set to the left diagram border on switching on search limits)
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:X:SLIMits:RIGHT 0 to MAX (frequency | sweep time)

This command sets the right limit of the search range for markers and delta markers in the selected measurement window. Depending on the x-axis domain the indicated value defines a frequency (span > 0) or time (span = 0). The function is independent of the selection of a marker, ie the numeric suffix in MARKer<1 to 4> is irrelevant.

If the time domain power measurement is active, this command limits the evaluation range to the trace.

Note:
The function is only available if the search limit for marker and delta marker is switched on `(CALC:MARK:X:SLIM ON)`.

Example:

`"CALC:MARK:X:SLIM ON"`	Switches the search limit function on for screen A.
`"CALC:MARK:X:SLIM:RIGH 20MHz"`	Sets the right limit of the search range in screen A to 20 MHz.

Characteristics: *RST value: - is set to the right diagram border on switching on search limits)
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:COUNt ON | OFF

This command switches on or off the frequency counter at the marker position in the selected measurement window. The count result is queried with `CALCulate:MARKer:COUNt:FREQuency?`.

Frequency counting is possible only for one marker at a time for each measurement window. If it is activated for another marker, it is automatically de-activated for the previous marker.

It should be noted that a complete sweep must be performed after switching on the frequency counter to ensure that the frequency to be measured is actually reached. The synchronization to the sweep end required for this is possible only in single-sweep mode.

Example:

`"INIT:CONT OFF"`	Switches to single-sweep mode.
`"CALC:MARK ON"`	Switches on marker 1 in screen A.
`"CALC:MARK:COUN ON"`	Switches on the frequency counter for marker 1.
`"INIT;*WAI"`	Starts a sweep and waits for the end.
`"CALC:MARK:COUN:FREQ?"`	Outputs the measured value in screen A.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:COUNt:RESolution 0.1 | 1 | 10 | 100 | 1000 | 10000 Hz

This command specifies the resolution of the frequency counter in the selected measurement window.The setting is independent of the selected marker, ie the numeric suffix in MARKer<1 to 4> is irrelevant.

Example:

`"CALC:MARK:COUN:RES 1kHz"`	Sets the resolution of the frequency counter to 1 kHz.

Characteristics: *RST value: 1kHz
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:COUNt:FREQuency?

This command queries the result of the frequency counter for the indicated marker in the selected measurement window. Before the command, the frequency counter should be switched on and a complete measurement performed to obtain a valid count result. Therefore, a single sweep with synchronization must be performed between switching on the frequency counter and querying the count result.

Example:

`"INIT:CONT OFF"`	Switches to single-sweep mode.
`"CALC:MARK2 ON"`	Switches marker 2 in screen A.
`"CALC:MARK2:COUN ON"`	Switches the frequency counter for marker 2.
`"INIT;*WAI"`	Starts a sweep and waits for the end.
`"CALC:MARK2:COUN:FREQ?"`	Outputs the measured value of delta marker 2 in screen A.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is only a query and thus has no *RST value.

CALCulate<1|2>:MARKer<1 to 4>:LOEXclude ON | OFF

This command switches the local oscillator suppression for peak search on or off. This setting is valid for all markers and delta markers in all measurement windows.

Example: "CALC:MARK:LOEX ON"

Characteristics: *RST value: ON
SCPI: device-specific

Mode: A-F

The numeric suffixes 1|2 and 1 to 4 are irrelevant.

CALCulate<1|2>:MARKer<1 to 4>:Y?

This command queries the selected marker value in the selected measurement window. The corresponding marker is activated first or switched to the marker mode, if necessary.

A complete sweep with synchronization to sweep end must be performed between switching on the marker and querying the y value to obtain a valid query result. This is only possible in single sweep mode.

The query result is output in the unit defined with CALCulate:UNIT.

Example:

"INIT:CONT OFF"	Switches to single-sweep mode.
"CALC:MARK2 ON"	Switches marker 2 in screen A.
"INIT;*WAI"	Starts a sweep and waits for the end.
"CALC:MARK2:Y?"	Outputs the measured value of marker 2 in screen A.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1...4>:Y:PERCent 0 to100%

This command positions the selected marker in the selected window to the given probability. If marker 2, 3 or 4 is selected and used as a delta marker, it is switched to marker mode.

Note: *The command is only available with the CCDF measurement switched on. The associated level value can be determined with the CALC:MARK:X? command.*

Example: "CALC1:MARK:Y:PERC 95PCT" positions marker 1 in screen A to a probability of 95%.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:MAXimum[:PEAK]

This command positions the marker to the current maximum value of the corresponding trace in the selected measurement window. The corresponding marker is activated first or switched to the marker mode.

Note: *If no maximum value is found on the trace (level spacing to adjacent values < peak excursion), an execution error (error eode: -200) is produced.*

Example: "CALC:MARK2:MAX" Positions marker 2 in screen A to the maximum value of the trace.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:MAXimum:NEXT

This command positions the marker to the next smaller maximum value of the corresponding trace in the selected measurement window.

Note: *If no next smaller maximum value is found on the trace (level spacing to adjacent values < peak excursion), an execution error (error code: -200) is produced.*

Example: "CALC:MARK2:MAX:NEXT" Positions marker 2 in screen A to the next lower maximum value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:MAXimum:RIGHt

This command positions the marker to the next smaller maximum value to the right of the current value (ie in ascending X values) on the corresponding trace in the selected measurement window.

Note: *If no next smaller maximum value is found on the trace (level spacing to adjacent values < peak excursion), an execution error (error code: -200) is produced.*

Example: `"CALC:MARK2:MAX:RIGH"` Positions marker 2 in screen A to the next lower maximum value to the right of the current value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:MAXimum:LEFT

This command positions the marker to the next smaller maximum value to the left of the current value (ie in descending X values) on the trace in the selected measurement window.

Note: *If no next smaller maximum value is found on the trace (level spacing to adjacent values < peak excursion), an execution error (error code: -200) is produced.*

Example: `"CALC:MARK2:MAX:LEFT"` Positions marker 2 in screen A to the next lowe maximum value to the left of the current value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:MINimum[:PEAK]

This command positions the marker to the current minimum value of the corresponding trace in the selected measurement window. The corresponding marker is activated first or switched to marker mode, if necessary.

Note: *If no minimum value is found on the trace (level spacing to adjacent values < peak excursion), an execution error (error code: -200) is produced.*

Example: `"CALC:MARK2:MIN"` Positions marker 2 in screen A to the minimum value of the trace.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:MINimum:NEXT

This command positions the marker to the next higher minimum value of the corresponding trace in the selected measurement window.

Note: *If no next higher minimum value is found on the trace (level spacing to adjacent values < peak excursion), an execution error (error code: -200) is produced.*

Example: "CALC:MARK2:MIN:NEXT" Positions marker 2 in screen A to the next higher maximum value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:MINimum:RIGHt

This command positions the marker to the next higher minimum value to the right of the current value (ie in ascending X direction) on the corresponding trace in the selected measurement window.

Note: *If no next higher minimum value is found on the trace (level spacing to* adjacent values *< peak excursion), an execution error (error code: -200) is produced.*

Example: "CALC:MARK2:MIN:RIGH" Positions marker 2 in screen A to the next higher minimum value to the right of the current value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:MINimum:LEFT

This command positions the marker to the next higher minimum value to the left of the current value (ie in descending X direction) on the corresponding trace in the selected measurement window.

Note: *If no next higher minimum value is found on the trace (level spacing to* adjacent values *< peak excursion), an execution error (error code: -200) is produced.*

Example: "CALC:MARK2:MIN:LEFT" Positions marker 2 in screen A to the next higher minimum value to the left of the current value.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:PEXCursion <numeric_value>

This command defines the peak excursion., ie the spacing below a trace maximum which must be attained before a new maximum is recognized, or the spacing above a trace minimum which must be attained before a new minimum is recognized. The set value is valid for all markers and delta markers.

Example: `"CALC:MARK:PEXC 10dB"`

Characteristics: *RST value: 6dB
SCPI: device-specific

Mode: A

The numeric suffix in MARKer<1 to 4> is irrelevant.

CALCulate:MARKer:FUNCtion Subsystem

The measurement window is selected by CALCulate 1 (screen A) or 2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:MARKer<1 to 4>			
:FUNCtion			
:NDBDown	<numeric_value>	DB	
:STATe	<Boolean>		
:RESult?	--	--	query only
:FREQuency?	--	--	query only
:ZOOM	<numeric_value>	HZ	no query
:NOISe			
[:STATe]	<Boolean>		
:RESult?	--	--	query only
:DEModulation			option audio demodulator
:SELect	AM|FM		
[:STATe]	<Boolean>		
:HOLDoff	<numeric_value>	S	
:CONTinuous	<Boolean>		
:MDEPth			
[:STATe]	<Boolean>	--	
:RESult?	--		query only
:TOI			
[:STATe]	<Boolean>	--	
:RESult?	--		query only
:CENTer			no query
:CSTep			no query
:REFerence			no query

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:NDBDown <numeric_value>

This command defines the level spacing of the two delta markers to the right and left of marker 1 in the selected measurement window. Marker 1 is always used as the reference marker. The numeric suffix <1 to 4> is irrelevant for this command.

The temporary markers T1 and T2 are positioned by n dB below the active reference marker. The frequency spacing of these markers can be queried with `CALCulate:MARKer:FUNCtion:NDBDown:RESult?`.

Example: `"CALC:MARK:FUNC:NDBD 3dB"` Sets the level spacing in screen A to 3 dB.

Characteristics: *RST value: 6dB
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:NDBDown:STATe ON | OFF

This command switches the "N dB Down" function on or off in the selected measurement window. Marker 1 is activated first, if necessary. The numeric suffix <1 to 4> is irrelevant for this command.

Example: `"CALC:MARK:FUNC:NDBD:STAT ON"` Switches on the N-dB-down function in screen A.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:NDBDown:RESult?

This command queries the frequency spacing (bandwidth) of the N-dB-down markers in the selected measurement window. The numeric suffix <1 to 4> is irrelevant for this command.

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value in order to obtain a valid query result. This is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"              Switches to single-sweep mode.
"CALC:MARK:FUNC:NDBD ON"     Switches on the n-dB-down function in
                             screen A.
"INIT;*WAI"                  Starts a sweep and waits for the end.
"CALC:MARK:FUNC:NDBD:RES?"   Outputs the measured value of screen A.
```

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is only a query and is therefore not assigned an *RST value.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:NDBDown:FREQuency?

This command queries the two frequencies of the N-dB-down marker in the selected measurement window. The numeric suffix <1 to 4> is irrelevant for this command. The two frequency values are separated by comma and output in ascending order.

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"              Switches to single-sweep mode.
"CALC:MARK:FUNC:NDBD ON"     Switches on the n-dB-down function in
                             screen A.
"INIT;*WAI"                  Starts a sweep and waits for the end.
"CALC:MARK:FUNC:NDBD:FREQ?"  Outputs the frequencies of the temporary
                             markers in screen A.
```

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is only a query and is therefore not assigned an *RST value.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:ZOOM <numeric_value>

This command defines the range to be zoomed around marker 1 in the selected measurement window. Marker 1 is activated first, if necessary.

The subsequent frequency sweep is stopped at the marker position and the frequency of the signal is counted. This frequency becomes the new center frequency, and the zoomed span is set. In order to recognize the end of the operation the synchronization to the sweep end should be activated. This is only possible in single sweep mode.

Example:
```
"INIT:CONT OFF"                    Switches to single-sweep mode
"CALC:MARK:FUNC:ZOOM 1kHz;*WAI"    Activates zooming in screen A and
                                   waits for its end.
```

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:NOISe[:STATe] ON | OFF

This command switches the noise measurement on or off for all markers of the indicated measurement window. The noise power density is measured at the position of the markers. The result can be queried with `CALCulate:MARKer:FUNCtion:NOISe:RESult?`.

Example:
```
"CALC2:MARK:FUNC:NOIS ON"   Switches on the noise measurement for
                            screen B.
```

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:NOISe:RESult?

This command queries the result of the noise measurement.

A complete sweep with synchronization to the sweep end must be performed between switching on the function and querying the measured value in order to obtain a valid query result. This is only possible in single sweep mode.

Example:
```
"INIT:CONT OFF"              Switches to single-sweep mode.
"CALC:MARK2 ON"              Switches on marker 2 in screen A.
"CALC:MARK:FUNC:NOIS ON"     Switches on noise measurement in screen A.
"INIT;*WAI"                  Starts a sweep and waits for the end.
"CALC:MARK2:NOIS:RES?"       Outputs the noise result of marker 2 in
                             screen A.
```

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:DEModulation:SELect AM | FM

This command selects the demodulation type for the audio demodulator. The command is independent of the measurement window and of the selected marker, ie suffixes 1|2 and 1 to 4 are irrelevant.

This command is only available with the audio demodulator option FSP-B3.

Example: `"CALC:MARK:FUNC:DEM:SEL FM"`

Characteristics: *RST value: AM
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:DEModulation[:STATe] ON | OFF

This command switches on or off the audio demodulator when the indicated marker is reached in the selected measurement window. In the frequency domain (span > 0) the hold time can be defined at the corresponding marker position with `CALCulate:MARKer:FUNCtion: DEModulation:HOLD`. In the time domain (span = 0) the demodulation is permanently active.

The command is only available with option audio demodulator FSP-B3.

Example: `"CALC2:MARK3:FUNC:DEM ON"` Switches on the demodulation for marker 3 in screen B.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:DEModulation:HOLDoff 10ms to 1000s

This command defines the hold time at the marker position for the demodulation in the frequency domain (span > 0). The setting is independent of the measurement window and the selected marker, ie the suffixes <1|2> and <1 to 4> are irrelevant

The command is only available with option audio demodulator FSP-B3.

Example: `"CALC:MARK:FUNC:DEM:HOLD 3s"`

Characteristics: *RST value: - (DEModulation is set to OFF)
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation:CONTinuous ON | OFF

This command switches on or off the continuous demodulation in the frequency domain (span >0) in the selected measurement window. Thus acoustic monitoring of the signals can be performed in the frequency domain. The function does not depend on the selected marker, ie the suffix <1 to 4> is irrelevant.

The command is only available with option audio demodulator FSP-B3.

Example: `"CALC2:MARK3:FUNC:DEM:CONT ON"` switches on the continuous demodulation in screen B.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: **A**

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:MDEPth:[:STATe]

This command switches on the measurement of the AM modulation depth. An AM-modulated carrier is required on the screen for correct operation. If necessary, marker 1 is previously activated and set to the largest signal available.

The level value of marker 1 is regarded as the carrier level. On activating the function, marker 2 and marker 3 are automatically set as delta markers symetrically to the carrier to the adjacent maxima of the trace.

If the position of delta marker 2 is changed, delta marker 3 is moved symetrically with respect to the reference marker (marker 1). If the position of delta marker 3 is changed, fine adjustment can be performed independently of delta marker 2.

The FSP calculates the power at the marker positions from the measured levels. The AM modulation depth is calculated from the ratio of power values at the reference marker and the delta markers. If the two AM sidebands differ in power, the average value of the two power values is used for calculating the AM modulation depth.

The suffix <1 to 4> of :MARKer is irrelevant with this command.

Example:

`"CALC:MARK:X 10MHZ"`	Sets the reference marker (marker 1) to the carrier signal at 10 MHz
`"CALC:MARK:FUNC:MDEP ON"`	Switches on the modulation depth measurement in screen A.
`"CALC:DELT2:X 10KHZ"`	Sets delta markers 2 and 3 to the signals at 10 kHz from the carrier signal
`"CALC:DELT3:X 9.999KHZ"`	Corrects the position of delta marker 3 relative to delta marker 2.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:MDEPth:RESult?

This command queries the AM modulation depth in the indicated measurement window.

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

The suffix <1 to 4> of :MARKer is irrelevant for this command.

Example:

`"INIT:CONT OFF"`	Switches to single-sweep mode.
`"CALC:MARK:X 10MHZ"`	Sets the reference marker (marker 1) to the carrier signal at 10 MHz.
`"CALC:MARK:FUNC:MDEP ON"`	Switches on the modulation depth measurement in screen A.
`"INIT;*WAI"`	Starts a sweep and waits for the end.
`"CALC:MARK:FUNC:MDEP:RES?"`	Outputs the measured value of screen A.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:TOI[:STATe] ON | OFF

This command initiates the measurement of the third-order intercept point.

A two-tone signal with equal carrier levels is expected at the input of FSP. Marker 1 and marker 2 (both normal markers) are set to the maximum of the two signals. Delta marker 3 and delta marker 4 are positioned to the intermodulation products. The delta markers can be modified sperately afterwards with the commands `CALCulate:DELTamarker3:X` and `CALCulate:DELTamarker4:X`.

The FSP calculates the third-order intercept from the level spacing between the normal markers and the delata markers.

The suffix <1 to 4> of :MARKer is irrelevant for this command.

Example: `"CALC:MARK:FUNC:TOI ON"` Switches on the measurement of the third-order intercept in screen A.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:TOI:RESult?

This command queries the third-order intercept point measurement in the indicated measurement window.

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

The suffix <1 to 4> of :MARKer is irrelevant of this command.

Example:

`"INIT:CONT OFF"`	Switches to single-sweep mode.
`"CALC:MARK:FUNC:TOI ON"`	Switches the intercept measurement in screen A.
`"INIT;*WAI"`	Starts a sweep and waits for the end.
`"CALC:MARK:FUNC:TOI:RES?"`	Outputs the measured value of screen A.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:CENTer

This command sets the center frequency of the selected measurement window equal to the frequency of the indicated marker.

If marker 2, 3 or 4 is selected and used as delta marker, it is switched to the marker mode.

Example: `"CALC:MARK2:FUNC:CENT"` Sets the center frequency of screen A to the frequency of marker 2.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

This command is an "event" and therefore has no *RST value assigned and has no query.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:CSTep

This command sets the step width of the center frequency in the selected measurement window to the X value of the current marker. If marker 2, 3 or 4 is selected and used as delta marker, it is switched to the marker mode.

Example: `"CALC2:MARK3:FUNC:CST"` Sets the center frequency of screen B to the same value as the frequency of marker 3.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

This command is an event and therefore has no *RST value assigned and has no query.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:REFerence

This command sets the reference level in the selected measurement window to the power measured by the indicated marker. If marker 2, 3 or 4 is selected and used as delta marker, it is switched to marker mode.

Example: `"CALC:MARK2:FUNC:REF"` Sets the reference level of screen A to the the level of marker 2.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

This command is an event and therefore has no *RST value assigned and has no query.

CALCulate:MARKer:FUNCtion:POWer Subsystem

The CALCulate:MARKer:FUNCtion:POWER subsystem contains the commands for control of power measurement.

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:MARKer			
:FUNCtion			
:POWer			
:SELect	ACPower | CPOWer | OBANdwidth | OBWidth		
:RESult?	ACPower | CPOWer | OBANdwidth | OBWidth<Boolean>		query only
:PHZ	<Boolean>		
:PRESet	NADC | TETRA | PDC | PHS | CDPD | FWCDma | RWCDma | F8CDma | R8CDma | F19Cdma | R19Cdma | FW3Gppcdma | RW3Gppcdma | D2CDma | S2CDma | M2CDma | FIS95A | RIS95A | FIS95C0 | RIS95C0 | FIS95C1 | RIS95C1 | FJ008 | RJ008 | NONE		
[:STATe]	OFF		no query

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:POWer:SELect ACPower | CPOWer | OBANdwidth | OBWidth

This command selects the indicated power measurement and switches it on in the selected measurement window. The function is independent of the selected marker, ie the suffix <1 to 4> of MARKer is irrelevant.
The configuration of channel spacings and channel bandwidths is performed by means of subsystem `SENSe:POWer:ACHannel`.
It should be noted that selecting CPOWer causes the number of adjacent channels (command: `[SENSe<1|2>:]POWer:ACHannel:ACPairs`) to be set to 0. Selecting ACPower causes the number of adjacent channels to be set to 1, if the adjacent channel power measurement is not yet switched on. In both cases the behaviour of FSP differs from that of the FSE family.
Note: *The measurement of the channel/adjacent channel power is performed on the trace which has been selected with* `SENSe:POWer:TRACe 1|2|3`.

The measurement of the occupied bandwidth is performed on the trace on which marker 1 is positioned. In order to evaluate another trace, marker 1 should be positioned on another trace with `CALC:MARK:TRAC 1|2|3`.

Parameter:

ACPower	adjacent channel power measurement
CPOWer	channel power measurement (same as adjacent channel power measurement with No. of Adj Channels = 0)
OBANdwidth | OBWidth	occupied bandwidth power measurement

Example: `"CALC:MARK:FUNC:POW:SEL ACP"` Switches on the adjacent channel power measurement in screen A.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:POWer:RESult? ACPower | CPOWer | OBANdwidth | OBWidth

This command queries the results of the power measurement in the selected measurement window.The measurement is switched on first, if necessary.

The configuration of channel spacings and channel bandwidths is performed with subsytem `SENSe:POWer:ACHannel`.

To obtain a valid result, a complete sweep with synchronization to the sweep end must be performed before the query is executed. This is possible in single sweep mode only.

Parameter:

ACPower: adjacent channel power measurement

Results are output separated by commas in the following order:

1. Power of main channel
2. Power of lower adjacent channel
3. Power of upper adjacent channel
4. Power of lower alternate adjacent channel 1
5. Power of upper alternate adjacent channel 1
6. Power of lower alternate adjacent channel 2
7. Power of upper alternate adjacent channel 2

The number of results depends on the number of adjacent channels selected with command `SENSe:POWer:ACHannel:ACPairs`.

With logarithmic scaling (RANGE LOG), the power is output in dBm, with linear scaling (RANGE LIN dB or LIN %) in W. If SENSe:POWer:ACHannel:MODE REL is selected, adjacent channel power is output in dB.

CPOWer channel power measurement

With logarithmic scaling (RANGE LOG), the channel power is output in dBm, with linear scaling (RANGE LIN dB or LIN %) in W.

OBANdwidth | OBWidth occupied bandwidth power measurement

The return value is the occupied bandwidth in Hz.

Example of channel/adjacent power measurement:

`"SENS2:POW:ACH:ACP 3"`	Sets the number of adjacent channels in screen B to 3.
`"SENS2:POW:ACH:BAND 30KHZ"`	Sets the bandwidth of the main channel to 30 kHz.
`"SENS2:POW:ACH:BAND:ACH 40KHZ"`	Sets the bandwidth of all adjacent channels to 40 kHz.
`"SENS2:POW:ACH:BAND:ALT1 50KHZ"`	Sets the bandwidth of all alternate adjacent channels to 50 kHz.
`"SENS2:POW:ACH:BAND:ALT2 60KHZ"`	Sets the bandwidth of alternate adjacent channel 2 to 60 kHz.
`"SENS2:POW:ACH:SPAC 30KHZ"`	Sets the spacing between channel to adjacent channel to 30 kHz as well as between channel and alternate adjacent channel to 60 kHz and 2nd alternate adjacent channel to 90 kHz.
`"SENS2:POW:ACH:SPAC:ALT1 100KHZ"`	Sets the spacing between channel and alternate adjacent channel to 100 kHz as well as 2nd alternate adjacent channel to 150 kHz.
`"SENS2:POW:ACH:SPAC:ALT2 140KHZ"`	Sets the spacing between channel and alternate adjacent channel 2 to 140 kHz.

```
"SENS2:POW:ACH:MODE ABS"
```
Switches on the measurement of absolute power values.

```
"CALC2:MARK:FUNC:POW:SEL ACP"
```
Switches the adjacent channel power measurement in screen B.

```
"INIT:CONT OFF"
"INIT;*WAI"
"CALC2:MARK:FUNC:POW:RES? ACP"
```
Switches to single-sweep mode.
Starts a sweep and waits for the end
Queries the result of the adjacent channel power measurement in screen B.

In case of relative measurement, the measured channel power can be defined as the reference power with command.

```
"SENS2:POW:ACH:REF:AUTO ONCE".
```

If only the **channel power** is to be measured, all commands for defining the bandwidths of adjacent channels as well as the channel spacings are not necessary. The number of adjacent channels is set to 0 with `SENS2:POW:ACH:ACP 0`.

Example of occupied bandwidth measurement:

```
"SENS2:POW:BAND 90PCT"
```
Sets the percentage of the power contained in the bandwidth under request to 90%.

```
"INIT:CONT OFF"
```
Switches to single-sweep mode.

```
"INIT;*WAI"
```
Starts a sweep and waits for the end.

```
"CALC2:MARK:FUNC:POW:RES? OBW"
```
Queries the result of the occupied bandwidth in screen B.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

This command is only a query and is therefore not assigned an *RST value.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:POWer:RESult:PHZ ON | OFF

This command switches the query response of the power measurement results in the indicated measurement window between output of absolute values (OFF) and output referred to the measurement bandwith (ON).

The measurement results are output with `CALCulate:MARKer:FUNCtion:POWer:RESult?`

Parameter:

ON: Results output referred to measurement bandwidth.

OFF: Results output in absolute values.

Example of channel/adjacent channel measurement:

`"SENS2:POW:ACH:ACP 3"`	Sets the number of adjacent channels in screen B to 3.
`"SENS2:POW:ACH:BAND 30KHZ"`	Sets the bandwidth of the main channel to 30 kHz.
`"SENS2:POW:ACH:BAND:ACH 40KHZ"`	Sets the bandwidth of all adjacent channels to 40 kHz.
`"SENS2:POW:ACH:BAND:ALT1 50KHZ"`	Sets the bandwidth of all alternate adjacent channels to 50 kHz.
`"SENS2:POW:ACH:BAND:ALT2 60KHZ"`	Sets the bandwidth of alternate adjacent channel 2 to 60 kHz.
`"SENS2:POW:ACH:SPAC 30KHZ"`	Sets the spacing between channel and adjacent channel as well as between all adjacent channels to 30 kHz.
`"SENS2:POW:ACH:SPAC:ALT1 40KHZ"`	Sets the spacing between adjacent channel and alternate adjacent channel as well as between all alternate adjacent channels to 40 kHz.
`"SENS2:POW:ACH:SPAC:ALT2 50KHZ"`	Sets the spacing between alternate adjacent channel 1 and alternate adjacent channel 2 to 50 kHz.
`"SENS2:POW:ACH:MODE ABS"`	Switches on absolute power measurement.
`"CALC2:MARK:FUNC:POW:SEL ACP"`	Switches the adjacent channel power measurement in screen B.
`"INIT:CONT OFF"`	Switches to single-sweep mode.
`"INIT;*WAI"`	Starts a sweep and waits for the end.
`"CALC2:MARK:FUNC:POW:RES:PHZ ON"`	Output of results referred to the channel bandwidth.
`"CALC2:MARK:FUNC:POW:RES? ACP"`	Queries the result of the adjacent channel power measurement in screen B referred to the channel bandwidth.

If only the **channel power** is to be measured, all commands for defining the bandwidths of adjacent channels as well as the channel spacings are not necessary. The number of adjacent channels is set to 0 with `SENS2:POW:ACH:ACP 0`.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:POWer[:STATe] OFF

This command switches off the power measurement in the selected measurement window.

Example: "CALC:MARK:FUNC:POW OFF" Switches off the power measurement in screen B.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

This command is an event and is therefore not assigned an *RST value.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:POWer:PRESet NADC | TETRA | PDC | PHS | CDPD | FWCDma | RWCDma | F8CDma | R8CDma | F19Cdma | R19Cdma | FW3Gppcdma | RW3Gppcdma | D2CDma | S2CDma | M2CDma | FIS95A | RIS95A | FIS95C0 | RIS95C0 | FJ008 | RJ008 | FIS95C1 | RIS95C1 | NONE

This command selects the power measurement setting for a standard in the indicated measurement window and previously switches on the corresponding measurement, if required. The function is independent of the marker selection, ie the suffix <1 to 4> of MARKer is irrelevant.

The configuration for a standard comprises of the parameters weighting filter, channel bandwidth and spacing, resolution and video bandwidth, as well as detector and sweep time.

Meaning of the CDMA standard abbreviations:

FIS95A, F8CDma	CDMA IS95A forward
RIS95A, R8CDma	CDMA IS95A reverse
FJ008, F19CDma	CDMA J-STD008 forward
RJ008, R19CDma	CDMA J-STD008 reverse
FIS95C0	CDMA IS95C Class 0 forward
RIS95C0	CDMA IS95C Class 0 reverse
FIS95C1	CDMA IS95C Class 1 forward
RIS95C1	CDMA IS95C Class 1 reverse
FWCDma	W-CDMA 4.096 MHz forward
RWCDma	W-CDMA 4.096 MHz reverse
FW3Gppcdma	W-CDMA 3.84 MHz forward
RW3Gppcdma	W-CDMA 3.84 MHz reverse
D2CDma	CDMA 2000 direct sequence
S2CDma	CDMA 2000 MC1 multi carrier with 1 carrier
M2CDma	CDMA 2000 MC3 multi carrier with 3 carriers

Note:
The settings for standards IS95A and C differ as far as the calculation method of channel spacings is concerned. For IS95A the spacing is calculated from the center of the main channel to the center of the corresponding adjacent channel, for IS95C from the center of the main channel to the nearest border of the adjacent channel.

Example: "CALC2:MARK:FUNC:POW:PRES NADC" selects the standard setting for NADC in screen B

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

CALCulate:MARKer:FUNCtion:STRack Subsystem

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:MARKer			
:FUNCtion			
:STRack			
[:STATe]	<Boolean>		
:BANDwidth	<numeric_value>	HZ	
:BWIDth	<numeric_value>	HZ	
:THReshold	<numeric_value>	DBM	
:TRACe	<numeric_value>		

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:STRack[:STATe] ON | OFF

This command switches the signal-track function on or off for the the selected measurement window. The function is independent of the selected marker, ie the suffix <1 to 4> of MARKer is irrelevant.

With signal track activated, the maximum signal is determined after each frequency sweep and the center frequency is set to the frequency of this signal. Thus with drifting signals the center frequency follows the signal.

Example: `"CALC:MARK:FUNC:STR ON"` Switches on the signal track function for screen A.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A-F

CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack:BANDwidth 10Hz to MAX(SPAN)
CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack:BWIDth 10Hz to MAX(SPAN)

These commands have the same function. For the selected measurement window they define the bandwidth around the center frequency within which the largest signal is searched. The function is independent of the selected marker, ie the suffix <1 to 4> of MARKer is irrelevant. It is only available in the frequency domain (span > 0).

Note:
The entry of the search bandwidth is only possible if the Signal Track function is switched on (`CALC:MARK:FUNC:STR ON`).

Example: `"CALC:MARK:FUNC:STR:BAND 1MHZ"` Sets the search bandwidth for screen A to 1 MHz.

`"CALC:MARK:FUNC:STR:BWID 1MHZ"` Alternative command for the same function.

Characteristics: *RST value: -- (= span/10 on activating the function)
SCPI: device-specific

Mode: A-F

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:STRack:THReshold -330dBm to +30dBm

This command defines the threshold above which the largest signal is searched for in the selected measurement window. The function is independent of the selected marker, ie the suffix <1 to 4> of MARKer is irrelevant. It is only available in the frequency domain (span > 0).

The response unit depends on the settings defined with `CALC:UNIT`.

Note:
The entry of the search bandwidth is only possible if the Signal Track function is switched on (`CALC:MARK:FUNC:STR ON`).

Example: `"CALC:MARK:FUNC:STR:THR -50DBM"` Sets the threshold for signal tracking in screen A to -50 dBm.

Characteristics: *RST value: -120 dBm
SCPI: device-specific

Mode: A-F

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:STRack:TRACe 1 to 3

This command defines the trace on which the largest signal is searched for in the selected measurement window. The function is independent of the selected marker, ie the suffix <1 to 4> of MARKer is irrelevant. It is only available in the frequency domain (span > 0).

Example: `"CALC2:MARK:FUNC:STR:TRAC 3"` Defines trace 3 in screen B as the trace for signal tracking.

Characteristics: *RST value: 1
SCPI: device-specific

Mode: A-F

CALCulate:MARKer:FUNCtion:SUMMary Subsystem

This subsystem contains the commands for controlling the time domain power functions. These are provided in the marker subsytem for reasons of compatibility with the FSE family.

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:MARKer			
:FUNCtion			
:SUMMary			
[:STATe]	<Boolean>		
:PPEak			
[:STATe]	<Boolean>		
:RESult?			query only
:AVERage			
:RESult?			query only
:PHOLd			
:RESult?			query only
:RMS			
[:STATe]	<Boolean>		
:RESult?			query only
:AVERage			
:RESult?			query only
:PHOLd			
:RESult?			query only
:MEAN			
[:STATe]	<Boolean>		
:RESult?			query only
:AVERage			
:RESult?			query only
:PHOLd			
:RESult?			query only
:SDEViation			
[:STATe]	<Boolean>		
:RESult?			query only
:AVERage			
:RESult?			query only
:PHOLd			
:RESult?			query only
:PHOLd	<Boolean>		
:AVERage	<Boolean>		
:MODE	ABSolute|RELative		
:REFerence			
:AUTO	ONCE		
:AOFF			no query

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary[:STATe] ON | OFF

This command switches on or off the previously selected time domain power measurements. Thus one or several measurements can be first selected and then switched on and off together with `CALC:MARK:FUNC:SUMMary:STATe`.

The function is independent of the marker selection, ie the suffix of MARKer is irrelevant. It is only available in the time domain (span = 0).

Example: `"CALC:MARK:FUNC:SUMM:STAT ON"`

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A-T

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:PPEak[:STATe] ON | OFF

This command switches on or off the measurement of the positive peak value in the selected measurement window.

The function is independent of the marker selection, ie the suffix <1 to 4> of MARKer is irrelevant. It is only available in the time domain (span = 0).

Example: `"CALC:MARK:FUNC:SUMM:PPE ON"` Switches on the function in screen A.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A-T

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:PPEak:RESult?

This command is used to query the result of the measurement of the positive peak value in the selected measurement window. The measurement may have to be switched on previously.

The function is independent of the marker selection, ie the suffix <1 to 4> of MARKer is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

`"INIT:CONT OFF"`	Switches to single-sweep mode.
`"CALC:MARK:FUNC:SUMM:PPE ON"`	Switches on the function in screen A.
`"INIT;*WAI"`	Starts a sweep and waits for the end.
`"CALC:MARK:FUNC:SUMM:PPE:RES?"`	Outputs the result of screen A.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:PPEak:AVERage:RESult?

This command is used to query the result of the measurement of the averaged positive peak value in the selected measurement window. The query is only possible if averaging has been activated previously using `CALCulate<1|2>:MARKer<1 to 4>:FUNCtion: SUMMary:AVERage`.

The function is independent of the marker selection, ie the suffix <1 to 4> in MARKer is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"                          Switches to single-sweep mode.
"CALC:MARK:FUNC:SUMM:PPE ON"             Switches on the function in screen A.
"CALC:MARK:FUNC:SUMM:AVER ON"            Switches on the calculation of average
                                         in screen A.
"INIT;*WAI"                              Starts a sweep and waits for the end.
"CALC:MARK:FUNC:SUMM:PPE:AVER:RES?"      Outputs the result of screen A.
```

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:PPEak:PHOLd:RESult?

This command is used to query the result of the measurement of the positive peak value with active peak hold function. The query is only possible if the peak hold function has been activated previously using `CALCulate<1|2>:MARKer<1 to 4>: FUNCtion:SUMMary:PHOLd`.

The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"                          Switches to single-sweep mode.
"CALC:MARK:FUNC:SUMM:PPE ON"             Switches on the function in screen A.
"CALC:MARK:FUNC:SUMM:PHOL ON"            Switches on the measurement of the
                                         peak value in screen A.
"INIT;*WAI"                              Starts a sweep and waits for the end.
"CALC:MARK:FUNC:SUMM:PPE:PHOL:RES?"      Outputs the result of screen A.
```

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:RMS[:STATe] ON | OFF

This command switches on or off the measurement of the effective (RMS) power in the selected measurement window. If necessary the function is switched on previously.

The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

Example: `"CALC2:MARK:FUNC:SUM:RMS ON"` Switches on the function in screen B.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A-T

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:RMS:RESult?

This command queries the result of the measurement of the RMS power value in the selected measurement window.

The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

`"INIT:CONT OFF"`	Switches to single-sweep mode.
`"CALC:MARK:FUNC:SUMM:RMS ON"`	Switches on the function in screen A.
`"INIT;*WAI"`	Starts a sweep and waits for the end.
`"CALC:MARK:FUNC:SUMM:RMS:RES?"`	Outputs the result of screen A.

Characteristics: *RST- value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:RMS:AVERage:RESult?

This command queries the result of the measurement of the averaged RMS value in the selected measurement window. The query is only possible if averaging has been activated previously using `CALCulate<1|2>:MARKer<1 to 4>:FUNCtion: SUMMary:AVERage`.

The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

`"INIT:CONT OFF"`	Switches to single-sweep mode.
`"CALC:MARK:FUNC:SUMM:RMS ON"`	Switches on the function in screen A.
`"CALC:MARK:FUNC:SUMM:AVER ON"`	Swtiches on the average value calculation in screen A.
`"INIT;*WAI"`	Starts a sweep and waits for the end.
`"CALC:MARK:FUNC:SUMM:RMS:AVER:RES?"`	Outputs the result of screen A.

Characteristics: *RST- value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:RMS:PHOLd:RESult?

This command queries the result of the measurement of the RMS value with active peak hold in the selected measurement window. The query is only possible only if the peak hold function has been activated previously using `CALCulate<1|2>:MARKer<1 to 4>: FUNCtion:SUMMary:PHOLd`.

The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"                    Switches to single-sweep mode.
"CALC:MARK:FUNC:SUMM:RMS ON"       Switches on the function in screen A.
"CALC:MARK:FUNC:SUMM:PHOL ON"      Switches on the peak value
                                   measurement in screen A.
"INIT;*WAI"                        Starts a sweep and waits for the end.
"CALC:MARK:FUNC:SUMM:RMS:PHOL:RES?" Outputs the result of screen A.
```

Characteristics: *RST- value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:MEAN[:STATe] ON | OFF

This command switches on or off the measurement of the mean value in the selected measurement window.

The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

Note: *The measurement is performed on the trace on which marker 1 is positioned. In order to evaluate another trace, marker 1 must be positioned on another trace with* `CALC:MARK:TRAC 1|2|3`.

Example: `"CALC:MARK:FUNC:SUMM:MEAN ON"` Switches on the function in screen A.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A-T

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:MEAN:RESult?

This command queries the result of the measurement of the mean value in the selected measurement window. The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"                    Switches to single-sweep mode.
"CALC:MARK:FUNC:SUMM:MEAN ON"      Switches on the function in screen A.
"INIT;*WAI"                        Starts a sweep and waits for the end.
"CALC:MARK:FUNC:SUMM:MEAN:RES?"    Outputs the result of screen A.
```

Characteristics: *RST- value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:MEAN:AVERage:RESult?

This command queries the result of the measurement of the averaged mean value in the selected measurement window. The query is only possible if averaging has been activated previously using `CALCulate<1|2>:MARKer<1 to 4>:FUNCtion: SUMMary:AVERage`.

The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"                    Switches to single-sweep mode.
"CALC:MARK:FUNC:SUMM:MEAN ON"      Switches on the function in screen A.
"CALC:MARK:FUNC:SUMM:AVER ON"      Switches on the average value
                                   calculation in screen A.
"INIT;*WAI"                        Starts a sweep and waits for the end.
"CALC:MARK:FUNC:SUMM:MEAN:AVER:RES?" Outputs the result of screen A.
```

Characteristics: *RST- value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:MEAN:PHOLd:RESult?

This command queries the result of the measurement of the mean value with active peak hold in the selected measurement window. The query is only possible if the peak hold function has been switched on previously using `CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:PHOLd`.

The query is possible only if the peak hold function is active. The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

`"INIT:CONT OFF"`	Switches to single-sweep mode
`"CALC:MARK:FUNC:SUMM:MEAN ON"`	Switches on the function in screen A
`"CALC:MARK:FUNC:SUMM:PHOL ON"`	Switches on the peak value measurement in screen A
`"INIT;*WAI"`	Starts a sweep and waits for the end
`"CALC:MARK:FUNC:SUMM:MEAN:PHOL:RES?"`	Outputs the result of screen A.

Characteristics: *RST- value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:SDEViation[:STATe] ON | OFF

This command switches on or off the measurement of the standard deviation in the selected measurement window.The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

On switching on the measurement, the mean power measurement is switched on as well.

Example: `"CALC2:MARK:FUNC:SUMM:SDEV ON"` Switches on the measurement of the standard deviation in screen B.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:SDEViation:RESult?

This command queries the results of the standard deviation measurement. The function is independent of the marker selection, ie the suffix <1 to 4> of :MARKer is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"                    Switches to single-sweep mode.
"CALC:MARK:FUNC:SUMM:SDEV ON"      Switches on the function in screen A.
"INIT;*WAI"                        Starts a sweep and waits for the end.
"CALC:MARK:FUNC:SUMM:SDEV:RES?"    Outputs the result of screen A.
```

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:SDEViation:AVERage:RESult?

This command queries the result of the averaged standard deviation determined in several sweeps in the selected measurement window. The query is possible only if averaging is active. The function is independent of the marker selection, ie the suffix <1 to 4> of :MARKer is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"                    Switches to single-sweep mode.
"CALC:MARK:FUNC:SUMM:SDEV ON"      Switches on the function in screen A.
"CALC:MARK:FUNC:SUMM:AVER ON"      Switches on the calculation of average
                                   in screen A.
"INIT;*WAI"                        Starts a sweep and waits for the end.
"CALC:MARK:FUNC:SUMM:MEAN:SDEV:RES?"  Outputs the result of screen A.
```

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:SDEViation:PHOLd:RESult?

This command queries the maximum standard deviation value determined in several sweeps in the selected measurement window. The query is possible only if the peak hold function is active.

The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

A complete sweep with synchronization to sweep end must be performed between switching on the function and querying the measured value to obtain a valid query result. This is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"                    Switches to single-sweep mode.
"CALC:MARK:FUNC:SUMM:SDEV ON"      Switches on the function in screen A.
"CALC:MARK:FUNC:SUMM:PHOL ON"      Switches on the peak value
                                   measurement in screen A.
"INIT;*WAI"                        Starts a sweep and waits for the end.
"CALC:MARK:FUNC:SUMM:SDEV:PHOL:RES?" Outputs the result of screen A.
```

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-T

This command is only a query and thus has no *RST value assigned.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:PHOLd ON | OFF

This command switches on or off the peak-hold function for the active time domain power measurement in the indicated measurement window. The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

The peak-hold function is reset by switching it off and on again.

Example:

```
"CALC:MARK:FUNC:SUMM:PHOL ON"      Switches on the function in screen A.
```

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A-T

The peak-hold function is reset by switching off and on, again.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:AVERage ON | OFF

This command switches on or off averaging for the active time domain power measurement in the indicated window. The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

Averaging is reset by switching it off and on again.

The number of results required for the calculation of average is defined with `[SENSe<1|2>:]AVERage:COUNt`.

It should be noted that synchronization to the end of averaging is only possible in single sweep mode.

Example:

```
"INIT:CONT OFF"                    Switches to single-sweep mode.
"CALC2:MARK:FUNC:SUMM:AVER ON"     Switches on the calculation of average
                                   in screen B.
"AVER:COUN 200"                    Sets the measurement counter to 200.
"INIT;*WAI"                        Starts a sweep and waits for the end.
```

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A-T

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:MODE ABSolute | RELative

This command selects absolute or relative time domain power measurement in the indicated measurement window. The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

The reference power for relative measurement is defined with `CALCulate:MARKer:FUNCtion :SUMMary:REFerence:AUTO ONCE`. If the reference power is not defined, the value 0 dBm is used.

Example:

```
"CALC:MARK:FUNC:SUMM:REF:MODE REL"
                                   Switches the time domain power
                                   measurement to relative.
```

Characteristics: *RST value: ABSolute
SCPI: device-specific

Mode: A-T

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:REFerence:AUTO ONCE

With this command the currently measured average value (`...:SUMMary:MEAN`) and RMS value (`...:SUMMary:RMS`) are declared as reference values for relative measurements in the indicated measurement window. The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

If the measurement of RMS value and average is not activated, the reference value 0 dBm is used.

If the function `...:SUMMary:AVERage` or `...:SUMMary:PHOLd` is switched on, the current value is the accumulated measurement value at the time considered.

Example: `"CALC:MARK:FUNC:SUMM:REF:AUTO ONCE"`
Takes the currently measured power in screen A as reference value for the relative time domain power measurement.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-T

This command is an event and therefore has no *RST value assigned and has no query.

CALCulate<1|2>:MARKer<1 to 4>:FUNCtion:SUMMary:AOFF

This command switches off all time domain measurements in the selected measurement window.The function is independent of the marker selection, ie the suffix `<1 to 4>` of `:MARKer` is irrelevant. It is only available in the time domain (span = 0).

Example: `"CALC2:MARK:FUNC:SUMM:AOFF"` Switches off the time domain power measurement functions in screen B.

Characteristics: *RST value: _
SCPI: device-specific

Mode: A-T

This command is an event and therefore has no *RST value assigned and has no query.

CALCulate:MATH Subsystem

The CALCulate:MATH subsystem allows to process data from the SENSe-subsystem in numeric expressions. The measurement windows are selected by CALCulate1 (screen A) or CALCulate2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2>			
:MATH			
[:EXPRession]			
[:DEFine]	<expr>	--	
:POSition	<numeric_value>	PCT	
:STATe	<Boolean>	--	
:MODE	LINear | LOGarithmic	--	

CALCulate<1|2>:MATH[:EXPression][:DEFine] <expr>

This command defines the mathematical expression for relating traces to trace1.

The zero point of the result display can be defined with `CALC:MATH:POS`. Command `CALCulate:MATH:STATe` switches the mathematical relation of traces on or off .

Parameter: <expr>::= 'OP1 - OP2'
OP1 ::= TRACE1
OP2 ::= TRACE2 | TRACE3

Example: `"CALC1:MATH (TRACE1 - TRACE2)"` Selects the subtraction of trace 1 from trace 2 in screen A.

`"CALC2:MATH (TRACE1 - TRACE3)"` Selects the subtraction of trace 1 from trace 3 in screen B.

Characteristics: *RST value: -
SCPI: conforming

Mode: A

CALCulate<1|2>:MATH:POSition -100PCT to 200PCT

This command defines the position of the result of the trace mathematics in the selected measurement window. The indication is in % of the screen height, with 100% corresponding to the upper diagram border.

Example: `"CALC:MATH:POS 50PCT"` Sets the position in screen A to the horizontal diagram center.

Characteristics: *RST value: 50 %
SCPI: device-specific

Mode: A

CALCulate<1|2>:MATH:STATe ON | OFF

This command switches the mathematical relation of traces on or off.

Example: `"CALC:MATH:STAT ON"` Switches on the trace mathematics in screen A.

Characteristics: *RST value: OFF
SCPI: conforming

Mode: A

CALCulate<1|2>:MATH:MODE LINear | LOGarithmic

This command selects linear or logarithmic (= video) calculation of the mathematical functions related to the traces. The calculation of the average is one of the affected functions. The setting is valid for all measurement windows, ie the suffix `<1|2>` of `CALCulate` is irrelevant.

Example: `"CALC:MATH:MODE LIN"` Switches on the linear calculation.

Characteristics: *RST value: LOG
SCPI: device-specific

Mode: A

CALCulate:STATistics Subsystem

The CALCulate:STATistics subsystem controls the statistical measurement functions in the instrument. The measurement window cannot be selected with these functions. The numeric suffix in CALCulate is therefore ignored.

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate			
:STATistics			
:APD			
[:STATe]	<Boolean>	--	
:CCDF			
[:STATe]	<Boolean>	--	
:NSAMples	<numeric_value>		
:SCALe			
:AUTO	ONCE		
:X			
:RLEVel	<numeric_value>	DBM	
:RANGe	<numeric_value>	DB	
:Y			
:UPPer	<numeric_value>		
:LOWer	<numeric_value>		
:PRESet			
:RESult<1 to 3>?	MEAN | PEAK | CFACtor | ALL		query only

CALCulate:STATistics:APD[:STATe] ON | OFF

This command switches on or off the measurement of amplitude distribution (APD). On activating this function, the CCDF measurement is switched off.

Example: `"CALC:STAT:APD ON"` Switches on the APD measurement.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate:STATistics:CCDF[:STATe] ON | OFF

This command switches on or off the measurement of the complementary cumulative distribution function (CCDF). On activating this function, the APD measurement is switched off.

Example: `"CALC:STAT:CCDF ON"` Switches on the `CCDF` measurement.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate:STATistics:NSAMples 100 to 1E9

This command sets the number of measurement points to be acquired for the statistical measurement functions.

Example: "CALC:STAT:NSAM 500" Sets the number of measurement points to be acquired to 500.

Characteristics: *RST value: 100000
SCPI: device-specific

Mode: A

CALCulate:STATistics:SCALe:AUTO ONCE

This command optimizes the level setting of the FSP depending on the measured peak power, in order to obtain maximum instrument sensitivity.

To obtain maximum resolution, the level range is set as a function of the measured spacing between peak power and the minimum power for the APD measurement and of the spacing between peak power and mean power for the CCDF measurement. In addition, the probability scale for the number of test points is adapted.

Note:
*Subsequent commands have to be synchronized with *WAI, *OPC or *OPC? to the end of the autorange process which would otherwise be aborted.*

Example: "CALC:STAT:SCAL:AUTO ONCE;*WAI" Adapts the level setting for statistical measurements.

Characteristics: *RST value: --
SCPI: device-specific

Mode: A

This command is an event and therefore has no *RST value assigned and has no query.

CALCulate:STATistics:SCALe:X:RLEVel -130dBm to 30dBm

This command defines the reference level for the X-axis of the measurement diagram. The setting is identical to the reference level setting using the command DISPlay:WINDow:TRACe:Y: RLEVel.

With the reference level offset <> 0 the indicated value range of the reference level is modified by the offset.

The unit depends on the setting performed with CALC:UNIT.

Example: "CALC:STAT:SCAL:X:RLEV -60dBm"

Characteristics: *RST value: -20dBm
SCPI: device-specific

Mode: A

CALCulate:STATistics:SCALe:X:RANGe 10dB to 200dB

This command defines the level range for the X-axis of the measurement diagram. The setting is identical to the level range setting defined with the command `DISPlay:WINDow:TRACe:Y:SCALe`.

Example: `"CALC:STAT:SCAL:X:RANG 20dB"`

Characteristics: *RST value: 100dB
SCPI: device-specific

Mode: A

CALCulate:STATistics:SCALe:Y:UPPer 1E-8 to 1.0

This command defines the upper limit for the Y-axis of the diagram in statitistical measurements. Since probabilities are specified on the Y-axis, the entered numerical values are dimensionless.

Example: `"CALC:STAT:Y:UPP 0.01"`

Characteristics: *RST value: 1.0
SCPI: device-specific

Mode: A

CALCulate:STATistics:SCALe:Y:LOWer 1E-9 to 0.1

This command defines the lower limit for th Y-axis of the diagram in statistical measurements. Since probabilities are specified on the Y-axis, the entered numerical values are dimensionless.

Example: `"CALC:STAT:SCAL:Y:LOW 0.001"`

Characteristics: *RST value: 1E-6
SCPI: device-specific

Mode: A

CALCulate:STATistics:PRESet

This command resets the scaling of the X- and Y-axes in a statistical measurement. The following values are set:

X-axis ref level: -20 dBm
X-axis range APD: 100 dB
X-axis range CCDF: 20 dB

Y-axis upper limit: 1.0
Y-axis lower limit: 1E-6

Example: `"CALC:STAT:PRES"` Resets the scaling for statistical functions

Characteristics: *RST value: --
SCPI: device-specific

Mode: A

This command is an event and therefore has no *RST value assigned and has no query.

CALCulate:STATistics:RESult<1 to 3>? MEAN | PEAK | CFACtor | ALL

This command reads out the results of statistical measurements of a recorded trace. The trace is selected with the numeric suffix <1 to 3> attached to RESult.

Parameter: The required result is selected via the following parameters:

MEAN Average (=RMS) power in dBm measured during the measurement time.

PEAK Peak power in dBm measured during the measurement time.

CFACtor Determined CREST factor (= ratio of peak power to average power) in dB.

ALL Results of all three measurements mentioned before, separated by commas:
<mean power>,<peak power>,<crest factor>

Example: `"CALC:STAT:RES2? ALL"` Reads out the three measurement results of trace 2. Example of answer string:
5.56,19.25,13.69
ie mean power: 5.56 dBm, peak power 19.25 dBm, CREST factor 13.69 dB

Characteristics: *RST value: --
SCPI: device-specific

Mode: A

CALCulate:THReshold Subsystem

The CALCulate:THReshold subsystem controls the threshold value for the maximum/minimum search of markers. The measurement windows are selected by CALCulate 1 (screen A) or 2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2> :THReshold :STATe	<numeric_value> <Boolean>	DBM | DB	

CALCulate<1|2>:THReshold MINimum to MAXimum (depending on current unit)

This command defines the threshold value for the maximum/minimum search of markers with marker search functions MAX PEAK, NEXT PEAK, etc. in the selected measurement window. The associated display line is automatically switched on.

Example: `"CALC:THR -82DBM"` Sets the threshold value for screen A to -82 dBm.

Example: `"CALC:THR -82dBm"`

Characteristics: *RST value: - (STATe to OFF)
SCPI: device-specific

Mode: A

CALCulate<1|2>:THReshold:STATe ON | OFF

This command switches on or off the threshold line in the selected measurement window.The unit depends on the setting performed with `CALC:UNIT`.

Example: `"CALC2:THR:STAT ON"` Switches on the threshold line in screen B.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

CALCulate:UNIT Subsystem

The CALCulate:Unit subsystem defines the units for power measurement settings.

COMMAND	PARAMETERS	UNIT	COMMENT
CALCulate<1|2> :UNIT :POWer	DBM | V | A | W | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere		

CALCulate<1|2>:UNIT:POWer DBM | V | A | W | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere

This command selects the unit for power in the selected measurement window.

Example: "CALC:UNIT:POW DBM" Sets the power unit for screen A to dBm.

Characteristics: *RST value: dBm
SCPI: device-specific

Mode: A

CALibration Subsystem

The commands of the CALibration subsystem determine the data for system error correction in the instrument.

COMMAND	PARAMETERS	UNIT	COMMENT
CALibration			
[:ALL]?	--	--	query only
:ABORt	--	--	no query
:RESult?	--	--	query only
:STATe	<Boolean>	--	

CALibration[:ALL]?

This command initiates the acquisition of system error correction data. A "0" is returned if the acquisition was successful.

Note: *During the acquisition of correction data the instrument does not accept any remote control commands, except*
**RST*
CALibration:ABORt

In order to recognize when the acquisition of correction data is completed, the MAV bit in the status byte can be used. If the associated bit is set in the Service Request Enable Register, the instrument generates a service request after the acquisition of correction data has been completed.

Example:

"*CLS"	Resetting the status management.
"*SRE 16"	Enable MAV bit in the Service Request Enable Register.
"*CAL?"	Starts the correction data recording and then a service request is generated.

Characteristics: *RST value: -
SCPI: conforming

Mode: all

CALibration:ABORt

This command aborts the acquisition of correction data and restores the last complete correction data set.

Example: "CAL:ABOR"

Characteristics: *RST value: -
SCPI: device-specific

Mode: all

This command is an event and therefore has no *RST value assigned and has no query.

CALibration:RESult?

This command outputs the results of the correction data acquisition. The lines of the result table (see section "Recording the correction data of FSP – *CAL* key") are output as string data separated by commas:

```
"Total Calibration Status: PASSED","Date (dd/mm/yyyy): 12/07/1999",
"Time: 16:24:54","Runtime:00.06"
```

Example: "CAL:RES?"

Characteristics: *RST value: --
SCPI: device-specific

Mode: all

CALibration:STATe ON | OFF

This command determines whether the current calibration data are taken into account by the instrument (ON) or not (OFF).

Example: "CAL:STAT OFF" Sets up the instrument to ignore the calibration data.

Characteristics: *RST value: -
SCPI: conforming

Mode: all

DIAGnostic Subsystem

The DIAGnostic subsystem contains the commands which support instrument diagnostics for maintenance, service and repair. In accordance with the SCPI standard, all of these commands are device-specific.

COMMAND	PARAMETERS	UNIT	COMMENT
DIAGnostic			
:SERVice			
:INPut			
[:SELect]	CALibration | RF	--	no query
:SFUNCtion	<string>		
:NSOurce	<Boolean>		
:CSOurce			
[:POWer]	<numeric_value>	DBM	
:STESt			
:RESult?			query only

DIAGnostic:SERVice:INPut[:SELect] CALibration | RF

This command toggles between the RF input on the front panel and the internal 128-MHz reference signal. The level of the 128-MHz signals can be selected by command `DIAG:SERV:CSOurce`.

Example: `"DIAG:SERV:INP CAL"`

Characteristics: *RST value: RF
SCPI: device-specific

Mode: all

DIAGnostic:SERVice:SFUNction <string>...

This command activates a service function which can be selected by indicating the five parameters: function group number, board number, function number, parameter 1 and parameter 2 (see service manual). The contents of the parameter string is identical to the code to be entered in the data entry field of manual operation.

The entry of a service function is accepted only if the system password Level 1 or Level 2 has been entered previously (command: `SYSTem:SECurity`).

Note: *The service functions of the FSP family are not identical to those of the FSE family. That is why the IEC/IEEE-bus command differs in syntax and data format.*

Example: `"DIAG:SERV:SFUN '2.0.2.12.1'"`

Characteristics: *RST value: -
SCPI: device-specific

Mode: all

DIAGnostic:SERVice:NSOurce ON | OFF

This command switches the 28-V supply of the noise source at the rear panel on or off.

Example: `"DIAG:SERV:NSO ON"`

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: all

DIAGnostic:SERVice:CSOource[:POWer] <numeric_value>

This command switches the level of the 128 MHz reference signal source between 0 dBm and -30 dBm.

Example: `"DIAG:SERV:CSO 0DBM"`

Characteristics: *RST value: -30 dBm
SCPI: device-specific

Mode: all

DIAGnostic:SERVice:STESt:RESult?

This command reads the results of the selftest out of the instrument. The lines of the result table are output as string data separated by commas:

```
"Total Selftest Status: PASSED","Date (dd/mm/yyyy): 09/07/1999
TIME: 16:24:54","Runtime: 00:06","...
```

Example: `"DIAG:SERV:STES:RES?"`

Characteristics: *RST value: --
SCPI: device-specific

Mode: all

DISPlay Subsystem

The DISPLay subsystem controls the selection and presentation of textual and graphic information as well as of measurement data on the display.
The measurement windows are selected by WINDow1 (screen A) or WINDow2 (screen B) .

COMMAND	PARAMETERS	UNIT	COMMENT
DISPlay			
:FORMat	SINGle|SPLit		
:ANNotation			
:FREQuency	<Boolean>		
:LOGO	<Boolean>		
:PSAVe			
[:STATe]	<Boolean>		
:HOLDoff	1...60	--	
:CMAP<1...26>			
:DEFault<1|2>			
:HSL	0..1,0..1,0..1		
:PDEFined	BLACk | BLUE | BROWn | GREen | CYAN | RED | MAGenta | YELLow | WHITe | DGRAy | LGRAy | LBLUe | LGREen | LCYan | LRED | LMAGenta		
[:WINDow<1|2>]			no query
:SELect			
:TEXT			
[:DATA]	<string>		
:STATe	<Boolean>		
:TIME	<Boolean>		
:TRACe<1...3>			
:X			
[:SCALe]			
:Y			
[:SCALe]	<numeric_value>	DB	
:MODE	ABSolute | RELative		
:RLEVel	<numeric_value>	DBM	
:OFFSet	<numeric_value>	DB	
:RVALue	<numeric_value>	DB	
:RPOSition	<numeric_value>	PCT	
:SPACing	LINear|LOGarithmic	--	
:MODE	WRITe|VIEW|AVERage|MAXHold|MINHold	--	
[:STATe]	<Boolean>	--	

DISPlay:FORMat SINGle | SPLit

This command switches the measurement result display between FULL SCREEN and SPLIT SCREEN. The coupling of settings between screen A and screen B can be selected with the command `INSTrument:COUPle`.
In full-screen display the active measurement window can be selected with `DISPlay:WINDow<1|2>:SELect`.

Example: `"DISP:FORM SPL"` Switches the display to 2 measurement windows.

Characteristics: *RST value: SINGle
SCPI: device-specific

Mode: A

DISPlay:ANNotation:FREQuency ON | OFF

This command switches the X-axis annotation on or off.

Example: `"DISP:ANN:FREQ OFF"`

Characteristics: *RST value: ON
SCPI: conforming

Mode: all

DISPlay:LOGO ON | OFF

This command switches the company logo on the screen on or off.

Example: `"DISP:LOGO OFF"`

Characteristics: *RST value: ON
SCPI: device-specific

Mode: all

DISPlay:PSAVe[:STATe] ON | OFF

This command switches on or off the power-save mode of the display. With the power-save mode activated the display including backlight is completely switched off after the elapse of the response time (see command `DISPlay:PSAVe:HOLDoff`).

Note: *This mode is recommended for preserving the display especially if the instrument is exclusively operated via remote control.*

Example: `"DISP:PSAVe ON"` Switches on the power-save mode.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: all

DISPlay:PSAVe:HOLDoff 1 to 60

This command sets the holdoff time for the power-save mode of the display. The available value range is 1 to 60 minutes, the resolution 1 minute. The entry is dimensionless.

Example: `"DISP:PSAV:HOLD 30"`

Characteristics: *RST value: 15
SCPI: device-specific

Mode: all

DISPlay:CMAP<1 to 26>:DEFault<1|2>

This command resets the screen colors of all display items to their default settings. Two default settings DEFault1 and DEFault2 are available. The numeric suffix of CMAP is irrelevant.

Example: "DISP:CMAP:DEF2" Selects default setting 2 for setting the colors.

Characteristics: *RST value: --
SCPI: conforming

Mode: all

This command is an event and is therefore not assigned a query and has no *RST value.

DISPlay:CMAP<1 to 26>:HSL <hue>,<sat>,<lum>

This command defines the color table of the instrument.

Each numeric suffix of CMAP is assigned one or several graphical elements which can be modified by varying the corresponding color setting. The following assignment applies:

CMAP1 Background
CMAP2 Grid
CMAP3 Function field + status field + data entry text
CMAP4 Function field LED on
CMAP5 Function field LED warn
CMAP6 Enhancement label text
CMAP7 Status field background
CMAP8 Trace 1
CMAP9 Trace 2
CMAP10 Trace 3
CMAP11 Marker
CMAP12 Lines
CMAP13 Measurement status + limit check pass
CMAP14 Limit check fail
CMAP15 Table + softkey background
CMAP16 Table + softkey text
CMAP17 Table selected field text
CMAP18 Table selected field background
CMAP19 Table + data entry field opaq titlebar
CMAP20 Data entry field opaq text
CMAP21 Data entry field opaq background
CMAP22 3D shade bright part
CMAP23 3D shade dark part
CMAP24 Softkey state on
CMAP25 Softkey state data entry
CMAP26 Logo

Parameter: hue = TINT

sat = SATURATION

lum = BRIGHTNESS

The value range is 0 to 1 for all parameters.

Example: "DISP:CMAP2:HSL 0.3,0.8,1.0" Changes the grid color.

Characteristics: *RST value: --
SCPI: conforming

Mode: all

The values set are not changed by *RST.

DISPlay:CMAP<1 to 26>:PDEFined BLACk | BLUE | BROWn | GREen | CYAN | RED | MAGenta | YELLow | WHITe | DGRAy | LGRAy | LBLUe | LGREen | LCYan | LRED | LMAGenta

This command defines the color table of the instrument using predefined color values. Each numeric suffix of CMAP is assigned one or several graphical elements which can be modified by varying the corresponding color setting.
The same assignment as for `DISPlay:CMAP<1 to 26>:HSL` applies.

Example: `"DISP:CMAP2:PDEF GRE"`

Characteristics: *RST value: --
SCPI: conforming

Mode: all

The values set are not changed by *RST.

DISPlay[:WINDow<1|2>]:SELect

This command selects the active measurement window. WINDow1 corresponds to SCREEN A, WINDow2 to SCREEN B.
In FULL SCREEN mode, the measurements are only performed in the active measurement window. Measurements are therefore initiated in the active window and result queries (marker, trace data and other results) answered also in the active window.
Initiating measurements and querying results in the inactive window yields an error message (execution error).

In split screen mode, the selection of the active window for result queries is irrelevant.

Note: *In FULL SCREEN mode, settings can also be performed in the inactive measurement window. They become effective as soon as the corresponding window becomes active.*

Example: `"DISP:WIND2:SEL` Selects SCREEN B as active measurement window.

Characteristics: *RST value: SCREEN A active
SCPI: device-specific

Mode: A

This command is an event and is therefore not assigned a query.

DISPlay[:WINDow<1|2>]:TEXT[:DATA] <string>

This command defines a comment (max. 20 characters) which can be displayed on the screen in the selected measurement window.

Example: `"DISP:WIND2:TEXT 'Noise Measurement'"`
Defines the title for screen B

Characteristics: *RST value: "" (empty)
SCPI: conforming

Mode: all

DISPlay[:WINDow<1|2>]:TEXT:STATe ON | OFF

This command switches on or off the display of the comment (screen title) in the selected measurement window.

Example: "DISP:TEXT:STAT ON" Switches on the title of screen B.

Characteristics: *RST value: OFF
SCPI: conforming

Mode: all

DISPlay[:WINDow<1|2>]:TIME ON | OFF

This command switches on or off the screen display of date and time. The numeric suffix in WINDow<1| 2> is irrelevant.

Example: "DISP:TIME ON"

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: all

DISPlay[:WINDow<1|2>]:TRACe<1 to 3>:Y[:SCALe] 10dB to 200dB

This command defines the display range of the Y-axis (level axis) in the selected measurement window with logarithmic scaling (DISP:TRAC:Y:SPAC LOG).

For linear scaling, (DISP:TRAC:Y:SPAC LIN | PERC) the display range is fixed and cannot be modified. The numeric suffix in TRACe<1 to 3> is irrelevant.

Example: "DISP:TRAC:Y 110dB"

Characteristics: *RST value: 100dB
SCPI: device-specific

Mode: A

DISPlay[:WINDow<1|2>]:TRACe<1 to 3>:Y[:SCALe]:MODE ABSolute | RELative

This command defines the scale type of the Y-axis (absolute or relative) in the selected measurement window.

When SYSTem:DISPlay is set to OFF, this command has no immediate effect on the screen. The numeric suffix in TRACe<1 to 3> is irrelevant.

Example: "DISP:TRAC:Y:MODE REL"

Characteristics: *RST value: ABS
SCPI: device-specific

Mode: A

DISPlay[:WINDow<1|2>]:TRACe<1 to 3>:Y[:SCALe]:RLEVel -130dBm to 30dBm

This command defines the reference level in the selected measurement window. Depending on the coupling of the measurement windows, it is valid for both screens (`INSTrument:COUPle ALL`) or only for the selected measurement window (`INSTrument:COUPle NONE`).

With the reference level offset <> 0 the indicated value range of the reference level is modified by the offset.

The unit depends on the setting defined with `CALCulate:UNIT`. The numeric suffix in TRACe<1 to 3> is irrelevant.

Example: `"DISP:TRAC:Y:RLEV -60dBm"`

Characteristics: *RST value: -20dBm
SCPI: conforming

Mode: A

DISPlay[:WINDow<1|2>]:TRACe<1 to 3>:Y[:SCALe]:RLEVel:OFFSet -200dB to 200dB

This command defines the offset of the reference level in the selected measurement window. Depending on the coupling of the measurement windows, it is valid for both screens (`INSTrument:COUPle ALL`) or only for the selected measurement window (`INSTrument:COUPle NONE`).

The numeric suffix at TRACe<1 to 3> is irrelevant.

Example: `"DISP:TRAC:Y:RLEV:OFFS -10dB"`

Characteristics: *RST value: 0dB
SCPI: conforming

Mode: A

DISPlay[:WINDow<1|2>]:TRACE<1 to 3>:Y[:SCALe]:RVALue <numeric_value>

If the tracking generator option or the external generator control option (FSP-B9/B10) is mounted and the normalization in the NETWORK mode is activated, this value defines the power value assigned to the reference position in the selected measurement window. This value corresponds to the parameter REFERENCE VALUE in manual operation.

The numeric suffix at TRACe<1 to 3> is irrelevant.

Example:

`"DISP:TRAC:Y:RVAL 0"` sets the power value assigned to the reference position to 0 dB.

Characteristics: *RST value:
0 dB
SCPI: device specific

Modes: A

DISPlay[:WINDow<1|2>]:TRACe<1 to 3>:Y[:SCALe]:RPOSition 0 to 100PCT

This command defines the position of the reference value in the selected measurement window. The numeric suffix in TRACe<1 to 3> is irrelevant.

In operating mode NETWORK (Tracking Generator /Ext. Generator Option FSP-B9/B10) with active normalization, RPOSition defines the reference point for the output of the normalized measurement results.

Example: `"DISP:TRAC:Y:RPOS 50PCT"`

Characteristics: *RST value: 100PCT
SCPI: conforming

Mode: A

DISPlay[:WINDow<1|2>]:TRACe<1 to 3>:Y:SPACing LINear | LOGarithmic

This command toggles between linear and logarithmic display in the selected measurement window.

The numeric suffix in TRACe<1 to 3> is irrelevant.

Example: `"DISP:TRAC:Y:SPAC LIN"`

Characteristics: *RST value: LOGarithmic
SCPI: conforming

Mode: A

DISPlay[:WINDow<1|2>]:TRACe<1 to 3>:MODE WRITe | VIEW | AVERage | MAXHold | MINHold

This command defines the type of display and the evaluation of the traces in the selected measurement window. WRITE corresponds to the Clr/Write mode of manual operation. The trace is switched off (= BLANK in manual operation) with `DISP:WIND:TRAC:STAT OFF`.

The number of measurements for AVERage, MAXHold and MINHold is defined with the command `SENSe:AVERage:COUNt` or `SENSe:SWEep:COUNt`. It should be noted that synchronization to the end of the indicated number of measurements is only possible in single sweep mode.

If calculation of average values is active, selection between logarithmic and linear averaging is possible. For more detail see command `SENSe:AVERage:TYPE`.

Example:

`"SWE:CONT OFF"`	Switching to single-sweep mode.
`"SWE:COUN 16"`	Sets the number of measurements to 16.
`"DISP:WIND1:TRAC3:MODE MAXH"`	Switches on the calculation of the for trace 3 in screen A.
`"INIT;*WAI"`	Starts the measurement and waits for the end of the 16 sweeps.

Characteristics: *RST value: WRITe for TRACe1, STATe OFF for TRACe2/3
SCPI: device-specific

Mode: all

DISPlay[:WINDow<1|2>]:TRACE<1 to 3>[:STATe] ON | OFF

This command switches on or off the display of the corresponding trace in the selected measurement window.

Example: "DISP:WIND1:TRAC3 ON"

Characteristics: *RST value: ON for TRACe1, OFF for TRACe2 to 4
SCPI: conforming

Mode: all

FORMat Subsystem

The FORMat subsystem specifies the data format of the data transmitted from and to the instrument.

COMMAND	PARAMETERS	UNIT	COMMENT
FORMat [:DATA] :DEXPort :DSEParator	 ASCii|REAL[,<numeric_value>] POINt|COMMa	 - 	

FORMat[:DATA] ASCii | REAL [, 32]

This command specifies the data format for the data transmitted from the instrument to the control PC.

Example: `"FORM REAL,32"`
`"FORM ASC"`

Characteristics: *RST value: ASCII
SCPI: conforming

Mode: all

The data format is either ASCii or one of the formats REAL . ASCii data are transmitted in plain text, separated by commas. REAL data are transmitted as 32-bit IEEE 754 floating-point numbers in the "definite length block format".

The FORMat command is valid for the transmission of trace data. The data format of trace data received by the instrument is automatically recognized, regardless of the format which is programmed.

Format setting for the binary transmission of trace data (see also `TRACE:DATA?`):

Analyzer mode: REAL, 32

FORMat:DEXPort:DSEParator POINt|COMMA

This command defines which decimal separator (decimal point or comma) is to be used for outputting measurement data to the file in ASCII format. Different languages of evaluation programs (eg MS-Excel) can thus be supported.

Example: `"FORM:DEXP:DSEP POIN` Sets the decimal point as separator.

Characteristics: *RST value: -- (factory setting is POINt; *RST does not affect setting)
SCPI: device-specific

Mode: all

HCOPy Subsystem

The HCOPy subsystem controls the output of display information for documentation purposes on output devices or files. The instrument allows two independent printer configurations which can be set separately with the numeric suffix <1|2>.

COMMAND	PARAMETERS	UNIT	COMMENT
HCOPy			
:ABORt	--	--	no query
:DESTination<1|2>	<string>		no query
:DEVice			
:COLor	<Boolean>		
:LANGuage<1|2>	WMF|GDI|EWMF|BMP		
[:IMMediate<1|2>]	--	--	no query
:ITEM			
:ALL			no query
:WINDow<1|2>			
:TABle			
:STATe	<Boolean>		
:TEXT	<string>		
:TRACe			
:STATe	<Boolean>		
:PAGE			
:ORIentation<1|2>	LANDscape|PORTrait		

HCOPy:ABORt

This command aborts a running hardcopy output.

Example: `"HCOP:ABOR"`

Characteristics: *RST value: -
SCPI: conforming

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

HCOPy:DESTination<1|2> <string>

This command selects the printer output medium (Disk, Printer or Clipboard) associated with configuration 1 or 2.

Note: *The type of instrument is selected with* `SYSTem:COMMunicate:PRINter:SELect`*, which will automatically select a default output medium. Therefore the command* `HCOPy:DESTination` *should always be sent after setting the device type.*

Parameter:

<string>::=	`'MMEM' | 'SYST:COMM:PRIN' | 'SYST:COMM:CLIP'`
`'MMEM'`	directs the hardcopy to a file. Command `MMEM:NAME <file_name>` defines the file name. All formats can be selected for `HCOPy:DEVice:LANGuage`.
`'SYST:COMM:PRIN'`	directs the hardcopy to the printer. The printer is selected with command `SYSTEM:COMMunicate:PRINter:SELect`. `GDI` should be selected for `HCOPy:DEVice:LANGuage`.
`'SYST:COMM:CLIP'`	directs the hardcopy to the clipboard. `EWMF` should be selected for `HCOPy:DEVice:LANGuage`.

Example:

`"SYST:COMM:PRIN:SEL2 'LASER on LPT1'"`	Selects the printer and output medium for device 2
`"HCOP:DEST2 'SYST:COMM:PRIN'"`	Selects the printer interface as device 2.

Characteristics: *RST value: -
SCPI: conforming

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

HCOPy:DEVice:COLor ON|OFF

This command selects between color and monochrome hardcopy of the screen.

Example: `"HCOP:DEV:COL ON"`

Characteristics: *RST value: OFF
SCPI: conforming

Mode: all

HCOPy:DEVice:LANGuage<1|2> GDI | WMF | EWMF | BMP

This command determines the data format of the printout.

Parameter:

GDI — Graphics Device Interface:
Default format for the output to a printer configured under Windows. Must be selected for the output to the printer interface (`HCOPy:DEVice 'SYST:COMM:PRIN'`).
Can be used for the output to a file (`HCOPy:DEVice 'SYST:COMM:MMEM'`). The printer driver configured under Windows is used in this case and a printer-specific file format is thus generated.

WMF and EWMF — WINDOWS Metafile and Enhanced Metafile Format:
Data formats for output files which can be integrated in corresponding programs for documentation purposes at a later time. WMF can only be used for output to a file (`HCOPy:DEVice 'SYST:COMM:MMEM'`) and EWMF also for the output to the clipboard (`HCOPy:DEVice 'SYST:COMM:CLIP'`).

BMP — Bitmap.
Data format for output to files only (`HCOPy:DEVice 'SYST:COMM:MMEM'`).

Example: `"HCOP:DEV:LANG WMF"`

Characteristics: *RST value: -
SCPI: conforming

Mode: all

HCOPy[:IMMediate<1|2>]

This command starts a hardcopy output. The numeric suffix selects which printer configuration (1 or 2) is to be used for the hardcopy output. If there is no suffix, configuration 1 is automatically selected.

`HCOPy:IMM[1]` Starts the hardcopy output to device 1 (default).
`HCOPy:IMM2` Starts the output to device 2.

Example: `"HCOP"`

Characteristics: *RST value: -
SCPI: conforming

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

HCOPy:ITEM:ALL

This command selects the complete screen to be output.

Example: `"HCOP:ITEM:ALL"`

Characteristics: *RST value: OFF
SCPI: conforming

Mode: all

The hardcopy output is always provided with comments, title, time and date. As an alternative to the whole screen, only traces (commands `'HCOPy:DEVice:WINDow:TRACe: STATe ON'`) or tables (command `'HCOPy:DEVice:WINDow:TABLe:STATe ON'`) can be output.

HCOPy:ITEM:WINDow<1|2>:TABle:STATe ON | OFF

This command selects the output of the currently displayed tables.

Example: `"HCOP:ITEM:WIND:TABL:STAT ON"`

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: all

The command `HCOPy:DEVice:ITEM:WINDow<1|2>:TABle:STATe OFF` as well as command `HCOPy:DEVice:ITEM:ALL` enables the output of the whole screen.

HCOPy:ITEM:WINDow<1|2>:TEXT <string>

This command defines the comment text for measurement window 1 or 2 for printout, with a maximum of 100 characters; line feed by means of character @).

Example: `"HCOP:ITEM:WIND2:TEXT 'comment'"`

Characteristics: *RST value: -
SCPI: device-specific

Mode: all

HCOPy:ITEM:WINDow<1|2>:TRACe:STATe ON | OFF

This command selects the output of the currently displayed trace.

Example: `"HCOP:ITEM:WIND:TRACe:STAT ON"`

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: all

The command `HCOPy:ITEM:WINDow<1|2>:TRACe:STATe OFF` as well as command `HCOPy:ITEM:ALL` enables the output of the whole screen.

HCOPy:PAGE:ORIentation<1|2> LANDscape | PORTrait

The command selects the format of the output (portrait and landscape) (hardcopy unit 1 or 2).

Note:
The command is only available provided that the output device "printer" `(HCOP:DEST 'SYST:COMM:PRIN')` *has been selected.*

Example: `"HCOP:PAGE:ORI LAND"`

Characteristics: *RST value: -
SCPI: conforming

Mode: all

INITiate Subsystem

The INITiate subsystem is used to control the init-measurement function in the selected measurement window. The measurement windows are assigned to INITiate1 (screen A) and INITiate2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
INITiate<1|2>			
:CONTinuous	<boolean>	--	
:CONMeas	--	--	no query
[:IMMediate]	--	--	no query
:DISPlay	<boolean>	--	

INITiate<1|2>:CONTinuous ON | OFF

This command determines whether the trigger system is continuously initiated (continuous) or performs single measurements (single). In the spectrum analysis mode, this setting refers to the sweep sequence (switching between continuous/single sweep).

Example: `"INIT2:CONT OFF"` Switches the sequence in screen B to single sweep.

`"INIT2:CONT ON"` Switches the sequence to continuous sweep.

Characteristics: *RST value: ON
SCPI: conforming

Mode: all

INITiate<1|2>:CONMeas

This command continues a stopped measurement at the current position in single sweep mode. The function is useful especially for trace functions MAXHold, MINHold and AVERage if the previous results are not to be cleared with Sweep Count > 0 or Average Count > 0 on restarting the measurement (INIT:IMMediate resets the previous results on restarting the measurement).

The single-sweep mode is automatically switched on. Synchronization to the end of the indicated number of measurements can then be performed with the command *OPC, *OPC? or *WAI. In the continuous-sweep mode, synchronization to the sweep end is not possible since the overall measurement "never" ends.

Example:

```
"INIT:CONT OFF"                 Switches to single-sweep mode.
"DISP:WIND:TRAC:MODE AVER       Switches on trace averaging.
"SWE:COUN 20"                   Setting the sweep counter to 20 sweeps.
"INIT;*WAI"                     Starts the measurement and waits for the
                                end of the 20 sweeps.
"INIT:CONM;*WAI"                Continues the measurement (next 20
                                sequences) and waits for the end.
```

Characteristics: *RST value: -
SCPI: device-specific

Mode: all

This command is an event and therefore has no *RST value and has no query.

INITiate<1|2>[:IMMediate]

The command initiates a new sweep in the indicated measurement window. With Sweep Count > 0 or Average Count > 0, this means a restart of the indicated number of measurements. With trace functions MAXHold, MINHold and AVERage, the previous results are reset on restarting the measurement.

In single sweep mode, synchronization to the end of the indicated number of measurements can be achieved with the command *OPC, *OPC? or *WAI. In continuous-sweep mode, synchronization to the sweep end is not possible since the overall measurement never ends.

Example:

```
"INIT:CONT OFF"          Switches to single-sweep mode.
"DISP:WIND:TRAC:MODE AVER Switches on trace averaging.
"SWE:COUN 20"            Setting the sweep counter to 20 sweeps.
"INIT;*WAI"              Starts the measurement and waits for the
                         end of the 20 sweeps.
```

Characteristics: *RST value: -
SCPI: conforming

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

INITiate<1|2>:DISPlay ON | OFF

This command configures the behavior of the display during a single sweep.
`INITiate:DISPlay OFF` means that the display is switched off during the measurement,
`INITiate:DISPlay ON` means that the display is switched on during the measurement.
The numeric suffix of INITiate is irrelevant with this command.

Example:

```
"INIT:CONT OFF"          Switches to single-sweep mode
"INIT:DISP OFF           Sets the display behavior to OFF
"INIT;*WAI"              Starts the measurement with display
                         switched off.
```

Characteristics: *RST value: ON
SCPI: device-specific

Mode: A

INPut Subsystem

The INPut subsystem controls the input characteristics of the RF inputs of the instrument. The measurement windows are assigned to INPut1 (screen A) and INPut2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
INPut<1|2>			
:ATTenuation	<numeric_value>	DB	
:AUTO	<Boolean>	--	
:EATT	<numeric_value>	DB	Only with option FSP-B25
:AUTO	<Boolean>	--	Only with option FSP-B25
:STATe	<Boolean>	--	Only with option FSP-B25
:IMPedance	50 | 75	OHM	
:GAIN			
:STATe	<Boolean>		Only with option FSP-B25

INPut<1|2>:ATTenuation 0 to 70/75 dB

This command programs the input attenuator. To protect the input mixer against damage from overloads, the setting 0 dB can be obtained by entering numerals, not by using the command DEC.

The step width is 10 dB without the option electronic attenuator, the range 0 dB to 70 dB.
The input attenuation can be set in 5 dB steps between 0 dB and 75 dB with the option electronic attenuator.

In the default state, the attenuation set on the step attenuator is coupled to the reference level of the instrument. If the attenuation is programmed directly, the coupling to the reference level is switched off.

Example: `"INP:ATT 40dB"` Sets the attenuation on the attenuator to 40 dB and switches off the coupling to the reference level.

Characteristics: *RST value: 10 dB (AUTO is set to ON)
SCPI: conforming

Mode: all

INPut<1|2>:ATTenuation:AUTO ON | OFF

This command automatically couples the input attenuation to the reference level (state ON) or switches the input attenuation to manual entry (state OFF). The minimum input attenuation set with the coupling switched on is 10 dB (with electronic attenuator option: 5 dB).

Example: `"INP:ATT:AUTO ON"` Couples the attenuation set on the attenuator to the reference level.

Characteristics: *RST value: ON
SCPI: conforming

Mode: all

INPut<1|2>:EATT 0 to 30dB

This command programs the attenuation of the electronic input attenuator. The attenuation can be varied in 5 dB steps from 0 to 30 dB. Other entries are rounded to the next lower integer value. If the attenuation is programmed directly, the coupling to the reference level is switched off.

If the defined reference level cannot be set with the given RF attenuation, this level is adapted to the maximum possible value.

The electronic attenuator is swiched off in the default state.

Example: `"INP:EATT:STAT ON"` Switches the electronic attenuator into the signal path.

`"INP:EATT 15dB"` Sets the attenuation of the electronic attenuator to 15 dB and switches off the coupling to the reference level.

Characteristics: *RST value: 0 dB (state is set to OFF)
SCPI: device-specific

Mode: all

The command is only available with the electronic attenuator option FSP-B25.

INPut<1|2>:EATT:AUTO ON | OFF

This command automatically couples the electronic input attenuation to the reference level and the attenuation of the mechanical attenuator (state ON) or switches the input attenuation to manual entry (state OFF).

Example: `"INP:EATT:STAT ON"` Switches the electronic attenuator into the signal path.

Example: `"INP:EATT:AUTO ON"` Couples the attenuation of the electronic attenuator to the reference level.

Characteristics: *RST value: ON
SCPI: device-specific

Mode: all

The command is only available with the electronic attenuator option FSP-B25.

INPut<1|2>:EATT:STATe ON | OFF

This command switches the electronic input attenuation into the signal path (state ON) or removes it from the signal path (state OFF).

Example: "INP:EATT:STAT ON" Switches the electronic attenuator into the signal path.

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: all

The command is only available with the option electronic attenuator FSP-B25.

INPut<1|2>:IMPedance 50 | 75

This command sets the nominal input impedance of the instrument. The set impedance is taken into account in all level indications of results.

The setting 75 Ω should be selected, if the 50 Ω input impedance is transformed to a higher impedance using a 75 Ω adapter of the RAZ type (= 25 Ω in series to the input impedance of the analyzer). The correction value in this case is 1.76 dB = 10 log (75Ω / 50Ω).

Example: `"INP:IMP 75"`

Characteristics: *RST value: 50
SCPI: conforming

Mode: all

INPut<1|2>:GAIN:STATe ON | OFF

This command switches on the preamplifier for the instrument. The switchable gain is fixed to 20 dB.

Example: `"INP:GAIN ON"`

Characteristics: *RST value: OFF
SCPI: conforming

Modes: A

The command is only available with the option electronic attenuator FSP-B25.

INSTrument Subsystem

COMMAND	PARAMETERS	UNIT	COMMENT
INSTrument			
[:SELect]	SANalyzer		
:NSELect	<numeric_value>		no query
:COUPle	NONE | RLEVel | CF_B | CF_A		

INSTrument[:SELect] SANalyzer

This command switches between the operating modes by means of text parameters.

Parameter: SANalyzer: Spectrum analysis

Example: `"INST SAN"` Switches the instrument to spectrum analyzer mode.

Characteristics: *RST value: SANalyzer
SCPI: conforming

Mode: all

INSTrument:NSELect 1

This command switches between the operating modes by means of numbers.

Example: `"INST:NSEL 1"` Switches the instrument to spectrum analyzer mode.

Characteristics: *RST value: 1
SCPI: conforming

Mode: all

INSTrument:COUPle NONE | RLEVel | CF_B | CF_A

In operating mode *SPECTRUM* this command selects the parameter coupling between the two measurement windows screen A and B.

Parameter:	NONE	No coupling. The two measurement windows are operated like two independent "virtual" devices.
	RLEVel	The reference levels of the two measurement windows are coupled.
	CF_B	The center frequency of screen B is coupled to the frequency of marker 1 in screen A.
	CF_A	The center frequency of screen A is coupled to the frequency of marker 1 in screen B.
Example:	`"INST:COUP NONE"`	Switches off the coupling of measurement windows. This leads to two independent "virtual" devices.
Characteristics:	*RST value:	NONE
	SCPI:	device specific
Mode:	A	

MMEMory Subsystem

The MMEMory (mass memory) subsystem provides commands which allow for access to the storage media of the instrument and for storing and loading various instrument settings.

The various drives can be addressed via the "mass storage unit specifier" <msus> using the conventional DOS syntax. The internal hard disk is addressed by "D:", the floppy-disk drive by "A:".

***Note**: For reasons of compatibility with the FSE instruments, addressing the hard disk by "C:" is also accepted. Since hard disk "C:" is reserved for instrument software in the FSP, all read and write operations are rerouted to hard disk "D:" in normal operation (service level0).*

The file names <file_name> are indicated as string parameters with the commands being enclosed in quotation marks. They also comply with DOS conventions.

DOS file names consist of max. 8 ASCII characters and an extension of up to three characters separated from the file name by a dot "." Both, the dot and the extension are optional. The dot is not part of the file name. DOS file names do not distinguish between uppercase and lowercase notation. All letters and digits are permitted as well as the special characters "_", "^", "$", "~", "!", "#", "%", "&", "-", "{", "}", "(", ")", "@" and "`". Reserved file names are CLOCK$, CON, AUX, COM1 to COM4, LPT1 to LPT3, NUL and PRN.

The two characters "*" and "?" have the function of so-called "wildcards", i.e., they are variables for selection of several files. The question mark "?" replaces exactly one character, the asterisk means any of the remaining characters in the file name. "*.*" thus means all files in a directory.

COMMAND	PARAMETERS	UNIT	COMMENT
MMEMory			
:CATalog?	<string>		
:CDIRectory	<directory_name>	--	
:COPY	<file_name>,<file_name>	--	no query
:DATA	<file_name>[,<block>]	--	
:DELete	<file_name>	--	no query
:INITialize	<msus>	--	no query
:LOAD			
:STATe	1,<file_name>	--	no query
:AUTO	1,<file_name>	--	no query
:MDIRectory	<directory_name>	--	no query
:MOVE	<file_name>,<file_name>	--	no query e
:MSIS	<msus>	--	
:NAME	<file_name>	--	
:RDIRectory	<directory_name>	--	no query
:STORe<1|2>			
:STATe	1,<file_name>	--	no query
:TRACe	<numeric_value>, <file_name>		
:CLEar			
:STATe	1,<file_name>	--	no query
:ALL			k no query
:SELect			
[:ITEM]			
:HWSettings	<Boolean>		
:TRACe			
[:ACTive]	<Boolean>		
:LINes			
:ALL	<Boolean>		
:SCData	<Boolean>		Tracking generator option
:ALL	--		no query
:NONE	--		no query
:DEFault	--		no query
:COMMent	<string>		

MMEMory:CATalog? <path>

This command reads the indicated directory. According to DOS convention, wild card characters can be entered in order to query eg a list of all files of a certain type.

The path name should be in conformance with DOS conventions and may also include the drive name.

Parameter: <path>::= DOS Path name

Example:

`"MMEM:CAT? 'D:\USER\DATA'` Returns the contents of the D:\USER\DATA directory

`"MMEM:CAT? 'D:\USER\DATA\*.LOG'` Returns all files in D:\USER\DATA with extension ".LOG"

`"MMEM:CAT? 'D:\USER\DATA\SPOOL?.WMF'`
Returns all files in D:\USER\DATA whose names start with SPOOL, have 6 letters and the extension ".WMF".

Response value: List of file names in the form of strings separated by commas, ie
`'SPOOL1.WMF','SPOOL2.WMF','SPOOL3.WMF'`

Characteristics: *RST value: -
SCPI: conformal

Operating mode: all

MMEMory:CDIRectory <directory_name>

This command changes the current directory.

In addition to the path name, the indication of the directory may contain the drive name. The path name complies with the DOS conventions.

Parameter: <directory_name>::= DOS path name

Example: "MMEM:CDIR 'D:\USER\DATA'" Returns the list of files in directory D:\USER\DATA.

Characteristics: *RST value: -
SCPI: conforming

Mode: all

MMEMory:COPY <file_source>,<file_destination>

This command copies the files indicated in <file_source> to the destination directory indicated with <file_destination> or to the destination file indicated by <file_destination> when <file_source> is just a file.

The indication of the file name may include the path and the drive name. The file names and path information must be in accordance with the DOS conventions.

Parameter: <file_source>,<file_destination> ::= <file_name>
<file_name> ::= DOS file name

Example: "MMEM:COPY 'D:\USER\DATA\SETUP.CFG','A:'"

Characteristics: *RST value: -
SCPI conforming

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:DATA <file_name>[,<block data>]

This command writes the block data contained in <block> into the file characterized by <file_name>. The IEC/IEEE-bus delimiter must be set to EOI to obtain error-free data transfer.

The associated query command reads the indicated file from the mass memory and transfers it to the control computer via the IEC/IEEE bus. It should be noted that the buffer memory of the control computer should be large enough to store the file. The setting of the IEC/IEEE-bus delimiter is irrelevant in this case.

The command is useful for reading stored device settings or trace data from the instrument or for transferring them to the instrument.

Syntax:

MMEMory:DATA <file_name>,<block data>	Data transfer from control computer to instrument.
MMEMory:DATA? <file_name>	Data transfer from instrument to control computer.

<file_name> selects the file to be transferred.

The binary data block <block> has the following structure:

- it always begins with the character '#',
- followed by a digit for the length of the length information,
- followed by the indicated number of digits as length information (number of bytes) for the binary data themselves,
- finally the binary data with the indicated number of bytes

Example:

`"MMEM:DATA 'TEST01.HCP', #217This is the file"`	means: #2: the next 2 characters are the length indication 17: number of subsequent binary data bytes This is the file: 17 bytes stored as binary data in the file TEST01.HCP.
`"MMEM:DATA? 'TEST01.HCP'"`	Transfers the file TEST01.HCP from the instrument to the control computer.

Characteristics:

*RST value:	-
SCPI:	conforming

Mode: all

MMEMory:DELete <file_name>

This command deletes the indicated files.

The indication of the file name contains the path and, optionally, the drive name. Indication of the path complies with DOS conventions.

Parameter: <file_name> ::= DOS file name

Example: "MMEM:DEL 'TEST01.HCP'" The file TEST01.HCP is deleted.

Characteristics: *RST value: -
SCPI: conforming

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:INITialize 'A:'

This command formats the disk in drive A. Formatting deletes all data stored on the floppy disk.

Parameter: <msus> ::= 'A:'
Only drive name A: is accepted.

Example: "MMEM:INIT 'A:'"

Characteristics: *RST value: -
SCPI: conforming

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:LOAD:STATe 1,<file_name>

This command loads device settings from files.The contents of the file are loaded and set as the new device state. The device automatically recognizes the files that are required for the whole setup from the list of file extensions:

Contents	Extension
Current setting of measurement hardware and associated title, if indicated	.SET
Activated limit lines	.LIN
Current configuration of general device parameters	.CFG
Configuration for the hardcopy output	.HCS
User-defined color setting	.COL
All defined limit lines	.LIA
Measured data trace 1 to trace 3 screen A	.TR1 to 3
Measured data trace 1 to trace 3 screen B	.TR4 to 6
Tracking generator settings (only with Tracking Generator Option FSP-B9 or Ext. Generator Control FSP-B10)	.TCi
Setting for source calibration (only with Tracking Generator Option FSP-B9 or Ext. Generator Control FSP-B10)	.TS1 .TS2
Correction data for source calibration (only with Tracking Generator Option FSP-B9 or Ext. Generator Control FSP-B10)	.TC1 .TC2

The file name includes indication of the path and may also include the drive name. The path name complies with DOS conventions.

Parameter: <file_name> ::= DOS file name without extension, extensions see table

Example: `"MMEM:LOAD:STAT 1,'A:TEST'"`

Characteristics: *RST value: -
SCPI: conforming

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:LOAD:AUTO 1,<file_name>

This command defines which device setting is automatically loaded after the device is switched on. The contents of the file are read after switching on the device and used to define the new device state. The file name includes indication of the path and may also include the drive. The path name complies with DOS conventions.

Note:
*The data set defined as auto recall set will also be restored by a *RST-command.*

Parameter: <file_name> ::= DOS file name without extension;
FACTORY denotes the data set previously in the instrument

Example: "MMEM:LOAD:AUTO 1,'D:\USER\DATA\TEST'"

Characteristics: *RST value: FACTORY
SCPI: device-specific

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:MDIRectory <directory_name>

This command creates a new directory. The file name includes indication of the path and may also include the drive name. The path name complies with DOS conventions.

Parameter: <directory_name>::= DOS path name

Example: "MMEM:MDIR 'D:\USER\DATA'"

Characteristics: *RST value: -
SCPI: device-specific

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:MOVE <file_source>,<file_destination>

This command renames existing files, if <file_destination> contains no path indication. Otherwise the file is moved to the indicated path and stored under the file name specified there, if any.

The file name includes indication of the path and may also include the drive. The path name complies with DOS conventions.

Parameter: <file_source>,<file_destination> ::= <file_name>
<file_name> ::= DOS file name

Example: `"MMEM:MOVE 'D:\TEST01.CFG','SETUP.CFG'"`
Renames TEST01.CFG in SETUP.CFG in directory D:\.

`"MMEM:MOVE 'D:\TEST01.CFG','D:\USER\DATA'"`
Moves TEST01.CFG from D:\ to D:\USER\DATA.

`"MMEM:MOVE 'D:\TEST01.CFG','D:\USER\DATA\SETUP.CFG'"`
Moves TEST01.CFG from D:\ to D:\USER\DATA and renames the file in SETUP.CFG.

Characteristics: *RST value: -
SCPI: conforming

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:MSIS <device>

This command changes to the drive indicated.The drive may be the internal hard disk D: or the floppy-disk drive A:.

Example: `"MMEM:MSIS 'A:'"`

Characteristics: *RST value: "D:'
SCPI: conforming

Mode: all

MMEMory:NAME <file_name>

This command defines a destination file for the printout started with the command `HCOPy:IMMediate`. In this case the printer output must be routed to destination *FILE* using the command `"HCOP:DEST 'MMEM' "`.

The file name includes indication of the path and may also include the drive name. The file name and path information comply with DOS conventions.

Parameter: <file_name> ::= DOS filename

Example:

`"HCOP:DEV:LANG BMP"`	Selection of data format.
`"HCOP:DEST 'MMEM' "`	Selection of the output device
`"MMEM:NAME 'PRINT1.BMP'"`	Selection of file name.
`"HCOP:IMM"`	Start of the printout.

Characteristics: *RST value: -
SCPI: conforming

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:RDIRectory <directory_name>

This command deletes the indicated directory. The directory name includes indication of the path and may also include the drive name. The path name complies with DOS conventions.

Parameter: <directory_name>::= DOS path name

Example: "MMEM:RDIR 'D:\TEST'"

Characteristics: *RST value: -
SCPI: device-specific

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:STORe<1|2>:STATe 1,<file_name>

This command stores the current device settings in a series of files which have the indicated file name, but different extensions. The file name includes indication of the path and may also include the drive name. The path name complies with DOS conventions. The numeric suffix in STORe<1|2> is irrelevant with this command.

A list of the extensions used is contained under MMEMory:LOAD:STATe.

Parameter: <file_name> := DOS file name without extension

Example: "MMEM:STOR:STAT 1,'TEST'"

Characteristics: *RST value: -
SCPI: conforming

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:STORe<1|2>:TRACe 1 to 3,<file_name>

This command stores the selected trace (1 to 3) in the measurement window indicated by STORe<1|2> (screen A or B) in a file with ASCII format. The file format is described in chapter 4 in the TRACE menu under the *ASCII-FILE EXPORT* softkey.

The decimal separator (decimal point or comma) for floating-point numerals contained in the file is defined with the command FORMat:DEXPort:DSEParator.

The file name includes indication of the path and the drive name. Indication of the path complies with DOS conventions.

Parameter: 1 to 3 := selected measurement curve Trace 1 to 3
<file_name> := DOS file name

Example: "MMEM:STOR2:TRAC 3,'A:\TEST.ASC'"
Stores trace 3 from screen B in the file TEST.ASC on a disk.

Characteristics: *RST value: -
SCPI: device-specific

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:CLEar:STATe 1,<file_name>

This command deletes the instrument setting selected by <file_name>. All associated files on the mass memory storage are cleared. A list of the extensions used is included under `MMEMory:LOAD:STATe`.

The file name includes indication of the path and may also include the drive. The path name complies with DOS conventions.

Parameter: <file_name> ::= DOS file name without extension

Example: `"MMEM:CLE:STAT 1,'TEST'"`

Characteristics: *RST value: -
SCPI: device-specific

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:CLEar:ALL

This command deletes all device settings in the current directory.The current directory can be selected with `MMEM:CDIR`. The default directory is D:.

Example: `"MMEM:CLE:ALL"`

Characteristics: *RST value: -
SCPI: device-specific

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

MMEMory:SELect[:ITEM]:HWSettings ON | OFF

This command includes the hardware settings in the list of data subsets of a device setting to be stored/loaded. The hardware settings of the FSP include:

- current configuration of general device parameters (general setup)
- current setting of the measurement hardware including markers
- activated limit lines:
  A data set may include 8 limit lines at maximum in each measurement window. This number includes the activated limit lines and, if available, the de-activated limit lines last used. Therefore the combination of the non-activated restored limit lines depends on the sequence of use with the command `MMEM:LOAD`.
- user-defined color setting
- configuration for the hardcopy output
- Tracking generator settings
  (only in conjunction with option Tracking Generator FSP-B9 or External Generator Control FSP-B10)
- Correction data for source calibration
  (only in conjunction with option Tracking Generator FSP-B9 or External Generator Control FSP-B10)

Example: `"MMEM:SEL:HWS ON"`

Characteristics: *RST value: ON
SCPI: device-specific

Mode: all

MMEMory:SELect[:ITEM]:TRACE ON | OFF

This command adds the active traces to the list of data subsets of a save/recall device setting. Active traces are all traces whose state is not blank.

Example: "MMEM:SEL:TRAC ON"

Characteristics: *RST value: OFF, ie no traces will be stored
SCPI: device-specific

Mode: all

MMEMory:SELect[:ITEM]:LINes:ALL ON | OFF

This command adds all limit lines (activated and de-activated) to the list of device settings to be stored/loaded.

Example: "MMEM:SEL:LIN:ALL ON"

Characteristics: *RST value: ON
SCPI: device-specific

Mode: all

MMEMory:SELect[:ITEM]:SCData ON | OFF

This command adds the tracking generator calibration data to the list of device settings to be stored/loaded.

Example: "MMEM:SEL:SCD ON" Inserts the tracking generator correction data in the list of data subsets

Characteristics: *RST value: OFF
SCPI: device-specific

Modes: all

This command is only available in conjunction with the tracking generator option FSP-9 or external generator control option FSP-10.

MMEMory:SELect[:ITEM]:ALL

This command includes all data subsets in the list device settings to be stored/loaded.

Example: "MMEM:SEL:ALL"

Characteristics: *RST value: --
SCPI: device-specific

Mode: all

This command is an event and therefore has no *RST value assigned.

MMEMory:SELect[:ITEM]:NONE

This command deletes all data subsets from the list of device settings to be stored/loaded.

Example: "MMEM:SEL:NONE"

Characteristics: *RST value: --
SCPI: device-specific

Mode: all

This command is an event and therefore has no *RST value assigned.

MMEMory:SELect[:ITEM]:DEFault

This command sets the default list of device settings to be stored/loaded.The latter includes:

- current configuration of general device parameters (general setup)
- current setting of the measurement hardware including markers
- activated limit lines
- user-defined color setting
- configuration for the hardcopy output

Trace data and non-used limit lines are not included.

Example: "MMEM:SEL:DEFault"

Characteristics: *RST value: --
SCPI: device-specific

Mode: all

This command is an event and therefore has no *RST value assigned.

MMEMory:COMMent <string>

This command defines a comment (max. 60 characters) for a device setting to be stored.

Example: "MMEM:COMM 'Setup for GSM measurement'"

Characteristics: *RST value: blank comment
SCPI: device-specific

Mode: all

OUTPut Subsystem

The OUTPut subsystem controls the output features of the instrument.
In conjunction with the tracking generator option, a distinction is made between OUTPut1 (screen A) and OUTPut2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
OUTPut<1|2> [:STATe]	<boolean>	--	Tracking generator option

OUTPut<1|2>[:STATe] ON | OFF

This command switches the tracking generator on or off.

Notes:
With the tracking generator switched on, the maximum stop frequency is limited to 3 GHz. This upper limit is automatically modified by the set frequency offset of the generator.

If measurements in compliance with specs are to be performed with the tracking generator, the start frequency has to be ≥3 x resolution bandwidth.

The minimum sweep time for measurements in compliance with the data sheet is 100 ms in the frequency domain (span >0). If a shorter sweep time is selected, the sweep time indicator SWT on the screen is marked with a red asterisk and the message UNCAL is also displayed.

With the tracking generator switched on, the FFT filters (`BAND:MODE:FFT`) are not available.

Example: `"OUTP ON"` Switches on the tracking generator in screen A.

Characteristics: *RST value: -
SCPI: conforming

Modes: E, A, VA

This command is only valid in conjunction with one of the option tracking generator FSP-B9.

SENSe Subsystem

The SENSe subsystem is organized in several subsystems. The commands of these subsystems directly control device-specific settings, they do not refer to the signal characteristics of the measurement signal.
The SENSe subsystem controls the essential parameters of the analyzer. In accordance with the SCPI standard, the keyword "SENSe" is optional for this reason, which means that it is not necessary to include the SENSe node in command sequences.
The measurement windows are selected by SENSe1 and SENSe2:

SENSe1 = Modification of screen A settings
SENSe2 = Modification of screen B settings.

Screen A is automatically selected if 1 or 2 is missing.

SENSe:AVERage Subsystem

The SENSe:AVERage subsystem calculates the average of the acquired data. A new test result is obtained from several successive measurements.
There are two types of average calculation: logarithmic and linear. In case of logarithmic average calculation (denoted with VIDeo), the average value of the measured logarithmic power is calculated and in case of linear average calculation, the linear power is averaged before the logarithm is applied.
The measurement windows are selected by SENSe1 (screen A) and SENSe2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
[SENSe<1|2>]			
:AVERage			
:COUNt	<numeric_value>	--	
[:STATe<1 to 3>]	<Boolean>	--	
:TYPE	VIDeo | LINear	--	

[SENSe<1|2>:]AVERage:COUNt 0 to 32767

This command defines the number of measurements which contribute to the average value.

It should be noted that continuous averaging will be performed after the indicated number has been reached in continuous sweep mode.

In single sweep mode, the sweep is stopped as soon as the indicated number of measurements (sweeps) is reached. Synchronization to the end of the indicated number of measurements is only possible in single sweep mode.

The command `[SENSe<1|2>:]AVERage:COUNt` is the same as command `[SENSe<1|2>:]SWEep:COUNt`. In both cases, the number of measurements is defined whether the average calculation is active or not.

The number of measurements is valid for all traces in the indicated measurement window.

Example:

```
"SWE:CONT OFF"      Switching to single-sweep mode.
"AVER:COUN 16"      Sets the number of measurements to 16.
"AVER:STAT ON"      Switches on the calculation of average.
"INIT;*WAI"         Starts the measurement and waits for the end of the 16
                    sweeps.
```

Characteristics: *RST value: 0
SCPI: conforming

Mode: all

[SENSe<1|2>:]AVERage[:STATe<1 to 3>] ON | OFF

This command switches on or off the average calculation for the selected trace (STATe<1 to 3>) in the selected measurement window.

Example:

```
"AVER OFF"          Switches off the average calculation for trace 1 in screen A.
"SENS2:AVER:STAT3 ON"   Switches on the average calculation for trace 3 in
                        screen B.
```

Characteristics: *RST value: OFF
SCPI: conforming

Mode: all

[SENSe<1|2>:]AVERage:TYPE VIDeo | LINear

This command selects the type of average function.If VIDeo is selected, the logaritmic power is averaged and, if LINear is selected, the power values are averaged before they are converted to logarithmic values.

The type of average calculation is equally set for all traces in one measurement window.

Example:

```
"AVER:TYPE LIN"     Switches screen A to linear average calculation.
```

Characteristics: *RST value: VIDeo
SCPI: device-specific

Mode: A

SENSe:BANDwidth Subsystem

This subsystem controls the setting of the instrument's filter bandwidths. Both groups of commands (BANDwidth and BWIDth) perform the same functions. The measurement windows are selected by SENSe1 (screen A) and SENSe2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
[SENSe<1|2>]			
:BANDwidth			
[:RESolution]	<numeric_value>	HZ	
:AUTO	<Boolean>	--	
:RATio	<numeric_value>	--	
:TYPE	NORMal | FFT | CFILter | RRC	--	
:VIDeo	<numeric_value>	HZ	
:AUTO	<Boolean>	--	
:RATio	<numeric_value>	--	
:BWIDth			
[:RESolution]	<numeric_value>	HZ	
:AUTO	<Boolean>	--	
:RATio	<numeric_value>	--	
:TYPE	NORMal | FFT | CFILter | RRC	--	
:VIDeo	<numeric_value>	HZ	
:AUTO	<Boolean>	--	
:RATio	<numeric_value>	--	

[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution] <numeric_value>

This command defines the analyzer's resolution bandwidth. Analog resolution filters of 10 Hz to 10 MHz in 1, 3, 10 steps are available. These filters are implemented as 4-circuit LC filters in the range of 300 kHz to 10 MHz and as digital filters with analog characteristic in the range of 10 Hz to 100 kHz.

In addition, the EMI bandwidths 200 Hz, 9 kHz and 120 kHz are available (6 dB bandwidths each). These bandwidths can only be obtained by entering numeric values and not with the commands `INCrement` and `DECrement`.

FFT filters of 1 Hz to 30 kHz in 1, 3, 10 steps (3 dB bandwidth each) are also available in the frequency domain (span > 0) for fast measurements on periodic signals. The instrument automatically switches to analog filters above 30 kHz.

A number of especially steep-edged channel filters can be selected from firmware version 1.10 or higher provided that parameters `CFILter` or `RRC` are selected using the `BAND:TYPE` command. The possible combinations of filter type and filter bandwidth are listed in the table "List of available channel filters" of chapter 4, section "Setting Bandwidths and Sweep Time– Key *BW*".

If the resolution bandwidth is modified, the coupling to the span is automatically switched off.

Example: `"BAND 1MHz"` sets the resolution bandwidth to 1 MHz

Characteristics: *RST value: - (AUTO is set to ON)
SCPI: conforming

Mode: all

[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:AUTO ON | OFF

This command either automatically couples the resolution bandwidth of the instrument to the span or cancels the coupling.

The automatic coupling adapts the resolution bandwidth to the currently set frequency span according to the relationship between frequency span and resolution bandwidth. The 6 dB bandwidths 200 Hz, 9 kHz and 120 kHz and the channel filters available from Version 1.10 are not set by the automatic coupling.

The ratio resolution bandwidth/span can be modified with the command `[SENSe<1|2>:]BANDwidth[:RESolution]:RATio`.

Example: `"BAND:AUTO OFF"` Switches off the coupling of the resolution bandwidth to the span.

Characteristics: *RST value: ON
SCPI: conforming

Mode: A

[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:RATio 0.0001 to 1

This command defines the ratio resolution bandwidth (Hz) / span (Hz). The ratio to be entered is reciprocal to the ratio span/RBW used in manual control.

Example: `"BAND:RAT 0.1"`

Characteristics: *RST value: 0.02 with BAND:TYPE NORMal or RBW > 30 kHz
0.01 with BAND:TYPE FFT for RBW ≤ 30 kHz
SCPI: conforming

Mode: A

[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:TYPE NORMal | FFT | CFILter | RRC

This command switches the filter type for the resolution bandwidth between "normal" analog or FIR filters in 1, 3, 10 steps and the FFT filtering for bandwidths <100 kHz.

The advantage of FFT filtering is the higher measurement speed compared to digital filters with analog filter characteristic. However, FFT filters are only suitable for periodic signals, and they are only available for span > 0 Hz.

Since firmware version 1.10 steep-edged channel filters and filters with RRC (Root Raised Cosine) characteristic are available. The possible combinations of filter type and filter bandwidth are listed in the table "List of available channel filters" in chapter 4, section "Setting Bandwidths and Sweep Time– Key *BW*".

Note:
When changing the filter type, the next larger filter bandwidth is selected if the same filter bandwidth is not available for the new filter type.

Example: `"BAND:TYPE NORM"`

Characteristics: *RST value: NORMal
SCPI: device-specific

Operating mode: A

[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo 1Hz to 10MHz

This command defines the instrument's video bandwidth. Bandwidths from 10 Hz to 10 MHz in 1, 3, 10 steps are available. The command is not available if FFT filtering is switched on and the set bandwidth is ≤ 30 kHz or if the quasi-peak detector is switched on.

Example: `"BAND:VID 10kHz"`

Characteristics: *RST value: - (AUTO is set to ON)
SCPI: conforming

Mode: A

[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo:AUTO ON | OFF

This command either automatically couples the instrument's video bandwidth to the resolution bandwidth or cancels the coupling.

The ratio video bandwidth/resolution bandwidth can be modified with the command `[SENSe<1|2>:]BANDwidth:VIDeo:RATio`.

Example: `"BAND:VID:AUTO OFF"`

Characteristics: *RST value: ON
SCPI: conforming

Mode: A

[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo:RATio 0.01 to 1000

This command defines the ratio video bandwidth (Hz) / resolution bandwidth (Hz).The ratio to be entered is reciprocal to the ratio RBW/VBW used in manual control.

Example: `"BAND:VID:RAT 3"` Sets the coupling of video bandwidth to video bandwidth = 3*resolution bandwidth

Characteristics: *RST value: 3
SCPI: conforming

Mode: A

SENSe:CORRection Subsystem

This subystem controls calibration and normalization during operation with the tracking generator options (FSP-B9/10). The measurement windows are selected by SENSe1 (screen A) and SENSe2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
[SENSe<1|2>]			
:CORRection			Tracking Generator option
:METHod	TRANsmission | REFLexion		
:COLLect			
[:ACQuire]	THRough | OPEN		no query
[:STATe]	<Boolean>		
:RECall			no query

[SENSe<1|2>:]CORRection[:STATe] ON | OFF

This command activates/deactivates the normalization of the measurement results in the selected window provided that the tracking generator is active. The command is available only after aquisition of a reference trace for the selected type of measurement (transmission/reflection, see command `[SENSe<1|2>:]CORRection:COLLect[:ACQire]`).

Example: `"CORR ON "` activates normalization in screen A.

Characteristics: *RST value: OFF
SCPI: conforming

Mode: A

This command is only valid in conjunction with the tracking generator / ext. generator control option (FSP-B9/B10).

[SENSe<1|2>:]CORRection:METHod TRANsmission | REFLexion

This command selects the type of measurement with active tracking generator (transmission/reflexion).

Example: `"CORR:METH TRAN "` sets the type of measurement in screen A to "transmission".

Characteristics: *RST value: TRANsmission
SCPI: device specific

Mode: A

This command is only valid in conjunction with the tracking generator / ext. generator control option (FSP-B9/B10).

[SENSe<1|2>:]CORRection:COLLect[:ACQuire] THRough | OPEN

This command selects the kind of measurement for the reference values of the normalization (response calibration).

THRough	"TRANsmission" mode:	calibration with direct connection between tracking generator and device input.
	"REFLexion" mode:	calibration with short circuit at the input
OPEN	only valid in "REFLexion" mode:calibration with open input	

This command is an event and is therefore not assigned an *RST value and has no query. It is only valid in conjunction with the tracking generator / ext. generator control option (FSP-B9/B10).

Example:	`"CORR:COLL THR"`	selects single sweep operation
	`"CORR:COLL THR;*WAI"`	starts the measurement of reference data using direct connection between generator and device input and waits for the sweep end.

Characteristics: *RST value: --
SCPI: conforming

Mode: A

[SENSe<1|2>:]CORRection:RECall

This command restores the instrument setting that was valid for the measurement of the reference data, provided that the tracking generator is active.

Example: `"CORR:REC"`

Characteristics: *RST value: -
SCPI: conforming

Mode: A

This command is an event and is therefore not assigned an *RST value and has no query. It is only valid in conjunction with the tracking generator / ext. generator control option (FSP-B9/B10).

SENSe:DETector Subsystem

The SENSe:DETector subsystem controls the acquisition of measurement data via the selection of the detector for the corresponding trace. The measurement windows are selected by SENSe1 (screen A) and SENSe2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
[SENSe<1|2>]			
:DETector<1 to 3>			
[:FUNCtion]	APEak | NEGative| POSitive | SAMPle| RMS | AVERage | QPEak		
:AUTO	<Boolean>		

[SENSe<1|2>:]DETector<1..3>[:FUNCtion] APEak | NEGative | POSitive | SAMPle | RMS | AVERage | QPEak

This command switches on the detector for the data acquisition in the selected trace and the indicated measurement window.

- The APEak detector (AutoPeak) displays the positive and also the negative peak value of the noise floor. If a signal is detected, only the positive peak value is displayed.
- The POSitive or NEGative detector only displays the positive or the negative peak value.
- With the Sample detector the value measured at the sampling time is displayed, whereas the RMS value of the power measured at each test point is displayed with the RMS detector.
- The AVERage detector displays the power average value at each test point.
- The QPEak detector performs a signal evaluation for EMC measurements.

If QPEak is selected, the video filter is automatically switched off. The couplings between span and RBW as well as between RBW and sweep time are also switched off and restored on selecting another detector. A long sweep time should be selected so that the quasi-peak detector can fully settle at each test point.

The trace is indicated as numeric suffix in `DETector`.

Example: `"DET POS"` Sets the detector in screen A to "positive peak".

Characteristics: *RST value: APEak
SCPI: conforming

Mode: A

[SENSe<1|2>:]DETector<1 to 3>[:FUNCtion]:AUTO ON | OFF

This command either couples the detector in the selected measurement window to the current trace setting or turns coupling off. The trace is selected by the numeric suffix at DETector.

Example: `"DET:AUTO OFF"`

Characteristics: *RST value: ON
SCPI: conforming

Mode: A

SENSe:FREQuency Subsystem

The SENSe:FREQuency subsystem defines the frequency-axis of the active display. The frequency-axis can either be defined via the start/stop frequency or via the center frequency and span. The measurement windows are selected by SENSe1 (screen A) and SENSe2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
[SENSe<1|2>]			
:FREQuency			
:CENTer	<numeric_value>	HZ	
:STEP	<numeric_value>	HZ	
:LINK	SPAN|RBW|OFF	--	
:FACTor	<numeric_value>	PCT	
:SPAN	<numeric_value>	HZ	
:FULL	--	--	
:STARt	<numeric_value>	HZ	
:STOP	<numeric_value>	HZ	
:MODE	CW|FIXed|SWEep		
:OFFSet	<numeric_value>	HZ	

[SENSe<1|2>:]FREQuency:CENTer 0 to f_{max}

This command defines the center frequency of the analyzer or the measuring frequency for span = 0.

Example: `"FREQ:CENT 100MHz"`

Characteristics: *RST value: f_{max} /2 with f_{max} = maximum frequency of the analyzer
SCPI: conforming

Mode: all

[SENSe<1|2>:]FREQuency:CENTer:STEP 0 to f_{max}

This command defines the step width of the center frequency.

Example: `"FREQ:CENT:STEP 120MHz"`

Characteristics: *RST value: - (AUTO 0.1 × SPAN is switched on)
SCPI: conforming

Mode: all

[SENSe<1|2>:]FREQuency:CENTer:STEP:LINK SPAN | RBW | OFF

This command couples the step width of the center frequency to span (span >0) or to the resolution bandwidth (span = 0) or cancels the couplings.

Parameters:

SPAN = Coupling to frequency display range (for span > 0)
RBW = Coupling to resolution bandwidth (for span = 0)
OFF = manual input, no coupling.

Example: `"FREQ:CENT:STEP:LINK SPAN"`

Characteristics: *RST value: SPAN
SCPI: device-specific

Mode: A

[SENSe<1|2>:]FREQuency:CENTer:STEP:LINK:FACTor 1 to 100 PCT

This command couples the step width of the center frequency with a factor to the span (span >0) or to the resolution bandwidth (span = 0).

Example: `"FREQ:CENT:STEP:LINK:FACT 20PCT"`

Characteristics: *RST value: - (AUTO 0.1 × SPAN is switched on)
SCPI: device-specific

Mode: A

[SENSe<1|2>:]FREQuency:SPAN 0 to f_{max}

This command defines the frequency span of the analyzer.

Example: `"FREQ:SPAN 10MHz"`

Characteristics: *RST value: f_{max} with f_{max} = maximum frequency of the analyzer
SCPI: conforming

Mode: A

[SENSe<1|2>:]FREQuency:SPAN:FULL

This command sets the frequency span of the analyzer to its maximum.

Example: `"FREQ:SPAN:FULL"`

Characteristics: *RST value: -
SCPI: conforming

Mode: A

[SENSe<1|2>:]FREQuency:STARt 0 to f_{max}

This command defines the start frequency of the analyzer. This command is only available in the frequency domain (span >0).

Example: `"FREQ:STAR 20MHz"`

Characteristics: *RST value: 0
SCPI: conforming

Mode: E, A

[SENSe<1|2>:]FREQuency:STOP 0 to f_{max}

This command defines the stop frequency of the analyzer.This command is only available in the frequency domain (span >0).

Example: `"FREQ:STOP 2000MHz"`

Characteristics: *RST value: f_{max}
SCPI: conforming

Mode A

[SENSe<1|2>:]FREQuency:MODE CW | FIXed | SWEep

This command switches between frequency domain (SWEep) and time domain (CW | FIXed) in the analyzer mode.

For CW and FIXed, the frequency setting is via command `FREQuency:CENTer`. In the SWEep mode, the setting is via commands `FREQuency:STARt`, `STOP`, `CENTer` and `SPAN`.

Example: `"FREQ:MODE SWE"`

Characteristics: *RST value: SWEep
SCPI: conforming

Mode: A

[SENSe<1|2>:]FREQuency:OFFSet <numeric_value>

This command defines the frequency offset of the instrument.

Example: `"FREQ:OFFS 1GHZ"`

Characteristics: *RST value: 0 Hz
SCPI: conforming

Mode: A

SENSe:LIST Subsystem

The commands of this subsystem are used for measuring the power at a list of frequency points with different device settings. The measurement is always performed in the time domain (span = 0 Hz).

A new trigger event is required for each test point (exception: Trigger FREE RUN).

The results are output as a list in the order of the entered frequency points. The number of results per test point depends on the number of concurrently active measurements (peak/RMS/average).

Selection of concurrently active measurements and setting of parameters that are constant for the whole measurement is via a configuration command (SENSe:LIST:POWer:SET). This also includes the setting for trigger and gate parameters.

The following setting parameters can be selected independently for each frequency point:

- Analyzer frequency
- Reference level
- RF attenuation
- RF attenuation of attenuator (only with option FSP-B25)
- Resolution filter
- Resolution bandwidth
- Video bandwidth
- Measurement time
- Detector

The number of frequencies is limited to 100 entries.

The commands of this subsystem can be used in two different ways:

1. Instrument setup, measurement and querying of the results in a single command: With this method, there is the least delay between the measurement and the result output. However, it requires the control computer to wait for the response from the instrument.
2. Instrument setup and querying of the result list at the end of the measurement: With this method, the control computer may be used for other activities while the measurement is being performed. However, more time is needed for synchronization via service request.

Note:
Settings that are not included in the commands of this subsystem can be configured executing the corresponding commands before the commands of the SENSe:LIST subsystem.
Please note that settings of the trigger level have to be executed in time domain (span = 0 Hz) in order to take effect for the SENSe:LIST commands.

COMMAND	PARAMETER	UNIT	COMMENT
[SENSe<1|2>]			
:LIST			
:POWer			
:RESult?			Query only
[:SEQuence]	<numeric_value>, <numeric_value>, <numeric_value>, <numeric_value> | OFF, NORMal | CFILter | RRC, <numeric_value>, <numeric_value>, <numeric_value>, <numeric_value> ...	HZ, DBM, DB, DB, --, HZ, HZ, S, PCT	
:SET	<Boolean>, <Boolean>, <Boolean>, IMMediate | EXTernal | VIDeo | IFPower, POSitive|NEGative, <numeric_value>, <numeric_value>	--, --, --, --, --, S, S	
:STATe	OFF		

[SENSe<1|2>:]LIST:POWer[:SEQuence] <analyzer freq>,<ref level>,<rf att>,<el att>,
<filter type>,<rbw>,<vbw>,<meas time>,<trigger level>,...

This command configures the list of settings (max. 100 entries) for the multiple power measurement and starts a measurement sequence. When synchronizing the command with *OPC, a service request is generated as soon as all frequency points are processed and the defined number of individual measurements (# of meas) is reached.

To reduce the setting time, all indicated parameters are set up simultaneously at each test point.

The query form of the command processes the list and immediately returns the list of results. The number of results per test point depends on the setting of the "SENSe:LIST:POWer:SET" command.

Parameter:

Note:
The following parameters are the settings for an individual frequency point. They are repeated for every other frequency point.

<analyzer freq>: Receive frequency for the signal to be measured
(= center frequency in manual operation)
Range of values: 0 Hz to max. analyzer frequency, depending on the instrument model.

<ref level>: Reference level
Range of values: +30 dBm to -70 dBm in 10 dB steps
+30 dBm to -75 dBm in 5 dB steps with EI. Attenuator option FSP-B25

<rf att>: RF input attenuation
Range of values: 0 dB to 70 dB in 10 dB steps
0 dB to 75 dB in 5 dB steps with EI. Attenuator Option FSP-B25

<el att>:	RF input attenuation of electronic attenuator		
	Range of values:	0 dB to 30 dB	in 10 dB steps
		OFF	electronic attenuator not in signal path
	If option FSP-B25 is missing, OFF is to be given.		
<filter type>:	NORMal:	normal resolution filter	
	CFILter:	channel filter. These are especially steep-edged filters, which are used for example in Fast ACP measurement to ensure the band-limiting of a transmission channel in the time domain.	
	RRC:	Root Raised Cosine filter. This special filter form is used to determine the channel power for some mobile radio standards.	
<rbw>:	Resolution bandwidth		
	Range of values:	10 Hz to 10 MHz	in 1, 3, 10 steps for <filter type> = NORMal.
		See filter table	for <filter type> = CFILter and <filter type> = RRC. Possible combinations of filter type and filter bandwidth see table "List of available channel filters" in section "Setting Bandwidths and Sweep Time – Key *BW*".
<vbw>:	Video bandwidth		
	Range of values:	1 Hz to 10 MHz	in 1, 3, 10 steps. The value is ignored for <filter type> = CFILter or RRC
<meas time>:	Measurement time		
	Range of values:	1us to 30s	
<trigger level>:	Reserved. Must be set to 0.		

Returned values:

The query command returns a list of comma-separated values (CSV) which contains the power measurement results in floating-point format. The unit depends on the setting with `CALC:UNIT`.

Command

```
"SENSe:LIST:POWer?  935.2MHz,-20dBm,10dB,OFF,NORM,1MHz,3MHz,434us,0,
                    935.4MHz,-20dBm,10dB,10dB,NORM,30kHz,100kHz,434us,0,
                    935.6MHz,-20dBm,10dB,20dB,NORM,30kHz,100kHz,434us,0"
```

thus returns the following list, for example:

-28.3,-30.6,-38.1

If the command sequence is extended to

```
"SENSe:LIST:POWer:SET ON,ON,ON,IMM,POS,0,0"
"SENSe:LIST:POWer?  935.2MHz,-20dBm,10dB,OFF,NORM,1MHz,3MHz,434us,0,
                    935.4MHz,-20dBm,10dB,10dB,NORM,30kHz,100kHz,434us,0,
                    935.6MHz,-20dBm,10dB,20dB,NORM,30kHz,100kHz,434us,0"
```

the result list is extended to 3 results per frequency point (peak, RMS and average):

-28.3, -29.6, 1.5, -30.6, -31.9, 0.9, -38.1, -40.0, 2.3

Examples:

```
"SENSe:LIST:POWer   935.2MHz,-20dBm,10dB,OFF,NORM,1MHz,3MHz,434us,0,
                    935.4MHz,-20dBm,10dB,10dB,CFIL,30kHz,100kHz,434us,0,
                    935.6MHz,-20dBm,10dB,20dB,CFIL,30kHz,100kHz,434us,0"
```

performs a measurement sequence with the following settings:

Step	Freq. [MHz]	Ref Level	RF Att	el Att	Filtertyp	RBW	VBW	Meas Time	TRG Level (reserved)
1	935.2	-20 dBm	10 dB	OFF	Normal	1 MHz	3 MHz	434 us	0
2	935.4	-20 dBm	10 dB	10dB	Channel	30 kHz	100 kHz	434 us	0
3	935.6	-20 dBm	10 dB	20dB	Channel	30 kHz	100 kHz	434 us	0

```
"SENSe:LIST:POWer?  935.2MHz,-20dBm,10dB,OFF,NORM,1MHz,3MHz,434us,0,
                    935.4MHz,-20dBm,10dB,10dB,CFIL,30kHz,100kHz,434us,0,
                    935.6MHz,-20dBm,10dB,20dB,CFIL,30kHz,100kHz,434us,0"
```

performs the same measurement and returns the result list immediately after the last frequency point.

Notes: *The measurement is performed in the time domain and therefore the span is set to 0 Hz. If the time domain is quit, the function is automatically switched off.*

The measurement is not compatible with other measurements, especially as far as marker, adjacent channel power measurement or statistics are concerned. The corresponding commands thus automatically deactivate the function.

The function is only available in REMOTE operation. It is deactivated when switching the instrument back to LOCAL.

Characteristics: *RST value: --
SCPI: device-specific

Mode: A-F, A-T

[SENSe<1|2>:]LIST:POWer:SET <PEAK meas>,<RMS meas>,<AVG meas>,
<trigger mode>,<trigger slope>,<trigger offset>,<gate length>

This command defines the constant settings for the list during multiple power measurement.

Parameters <PEAK meas>, <RMS meas> and <AVG meas> define, which measurements are to be performed at the same time at the frequency point. Correspondingly, one, two or three results per frequency point are returned for the SENS:LIST:POW? command. If all three parameters are set to OFF, the command generates an execution error.

Parameter:

<PEAK meas>: ON activates the measurement of the peak power (peak detector).
OFF deactivates the measurement of the peak power.

<RMS meas>: ON activates the measurement of the RMS power (RMS detector).
OFF deactivates the measurement of the RMS power.

<AVG meas>: ON activates the measurement of the average power (average detector).
OFF deactivates the measurement of the average power.

<trigger mode>: Selection of the trigger source used for the list measurement.
Possible values:
IMMediate | VIDeo | EXTernal | IFPower

<trigger slope>: Used trigger slope.
Possible values:
POSitive | NEGative

<trigger offset>: Offset between the detection of the trigger signal and the start of the measurement at the next frequency point.
Range of values: 0 s, 125 ns to 100s

<gate length>: Gate length with Gated Sweep.
Range of values: 0 s, 125 ns to 100s

Note:

- *The value 0 s deactivates the use of GATED TRIGGER; other values activate the GATED TRIGGER function.*
- *Values <> 0 s are only possible if <trigger mode> is different from IMMediate. Otherwise, an execution error is triggered.*

Returned values:

The query command returns a list of comma-separated values (CSV) of the settings, ie

```
ON,ON,ON,IMM,POS,0,0
```

if the configuration has been set with the command

```
"SENSe:LIST:POWer:SET ON,ON,ON,IMM,POS,0,0"
```

Examples:

```
"SENSe:LIST:POWer:SET ON,OFF,OFF,EXT,POS,10US,434US"
"SENSe:LIST:POWer:SET ON,ON,ON,VID,NEG,10US,0"
```

Characteristics: *RST values: ON,OFF,OFF,IMM,POS,0S,0S
SCPI: device-specific

Mode: A-F, A-T

[SENSe<1|2>:]LIST:POWer:RESult?

This command queries the result of a previous list measurement as configured and initiated with SENSe:LIST:POWer[:SEQuence]. The measured results are output in a list of floating point values separated by commas. The unit of the results depends on the setting made with the CALC:UNIT command.

This command may be used to obtain measurement results in an asynchronous way, using the service request mechanism for synchronization with the end of the measurement.

If no measurement results are available, the command will return a query error.

Example:

```
'Configuration of the FSP status reporting system for the generation of an
SRQ on operation complete
*ESE 1
*SRE 32
'Configuring and starting the measurement
"SENSe:LIST:POWer 935.2MHz,-20dBm,10dB,OFF,NORM,1MHz,3MHz,434us,0,
                  935.4MHz,-20dBm,10dB,10dB,NORM,30kHz,100kHz,434us,0,
                  935.6MHz,-20dBm,10dB,20dB,NORM,30kHz,100kHz,434us,0;
                  *OPC"
'Further actions of the control computer during measurement
...
'Response to service request
On SRQ:
SENSe:LIST:POWer:RESult?
```

Characteristics: *RST value: --
SCPI: device-specific

Mode: A-F, A-T

[SENSe<1|2>:]LIST:POWer:STATe OFF

This command deactivates the list measurement.

Example:

```
SENSe:LIST:POWer:STATe OFF
```

Characteristics: *RST value: --
SCPI: device-specific

Mode: A-F, A-T

SENSe:MPOWer – Subsystem

The commands of this subsystem are used to determine the mean burst power or peak burst power for a given number of signal bursts, and for outputting the results in a list. Since all the settings required for a measurement are combined in a single command, the measurement speed is considerably higher than when using individual commands.

For measuring the signal bursts, the GATED SWEEP function is used in the time domain. The gate is controlled either by an external trigger signal or by the video signal. An individual trigger event is required for each burst to be measured. If an external trigger signal is used, the threshold is fixed to TTL level, while with a video signal the threshold can be set as desired.

The following graphics shows the relation between trigger time, trigger offset (for delayed gate opening) and measurement time.

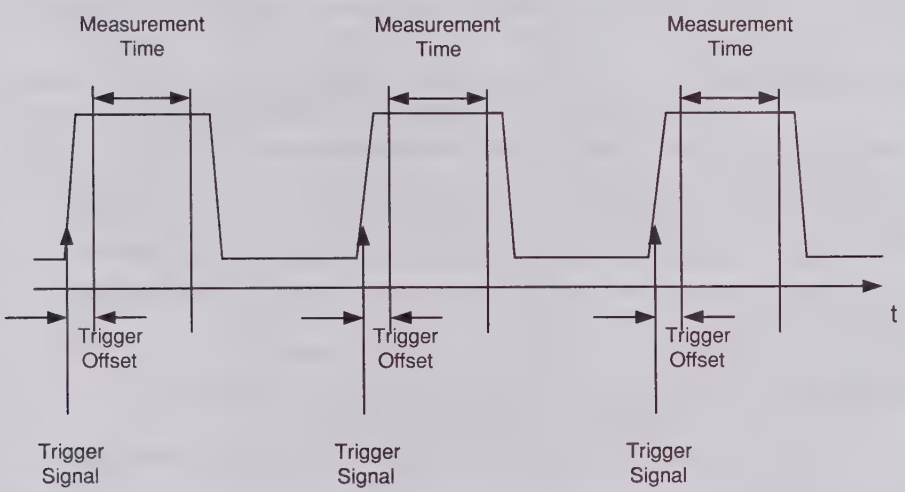

Depending on the settings made, the measurements are performed with the RMS detector for RMS power or the PEAK detector for peak power. For all these measurements, TRACE 1 of the selected system is used.

The setting parameters for this measurement are:

- analyzer frequency
- resolution bandwidth
- measurement time used for a single burst
- trigger source
- trigger level
- trigger offset
- type of power measurement (PEAK, MEAN)
- number of bursts to be measured

The commands of this subsystem can be used in two different ways:

1. Setting up the instrument and at the same time querying the result list:
   This method ensures the smallest delay between measurement and the output of the measured values, but requires the control computer to wait actively for the response of the instrument.
2. Setting up the instrument and querying the result list after synchronisation to the end of measurement:
   With this method the control computer can be used for other activities while the FSP is performing the measurement at the cost of additional time needed for synchronisation via service request.

COMMAND	PARAMETER	UNIT	COMMENT
[SENSe<1|2>]			
:MPOWer			
[:SEQuence]	<numeric_value>, <numeric_value>, <numeric_value>, EXTernal | VIDeo, <numeric_value>, <numeric_value>, MEAN | PEAK, <numeric_value>	HZ, HZ, S, --, PCT, S, --, --	
:RESult			
[:LIST]?			Query only
:MIN?			Query only

[SENSe<1|2>:]MPOWer[:SEQuence] <analyzer freq>,<rbw>,<meas time>,<trigger source>, <trigger level>,<trigger offset>,<type of meas>,<# of meas>

This command configures the instrument setup for multiple burst power measurement and starts a measurement sequence. When synchronizing the command with *OPC, a service request is generated as soon as the defined number of individual measurements (# of meas) is reached.

To reduce the setting time, the setup is performed simultaneously for all selected parameters.

The command in the form of a query makes the instrument settings, performs the defined number of measurements and outputs the measurement results list.

Parameters:

<analyzer freq>: Receive frequency for the burst signals to be measured (= center frequency in manual operation)

Range: 0 Hz to max. analyzer frequency, depending on instrument model

<rbw>: resolution bandwidth for the measurement

Range: 10 Hz to 10 MHz in steps of 1, 3, 10

<meas time>: Time span during which measurement samples are sampled for RMS / peak measurement The type of measurement is selected by <type of meas>.

Range: 1us to 30s

<trigger source>: trigger signal source. Possible settings:

EXTernal The trigger signal is fed from the "Ext. Trigger/Gate" input on the rear of the unit.

VIDeo The internal video signal is used as trigger signal.

<trigger level>: Signal level of the video signal as a percentage of the diagram height at which the trigger becomes active. If <trigger source> = EXTernal is selected, the value entered here is ignored, as in this case the trigger input uses TTL levels.

Range: 0 – 100PCT

<trigger offset>: Offset between the detection of the trigger signal and the start of the measurement.

Range: 125 ns to 100s

<type of meas>: Determines whether mean power (RMS) or peak power (PEAK) is to be measured. The FSP detector is selected accordingly.

Possible values:MEAN, PEAK

<# of meas>: Number of individual bursts to be measured.

Range: 1 to 501

Return values:

The query command returns a list separated by commas (comma separated values = CSV), which contains the power measurement results in floating-point format. The unit used for the return values is always dBm.

The command `"SENSe:MPOWer? 935.2MHz,1MHz,434us,VIDEO,50PCT,5us,MEAN,20"` may, for instance, cause the following list to be returned:

18.3,18.6,18.1,18.0,17.9,18.3,18.6,18.1,18.0,17.9,18.3,18.6,18.1,18.0,17.9,18.3,18.6,18.1,18.0,17.9

Examples: `"SENSe:MPOWer 935.2MHz,1MHz,434us,VIDEO,50PCT,5us,MEAN,20"`
performs a measurement sequence with the following settings:

Frequency	= 935.2 MHz,
Resolution bandwidth	= 1 MHz
Measurement time	= 434 µs
Trigger source	= VIDEO
Trigger threshold	= 50%
Trigger offset	= 5 µs
Type of measurement	= MEAN power
No. of measurements	= 20

`"SENSe:MPOWer? 935.2MHz,1MHz,434us,VIDEO,50PCT,5us,MEAN,20"`
performs the same measurement and in addition returns the results list immediately after completion of the last measurement.

Notes: *The measurement function always uses trace 1 in the selected screen, and activates the selected screen.*
Repeated use of the command without changes to its parameters (ie using the same settings again) will speed up the measurement since the FSP will cache the previous hardware settings and therefore avoid additional hardware settling times. This also holds true if only part of the parameters (e.g. only the trigger delay) are changed, as in this case the rest of the parameters will be cached.

This measurement is not compatible with other measurements, especially as far as marker functions, adjacent-channel measurement or statistics are concerned. The corresponding functions are therefore automatically switched off. In return incompatible commands will automatically deactivate the multi burst power function.

The function is only available in the REMOTE operation. It is deactivated on switching back to LOCAL.

Characteristics: *RST value: --
SCPI: instrument-specific

Mode: A-F, A-T

SENSe:MPOWer:RESult[:LIST]?

This command queries the results of a multiple burst power measurement as configured and initiated with `SENSe:MPOWer[:SEQuence]`. The results are output in a comma-separated list of floating point values. The unit used for the return values is always dBm.

This command may be used to obtain measurement results in an asynchronous way using the service request mechanism for synchronization with the end of the measurement.

If no measurement results are available, the command will return a query error.

Example:

```
'Configuration of FSP status reporting systems for the
'generation of an SRQ on operation complete
*ESE 1
*SRE 32
'Configuring and starting the measurement
SENSe:MPOWer
935.2MHz,1MHz,434us,VIDEO,50PCT,5us,MEAN,20;*OPC
'Further actions of the control computer during measurement
...
'Response to service request
On SRQ:
SENSe:MPOWer:RESult?
```

Characteristics: *RST value: --
SCPI: instrument-specific

Mode: A-F, A-T

SENSe:MPOWer:RESult:MIN?

This command queries the minimum power value in a multiple burst power measurement as configured and initiated with `SENSe:MPOWer[:SEQuence]`. The unit used for the return values is always dBm.

If no measurement result is available, the command will return a query error.

Example:

```
'Configuration of the FSP status reporting
system for the 'generation of an SRQ on operation complete
*ESE 1
*SRE 32
'Configuring and starting the measurement
SENSe:MPOWer
935.2MHz,1MHz,434us,VIDEO,50PCT,5us,MEAN,20;*OPC
'Further actions of the control computer during measurement
...
'Response to service request
On SRQ:
SENSe:MPOWer:RESult:MIN?
```

Characteristics: *RST value: --
SCPI: instrument-specific

Mode: A-F, A-T

SENSe:POWer Subsystem

This subsystem controls the setting of the instrument's channel and adjacent channel power measurements. The measurement windows are selected by SENSe1 (screen A) and SENSe2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
[SENSe<1|2>]			
:POWer			
:ACHannel			
:SPACing			
[:ACHannel]	<numeric_value>	HZ	
:ALTernate<1|2>	<numeric_value>	HZ	
:ACPairs	0 | 1 | 2 | 3		
:BANDwidth			
[:CHANnel]	<numeric_value>	HZ	
:ACHannel	<numeric_value>	HZ	
:ALTernate<1|2>	<numeric_value>	HZ	
:BWIDth			
[:CHANnel]	<numeric_value>	HZ	
:ACHannel	<numeric_value>	HZ	
:ALTernate<1|2>	<numeric_value>	HZ	
:MODE	ABSolute | RELative		
:REFerence			
:AUTO	ONCE		no query
:PRESet	ACPower | CPOWer | OBANdwidth | OBWidth		
:RLEVel			
:BANDwidth	<numeric_value>	PCT	
:BWIDth	<numeric_value>	PCT	
:HSPeed	<Boolean>		
:NCORrection	<Boolean>		
:TRACe	<numeric_value>	--	

[SENSe<1|2>:]POWer:ACHannel:SPACing:ACHannel 100 Hz to 2000 MHz

This command defines the channel spacing of the adjacent channel to the TX channel. At the same time, the spacing of alternate adjacent channels 1 and 2 is set to the double or triple of the entered value.

The command is only available in the frequency domain (span > 0).

Example: `"POW:ACH:SPAC:ACH 33kHz"` Sets the spacing between the carrier signal and
- the adjacent channel to 33 kHz
- the alternate adjacent channel 1 to 66 kHz
- the alternate adjacent channel 2 to 99 kHz

Characteristics: *RST value: 14 kHz
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:ACHannel:SPACing:ALTernate<1|2> 100 Hz to 2000 MHz

This command defines the spacing between the first (ALTernate1) or the second alternate adjacent channel (ALTernate2) and the TX channel.If the spacing to the alternate adjacent channel ALTernate1 is modified, the spacing to alternate adjacent channel 2 is set to 1.5 times the entered value.

This command is only available in the frequency domain (span > 0).

Example: `"POW:ACH:SPAC:ALT1 100kHz"` Sets the spacing between TX channel and alternate adjacent channel 1 to 100 kHz and between TX channel and alternate adjacent channel 2 to 150 kHz.

Characteristics: *RST value: 40 kHz (ALT1)
60 kHz (ALT2)
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:ACHannel:ACPairs 0 | 1.| 2 | 3

This command sets the number of adjacent channels (upper and lower channel in pairs).The figure 0 stands for pure channel power measurement.

The command is only available in the frequency domain (span > 0).

Example: `"POW:ACH:ACP 3"` Sets the number of adjacent channels to 3, ie the adjacent channel and alternate adjacent channels 1 and 2 are switched on.

Characteristics: *RST value: 1
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:ACHannel:BANDwidth|BWIDth[:CHANnel] 100 Hz to 1000 MHz

This command sets the channel bandwidth of the radio communication system.The bandwidths of adjacent channels are not influenced by this modification (in contrast to the FSE family).

With `SENS:POW:HSP ON` the steep-edged channel filters from the table "List of available channel filters" in Section "Setting Bandwidths and Sweep Time – Key *BW*" are available.

Example: `"POW:ACH:BWID 30kHz"` Sets the banwidth of the TX channel to 30 kHz.

Characteristics: *RST value: 14 kHz
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:ACHannel:BANDwidth|BWIDth:ACHannel 100 Hz to 1000 MHz

This command defines the channel bandwidth of the adjacent channel of the radio transmission system. If the bandwidth of the adjacent channel is changed, the bandwidths of all alternate adjacent channels are automatically set to the same value.

With `SENS:POW:HSP ON` the steep-edged channel filters from the table "List of available channel filters" in Section "Setting Bandwidths and Sweep Time – Key *BW*" are available.

Example: `"POW:ACH:BWID:ACH 30kHz"` Sets the bandwidth of all adjacent channels to 30 kHz.

Characteristics: *RST value: 14 kHz
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:ACHannel:BANDwidth|BWIDth:ALTernate<1|2> 100 Hz to 1000 MHz

This command defines the channel bandwidth of the first/second alternate adjacent channel of the radio transmission system. If the channel bandwidth of alternate adjacent channel 1 is changed, the bandwith of alternate adjacent channel 2 is automatically set to the same value.

With `SENS:POW:HSP ON` the steep-edged channel filters from the table "List of available channel filters" in Section "Setting Bandwidths and Sweep Time – Key *BW*" are available.

Example: `"POW:ACH:BWID:ALT2 30kHz"`

Characteristics: *RST value: 14 kHz
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:ACHannel:MODE ABSolute | RELative

This command toggles between absolute and relative adjacent channel measurement.

For the relative measurement the reference value is set to the currently measured channel power by command `SENSe:POWer:ACHannel:REFerence:AUTO ONCE`.

The command is only available in the frequency domain (span > 0).

Example: `"POW:ACH:MODE REL"`

Characteristics: *RST value: ABSolute
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:ACHannel:REFerence:AUTO ONCE

This command sets the reference value for the relative measurement to the currently measured channel power.

The command is only available in the frequency domain (span > 0).

Example: `"POW:ACH:REF:AUTO ONCE"`

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

This command is an event and is therefore not assigned an *RST value and has no query.

[SENSe<1|2>:]POWer:ACHannel:PRESet ACPower | CPOWer | OBANdwidth|OBWidth

This command adapts the frequency span, the bandwidths and the detector to the number of channels, channel bandwidths and channel spacings of the active power measurement and switches on the adjacent channel power measurement, if required.

To ensure that the results are valid, a complete sweep including synchronization to the sweep end must be performed after the configuration. Synchronization is only possible in single sweep mode.

The results are queried with `CALCulate:MARKer:FUNCtion:POWer:RESult?`.

The command is only available in the frequency domain (span > 0).

Example:

```
"POW:ACH:REF:PRES ACP"
```
Sets the frequency range, bandwidths and detector suitable for ACP measurement in screen A.

```
"INIT:CONT OFF"
```
Switches to single-sweep mode.

```
"INIT;*WAI"
```
Starts a sweep and waits for the end.

```
"CALC:MARK:FUNC:POW:RES? ACP"
```
Queries the result of the adjacent channel power measurement.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:ACHannel:PRESet:RLEVel

This command adapts the reference level of the FSP to the measured channel power and – if required - switches on previously the adjacent channel power measurement. This ensures that the signal path of the FSP is not overloaded. Since the measurement bandwidth is significantly smaller than the signal bandwidth in channel power measurements, the signal path can be overloaded although the trace is still significantly below the reference level. If the measured channel power equals the reference level, the signal path is not overloaded.

The command is only available in the frequency domain (span > 0).

Note:
*The following commands have to be synchronized with *WAI, *OPC or *OPC? to the end of the autorange process which would otherwise be aborted.*

Example:

```
"POW:ACH:REF:PRES:RLEV;*WAI"
```
Adapts the reference level to the measured channel power.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:BANDwidth|BWIDth 10 to 99.9PCT

This command defines the percentage of the power with respect to the total power. This value is the basis for the occupied bandwidth measurement (command: `POWer:ACHannel:PRESet OBW`).

The command is only available in the frequency domain (span > 0).

Example: `"POW:BWID 95PCT"`

Characteristics: *RST value: 99PCT
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:HSPeed ON | OFF

This command switches on or off the high-speed channel/adjacent channel power measurement. The measurement itself is performed in the time domain on the center frequencies of the individual channels. The command automatically switches to the time domain and back.

Depending on the selected mobile radio standard, weighting filters with √cos characteristic or very steep-sided channel filters are used for band limitation.

The command is only available in the frequency domain (span > 0).

Example: `"POW:HSP ON"`

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A-F

[SENSe<1|2>:]POWer:TRACe 1 to 3

This command assigns the channel/adjacent channel power measurement to the indicated trace in the selected measurement window. The corresponding trace must be active, ie its state must be different from blank.

Note: *The measurement of the occupied bandwidth (OBW) is performed on the trace on which marker 1 is positioned. To evaluate another trace, marker 1 must be positioned to another trace with* `CALCulate:MARKer:TRACe`.

Example: `"POW:TRAC 2"` Assigns the measurement in screen A to trace 2.
`"SENS2:POW:TRAC 3"` Assigns the measurement in screen B to trace 3.

Characteristics: *RST value: -
SCPI: device-specific

Mode: A

SENSe:ROSCillator Subsystem

This subsystem controls the reference oscillator. The numeric suffix in SENSe is irrelevant for the commands of this subsystem.

COMMAND	PARAMETERS	UNIT	COMMENT
[SENSe<1|2>]			
:ROSCillator			
:SOURce	INTernal | EXTernal	--	
[:INTernal]			
:TUNe	<numeric_value>		
:SAVe			no query

[SENSe<1|2>:]ROSCillator:SOURce INTernal | EXTernal

This command controls selection of the reference oscillator.

If the external reference oscillator is selected, the reference signal must be connected to the rear panel of the instrument.

Example: `"ROSC:SOUR EXT"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

[SENSe<1|2>:]ROSCillator[:INTernal]:TUNe 0 to 4095

This command defines the value for the tuning of the internal reference oscillator.

The reference oscillator should be tuned only if an error has been detected in the frequency accuracy check. After rebooting the instrument, the factory-set reference frequency or the previously saved reference frequency is restored.

Note: *This command is only available at service level 1.*

Example: `"ROSC:TUN 128"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

[SENSe<1|2>:]ROSCillator[:INTernal]:TUNe:SAVe

This command saves the new value for the tuning of the internal reference oscillator. The factory-set value in the EEPROM is overwritten.

Note: *This command is only available at service level 1.*

Example: `"ROSC:TUN:SAV"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

SENSe:SWEep Subsystem

This subsystem controls the sweep parameters. The measurement windows are selected by SENSe1 (screen A) and SENSe2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
[SENSe<1|2>]			
:SWEep			
:TIME	<numeric_value>	S	
:AUTO	<Boolean>	--	
:COUNt	<numeric_value>	--	
:EGATe	<Boolean>	--	
:TYPE	LEVel|EDGE	--	
:POLarity	POSitive|NEGative	--	
:HOLDoff	<numeric_value>	S	
:LENGth	<numeric_value>	S	
:SOURce	EXTernal | IFPower		

[SENSe<1|2>:]SWEep:TIME 2,5ms ... 16000s (frequency domain) | 1µs... 16000s (time domain)

This command defines the sweep time. The available time values are different in the frequency domain (2.5 ms to 16000s with span > 0) and in the time domain (1µs to 16000s with span = 0).

If `SWEep:TIME` is directly programmed, automatic coupling to resolution bandwidth and video bandwidth is switched off.

Example: `"SWE:TIME 10s"`

Characteristics: *RST value - (AUTO is set to ON)
SCPI: conforming

Mode: A

[SENSe<1|2>:]SWEep:TIME:AUTO ON | OFF

This command controls the automatic coupling of the sweep time to the frequency span and bandwidth settings.

If `SWEep:TIME` is directly programmed, automatic coupling is switched off.

Example: `"SWE:TIME:AUTO ON"` Switches on the coupling to frequency span and bandwidths.

Characteristics: *RST value: ON
SCPI: conforming

Mode: A

[SENSe<1|2>:]SWEep:COUNt 0 to 32767

This command defines the number of sweeps started with single sweep, which are used for calculating the average or maximum value. In average mode, the value 0 defines a continuous averaging of measurement data over 10 sweeps.

Example:
```
"SWE:COUN 64"          Sets the number of sweeps to 64.
"INIT:CONT OFF"        Switches to single-sweep mode.
"INIT;*WAI"            Starts a sweep and waits for its end.
```

Characteristics: *RST value: 0
SCPI: conforming

Mode: A

[SENSe<1|2>:]SWEep:EGATe ON | OFF

This command switches on/off the sweep control by an external gate signal. If the external gate is selected the trigger source is automatically switched to EXTernal as well.

In case of measurement with external gate, the measured values are recorded as long as the gate is opened. There are two possibilities:

1. The gate is edge-triggered (`"SWEep:EGATe:TYPE EDGE"`):
   After detection of the set gate signal edge, the gate remains open until the gate delay (`SWEep:EGATe:HOLDoff`) has expired.
2. The gate is level-triggered (`"SWEep:EGATe:TYPE LEVel"`):
   After detection of the gate signal, the gate remains open until the gate signal disappears.

A delay between applying the gate signal and the start of recording measured values can be defined with `SWEep:EGATe:HOLDoff`.

During a sweep the gate can be opened and closed several times. The synchronization mechanisms with *OPC, *OPC? and *WAI remain completely unaffected.

The sweep end is detected when the required number of measurement points (501 in analyzer mode) has been recorded.

Example:
```
"SWE:EGAT ON"          Switches on the external gate mode.
"SWE:EGAT:TYPE EDGE"   Switches on the edge-triggered mode.
"SWE:EGAT:HOLD 100US"  Sets the gate delay to 100 µs.
"SWE:EGAT:LEN 500US"   Sets the gate opening time to 500 µs.
"INIT;*WAI"            Starts a sweep and waits for its end.
```

Characteristics: *RST value: OFF
SCPI: device-specific

Mode: A

[SENSe<1|2>:]SWEep:EGATe:TYPE LEVel | EDGE

This command sets the type of triggering (level or edge) by the external gate signal.

The gate opening time cannot be defined with the parameter `EGATe:LENGth` in case of level triggering. The gate is closed when the gate signal disappears.

Example:
```
"SWE:EGAT:TYPE EDGE"
```

Characteristics: *RST value: EDGE
SCPI: device-specific

Mode: A

[SENSe<1|2>:]SWEep:EGATe:POLarity POSitive | NEGative

This command determines the polarity of the external gate signal. The setting is valid both for the edge of an edge-triggered signal and the level of a level-triggered signal.

Example: `"SWE:EGAT:POL POS"`

Characteristics: *RST value: POSitive
SCPI: device-specific

Mode: A

[SENSe<1|2>:]SWEep:EGATe:HOLDoff 125 ns to 100 s

This command defines the delay time between the external gate signal and the continuation of the sweep.

Example: `"SWE:EGAT:HOLD 100us"`

Characteristics: *RST value: 0s
SCPI: device-specific

Mode: A

[SENSe<1|2>:]SWEep:EGATe:LENGth 0 to 100 s

In case of edge triggering, this command determines the time interval during which the instrument sweeps.

Example: `"SWE:EGAT:LENG 10ms"`

Characteristics: *RST value: 0s
SCPI: device-specific

Mode: A

[SENSe<1|2>:]SWEep:EGATe:SOURce EXTernal | IFPower

This command toggles between external gate signal and IF power signal as a signal source for the gate mode. If an IF power signal is used, the gate is opened as soon as a signal at > -20 dBm is detected within the IF path bandwidth (10 MHz).

Example: `"SWE:EGAT:SOUR IFP"` Switches the gate source to IF power.

Characteristics: *RST value: IFPower
SCPI: device-specific

Mode: A

SOURce Subsystem

The SOURce subsystem controls the output signals of the analyzer if the options tracking generator (FSP-B9) or External Generator Control (FSP-B10) are installed. The measurement window is selected by SOURce1 (screen A) and SOURce2 (screen B).

Internal Tracking Generator

COMMAND	PARAMETERS	UNIT	COMMENT
SOURce<1|2>			Tracking generator option
:AM			
:STATe	<Boolean>		
:DM			
:STATe	<Boolean>		
:FM			
:STATe	<Boolean>		
:DEViation	<numeric_value>	HZ	
:FREQuency			
:OFFSet	<numeric_value>	HZ	
:POWer			
[:LEVel]			
[:IMMediate]			
[:AMPLitude]	<numeric_value>	DBM	
:OFFSet	<numeric_value>	DB	

SOURce<1|2>:AM:STATe ON | OFF

This command switches on or off the external amplitude modulation of the tracking generator in the selected measurement window.

External I/Q modulation is switched off, if active. This command is only valid in conjunction with the tracking generator option FSP-B9.

Example: `"SOUR:AM:STAT ON "` Switches on the external amplitude modulation of the tracking generator for screen A.

Characteristics: *RST value: OFF
SCPI: conforming

Modes: all

SOURce<1|2>:DM:STATe ON | OFF

This command switches on or off the external I/Q modulation of the tracking generator in the selected measurement window.

External AM and external FM are switched off, if active. This command is only valid in conjunction with the tracking generator option FSP-B9.

Example: `"SOUR2:DM:STAT ON "` Switches on the external I/Q modulation of the tracking generator for screen B.

Characteristics: *RST- value: OFF
SCPI: conforming

Modes: all

SOURce<1|2>:FM:STATe ON | OFF

This command switches on or off the external frequency modulation of the tracking generator in the selected measurement window.

External I/Q modulation is switched off, if active. This command is only valid in conjunction with the tracking generator option FSP-B9.

Example: `"SOUR:FM:STAT ON "` Switches on the external frequency modulation of the tracking generator for screen A.

Characteristics: *RST value: OFF
SCPI: conforming

Modes: all

SOURce<1|2>:FM:DEViation 100Hz...10MHz

This command defines the maximum frequency deviation at 1 V input voltage at the FM input of the tracking generator.

The possible value range is 100 Hz to 10 MHz in steps of one decade.

This command is only available in connection with the Tracking Generator Option FSP-B9.

Example: `"SOUR:FM:DEV 1MHz "` sets the maximum frequency deviation of the tracking generator for screen A to 1 MHz.

Characteristics: *RST value: 10 MHz
SCPI: conforming

Operating mode: all

SOURce<1|2>:FREQuency:OFFSet -150MHz to 150MHz

This command defines a frequency offset of the tracking generator for the indicated measurement window. Frequency-converting DUTs can be measured with this setting.

The possible value range is -150 MHz to 150 MHz. It should be noted that the terms (start frequency - tracking frequency offset) and (stop frequency - tracking frequency offset) are both > 1 kHz or both < -1 kHz.

External I/Q modulation is switched off, if active. This command is only valid in conjunction with the tracking generator option FSP-B9.

Example: `"SOUR:FREQ:OFFS 10MHz"` Switches on the frequency offset of the tracking generator for screen A to 10 MHz.

Characteristics: *RST value: 0 Hz
SCPI: conforming

Modes: all

SOURce<1|2>:POWer[:LEVel][:IMMediate][:AMPLitude] <numeric_value>

This command defines the output level of the tracking generator in the current measurement window.

This command is only valid in conjunction with the tracking generator option FSP-B9.

Parameter: <numeric value>::= -30dBm ... 0dBm. In the external tracking generator mode the limits depend on the type of the generator used.

Example: `"SOUR:POW -20dBm"` Sets the tracking generator level in screen A to -20 dBm.

Characteristics: *RST- value: -20 dBm
SCPI: conforming

Modes: all

SOURce<1|2>:POWer[:LEVel][:IMMediate]:OFFSet -200dB to +200dB

This command defines a level offset for the tracking generator level in screen A. Thus, for example, attenuators or amplifiers at the output of the tracking generator can be taken into account for the setting.

This command is only valid in conjunction with the tracking generator option FSP-B9.

Example: `"SOUR:POW:OFFS -10dB"` Sets the level offset of the tracking generator in screen A to - 20 dBm.

Characteristics: *RST- value: 0dB
SCPI: conforming

Modes: all

SOURce:EXTernal Subsystem

The SOURce:EXTernal subsystem controls the operation of the unit with option Ext. Generator Control (FSP-B10). The commands are only valid for the selected window, with SOURce1 changing the setting in screen A and Source2 the setting in screen B.

The selection of the external generator 1 or 2 is via EXTernal<1|2>.

Note:
The commands of the SOURce:EXTernal subsystem assume that the addressed generator was correctly configured with the commands of subsystem
SYSTem:COMMunicate:GPIB:RDEVice:GENerator.

If no external generator is selected, if the IECBUS address is not correct or the generator is not ready for operation, an execution error will be generated.

COMMAND	PARAMETER	UNIT	COMMENT
SOURce<1|2>			
:EXTernal<1|2>			Ext. generator option
[:STATe]	<Boolean>		
:FREQuency			
:OFFSet	<numeric_value>	HZ	
[:FACTor]			
:NUMerator	<numeric_value>		
:DENominator	<numeric_value>		
:SWEep			
[:STATe]	<Boolean>		
:POWer			
[:LEVel]	<numeric_value>	DBM	

SOURce<1|2>:EXTernal<1|2>[:STATe] ON | OFF

This command activates or deactivates the external generator selected with `SOUR:EXT<1|2>:FREQ:SWE ON` in the selected window.

The suffix behind EXTernal is irrelevant for this command.

This command is only available in connection with option Ext. Generator Control FSP-B10.

Example:
`"SYST:COMM:RDEV:GEN1:TYPE 'SMP02'"`
selects SMP02 as generator 1.

`"SYST:COMM:RDEV:GEN1:LINK TTL"`
selects IECBUS + TTL link as interface.

`"SYST:COMM:RDEV:GEN1:ADDR 28"`
sets the generator address to 28.

`"SOUR:EXT1:FREQ:SWE ON"`
activates the frequency sweep for generator 1.

`"SOUR:EXT ON"` activates the external generator

Characteristics: *RST value: OFF
SCPI: device-specific

Operating mode: all

SOURce<1|2>:EXTernal<1|2>:FREQuency[:FACTor]:DENominator <numeric_value>

This command defines the denominator of the factor with which the analyzer frequency is multiplied in order to obtain the transmit frequency of the selected generator 1 or 2 in the selected window.

Note:
Select the multiplication factor in a way that the frequency range of the generator is not exceeded by the following formula

$$F_{Generator} = F_{Analyzer} * \frac{Numerator}{Deno\min ator} + F_{Offset}$$

if applied to the start and stop frequency of the analyzer.

This command is only valid in combination with option Ext. Generator Control FSP-B10.

Example: `"SOUR:EXT:FREQ:NUM 4"`
`"SOUR:EXT:FREQ:DEN 3"`
sets a multiplication factor of 4/3, ie the transmit frequency of the generator is 4/3 times the analyzer frequency.

Characteristics: *RST value: 1
SCPI: device-specific

Operating mode: all

SOURce<1|2>:EXTernal<1|2>:FREQuency[:FACTor]:NUMerator <numeric_value>

This command defines the numerator of the factor with which the analyzer frequency is multiplied to obtain the transmit frequency of the selected generator 1 or 2 in the selected window.

Note:
Select the multiplication factor so that the frequency range of the generator is not exceeded if the following formula

$$F_{Generator} = F_{Analyzer} * \frac{Numerator}{Deno\min ator} + F_{Offset}$$

is applied to the start and stop frequency of the analyzer.

This command is only valid in combination with option Ext. Generator Control FSP-B10.

Example: `"SOUR:EXT:FREQ:NUM 4"`
`"SOUR:EXT:FREQ:DEN 3"`
sets a multiplication factor of 4/3, ie the transmit frequency of the generator is 4/3 times the analyzer frequency.

Characteristics: *RST value: 1
SCPI: device-specific

Operating mode: all

SOURce<1|2>:EXTernal<1|2>:FREQuency:OFFSet <numeric_value>

This command defines the frequency offset of the selected generator 1 or 2 with reference to the receive frequency in the selected window.

Note:
Select the frequency offset of the generator so that the frequency range of the generator is not exceeded with the following formula

$$F_{Generator} = F_{Analyzer} * \frac{Numerator}{Denominator} + F_{Offset}$$

applied to the start and stop frequency of the analyzer.

This command is only valid in combination with option Ext. Generator Control FSP-B10.

Example: `"SOUR:EXT:FREQ:OFFS 1GHZ"` sets a frequency offset of the generator transmit frequency compared to the analyzer receive frequency of 1 GHz.

Characteristics: *RST value: 0 Hz
SCPI: device-specific

Operating mode: all

SOURce<1|2>:EXTernal<1|2>:FREQuency:SWEep[:STATe] ON | OFF

This command activates or deactivates the frequency sweep for generator 1 or 2 in the selected window.

This command is only valid in combination with option Ext. Generator Control FSP-B10.

Example: `"SOUR:EXT1:FREQ:SWE ON"` activates the frequency sweep for ext. generator 1.

Characteristics: *RST value: OFF
SCPI: device-specific

Operating mode: all

SOURce<1|2>:EXTernal<1|2>:POWer[:LEVel] <numeric_value>

This command sets the output power of the selected generator 1 or 2 in the selected window.

This command is only valid in combination with option Ext. Generator Control FSP-B10.

Example: `"SOUR:EXT:POW -30dBm"` sets the generator level to –30 dBm

Characteristics: *RST value: -20 dBm
SCPI: device-specific

Operating mode: all

STATus Subsystem

The STATus subsystem contains the commands for the status reporting system (see Section 3.8, Status Reporting System"). *RST does not influence the status registers.

COMMAND	PARAMETERS	UNIT	COMMENT
STATus			
:OPERation			
[:EVENt]?	--	--	
:CONDition?	--	--	
:ENABle	0 to 65535	--	
:PTRansition	0 to 65535	--	
:NTRansition	0 to 65535	--	
:PRESet	--	--	
:QUEStionable			
[:EVENt]?	--	--	
:CONDition?	--	--	
:ENABle	0 to 65535	--	
:PTRansition	0 to 65535	--	
:NTRansition	0 to 65535	--	
:POWer			
[:EVENt]?	--	--	
:CONDition?	--	--	
:ENABle	0 to 65535	--	
:PTRansition	0 to 65535	--	
:NTRansition	0 to 65535	--	
:LIMit<1|2>			
[:EVENt]?	--	--	
:CONDition?	--	--	
:ENABle	0 to 65535	--	
:PTRansition	0 to 65535	--	
:NTRansition	0 to 65535	--	
:LMARgin<1|2>			
[:EVENt]?	--	--	
:CONDition?	--	--	
:ENABle	0 to 65535	--	
:PTRansition	0 to 65535	--	
:NTRansition	0 to 65535	--	
:ACPLimit			
[:EVENt]?	--	--	
:CONDition?	--	--	
:ENABle	0 to 65535	--	
:PTRansition	0 to 65535	--	
:NTRansition	0 to 65535	--	
:FREQuency	--	--	
[:EVENt]?	0 to 65535	--	
:CONDition?	0 to 65535	--	
:ENABle	0 to 65535	--	
:PTRansition	--	--	
:NTRansition	--	--	
:QUEue?	--	--	
[:NEXT]?	--	--	

STATus:OPERation[:EVENt]?

This command queries the contents of the EVENt section of the STATus:OPERation register. The contents of the EVENt section are deleted after readout.

Example: `"STAT:OPER?"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:OPERation:CONDition?

This command queries the CONDition section of the STATus:OPERation register. Readout does not delete the contents of the CONDition section. The value returned reflects the current hardware status.

Example: `"STAT:OPER:COND?"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:OPERation:ENABle 0 to 65535

This command sets the bits of the ENABle section of the STATus:OPERation register. The ENABle register selectively enables the individual events of the associated EVENt section for the summary bit in the status byte.

Example: `"STAT:OPER:ENAB 65535"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:OPERation:PTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:OPERation register from 0 to 1 for the transitions of the CONDition bit.

Example: `"STAT:OPER:PTR 65535"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:OPERation:NTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:OPERation register from 1 to 0 for the transitions of the CONDition bit.

Example: `"STAT:OPER:NTR 65535"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:PRESet

This command resets the edge detectors and ENABle parts of all registers to a defined value. All PTRansition parts are set to FFFFh, ie all transitions from 0 to 1 are detected. All NTRansition parts are set to 0, ie a transition from 1 to 0 in a CONDition bit is not detected. The ENABle part of the STATus:OPERation and STATus:QUEStionable registers are set to 0, ie all events in these registers are not passed on.

Example: `"STAT:PRES"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable[:EVENt]?

This command queries the contents of the EVENt section of the STATus:QUEStionable register. The contents of the EVENt section are deleted after the readout.

Example: `"STAT:QUES?"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable:CONDition?

This command queries the CONDition section of the STATus:QUEStionable register. Readout does not delete the contents of the CONDition section.

Example: `"STAT:QUES:COND?"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable:ENABle 0 to 65535

This command sets the bits of the ENABle section of the STATus-QUEStionable register.The ENABle register selectively enables the individual events of the associated EVENt section for the summary bit in the status byte.

Example: `"STAT:QUES:ENAB 65535"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable:PTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable register from 0 to 1 for the transitions of the CONDition bit.

Example: `"STAT:QUES:PTR 65535"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable:NTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:OPERation register from 1 to 0 for the transitions of the CONDition bit.

Example: `"STAT:QUES:NTR 65535"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable:POWer[:EVENt]?

This command queries the contents of the EVENt section of the STATus:QUEStionable:POWer register. Readout deletes the contents of the EVENt section.

Example: `"STAT:QUES?"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable:POWer:CONDition?

This command queries the contents of the CONDition section of the STATus:QUEStionable:POWer register. Readout does not delete the contents of the CONDition section.

Example: `"STAT:QUES:COND?"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable:POWer:ENABle 0 to 65535

This command sets the bits of the ENABle section of the STATus:QUEStionable:POWer register. The ENABle register selectively enables the individual events of the associated EVENt section for the summary bit.

Example: `"STAT:QUES:ENAB 65535"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable:POWer:PTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable:POWer register from 0 to 1 for the transitions of the CONDition bit.

Example: `"STAT:QUES:PTR 65535"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable:POWer:NTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable:POWer register from 1 to 0 for the transitions of the CONDition bit.

Example: `"STAT:QUES:NTR 65535"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

STATus:QUEStionable:LIMit<1|2> [:EVENt]?

This command queries the contents of the EVENt section of the STATus:QUEStionable:LIMit register. Readout deletes the contents of the EVENt section.

Example: `"STAT:QUES?"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:LIMit<1|2>:CONDition?

This command queries the contents of the CONDition section of the STATus:QUEStionable:LIMit register.

Readout does not delete the contents of the CONDition section.

Example: `"STAT:QUES:LIM:COND?"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:LIMit<1|2>:ENABle 0 to 65535

This command sets the bits of the ENABle section of the STATus:QUEStionable register.The ENABle register selectively enables the individual events of the associated EVENt section for the summary bit.

Example: `"STAT:QUES:ENAB 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:LIMit<1|2>:PTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable:LIMit register from 0 to 1 for the transitions of the CONDition bit.

Example: `"STAT:QUES:PTR 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:LIMit<1|2>:NTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable:LIMit register from 1 to 0 for the transitions of the CONDition bit.

Example: `"STAT:QUES:NTR 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:LMARgin<1|2> [:EVENt]?

This command queries the contents of the EVENt section of the STATus:QUEStionable:LMARgin register. Readout deletes the contents of the EVENt section.

Example: `"STAT:QUES:LMAR?"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:LMARgin<1|2>:CONDition?

This command queries the contents of the CONDition section of the STATus:QUEStionable:LMARgin register. Readout does not delete the contents of the CONDition section.

Example: `"STAT:QUES:LMAR:COND?"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:LMARgin<1|2>:ENABle 0 to 65535

This command sets the bits of the ENABle section of the STATus:QUEStionable:LMARgin register. The ENABle register selectively enables the individual events of the associated EVENt section for the summary bit.

Example: `"STAT:QUES:LMAR:ENAB 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:LMARgin<1|2>:PTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable:LMARgin register from 0 to 1 for the transitions of the CONDition bit.

Example: `"STAT:QUES:LMAR:PTR 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:LMARgin<1|2>:NTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable:LMARgin register from 1 to 0 for the transitions of the CONDition bit.

Example: `"STAT:QUES:LMAR:NTR 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:ACPLimit[:EVENt]?

This command queries the contents of the EVENt section of the STATus:QUEStionable:ACPLimit register. Readout deletes the contents of the EVENt section.

Example: `"STAT:QUES:ACPL?"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:ACPLimit:CONDition?

This command queries the contents of the CONDition section of the STATus:QUEStionable:ACPLimit register. Readout does not delete the contents of the CONDition section.

Example: `"STAT:QUES:ACPL:COND?"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:ACPLimit:ENABle 0 to 65535

This command sets the bits of the ENABle section of the STATus:QUEStionable:ACPLimit register. The ENABle register selectively enables the individual events of the associated EVENt section for the summary bit.

Example: `"STAT:QUES:ACPL:ENAB 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:ACPLimit:PTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable: ACPLimit register from 0 to 1 for the transitions of the CONDition bit.

Example: `"STAT:QUES:ACPL:PTR 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:ACPLimit:NTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable: ACPLimit register from 1 to 0 for the transitions of the CONDition bit.

Example: `"STAT:QUES:ACPL:NTR 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:FREQuency[:EVENt]?

This command queries the contents of the EVENt section of the STATus:QUEStionable: FREQuency register.

Example: `"STAT:QUES:FREQ?"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

Readout deletes the contents of the EVENt section.

STATus:QUEStionable:FREQuency:CONDition?

This command queries the contents of the CONDition section of the STATus:QUEStionable:FREQuency register. Readout does not delete the contents of the CONDition section.

Example: `"STAT:QUES:FREQ:COND?"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:FREQuency:ENABle 0 to 65535

This command sets the bits of the ENABle section of the STATus:QUEStionable:FREQuency register. The ENABle register selectively enables the individual events of the associated EVENt section for the summary bit.

Example: `"STAT:QUES:FREQ:ENAB 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:FREQuency:PTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable:FREQuency register from 0 to 1 for the transitions of the CONDition bit.

Example: `"STAT:QUES:FREQ:PTR 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEStionable:FREQuency:NTRansition 0 to 65535

This command sets the edge detectors of all bits of the STATus:QUEStionable:FREQuency register from 1 to 0 for the transitions of the CONDition bit.

Example: `"STAT:QUES:FREQ:NTR 65535"`

Characteristics: *RST value: –
SCPI: device-specific

Mode: all

STATus:QUEue[:NEXT]?

This command returns the earliest entry to the error queue and deletes it.

Positive error numbers indicate device-specific errors, negative error numbers are error messages defined by SCPI (cf. Chapter 9). If the error queue is empty, the error number 0, "no error", is returned. This command is identical with the command `SYSTem:ERRor`.

Example: `"STAT:QUE?"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

SYSTem Subsystem

This subsystem contains a series of commands for general functions.

COMMAND	PARAMETERS	UNIT	COMMENT
SYSTem			
:COMMunicate			
:GPIB			
[:SELF]			
:ADDRess	0...30	--	
:RTERminator	LFEoi | EOI		
:RDEVice			
:GENerator<1|2>			Option ext. Generator
:ADDRess	0...30		Option ext. Generator
:RDEVice			
:GENerator<1|2>			
:LINK	GPIB | TTL		tracking generator option
:TYPE	<name>		tracking generator option
:SERial			
:CONTrol			
:DTR	IBFull | OFF		
:RTS	IBFull | OFF		
[:RECeive]			
:BAUD	<numeric_value>	--	
:BITS	7 | 8	--	
:PARity			
[:TYPE]	EVEN | ODD | NONE		
:SBITs	1 | 2	--	
:PACE	XON | NONE		
:PRINter			
:ENUMerate			
[:NEXT?]			query only
:FIRSt?			query only
:SELect<1|2>	<printer_name>		
:DATE	<num>, <num>, <num>	--	
:DISPlay			
:FPANel	<Boolean>		
:UPDate	<Boolean>		
:ERRor?	--	--	query only
:PASSword			
[:CENable]	<string>		no querye
:PRESet	--	--	no query
:SET	<block>		
:SPEaker			audio demodulator option
:VOLume	<numeric_value>	--	
:TIME	0...23, 0...59, 0...59	--	
:VERSion?	--	--	query only

SYSTem:COMMunicate:GPIB[:SELF]:ADDRess 0 to 30

This command changes the IEC/IEEE-bus address of the unit.

Example: `"SYST:COMM:GPIB:ADDR 18"`

Characteristics: *RST value: - (no influence on this parameter)
SCPI: conforming

Mode: all

SYSTem:COMMunicate:GPIB[:SELF]:RTERminator LFEOI | EOI

This command changes the GPIB receive terminator.

According to the standard the terminator in ASCII is <LF> and/or <EOI>. For binary data transfers (eg trace data) from the control computer to the instrument, the binary code (0AH) used for <LF> might be included in the binary data block, and therefore should not be interpreted as a terminator in this particular case. This can be avoided by changing the receive terminator to EOI.

Output of binary data from the instrument to the control computer does not require such a terminator change.

Example: `"SYST:COMM:GPIB:RTER EOI"`

Characteristics: *RST value: LFEOI
SCPI: device-specific

Mode: all

SYSTem:COMMunicate:GPIB:RDEVice:GENerator<1|2>:ADDRess 0 to 30

This command changes the IEC/IEEE-bus address of the device selected as external generator 1 or 2.

Note:
If two generators are connected at the same time to IECBUS 2 their addresses must be different.

The command is only available with option Ext. Generator Control FSP-B10.

Example: `"SYST:COMM:GPIB:RDEV:GEN1:ADDR 19"` Changes the IECBUS address of generator 1 to 19

Characteristics: *RST value: 28
SCPI: device-specific

Operating mode: all

SYSTem:COMMunicate:RDEVice:GENerator<1|2>:LINK GPIB | TTL

This command selects the interface type of the external generator 1 or 2.
The following types are available

- IECBUS alone (= GPIB, for all the generators of other manufacturers and some Rohde & Schwarz units)

or

- IECBUS and TTL interface for synchronization (= TTL, for most of the Rohde & Schwarz generators, see table in command SYSTem:COMMunicate:RDEVice:GENerator:TYPE).

The difference between the two operating modes is the execution speed. While, during IECBUS operation, each settable frequency is transmitted separately to the generator, a whole frequency list can be programmed in one go if the TTL interface is also used. Frequency switching can then be performed per TTL handshake which results in considerable speed advantages.

Note:
Only one of the two generators can be operated via the TTL interface at a time. The other generator must be configured for IECBUS (GPIB).

The command is only available with option Ext. Generator Control FSP-B10.

Example: `"SYST:COMM:RDEV:GEN:LINK TTL"` selects IECBUS + TTL interface for generator operation

Characteristics: *RST value: GPIB
SCPI: device-specific

Operating mode: all

SYSTem:COMMunicate:RDEVice:GENerator<1|2>:TYPE <name>

This command selects the type of external generator 1 or 2. The following table shows the available generator types including the associated interface:

Generator	Interface Type	Generator Min Freq	Generator Max Freq	Generator Min Power dBm	Generator Max Power dBm
SME02	TTL	5 kHz	1.5 GHz	-144	+16
SME03	TTL	5 kHz	3.0 GHz	-144	+16
SME06	TTL	5 kHz	6.0 GHz	-144	+16
SMG	GPIB	100 kHz	1.0 GHz	-137	+13
SMGL	GPIB	9 kHz	1.0 GHz	-118	+30
SMGU	GPIB	100 kHz	2.16 GHz	-140	+13
SMH	GPIB	100 kHz	2.0 GHz	-140	+13
SMHU	GPIB	100 kHz	4.32 GHz	-140	+13
SMIQ02B	TTL	300 kHz	2.2 GHz	-144	+13
SMIQ02E	GPIB	300 kHz	2.2 GHz	-144	+13
SMIQ03B	TTL	300 kHz	3.3 GHz	-144	+13
SMIQ03E	GPIB	300 kHz	3.3 GHz	-144	+13
SMIQ04B	TTL	300 kHz	4.4 GHz	-144	+10
SMIQ06B	TTL	300 kHz	6.4 GHz	-144	+10
SML01	GPIB	9 kHz	1.1 GHz	-140	+13
SMR20	GPIB	1 GHz	20 GHz	-130 [2]	+11 [2]
SMR20B11 [1]	GPIB	10 MHz	20 GHz	-130 [2]	+13 [2]
SMR27	GPIB	1 GHz	27 GHz	-130 [2]	+11 [2]
SMR27B11 [1]	GPIB	10 MHz	27 GHz	-130 [2]	+12 [2]
SMR30	GPIB	1 GHz	30 GHz	-130 [2]	+11 [2]
SMR30B11 [1]	GPIB	10 MHz	30 GHz	-130 [2]	+12 [2]
SMR40	GPIB	1 GHz	40 GHz	-130 [2]	+9 [2]
SMR40B11 [1]	GPIB	10 MHz	40 GHz	-130 [2]	+12 [2]
SMP02	TTL	10 MHz	20 GHz	-130 [3]	+17 [3]
SMP03	TTL	10 MHz	27 GHz	-130 [3]	+13 [3]
SMP04	TTL	10 MHz	40 GHz	-130 [3]	+12 [3]
SMP22	TTL	10 MHz	20 GHz	-130 [3]	+20 [3]
SMT02	GPIB	5.0 kHz	1.5 GHz	-144	+13
SMT03	GPIB	5.0 kHz	3.0 GHz	-144	+13
SMT06	GPIB	5.0 kHz	6.0 GHz	-144	+13

[1] Requires mounting of option SMR-B11.

[2] Maximum/Minimum Power depends on the presence of option SMR-B15/-B17 and of the selected frequency range. For details please consult the SMR datasheet.

[3] Maximum/Minimum Power depends on the presence of option SMP-B15/-B17 and of the selected frequency range. For details please consult the SMP datasheet.

Generator	Interface Type	Generator Min Freq	Generator Max Freq	Generator Min Power dBm	Generator Max Power dBm
SMX	GPIB	100 kHz	1.0 GHz	-137	+13
SMY01	GPIB	9 kHz	1.04 GHz	-140	+13
SMY02	GPIB	9 kHz	2.08 GHz	-140	+13
HP8340A	GPIB	10 MHz	26.5 GHz	-110	10
HP ESG-A Series 1000A, 2000A, 3000A, 4000A	GPIB	250 kHz	4 GHz	-136	20
HP ESG-D SERIES E4432B	GPIB	250 kHz	3 GHz	-136	+10

Notes:
Generators with TTL interface can also be operated via IECBUS (= GPIB) alone.

With NONE selected, the corresponding generator 1 or 2 is deactivated.

The command is only available with option Ext. Generator Control FSP-B10.

Example: `"SYST:COMM:RDEV:GEN2:TYPE 'SME02'"` selects SME02 as generator 2.

Characteristics: *RST value: NONE
SCPI: device-specific

SYSTem:COMMunicate:SERial:CONTrol:DTR IBFull | OFF
SYSTem:COMMunicate:SERial:CONTrol:RTS IBFull | OFF

These commands switch the hardware handshake procedure for the serial interface off (OFF) or on (IBFull).

The two commands are equivalent.

Examples:
```
"SYST:COMM:SER:CONT:DTR OFF"
"SYST:COMM:SER:CONT:RTS IBF"
```

Characteristics: *RST value: OFF
SCPI: conforming

Mode: all

SYSTem:COMMunicate:SERial[:RECeive]:BAUD 110 | 300 | 600 | 1200 | 2400 | 9600 | 19200

This command sets the transmission speed for the serial interface (COM).

Example: `"SYST:COMM:SER:BAUD 2400"`

Characteristics: *RST value: 9600
SCPI: conforming

Mode: all

SYSTem:COMMunicate:SERial[:RECeive]:BITS 7 | 8

This command defines the number of data bits per data word for the serial interface (COM).

Example: `"SYST:COMM:SER:BITS 7"`

Characteristics: *RST value: 8
SCPI: conforming

Mode: all

SYSTem:COMMunicate:SERial[:RECeive]:PARity[:TYPE] EVEN | ODD | NONE

This command defines the parity check for the serial interface (COM).

Possible values are:
EVEN even parity
ODD odd parity
NONE no parity check.

Example: `"SYST:COMM:SER:PAR EVEN"`

Characteristics: *RST value: NONE
SCPI: conforming

Mode: all

SYSTem:COMMunicate:SERial[:RECeive]:SBITs 1|2

This command defines the number of stop bits per data word for the serial interface (COM).

Example: `"SYST:COMM:SER:SBITs 2"`

Characteristics: *RST value: 1
SCPI: conforming

Mode: all

SYSTem:COMMunicate:SERial[:RECeive]:PACE XON | NONE

This command switches on or off the software handshake for the serial interface.

Example: `"SYST:COMM:SER:PACE XON"`

Characteristics: *RST value: NONE
SCPI: conforming

Mode: all

SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt?

This command queries the name of the first printer (in the list of printers) available under Windows NT.

The names of other installed printers can be queried with command `SYSTem:COMMunicate:PRINter:ENUMerate:NEXT?`.

If no printer is configured an empty string is output.

Example: `"SYST:COMM:PRIN:ENUM:FIRS?"`

Characteristics: *RST value: NONE
SCPI: device-specific

Mode: all

SYSTem:COMMunicate:PRINter:ENUMerate:NEXT?

This command queries the name of the next printer installed under Windows NT.

The command

`SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt?`

should be sent previously to return to the beginning of the printer list and query the name of the first printer.

The names of other printers can then be queried with NEXT?. After all available printer names have been output, an empty string enclosed by quotation marks (") is output for the next query. Further queries are answered by a Query Error.

Example: `"SYST:COMM:PRIN:ENUM:NEXT?"`

Characteristics: *RST value: NONE
SCPI: device-specific

Mode: all

SYSTem:COMMunicate:PRINter:SELect <1|2> <printer_name>

This command selects one of the printers configured under Windows NT including the associated output destination.

The specified printer name must be a string as returned by the commands
`SYSTem:COMMunicate :PRINter:ENUMerate:FIRSt?` or
`SYSTem:COMMunicate :PRINter:ENUMerate:NEXT?`

Note: *Command `HCOPy:DESTination` is used to select an output medium other than the default one.*

Example: `"SYST:COMM:PRIN:SEL 'LASER on LPT1'"`

Characteristics: *RST value: NONE
SCPI: device-specific

Mode: all

SYSTem:DATE 1980 to 2099, 1 to 12, 1 to 31

This command is used to enter the date for the internal calendar.

The sequence of entry is year, month, day.

Example: `" SYST:DATE 2000,6,1"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

SYSTem:DISPlay:FPANel ON | OFF

This command activates or deactivates the display of the front panel keys on the screen.

With the display activated, the FSP can be operated on the screen using the mouse by pressing the corresponding buttons. This may be useful if the instrument is operated in a detached station by means of a remote program such as PCANYWHERE.

Notes: *With the display of the front panel keys activated, the screen resolution of the unit is set to 1024x768. Thus, only a section of the whole screen is visible on the internal LCD display, which will be moved by mouse moves.*

For a full display of the user interface, an external monitor has to be connected to the rear panel.

When the front panel display is deactivated, the original screen resolution is restored.

Example: `"SYST:DISP:FPAN ON"`

Characteristics: *RST value: OFF
SCPI: device-specific

Operating mode: all

SYSTem:DISPlay:UPDate ON | OFF

This command switches on or off the update of all display elements during remote control.

Note: *The best performance is obtained when the display output is switched off during remote control.*

Example: `" SYST:DISP:UPD ON`

Characteristics: *RST value: OFF
SCPI: device specific

Mode: all

SYSTem:ERRor?

This command queries the earliest entry in the error queue, and deletes it after the readout.

Positive error numbers indicate device-specific errors, negative error numbers are error messages defined by SCPI (cf. Chapter 9). If the error queue is empty, the error number 0, "no error", is returned. This command is identical with the command `STATus:QUEue:NEXT?`. This command is a query and is therefore not assigned an *RST value.

Example: `"SYST:ERR?"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

SYSTem:ERRor:LIST?

This command reads all system messages and returns a list of comma separated strings. Each string corresponds to an entry in the table SYSTEM MESSAGES.

If the error list is empty, an empty string "" will be returned.

This command is a query and is therefore not assigned an *RST value.

Example: `"SYST:ERR:LIST?"`

Characteristics: *RST value: –
SCPI: device specific

Mode: all

SYSTem:ERRor:CLEar:ALL

This command deletes all entries in the table SYSTEM MESSAGES.

This command is an event and is therefore not assigned a query or an *RST value.

Example: `"SYST:ERR:CLE:ALL?"`

Characteristics: *RST value: –
SCPI: device specific

Mode: all

SYSTem:PASSword[:CENable] <string>

This command enables access to the service functions by means of the password.

Example: `"SYST:PASS 'XXXX'"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

This command is an event and is therefore not assigned an *RST value and has no query.

SYSTem:PRESet

This command initiates an instrument reset.

The effect of this command corresponds to that of the *PRESET* key with manual control or to the *RST command.

Example: `"SYST:PRES"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

SYSTem:SET <block>

The query `SYSTem:SET?` causes the data of the current instrument setting to be transmitted to the control computer in binary format (SAVE function). The data can be read back into the instrument (RECALL function) by means of command `SYSTem:SET` <block>. Whilst the data records are stored on the instrument harddisk with SAVE/RECALL (`MMEMory:STORe` bzw. `MMEMory:LOAD`), it is possible to store the data in an external computer by means of `SYSTem:SET`.

The receive terminator has to be set to EOI to ensure reliable transfer of data (setting `SYST:COMM:GPIB:RTER EOI`).

Example: `"SYST:SET "`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

SYSTem:SPEaker:VOLume 0 to 1

This command sets the volume of the built-in loudspeaker for demodulated signals. Minimum volume is set by 0 and maximum volume by 1.

The value 0 is the lowest volume, the value 1 the highest volume.

Example: `"SYST:SPE:VOL 0.5"`

Characteristics: *RST value: 0
SCPI: device-specific

Mode: all

The command is only available with the audio demodulator option (FSP-B3).

SYSTem:TIME 0 to 23, 0 to 59, 0 to 59

This command sets the internal clock. The sequence of entry is hour, minute, second.

Example: `"SYST:TIME 12,30,30"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

SYSTem:VERSion?

This command queries the number of the SCPI version, which is relevant for the instrument.

Example: `"SYST:VERS?"`

Characteristics: *RST value: –
SCPI: conforming

Mode: all

This command is a query and is therefore not assigned an *RST value.

TRACe Subsystem

The TRACe subsystem controls access to the instrument's internal trace memory.

COMMAND	PARAMETERS	UNIT	COMMENT
TRACe<1|2>			
[:DATA]	TRACE1|TRACE2|TRACE3,<block>|<numeric_value>...	-	
:COPY	TRACE1|TRACE2|TRACE3, TRACE1|TRACE2|TRACE3	-	
:IQ			
:DATA?			nur Abfrage
:MEMory?	<numeric_value>, <numeric_value>	-- , --	nur Abfrage
:SET	NORMal, <numeric_value>, <numeric_value>, IMMediate | EXTernal, POSitive, <numeric_value>, <numeric_value>	--, HZ, HZ, --, --, --, --	
:SRATe	<numeric_value>	HZ	
[:STATe]	<Boolean>		

General Trace Commands

TRACe[:DATA] TRACE1| TRACE2| TRACE3, <block> | <numeric_value>

This command transfers trace data from the control computer to the instrument, the query reads trace data out of the instrument. The associated measurement window is selected with the numeric suffix of TRACe<1|2>.

Example:
```
"TRAC TRACE1,"+A$    (A$: data list in the current format)
"TRAC? TRACE1"
```

Characteristics: *RST value: -
SCPI: conforming

Mode: all

The trace data are transferred in the current format (corresponding to the command FORMat ASCii|REAL). The device-internal trace memory is addressed using the trace names 'TRACE1' to 'TRACE3'.
The transfer of trace data from the control computer to the instrument takes place by indicating the trace name and then the data to be transferred. In ASCII format, these data are values separated by commas. If the transfer takes place using the format real (REAL,32), the data are transferred in block format.

The parameter of the query is the trace name TRACE1 to TRACE3, it indicates which trace memory will be read out.

Saving and recalling trace data together with the device settings to/from the device-internal hard disk or to/from a floppy is controlled via the commands "`MMEMory:STORe:STATe`" and "`MMEMory:LOAD:STATe`" respectively. Trace data are selected with "`MMEMory:SELect[:ITEM]:ALL`" or ""`MMEMory:SELect[:ITEM]:TRACe`". Trace data in ASCII format (ASCCII FILE EXPORT) are exported with the command "`MMEM:STORe:TRACe`".

The transfer format for the trace data depends on the instrument setting:

Analyzer mode (span > 0 and zero span):

501 results are output in the unit selected for display.

Note: *With AUTO PEAK detector, only positive peak values can be read out. Trace data can be written into the instrument with logarithmic display only in dBm, with linear display only in volts.*

FORMAT REAL,32 is to be used as format for binary transmission.

TRACe:COPY TRACe:COPY TRACE1| TRACE2| TRACE3| TRACE4 , TRACE1| TRACE2| TRACE3| TRACE4

This command copies data from one trace to another. The second operand describes the source, the first operand the destination of the data to be copied.The associated measurement window is selected with the numeric suffix of TRACe<1|2>.

Example: `"TRAC:COPY TRACE1,TRACE2"`

Characteristics: *RST value:
SCPI: conforming

Mode: all

This command is an event and therefore has no query and no *RST value assigned.

TRACe:IQ-Subsystem

The commands of this subsystem are used for collection and output of measured IQ data. A special memory is therefore available in the FSP with 128k words for the I and Q data. The measurement is always performed in the time domain (span = 0 Hz) at the selected center frequency. The number of samples to be collected can be set. The sample rate can be set in the range from 15.625 kHz to 32 MHz. Prior to being stored in memory or output via GPIB, the measurement data are corrected in terms of frequency response.

Depending on the sample rate, the following maximum bandwidths can be obtained during the measurement.

Sample rate	Max. bandwidth	Notes
32 MHz	9.6 MHz	
16 MHz	7.72 MHz	
8 MHz	4.8 MHz	Signals outside the given bandwidth are folded back into the useful band due to the anti-aliasing filter.
4 MHz	2.8 MHz	
2 MHz	1.6 MHz	max. Bandwidth = 0.8 * Sample Rate for Sample Rate ≤ 2 MHz
1 MHz	800 kHz	
500 kHz	400 kHz	
250 kHz	200 kHz	
125 kHz	100 kHz	
62.5 kHz	50 kHz	
31.25 kHz	25 kHz	
15.625 kHz	12.5 kHz	

Due to the sampling concept (21.4 MHz IF, 32 MHz Sampling rate), the image frequency is suppressed only by the 10 MHz analog IF filter. When applying an input signal at the edge of the 10 MHz band (+5 MHz from center), the image frequency appears 800 kHz above the input signal.
The image frequency in MHz is calculated as follows:

$$f_{image} = 2 \cdot (f_{center} + 5.4\,MHz) - f_{signal}$$

where
f_{image} = image frequency in MHz
f_{center} = center frequency of the FSP in MHz
f_{signal} = frequency of the signal to be measured in MHz

For correct operation the RF input signal shall be limited in bandwidth. Signals more than 5.4 MHz above the FSP center frequency will be mirrored into the ± 5 MHz pass band.

For additional bandwidth limitation of the measurement data the analog filters (RBW ≥ 300 kHz) are available.

The trigger mode can be selected between FREE RUN and EXTERNAL. With external trigger the number of samples to be measured before the trigger point can be selected (this value has to be set to 0 for free run trigger mode).

The measurement results will be output as a list of values, with the Q-values following immediately after the list of I-values in the output buffer. The FORMAT command can be used to select between binary output (32 Bit IEEE 754 floating point values) and output in ASCII format.

The commands of this subsystem can be used in two ways:

1. Measurement and result query with one command:
   This method causes the least delay between measurement and output of the result data, but iit requires the control computer to wait actively for the response data.
2. Setting up the instrument, start of the measurement via "INIT" and query of the result list at the end of the measurement:
   With this method the control computer can be used for other activities during the measurement. In this case the additional time needed for synchronisation via service request must be taken into account.

TRACe<1|2>:IQ:DATA?

This command starts a measurement with the settings defined via TRACe:IQ:SET and returns the list of measurement results immediately after they are corrected in terms of frequency response. The number of measurement results depends on the settings defined with TRACe:IQ:SET, the output format depends on the settings of the FORMat – subsystem.

Note:

The command requires that all response data are read out completely before the instrument accepts further commands.

Parameter: none

Example:

```
'Enable acquisition of I/Q data
"TRAC:IQ:STAT ON"
'Measurement configuration:
'Filtertype:  Normal
'RBW:         10 MHz
'Sample Rate: 32 MHz
'Trigger Source:     External
'Trigger Slope:      Positive
'Pretrigger Samples: 0
'# of Samples:4096

"TRAC:IQ:SET  NORM,10MHz,32MHz,EXT,POS,0,4096"
'Select format of response data
"FORMat       REAL,32"
'Start measurement and read results:
"TRAC:IQ:DATA?"
```

Return values:

The result values are scaled linear in unit *Volt* and correspond to the voltage at the RF input of the instrument.

ASCII-Format (FORMat ASCII):

In this case the command returns a comma separated list of the measured voltage values in floating point format (Comma Separated Values = CSV). The number of values returned is 2 * number of samples, the first half being the I-values, the second half the Q-values.

Binary-Format (FORMat REAL,32):

In this case the command returns binary data (Definite Length Block Data according to IEEE 488.2), with the lists of I- and Q-data being arranged one after the other in 32 Bit IEEE 754 floating point data. The scheme of the response string is as follows:

#41024<I-value1><I-value2>...<I-value128><Q-value1><Q-value2>...<Q-value128>

with

#4	digits of the subsequent number of data bytes (4 in the example)
1024	number of subsequent data bytes (*# of DataBytes*, 1024 in the example)
<I-value x>	4-Byte-Floating Point I-value
<Q-value y>	4-Byte-Floating Point Q-value

The number of I- and Q-data can be calculated as follows:

$$\#\ of\ I-Data\ =\ \#\ of\ Q-Data\ =\ \frac{\#\ of\ DataBytes}{8}$$

The offset of Q-data in the output buffer can be calculated as follows:

$$Q-Data-Offset\ =\ \frac{(\#\ of\ DataBytes)}{2}+LengthIndicatorDigits$$

with LengthIndicatorDigits being the number of digits of the length indicator including the '#'. In the example above (#41024...) this results in a value of 6 for LengthIndicatorDigits and the offset for the Q-data will result in 512 + 6 = 518.

Characteristics: *RST-Value: --

Note:
*Using the command with the *RST-values for command TRAC:IQ:SET the following minimum buffer sizes for the response data are recommended:*
ASCII format:10 kBytes
Binary format:2 kBytes

SCPI: device specific

Mode: A-T

TRACe<1|2>:IQ:DATA:MEMory? <offset samples>,<# of samples>

This command permits the readout of previously acquired (and frequency response corrected) I/Q data from the memory, with indication of the offset related to the start of measurement and with indication of the number of measurement values. Therefore a previously acquired data set can be read out in smaller portions. The maximum amount of available data depends on the settings of command `TRACe:IQ:SET`, the output format on the settings in the `FORMat` – subsystem.

Note:
The command requires that all response data are read out completely before the instrument accepts further commands.

If there are not I/Q data available in memory because the corresponding measurement had not been started, the command will cause a Query Error.

Parameter:

<offset samples> Offset of the values to be read related to the start of the acquired data.

Value range: 0 to <# of samples> - 1,

with <# of samples> being the value indicated with command TRACe:IQ:SET.

<# of samples> Number of measurement values to be read.

Value range: 1 to <# of samples> - <offset samples>

with <# of samples> being the value indicated with command TRACe:IQ:SET.

Examples:

```
'Enable acquisition of I/Q data
"TRAC:IQ:STAT ON"
'Configure measurement:
'Filtertyp:    Normal
'RBW:          10 MHz
'Sample Rate:  32 MHz
'Trigger Source:      External
'Trigger Slope:       Positive
'Pretrigger Samples:  100
'# of Samples:4096

"TRAC:IQ:SET NORM,10MHz,32MHz,EXT,POS,100,4096"
'Start measurement and wait for sync
"INIT;*WAI"
'Determine output format
"FORMat                          REAL,32"
'Read results:
"TRAC:IQ:DATA:MEM? 0,2048"       'Reads 2048 I/Q data starting at the
                                 'beginning of data acquisition
"TRAC:IQ:DATA:MEM? 2048,1024"  'Reads 1024 I/Q data from half of the
                                 'recorded data
"TRAC:IQ:DATA:MEM? 100,512"      'Reads 512 I/Q data starting at the
                                 'trigger point(<Pretrigger Samples> was
                                 100)
```

Return values:

The result values are scaled linear in unit *Volt* and correspond to the voltage at the RF input of the instrument.

The format of the output buffer corresponds to the command `TRACe:IQ:DATA?`

Characteristics: *RST-value: --
SCPI: device specific

Mode: A-T

TRACe<1|2>:IQ:SET <filter type>,<rbw>,<sample rate>,<trigger source>,<trigger slope>,
<pretrigger samples>,<# of samples>

This command defines the settings of the analyzer hardware for the measurement of I/Q data. This allows setting the bandwidth of the analog filters in front of the A/D converter as well as setting the sample rate, trigger conditions and the record length.

Note:
If this command is omitted, the FSP will use the current analyzer settings for the corresponding parameters.

Parameter:

<filter type>: NORMAL selects the analog analyzer resolution filters as filter type. This is currently the only available filter type.

<rbw>: Bandwidth of the analog filters in front of the A/D converter.

Value range: 300 kHz – 10 MHz in steps of 1, 3, 10 for <filter type> = NORMal<sample rate>: Sampling rate for the data acquisition.

Value range: 15.625 kHz, 31.25 kHz, 62.5 kHz,
125 kHz, 250 kHz, 500 kHz,
1 MHz, 2 MHz, 4 MHz, 8 MHz, 16 MHz,
32 MHz for <filter type> = NORMal

<trigger mode>: Selection of the trigger source used for the measurement.

Values: IMMediate | EXTernal

<trigger slope>: Used trigger slope.

Values: POSitive (currently the only value supported)

<pretrigger samples>: Number of measurement values to be recorded before the trigger point.

Value range: 0 to 65023 (= 64*1024 – 512 - 1)

Note:
For <trigger mode> = IMMediate the value must be 0.

<# of samples>: Number of measurement values to record.

Value range:1 to 130560 (= 128*1024 – 512)

Examples:

`"TRAC:IQ:SET NORM,10MHz,32MHz,EXT,POS,0,2048"`	Reads 2048 I/Q-values starting at the trigger point. Filtertype: NORMAL (analog) RBW: 10 MHz Sample Rate: 32 MHz Trigger: External Slope: Positive
`"TRAC:IQ:SET NORM,1MHz,4MHz,EXT,POS,1024,512"`	Reads 512 I/Q-values from 1024 measurement points before the trigger point. Filtertype: NORMAL (analog) RBW: 1 MHz Sample Rate: 4 MHz Trigger: External Slope: Positive

Characteristics: *RST-values: `NORM,3MHz,32MHz,IMM,POS,0,128`

Note:
For using these default settings with command TRAC:IQ:DATA? the following minimum buffer sizes for the response data are recommended:
ASCII format:10 kBytes
Binary format:2 kBytes

SCPI: device specific

Mode: A-T

TRACe<1|2>:IQ:SRATe 15.625kHz...32MHz

This command sets the sampling rate for the I/Q data acquisition. Thus the sample rate can be modified without affecting the other settings.

Value range: 15.625 kHz, 31.25 kHz, 62.5 kHz,
125 kHz, 250 kHz, 500 kHz,
1 MHz, 2 MHz, 4 MHz, 8 MHz, 16 MHz, 32 MHz

Example: `"TRAC:IQ:SRAT 4MHZ"`

Characteristics: *RST-value: 32 MHz
SCPI: device specific

Betriebsart: A-T

TRACe<1|2>:IQ[:STATe] ON|OFF

This command switches the I/Q data acquisition on or off.

Note:
The I/Q data acquisition is not compatible with other measurement functions. Therefore all other measurement functions will be switched off as soon as the I/Q measurement function is switched on. Additionally a trace display is not possible in this operating mode. Therefore all traces are set to "BLANK". Finally split screen operation will automatically be stopped.

Example:

`TRAC:IQ ON` Switches on I/Q data acquisition

Characteristics: *RST-value: OFF
SCPI: device specific

Mode: A-T

TRIGger Subsystem

The TRIGger subsystem is used to synchronize instrument actions with events. It is thus possible to control and synchronize the start of a sweep. An external trigger signal can be applied to the connector at the rear panel of the instrument. A distinction is made between TRIGger1 (screen A) and TRIGger2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
TRIGger<1|2>			
[:SEQuence]			
:SOURce	IMMediate | VIDeo | IFPower | EXTernal		
:LEVel			
:VIDeo	<numeric_value>	PCT	
:HOLDoff	<numeric_value>	S	
:SLOPe	POSitive|NEGative	--	

TRIGger<1|2>[:SEQuence]:SOURce IMMediate | EXTernal | VIDeo | IFPower

This command selects the trigger source for the start of a sweep.

Parameter:
- IMMediate = automatic triggering the next measurement at the end of the previous one.The value IMMediate corresponds to the FREE RUN setting.
- EXTernal = the next measurement is triggered by the signal at the external trigger input.
- VIDeo = the next measurement is triggered by the detection of a signal at the video filter output.
- IFPower = the next measurement is triggered by the detection of a signal at the instrument IF (10 MHz bandwidth)

Example: `"TRIG:SOUR EXT"` selects the external trigger input as source of the trigger signal

Characteristics: *RST value: IMMediate
SCPI: conforming

Mode: all

TRIGger<1|2>[:SEQuence]:LEVel:VIDeo 0 to 100PCT

This command sets the level of the video trigger source.

Example: `"TRIG:LEV:VID 50PCT"`

Characteristics: *RST value: 50 PCT
SCPI: device-specific

Mode: all

TRIGger<1|2>[:SEQuence]:HOLDoff -100 to 100s

This command defines the length of the trigger delay.

A negative delay time (pretrigger) can be set in the time domain (span < 0 Hz) only. The maximum possible range and the maximum effective resolution of the pretrigger are limited by the set sweep time (max range= - 499/500 x sweep time; max. resolution = sweep time/500). Pretriggering is not possible when the RMS or the average detector is activated.

Example: `"TRIG:HOLD 500us"`

Characteristics: *RST value: 0s
SCPI: conforming

Mode: all

TRIGger<1|2>[:SEQuence]:SLOPe POSitive | NEGative

This command selects the slope of the trigger signal. The selected trigger slope applies to all trigger signal sources .

Exapmple: `"TRIG:SLOP NEG"`

Characteristics: *RST value: POSitive
SCPI: conforming

Mode: all

UNIT Subsystem

The UNIT subsystem is used to switch the basic unit of setting parameters. A distinction is made between UNIT1 (screen A) and UNIT2 (screen B).

COMMAND	PARAMETERS	UNIT	COMMENT
UNIT<1|2> :POWer	DBM | V | A | W | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere		

UNIT<1|2>:POWer DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | V | A | W

This command selects the default unit for the selected measurement window.

Example: `"UNIT:POW DBUV"` Sets the power unit for screen A to dBm.

Characteristics: *RST value: DBM
SCPI: conforming

Mode: A

Supported GPIB Commands of the HP 8590 Series

The FSP analyzer family has the capability to support a subset of the HP 8590 GPIB command set. Due to the differences in system architecture and features this can only be a limited support that comes to its limits where the corresponding parameters differ in their value ranges or default values or where hardware dependencies have to be taken into account. Nevertheless in many cases the subset supported by the FSP will make the adaption of existing GPIB programs for use with the FSP easier.

Supported Command Subset

Function Category	Function	HP 8590 Command	Supported Subset	Known differences
Amplitude				
	Attenuation	AT	AT <numeric_value> DB AT DN AT UP AT AUTO AT?	AT DN/UP: Stepsizes if option FSP-B25 is present. AT AUTO: Dependency calculation
	Amplitude Units	AUNITS	AUNITS DBM | DBMV | DBUV AUNITS?	
	Input Impedance	INZ	INZ 75 INZ 50 INZ?	
	Amplitude Scale Log	LG	LG <numeric_value> DB LG?	
	Amplitude Scale Lin	LN	LN	
	Reference Level	RL	RL <numeric_value> DB|DM RL DN RL UP RL?	Stepsize and default value
	Reference Level Position	RLPOS	RLPOS <numeric_value> RLPOS DN RLPOS UP RLPOS?	On the FSP this function affects the Reference Level Position also if tracking generator normalization is inactive.
	Reference Level Offset	ROFFSET	ROFFSET <numeric_value> DB ROFFSET?	
Auxiliary Control				
	AF Demodulator	DEMOD	DEMOD ON|OFF|AM|FM	requires Option FSP-B3 only
	Normalized Reference Level	NRL	NRL <numeric_value> DB NRL?	requires Option FSP-B9 or FSP-B10
	Source Normalization	SRCNORM	SRCNORM ON|OFF SRCNORM 1|0	requires Option FSP-B9 or FSP-B10
	Source Power Offset	SRCPOFS	SRCPOFS <numeric_value> DB SRCPOFS DN SRCPOFS UP SRCPOFS?	requires Option FSP-B9 or FSP-B10
	Source Power	SRCPWR	SRCPWR <numeric_value> DB SRCPWR DN SRCPWR UP SRCPWR ON SRCPWR OFF SRCPWR?	requires Option FSP-B9 or FSP-B10

Function Category	Function	HP 8590 Command	Supported Subset	Known differences
Bandwidth				
	Resolution Bandwidth	RB	RB <numeric_value> HZ|KHZ|MHZ|GHZ RB DN RB UP RB AUTO RB?	Value range. Formula for dependent parameters (video bandwidth, sweeptime).
	Video Bandwidth	VB	VB <numeric_value> HZ|KHZ|MHZ|GHZ VB DN VB UP VB AUTO VB?	Value range. Formula for dependent parameters (sweeptime).
	Video Bandwidth Ratio	VBR	VBR <numeric_value> VBR DN VBR UP VBR?	Default value.
Calibration				
	Start analyzer self alignment	CAL	CAL ALL CAL ON CAL OFF	The CAL commands do not automatically set the command complete bit (Bit 4) in the status byte. An additional DONE is required for that purpose.
Configuration				
	Time Display	TIMEDSP	TIMEDSP ON|OFF TIMEDSP 1|0 TIMEDSP?	
Display				
	Annotation	ANNOT	ANNOT ON|OFF ANNOT 1|0 ANNOT?	Only frequency axis annotation is affected.
	Threshold	TH	TH <numeric_value> DB|DM TH DN TH UP TH ON TH OFF TH AUTO TH?	Default value is different. Threshold line has no effect on trace data (TH AUTO is always active).
Frequency				
	Center Frequency	CF	CF <numeric_value> HZ|KHZ|MHZ|GHZ CF UP CF DN CF?	Default value. Range. Stepsize.
	Start Frequency	FA	FA <numeric_value> HZ|KHZ|MHZ|GHZ FA UP FA DN FA?	Range. Stepsize.
	Stop Frequency	FB	FB <numeric_value> HZ|KHZ|MHZ|GHZ FB UP FB DN FB?	Default value. Range. Stepsize.
	Frequency Offset	FOFFSET	FOFFSET <numeric_value> HZ|KHZ|MHZ|GHZ FOFFSET?	

Function Category	Function	HP 8590 Command	Supported Subset	Known differences
	CF Step Size	SS	SS <numeric_value> HZ|KHZ|MHZ|GHZ SS DN SS UP SS AUTO SS?	Stepsize.
Information				
	Clear all status bits	CLS	CLS	
	Service Request Bit mask	RQS	RQS	Bits supported: 1 (Units key pressed) 2 (End of Sweep) 3 (Device error) 4 (Command complete) 5 (Illegal command)
	Status byte query	STB	STB	Status bits will be mapped as stated under RQS *Note:* *Bit 2 and 4 will always be set together if "Command complete" or "End of Sweep" is detected. The FSP cannot distinguish between these two conditions. Additionally these bits cannot be used for synchronisation on the sweep end in continuous sweep mode.* The status byte obtained by a serial poll will always be conforming to IEEE 488.2 / SCPI.
Marker				
	Marker Frequency Query	MF	MF MF?	
	Set Marker Frequency	MKF	MKF <numeric_value> HZ|KHZ|MHZ|GHZ MKF?	
	Marker Amplitude	MKA	MKA?	
	Select the active marker	MKACT	MKACT 1 MKACT?	Only marker 1 is supported as the active marker.
	N dB Down	MKBW	MKBW <numeric_value> MKBW ON MKBW OFF	Different default value.
	Center Freq = Marker Freq	MKCF	MKCF	
	Delta Marker	MKD	MKD <numeric_value> HZ|KHZ|MHZ|GHZ MKD DN MKD UP MKD ON MKD OFF	Only Deltamarker 1 is supported. Different default value. Different stepsize.
	Frequency Counter	MKFC	MKFC ON|OFF MKFC 1|0	
	Frequency Counter Resolution	MKFCR	MKFCR <numeric_value> HZ|KHZ|MHZ|GHZ MKFCR DN MKFCR UP MKFCR?	

Function Category	Function	HP 8590 Command	Supported Subset	Known differences
	Marker -> Min	MKMIN	MKMIN	
	Normal Marker	MKN	MKN <numeric_value> HZ|KHZ|MHZ|GHZ MKN DN MKN UP MKN ON MKN OFF MKN?	
	Noise Measurement	MKNOISE	MKNOISE ON|OFF MKNOISE 1|0 MKNOISE?	
	Marker off	MKOFF	MKOFF MKOFF ALL	
	Marker Search	MKPK	MKPK MKPK HI MKPK NH MKPK NR MKPK NL	
	Peak Excursion	MKPX	MKPX <numeric_value> DB MKPX DN MKPX UP MKPX?	Different stepsize.
	Ref Level = Marker Level	MKRL	MKRL	
	CF Stepsize = Marker Freq	MKSS	MKSS	
	Marker to Trace	MKTRACE	MKTRACE TRA|TRB|TRC	
	Signal Track	MKTRACK	MKTRACK ON|OFF MKTRACK 1|0 MKTRACK?	
Preset				
	Instrument preset	IP	IP	Does not reset the status reporting information.*RST
Printer				
	Hardcopy	PRINT	PRINT	
Program Flow				
	Stop previous function	ABORT	ABORT	Does not automatically set the command complete bit (Bit 4) in the status byte. An additional DONE is required for that purpose.
Recall or Save				
	Recall analyzer state	RCLS	RCLS <numeric_value>	
	Save analyzer state	SAVES	SAVES <numeric_value>	

Function Category	Function	HP 8590 Command	Supported Subset	Known differences
Span				
	Full Span	FS	FS	Full span value.
	Frequency Span value	SP	SP <numeric_value> SP DN SP UP SP?	Default value. Stepsize. Formula for dependent values (Resolution Bandwidth, Video Bandwidth, Sweeptime)
Sweep				
	Continuous Sweep Mode	CONTS	CONTS	
	Single Sweep	SNGLS	SNGLS	
	Gated Sweep On/Off	GATE	GATE ON|OFF GATE 1|0	
	Gate Mode Edge/Level	GATECTL	GATECTL EDGE|LEVEL GATECTL?	
	Gate delay	GD	GD <numeric_value> US|MS|SC GD DN GD UP GD?	
	Gate length	GL	GL <numeric_value> US|MS|SC GL DN GL UP GL?	
	Gate polarity	GP	GP POS|NEG GP?	
	Sweep time value	ST	ST <numeric_value> US|MS|SC ST DN ST UP ST AUTO ST?	SWE:TIME Valid values. Range. Stepsize
Synchroni-zation				
	Synchronization on end of all previous commands	DONE	DONE DONE?	
	Start and complete a Full Sweep	TS	TS	Only available in single sweep mode

Function Category	Function	HP 8590 Command	Supported Subset	Known differences
Trace				
	Trace difference w. display line	AMBPL	AMBPL ON|OFF AMBPL 1|0 AMBPL?	
	Trace Position (Display Line)	DL	DL <numeric_value> DB|DM DL DN DL UP DL ON DL OFF DL?	The display line function is only supported in terms of trace position on the screen and video trigger level. The general display line function does not exist on the FSP. ON/OFF are accepted, but ignored; the line is automatically switched on/off with AMBPL ON/OFF. Its default position is different.
	Trace Blank	BLANK	BLANK TRA|TRB|TRC	
	Trace Copy	MOV	MOV TRA|TRB|TRC,TRA|TRB|TRC	
	Trace Clear/Write	CLRW	CLRW TRA|TRB|TRC	
	Detector selection	DET	DET POS|SMP|NEG DET?	DET? returns SAMP instead of SMP on the FSP. DET not automatically set the command complete bit (Bit 4) in the status byte. An additional DONE is required for that purpose.
	Trace Max Hold	MXMH	MXMH TRA|TRB	
	Trace Min Hold	MINH	MINH TRC	
	Video Averaging	VAVG	VAVG TRA|TRB|TRC	
	Trace View	VIEW	VIEW TRA|TRB|TRC	
Trigger				
	Trigger Mode	TM	TM FREE|VID|EXT TM?	
	Start new sweep	TS	TS	

Differences in Status Reporting

The major difference in status reporting between the FSP and the HP 8590 analyzers is that the FSP has a hierarchical status reporting system conforming to IEEE 488.2/SCPI, whereas the HP 8590 series has a very simple status reporting system that consists simply of the bit patterns in the status byte.
As described above, for the RQS and STB command the bit mapping of the HP 8590 analyzers is supported as described in the table below. For the status byte returned by a serial poll the bit mapping is different on the FSP. In detail this means that all of the bits enabled by the RQS command will be mapped onto **bit 5** of the Service Request Status Byte of the FSP.
This mechanism makes sure that a Service Request is generated as soon as one of the conditions enabled becomes true.
What the Service Request Routine should do rather than evaluating the return value of a serial poll is to use the STB command in order to identify the reason for the service request. The bits returned by the STB command are mapped in the same way as for the RQS command.

Bit enabled by RQS	Bit set in the status byte on serial poll
1 (Units key pressed)	5 (Event Status Register Summary Bit)
2 (End of Sweep)	5 (Event Status Register Summary Bit)
3 (Device Error)	5 (Event Status Register Summary Bit)
4 (Command Complete)	5 (Event Status Register Summary Bit)
5 (Illegal Command)	5 (Event Status Register Summary Bit)

What needs to be noted is that the FSP will notify any key pressed on the frontpanel rather than only the unit keys if bit 1 is set by the RQS command.
Additionally there is a difference in the handling of bit 6. This bit reflects the status of the SRQ line of the GPIB bus on the HP 8590 analyzers. With the FSP this is not possible. Therefore this bit will be set as soon as any of the bits 1 to 5 is set, but it will not be cleared on a serial poll.

Differences in GPIB behavior between the FSP and the FSE families of instruments

The following list of commands contains the differences in syntax and behavior between the GPIB command set of the FSP and the FSE families of instruments. FSE alone in column "Devices" denotes the instrument families FSE, FSIQ, FSET and ESI, unless otherwise noted in column "Notes".

Devices	Command	Parameter	Notes
FSP + FSE	*CAL?		FSP: executes total calibration FSE: executes short calibration
FSP + FSE	*CLS		
FSP + FSE	*ESE		
FSP + FSE	*ESR?		
FSP + FSE	*IDN?		model indicator and version index is different for FSP and FSE
FSP + FSE	*IST?		
FSP + FSE	*OPC?		
FSP + FSE	*OPT?		list of available options is slightly different for FSP and FSE, but equally available options have equal names
FSP + FSE	*PCB		
FSP + FSE	*PRE		
FSP + FSE	*PSC		
FSP + FSE	*RST		instrument settings are slightly different for FSP and FSE due to different instrument specs
FSP + FSE	*SRE		
FSP + FSE	*STB?		
FSP + FSE	*TRG		FSP: starts measurement in active screen FSE: starts measurement in both screens (split screen mode)
FSP + FSE	*TST?		
FSP + FSE	*WAI		
FSP + FSE	ABORt		
FSE	CALCulate:LIMit:CATalog?		not available in FSP
FSP	CALCulate:STATistics:APD[:STATe]	ON | OFF	new function for FSP
FSP	CALCulate:STATistics:CCDF[:STATe]	ON | OFF	new function for FSP
FSP	CALCulate:STATistics:NSAMples	100 to 1E9	new function for FSP
FSP	CALCulate:STATistics:PRESet		new function for FSP
FSP	CALCulate:STATistics:Result<1...3>?	MEAN|PEAK|CFACtor| ALL	new function for FSP
FSP	CALCulate:STATistics:SCALe:AUTO	ONCE	new function for FSP
FSP	CALCulate:STATistics:X:RANGe	-10dB to 200dB	new function for FSP
FSP	CALCulate:STATistics:X:RLEVel	-130dBm to 30dBm	new function for FSP
FSP	CALCulate:STATistics:Y:LOWer	-1E-9 to 0.1	new function for FSP
FSP	CALCulate:STATistics:Y:UPPer	-1E-8 to 1.0	new function for FSP
FSE	CALCulate<1|2>:CTHReshold	MIN to MAX	not available in FSP
FSE	CALCulate<1|2>:CTHReshold:STATe	ON | OFF	not available in FSP
FSP	CALCulate<1|2>:DELTamarker<1...4>:AOFF		markers 2...4 are either normal or delta markers; marker 1 always serves as the reference marker for all deltamarkers
FSE	CALCulate<1|2>:DELTamarker<1...4>:AOFF		there are 4markers and 4 deltamarkers; the most recently used marker serves as the reference marker for all deltamarkers

Devices	Command	Parameter	Notes
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:FIXed:RPOint:X	<numeric_value>	FSP: marker 1 can be moved independently from the reference point FSE: the marker and the reference point are linked to each other
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:FIXed:RPOint:Y	<numeric_value>	FSP: marker 1 can be moved independently from the reference point; FSE: the marker and the reference point are linked to each other
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:FIXed:RPOint:Y:OFFSet	<numeric_value>	
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:FIXed[:STATe]	ON | OFF	
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:PNOise:RESult?		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:PNOise[:STATe]	ON | OFF	
FSE	CALCulate<1|2>:DELTamarker<1...4>:MAXimum:APEak		not available for FSP
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:MAXimum:LEFT		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:MAXimum:NEXT		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:MAXimum:RIGHt		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:MAXimum[:PEAK]		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:MINimum:LEFT		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:MINimum:NEXT		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:MINimum:RIGHt		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:MINimum[:PEAK]		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:MODE	ABSolute | RELative	
FSE	CALCulate<1|2>:DELTamarker<1...4>:STEP:AUTO	ON | OFF	not available for FSP
FSE	CALCulate<1|2>:DELTamarker<1...4>:STEP[:INCRement]	<numeric_value>	not available for FSP
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:TRACe	1 to 3	FSP: 3 traces are available per screen; FSE: 4 traces are available in full screen mode and 2 traces per screen in split screen mode
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:X	0 to MAX (frequency | sweep time)	unit 'SYM' is not available for FSP
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:X:RELative		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>:Y?		
FSP + FSE	CALCulate<1|2>:DELTamarker<1...4>[:STATe]	ON | OFF	
FSE	CALCulate<1|2>:DLINe<1|2>	MIN to MAX	not available for FSP
FSE	CALCulate<1|2>:DLINe<1|2>:STATe	ON | OFF	not available for FSP
FSE	CALCulate<1|2>:FEED	'XTIM:DDEM:MEAS'| 'XTIM:DDEM:REF' | 'XTIM:DDEM:ERR:MPH' | 'XTIM:DDEM:ERR:VECT' | 'XTIM:DDEM:SYMB' | 'XTIM:AM' | 'XTIM:FM' | 'XTIM:PM' | 'XTIM:AMSummary' | 'XTIM:FMSummary' |'XTIM:PMSummary' | 'TCAP'	not available for FSP
FSET	CALCulate<1|2>:FEED	'XTIM:DDEM:MEAS' | 'XTIM:DDEM:REF' | 'XTIM:DDEM:ERR:MPH' | 'XTIM:DDEM:ERR:VECT' | 'XTIM:DDEM:SYMB' | 'TCAP'	not available for FSP
FSE	CALCulate<1|2>:FLINe<1|2>	0 to fmax	not available for FSP
FSE	CALCulate<1|2>:FLINe<1|2>:STATe	ON | OFF	not available for FSP
FSE	CALCulate<1|2>:FORMat	MAGNitude | PHASe | UPHase | RIMag | FREQuency | IEYE | QEYE | TEYE | FEYE | COMP | CONS	not available for FSP
FSE	CALCulate<1|2>:FSK:DEViation:REFerence	<numeric value>	not available for FSP
FSE	CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel	0 to 100 DB, 0 to 100 DB	compatible to CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel [:RELative] of FSP not available for FSET

Devices	Command	Parameter	Notes
FSP	CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel:ABSolute	-200 to 200 DBM, -200 to 200 DBM	new function for FSP
FSP	CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel:ABSolute:STATe	ON | OFF	new function for FSP
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel:RESult?		
FSE	CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel:STATe	ON | OFF	compatible to CALCulate<1|2>:LIMit<1...8>: ACPower:ACHannel[:RELative]:STATe of FSP not available for FSET
FSP	CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel[:RELative]	0 to 100 DB, 0 to 100 DB	compatible to CALCulate<1|2>:LIMit<1...8>: ACPower:ACHannel of FSE
FSP	CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel[:RELative]:STATe	ON | OFF	compatible to CALCulate<1|2>:LIMit<1...8>: ACPower:ACHannel:STATe of FSE
FSE	CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>	0 to 100 DB, 0 to 100 DB	compatible to CALCulate<1|2>:LIMit<1...8>: ACPower:ALTernate<1|2> [:RELative] of FSP not available for FSET
FSP	CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>:ABSolute	-200 to 200 DBM, -200 to 200 DBM	new function for FSP
FSP	CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>:ABSolute:STATe	ON | OFF	new function for FSP
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>:RESult?		
FSE	CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>:STATe	ON | OFF	compatible to CALCulate<1|2>:LIMit<1...8>: ACPower:ALTernate<1|2> [:RELative]:STATe of FSP not available for FSET
FSP	CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>[:RELative]	0 to 100 DB, 0 to 100 DB	compatible to CALCulate<1|2>:LIMit<1...8>: ACPower:ALTernate<1|2> of FSE
FSP	CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>	ON | OFF	compatible to CALCulate<1|2>:LIMit<1...8>: ACPower:ALTernate<1|2>: STATe of FSE
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:ACPower[:STATe]	ON | OFF	
FSE	CALCulate<1|2>:LIMit<1...8>:BURSt:POWer?		not available for FSP, FSET and ESI
FSE	CALCulate<1|2>:LIMit<1...8>:BURSt:PTEMplate?		not available for FSP, FSET and ESI
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:CLEar[:IMMediate]		
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:COMMent	<string>	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:CONTrol:DOMain	FREQuency | TIME	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:CONTrol:MODE	RELative | ABSolute	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:CONTrol:OFFset	<numeric value>	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:CONTrol:SHIFt	<numeric_value>	
FSE	CALCulate<1|2>:LIMit<1...8>:CONTrol:SPACing	LINear | LOGarithmic	not available for FSP
FSE	CALCulate<1|2>:LIMit<1...8>:CONTrol:UNIT[:TIME]	S | SYM	not available for FSP
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:CONTrol[:DATA]	<numeric value>, <numeric value>	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:COPY	1 to 8|<name>	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:DELete		
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:FAIL?		
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:LOWer:MARGin	<numeric value>	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:LOWer:MODE	RELative | ABSolute	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:LOWer:OFFset	<numeric value>	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:LOWer:SHIFt	<numeric_value>	
FSE	CALCulate<1|2>:LIMit<1...8>:LOWer:SPACing	LINear | LOGarithmic	not available for FSP
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:LOWer:STATe	ON | OFF	
FSP	CALCulate<1|2>:LIMit<1...8>:LOWer:THReshold	<numeric value>	new function for FSP
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:LOWer[:DATA]	<numeric value>	
FSE	CALCulate<1|2>:LIMit<1...8>:MARGin	0 to 100DB	not available for FSP, FSET and ESI
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:NAME	1 to 8|<string>	

Devices	Command	Parameter	Notes
FSE	CALCulate<1|2>:LIMit<1...8>:SPECtrum:MODulation:EXCeptions?	ARFCn | TXBand | RXBand| COMBined | DCSRx1800	not available for FSP, FSET and ESI
FSE	CALCulate<1|2>:LIMit<1...8>:SPECtrum:MODulation:FAILs?	ARFCn | TXBand | RXBand| COMBined | DCSRx1800	not available for FSP, FSET and ESI
FSE	CALCulate<1|2>:LIMit<1...8>:SPECtrum:MODulation?	ARFCn | TXBand | RXBand| COMBined | DCSRx1800	not available for FSP, FSET and ESI
FSE	CALCulate<1|2>:LIMit<1...8>:SPECtrum:SWITching:FAILs?		not available for FSP, FSET and ESI
FSE	CALCulate<1|2>:LIMit<1...8>:SPECtrum:SWITching?		not available for FSP, FSET and ESI
FSE	CALCulate<1|2>:LIMit<1...8>:SPURious:FAILs?	TXBand | OTXBand| RXBand | IDLeband	not available for FSP, FSET and ESI
FSE	CALCulate<1|2>:LIMit<1...8>:SPURious?	TXBand | OTXBand| RXBand | IDLeband	not available for FSP, FSET and ESI
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:STATe	ON | OFF	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:TRACe	1 to 3	FSP: 3 traces are available per screen FSE: 4 traces are available in full screen mode and 2 traces per screen in split screen mode
FSP	CALCulate<1|2>:LIMit<1...8>:UNIT	DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | DB | DBUV_M | DBUA_M | DEG | RAD | S | HZ | PCT | UNITLESS	Available units are compatible to the FSE
FSE/ FSIQ	CALCulate<1|2>:LIMit<1...8>:UNIT	DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | DB | DBUV_MHZ | DBMV_MHZ | DBUA_MHZ | |DBUV_M | DBUA_M | DBUV_MHZ | DBUA_MHZ | DEG | RAD | S | HZ | PCT | UNITLESS	only the following units are available for the FSP:DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | DB | DBUV_M | DBUA_M | DEG | RAD | S | HZ | PCT | UNITLESS
FSET/ ESI	CALCulate<1|2>:LIMit<1...8>:UNIT	DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | DB | DBUV_MHZ | DBMV_MHZ | DBUA_MHZ | |DBUV_M | DBUA_M | DBUV_MHZ | DBUA_MHZ | DEG | RAD | S | HZ | PCT | UNITLESS	only the following units are available for the FSP:DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | DB | DBUV_M | DBUA_M | DEG | RAD | S | HZ | PCT | UNITLESS
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:UPPer:MARGin	<numeric value>	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:UPPer:MODE	RELative | ABSolute	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:UPPer:OFFset	<numeric value>	
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:UPPer:SHIFt	<numeric_value>	
FSE	CALCulate<1|2>:LIMit<1...8>:UPPer:SPACing	LINear | LOGarithmic	not available for FSP
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:UPPer:STATe	ON | OFF	
FSP	CALCulate<1|2>:LIMit<1...8>:UPPer:THReshold	<numeric value>	new function for FSP
FSP + FSE	CALCulate<1|2>:LIMit<1...8>:UPPer[:DATA]	<numeric value>	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:ZOOM	<numeric value>	FSP: function uses always marker 1 as its reference marker; FSE: all available markers can be used as a reference marker
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:AOFF		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:COUNt	ON | OFF	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:COUNt:FREQuency?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:COUNt:RESolution	0.1 | 1 | 10 | 100 | 1000 | 10000 Hz	
FSE	CALCulate<1|2>:MARKer<1...4>:COUPled[STATe]	ON | OFF	not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:ADEMod		not available for FSP and FSET
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:ADEMod:AM[:RESult]?	PPEak | MPEak | MIDDle | RMS	not available for FSP and FSET
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:ADEMod:CARRier		not available for FSP and FSET

Devices	Command	Parameter	Notes
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:ADEMod:FERRor		not available for FSP and FSET
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:ADEMod:FM	PPEak | MPEak | MIDDle | RMS | RDEV	not available for FSP and FSET
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:ADEMod:PM	PPEak | MPEak | MIDDle | RMS	not available for FSP and FSET
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:ADEMod:SINad:RESult?		not available for FSP and FSET
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:ADEMod:SINad	ON | OFF	not available for FSP and FSET
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:CENTer		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:CSTep		
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:DDEMod:RESult?	MERM | MEPK | MEPS | PERM PEPK | PEPS | EVRM | EVPK | EVPS IQOF | IQIM |ADR | FERR | FEPK | RHO | DEV | FSRM | FSPK | FSPS | DTTS	not available for FSP
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation: CONTinuous		new function for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation:HOLDoff	10ms to 1000s	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation:SELect	AM | FM	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation[:STATe]	ON | OFF	
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:MDEPth:RESult?		new function for FSP
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:MDEPth[:STATe]		new function for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:MSTep		not available for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown	<numeric value>	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown:FREQuency?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown:STATe	ON | OFF	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:NOISe:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:NOISe:STATe	ON | OFF	
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:CFILter	ON | OFF	not available for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:PRESet	NADC | TETRA | PDC | PHS | CDPD | FWCDma | RWCDma | F8CDma | R8CDma | F19Cdma | R19Cdma | FW3Gppcdma| RW3Gppcdma | D2CDma | S2CDma | M2CDma | NONE	available standards are compatible to the FSE
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:RESult:PHZ	ON | OFF	new function for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:RESult?	ACPower | CPOWer | OBANdwidth | OBWidth	CN and CN0 are not available on the FSP ACPower and CPOWer are not available on the FSET
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:SELect?	ACPower | CPOWer | OBANdwidth | OBWidth	CN and CN0 are not available on the FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:SELect?	ACPower | CPOWer | OBANdwidth | OBWidth | CN | CN0	CN and CN0 are not available on the FSP and FSET
FSET	CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:SELect?	OBANdwidth | OBWidth	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer[:STATe]	OFF	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:REFerence		
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SFACtor	(60dB/3dB) | (60dB/6dB)	not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SFACtor:FREQuency?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SFACtor:RESult?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SFACtor:STATe	ON | OFF	not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:STARt		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:STOP		not available for FSP
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack: BANDwidth|BWIDth	10 Hz to MAX(span)	new function for FSP. Replaces DISP:FLINE of the FSE.
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack:THReshold	-330 to +30 dBm	new function for FSP
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack:TRACe	1 to 3	new function for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack[:STATe]	ON | OFF	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:AOFF		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:AVERage	ON | OFF	

Devices	Command	Parameter	Notes
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MAXimum:AVERage:RESult?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MAXimum:PHOLd:RESult?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MAXimum:RESult?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MAXimum[:STATe]	ON | OFF	not available for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN:AVERage:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN:PHOLd:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN[:STATe]	ON | OFF	
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MIDDle:AVERage:RESult?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MIDDle:PHOLd:RESult?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MIDDle: RESult?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MIDDle [:STATe]	ON | OFF	not available for FSP
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MODE	ABSolute | RELative	new function for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MPEak:AVERage:RESult?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MPEak:PHOLd:RESult?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MPEak: RESult?		not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MPEak [:STATe]	ON | OFF	not available for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PHOLd	ON | OFF	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak:AVERage:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak:PHOLd:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak[:STATe]	ON | OFF	
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:REFerence:AUTO	ONCE	new function for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS:AVERage:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS:PHOLd:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS:RESult?		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS[:STATe]	ON | OFF	
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation:RESult?		new function for FSP
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMarySDEViation:AVERage:RESult?		new function for FSP
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation:PHOLd:RESult?		new function for FSP
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation[:STATe]	ON | OFF	new function for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary[:STATe]	ON | OFF	
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:TOI:RESult?		new function for FSP
FSP	CALCulate<1|2>:MARKer<1...4>:FUNCtion:TOI[:STATe]	ON | OFF	new function for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:LOEXclude	ON | OFF	
FSE	CALCulate<1|2>:MARKer<1...4>:MAXimum:APEak		not available for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:MAXimum:LEFT		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:MAXimum:NEXT		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:MAXimum:RIGHt		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:MAXimum[:PEAK]		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:MINimum:LEFT		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:MINimum:NEXT		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:MINimum:RIGHt		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:MINimum[:PEAK]		
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:PEXCursion	<numeric value>	
FSE	CALCulate<1|2>:MARKer<1...4>:READout	MPHase | RIMaginary	not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:SCOupled[STATe]	ON | OFF	not available for FSP
FSE	CALCulate<1|2>:MARKer<1...4>:STEP:AUTO	ON | OFF	not available for FSP

Devices	Command	Parameter	Notes
FSE	CALCulate<1|2>:MARKer<1...4>:STEP[:INCRement]	<numeric_value>	not available for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:TRACe	1 to 3	FSP: 3 traces are available per screen FSE: 4 traces are available in full screen mode and 2 traces per screen in split screen mode
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:X	0 to MAX (frequency| sweep time)	additional unit SYM is available for FSE
FSP	CALCulate<1|2>:MARKer<1...4>:X:SLIMits:LEFT	0 to MAX (frequency|sweep time)	new function for FSP. Replaces DISP:FLIN and DISP:TLIN commands of the FSE
FSP	CALCulate<1|2>:MARKer<1...4>:X:SLIMits:RIGHt	0 to MAX (frequency|sweep time)	new function for FSP. Replaces DISP:FLIN and DISP:TLIN commands of the FSE
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:X:SLIMits[:STATe]	ON | OFF	
FSP + FSE	CALCulate<1|2>:MARKer<1...4>:Y?		
FSP	CALCulate<1|2>:MARKer<1...4>:Y:PERCent	<numeric_value>	new function for FSP
FSP + FSE	CALCulate<1|2>:MARKer<1...4>[:STATe]	ON | OFF	
FSP	CALCulate<1|2>:MATH:MODE	LINear | LOGarithmic	affects all traces on the FSP; therefore the numeric suffix :MATH<1...4> is not allowed for the FSP
FSE	CALCulate<1|2>:MATH<1...4>:MODE	LINear | LOGarithmic	for FSE, only the trace indicated by a numeric suffix is affected
FSP	CALCulate<1|2>:MATH:POS	-100PCT to 200PCT	new function for FSP; replacement for CALC:RLINe of the FSE
FSP + FSE	CALCulate<1|2>:MATH:STATe	ON | OFF	for FSP, traces can only be subtracted from trace 1; therefore there is no numeric suffix behind :MATH
FSP + FSE	CALCulate<1|2>:MATH[:EXPRession][:DEFine]	<expr>	for FSP, traces can only be subtracted from trace 1; therefore there is no numeric suffix behind :MATH and <expr> may only consist of (TRACE1-TRACE2) or (TRACE1-TRACE3)
FSE	CALCulate<1|2>:RLINe	MIN to MAX	not available for FSP (replaced by CALC:MATH:POS)
FSE	CALCulate<1|2>:RLINe:STATe	ON | OFF	not available for FSP (replaced by CALC:MATH:POS)
FSP + FSE	CALCulate<1|2>:THReshold	MIN to MAX	
FSP + FSE	CALCulate<1|2>:THReshold:STATe	ON | OFF	
FSE	CALCulate<1|2>:TLINe<1|2>	0 to 1000s	not available on the FSP; replaced by CALC:SLIMits:LEFT and CALC:SLIMits:RIGHt
FSE	CALCulate<1|2>:TLINe<1|2>:STATe	ON | OFF	not available on the FSP; replaced by CALC:SLIMits:LEFT and CALC:SLIMits:RIGHt
FSE	CALCulate<1|2>:UNIT:ANGLe	DEG | RAD	not available for FSP
FSP	CALCulate<1|2>:UNIT:POWer	DBM | V| A| W | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere	available units are compatible to the FSE
FSET/ ESI	CALCulate<1|2>:UNIT:POWer	DBM | V | W | DB | PCT | UNITLESS | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | DBPT | DBUV_MHZ | DBMV_MHZ | DBUA_MHZ | DBUV_M | DBUA_M | DBUV_MMHZ | DBUA_MMHZ	the FSP supports the following units:DBM | V| A| W | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere

Devices	Command	Parameter	Notes
FSE/ FSIQ	CALCulate<1|2>:UNIT:POWer	DBM | V | W | DB | PCT | UNITLESS | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | DBUV_MHZ | DBMV_MHZ | DBUA_MHZ | DBUV_M | DBUA_M | DBUV_MMHZ | DBUA_MMHZ	the FSP supports the following units:DBM | V| A| W | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere
FSE	CALCulate<1|2>:X:UNIT:TIME	S | SYM	not available for FSP
FSP	CALibration:ABORt		new function for FSP
FSE	CALibration:BANDwidth | BWIDth[:RESolution]?		not available for FSP
FSE	CALibration:IQ?		not available for FSP
FSE	CALibration:LDETector?		not available for FSP
FSE	CALibration:LOSuppression?		not available for FSP
FSE	CALibration:PPEak?		not available for FSP
ESI	CALibration:PRESelector?		not available for FSP
FSP	CALibration:RESult?		new function for FSP
FSE	CALibration:SHORt?		not available for FSP
FSP + FSE	CALibration:STATe	ON | OFF	
FSP + FSE	CALibration[:ALL]?		
FSE	CONFigure:BURSt:PFERror:COUNt	1 to 1000	not available for FSP and FSET
FSE	CONFigure:BURSt:PFERror[IMMediate]		not available for FSP and FSET
FSE	CONFigure:BURSt:POWer:CONDition	NORMal | EXTReme	not available for FSP and FSET
FSE	CONFigure:BURSt:POWer:COUNt	1 to 1000	not available for FSP and FSET
FSE	CONFigure:BURSt:POWer[IMMediate]		not available for FSP and FSET
FSE	CONFigure:BURSt:PTEMplate:[IMMediate]		not available for FSP and FSET
FSE	CONFigure:BURSt:PTEMplate:COUNt	1 to 1000	not available for FSP and FSET
FSE	CONFigure:BURSt:PTEMplate:SELect	FULL | TOP | RISing | FALLing	not available for FSP and FSET
FSE	CONFigure:BURst:REFerence:AUTO	ON | OFF	not available for FSP and FSET
FSE	CONFigure:SPECtrum:MODulation:COUNt	1 to 1000	not available for FSP and FSET
FSE	CONFigure:SPECtrum:MODulation:RANGe	ARFCn | TXBand | RXBand | COMBined | DCSRx1800	not available for FSP and FSET
FSE	CONFigure:SPECtrum:MODulation:TGATe	ON | OFF	not available for FSP and FSET
FSE	CONFigure:SPECtrum:MODulation[:IMMediate]		not available for FSP and FSET
FSE	CONFigure:SPECtrum:SWITching:COUNt	1 to 1000	not available for FSP and FSET
FSE	CONFigure:SPECtrum:SWITching[:IMMediate]		not available for FSP and FSET
FSE	CONFigure:SPURious:ANTenna	CONDucted | RADiated	not available for FSP and FSET
FSE	CONFigure:SPURious:COUN:RXBandt	1 to 1000	not available for FSP and FSET
FSE	CONFigure:SPURious:COUNt	1 to 1000	not available for FSP and FSET
FSE	CONFigure:SPURious:RANGe	TXBand | OTXBand | RXBand | IDLeband | COMBined	not available for FSP and FSET
FSE	CONFigure:SPURious:STEP:COUNt?		not available for FSP and FSET
FSE	CONFigure:SPURious:STEP<1..26>	ON | OFF	not available for FSP and FSET
FSE	CONFigure:SPURious[:IMMediate]		not available for FSP and FSET
FSE	CONFigure[:BTS]:ARFCn	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:BTS]:ARFCn:AUTO	ONCE	not available for FSP and FSET

Devices	Command	Parameter	Notes
FSE	CONFigure[:BTS]:CHANnel:SFH	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:BTS]:CHANnel:SLOT	0 to 7	not available for FSP and FSET
FSE	CONFigure[:BTS]:CHANnel:SLOT:AUTO	ONCE	not available for FSP and FSET
FSE	CONFigure[:BTS]:CHANnel:TSC	0 to 7	not available for FSP and FSET
FSE	CONFigure[:BTS]:CHANnel:TSC:AUTO	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:BTS]:COSiting	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:BTS]:LIMIt:FREQency	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:BTS]:LIMIt:PPEak	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:BTS]:LIMIt:PRMS	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:BTS]:LIMit:STANdard	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:BTS]:NETWork:PHASe	1|2[,PLUS]	not available for FSP and FSET
FSE	CONFigure[:BTS]:NETWork[:TYPE]	PGSM |PGSM900 | EGSM |EGSM900 | DCS |GSM1800 | PCS | GSM1900 | RGSM | RGSM900	not available for FSP and FSET
FSE	CONFigure[:BTS]:POWer:CLASs	1 to 8 | 1 to 4 | M1 | M2 | M3	not available for FSP and FSET
FSE	CONFigure[:BTS]:POWer:COUPled	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:BTS]:POWer:DYNamic	0 to 15	not available for FSP and FSET
FSE	CONFigure[:BTS]:POWer:EXPected	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:BTS]:POWer:LIMit	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:BTS]:POWer:SINGle:CLEar		not available for FSP and FSET
FSE	CONFigure[:BTS]:POWer:SINGle[:STATe]	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:BTS]:POWer:STATic	0 to 6	not available for FSP and FSET
FSE	CONFigure[:BTS]:PRESet		not available for FSP and FSET
FSE	CONFigure[:BTS]:SWEeptime	STANdard | AUTO	not available for FSP and FSET
FSE	CONFigure[:BTS]:TXSupp	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:BTS]MEASurement?		not available for FSP and FSET
FSE	CONFigure[:MS]:ARFCn	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:MS]:ARFCn:AUTO	ONCE	not available for FSP and FSET
FSE	CONFigure[:MS]:CHANnel:SFH	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:MS]:CHANnel:TSC	0 to 7	not available for FSP and FSET
FSE	CONFigure[:MS]:LIMIt:FREQuency	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:MS]:LIMIt:PPEak	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:MS]:LIMIt:PRMS	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:MS]:LIMit:STANdard	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:MS]:NETWork:PHASe	1|2[,PLUS]	not available for FSP and FSET

Devices	Command	Parameter	Notes
FSE	CONFigure[:MS]:NETWork[:TYPE]	PGSM |PGSM900 | EGSM |EGSM900 | DCS |GSM1800 | PCS | GSM1900 | RGSM | RGSM900	not available for FSP and FSET
FSE	CONFigure[:MS]:POWer:CLASs	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:MS]:POWer:COUPled	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:MS]:POWer:EXPected	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:MS]:POWer:LEVel	0 to 31	not available for FSP and FSET
FSE	CONFigure[:MS]:POWer:LIMit	<numeric_value>	not available for FSP and FSET
FSE	CONFigure[:MS]:POWer:SINGle:CLEar		not available for FSP and FSET
FSE	CONFigure[:MS]:POWer:SINGle[:STATe]	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:MS]:POWer:SMALl	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:MS]:PRESet		not available for FSP and FSET
FSE	CONFigure[:MS]:SWEeptime	STANdard | AUTO	not available for FSP and FSET
FSE	CONFigure[:MS]:TXSupp	ON | OFF	not available for FSP and FSET
FSE	CONFigure[:MS]MEASurement?		not available for FSP and FSET
FSET	DIAGnostic:INFO:CCOunt:ATTenuation?		not available for FSP
FSE	DIAGnostic:INFO:CCOunt:ATTenuation<1 | 10>?		not available for FSP
FSIQ	DIAGnostic:INFO:CCOunt:ATTenuation<1 | 2 | 3>?		not available for FSP
ESI	DIAGnostic:INFO:CCOunt:ATTenuation<1|2|4>?		not available for FSP
FSE	DIAGnostic:INFO:CCOunt:PRESelector<1..6>?		not available for FSP
FSP	DIAGnostic:SERVice:CSOurce[:POWer]	<numeric_value>	new function for FSP
FSE	DIAGnostic:SERVice:FUNCtion	<numeric_value>, <numeric_value> to	not available for FSP. Replaced by DIAG:SERV:SFUNction
FSET	DIAGnostic:SERVice:HGENerator	OFF | 10 kHz | 100 kHz | BALanced	not available for FSP
FSP + FSE	DIAGnostic:SERVice:INPut[:SELect]	CALibration | RF	
FSP + FSE	DIAGnostic:SERVice:NSOurce	ON | OFF	
FSP	DIAGnostic:SERVice:SFUNction	<string> to	replacement for DIAG:SERV:FUNC of FSP; necessary due to different parameter formats needed on the FSP
FSP	DIAGnostic:SERVice:STESt:RESult?		new function for FSP
FSP + FSE	DISPlay:ANNotation:FREQuency	ON | OFF	
	DISPlay:BARGraph:LEVel:LOWer		not available for FSP
	DISPlay:BARGraph:LEVel:UPPer		not available for FSP
FSP + FSE	DISPlay:CMAP<1...26>:DEFault<1|2>		larger selection of independently configurable items (1 to 26)
FSP + FSE	DISPlay:CMAP<1...26>:HSL	0 to 1,0 to 1,0 to 1	larger selection of independently configurable items (1 to 26)
FSP + FSE	DISPlay:CMAP<1...26>:PDEFined	<color>	larger selection of independently configurable items (1 to 26)
FSP + FSE	DISPlay:FORmat	SINGle | SPLit	
FSP + FSE	DISPlay:LOGO	ON | OFF	
FSE	DISPlay:PROGram[:MODE]	ON | OFF	not available for FSP
FSP + FSE	DISPlay:PSAVe:HOLDoff	0 to 60	
FSP + FSE	DISPlay:PSAVe[:STATe]	ON | OFF	
FSE	DISPlay[:WINDow<1|2>]:FEED	'AF' | 'VIDeo'	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:MINFo	ON | OFF	not available for FSP
FSP	DISPlay[:WINDow<1|2>]:SELect		new function for FSP
FSP + FSE	DISPlay[:WINDow<1|2>]:TEXT:STATe	ON | OFF	

Devices	Command	Parameter	Notes
FSP + FSE	DISPlay[:WINDow<1|2>]:TEXT[:DATA]	<string>	
FSP + FSE	DISPlay[:WINDow<1|2>]:TIME	ON | OFF	
FSP + FSE	DISPlay[:WINDow<1|2>]:TRACe<1...3>:MODE	WRITe | VIEW | AVERage | MAXHold | MINHold	FSP: 3 traces are available per screen FSE: 4 traces are available in full screen mode and 2 traces per screen in split screen mode
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:EYE:COUNt	1 to Result Length	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:MODE:ANALog	ON | OFF	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:MODE:CWRite	ON | OFF	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:MODE:HCONtinuous	ON | OFF	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:SYMBol	DOTS | BARS | OFF	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:X:SPACing	LINear | LOGarithmic	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:X[:SCALe]:RVALue	<numeric value>	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:X[:SCALe]:ZOOM	ON | OFF	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:X[:SCALe]:ZOOM [:FREQuency]:CENTer	<numeric_value>	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:X[:SCALe]:ZOOM [:FREQuency]:	<numeric_value>	not available for FSP
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:X[:SCALe]:ZOOM [:FREQuency]:	<numeric_value>	not available for FSP
FSP	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y:SPACing	LINear | LOGarithmic	FSP: TRACe<1...3>
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:Y:SPACing	LINear | LOGarithmic | PERCent	PERCent is not available for FSP + FSE: TRACE<1...4>
FSP + FSE	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]	10dB to 200dB	FSP: TRACe<1...3> FSE: TRACE<1...4>
FSET/ ESI	DISPlay[:WINDow<1|2>]:TRACe<1...4>:Y[:SCALe]:BOTTom	<numeric value>	not available for FSP
FSP + FSE	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:MODE	ABSolute | RELative	FSP: TRACe<1...3> FSE: TRACE<1...4>
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:Y[:SCALe]:PDIVision		not available for FSP
FSP + FSE	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RLEVel	-130dBm to 30dBm	FSP: TRACe<1...3> FSE: TRACE<1...4>
FSP + FSE	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RLEVel:OFFSet	-200dB to 200dB	FSP: TRACe<1...3> FSE: TRACE<1...4>
FSP + FSE	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RPOSition	0 to 100 PCT	FSP: TRACe<1...3> FSE: TRACE<1...4>
FSP + FSE	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RVALue	<numeric value>	FSP: TRACe<1...3> FSE: TRACE<1...4>
FSE	DISPlay[:WINDow<1|2>]:TRACe<1...4>:Y[:SCALe]:RVALue:AUTO	ON | OFF	not available for FSP
FSET/ ESI	DISPlay[:WINDow<1|2>]:TRACe<1...4>:Y[:SCALe]:TOP	<numeric value>	not available for FSP
FSP	DISPlay[:WINDow<1|2>]:TRACe<1...3>[:STATe]	ON | OFF	FSP: TRACe<1...3> FSE: TRACE<1...4>
FSE	FETCh:BURSt:FERRor:AVERage?		not available for FSP and FSET
FSE	FETCh:BURSt:FERRor:MAXimum?		not available for FSP and FSET
FSE	FETCh:BURSt:FERRor:STATus?		not available for FSP and FSET
FSE	FETCh:BURSt:PERRor:PEAK:AVERage?		not available for FSP and FSET
FSE	FETCh:BURSt:PERRor:PEAK:MAXimum?		not available for FSP and FSET
FSE	FETCh:BURSt:PERRor:PEAK:STATus?		not available for FSP and FSET
FSE	FETCh:BURSt:PERRor:RMS:AVERage?		not available for FSP and FSET
FSE	FETCh:BURSt:PERRor:RMS:MAXimum?		not available for FSP and FSET
FSE	FETCh:BURSt:PERRor:RMS:STATus?		not available for FSP and FSET
FSE	FETCh:BURSt:POWer[:IMMediate]?		not available for FSP and FSET
FSE	FETCh:MODulation[:ALL]?	ARFCn | TXBand | RXBand |COMBined | DCSRx1800	not available for FSP and FSET

Devices	Command	Parameter	Notes
FSE	FETCh:PTEMplate:REFerence?	TXBand	not available for FSP and FSET
FSE	FETCh:SPECtrum:MODulation:REFerence?	TXBand	not available for FSP and FSET
FSE	FETCh:SPECtrum:SWITching:REFerence?	TXBand	not available for FSP and FSET
FSE	FETCh:SPECtrum:SWITching[:ALL]?		not available for FSP and FSET
FSE	FETCh:SPURious:STEP?		not available for FSP and FSET
FSE	FETCh:SPURious[:ALL]?	TXBand OTXBand | RXBand | IDLeband	not available for FSP and FSET
FSE	FORMat:DEXPort:APPend[:STATe] ON|OFF[,32]		not available for FSP
FSP + FSE	FORMat:DEXPort:DSEParator	POINt|COMMa	
FSE	FORMat:DEXPort:HEADer[:STATe] ON|OFF[,32]		not available for FSP
FSP	FORMat[:DATA]	ASCii | REAL[,32]	
FSE	FORMat[:DATA]	ASCii | REAL | UINT [,32]	UINT is not available for FSP
FSP + FSE	HCOPy:ABORt		
FSP	HCOPy:DESTination<1|2>	'MMEM' | 'SYST:COMM:PRIN' | 'SYST:COMM:CLIP'	
FSE/	HCOPy:DESTination<1|2>	'SYST:COMM:GPIB' |'SYST:COMM:SER1' | 'SYST:COMM:SER2' | 'SYST:COMM:CENT' | 'MMEM' | 'SYST:COMM:PRIN'|'SYST :COMM:CLIP'	SYST:COMM:GPIB/SER1/SE R2 is not available for FSP
FSIQ/ ESI	HCOPy:DESTination<1|2>	"MMEM' | 'SYST:COMM:PRIN'| 'SYST:COMM:CLIP'	
FSP + FSE	HCOPy:DEVice:COLor	ON | OFF	
FSP	HCOPy:DEVice:LANGuage<1|2>	GDI | WMF | EWMF | BMP	
FSE/	HCOPy:DEVice:LANGuage<1|2>	HPGL | PCL4 | PCL5 | POSTscript | ESCP | WMF | PCX | HP7470 to	
FSIQ/ ESI	HCOPy:DEVice:LANGuage<1|2>	WMF | GDI | EWMF | BMP to	
FSE/	HCOPy:DEVice:PRESet<1|2>	ON | OFF	not available for FSP
FSE/	HCOPy:DEVice:RESolution<1|2>	150 | 300	not available for FSP
FSP + FSE	HCOPy:ITEM:ALL		
FSE	HCOPy:ITEM:FFEed<1|2>:STATe	ON | OFF	not available for FSP
FSE	HCOPy:ITEM:LABel:TEXT	<string>	not available for FSP
FSE	HCOPy:ITEM:PFEed<1|2>:STATe	ON | OFF	not available for FSP
FSP + FSE	HCOPy:ITEM:WINDow<1|2>:TABle:STATe	ON | OFF	
FSP + FSE	HCOPy:ITEM:WINDow<1|2>:TEXT	<string>	
FSE	HCOPy:ITEM:WINDow<1|2>:TRACe:CAINcrement	ON | OFF	not available for FSP
FSP + FSE	HCOPy:ITEM:WINDow<1|2>:TRACe:STATe	ON | OFF	
FSE	HCOPy:PAGE:DIMensions:FULL		not available for FSP
FSE	HCOPy:PAGE:DIMensions:QUADrant<1...4>		not available for FSP
FSP + FSE	HCOPy:PAGE:ORIentation<1|2>	LANDscape | PORTrait	
FSP + FSE	HCOPy[:IMMediate]		
FSET/ ESI	HOLD		not available for FSP
FSP + FSE	INITiate<1|2>:CONMeas	ON | OFF	
FSP + FSE	INITiate<1|2>:CONTinuous	ON | OFF	
FSP + FSE	INITiate<1|2>:DISPlay	ON | OFF	
FSP + FSE	INITiate<1|2>[:IMMediate]		
FSET	INPut:PRESelection:CATalog?		not available for FSP
FSET	INPut:PRESelection:USET:NAME	'name of user defined preselector set (to edit existing set or to create new set)'	not available for FSP
FSET	INPut:PRESelection:USET:CLEar		not available for FSP
FSET	INPut:PRESelection:USET:COMMent	'comment for preselector-set'	not available for FSP

Devices	Command	Parameter	Notes
FSET	INPut:PRESelection:USET:LRANge[:DATA]	<numeric value>, <numeric value>, <numeric_value>	not available for FSP
FSET	INPut:PRESelection:USET:MRANge[:DATA]	<numeric value>, <numeric value>, <numeric_value>	not available for FSP
FSP + FSE	INPut<1|2>:ATTenuation	0 to 70dB	
FSET	INPut<1|2>:ATTenuation	0 to 70 | 80dB	80 dB not available for FSP
FSP + FSE	INPut<1|2>:ATTenuation:AUTO	ON | OFF	
FSE	INPut<1|2>:ATTenuation:AUTO:MODE	NORMal | LNOise | LDIStorsion	not available for FSP
FSET/ ESI	INPut<1|2>:ATTenuation:PROTection	ON | OFF	not available for FSP
FSET	INPut<1|2>:ATTenuation:STEPsize	1dB | 10dB	not available for FSP
FSET	INPut<1|2>:IMPedance	150OHM | 600OHM | 10kOHM	not available for FSP
FSET	INPut<1|2>:COUPling	AC | DC	not available for FSP
FSP	INPut<1|2>:EATT	0 to 30dB	new function for FSP
FSP	INPut<1|2>:EATT:AUTO	ON | OFF	new function for FSP
FSP	INPut<1|2>:EATT:STATe	ON | OFF	new function for FSP
FSET	INPut<1|2>:GAIN	0 to 30dB	not available for FSP
FSET/ ESI	INPut<1|2>:GAIN:AUTO	ON | OFF	not available for FSP
FSP + FSE	INPut<1|2>:GAIN:STATe	ON | OFF	
FSP + FSE	INPut<1|2>:IMPedance	50 | 75	
FSE	INPut<1|2>:IMPedance:CORRection	RAM | RAZ	not available for FSP
FSET	INPut<1|2>:LISN:PEARth	GROunded | FLOating	not available for FSP
FSET	INPut<1|2>:LISN:PHASe	L1 | L2 | L3 | N	not available for FSP
FSET	INPut<1|2>:LISN[:TYPE]	TWOphase | FOURphase | OFF	not available for FSP
FSE	INPut<1|2>:MIXer	<numeric value>	not available for FSP
FSET	INPut<1|2>:PRESelection:COUPling	ON | OFF	not available for FSP
FSET	INPut<1|2>:PRESelection:COUPling:HIGH:FREQuency	5MHz to 500MHz	not available for FSP
FSET	INPut<1|2>:PRESelection:COUPling:HIGH:SET	'name of preselector set for high RBW'	not available for FSP
FSET	INPut<1|2>:PRESelection:COUPling:LOW:FREQuency	10Hz to 5MHz	not available for FSP
FSET	INPut<1|2>:PRESelection:COUPling:LOW:SET	"name of preselector set for low RBW'	not available for FSP
FSET	INPut<1|2>:PRESelection:COUPling:MID:SET	"name of preselector set for medium RBW'	not available for FSP
FSET	INPut<1|2>:PRESelection:FILTer:HPASS[:FREQuency]	100Hz to 5MHz	not available for FSP
FSET	INPut<1|2>:PRESelection:FILTer:LPASS[:FREQuency]	20KHz to 40MHz	not available for FSP
FSET	INPut<1|2>:PRESelection:FILTer[:STATe]	ON | OFF	not available for FSP
FSET	INPut<1|2>:PRESelection:SET	NARRow | NORMal | WIDE	not available for FSP
FSET	INPut<1|2>:PRESelection:USET[:SELect]	"name of user defined preselector set'	not available for FSP
FSET	INPut<1|2>:PRESelection[:STATe]	ON | OFF	not available for FSP
FSET	INPut<1|2>:TYPE	RF | BALanced	not available for FSP
ESI	INPut<1|2>:TYPE	INPUT1 | INPUT2	not available for FSP
FSE	INPut<1|2>:UPORt<1|2>:STATe	ON | OFF	not available for FSP
FSE	INPut<1|2>:UPORt<1|2>[:VALue]?		not available for FSP
ESI	INPut2:COUPling	AC | DC	not available for FSP
FSP	INSTrument:COUPle	NONE | RLEVel | CF_B | CF_A	available coupling modes between Screen A and Screen B have been changed between FSE and FSP
FSE	INSTrument:COUPle	NONE | MODE | X | Y | CONTrol | XY | XCONtrol | YCONtrol | ALL	Available coupling modes between screen A and screen B have been changed between FSE and FSP
FSP	INSTrument<1|2>:NSELect	1	currently only parameter value 1 available
ESI	INSTrument<1|2>:NSELect	1 to 3 | 6	4 parameter values are available
FSE/ FSIQ	INSTrument<1|2>:NSELect	1 to 5	5 parameter values are available
FSET	INSTrument<1|2>:NSELect	1 | 2 | 6	3 parameter values are available

Devices	Command	Parameter	Notes
FSP	INSTrument<1|2>[:SELect]	SANalyzer	Currently only SANalyzer available
FSE/ FSIQ	INSTrument<1|2>[:SELect]	SANalyzer | DDEMod | ADEMod | BGSM | MGSM	5 parameters are available.
ESI	INSTrument<1|2>[:SELect]	RECeiver | SANalyzer | DDEMod | ADEMod	4 parameters are available.
FSET	INSTrument<1|2>[:SELect]	ANalyzer | DDEMod | RECeiver	3 parameters are available.
FSP + FSE	MMEMory:CATalog?	string	
FSP + FSE	MMEMory:CDIRectory	directory name	
FSP + FSE	MMEMory:CLear:ALL		
FSP + FSE	MMEMory:CLear:STATe	1,path	
FSP + FSE	MMEMory:COMMent	<string>	
FSP + FSE	MMEMory:COPY	path\file, path\file	
FSP + FSE	MMEMory:DATA	filename [, <block data>]	
FSP + FSE	MMEMory:DELete	path\filename	
FSP + FSE	MMEMory:LOAD:AUTO	1,path	
FSP + FSE	MMEMory:LOAD:STATe	1,path	
FSP + FSE	MMEMory:MDIRectory	path	
FSP + FSE	MMEMory:MOVE	path	
FSP + FSE	MMEMory:MSIS	'A:' | 'D:'	FSP: valid drives are A: and D: FSE: valid drives are A: and C:
FSP + FSE	MMEMory:NAME	path\filename	
FSP + FSE	MMEMory:RDIRectory	directory	
FSP + FSE	MMEMory:SELect[:ITEM]:ALL		
FSE	MMEMory:SELect[:ITEM]:CSETup	ON | OFF	not available for FSP (default setting on the FSP)
FSE	MMEMory:SELect[:ITEM]:CVL:ALL	ON | OFF	not available for FSP and FSET
FSE	MMEMory:SELect[:ITEM]:CVL[:ACTive]	ON | OFF	not available for FSP and FSET
FSP + FSE	MMEMory:SELect[:ITEM]:DEFault		
FSE	MMEMory:SELect[:ITEM]:GSETup	ON | OFF	not available for FSP (default setting on the FSP)
FSE	MMEMory:SELect[:ITEM]:HCOPy	ON | OFF	not available for FSP (default setting on the FSP)
FSP + FSE	MMEMory:SELect[:ITEM]:HWSettings	ON | OFF	
FSP + FSE	MMEMory:SELect[:ITEM]:LINes:ALL	ON | OFF	
FSE	MMEMory:SELect[:ITEM]:LINes:ALL	ON | OFF	
FSE	MMEMory:SELect[:ITEM]:LINes[:ACTive]	ON | OFF	not available for FSP (default setting on the FSP)
FSE	MMEMory:SELect[:ITEM]:MACRos	ON | OFF	not available for FSP
FSP + FSE	MMEMory:SELect[:ITEM]:NONE		
FSP + FSE	MMEMory:SELect[:ITEM]:SCData	ON | OFF	
FSP	MMEMory:SELect[:ITEM]:TRACe[:ACTive]	ON | OFF	no numeric suffixes behind TRACe
FSE	MMEMory:SELect[:ITEM]:TRACe<1...4>	ON | OFF	numeric suffixes behind TRACe
FSE	MMEMory:SELect[:ITEM]:TRANsducer:ALL	ON | OFF	not available for FSP
FSE	MMEMory:SELect[:ITEM]:TRANsducer[:ACTive]	ON | OFF	not available for FSP
FSP + FSE	MMEMory:STORe:STATe	1,path	
FSP + FSE	MMEMory:STORe:TRACe	1 to 3,path	
FSE	OUTPut:AF:SENSitivity	<numeric_value>	not available for FSP and FSET
FSE	OUTPut:UPORt<1|2>:STATe	ON | OFF	not available for FSP
FSE	OUTPut:UPORt<1|2>[:VALue]	#B00000000 to #B11111111	not available for FSP
FSP + FSE	OUTPut<1|2>[:STATe]	ON | OFF	
FSE	READ:BURSt:FERRor:AVERage?		not available for FSP and FSET
FSE	READ:BURSt:FERRor:MAXimum?		not available for FSP and FSET
FSE	READ:BURSt:FERRor:STATus?		not available for FSP and FSET

Devices	Command	Parameter	Notes
FSE	READ:BURSt:PERRor:PEAK:AVERage?		not available for FSP and FSET
FSE	READ:BURSt:PERRor:PEAK:MAXimum?		not available for FSP and FSET
FSE	READ:BURSt:PERRor:PEAK:STATus?		not available for FSP and FSET
FSE	READ:BURSt:PERRor:RMS:AVERage?		not available for FSP and FSET
FSE	READ:BURSt:PERRor:RMS:MAXimum?		not available for FSP and FSET
FSE	READ:BURSt:PERRor:RMS:STATus?		not available for FSP and FSET
FSE	READ:BURSt:POWer:DYNamic?		not available for FSP and FSET
FSE	READ:BURSt:POWer:LEVel?		not available for FSP and FSET
FSE	READ:BURSt:POWer:STATic?		not available for FSP and FSET
FSE	READ:BURSt:POWer?		not available for FSP and FSET
FSE	READ:BURSt:REFerence[:IMMediate?]		not available for FSP and FSET
FSE	READ:SPECtrum:MODulation[:ALL]?		not available for FSP and FSET
FSE	READ:SPECtrum:SWITching[:ALL]?		not available for FSP and FSET
FSE	READ:SPURious:STEP?		not available for FSP and FSET
FSE	READ:SPURious[:ALL]?		not available for FSP and FSET
FSE	[SENSe<1|2>:]ADEMod:AF:COUPling	AC | DC	not available for FSP and FSET
FSE	[SENSe<1|2>:]ADEMod:RTIMe	ON | OFF	not available for FSP and FSET
FSE	[SENSe<1|2>:]ADEMod:SBAND	NORMal | INVerse	not available for FSP and FSET
FSE	[SENSe<1|2>:]ADEMod:SQUelch:LEVel	30 to 150 dBm	not available for FSP and FSET
FSE	[SENSe<1|2>:]ADEMod:SQUelch[:STATe]	ON | OFF	not available for FSP and FSET
FSET	[SENSe<1|2>:]AM:RANGe[:UPPer]	3PCT | 10 PCT | 100PCT	not available for FSP
FSE	[SENSe<1|2>:]AVERage:AUTO	ON | OFF	not available for FSP
FSP + FSE	[SENSe<1|2>:]AVERage:COUNt	0 to 32767	
FSE	[SENSe<1|2>:]AVERage:COUNt	0 to 32767	
FSP	[SENSe<1|2>:]AVERage:TYPE	VIDeo | LINear	command is used to select logarithmic or linear averaging on the FSP; therefore parameters are incompatible to the FSE
FSE	[SENSe<1|2>:]AVERage:TYPE	MAXimum | MINimum | SCALar	command is used to select logarithmic or linear averaging on the FSP; therefore parameters are incompatible to the FSE
FSP + FSE	[SENSe<1|2>:]AVERage[:STATe<1...3>]	ON | OFF	
FSE	[SENSe<1|2>:]BANDwidth|BWIDth:DEMod	<numeric_value>	not available for FSP and FSET
FSE	[SENSe<1|2>:]BANDwidth|BWIDth:PLL	AUTO | HIGH | MEDium | LOW	not available for FSP
FSP + FSE	[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo	1Hz to 10MHz	
FSET	[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo	1Hz to 500MHz	
FSP + FSE	[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo:AUTO	ON | OFF	
FSET	[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo:EXTernal[:STATe]	ON | OFF	not available for FSP
FSP	[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo:RATio	0.0001 to 1	only numeric values available. Parameter ranges differ between FSP and FSE
FSE	[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo:RATio	0.001 to 1000 | SINe | PULSe | NOISe	also text parameters are available. Parameter ranges differ between FSP and FSE not available for FSET

Devices	Command	Parameter	Notes
FSP + FSE	[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]	10Hz to 10MHz (anal. filter) 1Hz to 10MHz (FFT filter)	FSE: 10Hz to 10MHz (models 20) 1Hz to 10MHz (models 30)
FSET	[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]	10 Hz to 500MHz	
FSP + FSE	[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:AUTO	ON | OFF	
FSE	[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:MODE	ANALog | DIGital	not available for FSP and FSET
FSP + FSE	[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:MODE:FFT	ON | OFF	old command that is still supported, but has been replaced on the FSP by [SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:TYPE
FSP + FSE	[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:RATio	0.0001 to 1	
FSP	[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:TYPE	NORMal | FFT | CFILter | RRC	new function for FSP
FSP + FSE	[SENSe<1|2>:]CORRection:COLLect[:ACQuire]	THRough | OPEN	
FSE	[SENSe<1|2>:]CORRection:CVL:BAND	A|Q|U|V|E|W|F|D|G|Y|J	not available for FSP and FSET
FSE	[SENSe<1|2>:]CORRection:CVL:BIAS	<numeric_value>	not available for FSP and FSET
FSE	[SENSe<1|2>:]CORRection:CVL:CATalog?		not available for FSP and FSET
FSE	[SENSe<1|2>:]CORRection:CVL:CLEar		not available for FSP and FSET
FSE	[SENSe<1|2>:]CORRection:CVL:COMMent	<string>	not available for FSP and FSET
FSE	[SENSe<1|2>:]CORRection:CVL:DATA	<freq>,<level> to	not available for FSP and FSET
FSE	[SENSe<1|2>:]CORRection:CVL:MIXer	<string>	not available for FSP and FSET
FSE	[SENSe<1|2>:]CORRection:CVL:PORTs	2 | 3	not available for FSP and FSET
FSE	[SENSe<1|2>:]CORRection:CVL:SELect	<file_name>	not available for FSP and FSET
FSE	[SENSe<1|2>:]CORRection:CVL:SNUMber	<string>	not available for FSP and FSET
FSE	[SENSe<1|2>:]CORRection:CVL:TYPE	ODD | EVEN | EODD	not available for FSP and FSET
FSE/ FSIQ	[SENSe<1|2>:]CORRection:LOSS:INPut[:MAGNitude]	<numeric_value>	not available for FSP
FSP + FSE	[SENSe<1|2>:]CORRection:METHod	TRANsmission | REFLexion	
FSP + FSE	[SENSe<1|2>:]CORRection:RECall		
FSE	[SENSe<1|2>:]CORRection:RXGain:INPut[:MAGNitude]	<numeric_value>	not available for FSP, FSET and ESI
FSP + FSE	[SENSe<1|2>:]CORRection[:STATe]	ON | OFF	
FSE	[SENSe<1|2>:]CORRection:TRANsducer:ACTive?		not available for FSP
FSE	[SENSe<1|2>:]CORRection:TRANsducer:CATalog?		not available for FSP
FSE	[SENSe<1|2>:]CORRection:TRANsducer:COMMent	<string>	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TRANsducer:DATA	<freq>,<level> to	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TRANsducer:DELete		not available for FSP
FSE	[SENSe<1|2>:]CORRection:TRANsducer:SCALing	LINear|LOGarithmic	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TRANsducer:SELect	<name>	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TRANsducer:UNIT	<string>	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TRANsducer[:STATe]	ON | OFF	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TSET:ACTive?		not available for FSP
FSE	[SENSe<1|2>:]CORRection:TSET:BREak	ON | OFF	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TSET:CATalog?		not available for FSP
FSE	[SENSe<1|2>:]CORRection:TSET:COMMent	<string>	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TSET:DELete		not available for FSP
FSE	[SENSe<1|2>:]CORRection:TSET:RANGe<1...10>	<freq>,<freq>,<name> to	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TSET:SELect	<name>	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TSET:UNIT	<string>	not available for FSP
FSE	[SENSe<1|2>:]CORRection:TSET[:STATe]	ON | OFF	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:FILTer:ALPHa	0.2 to 1	not available for FSP

Devices	Command	Parameter	Notes
FSE	[SENSe<1|2>:]DDEMod:FILTer:MEASurement	OFF | RCOSine | RRCosine | GAUSsian | B22 | B25 | B44 | QFM | QFR | QRM | QRR | A25Fm | EMES | EREF	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:FILTer:REFerence	RCOSine | RRCosine | GAUSsian | B22 | B25 | B44 | QFM | QFR | QRM | QRR | A25Fm | EMES | EREF	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:FORMat	QPSK | PSK | MSK |QAM | FSK	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:FSK:NSTate	2 | 4	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:MSK:FORMat	TYPE1 | TYPE2 | NORMal | DIFFerential	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:NORMalize	ON | OFF	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:PRATe	1 | 2 | 4 | 8 | 16	not available for FSP
FSE/ ESI	[SENSe<1|2>:]DDEMod:PRESet	GSM | EDGe | NADC | TETRa | DCS1800 | PCS1900 | PHS | PDCup | PDCDown | APCO25CQPSK | APCO25C4FM | CDPD | DECT | CT2 | ERMes | MODacom | PWT | TFTS | F16 | F322 | F324 | F64 | FQCDma | RQCDma | FNADc | RNADc | BPSK18 | GMSK18 | QPSK18 | GMSK36	not available for FSP
FSIQ	[SENSe<1|2>:]DDEMod:PRESet	GSM | EDGe | NADC | TETRa | PHS | PDCup | PDCDown | APCO25CQPSK | APCO25C4FM | CDPD | DECT | CT2 | ERMes | MODacom | PWT | TFTS | F16 | F322 | F324 | F64 | FWCDma | RWCDma | FW3Gppcdma | RW3Gppcdma | BPSK18 | GMSK18 | QPSK18 | GMSK36	not available for FSP
FSET	[SENSe<1|2>:]DDEMod:PRESet	GSM | EDGe | NADC | TETRa | DCS1800 | PCS1900 | PHS | PDCup | PDCDown | APCO25CQPSK | APCO25C4FM | CDPD | DECT | CT2 | ERMes | MODacom | PWT | TFTS | F16 | F322 | F324 | F64 | FQCDma | RQCDma | FNADc | RNADc | BPSK18 | GMSK18 | QPSK18 | GMSK36	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:PSK:FORMat	NORMal | DIFFerential | N3Pi8	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:PSK:NSTate	2 | 8	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:QAM:NSTate	16	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:QPSK:FORMat	NORMal | DIFFerential | OFFSet | DPI4	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SBANd	NORMal | INVerse	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SEARch:PULSe:STATe	ON | OFF	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SEARch:SYNC:CATalog?		not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SEARch:SYNC:COMMent	<string>	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SEARch:SYNC:DATA	<string>	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SEARch:SYNC:NAME	<string>	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SEARch:SYNC:OFFSet	<numeric_value>	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SEARch:SYNC:PATTern	<string>	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SEARch:SYNC:SELect	<string>	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SEARch:SYNC:STATe	ON | OFF	not available for FSP
FSE	[SENSe<1|2>:]DDEMod:SEARch:TIME	100 to 1600	not available for FSP

Devices	Command	Parameter	Notes
FSE	[SENSe<1|2>:]DDEMod:SRATe	160 Hz to 1,6 MHz	not available for FSP
FSIQ	[SENSe<1|2>:]DDEMod:SRATe	160 Hz to 7 MHz	not available for FSP
	[SENSe<1|2>:]DDEMod:TIME	1 to Frame Length	not available for FSP
FSET	[SENSe<1|2>:]DEMod	OFF | AM | AMVideo | FM | PM	not available for FSP
ESI	[SENSe<1|2>:]DEMod	OFF | AM | FM	not available for FSP
FSET	[SENSe<1|2>:]DEMod:FILTer:HPASs:FREQuency	0 Hz | 10 Hz | 100 Hz | 1 kHZ	not available for FSP
FSET	[SENSe<1|2>:]DEMod:FILTer[:LPASs]:AUTO	ON | OFF	not available for FSP
FSET	[SENSe<1|2>:]DEMod:FILTer[:LPASs]:FREQuency	<numeric_value>	not available for FSP
FSE	[SENSe<1|2>:]DETector<1...4>:CMEM[:STATe]	ON | OFF	not available for FSP
FSP	[SENSe<1|2>:]DETector<1...3>[:FUNCtion]	APEak |NEGative | POSitive | SAMPle | RMS | AVERage | QPEak	FSP: number of traces restricted to 3; detector settings correspond to selected screen FSE: Qpeak not available
ESI	[SENSe<1|2>:]DETector<1..4>[:FUNCtion]	APEak |NEGative | POSitive | SAMPle | RMS | AVERage | QPEak	
FSP + FSE	[SENSe<1|2>:]DETector<1...3>[:FUNCtion]:AUTO	ON | OFF	number of traces restricted to 3
FSET	[SENSe<1|2>:]DETector<1...4>:PSTRetch:AUTO	ON | OFF	not available for FSP
FSET	[SENSe<1|2>:]DETecto<1...4>r:PSTRetch[:STATe]	ON | OFF	not available for FSP
ESI	[SENSe<1|2>:]DETector<1...4>:RECeiver[:FUNCtion]	POSitive |NEGative| RMS | AVERage | QPEak	not available for FSP
FSET	[SENSe<1|2>:]DETector<1...4>:RECeiver[:FUNCtion]	POSitive | NEGative | RMS | AVERage	not available for FSP
FSE	[SENSe<1|2>:]FILTer:CCITt[:STATe]	ON | OFF	not available for FSP and FSET
FSE	[SENSe<1|2>:]FILTer:CMESsage[:STATe]	ON | OFF	not available for FSP and FSET
FSE	[SENSe<1|2>:]FILTer:DEMPhasis:LINK	DISPlay | AUDio	not available for FSP and FSET
FSE	[SENSe<1|2>:]FILTer:DEMPhasis:TCONstant	<numeric_value>	not available for FSP and FSET
FSE	[SENSe<1|2>:]FILTer:DEMPhasis[:STATe]	ON | OFF	not available for FSP and FSET
FSE	[SENSe<1|2>:]FILTer:HPASs:FREQuency	30 Hz | 300 HZ	not available for FSP and FSET
FSET	[SENSe<1|2>:]FILTer:HPASs:FREQuency	10 kHz | 1 kHz | 100 Hz	not available for FSP
FSE	[SENSe<1|2>:]FILTer:HPASs[:STATe]	ON | OFF	not available for FSP
FSE	[SENSe<1|2>:]FILTer:LPASs:FREQuency	3 kHz| 15 kHz	not available for FSP and FSET
FSE	[SENSe<1|2>:]FILTer:LPASs[:STATe]	ON | OFF	not available for FSP and FSET
FSET	[SENSe<1|2>:]FILTer:NOTCh[:STATe]	ON | OFF	not available for FSP
FSET	[SENSe<1|2>:]FM[:DEViation]:RANGe:UPPer	ON | OFF	not available for FSP
FSET	[SENSe<1|2>:]FM[:DEViation]:RANGe[:UPPer]	<numeric_value>	not available for FSP
FSP + FSE	[SENSe<1|2>:]FREQuency:CENTer	0 to f_{max}	frequency ranges are different for FSP and FSE
FSE	[SENSe<1|2>:]FREQuency:CENTer:LINK	STARt | STOP | SPAN	not available for FSP
FSP + FSE	[SENSe<1|2>:]FREQuency:CENTer:STEP	0 to f_{max}	frequency ranges are different for FSP and FSE
FSP + FSE	[SENSe<1|2>:]FREQuency:CENTer:STEP:LINK	SPAN | RBW | OFF	
FSP + FSE	[SENSe<1|2>:]FREQuency:CENTer:STEP:LINK:FACTor	1 to 100 PCT	
FSP + FSE	[SENSe<1|2>:]FREQuency:MODE	CW|FIXed | SWEep	
FSP + FSE	[SENSe<1|2>:]FREQuency:OFFSet	<numeric_value>	
FSET	[SENSe<1|2>:]FREQuency:RANGe	2 GHz | 22 GHz	not available for FSP
FSP + FSE	[SENSe<1|2>:]FREQuency:SPAN	0 to f_{max}	frequency ranges are different for FSP and FSE
FSP + FSE	[SENSe<1|2>:]FREQuency:SPAN:FULL		
FSE	[SENSe<1|2>:]FREQuency:SPAN:LINK	CENTer | STOP | SPAN	not available for FSP
FSP + FSE	[SENSe<1|2>:]FREQuency:STARt	0 to f_{max}	frequency ranges are different for FSP and FSE
FSET	[SENSe<1|2>:]FREQuency:STARt:FLINe[:STATe]	ON | OFF	not available for FSP. Replaced by CALC:MARK:FUNC:SLIMits
FSE	[SENSe<1|2>:]FREQuency:STARt:LINK	CENTer | STOP | SPAN	not available for FSP

Devices	Command	Parameter	Notes
FSP + FSE	[SENSe<1|2>:]FREQuency:STOP	0 to f_{max}	frequency ranges are different for FSP and FSE
FSET	[SENSe<1|2>:]FREQuency:STOP:FLINe[:STATe]	ON | OFF	not available for FSP; replaced by CALC:MARK:FUNC:SLIMits.
FSE	[SENSe<1|2>:]FREQuency:STOP:LINK	CENTer | STARt | SPAN	not available for FSP
FSET/ ESI	[SENSe<1|2>:]FREQuency[:CW|:FIXed]	f_{min} to f_{max}	not available for FSP
FSET/ ESI	[SENSe<1|2>:]FREQuency[:CW|:FIXed]:STEP	f_{min} to f_{max}	not available for FSP
FSP	[SENSe<1|2>:]LIST:POWer:RESult?		new function for FSP
FSP	[SENSe<1|2>:]LIST:POWer[:SEQuence]	<analyzer freq>, <ref level>,<rf att>,<el att>, <filter type>,<rbw>,<vbw>, <meas time>, <trigger level>,...	new function for FSP
FSP	[SENSe<1|2>:]LIST:POWer:SET	<PEAK meas>, <RMS meas>, <AVG meas>, <trigger mode>, <trigger slope>, <trigger offset>, <gate length>	new function for FSP
FSP	[SENSe<1|2>:]LIST:POWer:STATe	ON | OFF	new function for FSP
FSE	[SENSe<1|2>:]MIXer:BIAS	<numeric_value>	not available for FSP
FSE	[SENSe<1|2>:]MIXer:BIAS:LIMit:MIN	<numeric_value>	not available for FSP
FSE	[SENSe<1|2>:]MIXer:BIAS:LIMit[:MAX]	<numeric_value>	not available for FSP
FSE	[SENSe<1|2>:]MIXer:BLOCk	ON | OFF	not available for FSP
FSE	[SENSe<1|2>:]MIXer:HARMonic	<numeric_value>	not available for FSP
FSE	[SENSe<1|2>:]MIXer:HARMonic:BAND	A | Q | U | V | E | W | F | D | G | Y | J	not available for FSP
FSE	[SENSe<1|2>:]MIXer:HARMonic:TYPE	ODD | EVEN | EODD	not available for FSP
FSE	[SENSe<1|2>:]MIXer:LOSS:HIGH	<numeric_value>	not available for FSP
FSE	[SENSe<1|2>:]MIXer:LOSS:TABLE	<file_name>	not available for FSP
FSE	[SENSe<1|2>:]MIXer:LOSS[:LOW]	<numeric_value>	not available for FSP
FSE	[SENSe<1|2>:]MIXer:PORTs	2 | 3	not available for FSP
FSE	[SENSe<1|2>:]MIXer:SIGNal	2 | 3	not available for FSP
FSE	[SENSe<1|2>:]MIXer:THReshold	0.1 to 100 dB	not available for FSP
FSE	[SENSe<1|2>:]MIXer[:STATe]	ON | OFF	not available for FSP
FSP	[SENSe<1|2>:]MPOWer[:SEQuence]	<analyzer freq>, <rbw>,<meas time>, <trigger source>, <trigger level>, <trigger offset>, <type of meas>, <# of meas>	new function for FSP
FSP	[SENSe<1|2>:]MPOWer:RESult[:LIST]?		new function for FSP
FSP	[SENSe<1|2>:]MPOWer:RESult:MIN?		new function for FSP
FSE	[SENSe<1|2>:]MSUMmary:AHOLd[:STATe]	ON | OFF	not available for FSP and FSET
FSE	[SENSe<1|2>:]MSUMmary:MODE	ABSolute | RELative	not available for FSP and FSET
FSE	[SENSe<1|2>:]MSUMmary:MTIMe	0.1S | 1S	not available for FSP and FSET
FSE	[SENSe<1|2>:]MSUMmary:REFerence	<numeric_value>	not available for FSP and FSET
FSE	[SENSe<1|2>:]MSUMmary:REFerence:AUTO	ONCE	not available for FSP and FSET
FSE	[SENSe<1|2>:]MSUMmary:RUNit	PCT | DB	not available for FSP and FSET
FSET	[SENSe<1|2>:]PM[:DEViation]:RANGe[:UPPer]	<numeric_value>	not available for FSP
FSP + FSE	[SENSe<1|2>:]POWer:ACHannel:ACPairs	0 to 3	FSP: new parameter value 0 for channel power measurement
FSP + FSE	[SENSe<1|2>:]POWer:ACHannel:BANDwidth|BWIDth:ACHannel	100 to 1000MHz	FSP: parameter range starts at 100Hz FSE: parameter range starts at 0 Hz

Devices	Command	Parameter	Notes
FSP + FSE	[SENSe<1|2>:]POWer:ACHannel:BANDwidth|BWIDth:ALTernate<1|2>	100 to 1000MHz	FSP: parameter range starts at 100Hz FSE: parameter range starts at 0 Hz
FSP + FSE	[SENSe<1|2>:]POWer:ACHannel:BANDwidth|BWIDth[:CHANnel]	100 to 1000MHz	FSP: parameter range starts at 100Hz FSE: parameter range starts at 0 Hz
FSP + FSE	[SENSe<1|2>:]POWer:ACHannel:MODE	ABSolute | RELative	
FSP + FSE	[SENSe<1|2>:]POWer:ACHannel:PRESet	ACPower | CPOWer | OBANdwidth | OBWidth	CN and CN0 are not available for FSP
FSP	[SENSe<1|2>:]POWer:ACHannel:PRESet:RLEVel		new function for FSP
FSP + FSE	[SENSe<1|2>:]POWer:ACHannel:REFerence:AUTO	ONCE	
FSP + FSE	[SENSe<1|2>:]POWer:ACHannel:SPACing[:ACHannel]	100Hz to 2000MHz	different parameter range
FSE	[SENSe<1|2>:]POWer:ACHannel:SPACing[:UPPer]	0 to 1000MHz	not available for FSP and FSET
FSP + FSE	[SENSe<1|2>:]POWer:ACHannel:SPACing:ALTernate<1|2>	100Hz to 2000MHz	different parameter range
FSP + FSE	[SENSe<1|2>:]POWer:BANDwidth|BWIDth	10 to 99.9PCT	different parameter range
FSP	[SENSe<1|2>:]POWer:HSPeed	ON | OFF	new function for FSP
FSP	[SENSe<1|2>:]POWer:NCORrection	ON | OFF	new function for FSP
FSP	[SENSe<1|2>:]POWer:TRACe	1 to 3	new function for FSP
FSP + FSE	[SENSe<1|2>:]ROSCillator:[INTernal:]TUNe	0 to 4095	
FSP + FSE	[SENSe<1|2>:]ROSCillator:[INTernal:]TUNe:SAVe		
FSE	[SENSe<1|2>:]ROSCillator:EXTernal:FREQuency	1MHz to 16MHz	not available for FSP
FSP + FSE	[SENSe<1|2>:]ROSCillator:SOURce	INTernal | EXTernal	
FSET/ ESI	[SENSe<1|2>:]SCAN<:RANGes[COUNt]	1 to 10	not available for FSP
FSE/ ESI	[SENSe<1|2>:]SCAN<1...10>:BANDwidth:RESolution	f_{min} to f_{max}	not available for FSP
FSET/ ESI	[SENSe<1|2>:]SCAN<1...10>:INPut:ATTenuation	dB_{min} to dB_{max}	not available for FSP
FSET/ ESI	[SENSe<1|2>:]SCAN<1...10>:INPut:ATTenuation:AUTO	ON | OFF	not available for FSP
FSET	[SENSe<1|2>:]SCAN<1...10>:INPut:BIMPedance	150OHM | 600OHM | 10kOHM	not available for FSP
FSET	[SENSe<1|2>:]SCAN<1...10>:INPut:GAIN	0dB to 30dB	not available for FSP
FSET/ ESI	[SENSe<1|2>:]SCAN<1...10>:INPut:GAIN:AUTO	ON | OFF	not available for FSP
ESI	[SENSe<1|2>:]SCAN<1...10>:INPut:GAIN:STATe	ON | OFF	not available for FSP
ESI	[SENSe<1|2>:]SCAN<1...10>:INPut:TYPE	INPUT1 | INPUT2	not available for FSP
FSET	[SENSe<1|2>:]SCAN<1...10>:INPut:TYPE	RF | BALanced	not available for FSP
FSET/ ESI	[SENSe<1|2>:]SCAN<1...10>:STARt	f_{min} to f_{max}	not available for FSP
FSET/ ESI	[SENSe<1|2>:]SCAN<1...10>:STEP	f_{min} to f_{max}	not available for FSP
FSET/ ESI	[SENSe<1|2>:]SCAN<1...10>:STOP	f_{min} to f_{max}	not available for FSP
FSET/ ESI	[SENSe<1|2>:]SCAN<1...10>:TIME	100 µs to 100 s	not available for FSP
FSP + FSE	[SENSe<1|2>:]SWEep:COUNt	0 to 32767	
FSP + FSE	[SENSe<1|2>:]SWEep:EGATe	ON | OFF	
FSP + FSE	[SENSe<1|2>:]SWEep:EGATe:HOLDoff	0 to 100s	
FSP + FSE	[SENSe<1|2>:]SWEep:EGATe:LENGth	0 to 100s	
FSE	[SENSe<1|2>:]SWEep:EGATe:LENGth	0 to 100s	
FSE	[SENSe<1|2>:]SWEep:EGATe:LEVel	-5V to +5V	not availabe for FSP
FSP + FSE	[SENSe<1|2>:]SWEep:EGATe:POLarity	POSitive | NEGative	
FSP + FSE	[SENSe<1|2>:]SWEep:EGATe:SOURce	EXTernal | IFPower	
FSP + FSE	[SENSe<1|2>:]SWEep:EGATe:TYPE	LEVel | EDGE	
FSE	[SENSe<1|2>:]SWEep:GAP	ON | OFF	not available for FSP
FSE	[SENSe<1|2>:]SWEep:GAP:LENGth	0 to 100s	not available for FSP
FSE	[SENSe<1|2>:]SWEep:GAP:PRETrigger	0 to 100s	not available for FSP
FSE	[SENSe<1|2>:]SWEep:GAP:TRGTogap	0 to 100s	not available for FSP
FSET/ ESI	[SENSe<1|2>:]SWEep:SPACing	LINear | LOGarithmic | AUTO	not available for FSP
FSE/ FSIQ	[SENSe<1|2>:]SWEep:SPACing	LINear | LOGarithmic	not available for FSP

Devices	Command	Parameter	Notes
FSP + FSE	[SENSe<1|2>:]SWEep:TIME	2.5ms to 1000s | 1µs to 16000s	different parameter ranges for FSP and FSE
FSP + FSE	[SENSe<1|2>:]SWEep:TIME:AUTO	ON | OFF	
FSE	[SENSe<1|2>:]TCAPture:LENGth	1024 | 2048 | 4096 | 8192 | 16384	not available for FSP
FSE	[SENSe<1|2>:]TV:PSOFfset	0 to 6.5 MHz	not available for FSP and FSET
FSE	[SENSe<1|2>:]TV[:STATe]	ON | OFF	not available for FSP and FSET
FSP + FSE	SOURce:AM:STATe	ON | OFF	
FSP + FSE	SOURce:DM:STATe	ON | OFF	
FSP	SOURce:EXTernal[:STATe]	ON | OFF	new command for FSP
FSP	SOURce:EXTernal:FREQuency:OFFset	<numeric_value>	new command for FSP
FSP	SOURce:EXTernal:FREQuency[:FACTor]:NUMerator	<numeric_value>	new command for FSP
FSP	SOURce:EXTernal:FREQuency[:FACTor]:DENominator	<numeric_value>	new command for FSP
FSP	SOURce:EXTernal:FREQuency:SWEep[:STATe]	ON | OFF	new command for FSP
FSP	SOURce:EXTernal:POWer[:LEVel]	<numeric_value>	new command for FSP
FSP + FSE	SOURce:FM:STATe	ON | OFF	
FSP + FSE	SOURce:FREQuency:OFFSet	-150Hz to 150MHz	different value ranges for FSP and FSE
FSE	SOURce:POWer:ALC:SOURce	INTernal | EXTernal	not available for FSP and FSET
FSP + FSE	SOURce:POWer[:LEVel][:IMMediate]:OFFSet	-200dB to +200dB	
FSP + FSE	SOURce:POWer[:LEVel][:IMMediate][:AMPLitude]	-30dBm to 0dBm	different value ranges for FSP and FSE
FSP + FSE	STATus:OPERation:CONDition?		
FSE	STATus:OPERation:CONDition?		
FSP + FSE	STATus:OPERation:ENABle	0 to 65535	
FSP + FSE	STATus:OPERation:NTRansition	0 to 65535	
FSP + FSE	STATus:OPERation:PTRansition	0 to 65535	
FSP + FSE	STATus:OPERation[:EVENt?]		
FSP + FSE	STATus:PRESet		
FSP + FSE	STATus:QUEStionable:ACPLimit:CONDition?		
FSP + FSE	STATus:QUEStionable:ACPLimit:ENABle	0 to 65535	
FSP + FSE	STATus:QUEStionable:ACPLimit:NTRansition	0 to 65535	
FSP + FSE	STATus:QUEStionable:ACPLimit:PTRansition	0 to 65535	
FSP + FSE	STATus:QUEStionable:ACPLimit[:EVENt]?		
FSP + FSE	STATus:QUEStionable:CONDition?		
FSP + FSE	STATus:QUEStionable:ENABle	0 to 65535	
FSP + FSE	STATus:QUEStionable:FREQuency:CONDition?		
FSP + FSE	STATus:QUEStionable:FREQuency:ENABle	0 to 65535	
FSP + FSE	STATus:QUEStionable:FREQuency:NTRansition	0 to 65535	
FSP + FSE	STATus:QUEStionable:FREQuency:PTRansition	0 to 65535	
FSP + FSE	STATus:QUEStionable:FREQuency[:EVENt]?		
FSP + FSE	STATus:QUEStionable:LIMit<1|2>:CONDition?		FSP: individual registers for screen A and B
FSP + FSE	STATus:QUEStionable:LIMit<1|2>:ENABle	0 to 65535	FSP: individual registers for screen A and B
FSP + FSE	STATus:QUEStionable:LIMit<1|2>:NTRansition	0 to 65535	FSP: individual registers for screen A and B
FSP + FSE	STATus:QUEStionable:LIMit<1|2>:PTRansition	0 to 65535	FSP: individual registers for screen A and B
FSP + FSE	STATus:QUEStionable:LIMit<1|2>[:EVENt]?		FSP: individual registers for screen A and B
FSP + FSE	STATus:QUEStionable:LMARgin<1|2>:CONDition?		FSP: individual registers for screen A and B
FSP + FSE	STATus:QUEStionable:LMARgin<1|2>:ENABle	0 to 65535	FSP: individual registers for screen A and B
FSP + FSE	STATus:QUEStionable:LMARgin<1|2>:NTRansition	0 to 65535	FSP: individual registers for screen A and B
FSP + FSE	STATus:QUEStionable:LMARgin<1|2>:PTRansition	0 to 65535	FSP: individual registers for screen A and B
FSP + FSE	STATus:QUEStionable:LMARgin<1|2>[:EVENt]?		FSP: individual registers for screen A and B
FSP + FSE	STATus:QUEStionable:NTRansition	0 to 65535	
FSP + FSE	STATus:QUEStionable:POWer:CONDition?		

Devices	Command	Parameter	Notes
FSP + FSE	STATus:QUEStionable:POWer:ENABle	0 to 65535	
FSP + FSE	STATus:QUEStionable:POWer:NTRansition	0 to 65535	
FSP + FSE	STATus:QUEStionable:POWer:PTRansition	0 to 65535	
FSP + FSE	STATus:QUEStionable:POWer[:EVENt]?		
FSP + FSE	STATus:QUEStionable:PTRansition	0 to 65535	
FSE	STATus:QUEStionable:SYNC:CONDition?		not available for FSP
FSE	STATus:QUEStionable:SYNC:ENABle	0 to 65535	not available for FSP
FSE	STATus:QUEStionable:SYNC:NTRansition	0 to 65535	not available for FSP
FSE	STATus:QUEStionable:SYNC:PTRansition	0 to 65535	not available for FSP
FSE	STATus:QUEStionable:SYNC[:EVENt]?		not available for FSP
FSE	STATus:QUEStionable:TRANsducer:CONDition?		not available for FSP
FSE	STATus:QUEStionable:TRANsducer:ENABle	0 to 65535	not available for FSP
FSE	STATus:QUEStionable:TRANsducer:NTRansition	0 to 65535	not available for FSP
FSE	STATus:QUEStionable:TRANsducer:PTRansition	0 to 65535	not available for FSP
FSE	STATus:QUEStionable:TRANsducer[:EVENt]?		not available for FSP
FSP + FSE	STATus:QUEStionable[:EVENt]?		
FSP + FSE	STATus:QUEue[:NEXT?]		
FSE	SYSTem:BINFo?		not available for FSP
FSP	SYSTem:COMMunicate:GPIB:RDEVice:GENerator<1|2>:ADDRess	0 to 30	new command for FSP
FSE	SYSTem:COMMunicate:GPIB:RDEVice<1|2>:ADDRess	0 to 30	not available for FSP
FSP + FSE	SYSTem:COMMunicate:GPIB[:SELF]:ADDRess	0 to 30	
FSP + FSE	SYSTem:COMMunicate:GPIB[:SELF]:RTERminator	LFEOI | EOI	
FSP + FSE	SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt?		
FSP + FSE	SYSTem:COMMunicate:PRINter:ENUMerate:NEXT?		
FSP	SYSTem:COMMunicate:PRINter:SELect<1|2>	<printer_name>	numeric suffix behind SELect
FSIQ/ ESI	SYSTem:COMMunicate:PRINter<1|2>:SELect	<printer_name>	numeric suffix behind PRINters
FSP	SYSTem:COMMunicate:RDEVice:GENerator<1|2>:LINK	GPIB | TTL	new function for FSP
FSP	SYSTem:COMMunicate:RDEVice:GENerator<1|2>:TYPE	<name>	new function for FSP
FSP + FSE	SYSTem:COMMunicate:SERial:CONTrol:DTR	IBFull | OFF	only SERial1 available for FSP
FSP + FSE	SYSTem:COMMunicate:SERial:CONTrol:RTS	IBFull | OFF	only SERial1 available for FSP
FSP + FSE	SYSTem:COMMunicate:SERial[:RECeive]:BAUD	110 | 300 | 600 | 1200 | 2400 | 9600 | 19200	only SERial1 available for FSP
FSP + FSE	SYSTem:COMMunicate:SERial[:RECeive]:BITS	7 | 8	only SERial1 available for FSP
FSP + FSE	SYSTem:COMMunicate:SERial[:RECeive]:PACE	XON | NONE	only SERial1 available for FSP
FSP + FSE	SYSTem:COMMunicate:SERial[:RECeive]:PARity[:TYPE]	EVEN | ODD | NONE	only SERial1 available for FSP
FSP + FSE	SYSTem:COMMunicate:SERial[:RECeive]:SBITs	1 | 2	only SERial1 available for FSP
FSP + FSE	SYSTem:DATE	1980 to 2099, 1 to 12, 1 to 31	
FSP	SYSTem:DISPlay:FPANel	ON | OFF	new function for FSP
FSP + FSE	SYSTem:DISPlay:UPDate	ON | OFF	
FSP + FSE	SYSTem:ERRor[:NEXT]?		new function for FSP, but compatible to SYSTem:ERRor? on the FSE
FSP	SYSTem:ERRor:LIST?		new function for FSP
FSP	SYSTem:ERRor:CLEar:ALL		new command for FSP
FSP + FSE	SYSTem:PASSword[:CENable]	'pass word	
FSP + FSE	SYSTem:PRESet		
ESI/ FSIQ	SYSTem:PRESet:COMPatible	FSE | OFF	not available for FSP
FSP + FSE	SYSTem:SET		
FSP + FSE	SYSTem:SPEaker:VOLume	0 to 1	
FSP + FSE	SYSTem:TIME	0 to 23, 0 to 59, 0 to 59	
FSP + FSE	SYSTem:VERSion?		
FSP + FSE	TRACe:COPY	TRACE1 | TRACE2 | TRACE3 , TRACE1 | TRACE2 | TRACE3	only TRACE1...TRACE3 available for FSP
FSET/ ESI	TRACe:FEED:CONTrol<1...4>	ALWays | NEVer	not available for FSP

Devices	Command	Parameter	Notes
FSP + FSE	TRACe[:DATA]	TRACE1 | TRACE2 | TRACE3 , <block> | <numeric_value>	only TRACE1...TRACE3 available for FSP
FSET/ ESI	TRACe[:DATA]	TRACE1| TRACE2| TRACE3| TRACE4| SINGle| SCAN| STATus, <block> | <numeric_value>	
FSP	TRACe:IQ:DATA?		new function for FSP
FSP	TRACe:IQ:DATA:MEMory?	<offset samples>, <# of samples>	new function for FSP
FSP	TRACe:IQ:SET	<filter type>, <rbw>, <sample rate>, <trigger source>, <trigger slope>, <pretrigger samples>, <# of samples>	new function for FSP
FSP	TRACe:IQ:SRATe	16kHz to 32MHz	new function for FSP
FSP	TRACe:IQ[:STATe]	ON | OFF	new function for FSP
FSP + FSE	TRIGger<1|2>[:SEQuence]:HOLDoff	0 to 100s	
FSE	TRIGger<1|2>[:SEQuence]:LEVel:AF	-120 to +120PCT	not available for FSP
FSE	TRIGger<1|2>[:SEQuence]:LEVel:VIDeo	0 to 100PCT	not available for FSP; replaced by TRIGger:SEQuence:SOURce :VIDeo
FSE	TRIGger<1|2>[:SEQuence]:LEVel[:EXTernal]	-5.0 to +5.0V	not available for FSP
FSP + FSE	TRIGger<1|2>[:SEQuence]:SLOPe	POSitive | NEGative	
FSP	TRIGger<1|2>[:SEQuence]:SOURce	IMMediate | LINE | EXTernal | VIDeo | IFPower	
FSE/ ESI	TRIGger<1|2>[:SEQuence]:SOURce	IMMediate | LINE | EXTernal | VIDeo | RFPower | TV | AF	
FSIQ	TRIGger<1|2>[:SEQuence]:SOURce	IMMediate | LINE | EXTernal | VIDeo | RFPower | AF	
FSET	TRIGger<1|2>[:SEQuence]:SOURce	IMMediate | LINE | EXTernal | VIDeo	
FSP + FSE	TRIGger<1|2>[:SEQuence]:SOURce:VIDeo	0 to 100PCT	
FSE/ ESI	TRIGger<1|2>[:SEQuence]:SYNChronize:ADJust:FRAMe	0 to 100s	not available for FSP
FSE	TRIGger<1|2>[:SEQuence]:SYNChronize:ADJust:FRAMe:AUTO	ONCE	not available for FSP and FSET
FSE	TRIGger<1|2>[:SEQuence]:SYNChronize:ADJust:SLOT	0 to 100s	not available for FSP and FSET
FSE	TRIGger<1|2>[:SEQuence]:SYNChronize:ADJust:SLOT:AUTO	ONCE	not available for FSP and FSET
FSE	TRIGger<1|2>[:SEQuence]:SYNChronize:SOURce	FRAMe | TSC	not available for FSP and FSET
FSE/ ESI	TRIGger<1|2>[:SEQuence]:VIDeo:FIELd:SELect	ALL | ODD | EVEN	not available for FSP
FSE/ ESI	TRIGger<1|2>[:SEQuence]:VIDeo:FORMat:LPFRame	525 | 625	not available for FSP
FSE/ ESI	TRIGger<1|2>[:SEQuence]:VIDeo:LINE:NUMBer	<numeric_value>	not available for FSP
FSE/ ESI	TRIGger<1|2>[:SEQuence]:VIDeo:SSIGnal:POLarity	NEGative | POSitive	not available for FSP
FSP	UNIT<1|2>:POWer	DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMP | V | A | W	available units are compatible to the FSE.
FSE/ FSIQ	UNIT<1|2>:POWer	DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMP | DB | PCT | UNITLESS | DBUV_MHZ | DBMV_MHZ | DBUA_MHZ | DBUV_M | DBIA_M | DBUV_MMHZ | DBUA_MMHZ	for FSP, the following units apply:DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMP | V | A | W

Devices	Command	Parameter	Notes
FSET/ ESI	UNIT<1|2>:POWer	DBM | DBPW | DBPT | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | V | W | DB | PCT | UNITLESS | DBUV_MHZ | DBMV_MHZ | DBUA_MHZ | DBUV_M | DBIA_M | DBUV_MMHZ | DBUA_MMHZ	for FSP, the following units apply:DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMP | V | A | W
FSE	UNIT<1|2>:PROBe	ON | OFF	not available for FSP

Alphabetical List of Commands

In the following, all remote-control commands are listed with their parameters and page numbers. Generally, they are arranged alphabetically according to the keywords of the command. The list of common commands starts the table.

Command	Parameter	Page
*CAL?		6.5
*CLS		6.5
*ESE	0 ... 255	6.5
*ESR?		6.5
*IDN?		6.5
*IST?		6.5
*OPC		6.5
*OPC?		6.5
*OPT?		6.6
*PCB	0 ... 30	6.6
*PRE	0 ... 255	6.6
*PSC	0 | 1	6.6
*RST		6.7
*SRE	0 ... 255	6.7
*STB?		6.7
*TRG		6.7
*TST?		6.7
*WAI		6.7
ABORt		6.8
CALCulate<1|2>:DELTamarker<1...4>:AOFF		6.10
CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:FIXed:RPOint:X	<numeric_value>	6.15
CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:FIXed:RPOint:Y	<numeric_value>	6.15
CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:FIXed:RPOint:Y:OFFSet	<numeric_value>	6.15
CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:FIXed[:STATe]	ON | OFF	6.14
CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:PNOise:RESult?		6.16
CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:PNOise[:STATe]	ON | OFF	6.16
CALCulate<1|2>:DELTamarker<1...4>:MAXimum:LEFT		6.13
CALCulate<1|2>:DELTamarker<1...4>:MAXimum:NEXT		6.12
CALCulate<1|2>:DELTamarker<1...4>:MAXimum[:PEAK]		6.12
CALCulate<1|2>:DELTamarker<1...4>:MAXimum:RIGHt		6.13
CALCulate<1|2>:DELTamarker<1...4>:MINimum:LEFT		6.14
CALCulate<1|2>:DELTamarker<1...4>:MINimum:NEXT		6.13
CALCulate<1|2>:DELTamarker<1...4>:MINimum[:PEAK]		6.13
CALCulate<1|2>:DELTamarker<1...4>:MINimum:RIGHt		6.14
CALCulate<1|2>:DELTamarker<1...4>:MODE	ABSolute | RELative	6.10
CALCulate<1|2>:DELTamarker<1...4>[:STATe]	ON | OFF	6.9
CALCulate<1|2>:DELTamarker<1...4>:TRACe	1...3	6.10
CALCulate<1|2>:DELTamarker<1...4>:X	0 ... MAX (Frequenz | Sweepzeit)	6.11
CALCulate<1|2>:DELTamarker<1...4>:X:RELative		6.11

Command	Parameter	Page
CALCulate<1|2>:DELTamarker<1...4>:Y?		6.12
CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel:ABSolute	-200...200 DBM, -200...200 DBM	6.24
CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel:ABSolute:STATe	ON | OFF	6.25
CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel[:RELative]	0...100 DB, 0...100 DB	6.22
CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel[:RELative]:STATe	ON | OFF	6.23
CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel:RESult?		6.26
CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>:ABSolute	-200...200 DBM, -200...200 DBM	6.29
CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>:ABSolute:STATe	ON | OFF	6.30
CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>[:RELative]	0...100 DB, 0...100 DB	6.27
CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>[:RELative]:STATe	ON | OFF	6.28
CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>:RESult?		6.31
CALCulate<1|2>:LIMit<1...8>:ACPower[:STATe]	ON | OFF	6.21
CALCulate<1|2>:LIMit<1...8>:CLEar[:IMMediate]		6.19
CALCulate<1|2>:LIMit<1...8>:COMMent	<string>	6.20
CALCulate<1|2>:LIMit<1...8>:CONTrol[:DATA]	<numeric value>,<numeric value>	6.32
CALCulate<1|2>:LIMit<1...8>:CONTrol:DOMain	FREQuency | TIME	6.32
CALCulate<1|2>:LIMit<1...8>:CONTrol:MODE	RELative | ABSolute	6.33
CALCulate<1|2>:LIMit<1...8>:CONTrol:OFFset	<numeric value>	6.33
CALCulate<1|2>:LIMit<1...8>:CONTrol:SHIFt	<numeric_value>	6.33
CALCulate<1|2>:LIMit<1...8>:COPY	1...8|<name>	6.20
CALCulate<1|2>:LIMit<1...8>:DELete		6.20
CALCulate<1|2>:LIMit<1...8>:FAIL?		6.19
CALCulate<1|2>:LIMit<1...8>:LOWer[:DATA]	<numeric value>	6.34
CALCulate<1|2>:LIMit<1...8>:LOWer:MARGin	<numeric value>	6.35
CALCulate<1|2>:LIMit<1...8>:LOWer:MODE	RELative | ABSolute	6.35
CALCulate<1|2>:LIMit<1...8>:LOWer:OFFset	<numeric value>	6.35
CALCulate<1|2>:LIMit<1...8>:LOWer:SHIFt	<numeric_value>	6.36
CALCulate<1|2>:LIMit<1...8>:LOWer:STATe	ON | OFF	6.35
CALCulate<1|2>:LIMit<1...8>:LOWer:THReshold	<numeric value>	6.36
CALCulate<1|2>:LIMit<1...8>:NAME	1...8|<string>	6.20
CALCulate<1|2>:LIMit<1...8>:STATe	ON | OFF	6.18
CALCulate<1|2>:LIMit<1...8>:TRACe	<numeric_value>	6.18
CALCulate<1|2>:LIMit<1..8>:UNIT	DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere | DB | DBUV_M | DBUA_M | DEG | RAD | S | HZ | PCT | UNITLESS	6.19
CALCulate<1|2>:LIMit<1...8>:UPPer[:DATA]	<numeric value>	6.37
CALCulate<1|2>:LIMit<1...8>:UPPer:MARGin	<numeric value>	6.38
CALCulate<1|2>:LIMit<1...8>:UPPer:MODE	RELative | ABSolute	6.39
CALCulate<1|2>:LIMit<1...8>:UPPer:OFFset	<numeric value>	6.38
CALCulate<1|2>:LIMit<1...8>:UPPer:SHIFt	<numeric_value>	6.39
CALCulate<1|2>:LIMit<1...8>:UPPer:STATe	ON | OFF	6.38
CALCulate<1|2>:LIMit<1...8>:UPPer:THReshold	<numeric value>	6.39
CALCulate<1|2>:MARKer:FUNCtion:ZOOM	<numeric value>	6.51

Command	Parameter	Page
CALCulate<1|2>:MARKer<1...4>:AOFF		6.41
CALCulate<1|2>:MARKer<1...4>:COUNt	ON | OFF	6.43
CALCulate<1|2>:MARKer<1...4>:COUNt:FREQuency?		6.43
CALCulate<1|2>:MARKer<1...4>:COUNt:RESolution	0.1 | 1 | 10 | 100 | 1000 | 10000 Hz	6.43
CALCulate<1|2>:MARKer<1...4>:FUNCtion:CENTer		6.54
CALCulate<1|2>:MARKer<1...4>:FUNCtion:CSTep		6.55
CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation:CONTinuous	ON | OFF	6.52
CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation:HOLDoff	10ms ... 1000s	6.52
CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation:SELect	AM | FM	6.52
CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation[:STATe]	ON | OFF	6.52
CALCulate<1|2>:MARKer<1...4>:FUNCtion:MDEPth:RESult?		6.53
CALCulate<1|2>:MARKer<1...4>:FUNCtion:MDEPth[:STATe]		6.53
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown	<numeric value>	6.49
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown:FREQuency?		6.50
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown:RESult?		6.50
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown:STATe	ON | OFF	6.50
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NOISe:RESult?		6.51
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NOISe[:STATe]	ON | OFF	6.51
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:PRESet	<standard>	6.60
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:RESult:PHZ	ON | OFF	6.59
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:RESult?	ACPower | CPOWer | OBANdwidth | OBWidth	6.57
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:SELect?	ACPower | CPOWer | OBANdwidth | OBWidth	6.56
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer[:STATe]	OFF	6.60
CALCulate<1|2>:MARKer<1...4>:FUNCtion:REFerence		6.55
CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack:BANDwidth|BWIDth	10 Hz...MAX(SPAN)	6.61
CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack[:STATe]	ON | OFF	6.61
CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack:THReshold	-330 dBm...+30 dBm	6.62
CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack:TRACe	1...3	6.62
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:AOFF		6.73
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:AVERage	ON | OFF	6.72
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN:AVERage:RESult?		6.68
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN:PHOLd:RESult?		6.69
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN:RESult?		6.68
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN[:STATe]	ON | OFF	6.67
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MODE	ABSolute | RELative	6.72
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PHOLd	ON | OFF	6.71
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak:AVERage:RESult?		6.65
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak:PHOLd:RESult?		6.65
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak:RESult?		6.64
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak[:STATe]	ON | OFF	6.64
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:REFerence:AUTO	ONCE	6.73
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS:AVERage:RESult?		6.66
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS:PHOLd:RESult?		6.67
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS:RESult?		6.66

Command	Parameter	Page
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS[:STATe]	ON | OFF	6.66
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation:AVERage:RESult?		6.70
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation:PHOLd:RESult?		6.71
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation:RESult?		6.70
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation[:STATe]	ON | OFF	6.69
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary[:STATe]	ON | OFF	6.64
CALCulate<1|2>:MARKer<1...4>:FUNCtion:TOI:RESult?		6.54
CALCulate<1|2>:MARKer<1...4>:FUNCtion:TOI[:STATe]	ON | OFF	6.54
CALCulate<1|2>:MARKer<1...4>:LOEXclude	ON | OFF	6.44
CALCulate<1|2>:MARKer<1...4>:MAXimum:LEFT		6.46
CALCulate<1|2>:MARKer<1...4>:MAXimum:NEXT		6.45
CALCulate<1|2>:MARKer<1...4>:MAXimum[:PEAK]		6.45
CALCulate<1|2>:MARKer<1...4>:MAXimum:RIGHt		6.46
CALCulate<1|2>:MARKer<1...4>:MINimum:LEFT		6.47
CALCulate<1|2>:MARKer<1...4>:MINimum:NEXT		6.47
CALCulate<1|2>:MARKer<1...4>:MINimum[:PEAK]		6.46
CALCulate<1|2>:MARKer<1...4>:MINimum:RIGHt		6.47
CALCulate<1|2>:MARKer<1...4>:PEXCursion	<numeric value>	6.48
CALCulate<1|2>:MARKer<1...4>[:STATe]	ON | OFF	6.40
CALCulate<1|2>:MARKer<1...4>:TRACe	1...3	6.41
CALCulate<1|2>:MARKer<1...4>:X	0 ... MAX (Frequenz|Sweepzeit)	6.41
CALCulate<1|2>:MARKer<1...4>:X:SLIMits:LEFT	0 ... MAX (Frequenz|Sweepzeit)	6.42
CALCulate<1|2>:MARKer<1...4>:X:SLIMits:RIGHt	0 ... MAX (Frequenz|Sweepzeit)	6.42
CALCulate<1|2>:MARKer<1...4>:X:SLIMits[:STATe]	ON | OFF	6.41
CALCulate<1|2>:MARKer<1...4>:Y:PERCent	0 ... 100%	6.44
CALCulate<1|2>:MARKer<1...4>:Y?		6.44
CALCulate<1|2>:MATH[:EXPRession][:DEFine]	<expr>	6.74
CALCulate<1|2>:MATH:MODE LINear | LOGarithmic		6.75
CALCulate<1|2>:MATH:POS	-100PCT ... 200PCT	6.74
CALCulate<1|2>:MATH:STATe	ON | OFF	6.75
CALCulate:STATistics:APD[:STATe]	ON | OFF	6.76
CALCulate:STATistics:CCDF[:STATe]	ON | OFF	6.76
CALCulate:STATistics:NSAMples	100 ... 1E9	6.77
CALCulate:STATistics:PRESet		6.78
CALCulate:STATistics:Result<1...3>?	MEAN|PEAK|CFACtor|ALL	6.79
CALCulate:STATistics:SCALe:AUTO	ONCE	6.77
CALCulate:STATistics:SCALe:X:RANGe	-10dB...200dB	6.78
CALCulate:STATistics:SCALe:X:RLEVel	-130dBm...30dBm	6.77
CALCulate:STATistics:SCALe:Y:LOWer	-1E-9...0.1	6.78
CALCulate:STATistics:SCALe:Y:UPPer	-1E-8...1.0	6.78
CALCulate<1|2>:THReshold	MIN ... MAX (abhängig von akt. Einheit)	6.80
CALCulate<1|2>:THReshold:STATe	ON | OFF	6.80
CALCulate<1|2>:UNIT:POWer	DBM | V| A| W | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMPere |	6.81
CALibration:ABORt		6.82

Command	Parameter	Page
CALibration[:ALL]?		6.82
CALibration:RESult?		6.83
CALibration:STATe	ON | OFF	6.83
DIAGnostic:SERVice:CSOurce[:POWer]	<numeric_value>	6.85
DIAGnostic:SERVice:INPut[:SELect]	CALibration | RF	6.84
DIAGnostic:SERVice:NSOurce	ON | OFF	6.85
DIAGnostic:SERVice:SFUNction	<string>...	6.84
DIAGnostic:SERVice:STESt:RESult?		6.85
DISPlay:ANNotation:FREQuency	ON | OFF	6.87
DISPlay:CMAP<1...26>:DEFault<1|2>		6.88
DISPlay:CMAP<1...26>:HSL	0..1,0..1,0..1	6.88
DISPlay:CMAP<1...26>:PDEFined	<color>	6.89
DISPlay:FORmat	SINGle | SPLit	6.87
DISPlay:LOGO	ON | OFF	6.87
DISPlay:PSAVe:HOLDoff	0...60	6.87
DISPlay:PSAVe[:STATe]	ON | OFF	6.87
DISPlay[:WINDow<1|2>]:SELect		6.89
DISPlay[:WINDow<1|2>]:TEXT[:DATA]	<string>	6.89
DISPlay[:WINDow<1|2>]:TEXT:STATe	ON | OFF	6.90
DISPlay[:WINDow<1|2>]:TIME	ON | OFF	6.90
DISPlay[:WINDow<1|2>]:TRACe<1...3>:MODE	WRITe | VIEW | AVERage | MAXHold | MINHold	6.92
DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]	10dB ... 200dB	6.90
DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:MODE	ABSolute | RELative	6.90
DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RLEVel	-130dBm ... 30dBm	6.91
DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RLEVel:OFFSet	-200dB ... 200dB	6.91
DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RPOSition	0...100 PCT	6.92
DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RVALue	<numeric value>	6.91
DISPlay[:WINDow<1|2>]:TRACe<1...3>[:STATe]	ON | OFF	6.93
DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y:SPACing	LINear | LOGarithmic	6.92
FORMat[:DATA]	ASCii | REAL[,32]	6.94
FORMat:DEXPort:DSEParator POINt|COMMa		6.94
HCOPy:ABORt		6.95
HCOPy:DESTination<1|2>	'' 'MMEM' | 'SYST:COMM:PRIN' | 'SYST:COMM:CLIP'	6.96
HCOPy:DEVice:COLor	ON | OFF	6.96
HCOPy:DEVice:LANGuage<1|2>	GDI | WMF | EWMF | BMP	6.97
HCOPy[:IMMediate]		6.97
HCOPy:ITEM:ALL		6.98
HCOPy:ITEM:WINDow<1|2>:TABle:STATe	ON | OFF	6.98
HCOPy:ITEM:WINDow<1|2>:TEXT	<string>	6.98
HCOPy:ITEM:WINDow<1|2>:TRACe:STATe	ON | OFF	6.98
HCOPy:PAGE:ORIentation<1|2>	LANDscape | PORTrait	6.99
INITiate<1|2>:CONMeas	ON | OFF	6.100
INITiate<1|2>:CONTinuous	ON | OFF	6.100
INITiate<1|2>:DISPlay	ON | OFF	6.101

Command	Parameter	Page
INITiate<1|2>[:IMMediate]		6.101
INPut<1|2>:ATTenuation	0 ... 70/75dB	6.102
INPut<1|2>:ATTenuation:AUTO	ON | OFF	6.102
INPut<1|2>:EATT (nur mit Option FSP-B25)	0 ... 30dB	6.103
INPut<1|2>:EATT:AUTO (nur mit Option FSP-B25)	ON | OFF	6.103
INPut<1|2>:EATT:STATe (nur mit Option FSP-B25)	ON | OFF	6.103
INPut<1|2>:GAIN:STATe (nur mit Option FSP-B25)	ON | OFF	6.104
INPut<1|2>:IMPedance (nur mit Option FSP-B25)	50 | 75	6.104
INSTrument:COUPle	NONE | RLEVel | CF_B | CF_A	6.106
INSTrument<1|2>:NSELect	1	6.105
INSTrument<1|2>[:SELect]	SANalyzer	6.105
MMEMory:CATalog?	Pfad	6.108
MMEMory:CDIRectory	Verzeichnisname	6.109
MMEMory:CLear:ALL		6.116
MMEMory:CLear:STATe	1,Pfad	6.116
MMEMory:COMMent	<string>	6.118
MMEMory:COPY	Pfad\Datei, Pfad\Datei	6.109
MMEMory:DATA	Dateiname[, <Blockdaten>]	6.110
MMEMory:DELete	Pfad\Dateiname	6.111
MMEMory:LOAD:AUTO	1,Pfad	6.113
MMEMory:LOAD:STATe	1,Pfad	6.112
MMEMory:MDIRectory	Pfad	6.113
MMEMory:MOVE	Pfad	6.114
MMEMory:MSIS	'A:' | 'D:'	6.114
MMEMory:NAME	Pfad\Dateiname	6.114
MMEMory:RDIRectory	Verzeichnisname	6.115
MMEMory:SELect[:ITEM]:ALL		6.117
MMEMory:SELect[:ITEM]:DEFault		6.118
MMEMory:SELect[:ITEM]:HWSettings	ON | OFF	6.116
MMEMory:SELect[:ITEM]:LINes:ALL	ON | OFF	6.117
MMEMory:SELect[:ITEM]:NONE		6.118
MMEMory:SELect[:ITEM]:SCData	ON | OFF	6.117
MMEMory:SELect[:ITEM]:TRACe[:ACTive]	ON | OFF	6.117
MMEMory:STORe<1|2>:STATe	1,Pfad	6.115
MMEMory:STORe<1|2>:TRACe	1...3,Pfad	6.115
OUTPut<1| 2>[:STATe]	ON | OFF	6.119
[SENSe<1|2>:]AVERage:COUNt	0...32767	6.121
[SENSe<1|2>:]AVERage[:STATe<1...3>]	ON | OFF	6.121
[SENSe<1|2>:]AVERage:TYPE	VIDeo | LINear	6.121
[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]	$10Hz...10MHz (Analoge Filter) 1Hz...10MHz (FFT-Filter)	6.122

Command	Parameter	Page
[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:AUTO	ON | OFF	6.123
[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:RATio	0.0001...1	6.123
[SENSe<1|2>:]BANDwidth|BWIDth[:RESolution]:TYPE	NORMal | FFT | CFILter | RRC	6.123
[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo	1Hz...10MHz	6.124
[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo:AUTO	ON | OFF	6.124
[SENSe<1|2>:]BANDwidth|BWIDth:VIDeo:RATio	0.01...1000	6.124
[SENSe<1|2>:]CORRection:COLLect[:ACQuire]	THRough | OPEN	6.126
[SENSe<1|2>:]CORRection:METHod	TRANsmission | REFLexion	6.125
[SENSe<1|2>:]CORRection:RECall		6.126
[SENSe<1|2>:]CORRection[:STATe]	ON | OFF	6.125
[SENSe<1|2>:]DETector[:FUNCtion]:AUTO	ON | OFF	6.127
[SENSe<1|2>:]DETector<1..4>[:FUNCtion]	APEak |NEGative | POSitive | SAMPle | RMS | AVERage | QPEak	6.127
[SENSe<1|2>:]FREQuency:CENTer	0 ... f_{max}	6.128
[SENSe<1|2>:]FREQuency:CENTer:STEP	0 ... f_{max}	6.128
[SENSe<1|2>:]FREQuency:CENTer:STEP:LINK	SPAN | RBW | OFF	6.128
[SENSe<1|2>:]FREQuency:CENTer:STEP:LINK:FACTor	1 ... 100 PCT	6.129
[SENSe<1|2>:]FREQuency:MODE	CW|FIXed | SWEep	6.130
[SENSe<1|2>:]FREQuency:OFFSet	<numeric_value>	6.130
[SENSe<1|2>:]FREQuency:SPAN	0 ... f_{max}	6.129
[SENSe<1|2>:]FREQuency:SPAN:FULL		6.129
[SENSe<1|2>:]FREQuency:STARt	0 ... f_{max}	6.129
[SENSe<1|2>:]FREQuency:STOP	0 ... f_{max}	6.129
[SENSe<1|2>:]LIST:POWer:RESult?		6.136
[SENSe<1|2>:]LIST:POWer[SEQuence]	<analyzer freq>,<ref level>, <rf att>, <el att>, <filter type>, <rbw>,<vbw>,<meas time>,<trigger level>,...	6.132
[SENSe<1|2>:]LIST:POWer:SET	<PEAK meas>, <RMS meas>, <AVG meas>, <trigger mode>, <trigger slope>,<trigger offset>,<gate length>	6.135
[SENSe<1|2>:]LIST:POWer:STATe OFF		6.136
[SENSe<1|2>:]MPOWer:RESult[:LIST]?		6.140
[SENSe<1|2>:]MPOWer:RESult:MIN?		6.140
[SENSe<1|2>:]MPOWer[:SEQuence]	<analyzer freq>,<rbw>,<meas time>,<trigger source>,<trigger level>,<trigger offset>,<type of meas>,<# of meas>	6.138
[SENSe<1|2>:]POWer:ACHannel:ACPairs	0 ... 3	6.142
[SENSe<1|2>:]POWer:ACHannel:BANDwidth|BWIDth:ACHannel	100 ... 1000MHz	6.143
[SENSe<1|2>:]POWer:ACHannel:BANDwidth|BWIDth:ALTernate<1|2>	100...1000MHz	6.143
[SENSe<1|2>:]POWer:ACHannel:BANDwidth|BWIDth[:CHANnel]	100 ... 1000MHz	6.142
[SENSe<1|2>:]POWer:ACHannel:MODE	ABSolute | RELative	6.143
[SENSe<1|2>:]POWer:ACHannel:PRESet	ACPower | CPOWer | OBANdwidth | OBWidth	6.144

Command	Parameter	Page
[SENSe<1|2>:]POWer:ACHannel:PRESet:RLEVel		6.144
[SENSe<1|2>:]POWer:ACHannel:REFerence:AUTO	ONCE	6.143
[SENSe<1|2>:]POWer:ACHannel:SPACing[:ACHannel]	100 ... 2000MHz	6.141
[SENSe<1|2>:]POWer:ACHannel:SPACing:ALTernate<1|2>	100 ... 2000MHz	6.142
[SENSe<1|2>:]POWer:BANDwidth|BWIDth	10 ... 99.9PCT	6.145
[SENSe<1|2>:]POWer:HSPeed	ON | OFF	6.145
[SENSe<1|2>:]POWer:TRACe	1 ... 3	6.145
[SENSe<1|2>:]ROSCillator:[INTernal:]TUNe	0 ... 4095	6.146
[SENSe<1|2>:]ROSCillator:[INTernal:]TUNe:SAVe		6.146
[SENSe<1|2>:]ROSCillator:SOURce	INTernal | EXTernal	6.146
[SENSe<1|2>:]SWEep:COUNt	0 ... 32767	6.148
[SENSe<1|2>:]SWEep:EGATe	ON | OFF	6.148
[SENSe<1|2>:]SWEep:EGATe:HOLDoff	125ns ... 100s	6.149
[SENSe<1|2>:]SWEep:EGATe:LENGth	0 ... 100s	6.149
[SENSe<1|2>:]SWEep:EGATe:POLarity	POSitive | NEGative	6.149
[SENSe<1|2>:]SWEep:EGATe:SOURce	EXTernal | IFPower	6.149
[SENSe<1|2>:]SWEep:EGATe:TYPE	LEVel | EDGE	6.148
[SENSe<1|2>:]SWEep:TIME	5ms ... 1000s | 1µs ... 16000s	6.147
[SENSe<1|2>:]SWEep:TIME:AUTO	ON | OFF	6.147
SOURce<1|2>:AM:STATe	ON | OFF	6.150
SOURce<1|2>:DM:STATe	ON | OFF	6.150
SOURce<1|2>:FM:DEViation	100Hz...10MHz	6.151
SOURce<1|2>:FM:STATe	ON | OFF	6.151
SOURce<1|2>:FREQuency:OFFSet	-150MHz .. 150MHz	6.151
SOURce<1|2>:EXTernal<1|2>:FREQuency[:FACTor]:DENominator	<numeric_value>	6.153
SOURce<1|2>:EXTernal<1|2>:FREQuency[:FACTor]:NUMerator	<numeric_value>	6.154
SOURce<1|2>:EXTernal<1|2>:FREQuency:OFFSet	<numeric_value>	6.155
SOURce<1|2>:EXTernal<1|2>:FREQuency:SWEep[:STATe]	ON | OFF	6.155
SOURce<1|2>:EXTernal<1|2>:POWer[:LEVel]	<numeric_value>	6.155
SOURce<1|2>:EXTernal<1|2>[:STATe]	ON | OFF	6.153
SOURce<1|2>:POWer[:LEVel][:IMMediate][:AMPLitude]	-30dBm ... 0dBm	6.152
SOURce<1|2>:POWer[:LEVel][:IMMediate]:OFFSet	-200dB ... +200dB	6.152
STATus:OPERation:CONDition?		6.157
STATus:OPERation:ENABle	0...65535	6.157
STATus:OPERation[:EVENt?]		6.157
STATus:OPERation:NTRansition	0...65535	6.157
STATus:OPERation:PTRansition	0...65535	6.157
STATus:PRESet		6.158
STATus:QUEStionable:ACPLimit:CONDition?		6.162
STATus:QUEStionable:ACPLimit:ENABle	0...65535	6.162
STATus:QUEStionable:ACPLimit[:EVENt]?		6.162
STATus:QUEStionable:ACPLimit:NTRansition	0...65535	6.163
STATus:QUEStionable:ACPLimit:PTRansition	0...65535	6.163
STATus:QUEStionable:CONDition?		6.158
STATus:QUEStionable:ENABle	0...65535	6.158
STATus:QUEStionable[:EVENt]?		6.158

Command	Parameter	Page
STATus:QUEStionable:FREQuency:CONDition?		6.163
STATus:QUEStionable:FREQuency[:EVENt]?		6.163
STATus:QUEStionable:FREQuency:ENABle	0...65535	6.163
STATus:QUEStionable:FREQuency:NTRansition	0...65535	6.164
STATus:QUEStionable:FREQuency:PTRansition	0...65535	6.164
STATus:QUEStionable:LIMit<1|2>:CONDition?		6.160
STATus:QUEStionable:LIMit<1|2>:ENABle	0...65535	6.160
STATus:QUEStionable:LIMit<1|2>:NTRansition	0...65535	6.161
STATus:QUEStionable:LIMit<1|2>:PTRansition	0...65535	6.161
STATus:QUEStionable:LMARgin<1|2>:CONDition?		6.161
STATus:QUEStionable:LMARgin<1|2>:ENABle	0...65535	6.161
STATus:QUEStionable:LMARgin<1|2>[:EVENt]?		6.161
STATus:QUEStionable:LMARgin<1|2>:NTRansition	0...65535	6.162
STATus:QUEStionable:LMARgin<1|2>:PTRansition	0...65535	6.162
STATus:QUEStionable:NTRansition	0...65535	6.159
STATus:QUEStionable:POWer:CONDition?		6.159
STATus:QUEStionable:POWer:ENABle	0...65535	6.159
STATus:QUEStionable:POWer[:EVENt]?		6.159
STATus:QUEStionable:POWer:NTRansition	0...65535	6.160
STATus:QUEStionable:POWer:PTRansition	0...65535	6.160
STATus:QUEStionable:PTRansition	0...65535	6.159
SYSTem:COMMunicate:GPIB:RDEVice:GENerator<1|2>:ADDRess	0...30	6.166
SYSTem:COMMunicate:GPIB:RDEVice:GENerator<1|2>:LINK	GPIB | TTL	6.166
SYSTem:COMMunicate:GPIB:RDEVice:GENerator<1|2>:TYPE	<name>	6.167
SYSTem:COMMunicate:GPIB[:SELF]:ADDRess	0...30	6.166
SYSTem:COMMunicate:GPIB[:SELF]:RTERminator	LFEOI | EOI	6.166
SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt?		6.170
SYSTem:COMMunicate:PRINter:ENUMerate:NEXT?		6.170
SYSTem:COMMunicate:PRINter:SELect<1|2> <printer_name>		6.170
SYSTem:COMMunicate:SERial:CONTrol:DTR	IBFull | OFF	6.168
SYSTem:COMMunicate:SERial:CONTrol:RTS	IBFull | OFF	6.168
SYSTem:COMMunicate:SERial[:RECeive]:BAUD	110 | 300 | 600 | 1200 | 2400 | 9600 | 19200	6.168
SYSTem:COMMunicate:SERial[:RECeive]:BITS	7 | 8	6.169
SYSTem:COMMunicate:SERial[:RECeive]:PACE	XON | NONE	6.169
SYSTem:COMMunicate:SERial[:RECeive]:PARity[:TYPE]	EVEN | ODD | NONE	6.169
SYSTem:COMMunicate:SERial[:RECeive]:SBITs	1 | 2	6.169
SYSTem:DATE	1980...2099, 1...12, 1...31	6.171
SYSTem:DISPlay:FPANel	ON | OFF	6.171
SYSTem:DISPlay:UPDate	ON | OFF	6.171
SYSTem:ERRor:CLEar:ALL		6.172
SYSTem:ERRor:LIST?		6.172
SYSTem:ERRor?		6.171
SYSTem:PASSword[:CENable]	'Passwort'	6.172
SYSTem:PRESet		6.172
SYSTem:SET		6.173

Command	Parameter	Page
SYSTem:SPEaker:VOLume	0...1	6.173
SYSTem:TIME	0...23, 0...59, 0...59	6.173
SYSTem:VERSion?		6.173
TRACe<1|2>:COPY	TRACE1 | TRACE2 | TRACE3 , TRACE1 | TRACE2 | TRACE3	6.175
TRACe<1|2>[:DATA]	TRACE1 | TRACE2 | TRACE3 , <block> | <numeric_value>	6.174
TRACe<1|2>:IQ:DATA:MEMory?	<offset sample>, <# of samples>	6.179
TRACe<1|2>:IQ:DATA?		6.177
TRACe<1|2>:IQ:SET	<filter type>, <rbw>,<sample rate>,<trigger source>,<trigger slope>,<pretrigger samples>,<# of samples>	6.180
TRACe<1|2>:IQ:SRATe	15.625kHz...32MHz	6.181
TRACe<1|2>:IQ[:STATe]	ON | OFF	6.181
TRIGger<1|2>[:SEQuence]:HOLDoff	0...100s	6.183
TRIGger<1|2>[:SEQuence]:LEVel:VIDeo	0...100PCT	6.182
TRIGger<1|2>[:SEQuence]:SLOPe	POSitive | NEGative	6.183
TRIGger<1|2>[:SEQuence]:SOURce	IMMediate | EXTernal | VIDeo | RFPower	6.182
UNIT<1|2>:POWer	DBM | DBPW | WATT | DBUV | DBMV | VOLT | DBUA | AMP | V | A | W	6.184

Table of Softkeys with IEC/IEEE-Bus Command Assignment

FREQUENCY Key

FREQ	
CENTER	[SENSe:]FREQuency:CENTer <num_value>
CF- SREPSIZE	
0.1 * SPAN	[SENSe:]FREQuency:CENTer:STEP:LINK SPAN; [SENSe:]FREQuency:CENTer:STEP:LINK:FACTor 10PCT
0.5 * SPAN	[SENSe:]FREQuency:CENTer:STEP:LINK SPAN; [SENSe:]FREQuency:CENTer:STEP:LINK:FACTor 50PCT
X * SPAN	[SENSe:]FREQuency:CENTer:STEP:LINK SPAN; [SENSe:]FREQuency:CENTer:STEP:LINK:FACTor <num_value>
0.1 * RBW	[SENSe:]FREQuency:CENTer:STEP:LINK RBW; [SENSe:]FREQuency:CENTer:STEP:LINK:FACTor 10PCT
0.5 * RBW	[SENSe:]FREQuency:CENTer:STEP:LINK RBW; [SENSe:]FREQuency:CENTer:STEP:LINK:FACTor 50PCT
X * RBW	[SENSe:]FREQuency:CENTer:STEP:LINK RBW; [SENSe:]FREQuency:CENTer:STEP:LINK:FACTor <num_value>
= CENTER	no corresponding IEC/IEEE-bus command
= MARKER	no corresponding IEC/IEEE-bus command
MANUAL	[SENSe:]FREQuency:CENTer:STEP <num_value>
START	[SENSe:]FREQuency:STARt <num_value>
STOP	[SENSe:]FREQuency:STOP <num_value>
FREQUENCY OFFSET	[SENSe:]FREQuency:OFFSet <num_value>
SIGNAL TRACK	
TRACK ON OFF	CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack[:STATe] ON | OFF
TRACK BW	CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack:BANDwidth <num_value>
TRACK THRESHOLD	CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack:THReshold <num_value>
SELECT TRACE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:STRack:TRACe 1 | 2 | 3

SPAN Key

SPAN	
SPAN MANUAL	`[SENSe:]FREQuency:SPAN <num_value>`
SWEEPTIME MANUAL	`[SENSe:]SWEeptime <num_value>`
FULL SPAN	`[SENSe:]FREQuency:SPAN:FULL`

ZERO SPAN	`[SENSe:]FREQuency:SPAN 0HZ`
	or
	`[SENSe:]FREQuency:MODE CW | FIXed`

LAST SPAN	no corresponding IEC/IEEE-bus command

AMPT Key

AMPT	
REF LEVEL	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RLEVel <num_value>
RANGE LOG 100 dB	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y:SPACing LOGarithmic; DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe] 100 dB
RANGE LOG MANUAL	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y:SPACing LOGarithmic; DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe] <num_value>
RANGE LINEAR	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y:SPACing LINear
UNIT	
dBm	CALCulate<1|2>:UNIT:POWer DBM
dBmV	CALCulate<1|2>:UNIT:POWer DBMV
dBµV	CALCulate<1|2>:UNIT:POWer DBUV
dBµA	CALCulate<1|2>:UNIT:POWer DBUA
dBpW	CALCulate<1|2>:UNIT:POWer DBPW
VOLT	CALCulate<1|2>:UNIT:POWer VOLT
AMPERE	CALCulate<1|2>:UNIT:POWer AMPere
WATT	CALCulate<1|2>:UNIT:POWer WATT
RF ATTEN MANUAL	INPut:ATTenuation <num_value>
RF ATTEN AUTO	INPut:ATTenuation:AUTO ON
REF LEVEL POSITION	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RPOSition <num_value>
REF LEVEL OFFSET	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RLEVel:OFFSet <num_value>
GRID ABS/REL	DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:MODE ABSolute|RELative
EL ATTEN AUTO	INPut:EATT:AUTO ON (nur mit Option FSP-B25)
EL ATTEN MANUAL	INPut:EATT <num_value> (nur mit Option FSP-B25)
EL ATTEN OFF	INPut:EATT:STATe OFF (nur mit Option FSP-B25)
RF INPUT 50Ω 75Ω	INPut:IMPedance 50 | 75

MKR Key

MKR

MARKER 1..4

```
CALCulate<1|2>:MARKer<1...4>[:STATe]   ON | OFF;
CALCulate<1|2>:MARKer<1...4>:X <numeric value>;
CALCulate<1|2>:MARKer<1...4>:Y?
CALCulate<1|2>:DELTamarker1[:STATe]   ON | OFF;
CALCulate<1|2>:DELTamarker<1...4>:X <numeric value>;
CALCulate<1|2>:DELTamarker<1...4>:Y?
```

MARKER NORM DELTA

```
CALCulate<1|2>:DELTamarker<1...4>[:STATe]   ON | OFF;
```

SIGNAL COUNT

```
CALCulate<1|2>:MARKer<1...4>:COUNt   ON | OFF;
CALCulate<1|2>:MARKer<1...4>:COUNt:FREQuency?
```

REFERENCE FIXED

REF FXD FREQUENCY

```
CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:FIXed[:STATe]  ON | OFF
```

REF POINT LEVEL

```
CALCulate<1|2>:DELTamarker<1..4>:FUNCtion:FIXed:RPOint:Y <num_value>
```

REF POINT LVL OFFSET

```
CALCulate<1|2>:DELTamarker<1..4>:FUNCtion:FIXed:RPOint:Y:OFFSet
                                                          <num_value>
```

REF POINT FREQUENCY

```
CALCulate<1|2>:DELTamarker<1..4>:FUNCtion:FIXed:RPOint:X  <num_value>
```

or:

REF POINT TIME

```
CALCulate<1|2>:DELTamarker<1..4>:FUNCtion:FIXed:RPOint:X  <num_value>
```

MARKER ZOOM

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:ZOOM <num_value>
```

ALL MARKER OFF

```
CALCulate<1|2>:MARKer<1...4>:AOFF
CALCulate<1|2>:DELTamarker<1...4>:AOFF
```

MKR-> TRACE

```
CALCulate<1|2>:MARKer<1...4>:TRACe <num_value>
CALCulate<1|2>:DELTamarker<1...4>:TRACe <num_value>
```

CNT RESOL ...

```
CALCulate<1|2>:MARKer<1...4>:COUNt:RESolution <numeric value>
```

MKR-> Key

MKR->	
SELECT MARKER	no corresponding IEC/IEEE-bus command
PEAK	CALCulate<1|2>:MARKer<1...4>:MAXimum[:PEAK] CALCulate<1|2>:DELTamarker<1...4>:MAXimum[:PEAK]
CENTER = MKR FREQ	CALCulate<1|2>:MARKer<1...4>:FUNCtion:CENTer
REF LEVEL = MKR LVL	CALCulate<1|2>:MARKer<1...4>:FUNCtion:REFerence
NEXT PEAK	CALCulate<1|2>:MARKer<1...4>:MAXimum:NEXT CALCulate<1|2>:DELTamarker<1...4>:MAXimum:NEXT
NEXT MODE	
ABSOLUTE PEAK / MIN	CALCulate<1|2>:MARKer<1...4>:MAXimum:NEXT CALCulate<1|2>:DELTamarker<1...4>:MAXimum:NEXT CALCulate<1|2>:MARKer<1...4>:MINimum:NEXT CALCulate<1|2>:DELTamarker<1...4>:MINimum:NEXT
SEARCH NEXT LEFT	CALCulate<1|2>:MARKer<1...4>:MAXimum:LEFT CALCulate<1|2>:DELTamarker<1...4>:MAXimum:LEFT CALCulate<1|2>:MARKer<1...4>:MINimum:LEFT CALCulate<1|2>:DELTamarker<1...4>:MINimum:LEFT
SEARCH NEXT RIGHT	CALCulate<1|2>:MARKer<1...4>:MAXimum:RIGHt CALCulate<1|2>:DELTamarker<1...4>:MAXimum:RIGHt CALCulate<1|2>:MARKer<1...4>:MINimum:RIGHt CALCulate<1|2>:DELTamarker<1...4>:MINimum:RIGHt
SEARCH LIMITS	
LEFT LIMIT	CALCulate<1|2>:MARKer<1...4>:X:SLIMits[STATe] ON | OFF CALCulate<1|2>:MARKer<1...4>:X:SLIMits:LEFT <num_value>
RIGHT LIMIT	CALCulate<1|2>:MARKer<1...4>:X:SLIMits[STATe] ON | OFF CALCulate<1|2>:MARKer<1...4>:X:SLIMits:RIGHt <num_value>
THRESHOLD	CALCulate<1|2>:THReshold[STATe] ON | OFF CALCulate<1|2>:THReshold <num_value>
SEARCH LIM OFF	CALCulate<1|2>:MARKer<1...4>:X:SLIMits[STATe] OFF CALCulate<1|2>:THReshold[STATe] ON | OFF
PEAK EXCURSION	CALCulate<1|2>:MARKer<1...4>:PEXCursion <num_value>
MKR-> TRACE	CALCulate<1|2>:MARKer<1...4>:TRACe <numeric value> CALCulate<1|2>:DELTamarker<1...4>:TRACe <numeric value>
MKR-> CF STEPSIZE	CALCulate<1|2>:MARKer<1...4>:FUNCtion:CSTep
MIN	CALCulate<1|2>:MARKer<1...4>:MINimum[:PEAK] CALCulate<1|2>:DELTamarker<1...4>:MINimum[:PEAK]
MIN NEXT	CALCulate<1|2>:MARKer<1...4>:MINimum:NEXT CALCulate<1|2>:DELTamarker<1...4>:MINimum:NEXT
NEXT MODE	see above
EXCLUDE LO	CALCulate<1|2>:MARKer<1...4>:LOEXclude ON | OFF

MKR FCTN Key

MKR FUNC

SELECT MARKER

no corresponding IEC/IEEE-bus command

PEAK

```
CALCulate<1|2>:MARKer<1...4>:MAXimum[:PEAK]
CALCulate<1|2>:DELTamarker<1...4>:MAXimum[:PEAK]
```

NOISE MEAS

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NOISe[:STATe] ON | OFF;
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NOISe:RESult?
```

PHASE NOISE

PH NOISE ON OFF

```
CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:PNOise[:STATe]  ON | OFF
CALCulate<1|2>:DELTamarker<1...4>:FUNCtion:PNOise:RESult?
```

REF POINT LEVEL

```
CALCulate<1|2>:DELTamarker<1..4>:FUNCtion:FIXed:RPOint:Y <num_value>
```

REF POINT LVL OFFSET

```
CALCulate<1|2>:DELTamarker<1..4>:FUNCtion:FIXed:RPOint:Y:OFFSet
                                                          <num_value>
```

REF POINT FREQUENCY

```
CALCulate<1|2>:DELTamarker<1..4>:FUNCtion:FIXed:RPOint:X  <num_value>
```

N dB DOWN

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown[:STATe] ON | OFF
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown <num_value>
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown:RESult?
CALCulate<1|2>:MARKer<1...4>:FUNCtion:NDBDown:FREQuency
```

MARKER DEMOD

with option audio demodulator FSP-B3 only

MKR DEMOD ON/OFF

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation[:STATe]  ON | OFF
```

AM

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation:SELect  AM
```

FM

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:DEModulation:SELect  FM
```

MKR STOP TIME

```
CALCulate<1|2>:MARKer<1..4>:FUNCtion:DEModulation:HOLDoff <num_value>
```

MKR-> TRACE

```
CALCulate<1|2>:MARKer<1...4>:TRACe <numeric value>
CALCulate<1|2>:DELTamarker<1...4>:TRACe <numeric value>
```

BW Key

BW	
RES BW MANUAL	[SENSe:]BANDwidth|BWIDth:AUTO OFF [SENSe:]BANDwidth|BWIDth[:RESolution] <num_value>
VIDEO BW MANUAL	[SENSe:]BANDwidth|BWIDth:VIDeo:AUTO OFF [SENSe:]BANDwidth|BWIDth:VIDeo <num_value>
SWEEP TIME MANUAL	[SENSe:]SWEep:TIME:AUTO OFF [SENSe:]SWEep:TIME <num_value>
RES BW AUTO	[SENSe:]BANDwidth|BWIDth[:RESolution]:AUTO ON
VIDEO BW AUTO	[SENSe:]BANDwidth|BWIDth:VIDeo:AUTO ON
SWEEP TIME AUTO	[SENSe:]SWEep:TIME:AUTO ON
COUPLING RATIO	--
RBW / VBW SINE [1/3]	[SENSe:]BANDwidth|BWIDth:VIDeo:RATio 3
RBW / VBW PULSE [.1]	[SENSe:]BANDwidth|BWIDth:VIDeo:RATio 10
RBW / VBW NOISE [10]	[SENSe:]BANDwidth|BWIDth:VIDeo:RATio 0.1
RBW / VBW MANUAL	[SENSe:]BANDwidth|BWIDth:VIDeo:RATio <num_value>
SPAN / RBW AUTO [50]	[SENSe:]BANDwidth|BWIDth[:RESolution]:RATio 0.02
SPAN / RBW MANUAL	[SENSe:]BANDwidth|BWIDth[:RESolution]:RATio <num_value>
COUPLING DEFAULT	[SENSe:]BANDwidth|BWIDth[:RESolution]:AUTO ON; [SENSe:]BANDwidth|BWIDth:VIDeo:AUTO ON; [SENSe:]SWEep:TIME:AUTO ON
FILTER TYPE	[SENSe:]BANDwidth|BWIDth[:RESolution]:TYPE NORMal | FFT | CFILter | RRC

SWEEP Key

SWEEP	
CONTINUOUS SWEEP	INITiate:CONTinuous ON
SINGLE SWEEP	INITiate:CONTinuous OFF; INITiate:IMMediate
CONTINUE SGL SWEEP	INITiate:CONMeasure
SWEEP TIME MANUAL	[SENSe:]SWEep:TIME <num_value>
SWEEP TIME AUTO	[SENSe:]SWEep:TIME:AUTO ON | OFF
SWEEP COUNT	[SENSe:]SWEep:COUNt <num_value>
SGL SWEEP DISP OFF	INITiate:DISPlay OFF INITiate:IMMediate

MEAS Key

MEAS

TIME DOM POWER

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS[:STATe] ON
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak[:STATe] ON
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN[:STATe] ON
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation[:STATe] ON
```

POWER ON OFF

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS[:STATe] ON|OFF
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak[:STATe] ON|OFF
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN[:STATe] ON|OFF
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation[:STATe] ON|OFF
```

RMS

```
CALCulate<1|2>:MARKer<1..4>:FUNCtion:SUMMary:RMS[:STATe] ON | OFF
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS:RESult?
```

PEAK

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak[:STATe] ON | OFF
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak:RESult?
```

MEAN

```
CALCulate<1|2>:MARKer<1..4>:FUNCtion:SUMMary:MEAN[:STATe] ON | OFF
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MEAN:RESult?
```

STANDARD DEVIATION

```
CALCulate<1|2>:MARKer<1..4>:FUNCtion:SUMMary:SDEViation[:STATe] ON|OFF
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation:RESult?
```

LIMITS ON OFF

```
CALCulate<1|2>:MARKer<1...4>:SLIMits ON | OFF
```

START LIMIT

```
CALCulate<1|2>:MARKer<1...4>:SLIMits:LEFT <num_value>
```

STOP LIMIT

```
CALCulate<1|2>:MARKer<1...4>:SLIMits:RIGHt <num_value>
```

SET REFERENCE

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:REFerence:AUTO ONCE
```

POWER ABS REL

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:MODE ABS | REL
```

MAX HOLD ON OFF

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PHOLd ON | OFF
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak:PHOLd:RESult?
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS:PHOLd:RESult?
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMar:MEAN:PHOLd:RESult?
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation:PHOLd:RESult?
```

AVERAGE ON OFF

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:AVERage ON | OFF
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:PPEak:AVERage:RESult?
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:RMS:AVERage:RESult?
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMar:MEAN:AVERage:RESult?
CALCulate<1|2>:MARKer<1...4>:FUNCtion:SUMMary:SDEViation:AVERage:RES?
```

NUMBER OF SWEEPS

```
[SENSe:]SWEep:COUNt <num_value>
```

CHAN PWR ACP

```
--
```

CP / ACP ON OFF

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:SELect CPOWer | ACPower;
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:RESult? CPOWer | ACPower;
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer[:STATe] OFF
```

CP / ACP STANDARD

```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:PRESet  <standard>
```

CP / ACP CONFIG

```
--
```

NO. OF ADJ CHAN

```
[SENSe:]POWer:ACHannel:ACPairs <num_value>
```

CHANNEL BANDWIDTH

```
[SENSe:]POWer:ACHannel:BANDwidth|BWIDth[:CHANnel] <num_value>
```

ADJ CHAN BANDWIDTH
```
[SENSe:]POWer:ACHannel:BANDwidth|BWIDth:ACHannel <num_value>
[SENSe:]POWer:ACHannel:BANDwidth|BWIDth:ALTernate<1|2> <num_value>
```

ADJ CHAN SPACING
```
[SENSe:]POWer:ACHannel:SPACing:ACHannel <num_value>
[SENSe:]POWer:ACHannel:SPACing:ALTernate<1|2> <num_value>
```

CP/ACP ABS/REL
```
[SENSe:]POWer:ACHannel:MODE ABSolute|RELative
```

FAST ACP ON OFF
```
[SENSe:]POWer:HSPeed ON | OFF
```

SELECT TRACE
```
[SENSe:]POWer:TRACe 1|2|3
```

ADJUST REF LVL
```
[SENSe:]POWer:ACHannel:PRESet:RLEVel
```

ADJUST SETTINGS
```
[SENSe:]POWer:ACHannel:PRESet ACPower|CPOWer|OBANdwidth|OBWidth
```

ACP LIMIT CHECK
```
CALCulate<1|2>:LIMit<1...8>:ACPower[:STATe] ON | OFF
CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel:RESult?
CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate<1|2>:RESult?
```

EDIT ACP LIMITS
```
CALCulate<1|2>:LIMit<1...8>:ACPower[:STATe] ON | OFF
CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel[:RELative]:STATe ON | OFF
CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel[:RELative]
                                        <num_val>,<num_val>
CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel:ABSolute:STATe ON | OFF
CALCulate<1|2>:LIMit<1...8>:ACPower:ACHannel:ABSolute
                                        <num_value>,<num_value>
CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate[:RELative]:STATe ON | OFF
CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate[:RELative]
                                        <num_value>,<num_value>
CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate:ABSolute:STATe ON | OFF
CALCulate<1|2>:LIMit<1...8>:ACPower:ALTernate:ABSolute
                                        <num_value>,<num_value>
```

SET CP REFERENCE
```
[SENSe:]POWer:ACHannel:REFerence:AUTO ONCE
```

CHAN PWR /HZ
```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:RESult:PHZ ON | OFF
```

SWEEP TIME
```
[SENSe:]SWEep:TIME <num_value>
```

ADJUST REF LVL
```
[SENSe:]POWer:ACHannel:PRESet:RLEVel
```

ADJUST SETTINGS
```
[SENSe:]POWer:ACHannel:PRESet ACPower|CPOWer|OBANdwidth|OBWidth
```

OCCUPIED PWR BANDW

OCCUP BW ON OFF
```
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:SELect OBANdwidth | OBWidth
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer:RESult? OBANdwidth| OBWidth
CALCulate<1|2>:MARKer<1...4>:FUNCtion:POWer[:STATe] OFF
```

% POWER BANDWIDTH
```
[SENSe:]POWer:BANDwidth|BWIDth <num_value>
```

CHANNEL BANDWIDTH
```
[SENSe:]POWer:ACHannel:BANDwidth|BWIDth <num_value>
```

NOISE CORR ON OFF
```
[SENSe:]POWer:NCORrection ON | OFF
```

ADJUST REF LVL
```
[SENSe:]POWer:ACHannel:PRESet:RLEVel
```

ADJUST SETTINGS
```
[SENSe:]POWer:PRESet ACPower|CPOWer|OBANdwidth|OBWidth
```

SIGNAL STATISTIC	
APD ON OFF	CALCulate:STATistics:APD[:STATe] ON | OFF CALCulate:STATistics:RESult<1...3>? MEAN | PEAK | CFACtor | ALL
CCDF ON OFF	CALCulate:STATistics:CCDF[:STATe] ON | OFF CALCulate:STATistics:RESult<1...3>? MEAN | PEAK | CFACtor | ALL
PERCENT MARKER	CALC:MARK:Y:PERC 0...100%
RES BW	[SENSe:]BANDwidth[:RESolution]:AUTO OFF [SENSe:]BANDwidth[:RESolution] <num_value>
NO OF SAMPLES	CALCulate:STATistics:NSAMples <num_value>
SCALING	--
X-AXIS REF LEVEL	CALCulate:STATistics:X:RLEVel <num_value>
X-AXIS RANGE	CALCulate:STATistics:X:RANGe <num_value>
Y-AXIS MAX VALUE	CALCulate:STATistics:Y:UPPER <num_value>
Y-AXIS MIN VALUE	CALCulate:STATistics:Y:LOWer <num_value>
ADJUST SETTINGS	CALCulate:STATistics:SCALe:AUTO ONCE
DEFAULT SETTINGS	CALCulate:STATistics:PRESet
ADJUST SETTINGS	CALCulate:STATistics:SCALe:AUTO ONCE
SINGLE MEAS	INITiate:CONTinuous OFF; INITiate:IMMediate
COUNT MEAS	INITiate:CONTinuous ON; INITiate:IMMediate
MODULATION DEPTH	CALCulate<1|2>:MARKer<1...4>:FUNCtion:MDEPth[:STATe] ON | OFF CALCulate<1|2>:MARKer<1...4>:FUNCtion:MDEPth:RESult?
TOI	CALCulate<1|2>:MARKer<1...4>:FUNCtion:TOI[:STATe] ON | OFF CALCulate<1|2>:MARKer<1...4>:FUNCtion:TOI:RESult?
SELECT MARKER	no corresponding IEC/IEEE-bus command

TRIG Key

TRIG	
FREE RUN	TRIGger[:SEQuence]:SOURce IMMediate
VIDEO	TRIGger[:SEQuence]:SOURce VIDeo TRIGger[:SEQuence]:LEVel:VIDeo <numeric value>
EXTERN	TRIGger[:SEQuence]:SOURce EXTernal [SENSe:]SWEep:EGATe:SOURce EXTernal
IF POWER	TRIGger[:SEQuence]:SOURce IFPower [SENSe:]SWEep:EGATe:SOURce IFPower
TRIGGER OFFSET	TRIGger[:SEQuence]:HOLDoff <num_value>
POLARITY POS/NEG	TRIGger[:SEQuence]:SLOPe POSitive | NEGative oder [SENSe:]SWEep:EGATe:POLarity POSitive | NEGative
GATED TRIGGER	[SENSe:]SWEep:EGATe ON | OFF [SENSe:]SWEep:EGATe:SOURce IFPower | EXTernal
GATE SETTINGS	--
GATE MODE LEVEL/EDGE	[SENSe:]SWEep:EGATe:TYPE LEVel | EDGE
POLARITY POS/NEG	[SENSe:]SWEep:EGATe:POLarity POSitive | NEGative
GATE DELAY	[SENSe:]SWEep:EGATe:HOLDoff <num_value>
GATE LENGTH	[SENSe:]SWEep:EGATe:LENGth <num_value>
SWEEP TIME	--

TRACE Key

TRACE	
SELECT TRACE	--
CLEAR/ WRITE	DISPlay[:WINDow<1|2>]:TRACe<1...3>:MODE WRITe
MAX HOLD	DISPlay[:WINDow<1|2>]:TRACe<1...3>:MODE MAXHold
AVERAGE	DISPlay[:WINDow<1|2>]:TRACe<1...3>:MODE AVERage oder: [SENSe:]AVERage[:STATe<1...3>] ON
VIEW	DISPlay[:WINDow<1|2>]:TRACe<1...3>:MODE VIEW
BLANK	DISPlay[:WINDow<1|2>]:TRACe<1...3>[:STATe] OFF
SWEEP COUNT	[SENSe:]SWEep:COUNt <num_value> oder: [SENSe:]AVERage:COUNt <num_value>
DETECTOR	--
AUTO SELECT	[SENSe:]DETector[:FUNCtion]:AUTO ON | OFF
DETECTOR AUTOPEAK	[SENSe:]DETector[:FUNCtion] APEak
DETECTOR MAX PEAK	[SENSe:]DETector[:FUNCtion] POSitive
DETECTOR MIN PEAK	[SENSe:]DETector[:FUNCtion] NEGative
DETECTOR SAMPLE	[SENSe:]DETector[:FUNCtion] SAMPle
DETECTOR RMS	[SENSe:]DETector[:FUNCtion] RMS
DETECTOR AVERAGE	[SENSe:]DETector[:FUNCtion] AVERage
DETECTOR QPK	[SENSe:]DETector[:FUNCtion] QPEak
TRACE MATH	--
T1-T2->T1	CALCulate<1|2>:MATH:STATe ON CALCulate<1|2>:MATH[:EXPRession][:DEFine] (TRACE1 - TRACE2)
T1-T3->T1	CALCulate<1|2>:MATH:STATe ON CALCulate<1|2>:MATH[:EXPRession][:DEFine] (TRACE1 - TRACE3)
TRACE POSITION	CALCulate<1|2>:MATH:POSition <num_value>
TRACE MATH OFF	CALCulate<1|2>:MATH:STATe OFF

MIN HOLD	DISPlay[:WINDow<1|2>]:TRACe<1...3>:MODE MINHold
AVG MODE LOG LIN	CALCulate<1|2>:MATH:MODE LINear | LOGarithmic or: [SENSe:]AVERage:TYPE VIDeo | LINear
ASCII FILE EXPORT	FORMat[:DATA] ASCii MMEMory:STORe<1|2>:TRACe 1,'TRACE.DAT'
DECIM SEP . ,	FORMat:DEXPort:DSEParator POINt | COMMa
COPY TRACE	TRACe:COPY TRACE1|TRACE2|TRACE3,TRACE1|TRACE2|TRACE3

LINES Key

LINES

SELECT LIMIT LINE

selection:
CALCulate<1|2>:LIMit<1...8>:NAME <string>;
CALCulate<1|2>:LIMit<1...8>:UPPer:STATe ON | OFF
CALCulate<1|2>:LIMit<1...8>:LOWer:STATe ON | OFF
limit check:
CALCulate<1|2>:LIMit<1...8>:STATe ON | OFF
INITiate[:IMMediate]; WAI*
CALCulate<1|2>:LIMit<1...8>:FAIL?
trace assignment:
CALCulate<1|2>:LIMit<1...8>:TRACe 1|2|3

NEW LIMIT LINE

NAME

name:
CALCulate<1|2>:LIMit<1...8>:NAME <string>;
domain:
CALCulate<1|2>:LIMit<1...8>:CONTrol:DOMain FREQuency|TIME
scaling:
CALCulate<1|2>:LIMit<1...8>:CONTrol:MODE RELative | ABSolute
CALCulate<1|2>:LIMit<1...8>:UPPer:MODE RELative | ABSolute
CALCulate<1|2>:LIMit<1...8>:LOWer:MODE RELative | ABSolute
unit:
CALCulate<1|2>:LIMit<1...8>:UNIT DBM| DBPW| WATT| DBUV|
VOLT|DBUA|AMPere| DB| DBUV_MHZ| DBUA_MHZ| DEG| RAD| S| HZ| PCT
margin:
CALCulate<1|2>:LIMit<1...8>:UPPer:MARGin <num_value>
CALCulate<1|2>:LIMit<1...8>:LOWer:MARGin <num_value>
threshold for relative y-scaling::
CALCulate<1|2>:LIMit<1...8>:UPPer:THReshold <num_value>
CALCulate<1|2>:LIMit<1...8>:LOWer:THReshold <num_value>
comment:
CALCulate<1|2>:LIMit<1...8>:COMMent <string>

VALUES

CALCulate<1|2>:LIMit<1...8>:CONTrol[:DATA] <num_value>, <num_value>..
CALCulate<1|2>:LIMit<1...8>:UPPer[:DATA] <num_value>, <num_value>..
CALCulate<1|2>:LIMit<1...8>:LOWer[:DATA] <num_value>,<num_value>..

INSERT VALUE

no corresponding IEC/IEEE-bus command

DELETE VALUE

no corresponding IEC/IEEE-bus command

SHIFT X LIMIT LINE

CALCulate<1|2>:LIMit<1...8>:CONTrol:SHIFt <num_value>

SHIFT Y LIMIT LINE

CALCulate<1|2>:LIMit<1...8>:UPPer:SHIFt <num_value>
CALCulate<1|2>:LIMit<1...8>:LOWer:SHIFt <num_value>

SAVE LIMIT LINE

automatically executed during IEC/IEEE-bus operation

EDIT LIMIT LINE

s. EDIT LIMIT LINE

COPY LIMIT LINE

CALCulate<1|2>:LIMit<1...8>:COPY 1...8 | <name>

DELETE LIMIT LINE

CALCulate<1|2>:LIMit<1...8>:DELete

X OFFSET

CALCulate<1|2>:LIMit<1...8>:CONTrol:OFFset <num_value>

Y OFFSET

CALCulate<1|2>:LIMit<1...8>:UPPer:OFFset <num_value>
CALCulate<1|2>:LIMit<1...8>:LOWer:OFFset <num_value>

DISP Key

DISP	
FULL SCREEN	DISPlay:FORmat SINGle DISPlay[:WINDow<1|2>]:SELect
SPLIT SCREEN	DISPlay:FORmat SPLit
REF LEVEL COUPLED	INSTrument:COUPle RLEVel | NONE
CENTER B = MARKER A	INSTrument:COUPle CF_B | NONE
CENTER A = MARKER B	INSTrument:COUPle CF_A | NONE
CONFIG DISPLAY	--
SCREEN TITLE	DISPlay[:WINDow<1|2>]:TEXT[:DATA] <string> DISPlay[:WINDow<1|2>]:TEXT:STATe ON | OFF
TIME/DATE ON OFF	DISPlay[:WINDow<1|2>]:TIME ON | OFF
LOGO ON/OFF	DISPlay:LOGO ON|OFF
ANNOTATION ON/OFF	DISPlay:ANNotation:FREQuency ON|OFF
DATAENTRY OPAQUE	ohne Funktion im IEC-Bus-Betrieb
DEFAULT COLORS 1	DISPlay:CMAP<1...13>:DEFault1
DEFAULT COLORS 2	DISPlay:CMAP<1...13>:DEFault2
DISPLAY PWR SAVE	DISPlay:PSAVe[:STATe] ON | OFF DISPlay:PSAVe:HOLDoff <num_value>
SELECT OBJECT	--
BRIGHTNESS	DISPlay:CMAP:HSL <hue>,<sat>,<lum>
TINT	DISPlay:CMAP<1...13>:HSL <hue>,<sat>,<lum>
SATURATION	DISPlay:CMAP<1...13>:HSL <hue>,<sat>,<lum>
PREDEFINED COLORS	DISPlay:CMAP<1...13>:PDEFined BLACk| BLUE| BROWn| GREen| CYAN| RED| MAGenta| YELLow| WHITe| DGRAy| LGRAy| LBLUe| LGREen| LCYan| LRED| MAGenta

FILE Key

FILE	
SAVE	MMEMory:STORe:STATe 1,<file_name>
RECALL	MMEMory:LOAD:STATe 1,<file_name>
EDIT COMMENT	MMEMory:COMMent <string>
ITEMS TO SAVE/RCL	
SELECT ITEMS	MMEMory:SELect[:ITEM]:HWSettings ON|OFF MMEMory:SELect[:ITEM]:TRACe[:ACTive] ON|OFF MMEMory:SELect[:ITEM]:LINes:ALL ON|OFF MMEMory:SELect[:ITEM]:NONE
DEFAULT CONFIG	MMEMory:SELect[:ITEM]:DEFault
DISABLE ALL ITEMS	MMEMory:SELect[:ITEM]:NONE
ENABLE ALL ITEMS	MMEMory:SELect[:ITEM]:ALL
DATA SET LIST	--
DATA SET CLEAR	MMEMory:CLEar:STATe 1,<file_name>
DATA SET CLEAR ALL	MMEMory:CLEar:ALL
STARTUP RECALL	MMEMory:LOAD:AUTO 1,<file_name>
FILE MANAGER	
EDIT PATH	MMEMory:MSIS <device> MMEMory:CDIRectory <directory_name>
MAKE DIRECTORY	MMEMory:MDIRectory <directory_name>
FORMAT DISK	MMEMory:INITialize <msus>
RENAME	MMEMory:MOVE <file_source>,<file_destination>
SORT MODE	no corresponding IEC/IEEE-bus command
COPY	MMEMory:COPY <file_source>,<file_destination>
DELETE	MMEMory:DELete <file_name> MMEMory:RDIRectory <directory_name>

CAL Key

CAL	
CAL TOTAL	CALibration[:ALL]?
CAL ABORT	CALibration:ABORt
CAL CORR ON OFF	CALibration:STATe ON | OFF
CAL RESULTS	CALibration:RESults?

SETUP Key

REFERENCE INT/EXT	[SENSe:]ROSCillator:SOURce INTernal|EXTernal
NOISE SCR ON OFF	DIAGnostic:SERVice:NSOurce ON | OFF <num_value>
PREAMP	INPut:GAIN <num_value> (nur mit Option Electronic Attenuator - FSP-B25)
GENERAL SETUP	--
GPIB ADDRESS	SYSTem:COMMunicate:GPIB[:SELF]:ADDRess 0...30
COM INTERFACE	SYSTem:COMMunicate:SERial[:RECeive:]BAUD <num_value> SYSTem:COMMunicate:SERial[:RECeive]:BITS 7 | 8 SYSTem:COMMunicate:SERial:RECeive:PARity[:TYPE] EVEN | ODD | NONE SYSTem:COMMunicate:SERial[:RECeive]:SBITs 1|2 SYSTem:COMMunicate:SERial:CONTrol:DTR IBFull | OFF SYSTem:COMMunicate:SERial:CONTrol:RTS IBFull | OFF SYSTem:COMMunicate:SERial[:RECeive]:PACE XON | NONE
TIME+DATE	SYSTem:TIME 0...23, 0...59, 0...59 SYSTem:DATE <num>,<num>,<num>
CONFIGURE NETWORK	with option LAN-Interface FSP-B16 only --
NETWORK LOGIN	with option LAN-Interface FSP-B16 only --
SOFT FRONTPANEL	--
SYSTEM INFO	--
HARDWARE INFO	--
STATISTICS	--
SYSTEM MESSAGES	SYSTem:ERRor?
CLEAR ALL MESSAGES	SYSTem:ERRor?
SAVE CHANGES	--
SERVICE	--
INPUT RF	DIAGnostic:SERVice:INPut[:SELect] RF
INPUT CAL	DIAGnostic:SERVice:INPut[:SELect] CALibration DIAGnostic:SERVice:CSOurce[:POWer] <num_value>
SELFTEST	*TST?
SELFTEST RESULTS	DIAGnostic:SERVice:STEst:RESult?
REFERENCE FREQUENCY	[SENSE<1|2>:]ROSCillator[:INTernal]:TUNe 0...4095
CAL SIGNAL POWER	--

SAVE CHANGES	[SENSE<1|2>:]ROSCillator[:INTernal]:TUNe:SAVe
ENTER PASSWORD	SYSTem:PASSword[:CENable] <string>
SERVICE FUNCTION	DIAGnostic:SERVice:SFUNction <string>
FIRMWARE UPDATE	--
RESTORE FIRMWARE	--

HCOPY Key

HCOPY	
PRINT SCREEN	HCOPy:ITEM:ALL HCOPy:IMMediate for printout into file add MMEMory:NAME <file_name>
PRINT TRACE	HCOPy:ITEM:WINDow<1|2>:TRACe:STATe ON | OFF HCOPy:IMMediate for printout into file add MMEMory:NAME <file_name>
PRINT TABLE	HCOPy:ITEM:WINDow<1|2>:TABle:STATe ON | OFF HCOPy:IMMediate for printout into file add MMEMory:NAME <file_name>
HARDCOPY ABORT	HCOPy:ABORt
DEVICE1	SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt? SYSTem:COMMunicate:PRINter:ENUMerate:NEXT? SYSTem:COMMunicate:PRINter:SELect <string> HCOPy:DESTination <string> HCOPy:DEVice:LANGuage GDI | WMF | EWMF | BMP HCOPy:PAGE:ORIentation<1|2> LANDscape | PORTrait
DEVICE2	SYSTem:COMMunicate:PRINter:ENUMerate:FIRSt? SYSTem:COMMunicate:PRINter:ENUMerate:NEXT? SYSTem:COMMunicate:PRINter:SELect "string> HCOPy:DESTination2 <string> HCOPy:DEVice:LANGuage GDI | WMF | EWMF | BMP HCOPy:PAGE:ORIentation<1|2> LANDscape | PORTrait
COLOR ON/OFF	HCOPy:DEVice:COLor ON | OFF
COMMENT SCREEN A/B	HCOPy:ITEM:WINDow<1|2>:TEXT <string>
INSTALL PRINTER	

Hotkeys

SPECTRUM

```
INSTrument[:SELect] SANalyzer
INSTrument:NSELect 1
```

NETWORK

with option tracking generator FSP-B9 or option external generator control FSP-B10 only.
--

SCREEN A/B

FULL SCREEN: Selection of the active window: `DISPlay[:WINDow<1|2>]:SELect`
The window valid for the setting is selected by the numeric suffix in the command, eg `SENSe<1|2>`

SPLIT SCREEN: The two measurement windows are active.
The window valid for the setting is selected by the numeric suffix in the command, eg `SENSe<1|2>`

Hotkey NETWORK

NETWORK

with option tracking generator FSP-B9 or option external generator control FSP-B10 only

--

SOURCE ON / OFF

with option tracking generator FSP-B9 only

```
OUTPut:STATe ON | OFF
```

SOURCE POWER

```
SOURce:POWer <num_value>
```

POWER OFFSET

```
SOURce:POWer:OFFSet <num_value>
```

SOURCE CAL

with option tracking generator FSP-B9 or option external generator control FSP-B10 only

CAL TRANS

```
[SENSe:]CORRection:METHod TRANsmission
[SENSe:]CORRection:COLLect[:ACQuire] THRough
```

CAL REFL SHORT

```
[SENSe:]CORRection:METHod REFLexion
[SENSe:]CORRection:COLLect[:ACQuire] THRough
```

CAL REFL OPEN

```
[SENSe:]CORRection:METHod REFLexion
[SENSe:]CORRection:COLLect[:ACQuire] OPEN
```

NORMALIZE

```
[SENSe:]CORRection[:STATe] ON | OFF
```

REF VALUE POSITION

```
DISP:WIND:TRAC:Y:RPOS <num_value>
```

REF VALUE

```
DISP:WIND:TRAC:Y:RVAL <num_value>
```

RECALL

```
[SENSe:]CORRection:RECall
```

FREQUENCY OFFSET

with option tracking generator FSP-B9 only

```
SOURce:FREQuency:OFFSet <num_value>
```

MODULATION

with option tracking generator FSP-B9 only

EXT AM

```
SOURce:AM:STATe ON|OFF
```

EXT FM

```
SOURce:FM:STATe ON|OFF
SOURce:FM:DEViation <num_value>
```

EXT I/Q

```
SOURce:DM:STATe ON|OFF
```

MODULATION OFF

```
--
```

EXT SOURCE

with option external generator control FSP-B10 only

EXT SRC ON / OFF

```
SOURce:EXTernal[:STATe] ON | OFF
```

SELECT GENERATOR

```
SYSTem:COMMunicate:RDEVice:GENerator:TYPE 'SME02'
SYSTem:COMMunicate:RDEVice:GENerator:LINK TTL
SYSTem:COMMunicate:GPIB:RDEVice:GENerator:ADDRess 28
```

FREQUENCY SWEEP

```
SOURce:EXTernal:POWer -30dBm
SOURce:EXTernal:FREQuency:NUMerator 4
SOURce:EXTernal:FREQuency:DENominator 3
SOURce:EXTernal:FREQuency:OFFSet 100MHZ
```

Contents - Chapter 7 "Remote Control - Programming Examples"

7 Remote Control - Programming Examples 7.1

Basic Steps of IEC/IEEE-Bus Programming 7.1

Including IEC-Bus Library for VisualBasic 7.1

Initialization and Default Status 7.2

Creating global variables 7.2

Initiate Controller 7.2

Initiate Instrument 7.3

Configuring Power Save Function of Display 7.3

Transmission of Simple Instrument Setting Commands 7.4

Return to manual control 7.4

Reading out Instrument Settings 7.4

Positioning a Marker and Displaying Values 7.5

Command synchronization 7.6

Service Request 7.7

Initiate Service Request 7.7

Service request routine 7.8

Read Out of Output Buffer 7.8

Read Out of Error Messages 7.9

Evaluation of SCPI Status Registers 7.9

Evaluation of Event Status Register 7.10

More Complex Programming Examples 7.11

Basic settings of the Analyzer 7.11

Setting the IEC/IEEE Bus Status Register 7.11

Default Setting for Measurements 7.12

Using Marker and Delta Marker 7.13

Marker Search Functions, Limitation of Search Range 7.13

Frequency Counting 7.15

Operation mit Fixed Reference Point (Reference Fixed) 7.16

Phase and Phase Noise Measurement 7.17

Shape Factor Measurement (using n-dB down) 7.18

Measuring the Third Order Intercept Point 7.19

Measuring the AM Modulation Depth 7.20

Limit Lines and Limit Test 7.21

Measuring the Channel and Adjacent Channel Power 7.23

Occupied Bandwidth Measurement 7.25

Time Domain Power Measurement 7.26

Reading Trace Data 7.27

Storing and Loading Device Settings 7.29

Storing Instrument Settings 7.29

Loading Device Settings 7.30

Setting the Data Set for Startup Recall 7.30

Reading and Writing Files 7.31

Reading a File from the Instrument 7.31

Creating a File in the Instrument 7.32

Configuring and Starting a Printout 7.33

7 Remote Control - Programming Examples

The following programming examples have a hierarchical structure, ie subsequent examples are based on previous ones. It is thus possible to compile very easily an operational program from the modules of the given examples.

Basic Steps of IEC/IEEE-Bus Programming

The examples explain the programming of the instrument and can serve as a basis to solve more complex programming tasks.

VISUAL BASIC has been used as programming language. However, the programs can be translated into other languages.

Including IEC-Bus Library for VisualBasic

Programming hints:

- **Output of texts using the "Print" function**

  The following programming examples are based on the assumption that all subroutines are part of a form (file extension: .FRM). In this case the syntax

  ```
  Print "Text"
  ```

  is allowed.

  If however the subroutines are stored as a so-called module (file extension: .BAS), the print instruction should be preceded by the name of a form which has the required print method. If, for example, there is a form with the name "Main", the associated print instruction is as follows:

  ```
  Main.Print "Text".
  ```

- **Access to funtions of GPIB.DLL**

  To create Visual Basic control applications the file GPIB.BAS (as from VB 6.0 VBIB-32.BAS) is added to a project so that the functions of the RSIB.DLL can be called. In addition, the file NIGLOBAL.BAS is added to the project. This file contains constants and definitions for the processing of errors, timeout values, etc.

- **Declaration of DLL functions as procedures**

  Since the functions all return an integer value, the functions in the file GPIB.BAS are all declared as follows:

  ```
  Declare Function xxx Lib "gpib.dll" ( ... ) As Integer
  ```

  The function value with the status variables `ibsta` should be allocated a variable when it is called up. Since this value is also returned via a reference parameter of the functions, the functions can be declared as procedures as follows:

  ```
  Declare Sub xxx Lib "rsib.dll" ( ... )
  ```

- **Generating a response buffer**

  Since the DLL returns zero-terminated strings in case of responses, a string of sufficient length should be generated prior to calling the functions `ibrd()` and `ilrd()`, since Visual Basic prefixes a length value to the strings which is not updated by the DLL.
  The following two possibilities are available to generate a length value for a string:

  - `Dim Rd as String * 100`
  - ```
    Dim Rd as String
    Rd = Space$(100)
    ```

Initialization and Default Status

Variables used by all subroutines should be stored at the beginning of every program.
Then the IEC/IEEE bus as well as the settings of the instrument are brought into a defined default status at the beginning of every program. Subroutines `"InitController"` and `"InitDevice"` are used to this effect.

Creating global variables

Global variables are placed in so-called "modules" (file extension: .BAS) in Visual Basic. Therefore, at least one module (z.B. "GLOBALS.BAS) should be created which contains the variables used by all subroutines, such as the device addresses used by the IEC/IEEE-bus driver.
The file should contain the following instructions for the programming examples below:

```
Global analyzer As Integer
Global boardId As Integer
```

Initiate Controller

```
REM ------------ Initiate controller ------------------------------------
Public SUB InitController()

iecaddress% = 20                          'IEC/IEEE-bus address of the
                                          'instrument
CALL IBFIND("GPIB0", boardId%)            'Open port to the controller
CALL IBFIND("DEV1", analyzer%)            'Open port to the instrument
CALL IBPAD(analyzer%, iecaddress%)        'Inform controller on instrument
                                          'address
CALL IBTMO(analyzer%, 11)                 'Response time to 1 sec
END SUB
REM ************************************************************************
```
```

Initiate Instrument

The IEC-bus status registers and instrument settings of the instrument are brought into the default status.

```
REM ------------ Initiate instrument -------------------------------------
Public SUB InitDevice()

CALL IBWRT(analyzer%, "*CLS")           'Reset status registers
CALL IBWRT(analyzer%, "*RST")           'Reset instrument
END SUB
REM*****************************************************************************
```

Configuring Power Save Function of Display

The results on the screen are often not required during IEC/IEEE-bus operation. Although the command "SYSTem:DISPlay:UPDate OFF" switches off the display of results which brings considerable advantages in terms of speed in the remote control mode, the display itself and in particular the backlighting remain switched on.

If required, the display should be switched off by means of the power-save function, the response time having to be set in minutes prior to activation.

Note: *The display is switched on as soon as a key is pressed on the instrument front panel.*

```
REM --------- Configure power save function -------------------------------
Public SUB PowerSave()

CALL IBWRT(analyzer%, "SYSTem:PSAVe:HOLDoff 1") 'Set holdoff to 1 minute
CALL IBWRT(analyzer%, "SYSTem:PSAVe ON")        'Power save function on
END SUB
REM*****************************************************************************
```

Transmission of Simple Instrument Setting Commands

Center frequency, span, and reference level of the instrument are set in this example.

```
REM -------- Instrument setting commands --------------------------------
PUBLIC SUB SimpleSettings()

CALL IBWRT(analyzer%, "FREQUENCY:CENTER 128MHz")  'Center frequency 128 MHz
CALL IBWRT(analyzer%, "FREQUENCY:SPAN 10MHZ")     'Span 10 MHz
CALL IBWRT(analyzer%, "DISPLAY:TRACE:Y:RLEVEL -10dBm")
                                                  'Reference level -10dBm
END SUB
REM ***************************************************************************
```

Return to manual control

```
REM -------- Switch instrument over to manual control --------------------
CALL IBLOC(analyzer%)                'Set instrument to Local state
REM ***************************************************************************
```

Reading out Instrument Settings

The settings made in the above example are read out here. The abbreviated commands are used.

```
REM --------- Reading out instrument settings ----------------------------
PUBLIC SUB ReadSettings()

CFfrequency$ = SPACE$(20)            'Provide text variables (20 characters)
CALL IBWRT(analyzer%, "FREQ:CENT?")  'Request center frequency
CALL IBRD(analyzer%, CFfrequency$)   'Read value

CFspan$ = SPACE$(20)                 'Provide text variables (20 characters)
CALL IBWRT(analyzer%, "FREQ:SPAN?")  'Query span
CALL IBRD(analyzer%, CFspan$)        'Read value

RLevel$ = SPACE$(20)                 'Provide text variables (20 characters)
CALL IBWRT(analyzer%, "DISP:TRAC:Y:RLEV?")
                                     'Query reference level
CALL IBRD(analyzer%, RLevel$)        'Read value
```

```
REM ---------------- Display values on the screen ------------------------
PRINT "Center frequency: "; CFfrequency$,
PRINT "Span:             "; CFspan$,
PRINT "Reference level:  "; RLevel$,
REM*************************************************************************
```

Positioning a Marker and Displaying Values

```
REM -------------- Examples of marker functions ---------------------------
PUBLIC SUB ReadMarker()

CALL IBWRT(analyzer%, "CALC:MARKER ON;MARKER:MAX")
            'Activate marker1 and start peak search
MKmark$ = SPACE$(30)              'Provide text variables (30 characters)
CALL IBWRT(analyzer%, "CALC:MARK:X?;Y?")    'Query frequency and level
CALL IBRD(analyzer%, MKmark$)               'Read value

REM --------------- Display values on the screen -------------------------
PRINT "Center frequency / level "; MKmark$,
REM ************************************************************************
```

Command synchronization

The possibilities for synchronization implemented in the following example are described in Chapter 5, Section "Command Order and Command Synchronization".

```
REM -------- Examples of command synchronization -------------------------
PUBLIC SUB SweepSync()


REM The command INITiate[:IMMediate] starts a single sweep if the command
REM INIT:CONT OFF was previously sent. It should be ensured that the next
REM command is only then executed when the entire sweep is complete.
CALL IBWRT(analyzer%, "INIT:CONT OFF")

REM -------- First possibility: Use of *WAI ------------------------------
CALL IBWRT(analyzer%, "ABOR;INIT:IMM; *WAI")


REM -------- Second possibility: Use of *OPC? ----------------------------
OpcOk$ = SPACE$(2)                  'Space for *OPC? - Provide response
CALL IBWRT(analyzer%, "ABOR;INIT:IMM; *OPC?")
REM -------- here the controller can service other instrument-------------
CALL IBRD(analyzer%, OpcOk$)                  'Wait for "1" from *OPC?


REM -------- Third possibility: Use of *OPC ------------------------------
REM In order to be able touse the service request function in conjugation
REM with a National Instruments GPIB driver, the setting "Disable
REM Auto Serial Poll" must be changed to "yes" by means of IBCONF!
CALL IBWRT(analyzer%, "*SRE 32")      'Permit service request for ESR
CALL IBWRT(analyzer%, "*ESE 1")       'Set event-enable bit for
                                      'operation-complete bit
CALL IBWRT(analyzer%, "ABOR;INIT:IMM; *OPC") 'Start sweep and
                                             'synchronize with OPC
CALL WaitSRQ(boardID%,result%)        'Wait for service request
REM Continue main program here.
END SUB
REM ************************************************************************
```

Service Request

The service request routine requires an extended initialization of the instrument in which the respective bits of the transition and enable registers are set.
In order to use the service request function in conjugation with National Instruments GPIB driver, the setting "Disable Auto Serial Poll" must be changed to "yes" by means of IBCONF.

Initiate Service Request

```
REM ---- Example of initialization of the SRQ in the case of errors --------
PUBLIC SUB SetupSRQ()

CALL IBWRT(analyzer%, "*CLS")                    'Reset status reporting system
CALL IBWRT(analyzer%,"*SRE 168")                 'Permit service request for
                                                 'STAT:OPER,STAT:QUES and ESR
                                                 'register
CALL IBWRT(analyzer%,"*ESE 60")                  'Set event-enable bit for
                                                 'command, execution, device-
                                                 'dependent and query error
CALL IBWRT(analyzer%,"STAT:OPER:ENAB 32767")     'Set OPERation enable bit for
                                                 'all events
CALL IBWRT(analyzer%,"STAT:OPER:PTR 32767")      'Set appropriate OPERation
                                                 'Ptransition bits
CALL IBWRT(analyzer%,"STAT:QUES:ENAB 32767")     'Set questionable enable bits
                                                 'for all events
CALL IBWRT(analyzer%,"STAT:QUES:PTR 32767")      'Set appropriate questionable
                                                 'Ptransition bits
CALL WaitSRQ(boardID%,result%)                   'Wait for Service Request
IF (result% = 1) THEN CALL Srq                   'If SRQ is recognized =>
                                                 'subroutine for evaluation
END SUB
REM ************************************************************************
```

Service request routine

A service request is then processed in the service request routine.
Note: the variables userN% and userM% must be pre-assigned usefully!

```
REM ------------ Service request routine ---------------------------------
Public SUB Srq()

ON ERROR GOTO noDevice                          'No user existing
CALL IBRSP(analyzer%, STB%)                     'Serial poll, read status byte
IF STB% > 0 THEN                                'This instrument has bits set
                                                'in the STB
     SRQFOUND% = 1
     IF (STB% AND 16)  > 0 THEN CALL Outputqueue
     IF (STB% AND 4)   > 0 THEN CALL ErrorQueueHandler
     IF (STB% AND 8)   > 0 THEN CALL Questionablestatus
     IF (STB% AND 128) > 0 THEN CALL Operationstatus
     IF (STB% AND 32)  > 0 THEN CALL Esrread
  END IF
noDevice:
END SUB                                          'End of SRQ routine
REM ************************************************************************
```

Reading out the status event registers, the output buffer and the error/event queue is effected in subroutines.

Read Out of Output Buffer

```
REM -------- Subroutine for the individual STB bits ----------------------
Public SUB Outputqueue()                        'Reading the output buffer

result$ = SPACE$(100)                           'Make space for response
CALL IBRD(analyzer%, result$)
PRINT "Contents of Output Queue : "; result$
END SUB
REM ************************************************************************
```

Read Out of Error Messages

```
REM -------- Subroutine for reading the error queue ----------------------
Public SUB ErrorQueueHandler()
ERROR$ = SPACE$(100)                    'Make space for error variable
CALL IBWRT(analyzer%, "SYSTEM:ERROR?")
CALL IBRD(analyzer%, ERROR$)
PRINT "Error Description : "; ERROR$
END SUB
REM ************************************************************************
```

Evaluation of SCPI Status Registers

```
REM ------ Subroutine for evaluating Questionable Status-Register ---------
Public SUB Questionablestatus()
Ques$ = SPACE$(20)                  'Preallocate blanks to text variable
CALL IBWRT(analyzer%, "STATus:QUEStionable:EVENt?")
CALL IBRD(analyzer%, Ques$)
PRINT "Questionable Status: "; Ques$
END SUB
REM ************************************************************************

REM ------ subroutine for evaluating Operation Status-Register ------------
Public SUB Operationstatus()
Oper$ = SPACE$(20)                  'Preallocate blanks to text variable
CALL IBWRT(analyzer%, "STATus:OPERation:EVENt?")
CALL IBRD(analyzer%, Oper$)
PRINT "Operation Status: "; Oper$
END SUB
REM ************************************************************************
```

Evaluation of Event Status Register

```
REM ------ Subroutine for evaluating the Event Status Register ------------
Public SUB Esrread()
Esr$ = SPACE$(20)              'Preallocate blanks to text variable
CALL IBWRT(analyzer%, "*ESR?")                              'Read ESR
CALL IBRD(analyzer%, Esr$)
IF (VAL(Esr$) AND 1) > 0 THEN PRINT "Operation complete"
IF (VAL(Esr$) AND 2) > 0 THEN PRINT "Request Control"
IF (VAL(Esr$) AND 4) > 0 THEN PRINT "Query Error"
IF (VAL(Esr$) AND 8) > 0 THEN PRINT "Device dependent error"
IF (VAL(Esr$) AND 16) > 0 THEN
    PRINT "Execution Error; Program aborted"'  Output error message
    STOP                                       'Stop software
    END IF
IF (VAL(Esr$) AND 32) > 0 THEN
    PRINT "Command Error; Program aborted"'    Output error message
    STOP                                       'Stop software
    END IF
IF (VAL(Esr$) AND 64) > 0 THEN PRINT "User request"
IF (VAL(Esr$) AND 128) > 0 THEN PRINT "Power on"
END SUB
REM ************************************************************************
```

More Complex Programming Examples

Basic settings of the Analyzer

The following settings are an example of how to modify the default setting of FSP.
It should be noted that only some settings are necessary depending on the example of application. In particular, the settings for resolution bandwidth, video bandwidth and sweep time are often not needed since these parameters are automatically calculated in the default setting on modifying the frequency range (span). The insertion loss is also automatically calculated depending on the reference level. The level detectors are coupled to the selected trace mode in the default setting.
The settings which are automatically calculated in the default setting are marked by (*) in the following programming example.

Setting the IEC/IEEE Bus Status Register

```
REM ************************************************************************
Public Sub SetupStatusReg()

'--------- IEEE 488.2 status register -------------------------------------
CALL IBWRT(analyzer%,"*CLS")                'Reset Status Registers
CALL IBWRT(analyzer%,"*SRE 168")            'Enable service request
                                            'for STAT:OPER-,STAT:QUES- and
                                            'ESR registers
CALL IBWRT(analyzer%,"*ESE 61")             'Set Event-Enable bit for:
                                            'Operation Complete
                                            'Command-, Execution-,Device
                                            'Dependent- and Query Error
'--------- SCPI status register -------------------------------------------
CALL IBWRT(analyzer%,"STAT:OPER:ENAB 0")    'Disable OPERation Status Reg
CALL IBWRT(analyzer%,"STAT:QUES:ENAB 0")    'Disable Questionable Status
                                            'Register
End Sub
REM ************************************************************************
```

Default Setting for Measurements

```
REM ************************************************************************
Public Sub SetupInstrument()

'-------------------- Basic settings ------------------------------------
CALL SetupStatusReg                          'Set status registers
CALL IBWRT(analyzer%,"*RST")                 'Reset instrument
CALL IBWRT(analyzer%,"SYST:DISP:UPD ON")     'ON: display indication on
                                             'OFF: off(improved
                                             '         performance)
CALL IBWRT(analyzer%,"DISP:FORM SINGle")     'Full screen
CALL IBWRT(analyzer%,"DISP:WIND1:SEL")       'Active screen A
CALL IBWRT(analyzer%,"INIT:CONT OFF")        'Single sweep
'--------- Set frequency -----------------------------------------------
CALL IBWRT(analyzer%,"FREQUENCY:CENTER 100MHz")       'Center frequency
CALL IBWRT(analyzer%,"FREQ:SPAN 1 MHz")               'Span
'--------- Set level ---------------------------------------------------
CALL IBWRT(analyzer%,"DISP:WIND:TRAC:Y:RLEV -20dBm")  'Reference level
CALL IBWRT(analyzer%,"INP:ATT 10dB")                  'Input attenuation (*)
'--------- Scale y-axis ------------------------------------------------
CALL IBWRT(analyzer%,"DISP:WIND:TRAC:Y:SPAC LOG")     'Log level axis
CALL IBWRT(analyzer%,"DISP:WIND:TRAC:Y:SCAL 100dB")   'Level range
CALL IBWRT(analyzer%,"DISP:WIND:TRAC:Y:SCAL:MODE ABS") 'Absolute scaling
CALL IBWRT(analyzer%,"CALC:UNIT:POW DBM")             'Unit of y-axis
'--------- Trace and detector settings ---------------------------------
CALL IBWRT(analyzer%,"DISP:WIND:TRAC1:MODE AVER")     'Trace1 average
CALL IBWRT(analyzer%,"AVER:TYPE VID")                 'Average mode video;
                                                      '"LIN" for linear
CALL IBWRT(analyzer%,"SWE:COUN 10")                   'Sweep count
CALL IBWRT(analyzer%,"DISP:WIND:TRAC2:STAT OFF")      'Trace2 blank
CALL IBWRT(analyzer%,"DISP:WIND:TRAC3:STAT OFF")      'Trace3 blank
CALL IBWRT(analyzer%,"CALC:MATH:STAT OFF")            'Trace mathematics off
CALL IBWRT(analyzer%,"DETECTOR1 RMS")                 'Detector Trace1   (*)
CALL IBWRT(analyzer%,"DET2:AUTO ON")                  'Detector Trace2   (*)
CALL IBWRT(analyzer%,"DET3:AUTO ON")                  'Detector Trace3   (*)
'--------- Band width and sweep time -----------------------------------
CALL IBWRT(analyzer%,"BAND:RES 100KHz")               'Resolution BW (*)
CALL IBWRT(analyzer%,"BAND:VID 1MHz")                 'Video bandwidth   (*)
CALL IBWRT(analyzer%,"SWE:TIM 100ms")                 'Sweep time        (*)
END SUB

REM ************************************************************************
```

Using Marker and Delta Marker

Marker Search Functions, Limitation of Search Range

The example below is based on an AM-modulated signal at 100 MHz with the following characteristics:

- Carrier signal level: –30 dBm
- AF frequency: 100 kHz
- Modulation depth: 50 %

Marker 1 and delta marker 2 are set one after the other to the highest maxima of the measurement curve and then the frequency and level are read out. The default setting of the analyzer can be used for the following measurements (SetupInstrument).

```
REM ************************************************************************
Public Sub MarkerSearch()

result$ = Space$(100)
CALL SetupInstrument                          'Basic setting
'--------- Peak search without search limit ------------------------------
CALL IBWRT(analyzer%,"INIT:CONT OFF")         'Switch to single sweep
CALL IBWRT(analyzer%,"CALC:MARK:PEXC 6DB")    'Peak Excursion
CALL IBWRT(analyzer%,"CALC:MARK:STAT ON")     'Switch on Marker 1
CALL IBWRT(analyzer%,"CALC:MARK:TRAC 1")      'Assign marker1 to Trace 1
CALL IBWRT(analyzer%,"INIT;*WAI")             'Sweep with sync
CALL IBWRT(analyzer%,"CALC:MARK:MAX;X?;Y?")   'Marker to peak; read out
CALL IBRD(analyzer%, result$)                 'frequency and level
Print "Marker 1: ";result$
CALL IBWRT(analyzer%,"CALC:DELT2:STAT ON;MAX;MAX:LEFT")
                                              'Switch on delta marker 2
                                              'Peak and then Next Peak Left
CALL IBWRT(analyzer%,"CALC:DELT:MODE ABS")    'Delta marker 2 frequeny output
                                              'absolute
CALL IBWRT(analyzer%,"CALC:DELT2:X?;Y?")      'Delta marker 2 - Read out
                                              'frequency and level
CALL IBRD(analyzer%, result$)
Print "Delta 2: ";result$
```

```
'--------- Peak search with search limit in x-direction --------------------
CALL IBWRT(analyzer%,"CALC:DELT:MODE REL")    'Delta marker frequency output
                                              'relative

CALL IBWRT(analyzer%,"CALC:MARK:X:SLIM:STAT ON;LEFT 0Hz;RIGHt 100.05MHz")
                                              'Search limit on and set below
                                              'LF on the right side

CALL IBWRT(analyzer%,"CALC:DELT3:STAT ON;MAX;MAX:RIGHt")
                                              'Delta marker 3      on
                                              'Peak and then Next Peak Right
CALL IBWRT(analyzer%,"CALC:DELT3:X?;Y?")      'Delta marker 3; Read out
                                              'frequency und level, both must

CALL IBRD(analyzer%, result$)                 'have the value 0
Print "Delta 3: ";result$

'--------- Peak search with search limit in y-direction --------------------
CALL IBWRT(analyzer%,"CALC:DELT:MODE REL")    'Deltamarker frequency output
                                              'relative

CALL IBWRT(analyzer%,"CALC:THR -35DBM;THR:STAT ON")
                                              'Threshold on and set above LF

CALL IBWRT(analyzer%,"CALC:DELT3:STAT ON;MAX;MAX:NEXT")
                                              'Delta marker 3 on
                                              'Peak and then Next Peak
                                              ' => is not found

CALL IBWRT(analyzer%,"CALC:DELT3:X:REL?;:CALC:DELT:Y?")
CALL IBRD(analyzer%, result$)                 'Delta marker 3; Read out
                                              'Frequency und level, both must
CALL IBRD(analyzer%, result$)                 'have the value 0
Print "Delta 3: ";result$

'---- Set center frequency and reference level by means of markers ---------
CALL IBWRT(analyzer%,"CALC:MARK2:FUNC:CENT") 'Delta marker 2 -> Marker and
                                              'center frequency = Marker 2

CALL IBWRT(analyzer%,"CALC:MARK2:FUNC:REF")   'Ref level = Marker 2

Call ibwrt(analyzer%,"INIT;*WAI")             'Sweep with sync

END SUB

REM ************************************************************************
```

Frequency Counting

The following example is based on a signal with a level of –30 dBm at 100 MHz. The default setting of the analyzer can also be used for this measurement (SetupInstrument). The objective of frequency counting is to determine the exact frequency of the signal at 100 MHz.

```
REM ************************************************************************
Public Sub MarkerCount()

result$ = Space$(100)
CALL SetupInstrument                                'Basic settings
'--------- Measure signal frequency with frequency counter ----------------
CALL IBWRT(analyzer%,"INIT:CONT OFF")               'Single sweep on
CALL IBWRT(analyzer%,"CALC:MARK:PEXC 6DB")          'Peak Excursion
CALL IBWRT(analyzer%,"CALC:MARK:STAT ON")           'Marker 1 on
CALL IBWRT(analyzer%,"CALC:MARK:TRAC 1")            'Assign marker1 to trace 1
CALL IBWRT(analyzer%,"CALC:MARK:X 100MHz")          'Set Marker1 to 100MHz
CALL IBWRT(analyzer%,"CALC:MARK:COUNT:RES 1HZ")'Frequency counter 1Hz
CALL IBWRT(analyzer%,"CALC:MARK:COUNT ON")          'frequency counter on
CALL IBWRT(analyzer%,"INIT;*WAI")                   'Sweep with sync
CALL IBWRT(analyzer%,"CALC:MARK:COUNT:FREQ?")       'Read out frequency
Print "Marker Count Freq: ";result$
END SUB
REM ************************************************************************
```

Operation mit Fixed Reference Point (Reference Fixed)

The following example is based on a signal with a level of –20 dBm at 100 MHz. The harmonics of the signal lie at 200 MHz, 300 MHz, etc. In the presence of high-quality signal sources these harmonics may lie out of the dynamic range of FSP. In order to measure harmonic suppression, however, the level should be set to higher sensitivity for measuring the harmonics; the carrier has to be suppressed by a notch filter to avoid overloading the analyzer RF input.

In the following example two measurements are therefore performed with different level settings, first with a high reference level at the carrier frequency and then with a low reference level at the frequency of the 3rd harmonic.

The default setting of the analyzer for measurements (SetupInstrument) is used as starting point and adaptations are then made for the measurement.

```
REM ************************************************************************
Public Sub RefFixed()

result$ = Space$(100)
CALL SetupInstrument                              'Basic settings
'--------------- Measure the reference point ------------------------------
CALL IBWRT(analyzer%,"INIT:CONT OFF")             'Single sweep
CALL IBWRT(analyzer%,"CALC:MARK:PEXC 6DB")        'Peak Excursion
CALL IBWRT(analyzer%,"CALC:MARK:STAT ON")         'Marker1 on
CALL IBWRT(analyzer%,"CALC:MARK:TRAC 1")          'Assign marker1 to Trace 1
CALL IBWRT(analyzer%,"INIT;*WAI")                 'Sweep with sync
CALL IBWRT(analyzer%,"CALC:MARK:MAX")             'Set Marker1 to 100MHz
CALL IBWRT(analyzer%,"CALC:DELT:FUNC:FIX ON")     'Reference fixed
'-----Setting freq., level and bandw. for meas. of harmonic distortion ----
CALL IBWRT(analyzer%,"FREQ:CENT 400MHz;Span 1MHz" )'Set freq. of 3rd harmonic
CALL IBWRT(analyzer%,"BAND:RES 1kHz")               'and appropriate RBW
CALL IBWRT(analyzer%,"SWEEP:TIME:AUTO ON")          'Couple sweep time
CALL IBWRT(analyzer%,"INP:ATT:AUTO ON")             'Optimize level
CALL IBWRT(analyzer%,"DISP:WIND:TRAC:Y:RLEV -50dBm")
CALL IBWRT(analyzer%,"INIT;*WAI")                 'Sweep with sync
CALL IBWRT(analyzer%,"CALC:DELT:MODE REL")        'Delta marker frequency
                                                  'relative
CALL IBWRT(analyzer%,"CALC:DELT:MAX;X?;Y?")       'Read out delta marker
Call ibrd(analyzer%, result$)                     'Read out frequency and level
Print "Deltamarker 1: "; result$
END SUB
REM ************************************************************************
```

Phase and Phase Noise Measurement

During phase noise measurement the noise power referred to 1 Hz is brought into proportion to the power of an adjacent carrier signal. The spacing often used between the measured frequency and the carrier frequency is 10 kHz.

For the noise measurement the measured absolute level is referred to a bandwith of 1 Hz.

The following example is again based on a signal with a level of –30 dBM at 100 MHz. Two markers are used to determine the noise and the phase noise at an offset of 10 kHz from the carrier signal.

```
REM ************************************************************************
Public Sub Noise()

result$ = Space$(100)
'--------- Basic settings ------------------------------------------------
CALL SetupStatusReg                          'Configure status register
CALL IBWRT(analyzer%,"*RST")                 'Reset instrument
CALL IBWRT(analyzer%,"INIT:CONT OFF")        'Single sweep
'--------- Set frequency -------------------------------------------------
CALL IBWRT(analyzer%,"FREQUENCY:CENTER 100MHz")       'Center frequency
CALL IBWRT(analyzer%,"FREQ:SPAN 100 kHz")             'Span
'--------- Set level -----------------------------------------------------
CALL IBWRT(analyzer%,"DISP:WIND:TRAC:Y:RLEV -20dBm")  'Reference level
CALL IBWRT(analyzer%,"INIT;*WAI")                'Sweep with sync
'--------- Set reference point -------------------------------------------
CALL IBWRT(analyzer%,"CALC:MARK:PEXC 6DB")       'Peak Excursion
CALL IBWRT(analyzer%,"CALC:MARK:STAT ON")        'Marker1 on
CALL IBWRT(analyzer%,"CALC:MARK:TRAC 1")         'Assign marker1 to trace1
CALL IBWRT(analyzer%,"CALC:MARK:MAX")            'Set marker1 to 100MHz
CALL IBWRT(analyzer%,"CALC:DELT:FUNC:PNO ON")    'Phase Noise on
'--------- Measure phase noise -------------------------------------------
CALL IBWRT(analyzer%,"CALC:DELT:X 10kHz")        'Set delta marker
CALL IBWRT(analyzer%,"CALC:DELT:FUNC:PNO:RES?")'Read out result of
Call ibrd(analyzer%, result$)                    'Phase Noise meas.
Print "Phase Noise [dBc/Hz]: "; result$
'--------- Measure noise -------------------------------------------------
CALL IBWRT(analyzer%,"CALC:MARK:X 99.96MHz")     'Set Marker 1
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:NOIS:RES?")'Read out result
Call ibrd(analyzer%, result$)
Print "Noise [dBm/Hz]: "; result$
END SUB
REM ************************************************************************
```

Shape Factor Measurement (using n-dB down)

The n-dB-down function of the analyzer is used twice to determine the shape factor of a filter (ratio of bandwidths at 60 dB and 3 dB below the filter maximum).

The following example is again based on a signal with a level of –30 dBm at 100 MHz. The shape factor is determined for the 30 kHz resolution bandwidth. The default setting of the analyzer is used for measurements (SetupInstrument).

```
REM ************************************************************************
Public Sub ShapeFactor()

result$ = Space$(100)
'--------- Basic settings analyzer ----------------------------------------
CALL SetupInstrument                              'Basic settings
CALL IBWRT(analyzer%,"INIT:CONT OFF")             'Single sweep
'--------- Set frequency --------------------------------------------------
CALL IBWRT(analyzer%,"FREQ:SPAN 1MHz")            'Span
CALL IBWRT(analyzer%,"BAND:RES 30kHz")            'Resolution bandwidth
CALL IBWRT(analyzer%,"INIT;*WAI")                 'Sweep with sync
'--------- Measure 60 dB value --------------------------------------------
CALL IBWRT(analyzer%,"CALC:MARK:PEXC 6DB")        'Peak Excursion
CALL IBWRT(analyzer%,"CALC:MARK:STAT ON")         'Marker1 on
CALL IBWRT(analyzer%,"CALC:MARK:TRAC 1")          'Assign marker1 to Trace 1
CALL IBWRT(analyzer%,"CALC:MARK:MAX")             'Set marker1 to 100MHz
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:NDBD 60dB")'Bandbreite bei 60dB messen
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:NDBD:RES?")'und auslesen
CALL IBRD(analyzer%,result$)
result60 = Val(result$)
'--------- Measure 3 dB Down value  ---------------------------------------
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:NDBD 3dB")'Read out bandwidth at 60dB
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:NDBD:RES?")
CALL IBRD(analyzer%,result$)
result3 = Val(result$)
'--------- Read out shape factor-------------------------------------------
Print "Shapefaktor 60dB/3dB: ";result60/result3
END SUB
REM ************************************************************************
```

Measuring the Third Order Intercept Point

The intercept point of 3rd order is the (virtual) level of two adjacent useful signals at which the intermodulation products of 3rd order have the same level as the useful signals.

The intermodulation product at f_{S2} is obtained by mixing the first harmonic of useful signal P_{N2} with signal P_{N1}, the intermodulation product at f_{S1} by mixing the first harmonic of useful signal P_{N1} with signal P_{N2}.

$f_{s1} = 2 \times f_{n1} - f_{n2}$ (1)

$f_{s2} = 2 \times f_{n2} - f_{n1}$ (2)

The following example is based on two adjacent signals with a level of –30 dBm at 100 MHz and 110 MHz. The intermodulation products lie at 90 MHz and 120 MHz according to the above formula. The frequency set is in a way that the examined mixture products are displayed on the diagram. Otherwise the default setting of the analyzer is used for measurements (SetupInstrument).

```
REM ************************************************************************
Public Sub TOI()

result$ = Space$(100)
'--------- Basic settings ------------------------------------------------
CALL SetupStatusReg                          'Set status registers
CALL IBWRT(analyzer%,"*RST")                 'Reset instrument
CALL IBWRT(analyzer%,"INIT:CONT OFF")        'Single sweep
CALL IBWRT(analyzer%,"SYST:DISP:UPD ON")     'ON: display indication on
                                             'OFF: off
'--------- Set frequency -------------------------------------------------
CALL IBWRT(analyzer%,"FREQ:STARt 85MHz;STOP 125 MHz") 'Span
'--------- Set level -----------------------------------------------------
CALL IBWRT(analyzer%,"DISP:WIND:TRAC:Y:RLEV -20dBm")  'Reference level
CALL IBWRT(analyzer%,"INIT;*WAI")              'Sweep with sync
'--------- TOI measurement -----------------------------------------------
CALL IBWRT(analyzer%,"CALC:MARK:PEXC 6DB")     'Peak Excursion
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:TOI ON")  'TOI on
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:TOI:RES?")'and read out results
CALL IBRD(analyzer%,result$)
'--------- Read out result -----------------------------------------------
Print "TOI [dBm]: ";result$
END SUB
REM ************************************************************************
```

Measuring the AM Modulation Depth

The example below is based on an AM-modulated signal at 100 MHz with the following characteristics:

- Carrier signal level: –30 dBm
- AF frequency: 100 kHz
- Modulation depth: 50 %

The default setting of the analyzer for measurements can be used for the measurements described below (SetupInstrument).

```
REM ************************************************************************
Public Sub AMMod()

result$ = Space$(100)
CALL SetupInstrument                          'Basic settings
'--------- Peak search ------------------------------------------------------
CALL IBWRT(analyzer%,"INIT:CONT OFF")         'Single sweep
CALL IBWRT(analyzer%,"INIT;*WAI")             'Sweep with sync
CALL IBWRT(analyzer%,"CALC:MARK:PEXC 6DB")    'Peak Excursion
CALL IBWRT(analyzer%,"CALC:MARK:STAT ON")     'Marker 1 on
CALL IBWRT(analyzer%,"CALC:MARK:TRAC 1")      'Assign marker1 to trace 1
'--------- Measure modulation depth-----------------------------------------
CALL IBWRT(analyzer%,"CALC:MARK:MAX;FUNC:MDEP ON") 'Marker to Peak;
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:MDEP:RES?")   'Mod. Depth on
CALL IBRD(analyzer%, result$)                      'Read out result
'--------- Read out result -------------------------------------------------
Print "AM Mod Depth [%]: ";result$
END SUB
REM ************************************************************************
```

Limit Lines and Limit Test

The example below shows the definition and use of a new limit line 5 for trace 1 on screen A and trace 2 on screen B with the following characteristics:

- Upper limit line
- Absolute x axis in the frequency range
- 5 reference values: 120 MHz / -70 DB, 126 MHz/-40 dB, 127 MHz/-40 dB, 128 MHz/-10 dB, 129 MHz/-40 dB, 130 MHz/-40 dB, 136 MHz / - 70 dB
- Relative y axis with unit dB
- Absolute threshold at -75 dBm
- No margin

The signal of the integrated calibration source (128 MHz, -30 dBm) is used to check the limit test.

```
REM ************************************************************************
Public Sub LimitLine()

result$ = Space$(100)
'--------- Basic settings -----------------------------------------------
CALL SetupInstrument                                    'Basic settings
CALL IBWRT(analyzer%,"FREQUENCY:CENTER 128MHz;Span 10MHz")'Span
Call ibwrt(analyzer%,"Diag:Serv:Inp Cal;CSO -30dBm")   'Cal signal on
'--------- Definition of limit lines ------------------------------------
CALL IBWRT(analyzer%,"CALC:LIM5:NAME 'TEST1'")          'Define name
CALL IBWRT(analyzer%,"CALC:LIM5:COMM 'Upper limit'")    'Define comment
CALL IBWRT(analyzer%,"CALC1:LIM5:TRAC 1")       'Assign trace in screen A
CALL IBWRT(analyzer%,"CALC2:LIM5:TRAC 2")       'Assign trace in screen B
CALL IBWRT(analyzer%,"CALC:LIM5:CONT:DOM FREQ")'Define x-axis range
CALL IBWRT(analyzer%,"CALC:LIM5:CONT:MODE ABS")'Define x-axis scaling
CALL IBWRT(analyzer%,"CALC:LIM5:UNIT DB")       'Define y-axis unit
CALL IBWRT(analyzer%,"CALC:LIM5:UPP:MODE REL")  'Define y-axis scaling
'--------- Definition of data points and threshold ----------------------
xlimit$ = "CALC:LIM5:CONT 120MHZ,126MHZ,127MHZ,128MHZ,129MHZ,130MHz,136MHz"
CALL IBWRT(analyzer%, xlimit$)                  'Set values for x-axis
CALL IBWRT(analyzer%,"CALC:LIM5:UPP -70,-40,-40,-20,-40,-40,-70")
                                                'Set values for y-axis


CALL IBWRT(analyzer%,"CALC:LIM5:UPP:THR -75DBM") 'Set y-threshold (only
                                                 'possible for relative
                                                 'y-axis)
'------------------------------------------------------------------------
'A margin or an x-/y offset can be defined here.
'----------- Activate and evaluate the limit line in screen A -------------
CALL IBWRT(analyzer%,"CALC1:LIM5:UPP:STAT ON")  'Activate line 5 in screen A
CALL IBWRT(analyzer%,"CALC1:LIM5:STAT ON")      'Activate limit check in
                                                'screen A
CALL IBWRT(analyzer%,"INIT;*WAI")               'Sweep with sync
```

```
CALL IBWRT(analyzer%,"CALC1:LIM5:FAIL?")        'Query result of limit
                                                'check
CALL IBRD(analyzer%, result$)                   'Result: 1 (= FAIL)
'--------- Read out result -----------------------------------------------
Print "Limit Result Line 5: ";result$

'------ Evaluate limit line in screen A by means of status registers -------
CALL IBWRT(analyzer%,"*CLS")                   'Reset status register
'--------- Measure -------------------------------------------------------
CALL IBWRT(analyzer%,"INIT;*OPC")               'Sweep with sync
CALL WaitSRQ(boardID%,status%)                  'Wait for service request
'--------- Read out result -----------------------------------------------
IF (status% = 1) THEN
   CALL IBWRT(analyzer%,"STAT:QUES:LIM1:COND?") 'Read out STAT:QUES:LIMit
   CALL IBRD(analyzer%, result$)                 'register
   IF ((Val(result$) And 16) <> 0) THEN
      Print "Limit5 failed"
   ELSE
      Print "Limit5 passed"
   END IF
END IF
END SUB
REM ***************************************************************************
```

Measuring the Channel and Adjacent Channel Power

In the following example the channel and adjacent channel power is first measured on a signal with a level of 0 dBm at 800 MHz to IS95. Then the channel and adjacent channel power is measured on a GSM signal at 935.2 MHz with fast ACP measurement (FAST ACP).

In addition, the limit test is activated.

```
REM ************************************************************************
Public Sub ACP()

result$ = Space$(100)
'--------- Basic settings ------------------------------------------------
CALL SetupStatusReg                          'Set status register
CALL IBWRT(analyzer%,"*RST")                 'Reset instrument
CALL IBWRT(analyzer%,"INIT:CONT OFF")        'Single sweep
CALL IBWRT(analyzer%,"SYST:DISP:UPD ON")     'ON: display indication on
                                             'OFF: off
'--------- Set frequency -------------------------------------------------
CALL IBWRT(analyzer%,"FREQ:CENT 800MHz")       'Set frequency
'--------- Set level -----------------------------------------------------
CALL IBWRT(analyzer%,"DISP:WIND:TRAC:Y:RLEV 10dBm")   'Reference level

'--------- Example 1: Configure CP/ACP for CDMA  -------------------------
CALL IBWRT(analyzer%,"CALC2:MARK:FUNC:POW:SEL ACP")   'ACP measurement on
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:POW:PRES F8CDMA")'Select CDMA800 FWD
CALL IBWRT(analyzer%,"SENS:POW:ACH:ACP 2")      'Select 2 adjacent channels
CALL IBWRT(analyzer%,"SENS:POW:ACH:PRES ACP")   'Optimize settings
CALL IBWRT(analyzer%,"SENS:POW:ACH:PRES:RLEV") 'Optimize reference level
CALL IBWRT(analyzer%,"SENS:POW:ACH:MODE ABS")   'Absolute measurement
CALL IBWRT(analyzer%,"SENS:POW:HSP ON")         'Fast ACP measurement
'--------- Measure and query result --------------------------------------
CALL IBWRT(analyzer%,"INIT;*WAI")               'Sweep with sync
CALL IBWRT(analyzer%,"CALC2:MARK:FUNC:POW:RES? ACP")   'Query result
CALL IBRD(analyzer%, result$)
'--------- Read out result -----------------------------------------------
Print "Result (CP, ACP low, ACP up, Alt low, Alt up): "
Print result$
```

```
'--------- Example 2: Configure CP/ACP manually für GSM ------------------

result$ = Space$(100)

CALL IBWRT(analyzer%,"FREQ:CENT 935.2MHz")      'Set frequency

CALL IBWRT(analyzer%,"CALC:MARK:FUNC:POW:SEL ACP")  'ACP measurement on

CALL IBWRT(analyzer%,"SENS:POW:ACH:ACP 1")          '1 adjacent channel

CALL IBWRT(analyzer%,"SENS:POW:ACH:BAND 200KHZ")    'Channel band width
CALL IBWRT(analyzer%,"SENS:POW:ACH:BAND:ACH 200KHZ")'Adjacent channel bandw.
CALL IBWRT(analyzer%,"SENS:POW:ACH:SPAC 200KHZ")    'Channel spacing

CALL IBWRT(analyzer%,"SENS:POW:ACH:PRES ACP")  'Optimize settings
CALL IBWRT(analyzer%,"SENS:POW:ACH:PRES:RLEV") 'Optimize reference level

CALL IBWRT(analyzer%,"SENS:POW:ACH:MODE ABS")  'Absolute measurement
'--------- Start measurement and query result -----------------------------

CALL IBWRT(analyzer%,"INIT;*WAI")              'Sweep with sync

CALL IBWRT(analyzer%,"CALC:MARK:FUNC:POW:RES? ACP")   'Query result
CALL IBRD(analyzer%, result$)

'--------- Read out result ------------------------------------------------

Print "Result (CP, ACP low, ACP up): "
Print result$

'--------- Active limit check ---------------------------------------------

result$ = Space$(100)

CALL IBWRT(analyzer%,"CALC:LIM:ACP:ACH 30DB, 30DB")   'Set relative limit

CALL IBWRT(analyzer%,"CALC:LIM:ACP:ACH:ABS -35DBM,-35DBM")
                                                    'Set absolute limit

CALL IBWRT(analyzer%,"CALC:LIM:ACP:ACH:STAT ON")      'Rel. limit check on
CALL IBWRT(analyzer%,"CALC:LIM:ACP:ACH:ABS:STAT ON")  'Abs. limit check on
CALL IBWRT(analyzer%,"CALC:LIM:ACP ON")               'Limit check on

'--------- Start measurement and query result -----------------------------

CALL IBWRT(analyzer%,"INIT;*WAI")                     'Sweep with sync

CALL IBWRT(analyzer%,"CALC:LIM:ACP:ACH:RES?")         'Query result of
CALL IBRD(analyzer%, result$)                         'limit check

'--------- Read out result ------------------------------------------------

Print "Result Limit Check: ";result$

END SUB

REM ************************************************************************
```

Occupied Bandwidth Measurement

In the following example, the bandwidth is to be found in which 95% of the power of a GSM signal is contained. Signal frequency is 935,2 MHz; channel bandwidth is 200 kHz.

```
REM ************************************************************************
Public Sub OBW()

result$ = Space$(100)
'--------- Basic settings ------------------------------------------------
CALL SetupStatusReg                          'Set status register
CALL IBWRT(analyzer%,"*RST")                 'Reset instrument
CALL IBWRT(analyzer%,"INIT:CONT OFF")        'Single sweep
CALL IBWRT(analyzer%,"SYST:DISP:UPD ON")     'ON: display indication on
                                             'OFF: off
'--------- Configure analyzer for OBW for GSM  ---------------------------
CALL IBWRT(analyzer%,"FREQ:CENT 935.2MHz")          'Set frequency
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:POW:SEL OBW")  'OBW measurement on
CALL IBWRT(analyzer%,"SENS:POW:ACH:BAND 200KHZ")    'Channel bandwidth
CALL IBWRT(analyzer%,"SENS:POW:BWID 95PCT")     'Percentage of power
CALL IBWRT(analyzer%,"SENS:POW:ACH:PRES OBW")   'Set frequency and
CALL IBWRT(analyzer%,"SENS:POW:ACH:PRES:RLEV") 'optimize level settings
CALL IBWRT(analyzer%,"SENS:POW:NCOR OFF")       'Noise correction
'--------- Measure and query result --------------------------------------
CALL IBWRT(analyzer%,"INIT;*WAI")               'Sweep with sync
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:POW:RES? OBW")   'Query result
CALL IBRD(analyzer%, result$)
Print result$
END SUB
REM ************************************************************************
```

Time Domain Power Measurement

In the following example the mean carrier power of a signal with 300 kHz bandwith at 100 MHz is to be determined. In addition, the peak power, the rms value and the standard deviation are measured. To do this, the time-domain-power measurement functions are used.

```
REM ************************************************************************
Public Sub TimeDomainPower()

result$ = Space$(100)
'--------- Basic settings ------------------------------------------------
CALL SetupStatusReg                          'Set status register
CALL IBWRT(analyzer%,"*RST")                 'Reset instrument
CALL IBWRT(analyzer%,"INIT:CONT OFF")        'Single sweep
CALL IBWRT(analyzer%,"SYST:DISP:UPD ON")     'ON: display indication on
                                             'OFF: off
'--------- Configure analyzer for time domain power measurement ------------
CALL IBWRT(analyzer%,"FREQ:CENT 100MHz;SPAN 0Hz")    'Set frequency
CALL IBWRT(analyzer%,"BAND:RES 300kHz")              'Resolution bandwidth
CALL IBWRT(analyzer%,"SWE:TIME 200US")               'Sweep time
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:SUMM:PPE ON")   'Pos. Peak measurement
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:SUMM:MEAN ON")  'Mean measurement
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:SUMM:RMS ON")   'RMS measurement
CALL IBWRT(analyzer%,"CALC:MARK:FUNC:SUMM:SDEV ON")  'Standard deviation
'------------------- Measure and query results ----------------------------
CALL IBWRT(analyzer%,"INIT;*WAI")                    'Sweep with sync
                                                     'Query results:
query$ =          " CALC:MARK:FUNC:SUMM:PPE:RES?;"   'Pos. Peak measurement
query$ = query$ + ":CALC:MARK:FUNC:SUMM:MEAN:RES?;"  'Mean measurement
query$ = query$ + ":CALC:MARK:FUNC:SUMM:RMS:RES?;"   'RMS measurement
query$ = query$ + ":CALC:MARK:FUNC:SUMM:SDEV:RES?"   'Standard deviation
Call IBWRT(analyzer%, query$)
CALL IBRD(analyzer%, result$)
Print result$
END SUB
REM ************************************************************************
```

Reading Trace Data

In the following example the trace data recorded together at the default setting are read out of the instrument and displayed on the screen in the form of a list. Reading is performed consecutively in the binary format and in the ASCII format, at span > 0 and also at span = 0.

In the binary format the message header is evaluated with the length indication and used to calculate the x axis values.

In the ASCII format only the list of level values is output.

The binary data are read out in 3 steps:

1. Reading the number of digits of the length indication
2. Reading the length indication
3. Reading trace data

This procedure is necessary with programming languages that support only structures with similar data types (arrays) (such as Visual Basic) since the data types of header and data differ in binary data.

```
REM ************************************************************************
Public Sub ReadTrace()

'--------- Define variables ------------------------------------------
Dim traceData(1002) As Single                 'Buffer for floating point
                                              'binary data
Dim digits As Byte                            'Number of digits of
                                              'length indication
Dim traceBytes As Integer                     'Length of trace data in bytes
Dim traceValues As Integer                    'Number of values in buffer

asciiResult$ = Space$(10000)                  'Buffer for ASCII trace data

result$ = Space$(100)                         'Buffer for simple results

startFreq$ = Space$(100)                      'Buffer for start frequency

span$ = Space$(100)                           'Buffer for span

'--------- Basic settings --------------------------------------------
CALL SetupInstrument                          'Basic settings

CALL IBWRT(analyzer%,"INIT:CONT OFF")         'Single sweep

CALL IBWRT(analyzer%,"INIT;*WAI")             'Sweep with sync

'--------- Define span for read out ----------------------------------
Call ibwrt(analyzer%,"FREQ:STARt?")           'Read out start frequency
Call ibrd(analyzer%,startFreq$)
startFreq = Val(startFreq$)

Call ibwrt(analyzer%,"FREQ:SPAN?")            'Read out span
Call ibrd(analyzer%,span$)
span = Val(span$)
```

```
'--------- Read out in binary format ------------------------------------
Call ibwrt(analyzer%, "FORMAT REAL,32")       'Select binary format
Call ibwrt(analyzer%, "TRAC1? TRACE1")        'Read out Trace 1
Call ilrd(analyzer%, result$, 2)              'Read out and store
digits = Val(Mid$(result$, 2, 1))             'number of digits of
                                              'length indication
result$ = Space$(100)                         'Initialize buffer again
Call ilrd(analyzer%, result$, digits)         'Read out
traceBytes = Val(Left$(result$, digits))      'and store indication of length
Call ibrd32(analyzer%, traceData(0), traceBytes) 'Read trace data into buffer
Call ilrd(analyzer%, result$, 1)              'Read the terminator <NL>
'--------- Read out binary data as pairs of frequency/level values ---------
traceValues = traceBytes/4                    'Single precision = 4 bytes
stepsize = span/traceValues                   'Calculate frequeny step width
For i = 0 To traceValues - 1
  Print "Value["; i; "] = "; startFreq+stepsize*i; ", "; traceData(i)
Next i
'--------- Basic settings time domain -----------------------------------
Call ibwrt(analyzer%,"FREQ:SPAN 0Hz")         'Zero span on
CALL IBWRT(analyzer%,"INIT;*WAI")             'Sweep with sync
'--------- Read out in ASCII format -------------------------------------
Call ibwrt(analyzer%,"FORMAT ASCII")          'Select ASCII format
CALL ibwrt(analyzer%,"TRAC1? TRACE1")         'Read out Trace 1
CALL ibrd(analyzer%, asciiResult$)
Print "Contents of Trace1: ",asciiResult$
END SUB
REM ************************************************************************
```

Storing and Loading Device Settings

Storing Instrument Settings

In the following example the settings/measurement data to be stored are determined; only the hardware settings are stored. The selection commands for the other settings are indicated with the status OFF for the sake of completeness.

```
REM ************************************************************************
Public Sub StoreSettings()


'This subroutine selects the settings to be stored and creates
'the data set "TEST1" in directory D:\USER\DATA. It uses
'the default setting and resets the instrument after storage
'of the setting.
'--------- Basic settings ------------------------------------------------
Call SetupInstrument
CALL IBWRT(analyzer%,"INIT:CONT OFF")        'Single sweep
CALL IBWRT(analyzer%,"INIT;*WAI")            'Sweep with sync
'--------- Select items to store -----------------------------------------
CALL IBWRT(analyzer%,"MMEM:SEL:HWS ON")      'Select hardware settings to
                                             'store
CALL IBWRT(analyzer%,"MMEM:SEL:TRAC OFF")    'Disable traces to store
CALL IBWRT(analyzer%,"MMEM:SEL:LIN:ALL OFF") 'Select active limit lines to
                                             'store
'--------- Define comment ------------------------------------------------
CALL IBWRT(analyzer%,"MMEM:COMM 'Test Setup'")
'--------- Store selected items ------------------------------------------
CALL IBWRT(analyzer%,"MMEM:STOR:STAT 1,'D:\USER\DATA\TEST1'")
'--------- Reset instrument ----------------------------------------------
CALL IBWRT(analyzer%,"*RST")
END SUB
REM ************************************************************************
```

Loading Device Settings

In the following example data set "TEST1" stored under D:\USER\DATA is reloaded into the isnstrument:

```
REM ************************************************************************
Public Sub LoadSettings()

'This subroutine loads data set "TEST1" in directory D:\USER\DATA.
'--------- Set status registers ----------------------------------------
Call SetupStatusReg                          'Set status register
'--------- Load data set -----------------------------------------------
CALL IBWRT(analyzer%,"MMEM:LOAD:STAT 1,'D:\USER\DATA\TEST1'")
'----Start measurement with the settings of the loaded data set ------------
CALL IBWRT(analyzer%,"DISP:TRAC1:MODE WRITE")   'Set trace to Clr/Write
CALL IBWRT(analyzer%,"INIT;*WAI")               'Start the sweep
END SUB
REM ************************************************************************
```

Setting the Data Set for Startup Recall

In the following example the analyzer is first reset. Then the data set TEST1 stored under D:\USER\DATA is selected for the function STARTUP RECALL, ie the data set is set for every *RST, PRESET and every device startup. For illustration, the command *RST is executed again.

```
REM ************************************************************************
Public Sub StartupRecallSettings()
'--------- Reset analyzer ----------------------------------------------
CALL IBWRT(analyzer%,"*RST")
'--------- Set status registers ----------------------------------------
Call SetupStatusReg                          'Set status register
'--------- Select startup recall data set------------------------------------
CALL IBWRT(analyzer%,"MMEM:LOAD:AUTO 1,'D:\USER\DATA\TEST1'")
'--------- Activate startup recall data set ----------------------------
CALL IBWRT(analyzer%,"*RST")
END SUB
REM ************************************************************************
```

Reading and Writing Files

Reading a File from the Instrument

In the following example file TEST1.SET stored under D:\USER\DATA is read from the instrument and stored in the controller.

```
REM ************************************************************************
Public Sub ReadFile()
'--------- Variables -----------------------------------------------------
Dim digits As Byte                          'Number of digits of
                                            'length indication
Dim fileBytes As Long                       'Length of file with trace data
                                            'in bytes
result$ = Space$(100)                       'Buffer for simple results
'--------- Basic settings status registers -------------------------------
Call SetupStatusReg                         'Set status register
'--------- Read out file -------------------------------------------------
Call ibwrt(analyzer%, "MMEM:DATA? 'D:\USER\DATA\TEST1.SET'")
                                            'Select file
Call ilrd(analyzer%, result$, 2)            'Read and store number of
                                            'digits in length
digits = Val(Mid$(result$, 2, 1))           'indication
Call ilrd(analyzer%, result$, digits)       'Read and store length
fileBytes = Val(Left$(result$, digits))     'indication
FileBuffer$ = Space$(fileBytes)             'Buffer for file
Call ilrd(analyzer%, FileBuffer, fileBytes) 'Read file into buffer
Call ilrd(analyzer%, result$, 1)            'Read terminator <NL>
'--------- Store file to controller --------------------------------------
Open "TEST1.SET" For Output As #1
Print #1, FileBuffer;                       ' ; to avoid linefeed at
                                            '   end of file
Close #1
END SUB
REM ************************************************************************
```

Creating a File in the Instrument

In the following example file TEST1.SET available on the controller is stored in the instrument under D:\USER\DATA\DUPLICAT.SET.

```
REM ************************************************************************

Public Sub WriteFile()

'--------- Variables -----------------------------------------------------

FileBuffer$ = Space$(100000)                    'Buffer for file
Dim digits As Long                              'Number of digits of
                                                'length indication
Dim fileBytes As Long                           'Length of file in bytes
fileSize$ = Space$(100)                         'Length of file in a string

result$ = Space$(100)                           'Buffer for simple results

'--------- Basic settings status registers -------------------------------

Call SetupStatusReg                             'Set status register

'--------- Prepare the definite length block data ------------------------

fileBytes = FileLen("H:\work\vb\test1.set")  'Determine length of file
fileSize$ = Str$(fileBytes)

digits = Len(fileSize$) - 1                     'Determine number of digits of
fileSize$ = Right$(fileSize$, digits)           'length indication

FileBuffer$ = "#" + Right$(Str$(digits), 1) + fileSize$
                                                'Put length indication into
                                                'file buffer

'--------- Read file from controller -------------------------------------

Open "H:\work\vb\TEST1.SET" For Binary As #1

FileBuffer$ = FileBuffer$ + Left$(Input(fileBytes, #1), fileBytes)

Close #1

'--------- Write file ----------------------------------------------------
-

Call ibwrt(analyzer%, "SYST:COMM:GPIB:RTER EOI")      'Set receive
                                                      'terminator in the
                                                      'instrument

Call ibwrt(analyzer%, "MMEM:DATA 'D:\USER\DATA\DUPLICAT.SET'," +
           FileBuffer$)                               'Select file

END SUB

REM ************************************************************************
```

Configuring and Starting a Printout

The following example shows the configuration of the output format and output device for printing out a measurement mask.
The procedure is in the following order:

1. Set the measurement required for the printout
2. Query available output devices
3. Select an output device
4. Select the output interface
5. Configure the output format
6. Start printout with synchronization to the end

It is assumed that the setting required is a signal with a power of –20 dBm at 100 MHz and also that the printer required is the 6th of the available printers. The printout is first performed to the selected printer, then to a file.

```
REM ************************************************************************
Public Sub HCopy()

DIM Devices(100) as string                          'Buffer for printer name
FOR i = 0 TO 49
   Devices$(i) = Space$(50)                         'Preallocate buffer for
                                                    'printer name
NEXT i
'--------- Basic settings -----------------------------------------------
CALL SetupStatusReg                                 'Set status register
CALL IBWRT(analyzer%,"*RST")                        'Reset instrument
CALL IBWRT(analyzer%,"INIT:CONT OFF")               'Single sweep
CALL IBWRT(analyzer%,"SYST:DISP:UPD ON")            'Display indication on
'--------- Configure measurement ----------------------------------------
CALL IBWRT(analyzer%,"FREQ:CENT 100MHz;SPAN 10MHz")     'Set frequency
CALL IBWRT(analyzer%,"DISP:WIND:TRAC:Y:RLEV -10dBm")    'Reference level
CALL IBWRT(analyzer%,"INIT;*WAI")                       'Start measurement
'--------- Query available output devices -------------------------------
CALL IBWRT(analyzer%,"SYST:COMM:PRIN:ENUM:FIRSt?")      'Read out first
CALL IBRD(analyzer%,Devices$(0))                        'printer and indicate
PRINT "Drucker 0: "+Devices$(0)                         'printer name
For i = 1 to 99
   CALL IBWRT(analyzer%,"SYST:COMM:PRIN:ENUM:NEXT?")    'Read out the next
   CALL IBRD(analyzer%,Devices$(i))                     'printer name
   IF Left$(Devices$(i),2) = "''" THEN GOTO SelectDevice 'Abort at end of
                                                         'list
   PRINT "Drucker"+Str$(i)+": " Devices$(i)             'Indicate printer name
NEXT i
```

```
SelectDevice:
'------------ Select device, printer language and interface ---------------
CALL IBWRT(analyzer%,"SYST:COMM:PRIN:SEL "+ Devices(6))'Select printer #6
8 CALL IBWRT(analyzer%,"HCOP:DEST 'SYST:COMM:PRIN'")  'Configuration:
                                                      '"Print out to
                                                      'printer interface"
CALL IBWRT(analyzer%,"HCOP:DEV:LANG GDI")            'Output language 'GDI'
'----- Select orientation (portrait/landscape) and color/BW ---------------
CALL IBWRT(analyzer%,"HCOP:PAGE:ORI PORTrait")       'Portrait
CALL IBWRT(analyzer%,"HCOP:DEV:COL OFF")             'Black and white
'----- Configure and start print out --------------------------------------
 CALL IBWRT (analyzer%,"HCOP:ITEM:ALL")        'Select complete screen
'CALL IBWRT (analyzer%,"HCOP:ITEM:WIND1:TRAC:STAT ON")  'alternative: only
'CALL IBWRT (analyzer%,"HCOP:ITEM:WIND2:TRAC:STAT ON")  'traces in
                                                       'screen A/B
CALL IBWRT (analyzer%,"*CLS")                  'Reset status registers
CALL IBWRT (analyzer%,"HCOP:IMMediate;*OPC")   'Start print out
CALL WaitSRQ(boardID%,result%)                 'Wait for service request
IF (result% = 1) THEN CALL Srq                 'If SRQ is recognized =>
                                               'Subroutines for evaluation
'---- Print out into file in WMF format (BMP format) ----------------------
CALL IBWRT(analyzer%,"HCOP:DEST 'MMEM'")       'Configuration:
                                               '"Print to file"
 CALL IBWRT(analyzer%,"HCOP:DEV:LANG WMF")     'File format WMF
'CALL IBWRT(analyzer%,"HCOP:DEV:LANG BMP")     'File format BMP
CALL IBWRT(analyzer%,"MMEM:NAME 'D:\USER\DATA\PRINT1.WMF'") 'Determine
                                                            'file name
CALL IBWRT (analyzer%,"*CLS")                  'Reset status registers
CALL IBWRT (analyzer%,"HCOP:IMMediate;*OPC")   'Start print out
CALL WaitSRQ(boardID%,result%)                 'Wait for service request
IF (result% = 1) THEN CALL Srq                 'If SRQ is recognized  =>
                                               'Subroutines for evaluation
END SUB
REM ************************************************************************
```

Contents - Chapter 8 "Maintenance and Instrument Interfaces"

8 Maintenance and Instrument Interfaces

Maintenance **8.1**
Mechanical and Electrical Maintenance 8.1
Storing and Packing 8.1
List of Power Cables Available 8.1

Instrument Interfaces **8.2**
AF Output 8.2
Probe Connector (PROBE POWER) 8.2
External Keyboard (KEYBOARD) 8.2
IEC Bus Interface 8.3
Interface Characteristics 8.3
Bus Lines 8.3
Interface Functions 8.4
IEC Bus Messages 8.4
Interface Messages 8.5
Instrument Messages 8.5
Printer Interface (LPT) 8.6
RS-232-C Interface (COM) 8.7
Interface Characteristics 8.7
Signal Lines 8.7
Transmission Parameters 8.8
Control Characters 8.9
Handshake 8.9
Monitor Connector (MONITOR) 8.10
Noise Source Control (NOISE SOURCE) 8.11
External Trigger Input (EXT TRIG/GATE) 8.11
Mouse Connector (MOUSE) 8.11
Reference Output/Input (REF IN and REF OUT) 8.11
IF Output 20.4 MHz (20.4 MHz OUT) 8.11

8 Maintenance and Instrument Interfaces

The following chapter contains information on the maintenance of the FSP and on the instrument interfaces.

Please follow the instructions in the service manual when exchanging modules or ordering spares. The order no. for spare parts can be found in the service manual.

The address of our support center and a list of all Rohde & Schwarz service centers can be found at the beginning of this manual.

The service manual includes further information particularly on troubleshooting, repair, exchange of modules (including battery exchange, adjustment of the OCXO oscillator) and calibration.

Maintenance

Mechanical and Electrical Maintenance

The CMU does not require any special maintenance. Remove any contamination on the instrument by means of a soft cloth. Make sure that the air vents are not obstructed.

Storing and Packing

The FSP can be stored at a temperature of –5°C to +60°C. When stored for an extended period of time the instrument should be protected against dust.

The original packing should be used, particularly the protective covers at the front and rear, when the instrument is to be transported or dispatched. If the original packing is no longer available, use a sturdy cardboard box of suitable size and carefully wrap the instrument to protect it against mechanical damage.

List of Power Cables Available

Table 8-1 List of power cables available

Stock No.	Earthed-contact connector	Preferably used in
DS 006.7013	BS1363: 1967' complying with IEC 83: 1975 standard B2	Great Britain
DS 006.7020	Type 12 complying with SEV-regulation 1011.1059, standard sheet S 24 507	Switzerland
DS 006.7036	Type 498/13 complying with US-regulation UL 498, or with IEC 83	USA/Canada
DS 006.7107	Type SAA3 10 A, 250 V, complying with AS C112-1964 Ap.	Australia
DS 0025.2365 DS 0099.1456	DIN 49 441, 10 A, 250 V, angular DIN 49 441, 10 A, 250 V, straight	Europe (except Switzerland)

Instrument Interfaces

AF Output

A miniature telephone jack can be used at the AF OUTPUT connector to connect an external loudspeaker, a headphone set or, e.g., a LF voltmeter. The internal resistance is 10 ohms and the output voltage can be controlled with the volume controller on the left side to the connector. When a jack is plugged in, the internal loudspeaker is automatically turned off.

The connector is only available with option FSP-B3, AF demodulator.

Probe Connector (PROBE POWER)

To allow the connection of probes, the FSP provides the PROBE POWER power connector. It delivers the power supply voltages +15 V and -12,6 V and ground.

The connector is also suited for powering the high-impedance probes from Hewlett Packard.

Pin	Signal
1	GND
2	-12,6 V; max 150 mA
3	+15 V; max 150 mA

Fig. 8-1 Pin assignments of PROBE POWER connector

External Keyboard (KEYBOARD)

A 6-pin PS/2 connector is provided on the front panel to allow connecting an external keyboard. The PSP-Z1 keyboard (Order No. 1091.4000.02, german) or the PSP-Z2 (Order No. 1091.4100.02, english) is recommended (Order No. 1009.5001.31). Also they include a trackball for mouse control. However, any other multi-function keyboard may also be used.



Pin	Signal
1	KEYBOARDDATA
2	MOUSEDATA
3	GND
4	5V, KEYBOARD
5	KEYBOARDCLK
6	MOUSECLK

Fig 8-2 Pin assignments of the KEYBOARD connector.

IEC Bus Interface

The standard instrument is equipped with an IEC/IEEE Bus connector. An IEEE 488 interface connector is located on the rear panel of the FSP. An external controller for remote control of the instrument can be connected via the IEEE 488 interface connector using a shielded cable.

Interface Characteristics

- 8-bit parallel data transfer
- bi-directional data transfer
- three-line handshake
- high data transfer rate of max. 350 kbyte/s
- up to 15 instruments can be connected
- maximal length of the interconnecting cables 15 m (single connection, 2m)
- wired-OR connection if several instruments are connected in parallel.

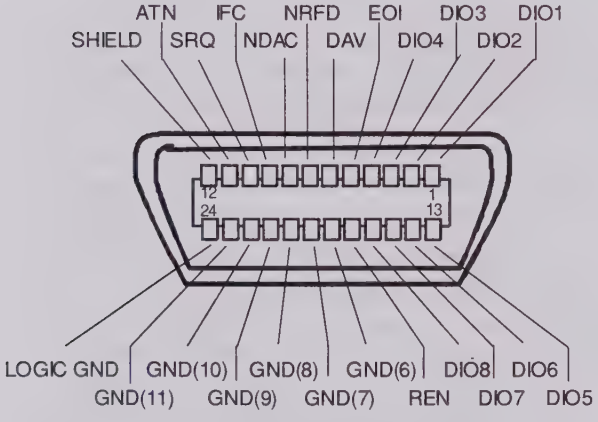

Fig. 8-3 Pin assignment of IEC-Bus interface

Bus Lines

1. **Data bus with 8 lines DIO 1 to DIO 8.**
   The transmission is bit-parallel and byte-serial in the ASCII/ISO code. DIO1 is the least significant, DIO8 the most significant bit.

2. **Control bus with 5 lines.**
   IFC (Interface Clear),
   active low resets the interfaces of the devices connected to the default setting.

   ATN (Attention),
   active low signals the transmission of interface messages
   inactive high signals the transmission of device messages.

   SRQ (Service Request),
   active low enables a device connected to send a service request to the controller.

REN (Remote Enable),
active low permits the switch over to remote control.

EOI (End or Identify),
has two functions in connection with ATN:
active low marks the end of data transmission when ATN=high
active low triggers a parallel poll when ATN=low.

3. **Handshake bus with three lines.**
   DAV (Data Valid),
   active low signals a valid data byte on the data bus.

   NRFD (Not Ready For Data),
   active low signals that one of the devices connected is not ready for data transfer .

   NDAC (Not Data Accepted),
   active low as long as the device connected is accepting the data present on the data bus.

Interface Functions

Instruments which can be remote controlled via the IEC bus can be equipped with different interface functions. Table 8-2 lists the interface functions appropriate for the instrument.

Table 8-2 Interface functions

Control character	Interface function
SH1	Handshake source function (source handshake), full capability
AH1	Handshake sink function (acceptor handshake), full capability
L4	Listener function, full capability, deaddressed by MTA.
T6	Talker function, full capability, ability to respond to serial poll, deaddressed by MLA
SR1	Service request function (Service Request), full capability
PP1	Parallel poll function, full capability
RL1	Remote/Local switch over function, full capability
DC1	Reset function (Device Clear), full capability
DT1	Trigger function (Device Trigger), full capability
C0	No controller function

IEC Bus Messages

The messages transferred via the data lines of the IEC bus can be divided into two groups:

- **interface messages** and
- **instrument messages.**

Interface Messages

Interface messages are transferred on the data lines of the IEC Bus when the "ATN" control line is active (LOW). They are used for communication between controller and instruments and can only be sent by the controller which currently has control of the IEC Bus.

Universal Commands

The universal commands are encoded 10 - 1F hex. They affect all instruments connected to the bus without addressing.

Table 8-3 Universal Commands

Command	QuickBASIC command	Effect on the instrument
DCL (Device Clear)	IBCMD (controller%, CHR$(20))	Aborts the processing of the commands just received and sets the command processing software to a defined initial state. Does not change the instrument settings.
IFC (Interface Clear)	IBSIC (controller%)	Resets the interfaces to the default setting.
LLO (Local Lockout)	IBCMD (controller%, CHR$(17))	The LOC/IEC ADDR key is disabled.
SPE (Serial Poll Enable)	IBCMD (controller%, CHR$(24))	Ready for serial poll.
SPD (Serial Poll Disable)	IBCMD (controller%, CHR$(25))	End of serial poll.
PPU (Parallel Poll Unconfigure)	IBCMD (controller%, CHR$(21))	End of the parallel-poll state.

Addressed Commands

The addressed commands are encoded 00 - 0F hex. They are only effective for instruments addressed as listeners.

Table 8-4 Addressed Commands

Command	QuickBASIC command	Effect on the instrument
SDC (Selected Device Clear)	IBCLR (device%)	Aborts the processing of the commands just received and sets the command processing software to a defined initial state. Does not change the instrument setting.
GTL (Go to Local)	IBLOC (device%)	Transition to the "Local" state (manual control).
PPC (Parallel Poll Configure)	IBPPC (device%, data%)	Configure instrument for parallel poll. Additionally, the QuickBASIC command executes PPE/PPD.

Instrument Messages

Instrument messages are transferred on the data lines of the IEC bus when the "ATN" control line is not active. ASCII code is used.
Structure and syntax of the instrument messages are described in Chapter 5. The commands are listed and explained in detail in Chapter 6.

Printer Interface (LPT)

The 25-pin LPT connector on the rear panel of the Fig. 8-4 is provided for the connection of a printer. The LPT interface is compatible with the CENTRONICS printer interface.

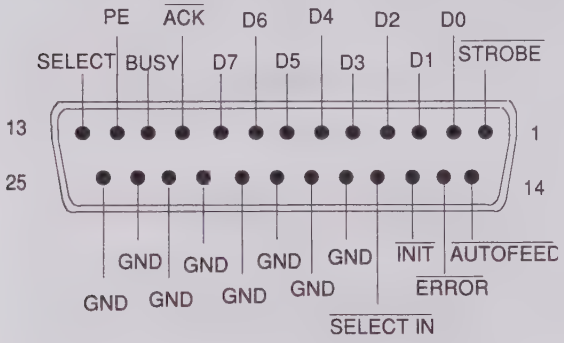

Pin	Signal	Input (I) Output (O)	Description
1	STROBE	O	Pulse for transmitting a data byte, min. 1µs pulse width (active LOW)
2	D0	O	Data Line 0
3	D1	O	Data Line 1
4	D2	O	Data Line 2
5	D3	O	Data Line 3
6	D4	O	Data Line 4
7	D5	O	Data Line 5
8	D6	O	Data Line 6
9	D7	O	Data Line 7
10	ACK	I	Indicates that the printer is ready to receive the next byte. (active LOW)
11	BUSY	I	Signal is active when the printer cannot accept data. (active HIGH)
12	PE	I	Signal is active when the paper tray is empty. (active HIGH)
13	SELECT	I	Signal is active when the printer is selected. (active HIGH)
14	AUTOFEED	O	When signal is active, the printer automatically performs a linefeed after each line. (active LOW)
15	ERROR	I	This signal is high when the printer has no paper, is not selected or has an error status. (active LOW)
16	INIT	O	Initialize the printer. (active LOW)
17	SELECT IN	O	If signal is active, the codes DC1/DC3 are ignored by the printer. (active LOW).
18 - 25	GND		Ground connection.

Fig. 8-4 Pin assignments for the LPT connector.

RS-232-C Interface (COM)

The standard FSP is equipped with a serial interfaces (RS-232-C; COM connector at the rear of the instrument). The interface can be set up and activated manually in the *SETUP-GENERAL SETUP* menu in the *COM PORT*table (Selection *OWNER = INSTRUMENT*).

Interface Characteristics

Serial data transmission in asynchronous mode
Bi-directional data transfer via two separate lines
Transmission rate selectable from 110 to 19200 baud
Logic '0' signal from+3 V to +15 V
Logic '1' signal from -15 V to -3 V
An external instrument (controller) can be connected.

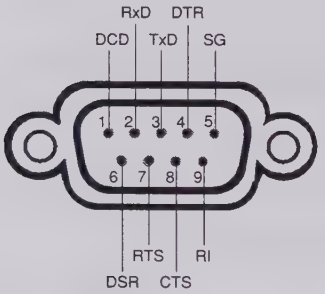

Fig. 8-5 Pin assignment of the RS-232-C interface

Signal Lines

DCD (Data Carrier Detect),
Not used in FSP.
Input; active LOW.
Using this signal, the local terminal recognizes that the modem of the remote station receives valid signals with sufficient level. DCD is used to disable the receiver in the local terminal and prevent reading of false data if the modem cannot interpret the signals of the remote station.

RxD (Receive Data)
Input, LOW = logic '1', HIGH = logic '0'.
Data line, local terminal receives data from remote station.

TxD (Transmit Data)
Output, LOW = logic '1', HIGH = logic '0'.
Data line, local terminal transmits data to remote station.

DTR (Data Terminal Ready),
Output, active LOW,
Indicates that the local terminal is ready to receive data.

GND
Interface ground, connected to instrument ground

DSR (Data Set Ready),
Input, active LOW,
Indicates that the remote station is ready to receive data.

RTS (Request To Send),
Output, active LOW.
Indicates that the local terminal wants to transmit data.

CTS (Clear To Send),
Input, active LOW.
Used to tell the local terminal that the remote station is ready to receive data.

RI (Ring Indicator),
Not used in FSP.
Input, active LOW.
Used by a modem to indicate that a remote station wants to establish a connection.

Transmission Parameters

To ensure error-free data transmission, the parameters of the instrument and the controller must have the same settings. The parameters are defined in the *SETUP-GENERAL SETUP* menu.

Transmission rate (baud rate) — the following transmission rates can be set in the analyzer: 110, 300, 600, 1200, 2400, 4800, 9600, 19200.

Data bits — Data transmission is in 7- or 8-bit ASCII code. The first bit transmitted is the LSB (least significant bit).

Start bit — Each data byte starts with a start bit. The falling edge of the start bit indicates the beginning of the data byte.

Parity bit — In order to detect errors, a parity bit may be transmitted. No parity, even parity or odd parity may be selected. In addition, the parity bit can be set to logic '0' or to logic '1'.

Stop bits — The transmission of a data byte is terminated by 1, 1,5 or 2 stop bits.

Example:
Transmission of character 'A' (41 hex) in 7-bit ASCII code, with even parity and 2 stop bits:



Control Characters

For interface control, several strings are defined and control characters are reserved which are based upon IEC Bus control.

Table 8-5 Control strings or control characters of the RS-232 interface

Control string or character	Function
'@REM'	Switch over to remote
'@LOC'	Switch over to local
'@SRQ'	Service Request SRQ (SRQ is sent by the instrument)
'@GET'	Group Execute Trigger (GET)
'@DCL'	Reset instrument (Device Clear DCL)
<Ctrl Q> 11 Hex	Enables character output / XON
<Ctrl S> 13 Hex	Inhibits character output / XOFF
0D Hex, 0A Hex	Terminator <CR>, <LF>

Handshake

Software handshake

In the software handshake mode of operation, the data transfer is controlled using the two control characters XON / XOFF.

The instrument uses the control character XON to indicate that it is ready to receive data. If the receive buffer is full, it sends the XOFF character via the interface to the controller. The controller then interrupts the data output until it receives another XON from the instrument. The controller indicates to the instrument that it is ready to receive data in the same way.

Cable required for software handshake

The connection of the instrument with a controller for software handshake is made by crossing the data lines. The following wiring diagram applies to a controller with a 9-pin or 25-pin configuration.

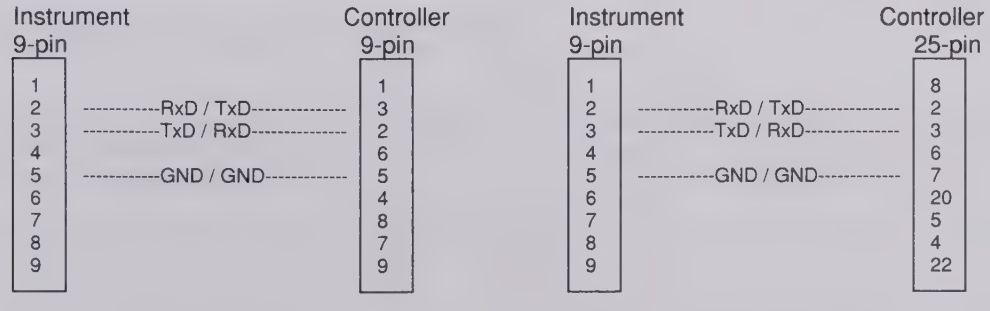

Fig. 8-1 Wiring of the data lines for software handshake

Hardware handshake

For hardware handshake, the instrument indicates that it is ready to receive data via the lines DTR and RTS. A logic '0' on both lines means 'ready' and a logic '1' means 'not ready'. The RTS line is always active (logic '0') as long as the serial interface is switched on. The DTR line thus controls the readiness of the instrument to receive data.

The readiness of the remote station to receive data is reported to the instrument via the CTS and DSR line. A logic '0' on both lines activates the data output and a logic '1' on both lines stops the data output of the instrument. The data output takes place via the TxD line.

Cable for hardware handshake

The connection of the instrument to a controller is made with a so-called zero modem cable. Here, the data, control and acknowledge lines must be crossed. The following wiring diagram applies to a controller with a 9-pin or 25-pin configuration.

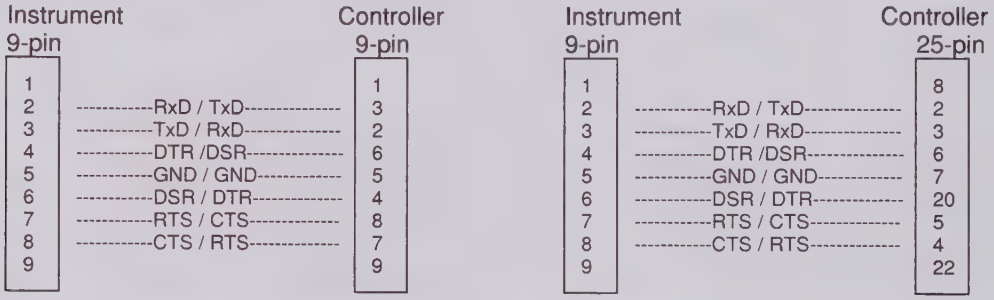

Fig. 8-2 Wiring of the data, control and acknowledge lines for hardware handshake

Monitor Connector (MONITOR)



Pin	Signal
1	R
2	G
3	B
4	(NC)
5	GND
6	GND
7	GND
8	GND
9	GND
10	GND
11	(NC)
12	(NC)
13	HSYNC
14	VSYNC
15	(NC)

Fig. 8-6 Pin assignments of the MONITOR connector.

Noise Source Control (NOISE SOURCE)

Using the NOISE SOURCE connector, an external noise source can be switched on/off, in order, e.g., to measure the noise figure of Units Under Test (UUTs). Usual noise sources require a +28 V signal to be turned on. At 0 V, they are turned off. These supply voltages are delivered by the connector. Maximum current is 100 mA.

External Trigger Input (EXT TRIG/GATE)

The EXT TRIG/GATE connector is used for controlling the measurement via an external signal. The trigger voltages are TTL level (Low < 0.7 V, High > 1.4 V), typ. input impedance is 10 kOhm

Mouse Connector (MOUSE)

A PS/2 connector is provided at the rear panel to connect a PS/2 mouse:



Pin	Signal
1	MOUSEDATA
2	KEYBOARDDATA
3	MOUSEGND
4	MOUSEVD5
5	MOUSECLK
6	KEYBOARDCLK

Fig 8-7 Pin assignments for the MOUSE connector.

Reference Output/Input (REF IN and REF OUT)

For operation with an external reference, the internal reference oscillator is then synchronized to the 10-MHz reference applied to the connector. The necessary level is > 0 dBm.

The internal 10 MHz reference signal is also available at the REF OUT connector and thus provides the capability of, e.g., synchronization of external instruments to the FSP. The output level is 0 dBm.

Selection between internal and external reference is possible in the *SETUP* menu.

IF Output 20.4 MHz (20.4 MHz OUT)

The 2o,4 MHz IF signal of the FSP is available at the 20.4 MHz OUT BNC connector. The bandwidth corresponds to the selected bandwidth for a resolution bandwidth between 100 kHz and 10 MHz. For a resolution bandwidth below 100 kHz, the bandwidth of the output is 2.6 times the resolution bandwidth with a minimum of 2.6 kHz.

The signal level at the IF output is 0 dBm for resolution bandwidth ≥ 100 kHz, and –10 dBm for resolution bandwidth < 100 kHz (mixer level ≥ 60 dBm) .

Contents - Chapter 9 "Error Messages"

9 Error Messages 9.1

SCPI-Specific Error Messages 9.2

Device-Specific Messages 9.8

9 Error Messages

Error messages are entered in the error/event queue of the status reporting system in the remote control mode and can be queried with the command SYSTem:ERRor?. The answer format of FSP to the command is as follows:

<error code>, "<error text with queue query>;
<remote control command concerned>"

The indication of the remote control command with prefixed semicolon is optional.

Example:

The command "TEST:COMMAND" generates the following answer to the query SYSTem:ERRor? :

-113,"Undefined header;TEST:COMMAND"

The subsequent list contains the description of error texts displayed on the instrument.

Distinction is made between error messages defined by SCPI, which are marked by negative error codes, and the device-specific error messages for which positive error codes are used.

The right-hand column in the following tables contains the error text in bold which is entered in the error/event queue and can be read out by means of query SYSTem:ERRor?. A short explanation of the error cause is given below. The left-hand column contains the associated error code.

SCPI-Specific Error Messages

No Error

Error code	Error text in the case of queue poll Error explanation
0	**No error** This message is output if the error queue does not contain any entries.

Command Error - Faulty command; sets bit 5 in the ESR register.

Error code	Error text in the case of queue poll Error explanation
-100	**Command Error** The command is faulty or invalid.
-101	**Invalid Character** The command contains an invalid sign. Example: A header contains an ampersand, "**SENSe&**".
-102	**Syntax error** The command is invalid. Example: The command contains block data the instrument does not accept.
-103	**Invalid separator** The command contains an imallowed sign instead of a separator. Example: A semicolon is missing after the command.
-104	**Data type error** The command contains an invalid value indication. Example: ON is indicated instead of a numeric value for frequency setting.
-105	**GET not allowed** A Group Execute Trigger (GET) is within a command line.
-108	**Parameter not allowed** The command contains too many parameters. Example: Command **SENSe:FREQuency:CENTer** permits only one frequency indication.

Continuation: Command Error

Error code	Error text in the case of queue poll Error explanation
-109	**Missing parameter** The command contains too few parameters. Example: The command **SENSe:FREQuency:CENTer** requires a frequency indication.
-110	**Command header error** The header of the command is faulty.
-111	**Header separator error** The header contains an imallowed separator. Example: the header is not followed by a "White Space", "***ESE255**"
-112	**Program mnemonic too long** The header contains more than 12 characters.
-113	**Undefined header** The header is not defined for the instrument. Example: ***XYZ** is undefined for every instrument.
-114	**Header suffix out of range** The header contains an imallowed numeric suffix. Example: **SENSe3** does not exist in the instrument.
-120	**Numeric data error** The command contains a faulty numeric parameter.
-121	**Invalid character in number** A number contains an invalid character. Example: An "A" in a decimal number or a "9" in an octal number.
-123	**Exponent too large** The absolute value of the exponent is greater than 32000.
-124	**Too many digits** The number includes too many digits.
-128	**Numeric data not allowed** The command includes a number which is not allowed at this position. Example: The command **INPut:COUPling** requires indication of a text parameter.
-130	**Suffix error** The command contains a faulty suffix.
-131	**Invalid suffix** The suffix is invalid for this instrument. Example: nHz is not defined.
-134	**Suffix too long** The suffix contains more than 12 characters.
-138	**Suffix not allowed** A suffix is not allowed for this command or at this position of the command. Example: The command ***RCL** does not permit a suffix to be indicated.
-140	**Character data error** The command contains a faulty text parameter
-141	**Invalid character data** The text parameter either contains an invalid character or it is invalid for this command. Example: Write error with parameter indication;**INPut:COUPling XC.**

Continuation: Command Error

Error code	**Error text in the case of queue poll** Error explanation
-144	**Character data too long** The text parameter contains more than 12 characters.
-148	**Character data not allowed** The text parameter is not allowed for this command or at this position of the command. Example: The command `*RCL` requires a number to be indicated.
-150	**String data error** The command contains a faulty string.
-151	**Invalid string data** The command contains a faulty string. Example: An END message has been received prior to the terminating apostrophe.
-158	**String data not allowed** The command contains a valid string at a position which is not allowed. Example: A text parameter is set in quotation marks, `INPut:COUPling "DC"`
-160	**Block data error** The command contains faulty block data.
-161	**Invalid block data** The command contains faulty block data. Example: An END message was received prior to reception of the expected number of data.
-168	**Block data not allowed** The command contains valid block data at an imallowed position. Example: The command `*RCL` requires a number to be indicated.
-170	**Expression error** The command contains an invalid mathematical expression.
-171	**Invalid expression** The command contains an invalid mathematical expression. Example: The expression contains mismatching parentheses.
-178	**Expression data not allowed** The command contains a mathematical expression at an imallowed position.

Execution Error - Error on execution of a command; sets bit 4 in the ESR register

Error code	Error text in the case of queue poll Error explanation
-200	**Execution error** Error on execution of the command.
-201	**Invalid while in local** The command is not executable while the device is in local due to a hard local control. Example: The device receives a command which would change the rotary knob state, but the device is in local so the command can not be executed.
-202	**Settings lost due to rtl** A setting associated with hard local control was lost when the device changed to LOCS from REMS or to LWLS from RWLS.
-210	**Trigger error** Error on triggering the device.
-211	**Trigger ignored** The trigger (GET, *TRG or trigger signal) was ignored because of device timing considerations. Example: The device was not ready to respond.
-212	**Arm ignored** An arming signal was ignored by the device.
-213	**Init ignored** Measurement initialisation was ignored as another measurement was already in progress.
-214	**Trigger deadlock** The trigger source for the initiation of measurement is set to GET and subsequent measurement is received. The measurement cannot be started until a GET is received, but the GET would cause an interrupted-error)
-215	**Arm deadlock** The trigger source for the initiation of measurement is set to GET and subsequent measurement is received. The measurement cannot be started until a GET is received, but the GET would cause an interrupted-error.
-220	**Parameter error** The command contains a faulty or invalid parameter.
-221	**Settings conflict** There is a conflict between setting of parameter value and instrument state.
-222	**Data out of range** The parameter value lies out of the allowed range of the instrument.
-223	**Too much data** The command contains too many data. Example: The instrument does not have sufficient storage space.
-224	**Illegal parameter value** The parameter value is invalid. Example: The text parameter is invalid , **`TRIGger:SWEep:SOURce TASTe`**

Continuation: Execution Error

Error code	**Error text in the case of queue poll** Error explanation
-230	**Data corrupt or stale** The data are incomplete or invalid. Example: The instrument has aborted a measurement.
-231	**Data questionable** The measurement accuracy is suspect.
-240	**Hardware error** The command cannot be executed due to problems with the instrument hardware.
-241	**Hardware missing** Hardware is missing. Example: An option is not fitted.
-250	**Mass storage error** A mass storage error occured.
-251	**Missing mass storage** The mass storage is missing. Example: An option is not installed.
-252	**Missing media** The media is missing. Example: There is no floppy in the floppy disk drive.
-253	**Corrupt media** The media is corrupt. Example: The floppy is bad or has the wrong format.
-254	**Media full** The media is full. Example: There is no room on the floppy.
-255	**Directory full** The media directory is full.
-256	**File name not found** The file name cannot be found on the media.
-257	**File name error** The file name is wrong. Example: An attempt is made to copy to a duplicate file name.
-258	**Media protected** The media is protected. Example: The write-protect tab on the floppy is present.
-260	**Expression error** The expression contains an error.

Device Specific Error; sets bit 3 in the ESR register

Error code	Error test in the case of queue poll Error explanation
-300	**Device-specific error** FSP-specific error not defined in greater detail.
-310	**System error** This error message suggests an error within the instrument. Please inform the R&S Service.
-313	**Calibration memory lost** Loss of the non-volatile data stored using the *CAL? command. This error occurs when the correction data recording has failed.
-330	**Self-test failed** The selftest could not be executed.
-350	**Queue overflow** This error code is entered in the queue instead of the actual error code if the queue is full. It indicates that an error has occurred but not been accepted. The queue can accept 5 entries.

Query Error - Error in data request; sets bit 2 in the ESR register

Error code	Error text in the case of queue poll Error explanation
-400	**Query error** General error occurring when data are requested by a query.
-410	**Query INTERRUPTED** The query has been interrupted. Example: After a query, the instrument receives new data before the response has been sent completely.
-420	**Query UNTERMINATED** The query is incomplete. Example: The instrument is addressed as a talker and receives incomplete data.
-430	**Query DEADLOCKED** The query cannot be processed. Example: The input and output buffers are full, the instrument cannot continue operation.
-440	**Query UNTERMINATED after indefinite response** A query is in the same command line after a query which requests an indefinite response.

Device-Specific Messages

Error code	**Error text in the case of queue poll** Error explanation
1036	**MS: The correction table based amplifier gain exceeds the amplifier range for CALAMP1 and CALAMP2 on IF board** This message is output when the setting range of the calibration amplifier is not sufficient for the required correction. The error occurs only with modules which are not correcty adjusted or defective.
1052	**Frontend LO is Unlocked** This message is output when the phase regulation of the local oscillator fails in the RF frontend.
1060	**Trigger-Block Gate Delay Error- gate length < Gate Delay** This message is output when the gate signal length is not sufficient for the pull-in delay with a predefined gate delay.
1064	**Tracking LO is Unlocked** This message is output when the phase regulation of the local oscillator fails on the tracking generator module.

Error code	**Error text in the case of queue poll** Error explanation
2022	**OPTIONS.INI invalid** This message is output when an error has been recognized in the file OPTIONS.INI which contains the clearing codes for retrofitable firmware applications. If this file is not correctly recognized, all firmware applications are blocked for this instrument.
2028	**Hardcopy not possible during measurement sequence** This message is output when a printout is started during scan sequences that cannot be interrupted. Such sequences are for example: • Recording the system error correction data (calibration) • Instrument selftest In such cases a synchronization to the end of the scan sequence should be performed prior to starting the printout.
2033	**Printer Not Available** This message is output when the selected printer is not included in the list of available output devices. A possible cause is that the required printer driver is missing or incorrectly installed.
2034	**CPU Temperature is too high** This message is output when the temperature of the processor exceeds 70 °C.

10 Index

Note: *All softkeys are listed alphabetically under keyword "Softkey" with their names. The page numbers 4.xxx refer to the detailed description of the softkeys in chapter 4. Generally, the number of the page in chapter 6 containing the equivalent remote control command is given in addition.*
A list of softkeys and equivalent remote control commands or command sequences is given in chapter 6, section "Table of Softkeys with IEC/IEEE-Bus Command Assignment".
Chapter 6 also contains an alphabetical list of all remote control commands.

*

** (enhancement lable) ... 3.6, 4.39*

0

0 to 9 (key) ... 3.11

1

1 - 2 (trace info) ... 4.49
1 - 3 (trace info) ... 4.49

2

20.4 MHz Out ... 8.11

7

75 Ω (enhancement lable) ... 3.6

A

Abort
print ... 4.153
recording of correction data ... 4.51
AC supply connection ... 1.13
ACP measurement ... 4.81
Addressed command ... 8.5
Adjacent-channel power measurement ... 4.83
Administrator function ... 1.17
AF demodulation ... 4.65
AF OUTPUT ... 8.2
AM demodulation ... 4.66
AM modulation ... 4.176
AM modulation depth ... 4.105
Amplitude ... 4.13
Amplitude probability distribution function ... 4.101
Amplitude statistics ... 4.99
Analyzer mode ... 4.5
Annotation ... 4.122
AP (trace info) ... 3.5
APD function ... 4.101
Ascii # ... 5.12
Attenuation ... 4.15
Autopeak detector ... 4.46
AV (trace info) ... 3.5
Average detector ... 4.45, 4.48
Averaging ... 4.38, 4.79
continuous sweep ... 4.38
lin/log ... 4.40
single sweep ... 4.38
sweep count ... 4.38
AVG (trace info) ... 3.5

B

BACK (key) ... 3.11
Bandfilter, digital ... 4.24
Bandpass ... 4.24
Bandwidth
occupied ... 4.96
resolution ... 4.19
video ... 4.20
Battery-powered memory ... 1.16
Baud rate ... 4.128
Block data ... 5.12
Boolean parameter ... 5.11
Brightness ... 4.124

C

Calibration
functioning ... 4.173, 4.188
reflection measurement ... 4.187
reflexion measurement ... 4.172
transmission measurement ... 4.166, 4.181
Calibration results ... 4.51
CANCEL (key) ... 3.11
CCDF function ... 4.101
Center frequency ... 4.6
Step size ... 4.7

power ... 4.90
bandwidth ... 4.89, 4.97
... 4.88
number ... 4.88
spacing ... 4.90
Channel power measurement ... 4.83
Characters, special ... 6.2
Clear/Write mode ... 4.37
CLWR (trace info) ... 3.5
Colon ... 5.12
Color ... 4.124
COM interface ... 4.128, *8.7*
Comma ... 5.12

Command
- # ... 5.12
- addressed ... 8.5
- alphabetical list ... 6.216
- assignment to softkey ... 6.226
- colon ... 5.12
- comma ... 5.12
- description ... 6.1
- header ... 5.8
- line ... 5.10
- list ... 6.216
- long form ... 5.9
- overlapping execution ... 5.15
- programming examples ... 7.1
- query ... 5.10
- question mark ... 5.10, 5.12
- quotation mark ... 5.12
- recognition ... 5.14
- sequence ... 5.15
- short form ... 5.9
- structure ... 5.7
- suffix ... 5.9
- syntax elements ... 5.12
- univeral ... 8.5
- white space ... 5.12

Common commands ... 6.4
CONDition register part ... 5.17
Configuration ... 4.125
- save ... 4.142

Continue single sweep ... 4.28
Continuous sweep ... 4.27
Control
- output level ... 4.165

Control characters ... 8.9
Copy
- file ... 4.150
- limit line ... 4.113
- trace ... 4.43

Correction data ... 4.50
Correction of entry ... 3.17
Correction values
- normalization ... 4.163, 4.179

Counter resolution ... 4.55
Coupling
- bandwidths ... 4.18
- default settings ... 4.21, 4.23
- frequency of diagrams ... 4.121
- reference level of diagramms ... 4.121
- resolution bandwidth ... 4.20
- sweep time ... 4.21
- video bandwidth ... 4.21

CP measurement ... 4.83
Culmulative distribution function ... 4.101

D

Date ... 4.122
- input ... 4.131

DCL ... 5.14
Decimal point ... 3.11
Default
- coupling ratios ... 4.21
- display settings ... 4.122
- scalings of x- and y-axis ... 4.103

Delay, gate signal ... 4.34
Delete
- file ... 4.150
- limit line ... 4.113

Demodulation ... 4.65
Detector
- autopeak ... 4.44
- average ... 4.45
- max peak ... 4.44
- min peak ... 4.44
- quasipeak ... 4.45
- RMS ... 4.45
- sample ... 4.44

Device reset (overall) ... 4.2
Directory
- create ... 4.150
- rename ... 4.150

Diskette, format ... 4.150
Display
- brightness ... 4.124
- color ... 4.124
- date ... 4.122
- deactivation during single sweep ... 4.28
- power-save mode ... 1.15, 4.123
- saturation ... 4.124
- time ... 4.122
- tint ... 4.124
- title ... 4.122

Display mode
- full screen ... 3.8, 4.120
- split screen ... 3.8, 4.120

Display range
- frequency ... 4.6
- level ... 4.13
- span ... 4.11

Distribution function ... 4.101
Double dagger ... 5.12

E

Editing
- limit line ... 4.114
- parameter ... 3.16
- table ... 3.21

Electrostatic discharge ... 1.12
EMI Protection ... 1.13
ENABle register part ... 5.17
Enabling the front panel keys ... 4.4
Enhancement labels ... 3.6
ENTER (key) ... 3.11
Entry
- abort ... 3.11
- activate ... 3.14, 3.23
- correct ... 3.17
- terminate ... 3.11

Error messages ... 4.138, 9.1
Error variable - iberr ... 4.213
Error-queue query ... 5.29
ESC (key) ... 3.11
ESE (event status enable register) ... 5.20
ESR (event status register) ... 5.20
EVENt register part ... 5.17
Event status enable register (ESE) ... 5.20
Event status register (ESR) ... 5.20
EXT (enhancement lable) ... 3.6
EXT TRIGGER/GATE input ... 4.30, 8.11
External noise source ... 4.126

F

Fast power measurement ... 4.91
FFT filter ... 4.24
File
- copy ... 4.150
- delete ... 4.150

rename ... 4.150
sort ... 4.150
Filter
Bandfilter ... 4.24
FFT ... 4.24
Firmware update ... 4.141
Firmware version ... 4.137
Fixed filter ... 4.24
FM demodulation ... 4.66
FM modulation ... 4.176
Free-run sweep ... 4.29
Frequency ... 4.6
axis labelling ... 3.4
center ... 4.6
counter ... 4.55
coupling of diagrams ... 4.121
display window ... 4.6, 4.11
offset ... 4.9
Offset (ext. generator) ... 4.189
offset (tracking generator) ... 4.174
span ... 4.11
start ... 4.9
stop ... 4.9
switching off display ... 4.122
Frequency-converting measurements ... 4.174, 4.189
FRQ (enhancement lable) ... 3.6
Full screen ... 3.8, 4.120
Full span ... 4.12

G

GAT (enhancement lable) ... 3.6
Gate
delay ... 4.34
external/internal ... 4.32
length ... 4.34
GET (Group Execute Trigger) ... 5.14
GHz/-dBm (key) ... 3.11

H

Hardcopy
format ... 4.155
orientation ... 4.155
screen ... 4.152
Hardware adjustment ... 4.141
Hardware settings, indication ... 3.3
Header ... 5.8
Help line editor ... 3.20
Hotkey
SCREEN A/B ... 4.3, 6.89
SPECTRUM ... 4.3, 4.5, 6.105
Hz/dB. (key) ... 3.11

I

I/Q modulation ... 4.177
IEC/IEEE bus
address ... 4.127
command description ... 6.1
interface ... 8.3
interface functions ... 8.4
programming examples ... 7.1
IFOVL ... 3.5
Impedance of input ... 4.16
Indication
hardware settings ... 3.3
instrument settings ... 3.6
marker information ... 3.4
Initial configuration ... 4.2
Input
EXT TRIGGER/GATE ... 4.30, 8.11
REF IN ... 8.11
Input impedance ... 4.16
Instrument functions ... 4.1
Interface functions
IEC/IEEE bus ... 8.4
Interfaces ... 8.2
Intermodulation product ... 4.106
Interrupt ... 5.28
IST flag ... 5.20

K

Key
0 to 9 ... 3.11
AMPT ... 4.13
BACK ... 3.11
BW ... 4.19
CAL ... 4.50
CANCEL ... 3.11
DISP ... 4.119
ENTER ... 3.11
ESC ... 3.11, 6.19
FILE ... 4.142
FREQ ... 4.6
GHz/-dBm ... 3.11
Hz/dB ... 3.11
kHz/dB ... 3.11
LINES ... 4.110
MEAS ... 4.75
MHz/dBm ... 3.11
MKR ... 4.52
MKR FCTN ... 4.59
MKR to ... 4.67
PRESET ... 4.2, 6.6, 6.172
roll-key ... 3.12
SETUP ... 4.125
SPAN ... 4.11
SWEEP ... 4.27
TRACE ... 4.36
TRIG ... 4.29
Keyboard
connection ... 1.18
connector ... 8.2
kHz/dB (key) ... 3.11

L

LAN-Interface ... 4.195
Level ... 4.13
display range ... 4.13
offset (phase noise) ... 4.63
offset (tracking generator) ... 4.165
range ... 4.13
reference ... 4.13
Limit
ACP measurement ... 4.92
evaluation range ... 4.78
probability range ... 4.103
Limit check ... 4.112
ACP measurement ... 4.92
Limit line
copy ... 4.113
delete ... 4.113
domain ... 4.115

edit ... 4.114
limit check ... 4.112
offset ... 4.113
save ... 4.118
scaling ... 4.116
select ... 4.111
shift ... 4.118
unit ... 4.116
value ... 4.118
Line
limit ... 4.111
reference (tracking generator) ... 4.169, 4.184
threshold ... 4.70
LO exclude ... 4.74
Login/out (NT controller) ... 1.17
Logo ... 4.122
Lower case ... 6.2
LPT interface ... 8.6

M

Maintenance ... 8.1
Manual operation
return to ... 5.4
switch to ... 4.4
Marker ... 4.52
center frequency to ... 4.68
CF stepsize to ... 4.73
indication ... 3.4
N dB Down ... 4.64
normal ... 4.52
peak ... 4.60, 4.67
reference level to ... 4.68
search limit ... 4.70
signal track ... 4.10
to trace ... 4.54, 4.66
zoom ... 4.58
Max hold ... 4.37
Max peak detector ... 4.47
MAXH (trace info) ... 3.5
Maximum peak value ... 4.79
Maximum search ... 4.67
Maximum value ... 4.77
Mean power (GSM burst) ... 4.78
Mean value ... 4.78
Measurement
frequency-converting ... 4.174, 4.189
reflection ... 4.187
reflexion ... 4.172
transmission ... 4.166, 4.181
Measurement example
ACP with user-specific channel configuration ... 4.94
adjacent-channel power for a specific standard ... 4.93
CCDF of a IS95 BTS signal ... 4.104
occupied bandwidth of a PDC signal ... 4.98
signal/noise power density (C/No) of an IS95 CDMA signal ... 4.95
Measurement Example
Harmonic ... 2.5
Measurement, save ... 4.142
Memory, battery-powered ... 1.16
Menu
call ... 3.10
change keys ... 3.10
Messages ... 4.138
acknowledgement ... 3.7
MHz/dBm (key) ... 3.11
MI (trace info) ... 3.5
Min hold ... 4.40
Min peak detector ... 4.47
MINH (trace info) ... 3.5
Minimum search ... 4.73
Mobile radio standard ... 4.84
Mode
analyzer ... 4.5
Modulation
external (tracking generator) ... 4.175
Modulation depth ... 4.105
Monitor
connection ... 1.20
connector ... 8.10
Mouse
connection ... 1.19
connector ... 8.11
Mouse-Buchse ... 8.2
MSG ... 3.5

N

Noise
source, external ... 4.126
Noise measurement ... 4.60
Noise Source ... 4.126
NOISE SOURCE ... 8.11
Normalization ... 4.168, 4.183
NT computer ... 1.17
NTRansition register part ... 5.17
Numerical values (command) ... 5.11

O

Occupied bandwidth ... 4.96
Offset
frequency ... 4.9
frequency (ext. generator) ... 4.189
gate signal ... 4.34
level (tracking generator) ... 4.165
limit line ... 4.113
phase noise ... 4.63
reference level ... 4.15
trigger ... 4.30
Operating time ... 4.137
Option
FSP-B16 – LAN Interface ... 4.195
Order number ... 4.136
Orientation ... 4.155
Output
AF OUTPUT ... 8.2
IF 20.4 MHz Out ... 8.11
noise source control ... 8.11
REF OUT ... 8.11
Output level
control ... 4.165
OVEN ... 3.5
Overwrite mode ... 4.37
OVLD ... 3.5, 4.173, 4.188

P

Packing ... 8.1
Parallel poll ... 5.29
Parallel poll enable register (PPE) ... 5.20
Parameter
block data ... 5.12
boolean ... 5.11
editing ... 3.16
numerical values ... 5.11

selection ... 3.13
string ... 5.12
text ... 5.12
Password
service functions ... 4.140
Windows NT ... 1.17
Path ... 4.149
Peak excursion ... 4.71
Peak search ... 4.60, 4.67
Phase noise measurement ... 4.62
PK (trace info) ... 3.5
Polarity
external trigger/gate ... 4.33
trigger edge ... 4.30
Power bandwidth percentage ... 4.96
Power cables ... 8.1
Power measurement ... 4.75
CP/ACP ... 4.81
Fast ... 4.91
occupied bandwidth ... 4.96
signal amplitude statistics ... 4.99
Time Domain ... 4.76
Power, mean ... 4.78
Power-save mode
display ... 1.15
hard disk ... 1.15
PPE (parallel poll enable register) ... 5.20
Preamplifier ... 4.126
Preparing the instrument for Operation ... 1.12
Preset instrument ... 4.2
Pretrigger ... 4.30
Print
abort ... 4.153
start ... 4.152
Printer
configuration ... 4.151
connection ... 1.21, 8.6
interface ... 8.6
PRN (enhancement lable) ... 3.6
Probe Power connector ... 8.2
PTRansition register part ... 5.17
Putting into operation
AC supply connection ... 1.13
Getting Started with the instrument ... 1.12

Q

QP (trace info) ... 3.5
Quasipeak detector ... 4.45
Query ... 5.10, 5.29
Question mark ... 5.10, 5.12
Quotation mark ... 5.12

R

Rackmounting ... 1.13
Recording the correction data ... 4.50
Reference
dataset (tracking generator) ... 4.173, 4.188
external ... 4.126
fixed ... 4.56
frequency ... 4.56
level to marker level ... 4.68
line (tracking generator) ... 4.169, 4.184
position for normalization ... 4.184
Reference level ... 4.13
channel power ... 4.85
coupling of diagrams ... 4.121
offset ... 4.15
position ... 4.15
to marker level ... 4.68
Reference point
frequency ... 4.56
frequency (phase noise) ... 4.64
level ... 4.56
offset ... 4.56
level (phase noise) ... 4.63
offset ... 4.63
time ... 4.57
x axis ... 4.57
channel power ... 4.85
... 4.79
Reflection measurement ... 4.172, 4.187
Remote control
basics ... 5.1
IEC/IEEE bus ... 5.4
RS-232-C ... 5.5
switch over ... 5.3
Remote Control
RSIB ... 4.211
Rename
directory ... 4.150
file ... 4.150
Reset
device ... 4.2
status reporting system ... 5.30
Resolution bandwidth ... 4.19
Resolution counter ... 4.55
RF ATTEN MANUAL ... 4.16
RF attenuation ... 4.15
RM (trace info) ... 3.5
RMS detector ... 4.45, 4.47
RMS value ... 4.77
Roll-key ... 3.12
RS-232-C
configuration ... 4.128
interface ... 8.7
transmission parameters ... 8.8

S

SA (trace info) ... 3.5
Sample detector ... 4.47
Sample number ... 4.102
Saturation ... 4.124
Save
configuration ... 4.142
limit line ... 4.118
measurement ... 4.142
Scalar reflection measurement ... 4.172, 4.187
Scaling
level axis ... 4.16
level display range ... 4.14
limit line ... 4.116
x- and y-axis (signal statistic) ... 4.102
SCPI
conformity information ... 6.1
introduction ... 5.7
SCPI version ... 5.1
Screen ... 3.1
full screen ... 4.120
split screen ... 3.8, 4.120
subdivision ... 3.2
Search
bandwidth ... 4.10
direction ... 4.69
minimum ... 4.73
peak ... 4.60, 4.67

peak excursion 4.71
range 4.70
Selftest 4.140
Sensitivity
APD measurement 4.103
CCDF measurement 4.103
Serial interface 8.7
configuration 4.128
Serial number 4.136
Serial poll 5.28
Service functions 4.139
Service request (SRQ) 5.19, 5.28
Service request enable register (SRE) 5.19
Setting up the Instrument 1.12
Settings, indication 3.6
Setup 4.125
general 4.127
SGL (enhancement lable) 3.6
Sign (key) 3.11
Signal amplitude statistics 4.99
Signal count 4.55
Signal tracking 4.10
search bandwidth 4.10
Single sweep 4.27
Softkey
% POWER BANDWIDTH 4.96, 6.145
= CENTER 4.7, 4.8
= MARKER 4.7, 4.8
0.1 * RBW 4.8, 6.128, 6.129
0.1 * SPAN 4.7, 6.128, 6.129
0.5 * RBW 4.8, 6.128, 6.129
0.5 * SPAN 4.7, 6.128, 6.129
ABSOLUTE PEAK/MIN 4.69, 6.12, 6.13
ACP LIMIT CHECK 4.92, 6.21
ADJ CHAN BANDWIDTH 4.89, 6.143
ADJ CHAN SPACING 4.90, 6.141, 6.142
ADJUST REF LVL 4.85, 4.97, 6.144
ADJUST SETTINGS 4.86, 4.103, 6.77, 6.144
ALL MARKER OFF 4.58, 6.10, 6.41
AM 4.66, 6.52
AMPERE 4.14, 6.81
ANNOTATION ON/OFF 4.122, 6.87
APD ON/OFF 4.101, 6.76, 6.79
area 3.9
ASCII FILE EXPORT 4.41, 6.94, 6.115
AUTO SELECT 4.46, 6.127
AVERAGE 4.38, 6.92, 6.121
AVERAGE ON/OFF ... 4.79, 6.65, 6.66, 6.68, 6.70, 6.72
AVG MODE LOG/LIN 4.40
AVG MODE VIDEO/LIN 6.75, 6.121
BLANK 4.39, 6.93
BRIGHTNESS 4.124, 6.88
CAL ABORT 4.51, 6.82
CAL CORR ON/OFF 4.51, 6.83
CAL REFL OPEN 4.172, 4.187
CAL REFL SHORT 4.172, 4.187
CAL RESULTS 4.51, 6.83
CAL TOTAL 4.50, 6.82
CAL TRANS 4.167, 4.182, 6.125
CCDF ON/OFF 4.101, 6.76, 6.79
CENTER 4.6, 6.128
CENTER = MKR FREQ 4.68, 6.54
CENTER A = MARKER B 4.121, 6.106
CENTER B = MARKER A 4.121, 6.106
CHAN PWR /ACP 4.83, 6.56
CHAN PWR /HZ 4.85, 6.59
CHANNEL BANDWIDTH 4.89, 4.97, 6.142
CLEAR ALL MESSAGES 4.138, 6.171, 6.172
CLEAR/WRITE 4.37, 6.92
CNT RESOL 4.55, 6.43
COLOR ON/ OFF 4.155, 6.96
COM INTERFACE 4.128, 6.168
command assignment 6.226
COMMENT SCREEN A/B 4.155, 6.98
CONFIG DISPLAY 6.87
CONFIGURE NETWORK 4.132
CONT DEMOD 4.66
CONT MEAS 4.104, 6.100, 6.101
CONTINUE SGL SWEEP 4.28, 6.100, 6.101
CONTINUOUS SWEEP 4.27, 6.100, 6.101
COPY 4.150, 6.109
COPY LIMIT LINE 4.113, 6.20
COPY TRACE 4.43, 6.175
COUPLING DEFAULT 4.23, 6.123, 6.147
COUPLING RATIO 4.21, 6.123
CP/ACP ABS/REL 4.90, 6.143
CP/ACP CONFIG 4.88, 6.21, 6.141
CP/ACP ON/OFF 4.83, 6.56, 6.57, 6.60
CP/ACP STANDARD 4.84, 6.60
DATA SET CLEAR 4.147, 6.116
DATA SET CLEAR ALL 4.147, 6.116
DATA SET LIST 4.147
DATAENTRY OPAQUE 4.122
dBm 4.14, 6.81
dBmV 4.14, 6.81
dBpW 4.14, 6.81
dBµA 4.14, 6.81
dBµV 4.14, 6.81
DECIM SEP 4.43, 6.94
DEFAULT COLORS 4.122, 6.88
DEFAULT CONFIG 4.147, 6.118
DEFAULT SETTINGS 4.103, 6.78
DELETE 4.150, 6.111, 6.115
DELETE LIMIT LINE 4.113, 6.20
DELETE VALUE 4.118
DETECTOR 4.46, 6.127
DETECTOR AUTOPEAK 4.46, 6.127
DETECTOR AVERAGE 4.48, 6.127
DETECTOR MAX PEAK 4.47, 6.127
DETECTOR MIN PEAK 4.47, 6.127
DETECTOR QPK 4.48, 6.127
DETECTOR RMS 4.47, 6.127
DETECTOR SAMPLE 4.47, 6.127
DEVICE 1/2 ..... 4.153, 6.96, 6.97, 6.99, 6.114, 6.170
DISPLAY PWR SAVE 4.123, 6.87
EDIT ACP LIMITS 4.92, 6.21, 6.22, 6.23, 6.24, 6.25, 6.26, 6.27, 6.28, 6.29, 6.30
EDIT COMMENT 4.145, 6.118
EDIT LIMIT LINE 4.115, 6.19, 6.32, 6.35, 6.37, 6.38, 6.39
EDIT PATH 4.149, 6.109, 6.114
ENABLE ALL ITEMS 4.147, 6.117
ENTER PASSWORD 4.140, 6.172
EXCLUDE LO 4.74, 6.44
EXT AM 4.176
EXT FM 4.176
EXT I/Q 4.177
EXT SOURCE 4.190
EXT SRC ON/OFF 4.190
EXTERN 4.30, 6.149, 6.182
FAST ACP ON/OFF 4.91, 6.145
FILE MANAGER 4.149, 6.109
FILTER TYPE 4.24, 6.123
FIRMWARE UPDATE 4.141
FM 4.66, 6.52
FORMAT DISK 4.150, 6.111
FREE RUN 4.29, 6.182
FREQUENCY OFFSET 4.9, 4.174, 4.189, 6.130
FREQUENCY SWEEP 4.193
FULL SCREEN 4.120, 6.87
FULL SPAN 4.12, 6.129
GATE DELAY 4.34, 6.149
GATE LENGTH 4.34, 6.149
GATE MODE LEVEL/EDGE 4.33, 6.148

GATE SETTINGS 4.33, 6.148
GATED TRIGGER 4.32, 6.148, 6.149
GENERAL SETUP 4.127
GPIB ADDRESS 4.127, 6.166
GRID ABS/REL 4.16, 6.90
HARDCOPY ABORT 4.153, 6.95
HARDWARE INFO 4.136, 6.6
IF POWER 4.30, 6.149, 6.182
INPUT CAL 4.139, 6.84, 6.85
INPUT RF 4.139, 6.84
INSERT VALUE 4.118
INSTALL PRINTER 4.155
ITEMS TO SAVE/RECALL 4.146, 6.116
LAST SPAN 4.12
LEFT LIMIT 4.70, 6.41, 6.42
LIMIT ON/OFF 4.78, 6.41
LOCAL 4.4
LOGO ON/OFF 4.122, 6.87
MAKE DIRECTORY 4.150, 6.113
MANUAL 4.7, 6.128
MARKER 1 to 4 ..... 4.53, 6.11, 6.12, 6.40, 6.41, 6.44
MARKER DEMOD 4.65, 6.52
MARKER NORM/DELTA 4.53, 6.9
MARKER ZOOM 4.58, 6.51
MAX HOLD 4.37, 6.92
MAX HOLD ON/OFF 4.79, 6.65, 6.67, 6.69, 6.71
MEAN 4.78, 6.67, 6.68
MIN 4.73, 6.13, 6.46
MIN HOLD 4.40, 6.92
MIN NEXT 6.13, 6.47
MKR -> CF STEPSIZE 4.73, 6.55
MKR -> TRACE 4.54, 4.66, 4.73, 6.10, 6.41
MKR CONT DEMOD 6.52
MKR DEMOD ON/OFF 4.65, 6.52
MKR STOP TIME 4.66, 6.52
MODULATION 4.175
MODULATION DEPTH 4.105, 6.53
MODULATION OFF 4.177
N dB DOWN 4.64, 6.49, 6.50
NAME 4.115, 6.19, 6.20, 6.32, 6.33, 6.36, 6.38
NETWORK 4.180
NETWORK LOGIN 4.133, 4.134
NEW LIMIT LINE 4.115, 6.19, 6.20, 6.32, 6.33, 6.35, 6.37
NEXT MIN 4.74, 6.47
NEXT MODE 4.69
NEXT PEAK 4.68, 6.12, 6.13, 6.14, 6.45, 6.46
NO OF SAMPLES 4.102, 6.77
NO. OF ADJ CHAN 4.88, 6.142
NOISE CORR ON/OFF 6.145
NOISE MEAS 4.60, 6.51
NOISE SRC ON/OFF 4.126, 6.85
NORMALIZE 4.168, 4.183
NUMBER OF SWEEPS 4.80, 6.148
OCCUP BW ON/OFF 4.96, 6.56, 6.57, 6.60
OCCUPIED BANDWIDTH 4.96, 6.56
PEAK 4.60, 4.67, 4.77, 6.12, 6.45, 6.64
PEAK EXCURSION 4.71, 6.48
PERCENT MARKER 6.44
PERCENT MARKER 4.101
PH NOISE ON/OFF 4.63, 6.16
PHASE NOISE 4.62, 6.16
POLARITY POS/NEG 4.30, 4.33, 6.149, 6.183
POWER ABS/REL 4.79, 6.72
POWER ON/OFF 4.77, 6.64, 6.66, 6.67, 6.69, 6.73
PREAMP 4.126
PREDEFINED COLORS 4.124, 6.89
PRINT SCREEN 4.152, 6.97, 6.98, 6.114
PRINT TABLE 4.152, 6.97, 6.98, 6.114
PRINT TRACE 4.152, 6.97, 6.98, 6.114
PWR OFFSET 4.165, 6.152
RANGE LINEAR 4.14, 6.92
RANGE LOG 100 dB 4.13, 6.90, 6.92
RANGE LOG MANUAL 4.14, 6.90, 6.92
RBW / VBW MANUAL 4.22, 6.124
RBW / VBW NOISE [10] 4.22, 6.124
RBW / VBW PULSE [.1] 4.22, 6.124
RBW / VBW SINE [1/3] 4.22, 6.124
RECALL 4.145, 6.112
REF FREQUENCY 6.146
REF FXD ON/OFF 4.56, 6.14
REF LEVEL 4.13, 6.91
REF LEVEL = MKR LVL 4.68, 6.55
REF LEVEL COUPLED 4.121, 6.106
REF LEVEL OFFSET 4.15, 6.91
REF LEVEL POSITION 4.15, 6.92
REF POINT FREQUENCY 4.56, 4.64, 6.15
REF POINT LEVEL 4.56, 4.63, 6.15
REF POINT LVL OFFSET 4.56, 4.63, 6.15
REF POINT TIME 4.57, 6.15
REF POINT x-LEVEL 4.57, 6.15
REF VALUE 4.170, 4.185
REF VALUE POSITION 4.169, 4.184
REFERENCE FIXED 4.56, 6.14
REFERENCE INT/EXT 4.126, 6.146
RENAME 4.150, 6.114
RES BW 4.102, 6.122
RES BW AUTO 4.20, 6.123
RES BW MANUAL 4.19, 6.122
RESTORE FIRMWARE 4.141
RF ATTEN AUTO 4.15, 6.102
RF ATTEN MANUAL 4.15, 4.16, 6.102
RF INPUT 50 Ω / 75 Ω 4.16, 6.104
RIGHT LIMIT 4.70, 6.41, 6.42
RMS 4.77, 6.66
SATURATION 4.124, 6.88
SAVE 4.145, 6.115
SAVE CHANGES 6.146
SAVE LIMIT LINE 4.118
SCALING 4.102, 6.77
SCREEN TITLE 4.122, 6.89, 6.90
SEARCH LIMIT OFF 4.70, 6.41
SEARCH LIMITS 4.70, 6.41
SEARCH NEXT LEFT 4.69, 6.13, 6.14, 6.47
SEARCH NEXT RIGHT 4.69, 6.13, 6.14, 6.46, 6.47
SELECT GENERATOR 4.190
SELECT ITEMS 4.146, 6.116, 6.117
SELECT LIMIT LINE 4.111, 6.18, 6.19, 6.35, 6.38
SELECT MARKER 4.60, 4.67, 4.108
SELECT OBJECT 4.123
SELECT TRACE 4.10, 4.37, 4.91, 6.62, 6.145
SELFTEST 4.140, 6.7
SELFTEST RESULTS 4.140, 6.85
SERVICE 4.139, 6.84
SERVICE FUNCTIONS 6.84
SET CP REFERENCE 4.85, 6.143
SET REFERENCE 4.79, 6.73
SGL SWEEP DISP OFF 4.28, 6.101
SHIFT X LIMIT LINE 4.118, 6.33
SHIFT Y LIMIT LINE 4.118, 6.39
SIGNAL COUNT 4.55, 6.43
SIGNAL STATISTIC 4.101, 6.76
SIGNAL TRACK 4.10, 6.61
SINGLE MEAS 4.104, 6.100, 6.101
SINGLE SWEEP 4.27, 6.100, 6.101
SORT MODE 4.150
SOURCE CAL 4.166, 4.181
SOURCE ON/OFF 4.164
SOURCE PWR 4.165, 4.180
SPAN MANUAL 4.11, 6.129
SPAN/RBW AUTO [50] 4.23, 6.123
SPAN/RBW MANUAL 4.23, 6.123
SPLIT SCREEN 4.120, 6.87

STANDARD DEVIATION 4.78, 6.69, 6.70
START 4.9, 6.129
START LIMIT 4.78, 6.42
STARTUP RECALL 4.148, 6.113
STATISTICS 4.137, 6.5
STEPSIZE MANUAL 4.8
STOP 4.9, 6.129
STOP LIMIT 4.78, 6.42
SWEEP COUNT 4.28, 4.39, 6.148
SWEEPTIME AUTO 4.21, 4.28, 6.147
SWEEPTIME MANUAL 4.11, 4.20, 4.28, 6.147
SYSTEM INFO 4.135
SYSTEM MESSAGES 4.138, 6.171, 6.172
T1-T2 ..... 4.49, 6.74
T1-T3 ..... 4.49, 6.74
THRESHOLD 4.70, 6.80
TIME DOM POWER 4.76, 6.64, 6.66, 6.67, 6.69
TIME+DATE 4.131, 6.171, 6.173
TIME+DATE ON/OFF 4.122, 6.90
TINT 4.124, 6.88
TOI 4.107, 6.54
TRACE MATH 4.49, 6.74
TRACE MATH OFF 4.49, 6.75
TRACE POSITION 4.49, 6.74
TRACK BW 4.10, 6.61
TRACK ON/OFF 4.10, 6.61
TRACK THRESHOLD 4.10, 6.62
TRACKING 4.164
TRIGGER OFFSET 4.30, 6.183
UNIT 4.14, 6.81, 6.184
VALUES 4.118, 6.32, 6.34, 6.37
VIDEO 4.29, 6.182
VIDEO BW AUTO 4.21, 6.124
VIDEO BW MANUAL 4.20, 6.124
VIEW 4.39, 6.92
VOLT 4.14, 6.81
WATT 4.14, 6.81
X * RBW 4.8, 6.128, 6.129
X * SPAN 4.7, 6.128, 6.129
X OFFSET 4.113, 6.33
X-AXIS RANGE 4.103, 6.78
X-AXIS REF LEVEL 4.102, 6.77
Y OFFSET 4.113, 6.35, 6.38
Y-AXIS MAX VALUE 4.103, 6.78
Y-AXIS MIN VALUE 4.103, 6.78
ZERO SPAN 4.12, 6.129
ZOOM x-AXIS 4.34
Span 4.11
Special characters **6.2**
Spectrum analyzer mode 4.5
Split screen 3.8, 4.120
Squelch 4.65
SRE (service request enable register) 5.19
SRQ (service request) 5.19, 5.28
Standard deviation 4.78
Standard, mobile radio 4.84
Start frequency 4.9
Statistics 4.99
Status byte (STB) 5.19
Status information **3.4**
IFOVL 3.5
MSG 3.5
OVEN 3.5
OVLD 3.5
UNCAL 3.4
Status register
CONDition part 5.17
ENABle part 5.17
ESE 5.20
ESR 5.20
EVENt part 5.17
NTRansition part 5.17
overview 5.18
PPE 5.20
PTRansition part 5.17
SRE 5.19
STATus\:OPERation 5.21
STATus\:QUEStionable
ACPLimit 5.23
FREQuency 5.24
LIMit 5.25
LMARgin 5.26
POWer 5.27
STB 5.19
structure 5.16
sum bit 5.17
Status reporting system 5.16
resetting values 5.30
STATus\:OPERation register 5.21
STATus\:QUEStionable register 5.22
ACPLimit register 5.23
FREQuency register 5.24
LIMit register 5.25
LMARgin register 5.26
POWer register 5.27
STB (status byte) 5.19
Stepsize 4.8
center frequency 4.7
coupling 4.8
Stop frequency 4.9
Stop time for demodulation 4.66
Storing 8.1
String 5.12
Suffix 5.9
Sum bit **5.17**
Supply voltage, external noise source 4.126
Sweep
continue single sweep 4.28
continuous 4.27
count 4.28
coupling 4.18
free run 4.29
gated 4.31, 4.32
settings 4.27
single 4.27
time 4.11, 4.28
coupling 4.21
Switching cycles 4.137
Switching on/off 1.14
Syntax elements of commands 5.12
System messages 4.138

T

T1-T2 (trace info) 3.5
T1-T3 (trace info) 3.5
Table
operation 3.21
scrolling 3.23
Test
functional 1.16
selftest 4.140
Text parameter 5.12
Third Order Intercept 4.106
Threshold
line 4.70
signal tracking 4.10
Time 4.122
input 4.131
Time axis 4.12
Tint 4.124
Title for the active diagram 4.122

TOI 4.106
Trace 4.36, 4.37
average 4.38
averaging 4.40
blank 4.39
Clear/Write 4.37
copy 4.43
freeze 4.39
math 4.49
max hold 4.37
min hold 4.40
position for 0 difference 4.49
select 4.36
signal tracking 4.10
Trace info 3.5
Tracking generator 4.163
Transmission measurement 4.166, 4.181
Transmission parameters RS-232-C/COM 8.8
TRG (enhancement lable) 3.6
Trigger
external 4.30
external gate 4.32
free run 4.29
gated sweep 4.33
IF power 4.30
offset 4.30
slope 4.30
sweep 4.29
video 4.29

U

UNCAL 3.4
Unit
level axis 4.14
limit line 4.116
Unit (key) 3.11
Universal command 8.5
Upper case 6.2

V

Video bandwidth 4.20
Video triggering 4.29
VIEW (trace info) 3.5
View trace 4.39

W

White space 5.12
Windows NT 1.17
administrator 1.17
login 1.17
password 1.17

Z

Zero span 4.12
Zoom 4.58
amplitude 4.39
x-AXIS (gate signal) 4.34

MP MASTER
MA34482